

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX052919\
 Data File : VX009947.D
 Acq On : 29 May 2019 18:00
 Operator : JC/SP
 Sample : K3074-06
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TP-3B-S

Quant Time: May 30 01:16:51 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X052819W.M
 Quant Title : SW846 8260
 QLast Update : Wed May 29 04:00:56 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	171564	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	280388	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	250946	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	108102	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.06	65	119365	49.25	ug/l	0.00
Spiked Amount			Recovery	=	98.50%	
35) Dibromofluoromethane	5.50	113	85812	48.68	ug/l	0.00
Spiked Amount			Recovery	=	97.36%	
50) Toluene-d8	8.71	98	356943	49.86	ug/l	0.00
Spiked Amount			Recovery	=	99.72%	
62) 4-Bromofluorobenzene	11.13	95	118578	46.12	ug/l	0.00
Spiked Amount			Recovery	=	92.24%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
5) Bromomethane	1.67	94	455	0.296	ug/l #	69
6) Chloroethane	1.67	64	501	0.320	ug/l #	46
8) Diethyl Ether	2.20	74	426	0.323	ug/l	71
11) Tert butyl alcohol	3.04	59	1192	1.999	ug/l	98
13) Acrolein	2.29	56	251	21.641	ug/l	92
16) Acetone	2.44	43	33149	23.674	ug/l	96
17) Carbon Disulfide	2.57	76	1137	0.599	ug/l	100
18) Methyl Acetate	2.78	43	3919	1.203	ug/l #	91
20) Methylene Chloride	2.86	84	82179	38.325	ug/l	100
25) 2-Butanone	4.68	43	5532	2.536	ug/l	94
29) Tetrahydrofuran	5.15	42	1529	1.093	ug/l #	91
30) Chloroform	5.21	83	990	0.282	ug/l	97
31) Cyclohexane	5.67	56	3950	1.071	ug/l #	1
36) 1,1-Dichloropropene	5.67	75	13494	4.743	ug/l #	50
38) Carbon Tetrachloride	5.67	117	16269	6.618	ug/l #	16
43) Isopropyl Acetate	6.45	43	10872	1.700	ug/l	96
48) Methyl methacrylate	7.68	41	7193	2.272	ug/l #	20
49) 1,4-Dioxane	7.84	88	23	0.391	ug/l #	18
51) 4-Methyl-2-Pentanone	8.61	43	75969	18.259	ug/l #	53
54) cis-1,3-Dichloropropene	8.62	75	30887	8.693	ug/l #	60
57) 1,3-Dichloropropane	9.54	76	7595	2.051	ug/l #	43
59) 2-Hexanone	9.44	43	10128	3.162	ug/l #	27
76) 1,2,3-Trichloropropane	11.13	75	61841	23.922	ug/l #	34
80) 1,3,5-Trimethylbenzene	11.51	105	2231	0.332	ug/l	92
81) trans-1,4-Dichloro-2-buten	11.13	75	61841	59.188	ug/l #	10
84) 1,2,4-Trimethylbenzene	11.80	105	2752	0.403	ug/l	98
95) Naphthalene	13.83	128	9257	1.167	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX052919\
Data File : VX009947.D
Acq On : 29 May 2019 18:00
Operator : JC/SP
Sample : K3074-06
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TP-3B-S

Quant Time: May 30 01:16:51 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X052819W.M
Quant Title : SW846 8260
QLast Update : Wed May 29 04:00:56 2019
Response via : Initial Calibration

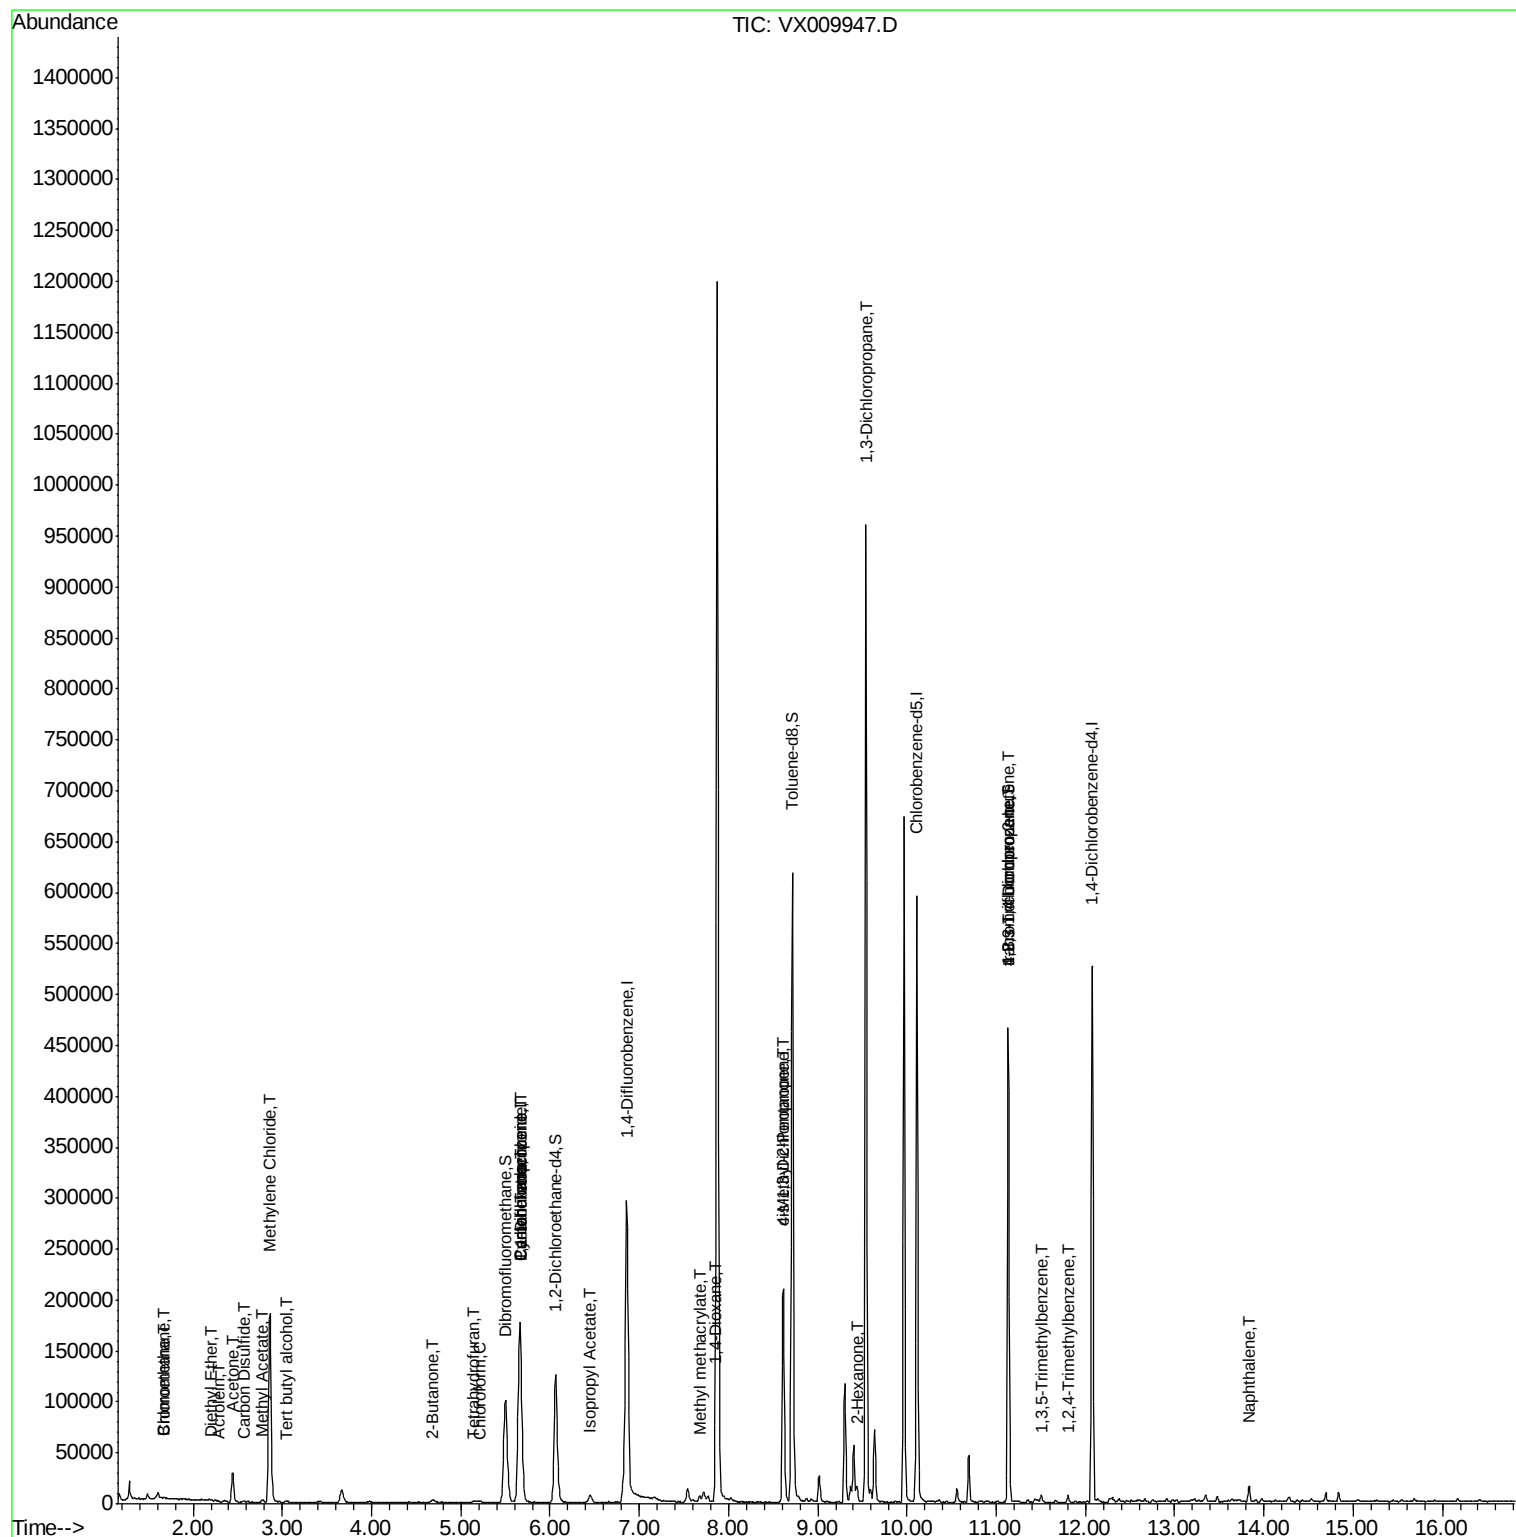



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 740

Delta R.T. -0.00 min

Lab File: VX009947.D

Acq: 29 May 2019 18:00

Instrument :

MSVOA_X

ClientSampleId :


TP-3B-S

Tot Ion:168 Resp: 171564

Ion Ratio Lower Upper




168 100

99 56.1 43.0 64.6

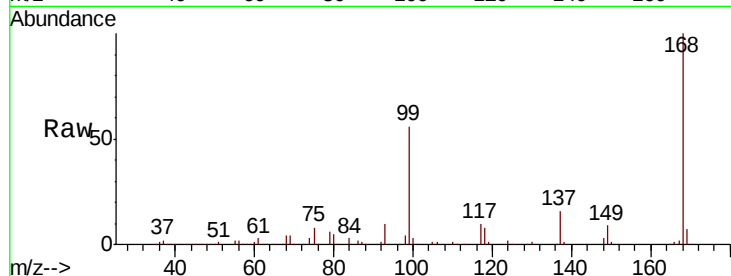

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

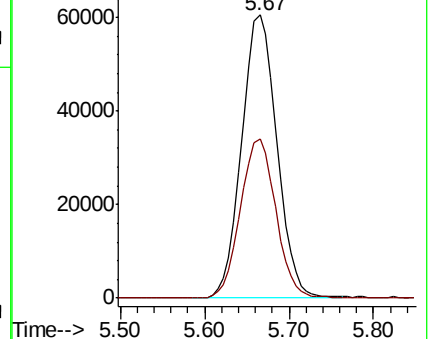

#5

Bromomethane

Concen: 0.296 ug/l

RT: 1.67 min Scan# 84

Delta R.T. 0.02 min

Lab File: VX009947.D


Acq: 29 May 2019 18:00

Tgt Ion: 94 Resp: 455

Ion Ratio Lower Upper



94 100


96 65.0 76.2 114.4#



Abundance Ion 93.90 (93.60 to 94.60): VX0

Ion 95.90 (95.60 to 96.60): VX0

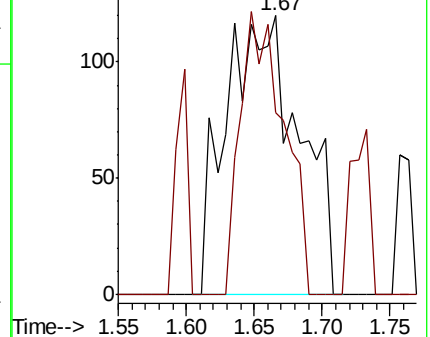



#6

Chloroethane

Concen: 0.320 ug/l

RT: 1.67 min Scan# 84

Delta R.T. -0.05 min

Lab File: VX009947.D

Acq: 29 May 2019 18:00

Instrument :

MSVOA_X

ClientSampleId :


TP-3B-S

Tot Ion: 64 Resp: 501

Ion Ratio Lower Upper

64 100

66 1.4 25.1 37.7#

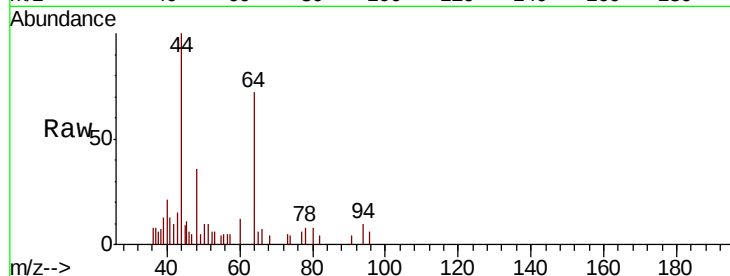

Abundance Ion 63.90 (63.60 to 64.60): VX0

Ion 65.90 (65.60 to 66.60): VX0

1.67

800

600



400

200

0

1.64 1.66 1.68 1.70

Time-->

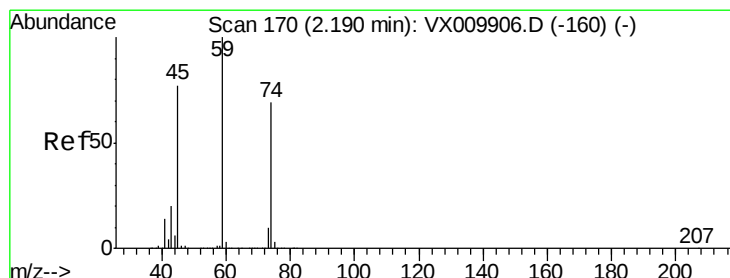

#8

Diethyl Ether

Concen: 0.323 ug/l

RT: 2.20 min Scan# 171

Delta R.T. 0.01 min

Lab File: VX009947.D


Acq: 29 May 2019 18:00

Tgt Ion: 74 Resp: 426

Ion Ratio Lower Upper

74 100

45 81.5 56.1 168.3

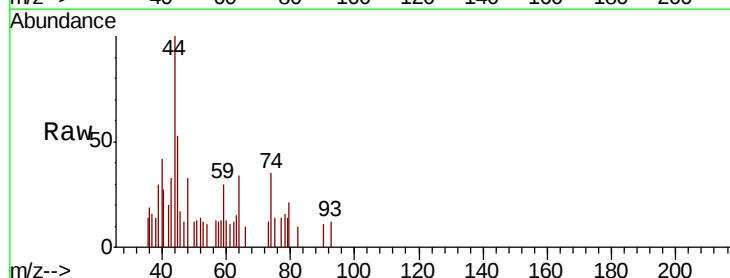

Abundance Ion 74.00 (73.70 to 74.70): VX0

Ion 45.00 (44.70 to 45.70): VX0

300


200


100

0

2.15 2.20 2.25

Time-->






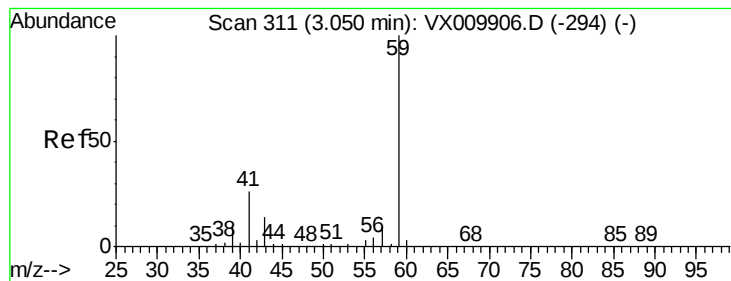


#11

Tert butyl alcohol
 Concen: 1.999 ug/l
 RT: 3.04 min Scan# 310
 Delta R.T. -0.01 min
 Lab File: VX009947.D
 Acq: 29 May 2019 18:00

Instrument :
 MSVOA_X
 ClientSampled :
 TP-3B-S




Tot Ion: 59 Resp: 1192
 Ion Ratio Lower Upper
 59 100
 57 9.5 8.2 12.2

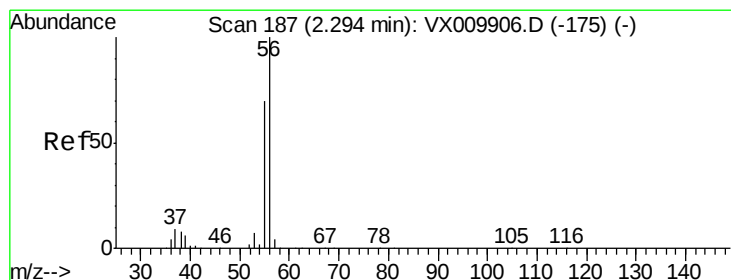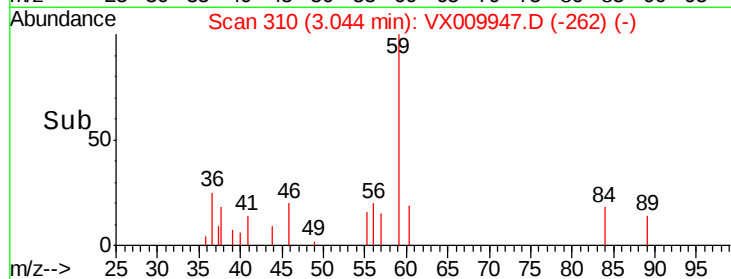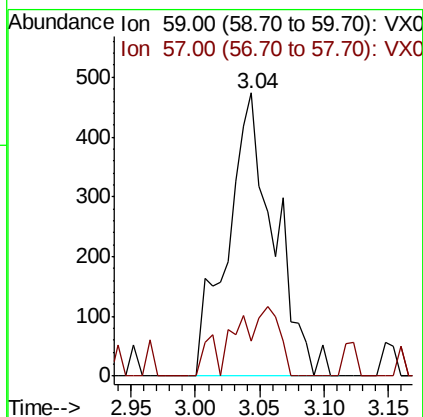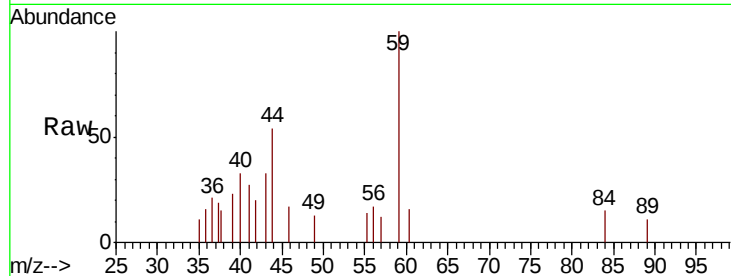


#13

Acrolein
 Concen: 21.641 ug/l
 RT: 2.29 min Scan# 186
 Delta R.T. -0.01 min
 Lab File: VX009947.D
 Acq: 29 May 2019 18:00

Tgt Ion: 56 Resp: 251
 Ion Ratio Lower Upper
 56 100
 55 78.1 57.0 85.4

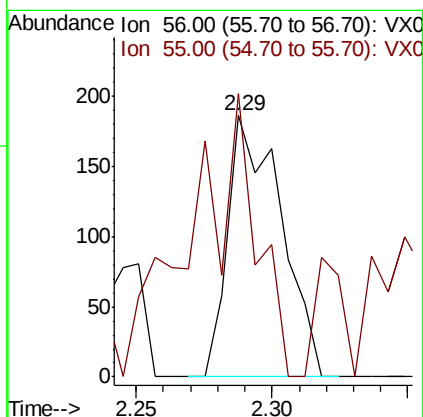

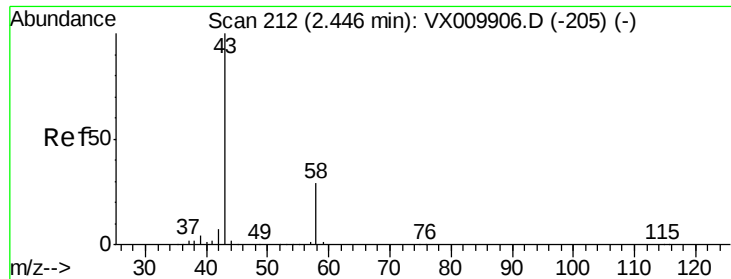

#16

Acetone

Concen: 23.674 ug/l

RT: 2.44 min Scan# 211

Delta R.T. -0.01 min

Lab File: VX009947.D

Acq: 29 May 2019 18:00

Instrument :

MSVOA_X

ClientSampleId :





TP-3B-S

Tot Ion: 43 Resp: 33149

Ion Ratio Lower Upper

43 100

58 26.8 23.2 34.8

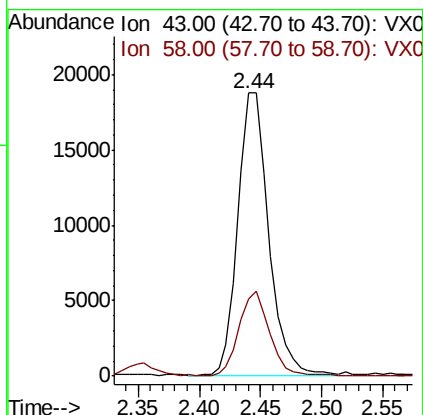

#17

Carbon Disulfide

Concen: 0.599 ug/l

RT: 2.57 min Scan# 233

Delta R.T. 0.01 min

Lab File: VX009947.D




Acq: 29 May 2019 18:00


Tgt Ion: 76 Resp: 1137

Ion Ratio Lower Upper

76 100

78 8.7 7.0 10.6


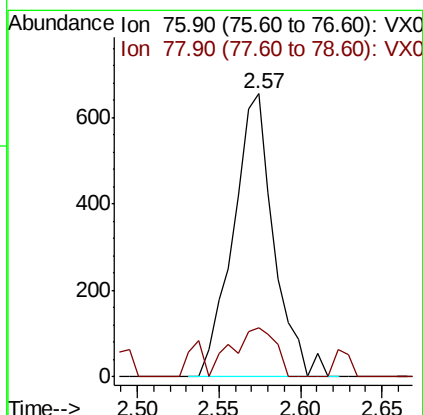




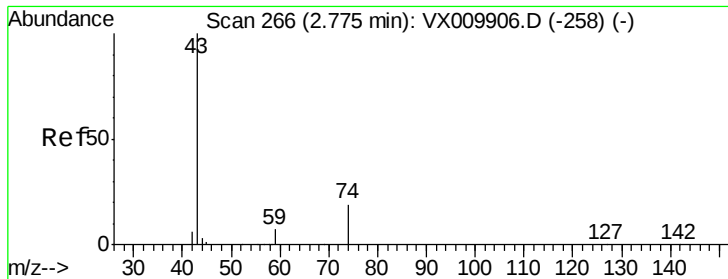

#18
Methvl Acetate
Concen: 1.203 ug/l
RT: 2.78 min Scan# 266
Delta R.T. -0.00 min
Lab File: VX009947.D
Acq: 29 May 2019 18:00




Instrument :
MSVOA_X
ClientSampleId :
TP-3B-S


Tot Ion: 43 Resp: 3919
Ion Ratio Lower Upper
43 100
74 24.0 15.8 23.6#

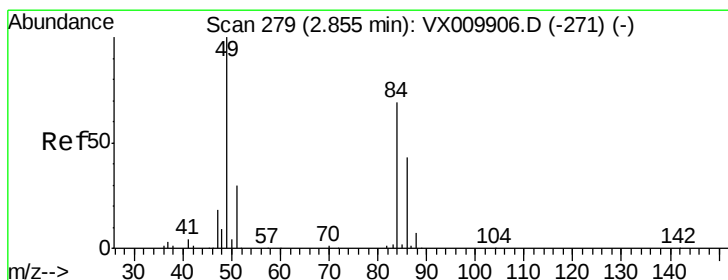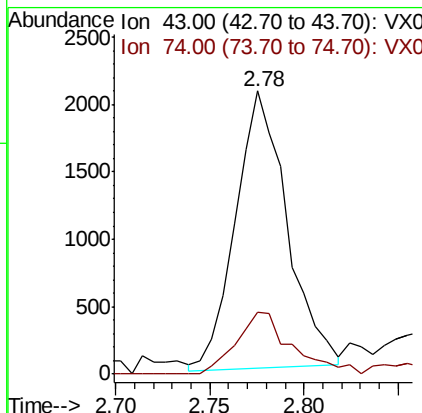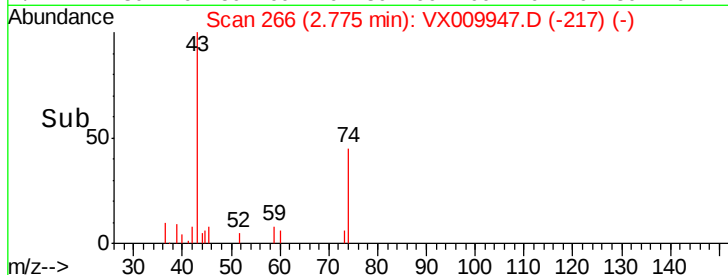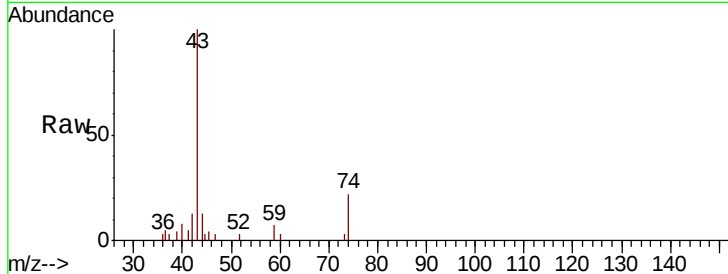

#20
Methylene Chloride
Concen: 38.325 ug/l
RT: 2.86 min Scan# 280
Delta R.T. 0.01 min
Lab File: VX009947.D
Acq: 29 May 2019 18:00

Tgt Ion: 84 Resp: 82179
Ion Ratio Lower Upper
84 100
49 144.9 115.8 173.6
51 43.1 34.4 51.6
86 62.9 49.7 74.5

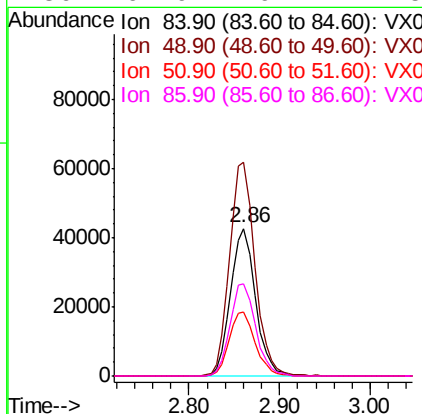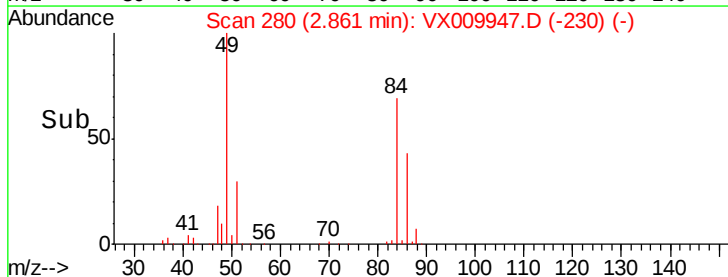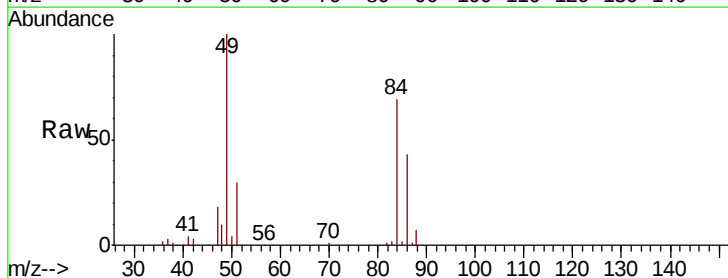

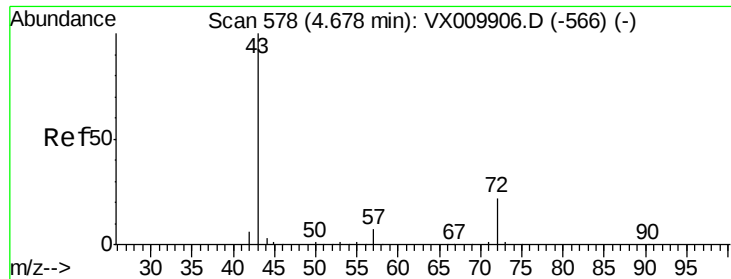

#25

2-Butanone

Concen: 2.536 ug/l

RT: 4.68 min Scan# 579

Delta R.T. 0.01 min

Lab File: VX009947.D

Acq: 29 May 2019 18:00

Instrument :

MSVOA_X

ClientSampleId :


TP-3B-S

Tot Ion: 43 Resp: 5532

Ion Ratio Lower Upper




43 100

72 24.6 17.5 26.3

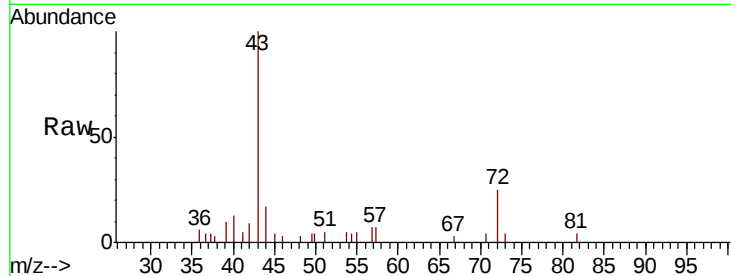

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 72.00 (71.70 to 72.70): VX0

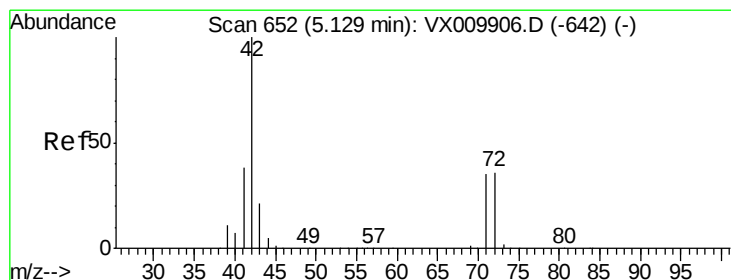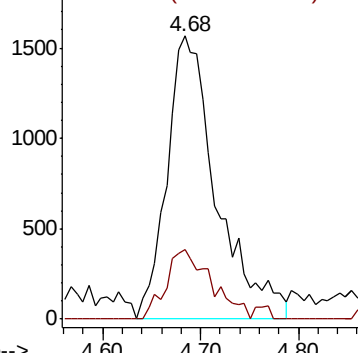

#29

Tetrahydrofuran

Concen: 1.093 ug/l

RT: 5.15 min Scan# 655

Delta R.T. 0.02 min

Lab File: VX009947.D

Acq: 29 May 2019 18:00


Tgt Ion: 42 Resp: 1529

Ion Ratio Lower Upper

42 100

72 34.3 29.2 43.8



71 42.6 27.6 41.4#




Abundance Ion 42.00 (41.70 to 42.70): VX0

Ion 72.00 (71.70 to 72.70): VX0

Ion 71.00 (70.70 to 71.70): VX0




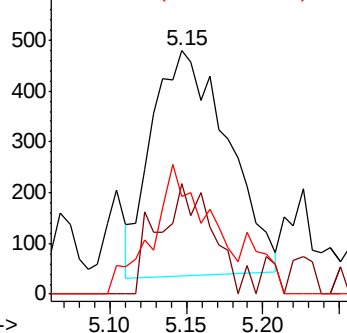




#30
Chloroform
Concen: 0.282 ug/l
RT: 5.21 min Scan# 666
Delta R.T. -0.00 min
Lab File: VX009947.D
Acq: 29 May 2019 18:00




Instrument :
MSVOA_X
ClientSampleId :
TP-3B-S


Tot Ion: 83 Resp: 990
Ion Ratio Lower Upper
83 100
85 63.0 52.6 78.8

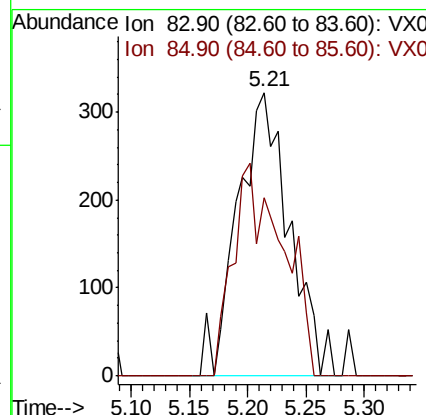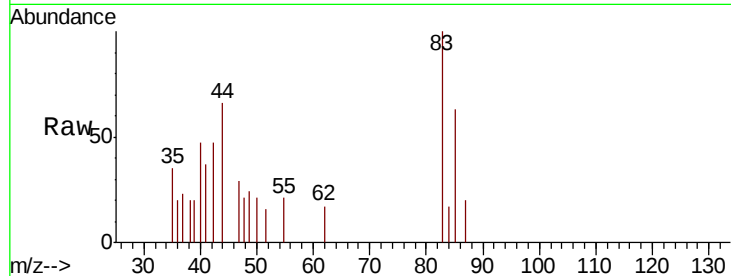

#31
Cyclohexane
Concen: 1.071 ug/l
RT: 5.67 min Scan# 740
Delta R.T. 0.09 min
Lab File: VX009947.D
Acq: 29 May 2019 18:00

Tgt Ion: 56 Resp: 3950
Ion Ratio Lower Upper
56 100
69 153.5 21.6 32.4#
84 120.2 56.8 85.2#



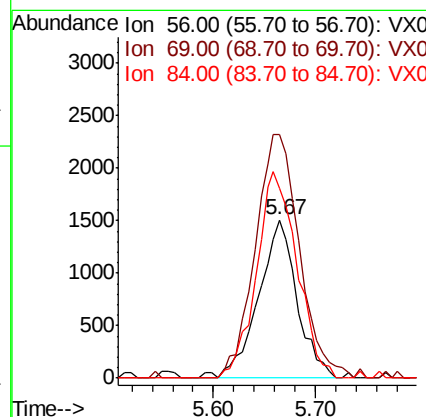
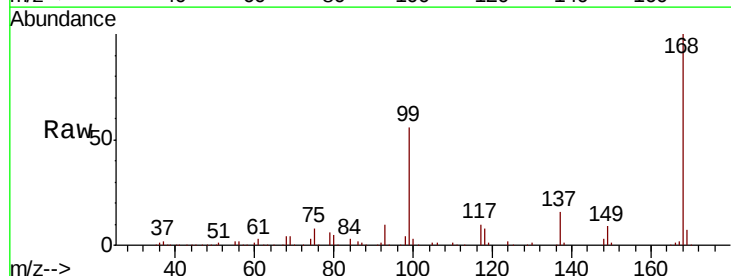


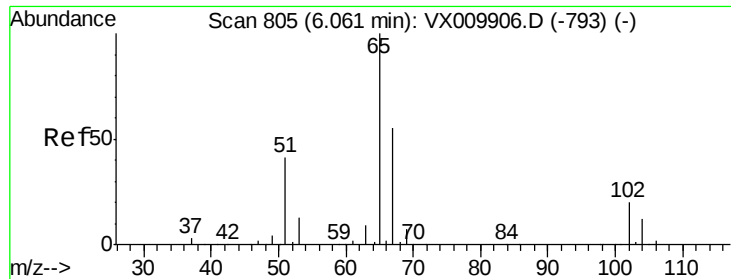

#33
 1,2-Dichloroethane-d4
 Concen: 49.253 ug/l
 RT: 6.06 min Scan# 805
 Delta R.T. -0.00 min
 Lab File: VX009947.D
 Acq: 29 May 2019 18:00




Instrument :
 MSVOA_X
 ClientSampled :
 TP-3B-S


Tot Ion: 65 Resp: 119365
 Ion Ratio Lower Upper
 65 100
 67 52.7 0.0 108.4

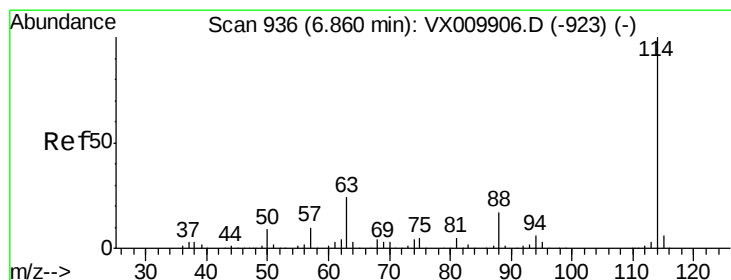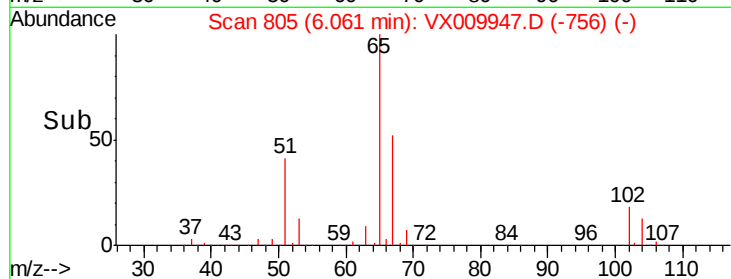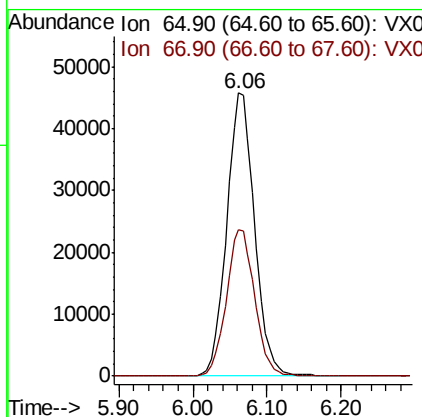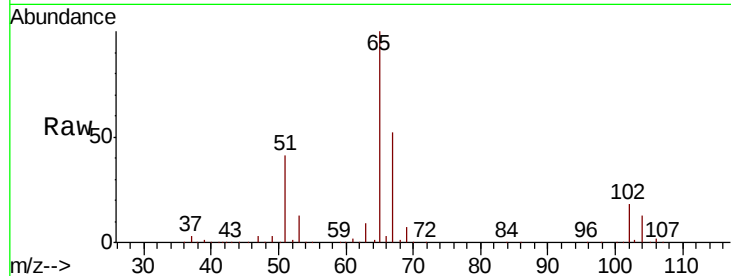

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.86 min Scan# 936
 Delta R.T. -0.00 min
 Lab File: VX009947.D
 Acq: 29 May 2019 18:00

Tgt Ion: 114 Resp: 280388
 Ion Ratio Lower Upper
 114 100
 63 23.5 0.0 47.4
 88 16.8 0.0 33.0


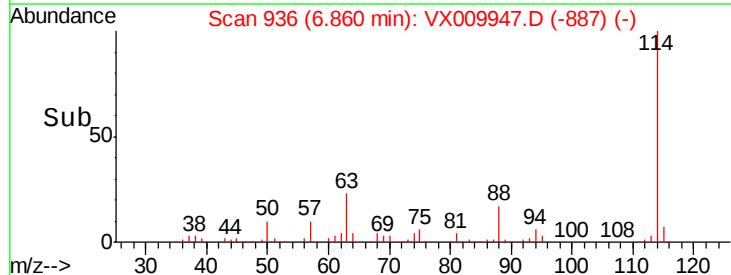
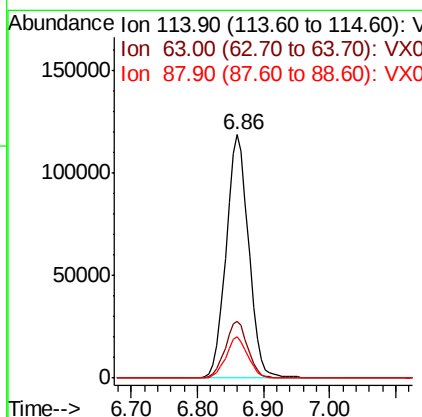



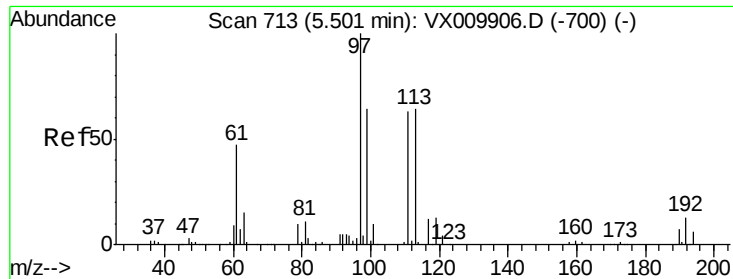

#35
Dibromofluoromethane
Concen: 48.679 ug/l
RT: 5.50 min Scan# 713
Delta R.T. -0.00 min
Lab File: VX009947.D
Acq: 29 May 2019 18:00




Instrument :
MSVOA_X
ClientSampleId :
TP-3B-S


Tot Ion:113 Resp: 85812
Ion Ratio Lower Upper
113 100
111 102.9 82.2 123.2
192 22.1 17.1 25.7

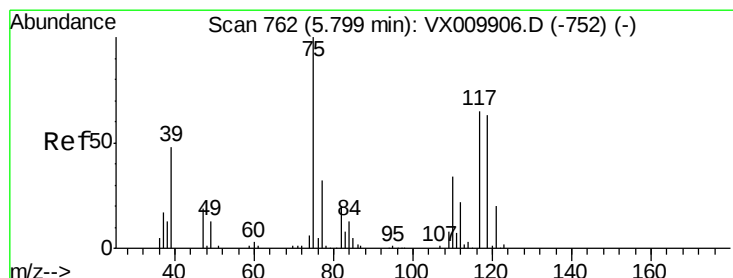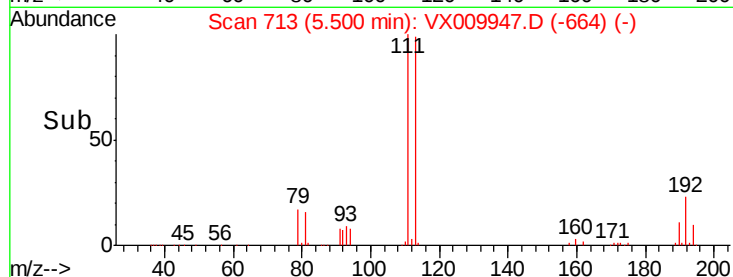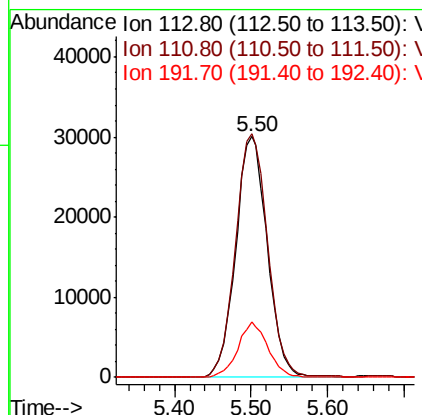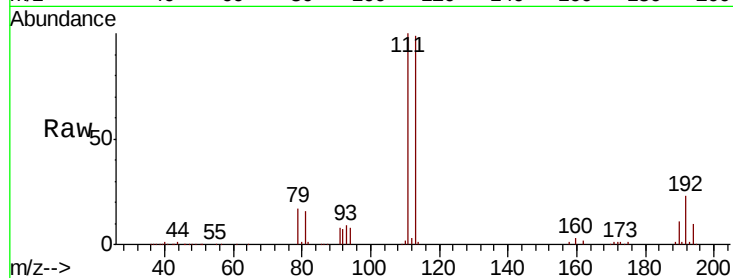

#36
1,1-Dichloropropene
Concen: 4.743 ug/l
RT: 5.67 min Scan# 740
Delta R.T. -0.13 min
Lab File: VX009947.D
Acq: 29 May 2019 18:00

Tgt Ion: 75 Resp: 13494
Ion Ratio Lower Upper
75 100
110 8.7 16.7 50.1#
77 0.0 25.0 37.4#

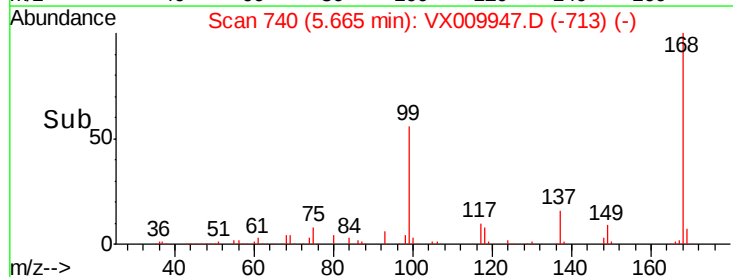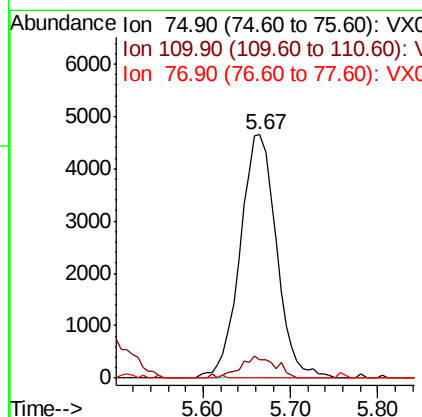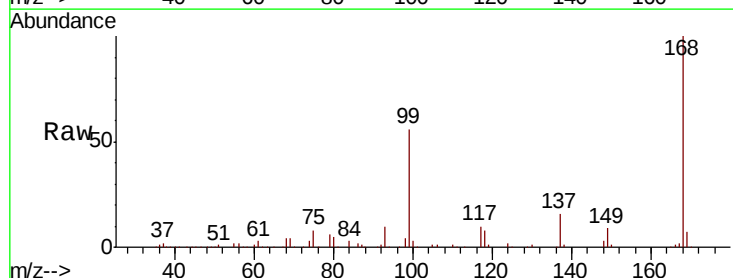

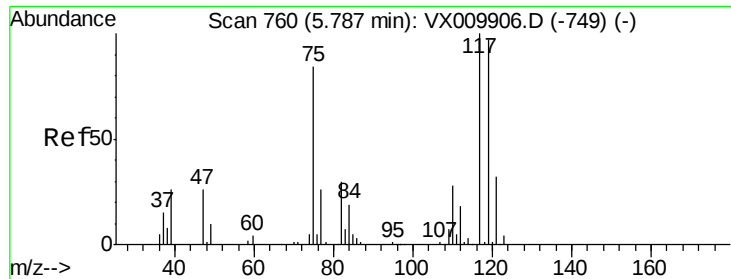

#38

Carbon Tetrachloride

Concen: 6.618 ug/l

RT: 5.67 min Scan# 740

Delta R.T. -0.12 min

Lab File: VX009947.D

Acq: 29 May 2019 18:00

Instrument :

MSVOA_X

ClientSampleId :

TP-3B-S


Tot Ion:117 Resp: 16269

Ion Ratio Lower Upper

117 100

119 6.1 77.3 115.9#




121 0.0 25.4 38.0#

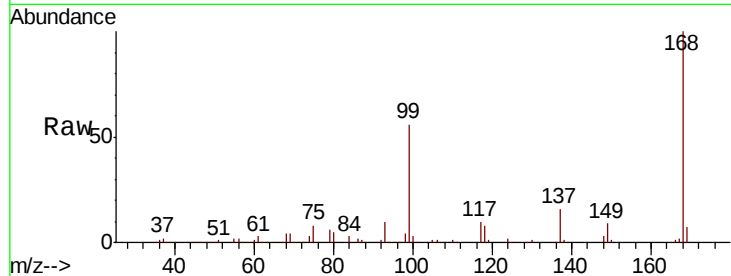

Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

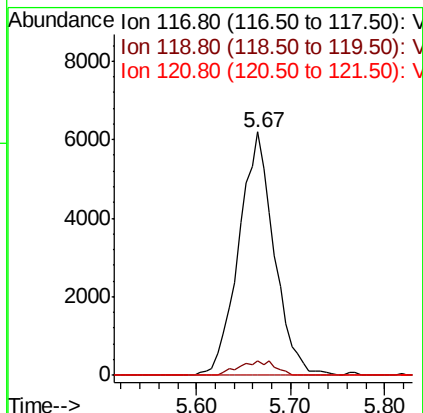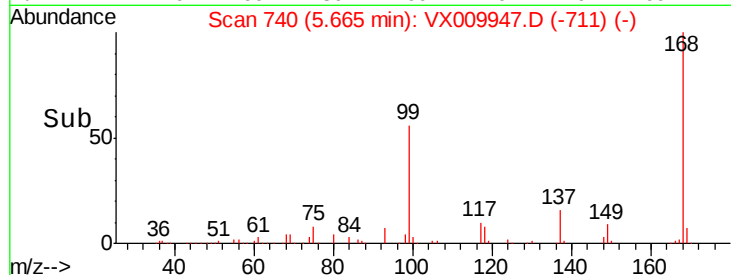

#43

Isopropyl Acetate

Concen: 1.700 ug/l

RT: 6.45 min Scan# 868

Delta R.T. -0.00 min

Lab File: VX009947.D

Acq: 29 May 2019 18:00


Tgt Ion: 43 Resp: 10872

Ion Ratio Lower Upper

43 100

61 21.0 14.6 21.8



87 10.7 8.7 13.1




Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 61.00 (60.70 to 61.70): VX0

Ion 87.00 (86.70 to 87.70): VX0

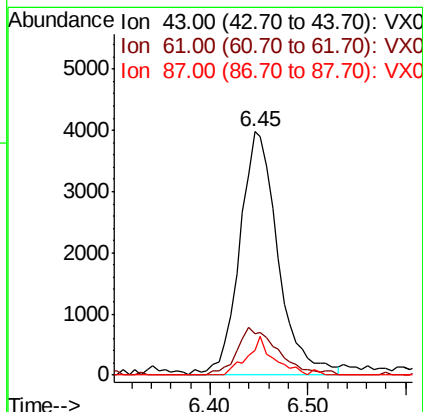



#48

Methvl methacrylate

Concen: 2.272 ug/l

RT: 7.68 min Scan# 1070

Delta R.T. -0.09 min

Lab File: VX009947.D

Acq: 29 May 2019 18:00

Instrument :

MSVOA_X

ClientSampleId :

TP-3B-S


Tot Ion: 41 Resp: 7193

Ion Ratio Lower Upper

41 100

69 0.0 56.4 84.6#




39 0.0 40.6 60.8#

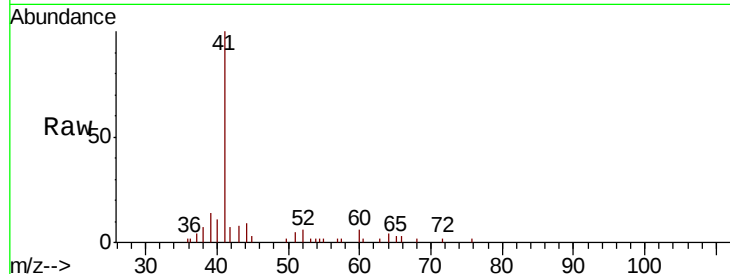

Abundance Ion 41.00 (40.70 to 41.70): VX0

Ion 69.00 (68.70 to 69.70): VX0

Ion 39.00 (38.70 to 39.70): VX0

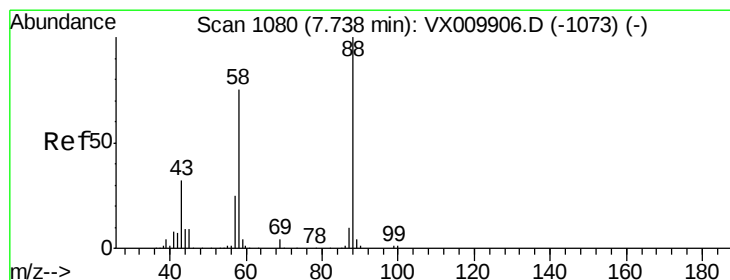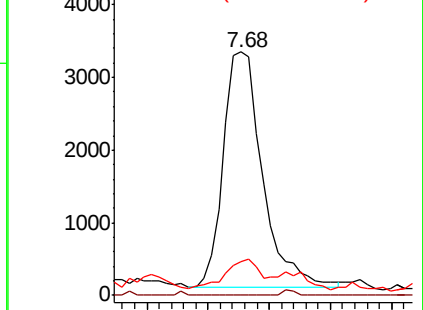

#49

1,4-Dioxane

Concen: 0.391 ug/l

RT: 7.84 min Scan# 1097

Delta R.T. 0.10 min

Lab File: VX009947.D

Acq: 29 May 2019 18:00


Tgt Ion: 88 Resp: 23

Ion Ratio Lower Upper

88 100

43 0.0 30.2 45.4#



58 0.0 64.0 96.0#

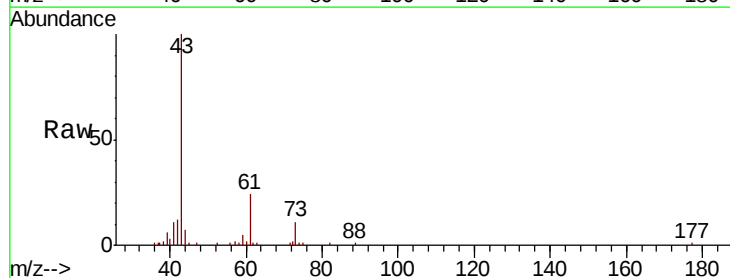


Abundance Ion 88.00 (87.70 to 88.70): VX0

Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

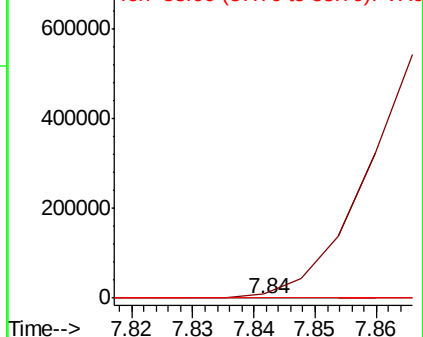

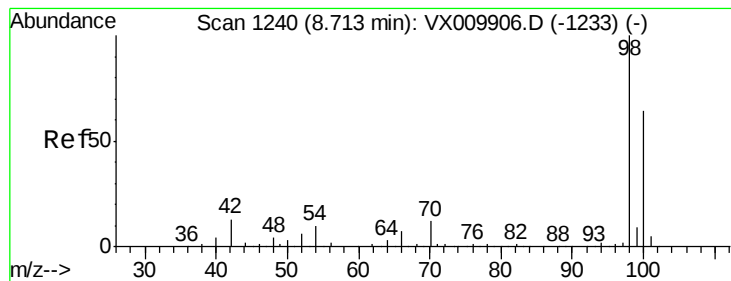

#50

Toluene-d8

Concen: 49.864 ug/l

RT: 8.71 min Scan# 1240

Delta R.T. -0.00 min

Lab File: VX009947.D

Acq: 29 May 2019 18:00

Instrument :

MSVOA_X

ClientSampled :


TP-3B-S

Tot Ion: 98 Resp: 356943

Ion Ratio Lower Upper




98 100

100 64.2 51.5 77.3



Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): VX

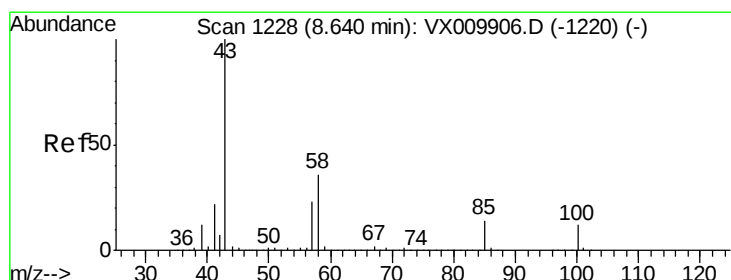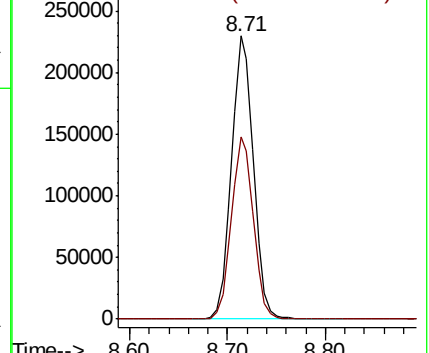

#51

4-Methyl-2-Pentanone

Concen: 18.259 ug/l

RT: 8.61 min Scan# 1223

Delta R.T. -0.03 min

Lab File: VX009947.D


Acq: 29 May 2019 18:00

Tgt Ion: 43 Resp: 75969

Ion Ratio Lower Upper



43 100


58 8.2 28.8 43.2#



Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

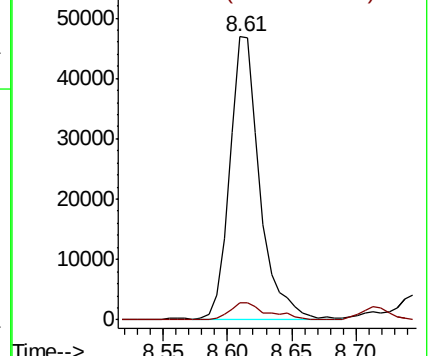







#54

cis-1,3-Dichloropropene
 Concen: 8.693 ug/l
 RT: 8.62 min Scan# 1224
 Delta R.T. 0.18 min
 Lab File: VX009947.D
 Acq: 29 May 2019 18:00

Instrument :
 MSVOA_X
 ClientSampled :
 TP-3B-S




Tot Ion: 75 Resp: 30887
 Ion Ratio Lower Upper
 75 100
 77 0.9 24.8 37.2#
 39 31.4 43.4 65.0#

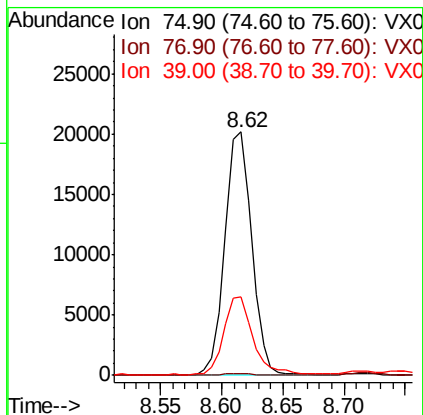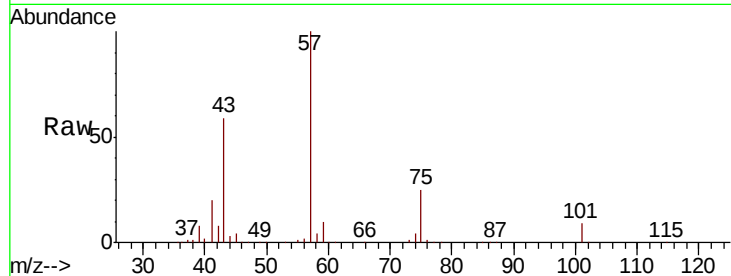


#57

1,3-Dichloropropane
 Concen: 2.051 ug/l
 RT: 9.54 min Scan# 1376
 Delta R.T. 0.17 min
 Lab File: VX009947.D
 Acq: 29 May 2019 18:00

Tgt Ion: 76 Resp: 7595
 Ion Ratio Lower Upper
 76 100
 78 0.3 25.4 38.0#


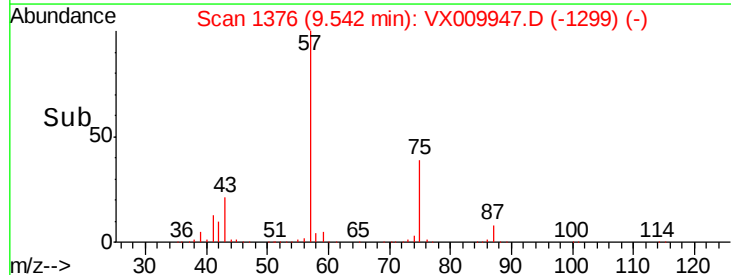
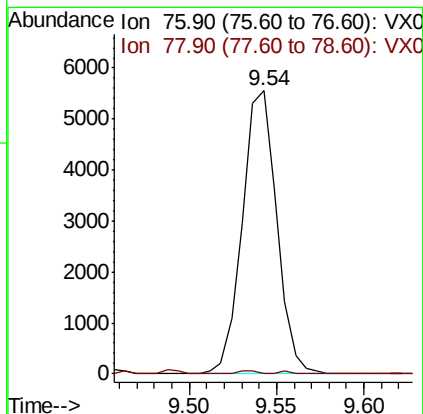



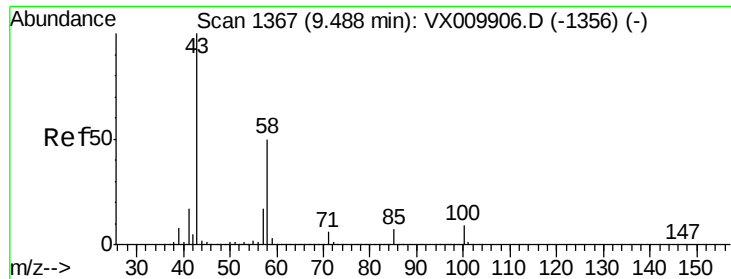

#59
2-Hexanone
Concen: 3.162 ug/l
RT: 9.44 min Scan# 1359
Delta R.T. -0.05 min
Lab File: VX009947.D
Acq: 29 May 2019 18:00




Instrument :
MSVOA_X
ClientSampleId :
TP-3B-S


Tot Ion: 43 Resp: 10128
Ion Ratio Lower Upper
43 100
58 0.0 25.1 75.3#

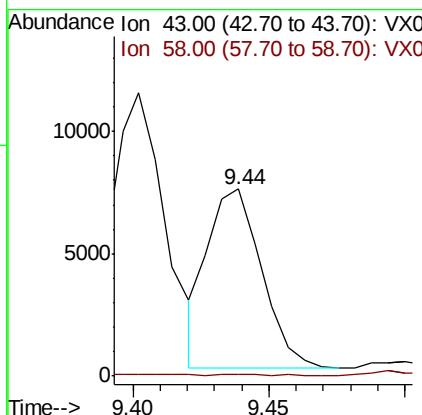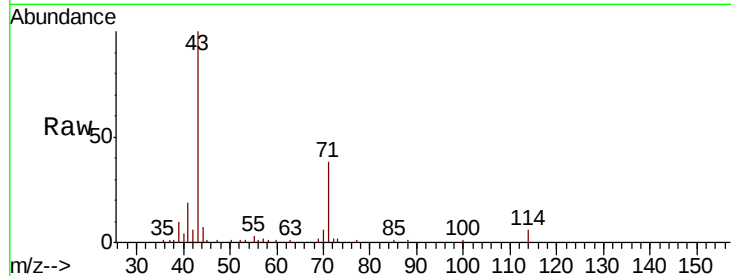

#62
4-Bromofluorobenzene
Concen: 46.118 ug/l
RT: 11.13 min Scan# 1637
Delta R.T. -0.00 min
Lab File: VX009947.D
Acq: 29 May 2019 18:00

Tgt Ion: 95 Resp: 118578
Ion Ratio Lower Upper
95 100
174 81.8 0.0 160.4
176 79.1 0.0 154.6

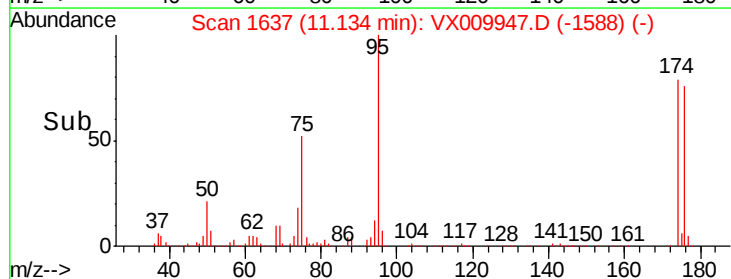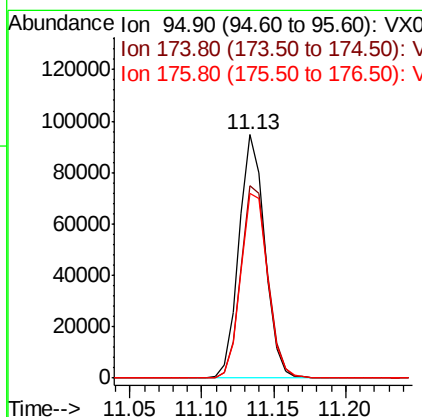


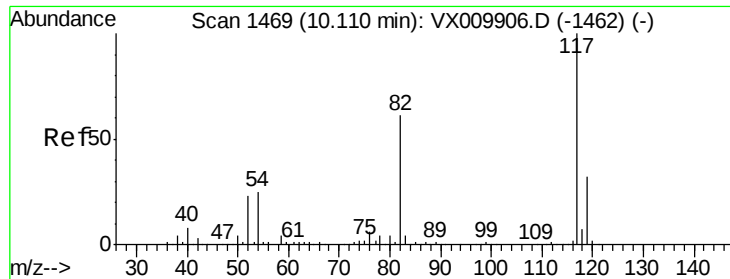




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.11 min Scan# 1469
Delta R.T. -0.00 min
Lab File: VX009947.D
Acq: 29 May 2019 18:00

Instrument :
MSVOA_X
ClientSampleId :
TP-3B-S

Tot Ion:117 Resp: 250946
Ion Ratio Lower Upper
117 100
82 59.8 49.2 73.8
119 32.2 25.2 37.8

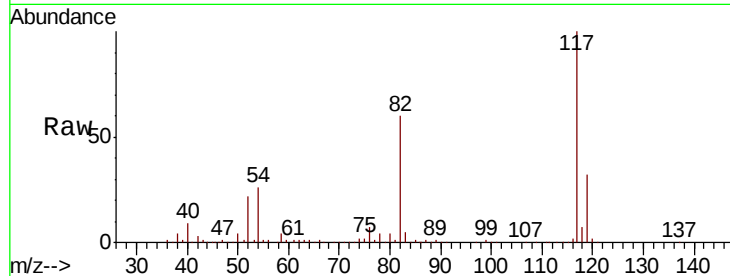


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): VX0
Ion 118.90 (118.60 to 119.60): V

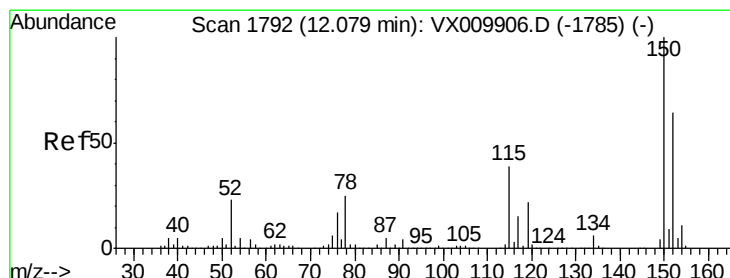
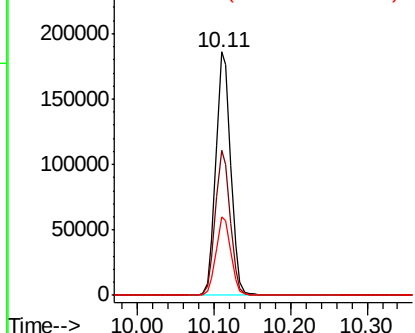



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.08 min Scan# 1792
Delta R.T. -0.00 min
Lab File: VX009947.D
Acq: 29 May 2019 18:00

Tgt Ion:152 Resp: 108102
Ion Ratio Lower Upper
152 100
115 58.1 41.4 124.2
150 154.5 0.0 345.2

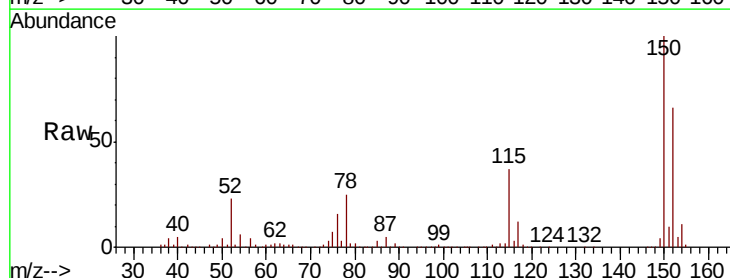

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V




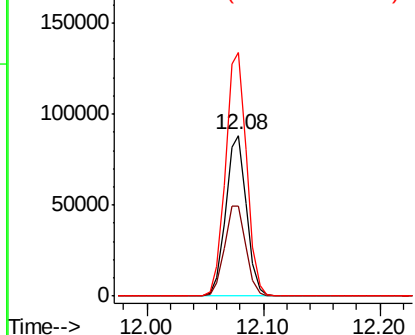


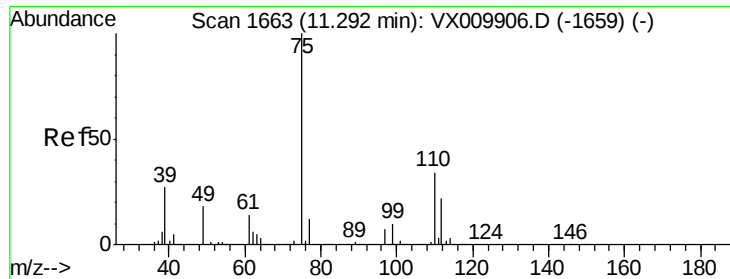

#76
 1,2,3-Trichloropropane
 Concen: 23.922 ug/l
 RT: 11.13 min Scan# 1637
 Delta R.T. -0.16 min
 Lab File: VX009947.D
 Acq: 29 May 2019 18:00




Instrument :
 MSVOA_X
 ClientSampleId :
 TP-3B-S


Tot Ion: 75 Resp: 61841
 Ion Ratio Lower Upper
 75 100
 77 1.4 22.1 66.1#

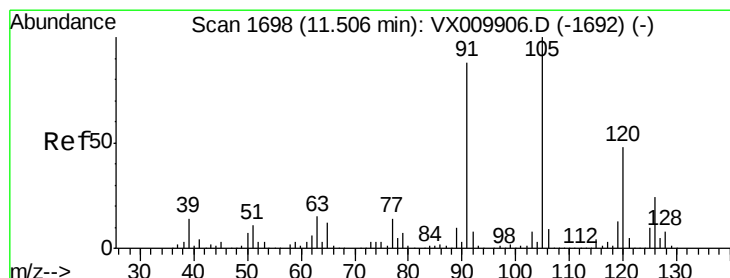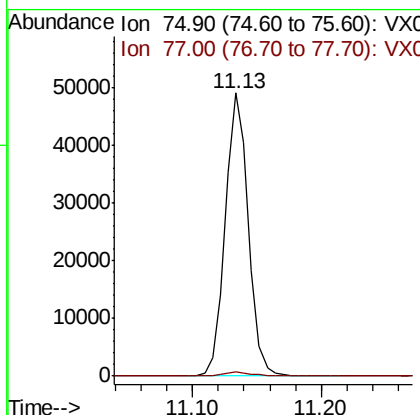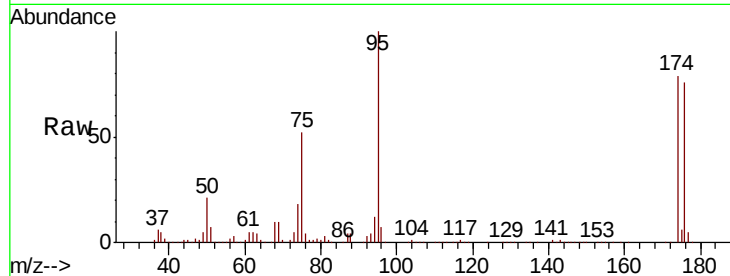

#80
 1,3,5-Trimethylbenzene
 Concen: 0.332 ug/l
 RT: 11.51 min Scan# 1698
 Delta R.T. -0.00 min
 Lab File: VX009947.D
 Acq: 29 May 2019 18:00

Tgt Ion: 105 Resp: 2231
 Ion Ratio Lower Upper
 105 100
 120 53.7 24.1 72.3

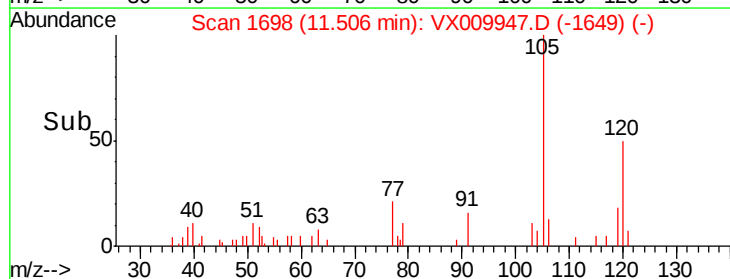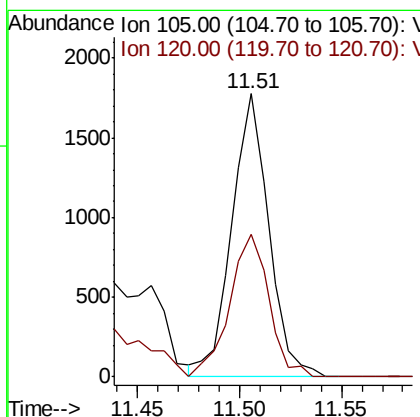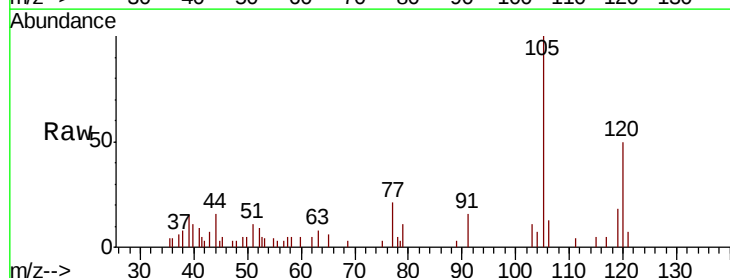

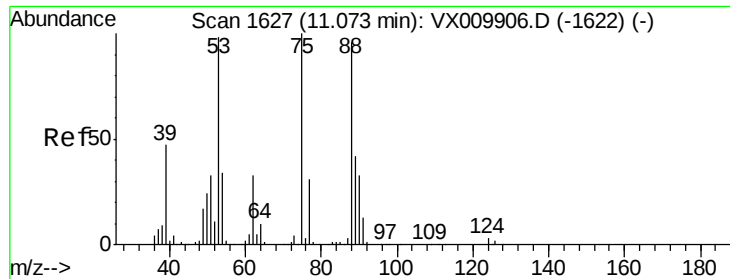

#81

trans-1,4-Dichloro-2-butene

Concen: 59.188 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. 0.06 min

Lab File: VX009947.D

Acq: 29 May 2019 18:00

Instrument :

MSVOA_X

ClientSampleId :

TP-3B-S


Tot Ion: 75 Resp: 61841

Ion Ratio Lower Upper




75 100

53 0.3 79.8 119.6#

89 0.0 34.2 51.4#

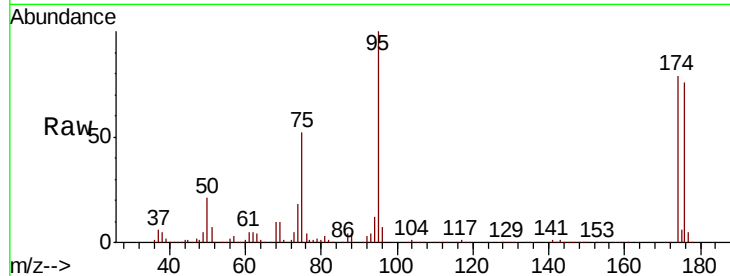

Abundance Ion 74.90 (74.60 to 75.60): VX0
Ion 53.00 (52.70 to 53.70): VX0
Ion 88.90 (88.60 to 89.60): VX0

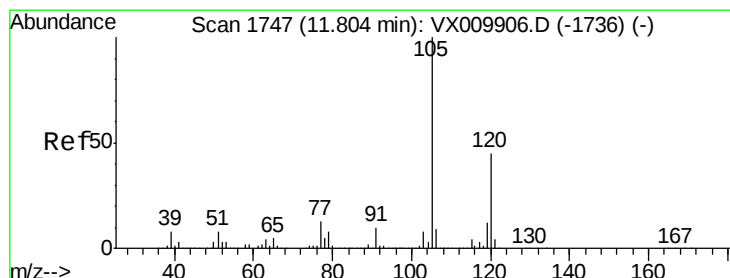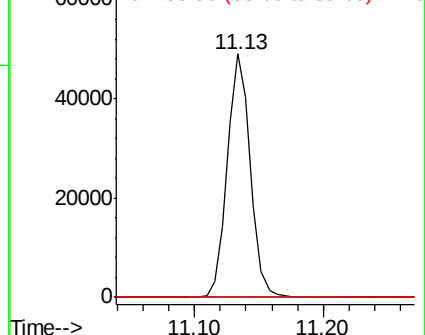

#84

1,2,4-Trimethylbenzene

Concen: 0.403 ug/l

RT: 11.80 min Scan# 1747

Delta R.T. -0.00 min

Lab File: VX009947.D


Acq: 29 May 2019 18:00

Tgt Ion: 105 Resp: 2752



Ion Ratio Lower Upper


105 100

120 45.2 22.1 66.1

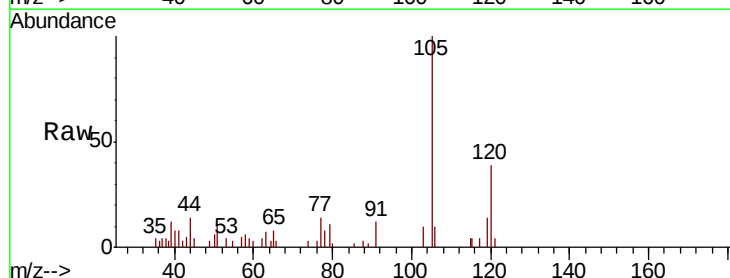

Abundance Ion 105.00 (104.70 to 105.70): V
Ion 120.00 (119.70 to 120.70): V

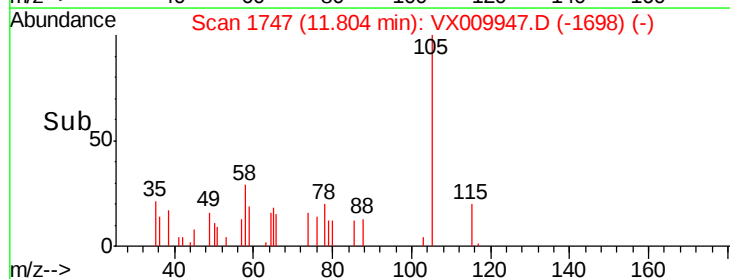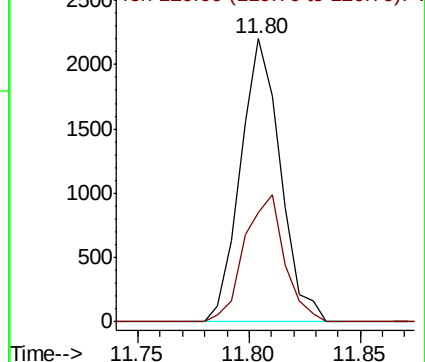

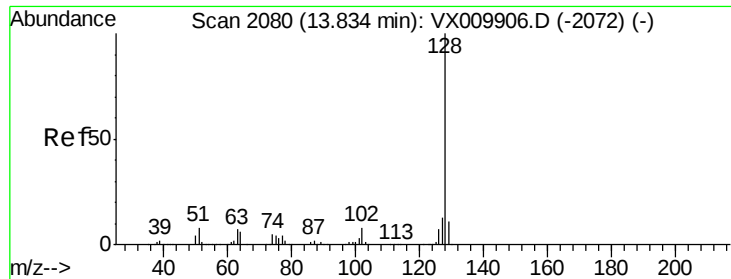

#95
Naphthalene
Concen: 1.167 ug/l
RT: 13.83 min Scan# 2080
Delta R.T. -0.00 min
Lab File: VX009947.D
Acq: 29 May 2019 18:00

Instrument :
MSVOA_X
ClientSampleId :
TP-3B-S

Tot Ion	Ratio	Lower	Upper
128	100		
127	13.4	10.6	16.0
129	11.7	8.8	13.2

