

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\WX052919\
 Data File : VX009948.D
 Acq On : 29 May 2019 18:23
 Operator : JC/SP
 Sample : K3074-10
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TP-3B-D

Quant Time: May 30 01:17:09 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X052819W.M
 Quant Title : SW846 8260
 QLast Update : Wed May 29 04:00:56 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.67	168	168928	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.86	114	275421	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.11	117	251021	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.08	152	110649	50.00	ug/l	0.00

System Monitoring Compounds

33) 1,2-Dichloroethane-d4	6.06	65	118757	49.77	ug/l	0.00
Spiked Amount	50.000		Recovery	=	99.54%	
35) Dibromofluoromethane	5.50	113	85629	49.45	ug/l	0.00
Spiked Amount	50.000		Recovery	=	98.90%	
50) Toluene-d8	8.71	98	355362	50.54	ug/l	0.00
Spiked Amount	50.000		Recovery	=	101.08%	
62) 4-Bromofluorobenzene	11.13	95	119283	47.23	ug/l	0.00
Spiked Amount	50.000		Recovery	=	94.46%	

Target Compounds

						Qvalue
8) Diethyl Ether	2.19	74	444	0.342	ug/l	80
11) Tert butyl alcohol	3.05	59	979	1.667	ug/l	96
13) Acrolein	2.29	56	197	21.530	ug/l #	73
16) Acetone	2.45	43	31529	22.868	ug/l	99
17) Carbon Disulfide	2.57	76	365	0.455	ug/l #	76
18) Methyl Acetate	2.78	43	5719	1.783	ug/l	96
20) Methylene Chloride	2.85	84	83076	39.348	ug/l	98
25) 2-Butanone	4.68	43	4463	2.078	ug/l #	79
29) Tetrahydrofuran	5.15	42	1687	1.225	ug/l #	52
30) Chloroform	5.21	83	924	0.267	ug/l	100
31) Cyclohexane	5.66	56	4101	1.129	ug/l #	1
36) 1,1-Dichloropropene	5.67	75	13585	4.861	ug/l #	50
37) Ethyl Acetate	4.68	43	4358	1.119	ug/l #	73
38) Carbon Tetrachloride	5.66	117	16135	6.682	ug/l #	16
43) Isopropyl Acetate	6.45	43	10777	1.715	ug/l	95
48) Methyl methacrylate	7.68	41	6938	2.231	ug/l #	20
49) 1,4-Dioxane	7.62	88	19	0.328	ug/l #	18
51) 4-Methyl-2-Pentanone	8.62	43	74791	18.300	ug/l #	53
54) cis-1,3-Dichloropropene	8.62	75	29746	8.522	ug/l #	58
57) 1,3-Dichloropropane	9.54	76	7186	1.975	ug/l #	45
59) 2-Hexanone	9.44	43	10046	3.193	ug/l #	27
76) 1,2,3-Trichloropropane	11.13	75	62624	23.668	ug/l #	34
80) 1,3,5-Trimethylbenzene	11.51	105	2228	0.324	ug/l	92
81) trans-1,4-Dichloro-2-buten	11.13	75	62624	58.558	ug/l #	10
84) 1,2,4-Trimethylbenzene	11.80	105	1776	0.254	ug/l	94
95) Naphthalene	13.83	128	3361	0.414	ug/l	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.67 min Scan# 740

Delta R.T. 0.00 min

Lab File: VX009948.D

Acq: 29 May 2019 18:23

Instrument :

MSVOA_X

ClientSampleId :


TP-3B-D

Tot Ion:168 Resp: 168928

Ion Ratio Lower Upper

168 100

99 56.6 43.0 64.6

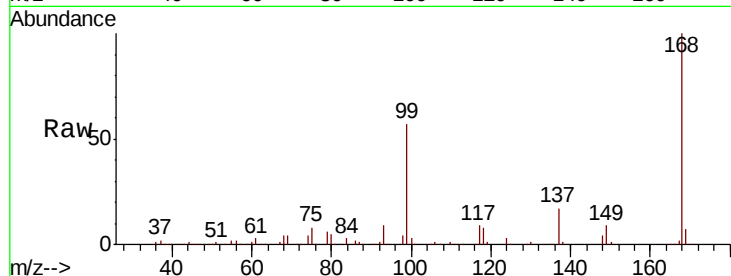

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.67



60000

40000

20000

0

Time--> 5.50 5.60 5.70 5.80



#8

Diethyl Ether

Concen: 0.342 ug/l

RT: 2.19 min Scan# 170

Delta R.T. 0.00 min

Lab File: VX009948.D


Acq: 29 May 2019 18:23

Tgt Ion: 74 Resp: 444

Ion Ratio Lower Upper

74 100

45 91.0 56.1 168.3



Abundance Ion 74.00 (73.70 to 74.70): VX0

Ion 45.00 (44.70 to 45.70): VX0

2.19

400


300


200

100

0

Time--> 2.15 2.20






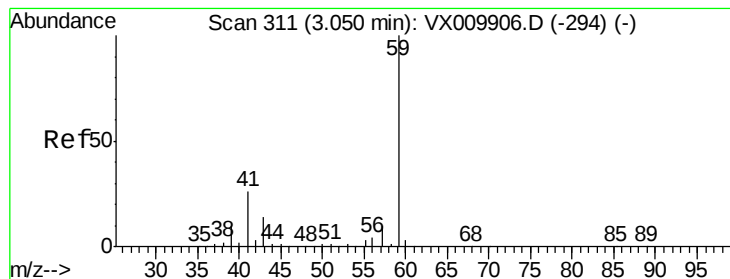


#11

Tert butyl alcohol
 Concen: 1.667 ug/l
 RT: 3.05 min Scan# 311
 Delta R.T. 0.00 min
 Lab File: VX009948.D
 Acq: 29 May 2019 18:23

Instrument :
 MSVOA_X
 ClientSampleId :
 TP-3B-D




Tot Ion: 59 Resp: 979
 Ion Ratio Lower Upper
 59 100
 57 8.6 8.2 12.2

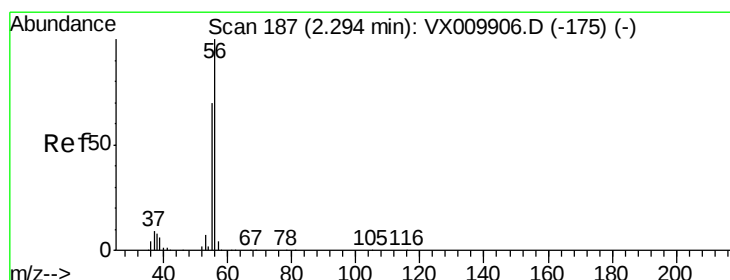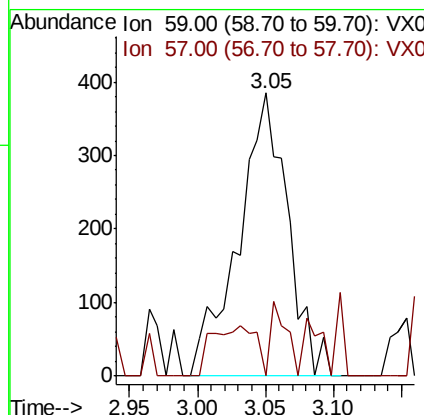


#13

Acrolein
 Concen: 21.530 ug/l
 RT: 2.29 min Scan# 187
 Delta R.T. 0.00 min
 Lab File: VX009948.D
 Acq: 29 May 2019 18:23

Tgt Ion: 56 Resp: 197
 Ion Ratio Lower Upper
 56 100
 55 48.7 57.0 85.4#

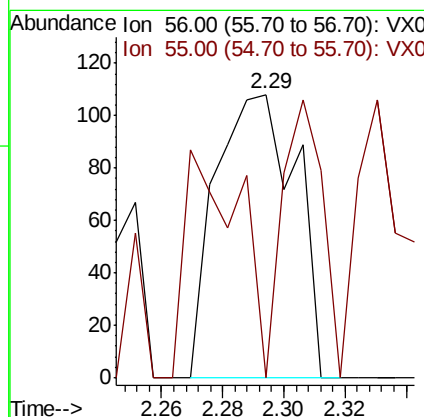

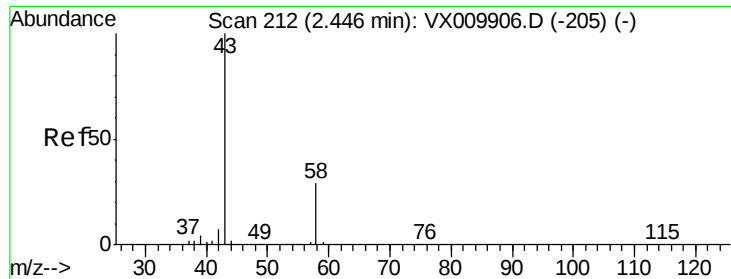

#16

Acetone

Concen: 22.868 ug/l

RT: 2.45 min Scan# 212

Delta R.T. 0.00 min

Lab File: VX009948.D

Acq: 29 May 2019 18:23

Instrument :

MSVOA_X

ClientSampled :


TP-3B-D

Tot Ion: 43 Resp: 31529




Ion Ratio Lower Upper

43 100

58 28.7 23.2 34.8



Abundance Ion 43.00 (42.70 to 43.70): VX0

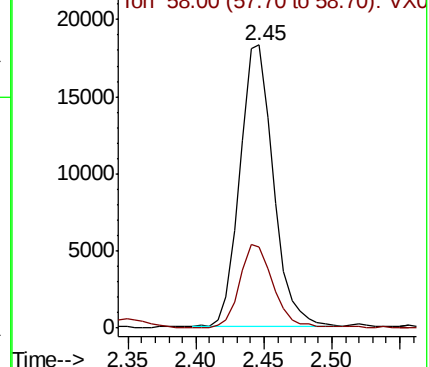

#17

Carbon Disulfide

Concen: 0.455 ug/l

RT: 2.57 min Scan# 232

Delta R.T. 0.00 min

Lab File: VX009948.D


Acq: 29 May 2019 18:23

Tgt Ion: 76 Resp: 365



Ion Ratio Lower Upper


76 100

78 0.0 7.0 10.6#



Abundance Ion 75.90 (75.60 to 76.60): VX0



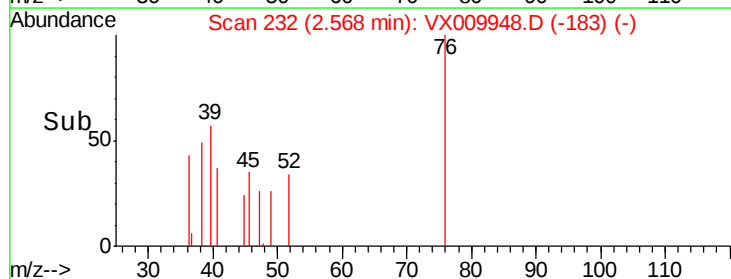
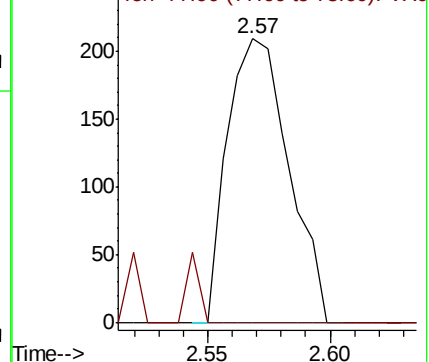


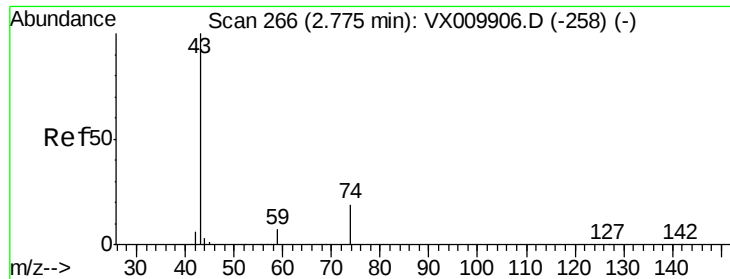

#18
Methyl Acetate
Concen: 1.783 ug/l
RT: 2.78 min Scan# 266
Delta R.T. 0.00 min
Lab File: VX009948.D
Acq: 29 May 2019 18:23




Instrument :
MSVOA_X
ClientSampleId :
TP-3B-D


Tot Ion: 43 Resp: 5719
Ion Ratio Lower Upper
43 100
74 21.4 15.8 23.6

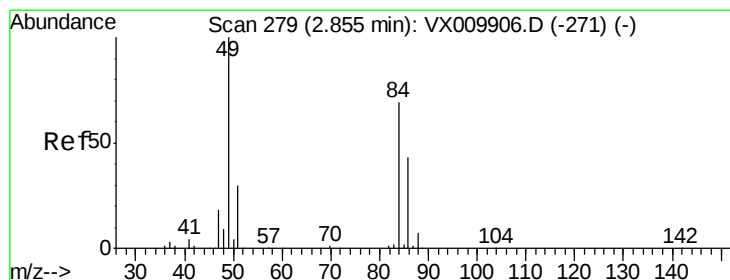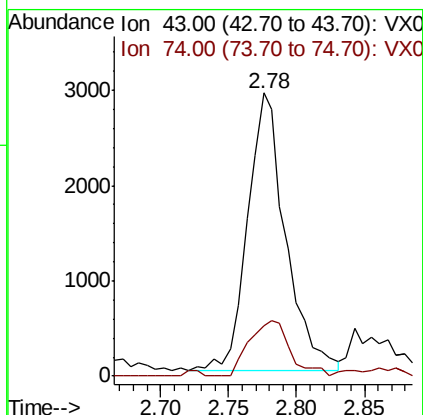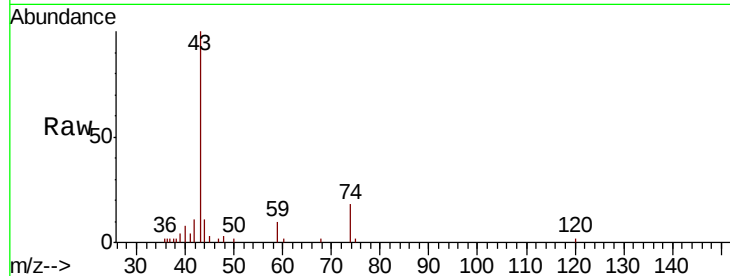

#20
Methylene Chloride
Concen: 39.348 ug/l
RT: 2.85 min Scan# 279
Delta R.T. 0.00 min
Lab File: VX009948.D
Acq: 29 May 2019 18:23

Tgt Ion: 84 Resp: 83076
Ion Ratio Lower Upper
84 100
49 142.2 115.8 173.6
51 43.7 34.4 51.6
86 63.7 49.7 74.5

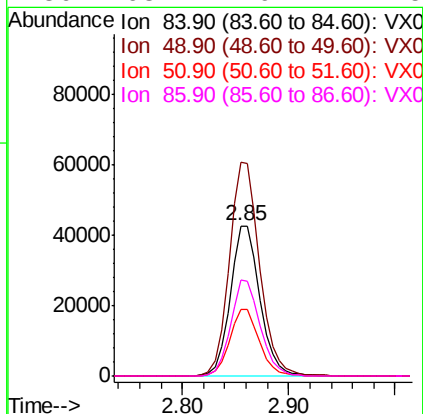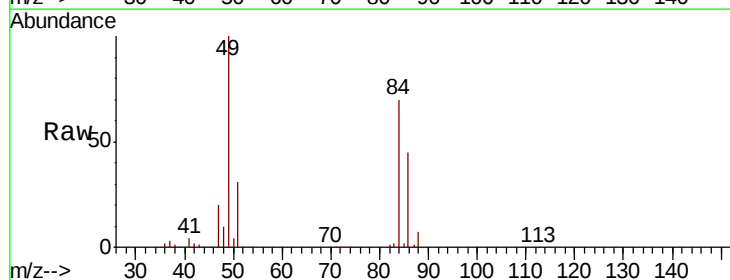

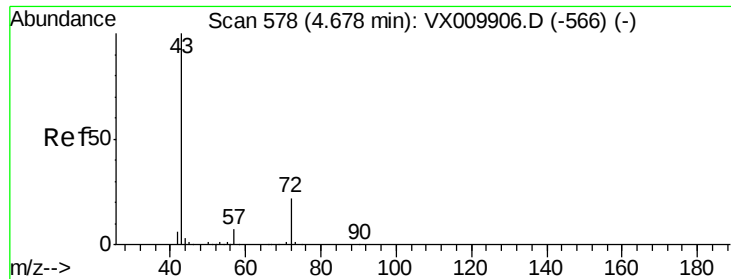

#25

2-Butanone

Concen: 2.078 ug/l

RT: 4.68 min Scan# 579

Delta R.T. 0.01 min

Lab File: VX009948.D

Acq: 29 May 2019 18:23

Instrument :

MSVOA_X

ClientSampleId :


TP-3B-D

Tot Ion: 43 Resp: 4463

Ion Ratio Lower Upper




43 100

72 31.7 17.5 26.3#

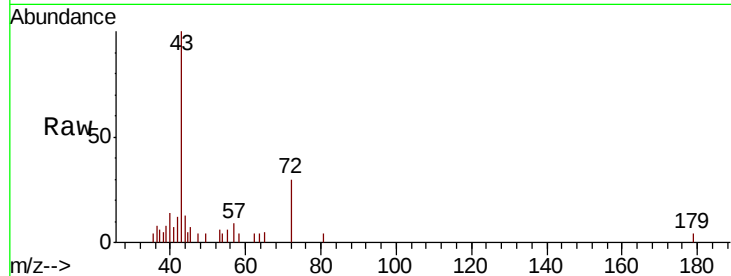

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 72.00 (71.70 to 72.70): VX0

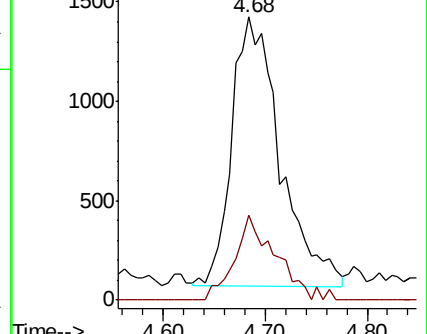

#29

Tetrahydrofuran

Concen: 1.225 ug/l

RT: 5.15 min Scan# 655

Delta R.T. 0.02 min

Lab File: VX009948.D

Acq: 29 May 2019 18:23


Tgt Ion: 42 Resp: 1687

Ion Ratio Lower Upper

42 100

72 0.0 29.2 43.8#



71 15.2 27.6 41.4#




Abundance Ion 42.00 (41.70 to 42.70): VX0

Ion 72.00 (71.70 to 72.70): VX0

Ion 71.00 (70.70 to 71.70): VX0




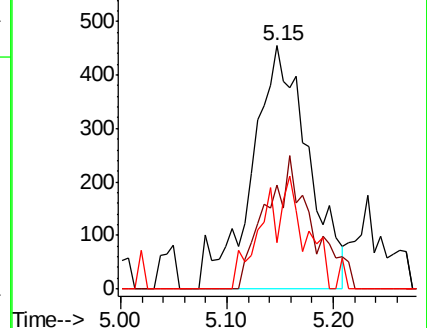




#30
Chloroform
Concen: 0.267 ug/l
RT: 5.21 min Scan# 665
Delta R.T. -0.01 min
Lab File: VX009948.D
Acq: 29 May 2019 18:23




Instrument :
MSVOA_X
ClientSampled :
TP-3B-D


Tot Ion: 83 Resp: 924
Ion Ratio Lower Upper
83 100
85 65.9 52.6 78.8

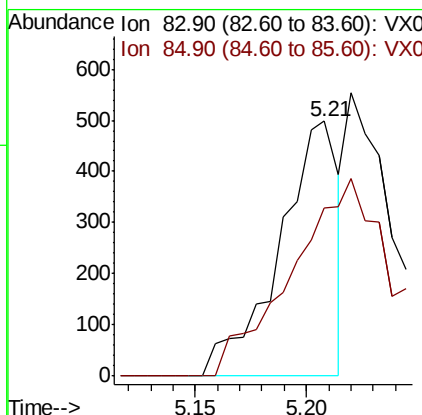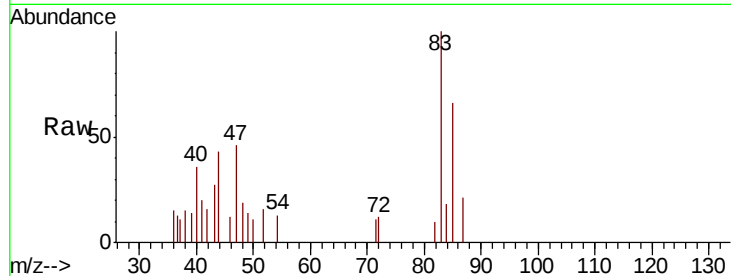

#31
Cyclohexane
Concen: 1.129 ug/l
RT: 5.66 min Scan# 739
Delta R.T. 0.08 min
Lab File: VX009948.D
Acq: 29 May 2019 18:23

Tgt Ion: 56 Resp: 4101
Ion Ratio Lower Upper
56 100
69 172.6 21.6 32.4#
84 115.9 56.8 85.2#

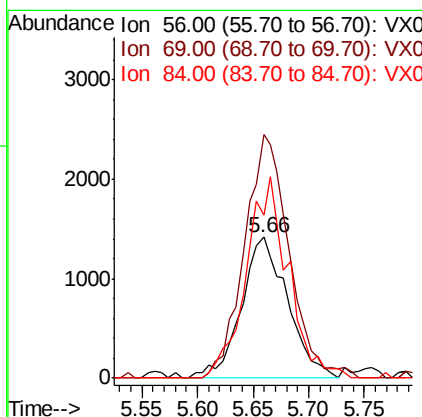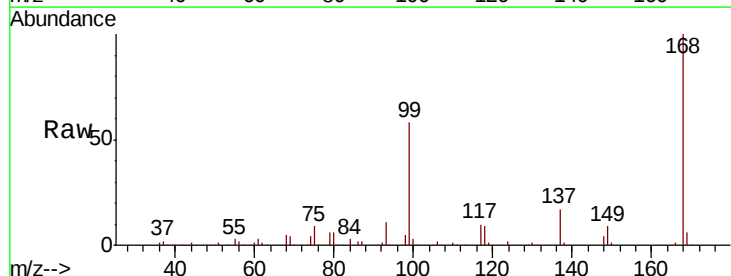

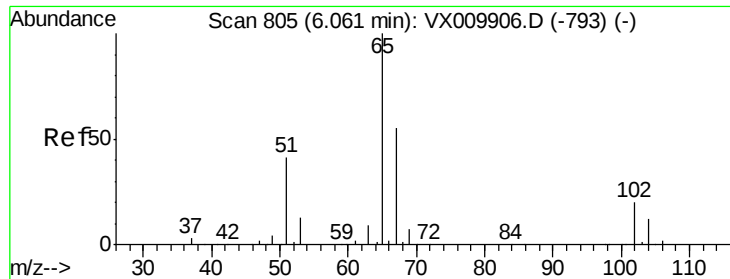

#33

1,2-Dichloroethane-d4

Concen: 49.767 ug/l

RT: 6.06 min Scan# 805

Delta R.T. 0.00 min

Lab File: VX009948.D

Acq: 29 May 2019 18:23

Instrument :

MSVOA_X

ClientSampled :


TP-3B-D

Tot Ion: 65 Resp: 118757

Ion Ratio Lower Upper




65 100

67 53.2 0.0 108.4

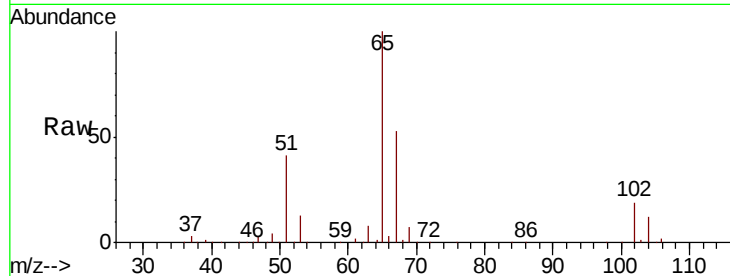

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

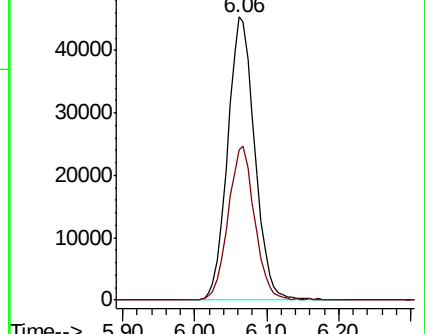

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.86 min Scan# 936

Delta R.T. 0.00 min

Lab File: VX009948.D

Acq: 29 May 2019 18:23


Tgt Ion: 114 Resp: 275421

Ion Ratio Lower Upper

114 100

63 24.1 0.0 47.4



88 16.8 0.0 33.0




Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

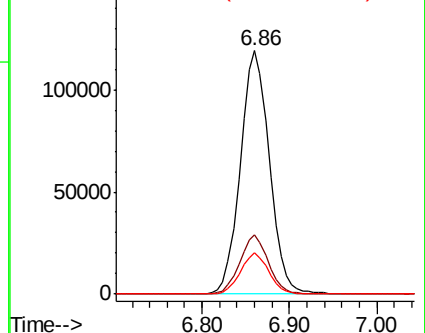

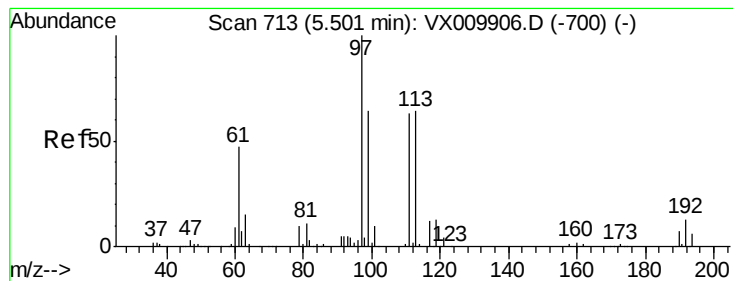

#35

Dibromofluoromethane

Concen: 49.451 ug/l

RT: 5.50 min Scan# 713

Delta R.T. 0.00 min

Lab File: VX009948.D

Acq: 29 May 2019 18:23

Instrument :

MSVOA_X

ClientSampleId :

TP-3B-D





Tot Ion:113 Resp: 85629

Ion Ratio Lower Upper

113 100

111 101.7 82.2 123.2

192 21.2 17.1 25.7

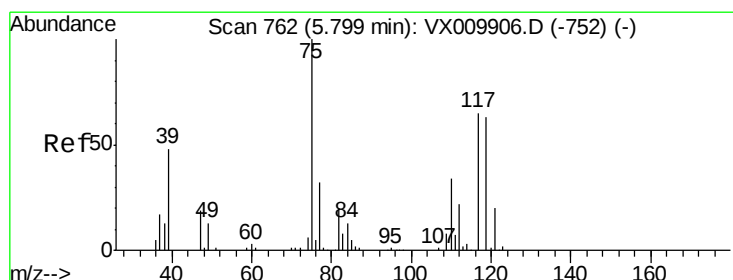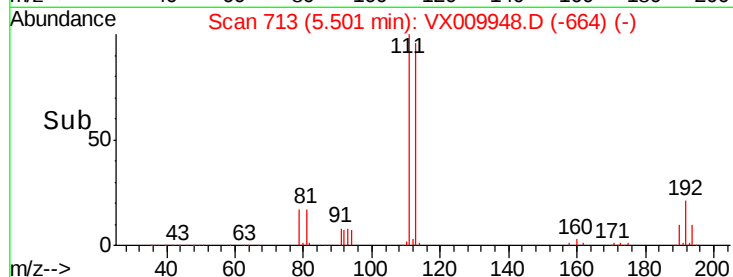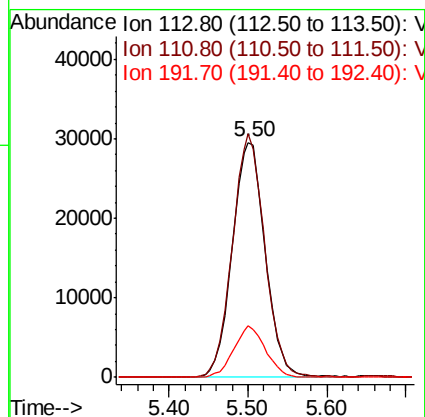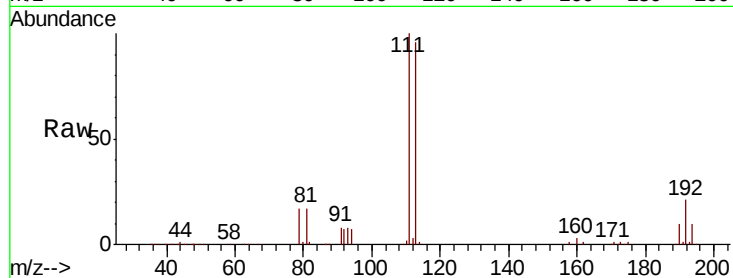

#36

1,1-Dichloropropene

Concen: 4.861 ug/l

RT: 5.67 min Scan# 740

Delta R.T. -0.13 min

Lab File: VX009948.D

Acq: 29 May 2019 18:23




Tgt Ion: 75 Resp: 13585


Ion Ratio Lower Upper

75 100

110 9.0 16.7 50.1#

77 0.0 25.0 37.4#

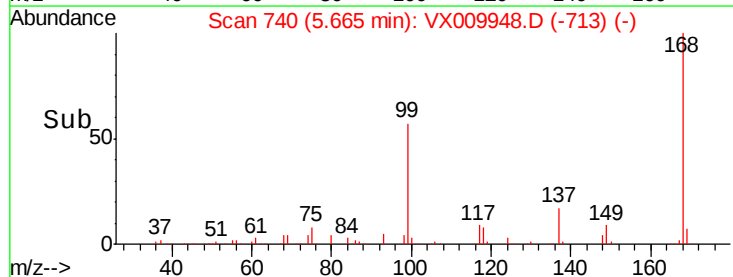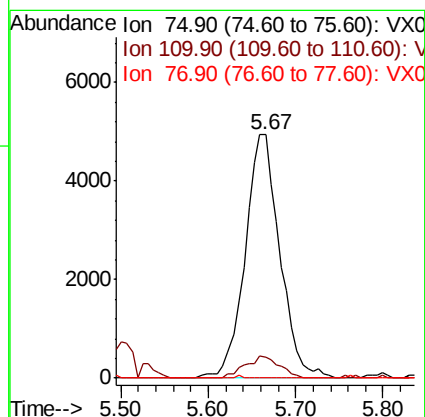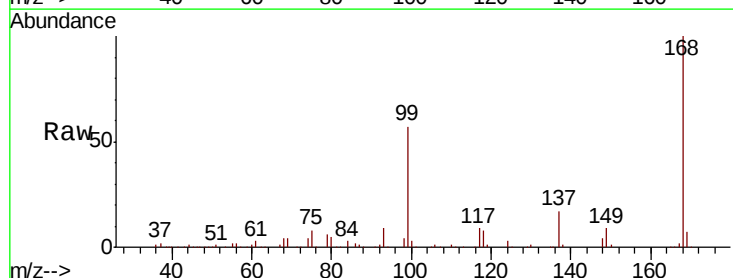

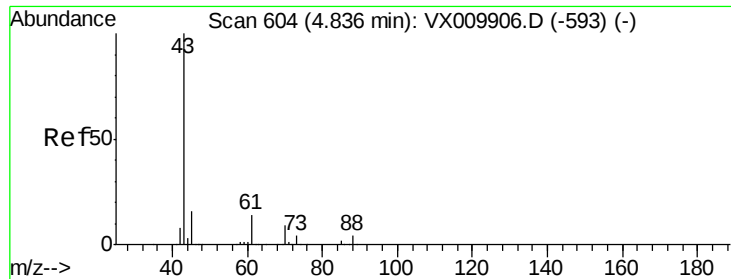

#37

Ethyl Acetate

Concen: 1.119 ug/l

RT: 4.68 min Scan# 579

Delta R.T. -0.15 min

Lab File: VX009948.D

Acq: 29 May 2019 18:23

Instrument :

MSVOA_X

ClientSampleId :

TP-3B-D


Tot Ion: 43 Resp: 4358

Ion Ratio Lower Upper

43 100

61 1.0 10.2 15.2#




70 0.5 7.4 11.2#

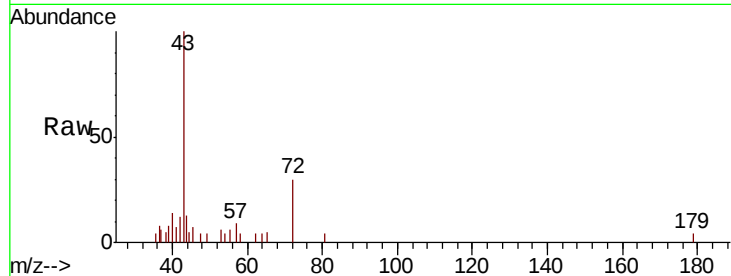

Abundance Ion 43.00 (42.70 to 43.70): VX0

Ion 60.90 (60.60 to 61.60): VX0

Ion 70.00 (69.70 to 70.70): VX0

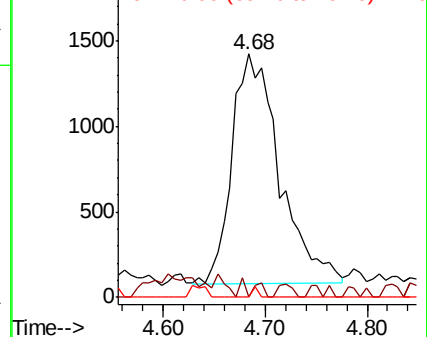

#38

Carbon Tetrachloride

Concen: 6.682 ug/l

RT: 5.66 min Scan# 739

Delta R.T. -0.13 min

Lab File: VX009948.D

Acq: 29 May 2019 18:23


Tgt Ion: 117 Resp: 16135

Ion Ratio Lower Upper

117 100

119 5.8 77.3 115.9#



121 0.0 25.4 38.0#




Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

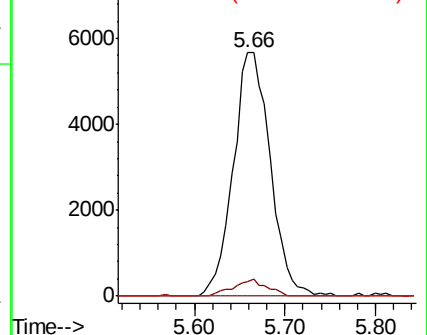



#43

Isopropyl Acetate

Concen: 1.715 ug/l

RT: 6.45 min Scan# 869

Delta R.T. 0.01 min

Lab File: VX009948.D

Acq: 29 May 2019 18:23

Instrument :

MSVOA_X

ClientSampled :

TP-3B-D


Tot Ion: 43 Resp: 10777

Ion Ratio Lower Upper




43 100

61 20.5 14.6 21.8

87 12.4 8.7 13.1

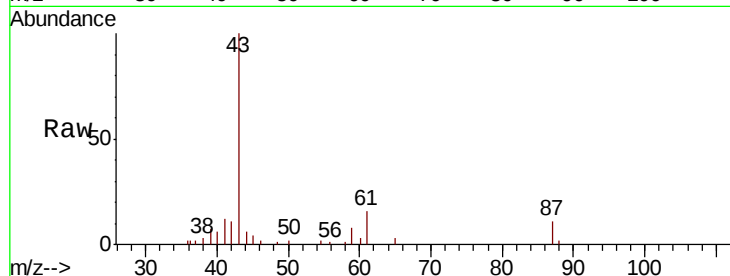

Abundance Ion 43.00 (42.70 to 43.70): VX0
Ion 61.00 (60.70 to 61.70): VX0
Ion 87.00 (86.70 to 87.70): VX0

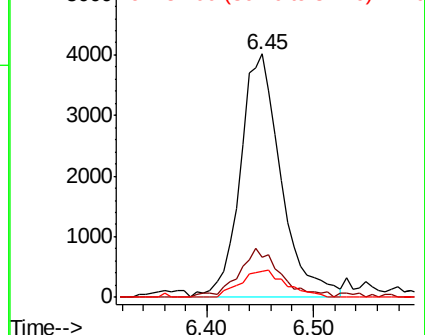

#48

Methyl methacrylate

Concen: 2.231 ug/l

RT: 7.68 min Scan# 1070

Delta R.T. -0.09 min

Lab File: VX009948.D

Acq: 29 May 2019 18:23


Tgt Ion: 41 Resp: 6938

Ion Ratio Lower Upper



41 100


69 0.0 56.4 84.6#

39 0.0 40.6 60.8#



Abundance Ion 41.00 (40.70 to 41.70): VX0
Ion 69.00 (68.70 to 69.70): VX0
Ion 39.00 (38.70 to 39.70): VX0

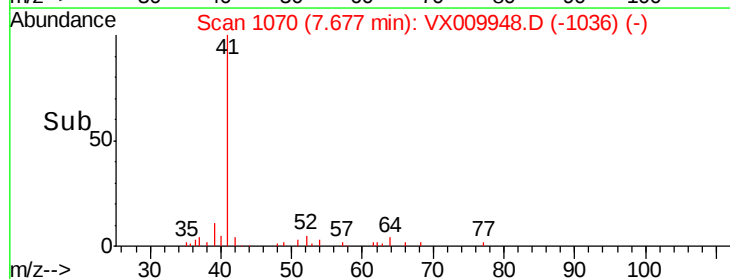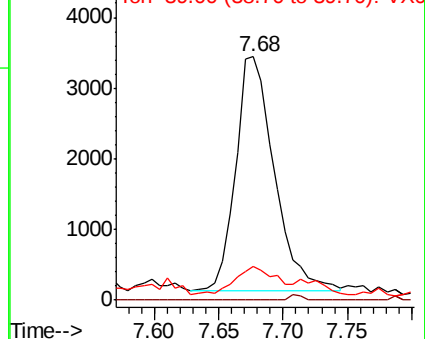

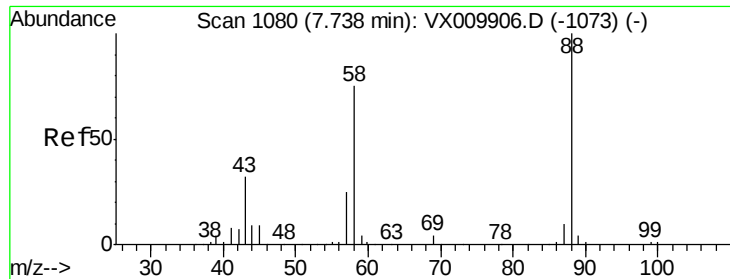

#49

1,4-Dioxane

Concen: 0.328 ug/l

RT: 7.62 min Scan# 1061

Delta R.T. -0.12 min

Lab File: VX009948.D

Acq: 29 May 2019 18:23

Instrument :

MSVOA_X

ClientSampled :

TP-3B-D


Tot Ion: 88 Resp: 19

Ion Ratio Lower Upper

88 100

43 0.0 30.2 45.4#




58 0.0 64.0 96.0#

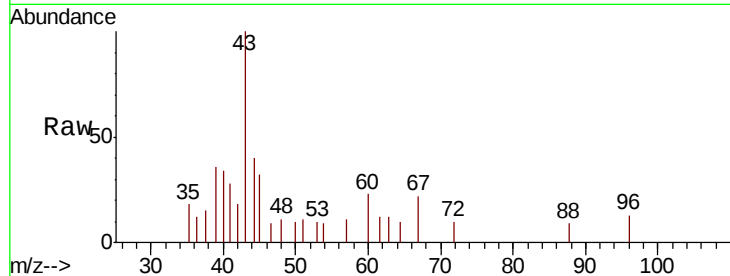

Abundance Ion 88.00 (87.70 to 88.70): VX0

Ion 43.00 (42.70 to 43.70): VX0

Ion 58.00 (57.70 to 58.70): VX0

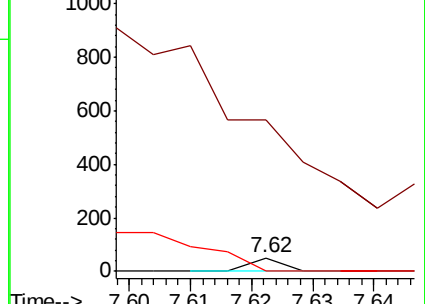

#50

Toluene-d8

Concen: 50.538 ug/l

RT: 8.71 min Scan# 1240

Delta R.T. 0.00 min

Lab File: VX009948.D


Acq: 29 May 2019 18:23

Tgt Ion: 98 Resp: 355362

Ion Ratio Lower Upper



98 100


100 64.3 51.5 77.3



Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): V



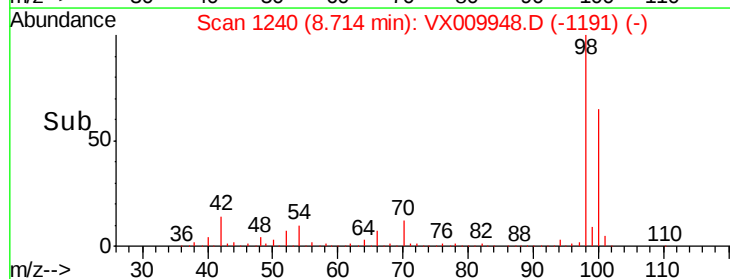
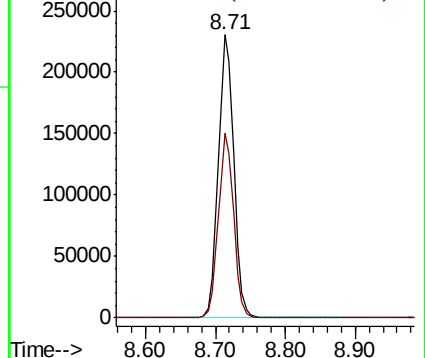


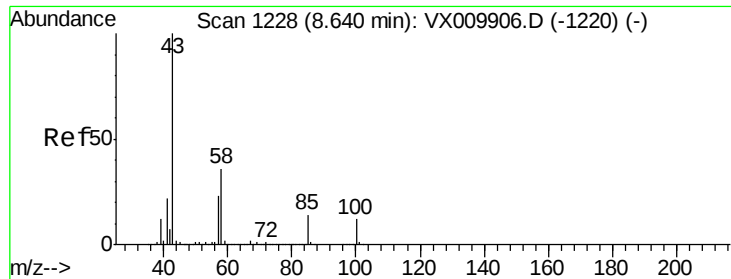

#51
 4-Methyl-2-Pentanone
 Concen: 18.300 ug/l
 RT: 8.62 min Scan# 1224
 Delta R.T. -0.02 min
 Lab File: VX009948.D
 Acq: 29 May 2019 18:23




Instrument :
 MSVOA_X
 ClientSampleID :
 TP-3B-D


Tot Ion: 43 Resp: 74791
 Ion Ratio Lower Upper
 43 100
 58 8.3 28.8 43.2#

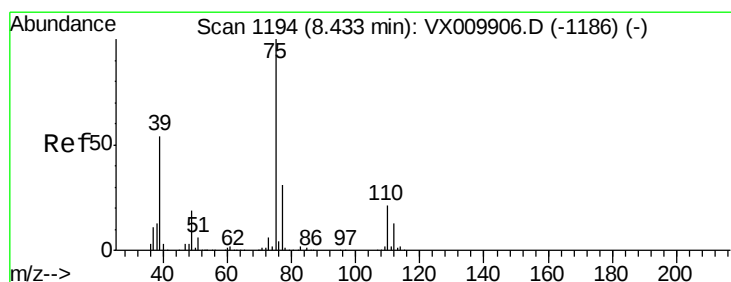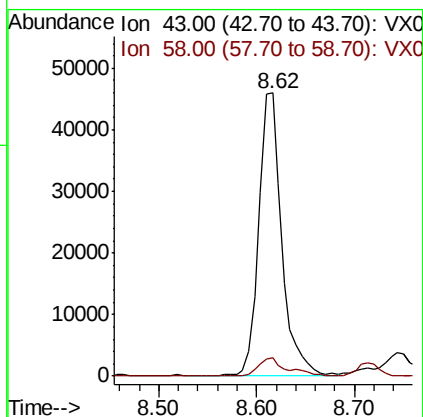

#54
 cis-1,3-Dichloropropene
 Concen: 8.522 ug/l
 RT: 8.62 min Scan# 1224
 Delta R.T. 0.18 min
 Lab File: VX009948.D
 Acq: 29 May 2019 18:23

Tgt Ion: 75 Resp: 29746
 Ion Ratio Lower Upper
 75 100
 77 0.6 24.8 37.2#
 39 30.1 43.4 65.0#



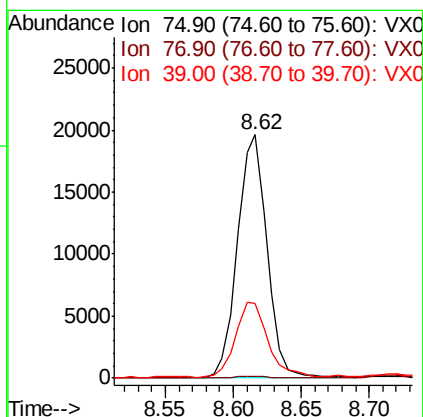



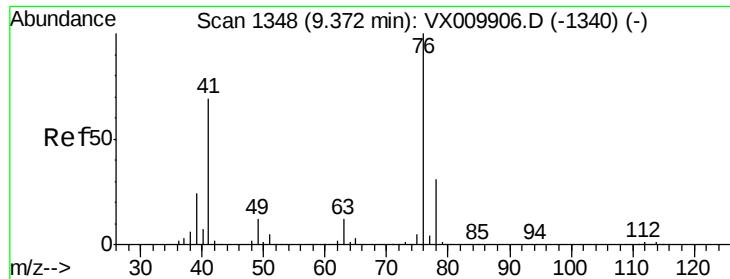

#57
 1,3-Dichloropropane
 Concen: 1.975 ug/l
 RT: 9.54 min Scan# 1376
 Delta R.T. 0.17 min
 Lab File: VX009948.D
 Acq: 29 May 2019 18:23




Instrument :
 MSVOA_X
 ClientSampled :
 TP-3B-D


Tot Ion: 76 Resp: 7186
 Ion Ratio Lower Upper
 76 100
 78 1.1 25.4 38.0#

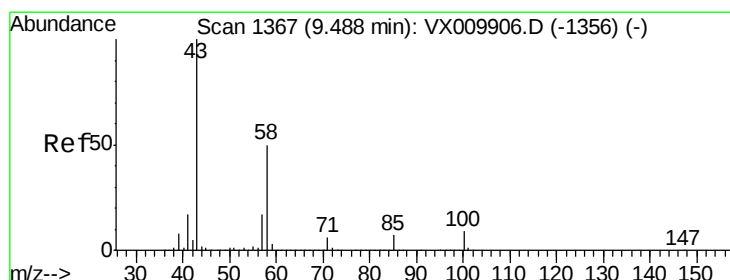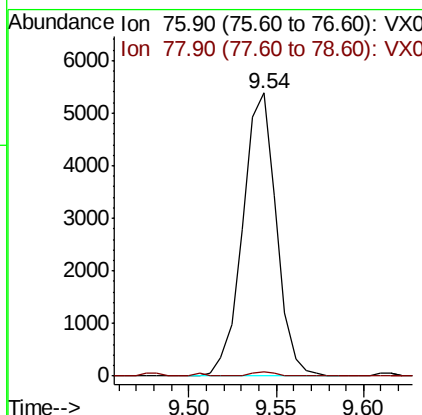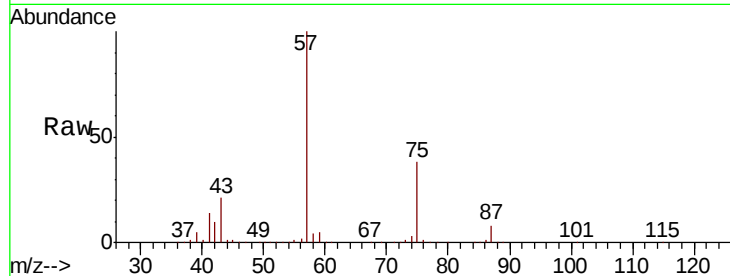

#59
 2-Hexanone
 Concen: 3.193 ug/l
 RT: 9.44 min Scan# 1359
 Delta R.T. -0.05 min
 Lab File: VX009948.D
 Acq: 29 May 2019 18:23

Tgt Ion: 43 Resp: 10046
 Ion Ratio Lower Upper
 43 100
 58 0.0 25.1 75.3#

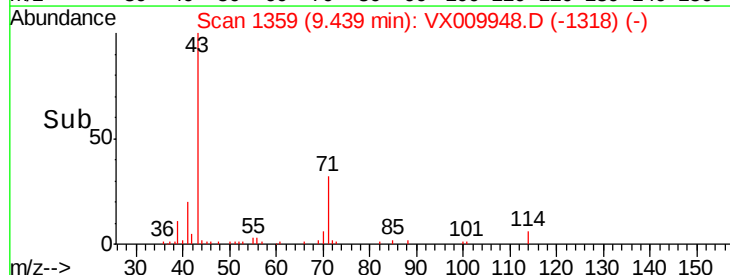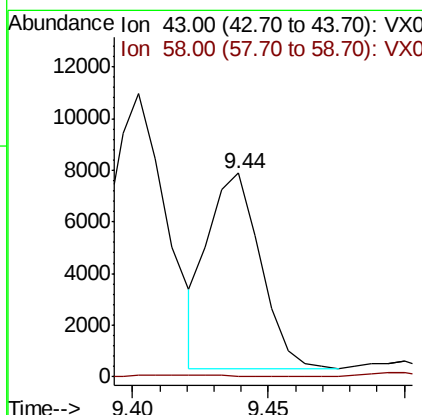

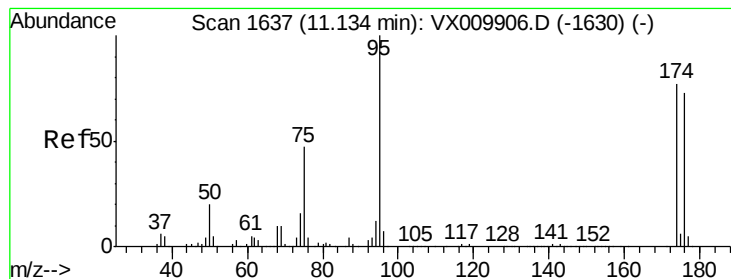

#62

4-Bromofluorobenzene

Concen: 47.229 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. 0.00 min

Lab File: VX009948.D

Acq: 29 May 2019 18:23

Instrument :

MSVOA_X

ClientSampleId :

TP-3B-D


Tot Ion: 95 Resp: 119283

Ion Ratio Lower Upper

95 100

174 82.4 0.0 160.4




176 79.1 0.0 154.6



Abundance Ion 94.90 (94.60 to 95.60): VX009948.D (-1588) (-)

Ion 173.80 (173.50 to 174.50): VX009948.D (-1588) (-)

Ion 175.80 (175.50 to 176.50): VX009948.D (-1588) (-)

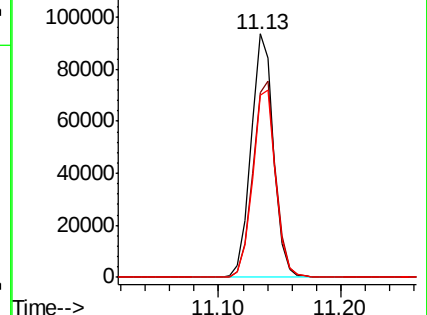

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.11 min Scan# 1469

Delta R.T. 0.00 min

Lab File: VX009948.D

Acq: 29 May 2019 18:23


Tgt Ion: 117 Resp: 251021

Ion Ratio Lower Upper

117 100

82 61.5 49.2 73.8



119 32.1 25.2 37.8




Abundance Ion 116.90 (116.60 to 117.60): VX009948.D (-1420) (-)

Ion 82.00 (81.70 to 82.70): VX009948.D (-1420) (-)

Ion 118.90 (118.60 to 119.60): VX009948.D (-1420) (-)

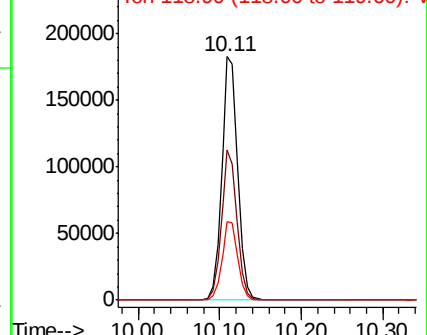

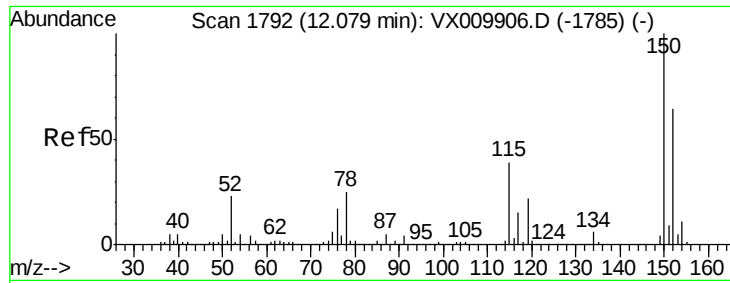

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.08 min Scan# 1792

Delta R.T. 0.00 min

Lab File: VX009948.D

Acq: 29 May 2019 18:23

Instrument :

MSVOA_X

ClientSampleId :

TP-3B-D


Tot Ion:152 Resp: 110649

Ion Ratio Lower Upper

152 100

115 58.5 41.4 124.2




150 156.3 0.0 345.2



Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

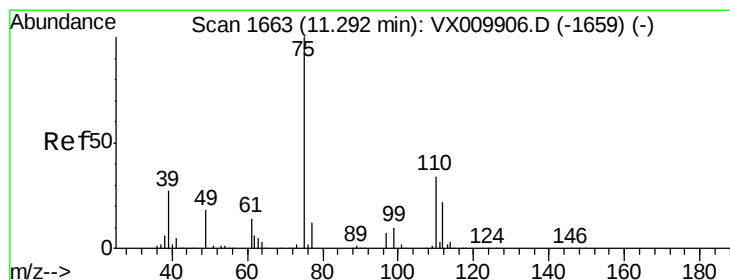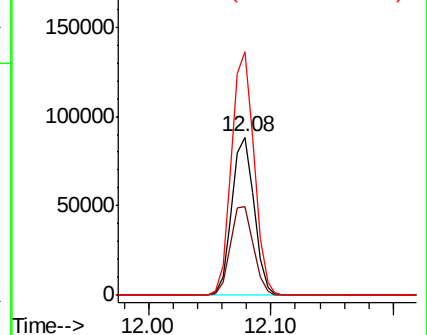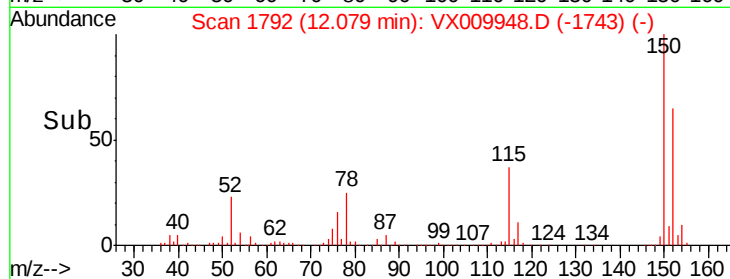

#76

1,2,3-Trichloropropane

Concen: 23.668 ug/l

RT: 11.13 min Scan# 1637

Delta R.T. -0.16 min

Lab File: VX009948.D


Acq: 29 May 2019 18:23

Tgt Ion: 75 Resp: 62624

Ion Ratio Lower Upper



75 100


77 1.3 22.1 66.1#



Abundance Ion 74.90 (74.60 to 75.60): VX0

Ion 77.00 (76.70 to 77.70): VX0



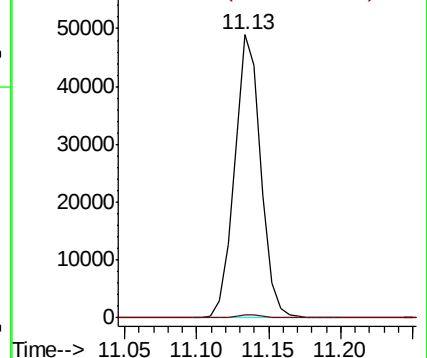



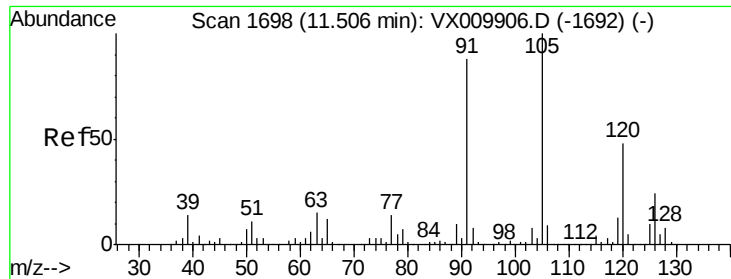

#80
 1,3,5-Trimethylbenzene
 Concen: 0.324 ug/l
 RT: 11.51 min Scan# 1698
 Delta R.T. 0.00 min
 Lab File: VX009948.D
 Acq: 29 May 2019 18:23




Instrument :
 MSVOA_X
 ClientSampleId :
 TP-3B-D


Tot Ion:105 Resp: 2228
 Ion Ratio Lower Upper
 105 100
 120 43.0 24.1 72.3

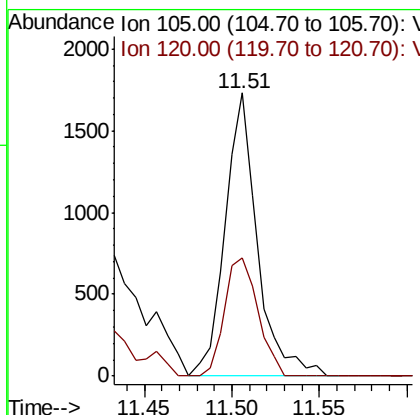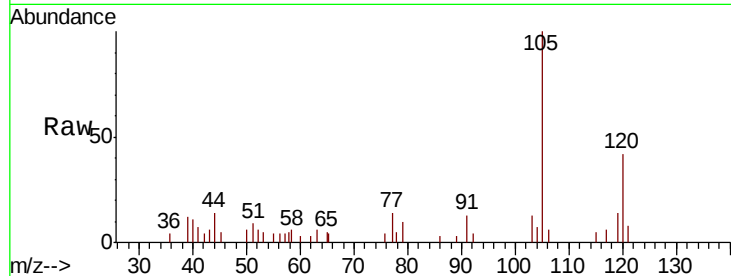

#81
 trans-1,4-Dichloro-2-butene
 Concen: 58.558 ug/l
 RT: 11.13 min Scan# 1637
 Delta R.T. 0.06 min
 Lab File: VX009948.D
 Acq: 29 May 2019 18:23

Tgt Ion: 75 Resp: 62624
 Ion Ratio Lower Upper
 75 100
 53 0.1 79.8 119.6#
 89 0.0 34.2 51.4#


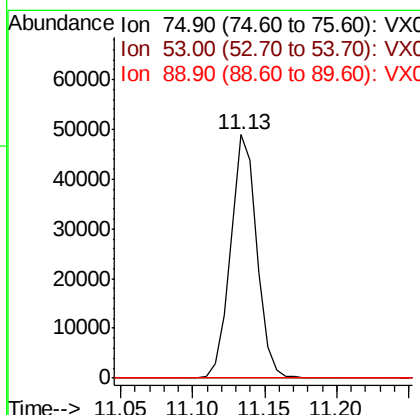






#84
 1,2,4-Trimethylbenzene
 Concen: 0.254 ug/l
 RT: 11.80 min Scan# 1747
 Delta R.T. 0.00 min
 Lab File: VX009948.D
 Acq: 29 May 2019 18:23

Instrument :
 MSVOA_X
 ClientSampled :
 TP-3B-D

Tot Ion:105 Resp: 1776
 Ion Ratio Lower Upper
 105 100
 120 40.4 22.1 66.1

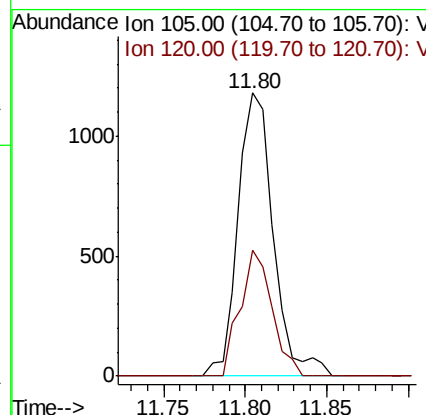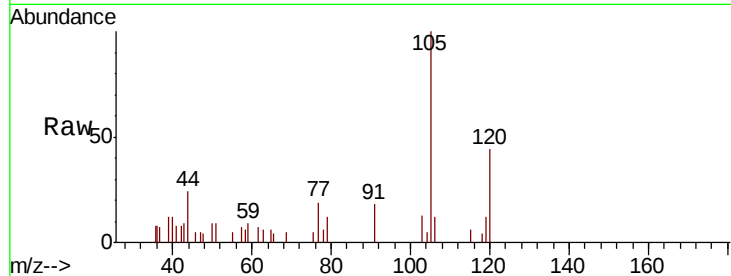

#95
 Naphthalene
 Concen: 0.414 ug/l
 RT: 13.83 min Scan# 2080
 Delta R.T. 0.00 min
 Lab File: VX009948.D
 Acq: 29 May 2019 18:23

Tgt Ion:128 Resp: 3361
 Ion Ratio Lower Upper
 128 100
 127 13.9 10.6 16.0
 129 11.8 8.8 13.2

