

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052921\Not Reviewed Data\
 Data File : VX022251.D
 Acq On : 28 May 2021 14:09
 Operator : JC/MD
 Sample : M2520-02 10X
 Misc : 15.03g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 WC-02-2021-05-24

Quant Time: May 28 19:15:20 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
 Quant Title : SW846 8260
 QLast Update : Wed May 19 14:23:10 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	68656	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	146828	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	130947	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	56603	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	58346	55.09	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	110.18%
35) Dibromofluoromethane	5.391	113	43563	46.79	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	93.58%
50) Toluene-d8	8.653	98	179234	49.97	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	99.94%
62) 4-Bromofluorobenzene	11.085	95	65817	49.65	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	99.30%

Target Compounds						Qvalue
5) Bromomethane	1.599	94	335	0.60	ug/l #	52
10) Methyl Iodide	2.459	142	379	0.43	ug/l #	82
11) Tert butyl alcohol	2.953	59	1589	6.56	ug/l #	73
16) Acetone	2.386	43	693	1.50	ug/l #	87
17) Carbon Disulfide	2.508	76	426	0.21	ug/l #	75
18) Methyl Acetate	2.709	43	553	0.45	ug/l #	47
20) Methylene Chloride	2.800	84	612	0.60	ug/l #	76
31) Cyclohexane	5.544	56	2143	1.61	ug/l #	21
36) 1,1-Dichloropropene	5.556	75	6481	4.77	ug/l #	49
38) Carbon Tetrachloride	5.556	117	7652	5.76	ug/l #	15
52) Toluene	8.714	92	587	0.22	ug/l	87
67) Ethyl Benzene	10.195	91	310597	61.94	ug/l	100
68) m/p-Xylenes	10.305	106	6823	3.60	ug/l	94
69) o-Xylene	10.646	106	7199	3.91	ug/l	98
70) Styrene	10.659	104	826	0.27	ug/l #	1
73) Isopropylbenzene	10.963	105	52853	11.03	ug/l	100
76) 1,2,3-Trichloropropane	11.085	75	34083	24.41	ug/l #	39
78) n-propylbenzene	11.305	91	20736	3.70	ug/l	99
79) 2-Chlorotoluene	11.402	91	4262	1.25	ug/l #	49
80) 1,3,5-Trimethylbenzene	11.402	105	33809	8.51	ug/l	73
81) trans-1,4-Dichloro-2-b...	11.085	75	34083	57.83	ug/l #	12
82) 4-Chlorotoluene	11.457	91	989	0.25	ug/l #	66
83) tert-Butylbenzene	11.756	119	26318	6.91	ug/l #	41
84) 1,2,4-Trimethylbenzene	11.756	105	219940	55.03	ug/l	100
85) sec-Butylbenzene	11.756	105	219940	45.45	ug/l #	57
86) p-Isopropyltoluene	12.012	119	20541	5.03	ug/l	90
89) n-Butylbenzene	12.317	91	14857	3.93	ug/l #	25
90) Hexachloroethane	12.701	117	55623	82.35	ug/l #	9
92) 1,2-Dibromo-3-Chloropr...	12.926	75	248	0.73	ug/l #	1
93) 1,2,4-Trichlorobenzene	13.591	180	270	0.24	ug/l #	1
95) Naphthalene	13.786	128	4992836	1127.85	ug/l	97
96) 1,2,3-Trichlorobenzene	13.975	180	327	0.29	ug/l #	1





(#) = qualifier out of range (m) = manual integration (+) = signals summed



#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.006 min
Lab File: VX022251.D
Acq: 28 May 2021 14:09




Instrument :
MSVOA_X
ClientSampleId :
WC-02-2021-05-24


Tgt Ion:168 Resp: 68656
Ion Ratio Lower Upper
168 100
99 65.1 45.8 68.6

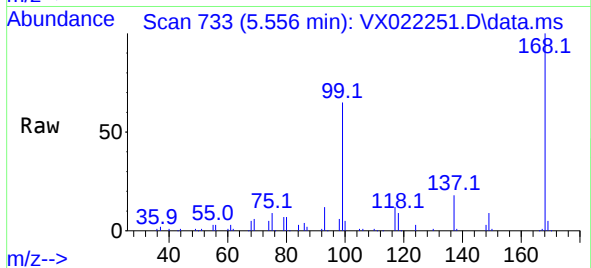

#5
Bromomethane
Concen: 0.60 ug/l
RT: 1.599 min Scan# 84
Delta R.T. -0.013 min
Lab File: VX022251.D
Acq: 28 May 2021 14:09

Tgt Ion: 94 Resp: 335
Ion Ratio Lower Upper
94 100
96 142.4 76.4 114.6#


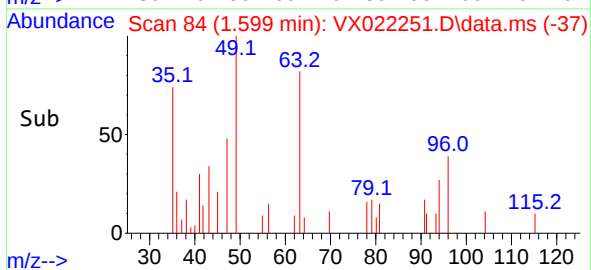




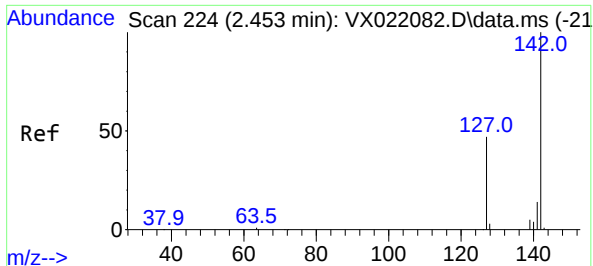

#10
Methyl Iodide
Concen: 0.43 ug/l
RT: 2.459 min Scan# 225
Delta R.T. 0.006 min
Lab File: VX022251.D
Acq: 28 May 2021 14:09




Instrument :
MSVOA_X
ClientSampleId :
WC-02-2021-05-24


Tgt Ion:142 Resp: 379
Ion Ratio Lower Upper
142 100
127 33.5 33.3 49.9
141 0.0 11.4 17.0#

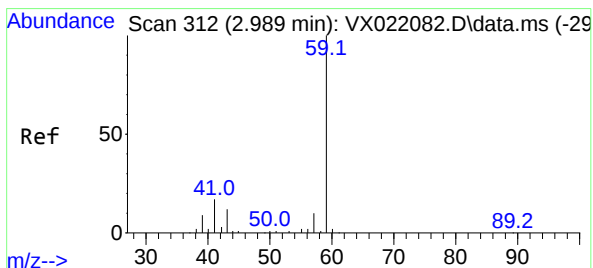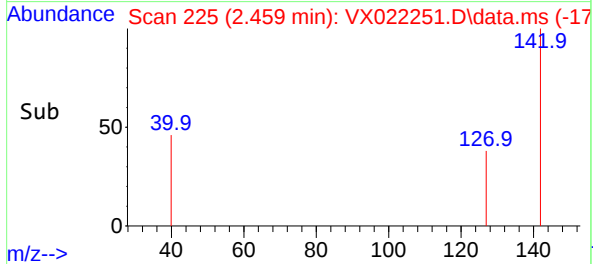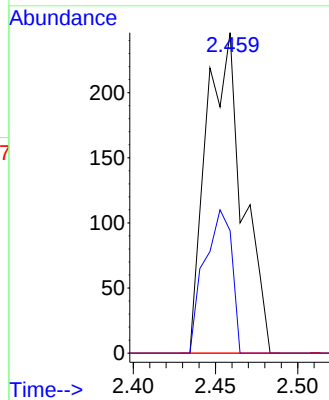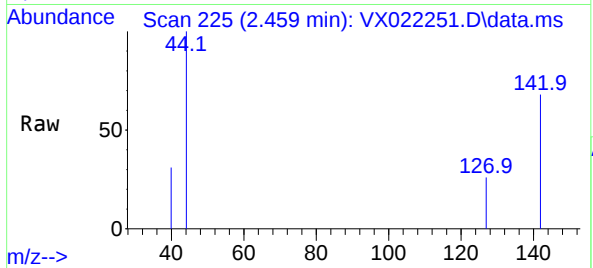

#11
Tert butyl alcohol
Concen: 6.56 ug/l
RT: 2.953 min Scan# 306
Delta R.T. -0.036 min
Lab File: VX022251.D
Acq: 28 May 2021 14:09

Tgt Ion: 59 Resp: 1589
Ion Ratio Lower Upper
59 100
57 0.0 7.8 11.8#


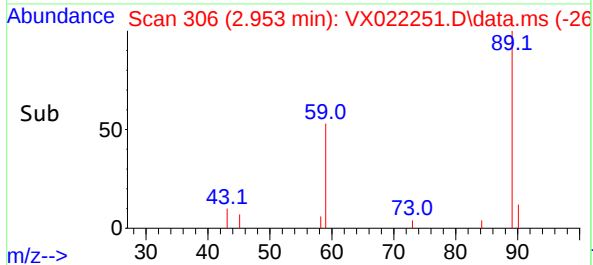
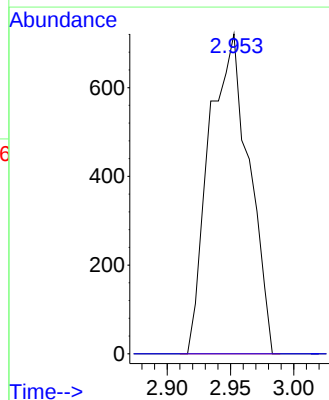
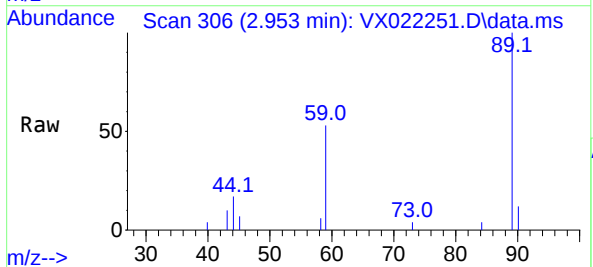


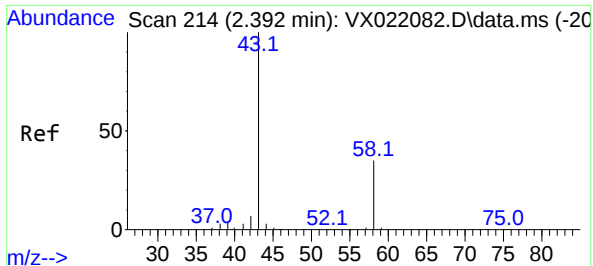

#16
Acetone
Concen: 1.50 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.006 min
Lab File: VX022251.D
Acq: 28 May 2021 14:09




Instrument :
MSVOA_X
ClientSampleId :
WC-02-2021-05-24


Tgt Ion: 43 Resp: 693
Ion Ratio Lower Upper
43 100
58 27.3 27.8 41.8#

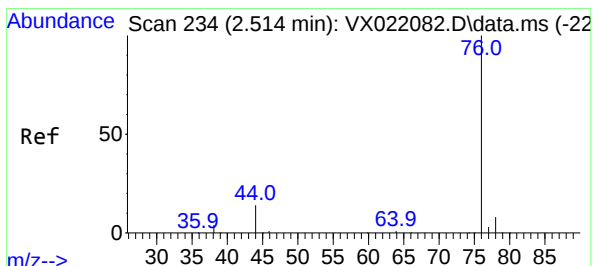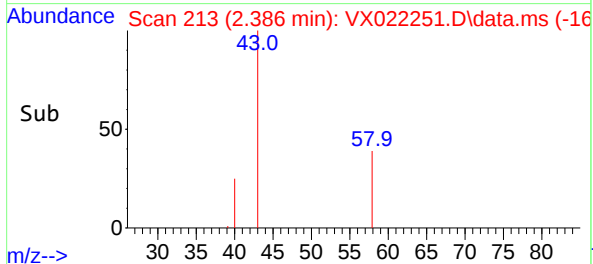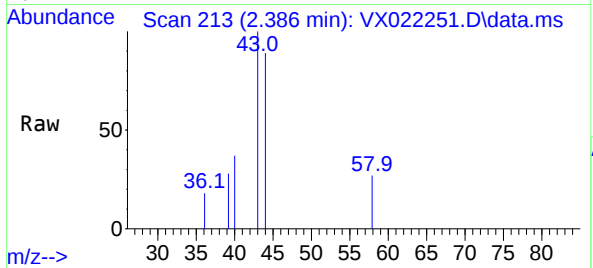

#17
Carbon Disulfide
Concen: 0.21 ug/l
RT: 2.508 min Scan# 233
Delta R.T. -0.006 min
Lab File: VX022251.D
Acq: 28 May 2021 14:09

Tgt Ion: 76 Resp: 426
Ion Ratio Lower Upper
76 100
78 0.0 7.2 10.8#


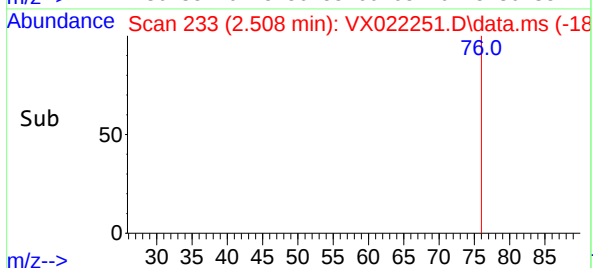
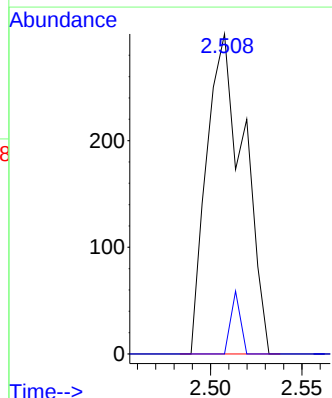
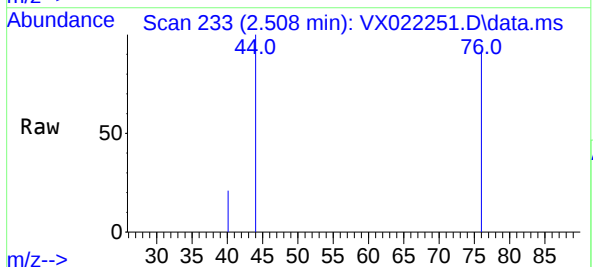




#18
Methyl Acetate
Concen: 0.45 ug/l
RT: 2.709 min Scan# 266
Delta R.T. -0.000 min
Lab File: VX022251.D
Acq: 28 May 2021 14:09




Instrument :
MSVOA_X
ClientSampleId :
WC-02-2021-05-24


Tgt Ion: 43 Resp: 553
Ion Ratio Lower Upper
43 100
74 0.0 21.9 32.9#

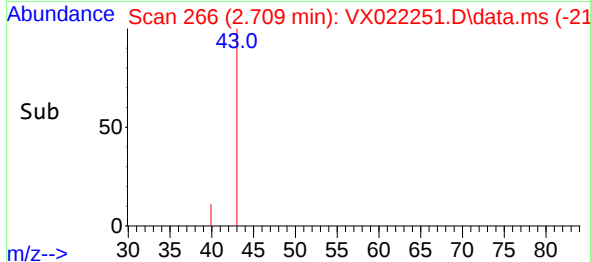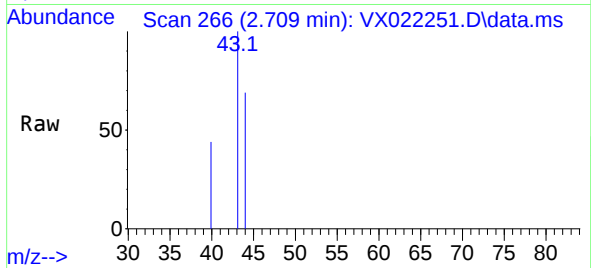

#20
Methylene Chloride
Concen: 0.60 ug/l
RT: 2.800 min Scan# 281
Delta R.T. 0.006 min
Lab File: VX022251.D
Acq: 28 May 2021 14:09


Tgt Ion: 84 Resp: 612
Ion Ratio Lower Upper
84 100
49 76.6 88.6 132.8#
51 26.6 27.0 40.6#
86 50.8 50.3 75.5

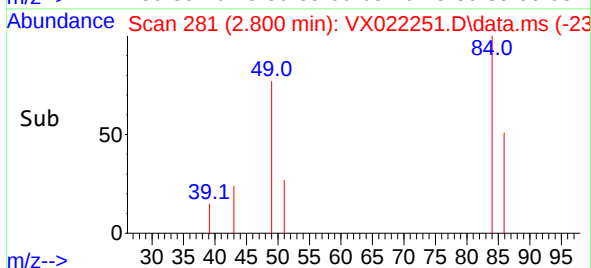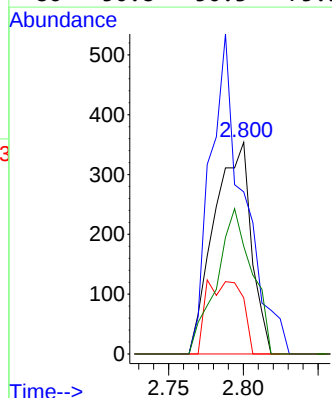



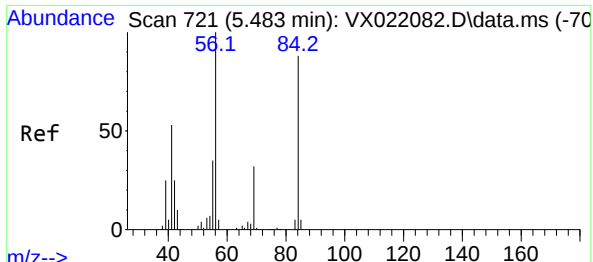


#31
Cyclohexane
Concen: 1.61 ug/l
RT: 5.544 min Scan# 731
Delta R.T. 0.061 min
Lab File: VX022251.D
Acq: 28 May 2021 14:09


Instrument :
MSVOA_X
ClientSampleId :
WC-02-2021-05-24

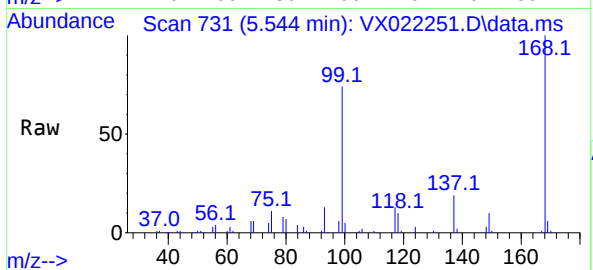



Tgt Ion: 56 Resp: 2143
Ion Ratio Lower Upper
56 100
69 161.6 25.3 37.9#
84 112.2 71.4 107.0#

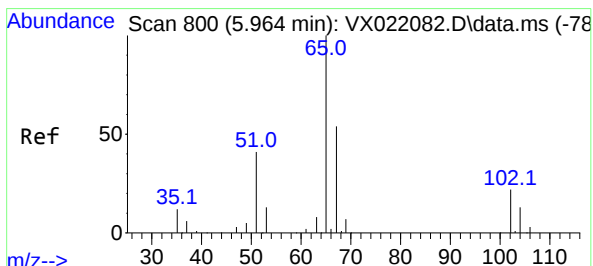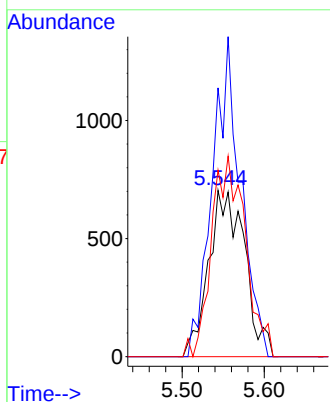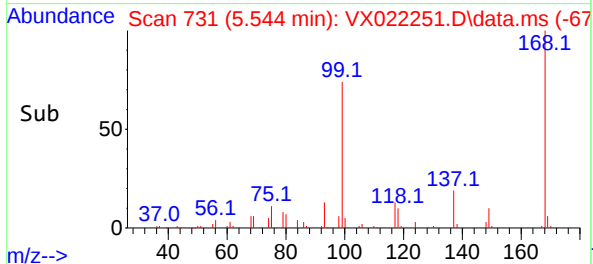


#33
1,2-Dichloroethane-d4
Concen: 55.09 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.000 min
Lab File: VX022251.D
Acq: 28 May 2021 14:09

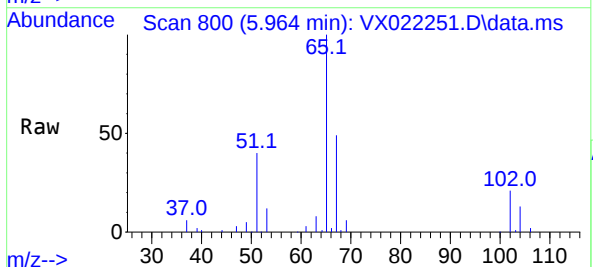

Tgt Ion: 65 Resp: 58346
Ion Ratio Lower Upper
65 100
67 51.1 0.0 105.4



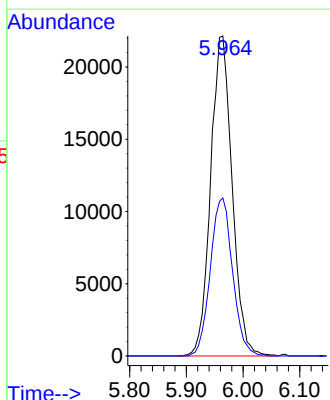
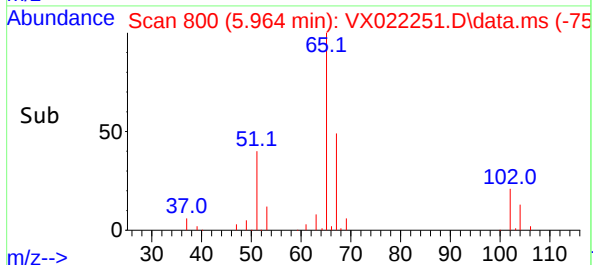


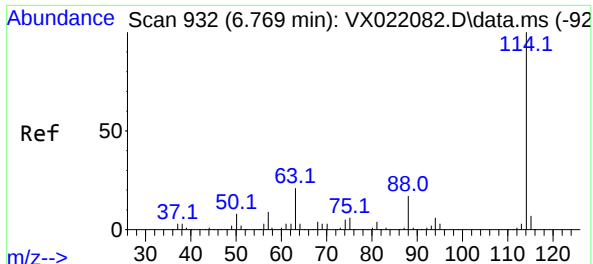

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 6.769 min Scan# 932
Delta R.T. 0.000 min
Lab File: VX022251.D
Acq: 28 May 2021 14:09




Instrument :
MSVOA_X
ClientSampleId :
WC-02-2021-05-24


Tgt Ion:114 Resp: 146828
Ion Ratio Lower Upper
114 100
63 19.6 0.0 40.8
88 16.4 0.0 32.8

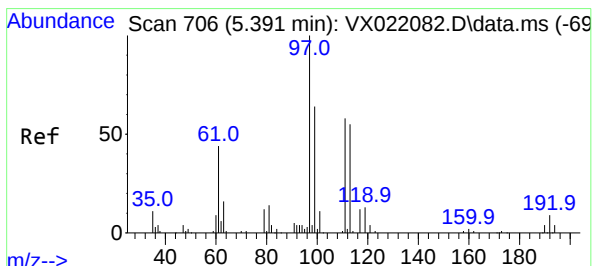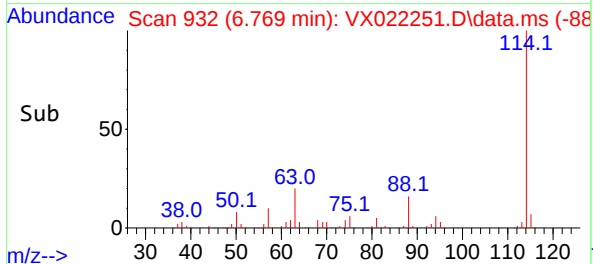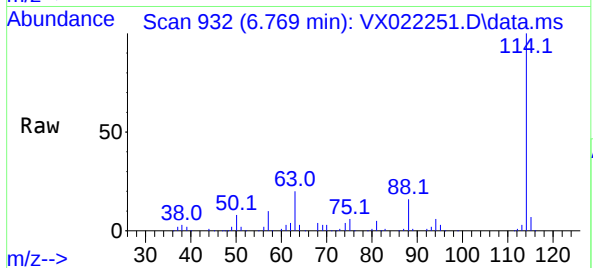

#35
Dibromofluoromethane
Concen: 46.79 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX022251.D
Acq: 28 May 2021 14:09

Tgt Ion:113 Resp: 43563
Ion Ratio Lower Upper
113 100
111 103.0 81.9 122.9
192 16.6 16.7 25.1#


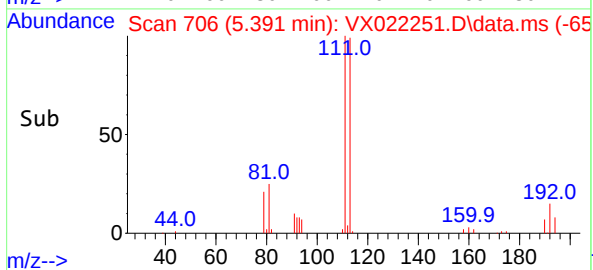

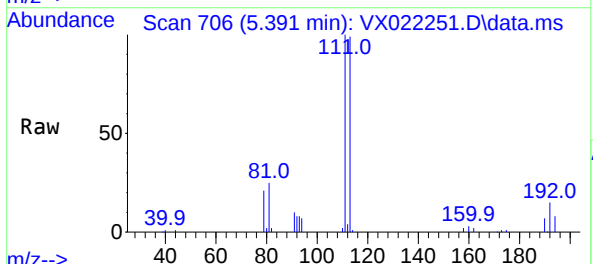




#36
1,1-Dichloropropene
Concen: 4.77 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.146 min
Lab File: VX022251.D
Acq: 28 May 2021 14:09




Instrument :
MSVOA_X
ClientSampleId :
WC-02-2021-05-24


Tgt Ion: 75 Resp: 6481
Ion Ratio Lower Upper
75 100
110 9.2 18.1 54.4#
77 0.0 25.3 37.9#

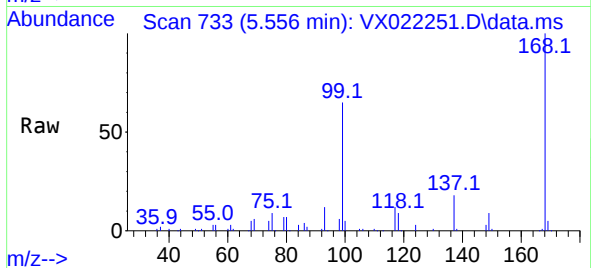

#38
Carbon Tetrachloride
Concen: 5.76 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.134 min
Lab File: VX022251.D
Acq: 28 May 2021 14:09

Tgt Ion: 117 Resp: 7652
Ion Ratio Lower Upper
117 100
119 2.8 76.2 114.2#
121 0.0 24.8 37.2#


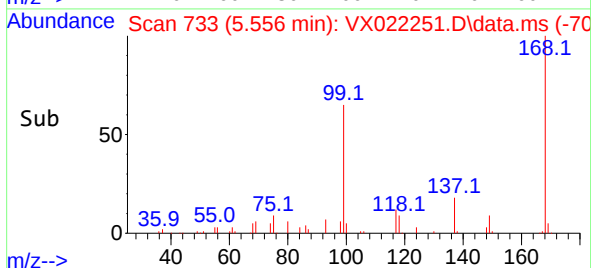
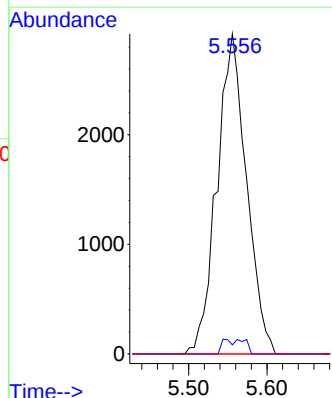



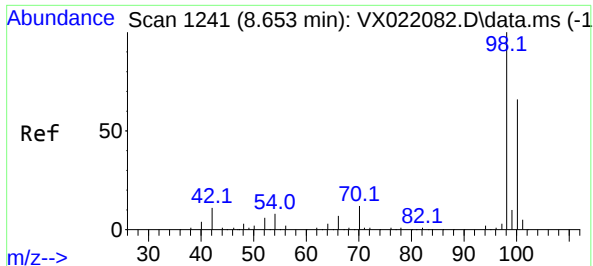

#50
Toluene-d8
Concen: 49.97 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX022251.D
Acq: 28 May 2021 14:09




Instrument :
MSVOA_X
ClientSampleId :
WC-02-2021-05-24


Tgt Ion: 98 Resp: 179234
Ion Ratio Lower Upper
98 100
100 65.7 51.9 77.9

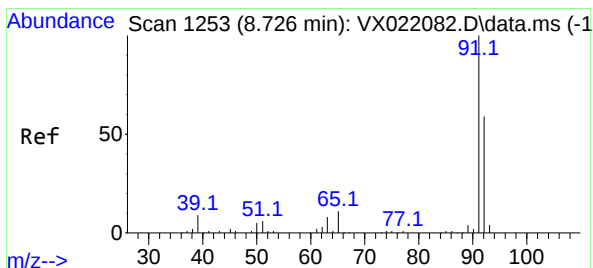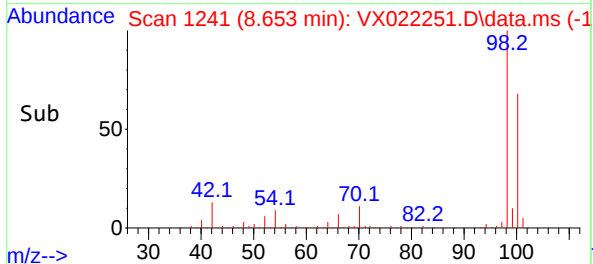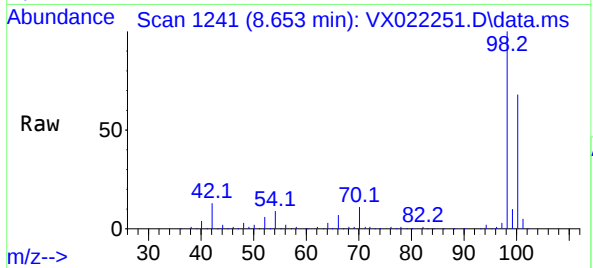

#52
Toluene
Concen: 0.22 ug/l
RT: 8.714 min Scan# 1251
Delta R.T. -0.012 min
Lab File: VX022251.D
Acq: 28 May 2021 14:09

Tgt Ion: 92 Resp: 587
Ion Ratio Lower Upper
92 100
91 189.4 137.1 205.7


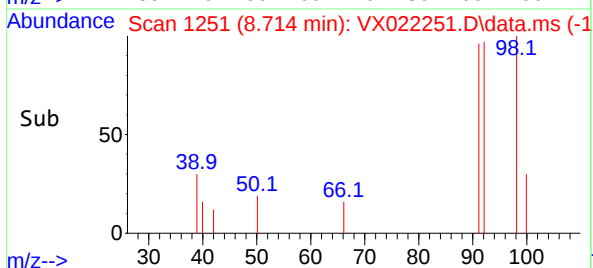

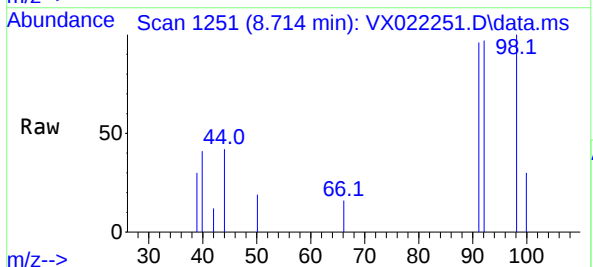




#62
4-Bromofluorobenzene
Concen: 49.65 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX022251.D
Acq: 28 May 2021 14:09




Instrument :
MSVOA_X
ClientSampleId :
WC-02-2021-05-24


Tgt Ion: 95 Resp: 65817
Ion Ratio Lower Upper
95 100
174 64.3 0.0 154.6
176 62.2 0.0 155.8

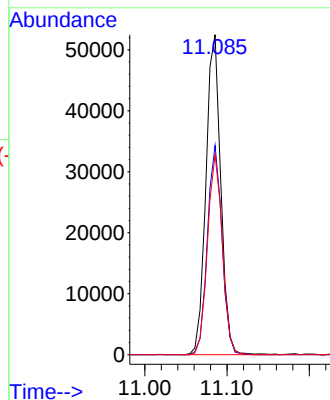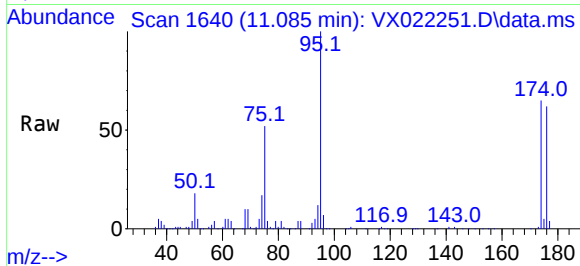

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.006 min
Lab File: VX022251.D
Acq: 28 May 2021 14:09

Tgt Ion: 117 Resp: 130947
Ion Ratio Lower Upper
117 100
82 59.3 47.4 71.2
119 30.5 26.6 39.8


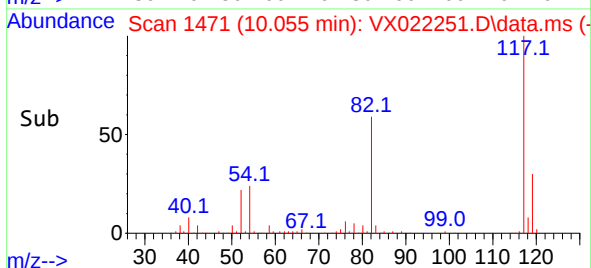
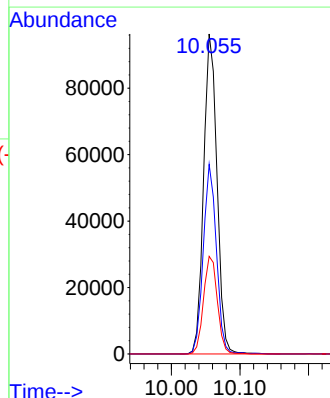
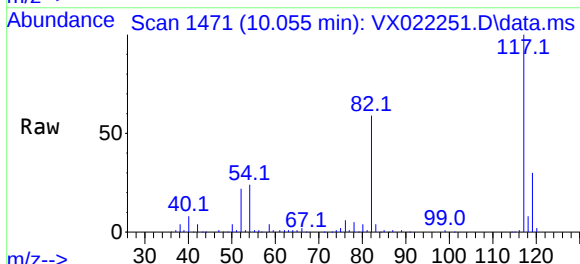




#67
Ethyl Benzene
Concen: 61.94 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX022251.D
Acq: 28 May 2021 14:09




Instrument :
MSVOA_X
ClientSampleId :
WC-02-2021-05-24


Tgt Ion: 91 Resp: 310597
Ion Ratio Lower Upper
91 100
106 30.8 24.6 37.0

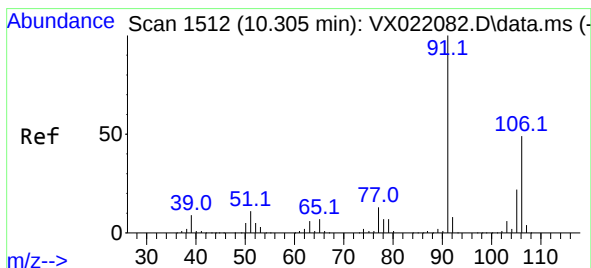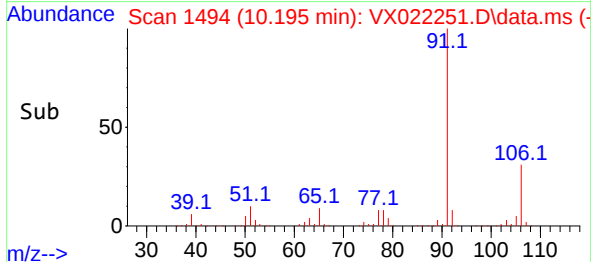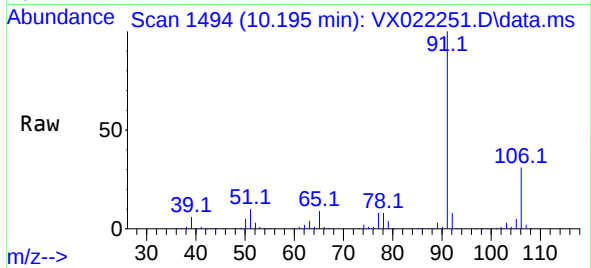

#68
m/p-Xylenes
Concen: 3.60 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. -0.000 min
Lab File: VX022251.D
Acq: 28 May 2021 14:09

Tgt Ion: 106 Resp: 6823
Ion Ratio Lower Upper
106 100
91 194.7 162.8 244.2


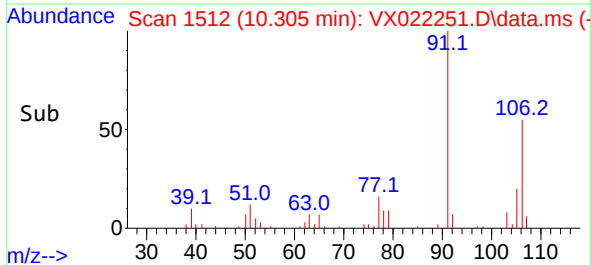

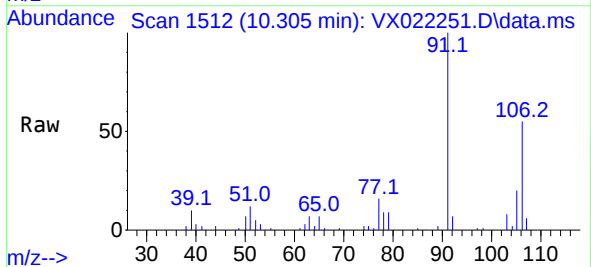


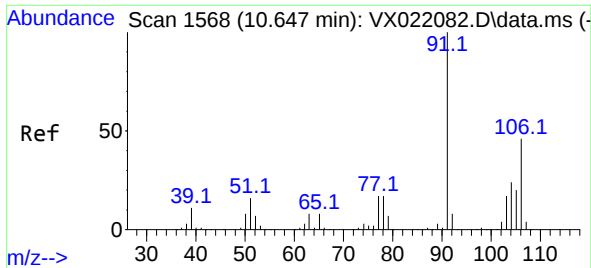

#69
o-Xylene
Concen: 3.91 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. -0.001 min
Lab File: VX022251.D
Acq: 28 May 2021 14:09




Instrument :
MSVOA_X
ClientSampleId :
WC-02-2021-05-24


Tgt Ion:106 Resp: 7199
Ion Ratio Lower Upper
106 100
91 219.4 108.1 324.2

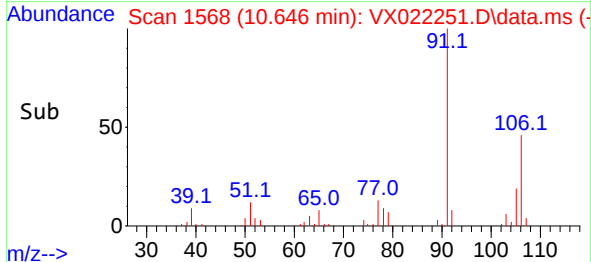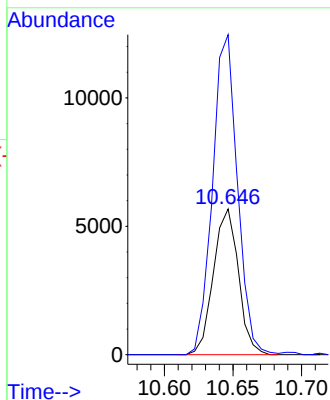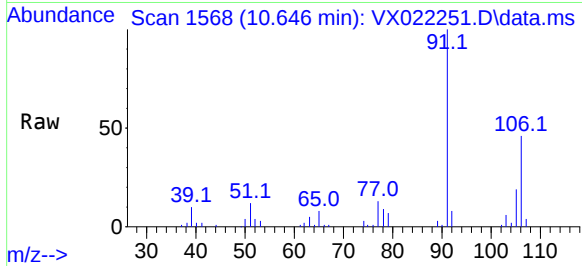

#70
Styrene
Concen: 0.27 ug/l
RT: 10.659 min Scan# 1570
Delta R.T. -0.000 min
Lab File: VX022251.D
Acq: 28 May 2021 14:09

Tgt Ion:104 Resp: 826
Ion Ratio Lower Upper
104 100
78 169.1 40.0 60.0#
103 132.1 43.4 65.0#


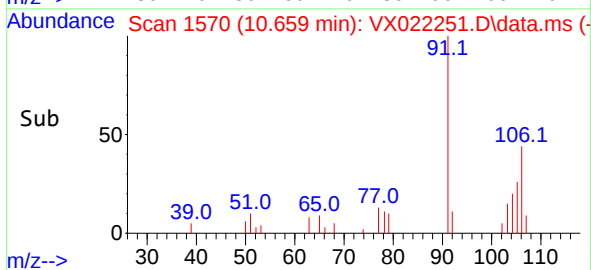
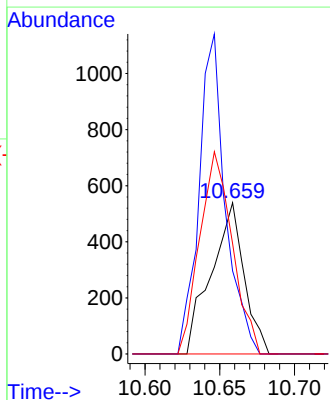
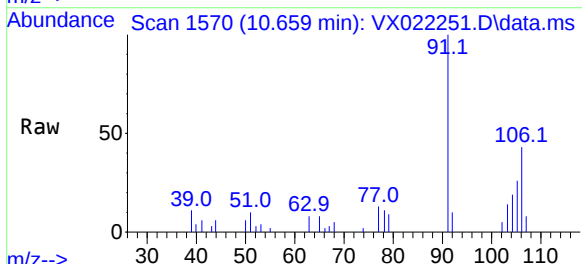




#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX022251.D
Acq: 28 May 2021 14:09




Instrument :
MSVOA_X
ClientSampleId :
WC-02-2021-05-24


Tgt Ion:152 Resp: 56603
Ion Ratio Lower Upper
152 100
115 69.4 41.1 123.3
150 154.0 0.0 349.0

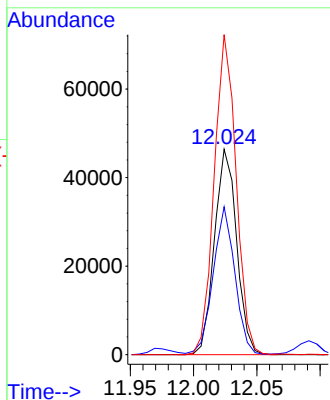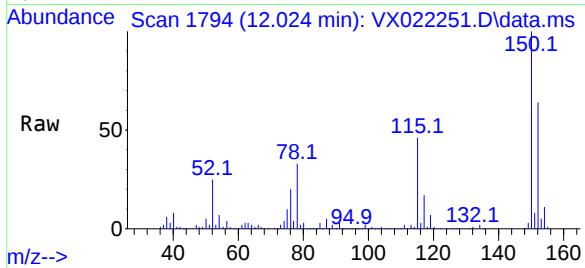

#73
Isopropylbenzene
Concen: 11.03 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. -0.001 min
Lab File: VX022251.D
Acq: 28 May 2021 14:09

Tgt Ion:105 Resp: 52853
Ion Ratio Lower Upper
105 100
120 26.6 13.2 39.6


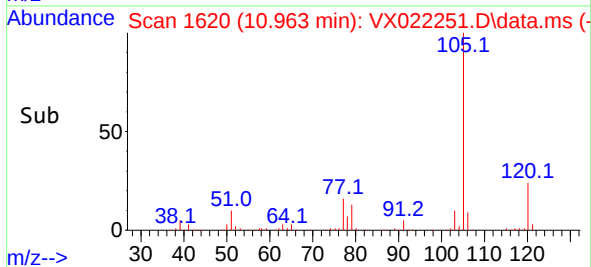
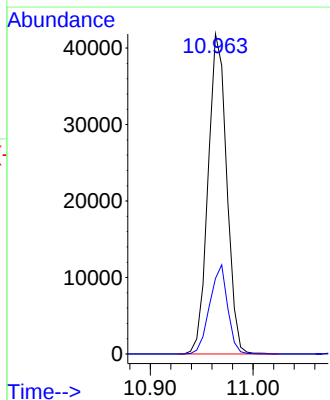
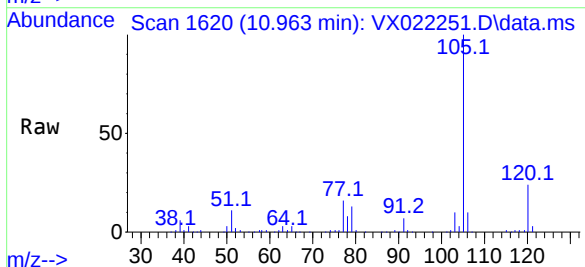




#76
1,2,3-Trichloropropane
Concen: 24.41 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. -0.159 min
Lab File: VX022251.D
Acq: 28 May 2021 14:09




Instrument :
MSVOA_X
ClientSampleId :
WC-02-2021-05-24


Tgt Ion: 75 Resp: 34083
Ion Ratio Lower Upper
75 100
77 1.4 19.1 57.5#

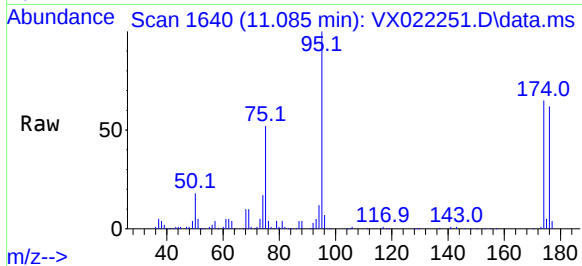

#78
n-propylbenzene
Concen: 3.70 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX022251.D
Acq: 28 May 2021 14:09

Tgt Ion: 91 Resp: 20736
Ion Ratio Lower Upper
91 100
120 22.3 11.5 34.5


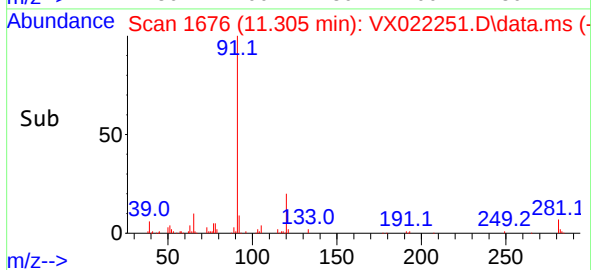

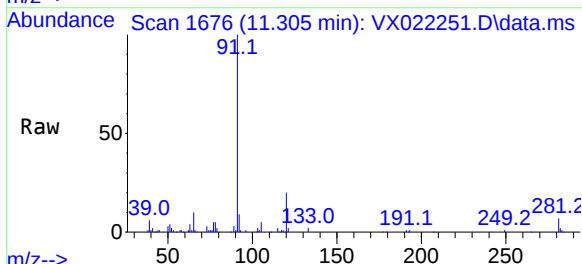




#79
2-Chlorotoluene
Concen: 1.25 ug/l
RT: 11.402 min Scan# 1692
Delta R.T. 0.036 min
Lab File: VX022251.D
Acq: 28 May 2021 14:09




Instrument :
MSVOA_X
ClientSampleId :
WC-02-2021-05-24


Tgt Ion: 91 Resp: 4262
Ion Ratio Lower Upper
91 100
126 4.2 16.6 49.8#

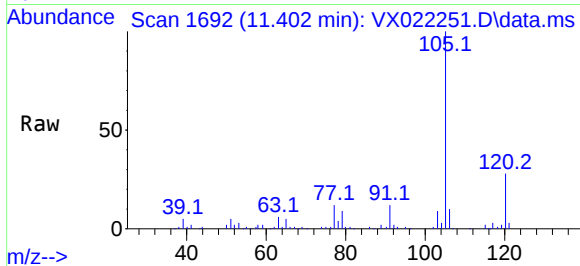

#80
1,3,5-Trimethylbenzene
Concen: 8.51 ug/l
RT: 11.402 min Scan# 1692
Delta R.T. -0.055 min
Lab File: VX022251.D
Acq: 28 May 2021 14:09

Tgt Ion: 105 Resp: 33809
Ion Ratio Lower Upper
105 100
120 29.5 23.8 71.5


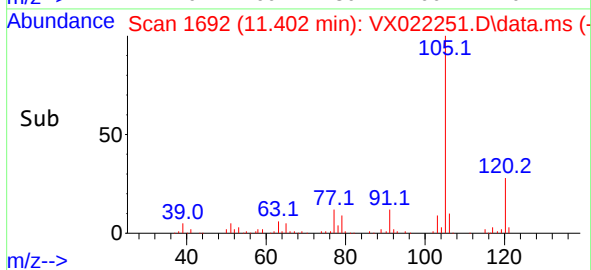

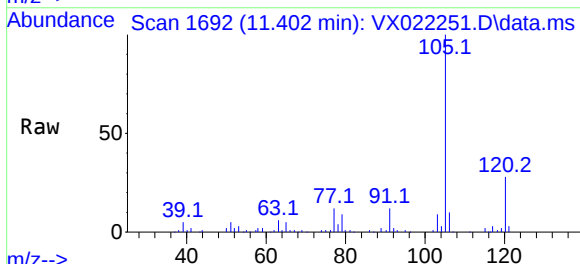




#81
trans-1,4-Dichloro-2-butene
Concen: 57.83 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.060 min
Lab File: VX022251.D
Acq: 28 May 2021 14:09




Instrument :
MSVOA_X
ClientSampleId :
WC-02-2021-05-24


Tgt Ion: 75 Resp: 34083
Ion Ratio Lower Upper
75 100
53 0.4 74.5 111.7#
89 0.0 37.9 56.9#

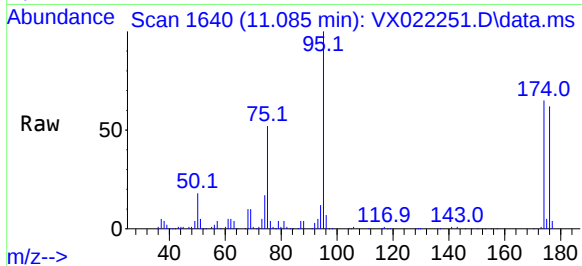

#82
4-Chlorotoluene
Concen: 0.25 ug/l
RT: 11.457 min Scan# 1701
Delta R.T. 0.000 min
Lab File: VX022251.D
Acq: 28 May 2021 14:09

Tgt Ion: 91 Resp: 989
Ion Ratio Lower Upper
91 100
126 11.1 14.9 44.5#


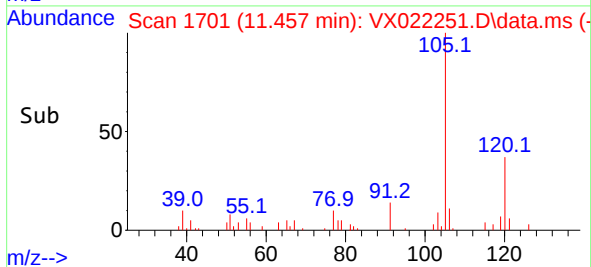

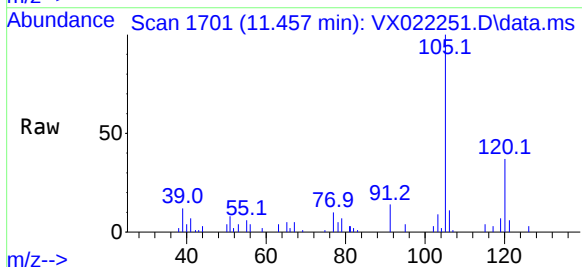




#83
tert-Butylbenzene
Concen: 6.91 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. 0.036 min
Lab File: VX022251.D
Acq: 28 May 2021 14:09




Instrument :
MSVOA_X
ClientSampleId :
WC-02-2021-05-24


Tgt Ion:119 Resp: 26318
Ion Ratio Lower Upper
119 100
91 102.4 27.9 83.7#
134 0.0 11.3 33.9#

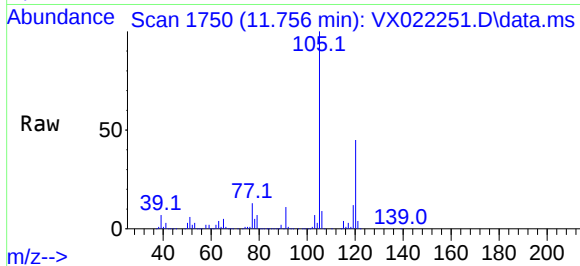

#84
1,2,4-Trimethylbenzene
Concen: 55.03 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.000 min
Lab File: VX022251.D
Acq: 28 May 2021 14:09

Tgt Ion:105 Resp: 219940
Ion Ratio Lower Upper
105 100
120 44.9 22.4 67.3


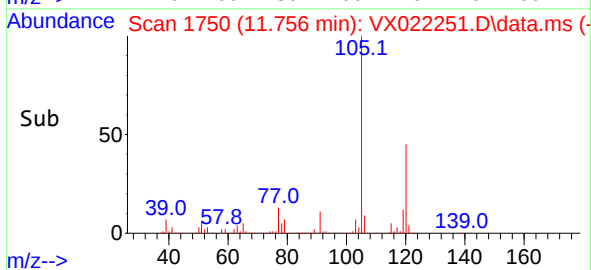

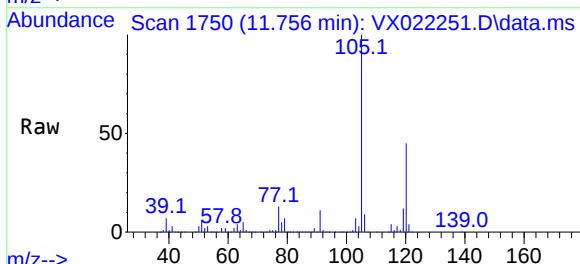




#85
 sec-Butylbenzene
 Concen: 45.45 ug/l
 RT: 11.756 min Scan# 1750
 Delta R.T. -0.140 min
 Lab File: VX022251.D
 Acq: 28 May 2021 14:09




Instrument :
 MSVOA_X
 ClientSampleId :
 WC-02-2021-05-24


Tgt Ion:105 Resp: 219940
 Ion Ratio Lower Upper
 105 100
 134 0.0 10.0 29.8#

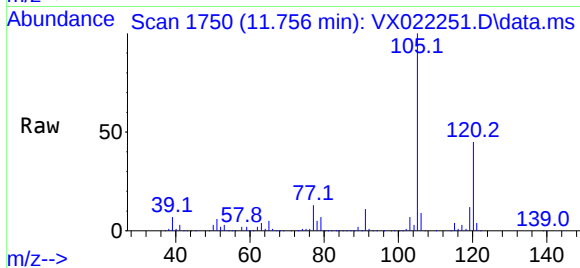

#86
 p-Isopropyltoluene
 Concen: 5.03 ug/l
 RT: 12.012 min Scan# 1792
 Delta R.T. -0.000 min
 Lab File: VX022251.D
 Acq: 28 May 2021 14:09

Tgt Ion:119 Resp: 20541
 Ion Ratio Lower Upper
 119 100
 134 24.4 12.9 38.7
 91 32.5 11.7 35.0


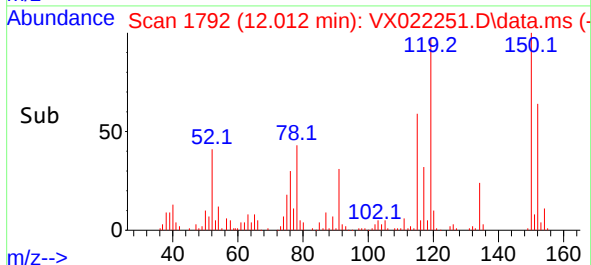
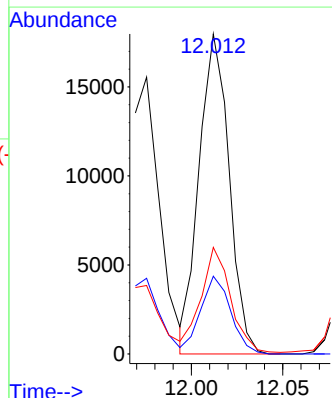
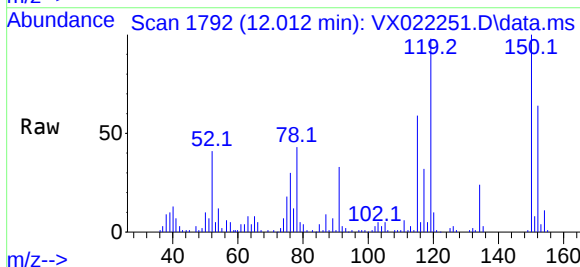




#89
n-Butylbenzene
Concen: 3.93 ug/l
RT: 12.317 min Scan# 1842
Delta R.T. -0.018 min
Lab File: VX022251.D
Acq: 28 May 2021 14:09




Instrument :
MSVOA_X
ClientSampleId :
WC-02-2021-05-24


Tgt Ion: 91 Resp: 14857
Ion Ratio Lower Upper
91 100
92 30.8 27.4 82.0
134 109.7 13.2 39.5#

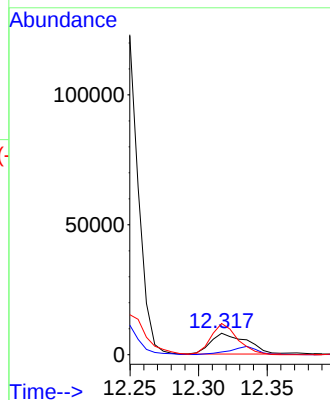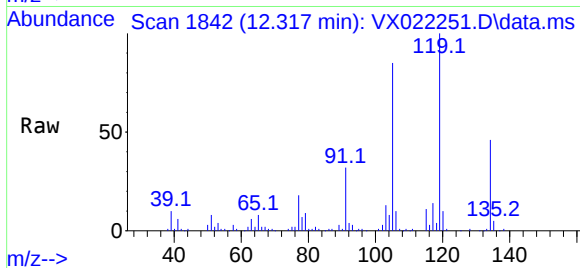

#90
Hexachloroethane
Concen: 82.35 ug/l
RT: 12.701 min Scan# 1905
Delta R.T. 0.158 min
Lab File: VX022251.D
Acq: 28 May 2021 14:09


Tgt Ion: 117 Resp: 55623
Ion Ratio Lower Upper
117 100
201 0.0 40.4 121.2#

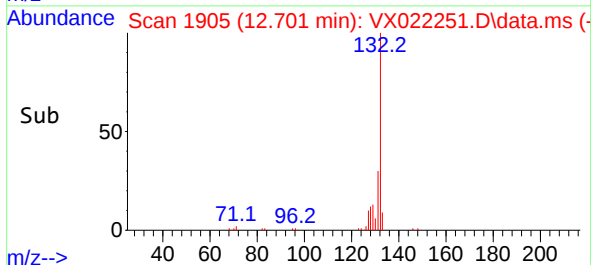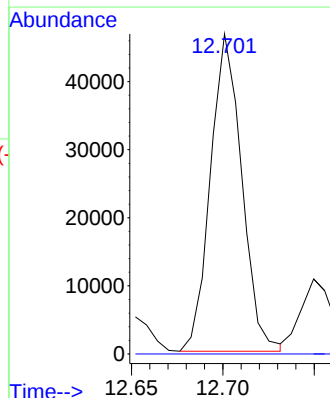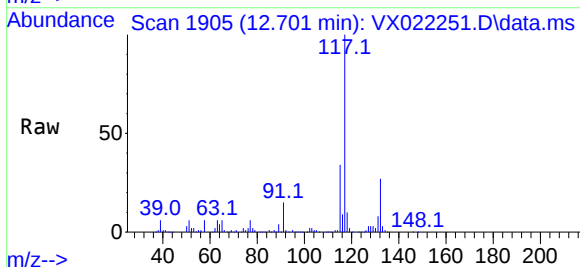






#92
 1,2-Dibromo-3-Chloropropane
 Concen: 0.73 ug/l
 RT: 12.926 min Scan# 1942
 Delta R.T. -0.019 min
 Lab File: VX022251.D
 Acq: 28 May 2021 14:09

Instrument :
 MSVOA_X
 ClientSampleId :
 WC-02-2021-05-24



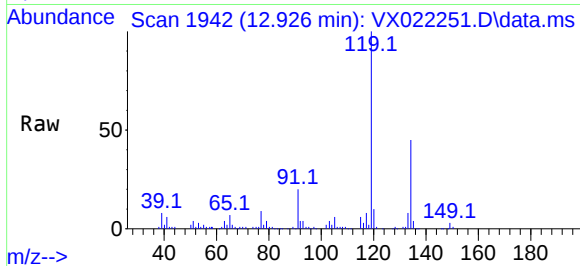



Tgt Ion: 75 Resp: 248
 Ion Ratio Lower Upper
 75 100
 155 0.0 45.3 135.9#
 157 0.0 57.7 173.1#



#93
 1,2,4-Trichlorobenzene
 Concen: 0.24 ug/l
 RT: 13.591 min Scan# 2051
 Delta R.T. -0.000 min
 Lab File: VX022251.D
 Acq: 28 May 2021 14:09

Tgt Ion: 180 Resp: 270
 Ion Ratio Lower Upper
 180 100
 182 71.1 47.7 143.1
 145 424.1 15.0 45.0#


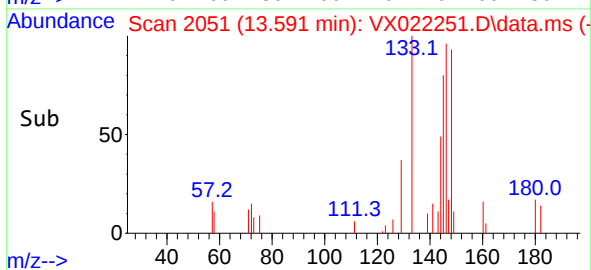
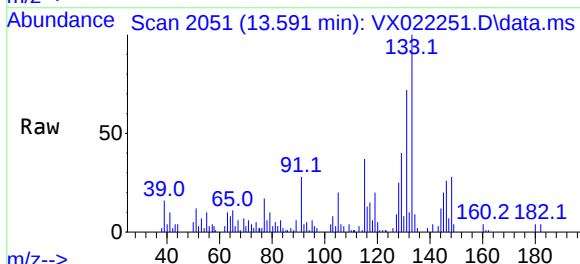





#95
Naphthalene
Concen: 1127.85 ug/l
RT: 13.786 min Scan# 2083
Delta R.T. 0.006 min
Lab File: VX022251.D
Acq: 28 May 2021 14:09

Instrument :
MSVOA_X
ClientSampleId :
WC-02-2021-05-24

Tgt Ion:128 Resp: 4992836
Ion Ratio Lower Upper
128 100
127 14.0 10.3 15.5
129 12.0 8.8 13.2

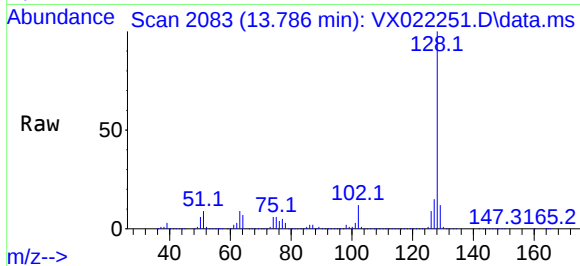

#96
1,2,3-Trichlorobenzene
Concen: 0.29 ug/l
RT: 13.975 min Scan# 2114
Delta R.T. 0.012 min
Lab File: VX022251.D
Acq: 28 May 2021 14:09

Tgt Ion:180 Resp: 327
Ion Ratio Lower Upper
180 100
182 38.2 47.6 142.9#
145 693.9 16.1 48.3#

