

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052921\
 Data File : VX022281.D
 Acq On : 29 May 2021 03:27
 Operator : JC/MD
 Sample : PB136709TB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PB136709TB

Quant Time: May 29 05:00:34 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
 Quant Title : SW846 8260
 QLast Update : Wed May 19 14:23:10 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.562	168	64245	50.00	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.769	114	138745	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.061	117	127908	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	56484	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	55343	55.84	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery = 111.68%			
35) Dibromofluoromethane	5.391	113	41661	47.35	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 94.70%			
50) Toluene-d8	8.653	98	171670	50.65	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery = 101.30%			
62) 4-Bromofluorobenzene	11.085	95	65216	52.06	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 104.12%			
Target Compounds						Qvalue
3) Chloromethane	1.294	50	401	0.48	ug/l	98
4) Vinyl Chloride	1.373	62	434	0.49	ug/l	# 48
5) Bromomethane	1.617	94	196	0.38	ug/l	83
6) Chloroethane	1.696	64	113	0.21	ug/l	# 43
11) Tert butyl alcohol	2.971	59	478	2.11	ug/l	# 73
13) Acrolein	2.239	56	102	0.68	ug/l	# 1
16) Acetone	2.385	43	19119	44.31	ug/l	91
18) Methyl Acetate	2.715	43	900	0.78	ug/l	# 73
20) Methylene Chloride	2.788	84	3639	3.80	ug/l	94
25) 2-Butanone	4.574	43	2770	3.97	ug/l	# 75
27) cis-1,2-Dichloroethene	4.495	96	3206	3.29	ug/l	90
29) Tetrahydrofuran	5.025	42	316	0.76	ug/l	# 86
31) Cyclohexane	5.556	56	1753	1.41	ug/l	# 64
36) 1,1-Dichloropropene	5.562	75	6161	4.80	ug/l	# 48
38) Carbon Tetrachloride	5.568	117	7518	5.99	ug/l	# 16
43) Isopropyl Acetate	6.348	43	15015	5.84	ug/l	93
44) Trichloroethene	7.135	130	7335	7.48	ug/l	94
48) Methyl methacrylate	7.598	41	4386	3.70	ug/l	# 10
49) 1,4-Dioxane	7.799	88	32	1.39	ug/l	# 1
51) 4-Methyl-2-Pentanone	8.555	43	53707	34.85	ug/l	# 45
52) Toluene	8.720	92	573	0.23	ug/l	85
54) cis-1,3-Dichloropropene	8.555	75	25160	14.83	ug/l	# 62
57) 1,3-Dichloropropane	9.488	76	15161	8.75	ug/l	# 42
59) 2-Hexanone	9.488	43	201768	174.10	ug/l	# 44
71) Bromoform	10.927	173	21	1.44	ug/l	# 29
74) N-amyl acetate	10.774	43	813	0.36	ug/l	# 35
76) 1,2,3-Trichloropropane	11.085	75	33887	24.32	ug/l	# 40
80) 1,3,5-Trimethylbenzene	11.457	105	3560	0.90	ug/l	89
81) trans-1,4-Dichloro-2-b...	11.085	75	33887	57.62	ug/l	# 12
82) 4-Chlorotoluene	11.463	91	1111	0.28	ug/l	# 45
90) Hexachloroethane	12.377	117	172	0.26	ug/l	78

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052921\
Data File : VX022281.D
Acq On : 29 May 2021 03:27
Operator : JC/MD
Sample : PB136709TB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PB136709TB


Quant Time: May 29 05:00:34 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
Quant Title : SW846 8260
QLast Update : Wed May 19 14:23:10 2021
Response via : Initial Calibration

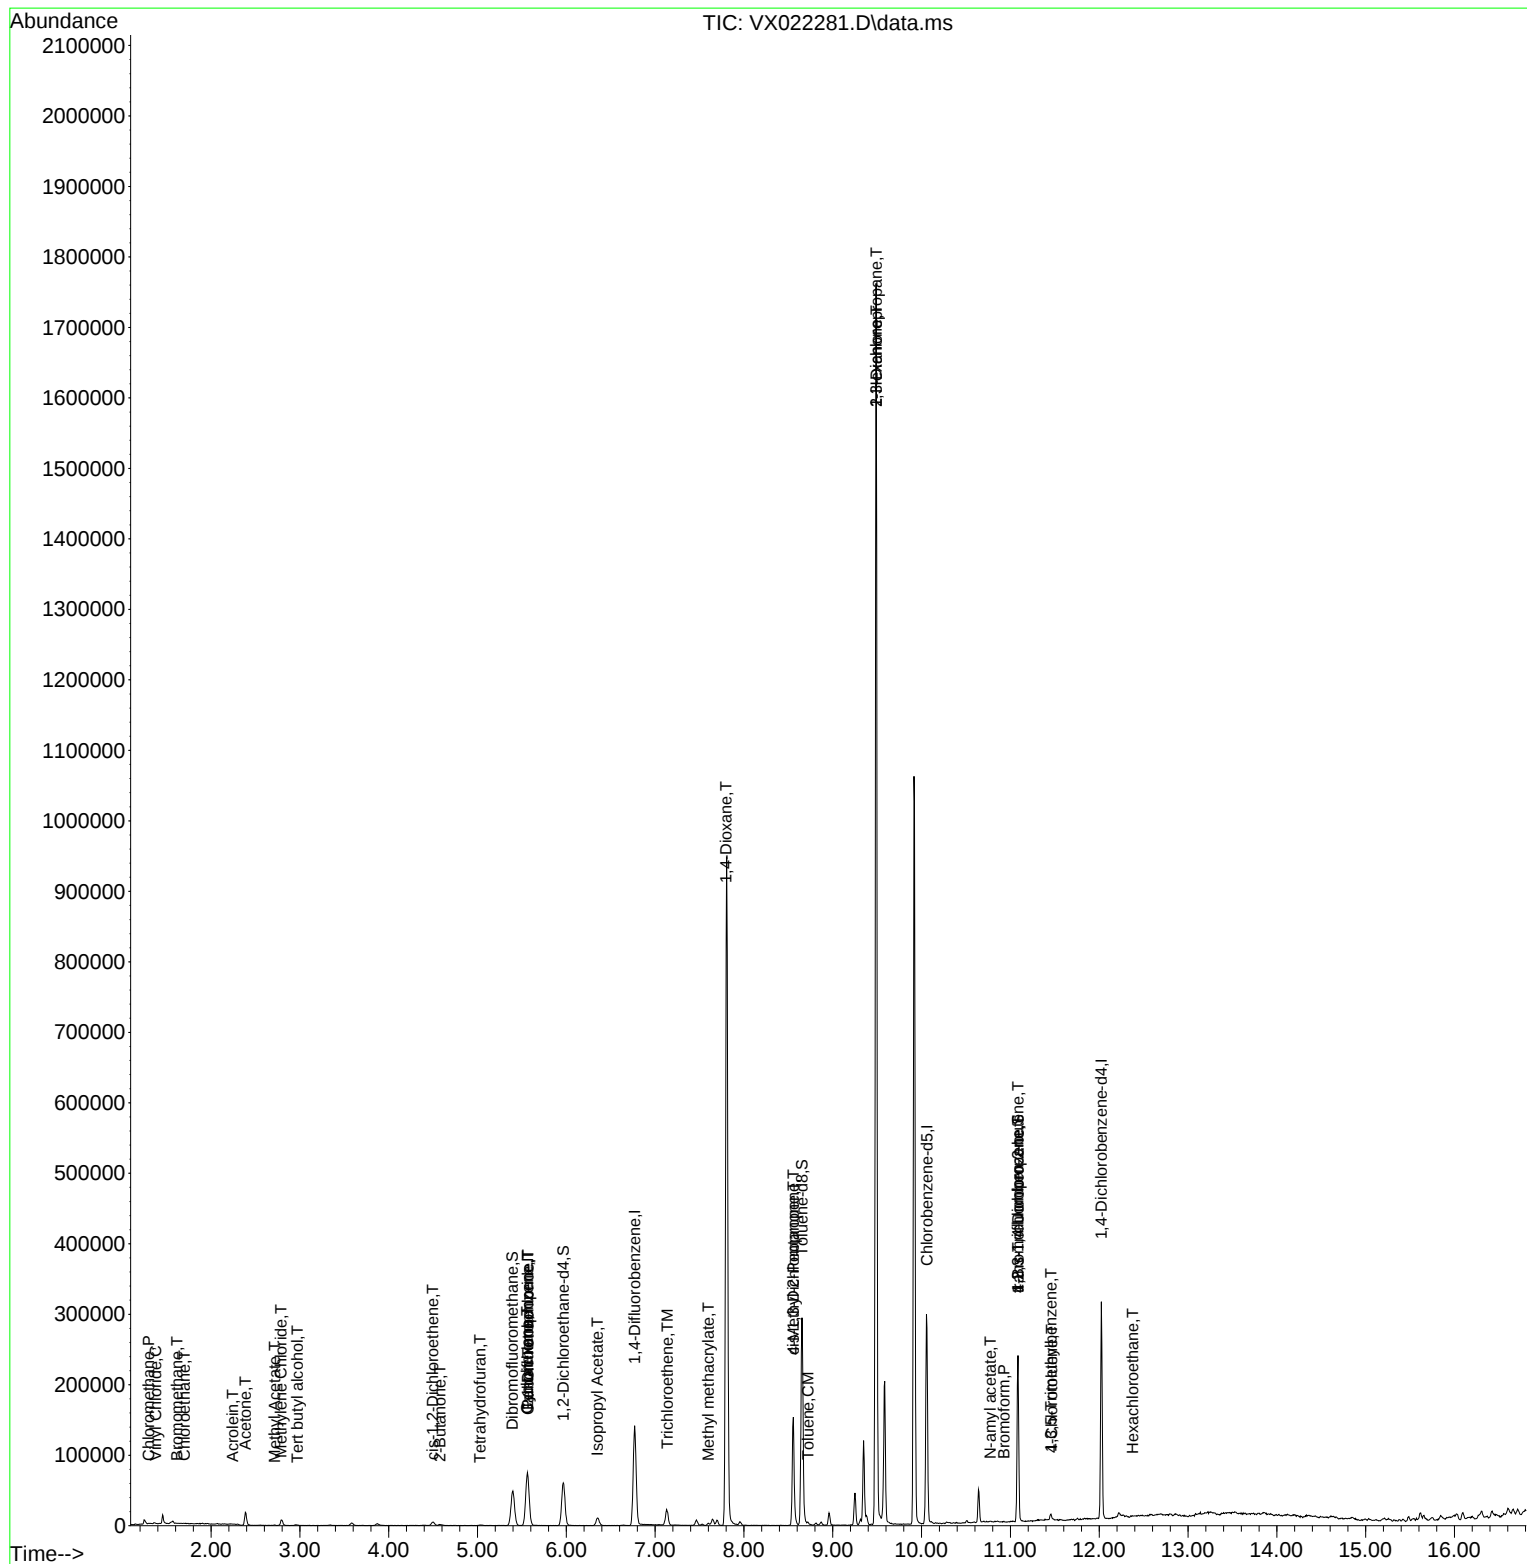






#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.000 min
Lab File: VX022281.D
Acq: 29 May 2021 03:27

Instrument :
MSVOA_X
ClientSampleId :
PB136709TB







Tgt Ion:168 Resp: 64245
Ion Ratio Lower Upper
168 100
99 70.1 45.8 68.6#

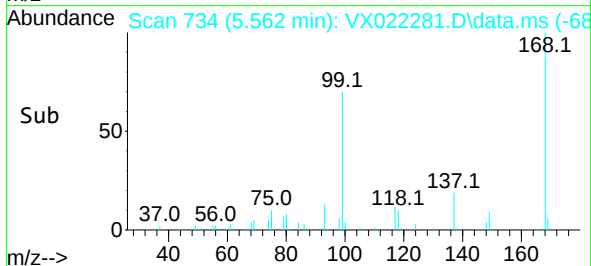

#3
Chloromethane
Concen: 0.48 ug/l
RT: 1.294 min Scan# 34
Delta R.T. -0.001 min
Lab File: VX022281.D
Acq: 29 May 2021 03:27

Tgt Ion: 50 Resp: 401
Ion Ratio Lower Upper
50 100
52 31.7 26.4 39.6


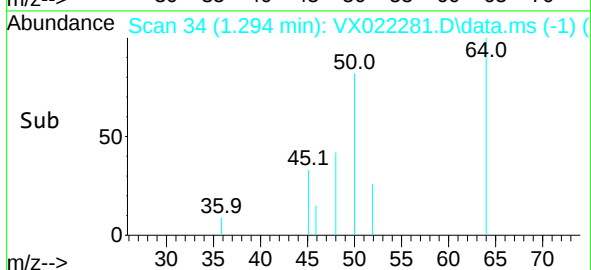

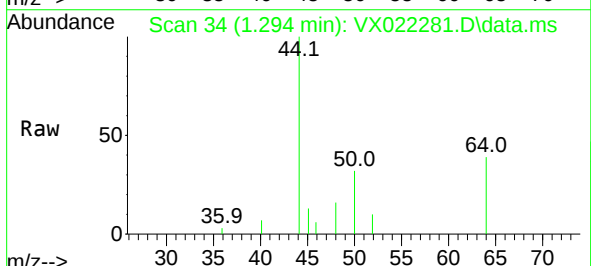


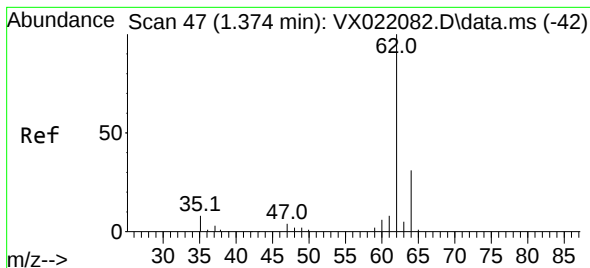

#4
 Vinyl Chloride
 Concen: 0.49 ug/l
 RT: 1.373 min Scan# 47
 Delta R.T. -0.001 min
 Lab File: VX022281.D
 Acq: 29 May 2021 03:27




Instrument :
 MSVOA_X
 ClientSampleID :
 PB136709TB


Tgt Ion: 62 Resp: 434
 Ion Ratio Lower Upper
 62 100
 64 61.1 25.7 38.5#

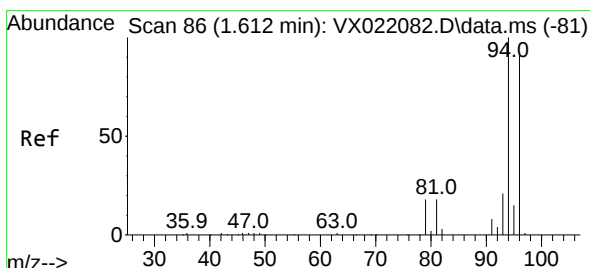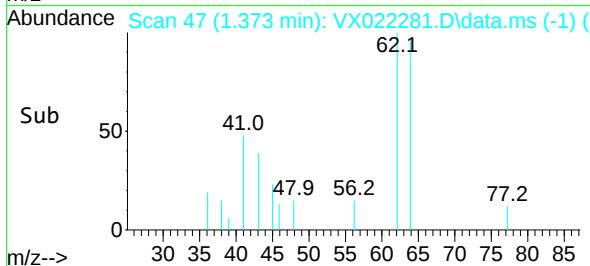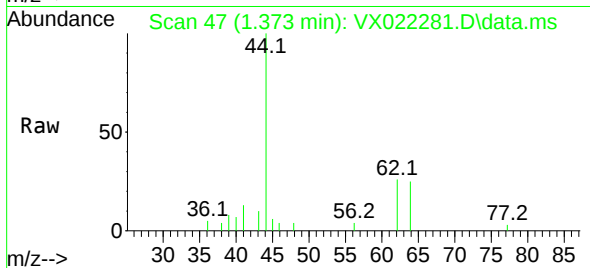

#5
 Bromomethane
 Concen: 0.38 ug/l
 RT: 1.617 min Scan# 87
 Delta R.T. 0.005 min
 Lab File: VX022281.D
 Acq: 29 May 2021 03:27

Tgt Ion: 94 Resp: 196
 Ion Ratio Lower Upper
 94 100
 96 112.5 76.4 114.6


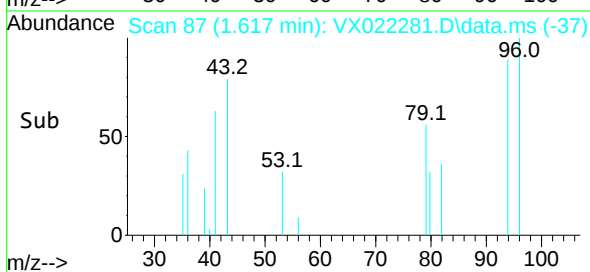

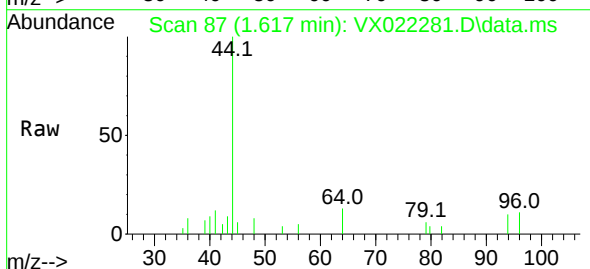


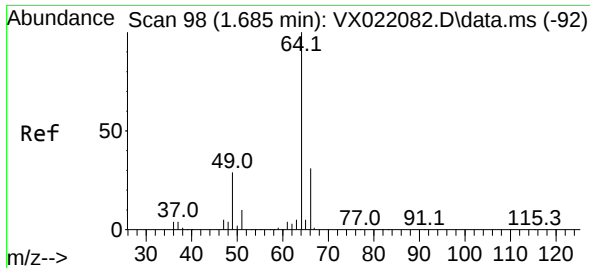

#6
Chloroethane
Concen: 0.21 ug/l
RT: 1.696 min Scan# 100
Delta R.T. 0.011 min
Lab File: VX022281.D
Acq: 29 May 2021 03:27




Instrument :
MSVOA_X
ClientSampleId :
PB136709TB


Tgt Ion: 64 Resp: 113
Ion Ratio Lower Upper
64 100
66 0.0 25.4 38.0#

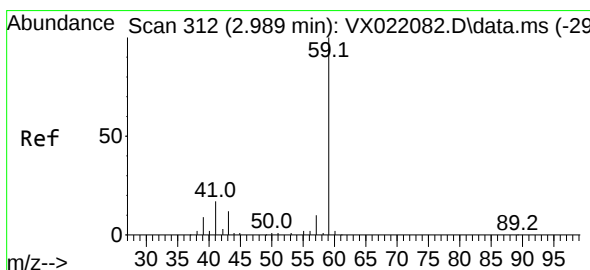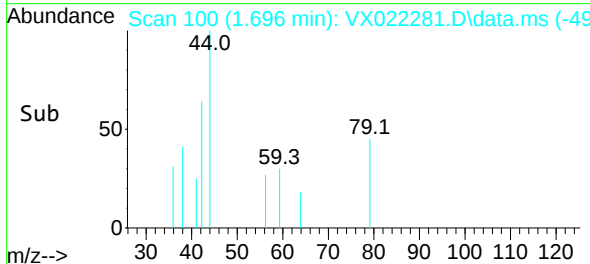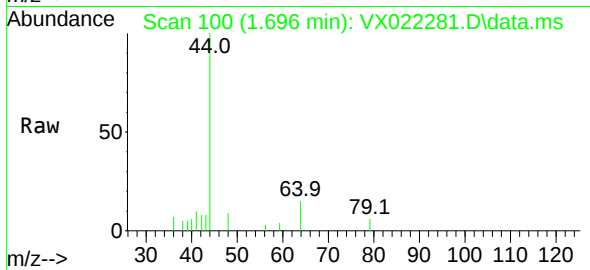

#11
Tert butyl alcohol
Concen: 2.11 ug/l
RT: 2.971 min Scan# 309
Delta R.T. -0.018 min
Lab File: VX022281.D
Acq: 29 May 2021 03:27

Tgt Ion: 59 Resp: 478
Ion Ratio Lower Upper
59 100
57 0.0 7.8 11.8#


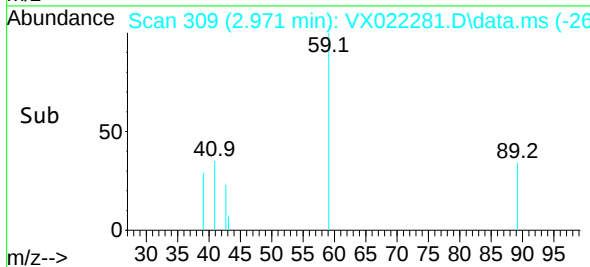

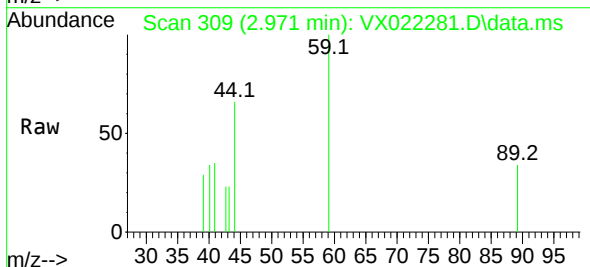




#13
Acrolein
Concen: 0.68 ug/l
RT: 2.239 min Scan# 189
Delta R.T. -0.001 min
Lab File: VX022281.D
Acq: 29 May 2021 03:27




Instrument :
MSVOA_X
ClientSampleId :
PB136709TB


Tgt Ion: 56 Resp: 102
Ion Ratio Lower Upper
56 100
55 215.7 56.4 84.6#

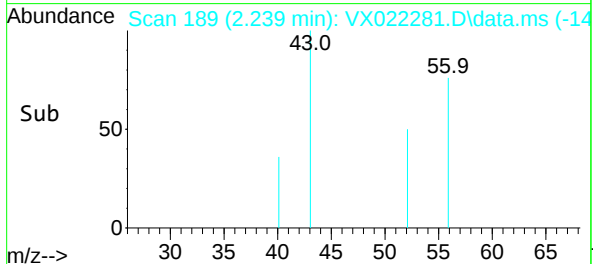

#16
Acetone
Concen: 44.31 ug/l
RT: 2.385 min Scan# 213
Delta R.T. -0.007 min
Lab File: VX022281.D
Acq: 29 May 2021 03:27


Tgt Ion: 43 Resp: 19119
Ion Ratio Lower Upper
43 100
58 29.6 27.8 41.8

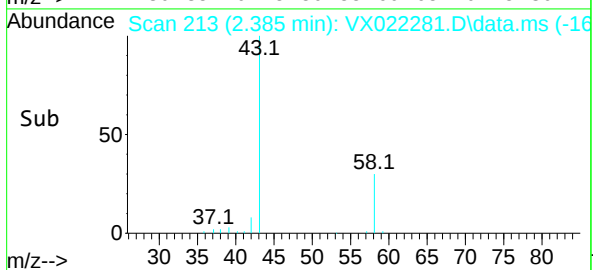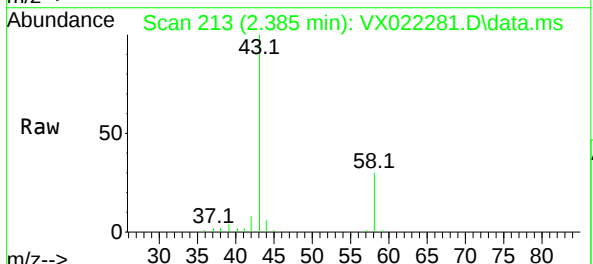






#18
Methyl Acetate
Concen: 0.78 ug/l
RT: 2.715 min Scan# 267
Delta R.T. 0.006 min
Lab File: VX022281.D
Acq: 29 May 2021 03:27

Instrument :
MSVOA_X
ClientSampleId :
PB136709TB



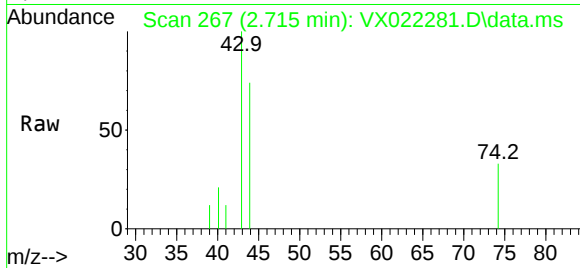



Tgt Ion: 43 Resp: 900
Ion Ratio Lower Upper
43 100
74 13.4 21.9 32.9#

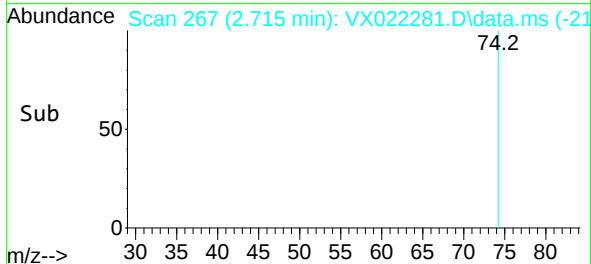

#20
Methylene Chloride
Concen: 3.80 ug/l
RT: 2.788 min Scan# 279
Delta R.T. -0.006 min
Lab File: VX022281.D
Acq: 29 May 2021 03:27

Tgt Ion: 84 Resp: 3639
Ion Ratio Lower Upper
84 100
49 106.3 88.6 132.8
51 36.7 27.0 40.6
86 54.3 50.3 75.5


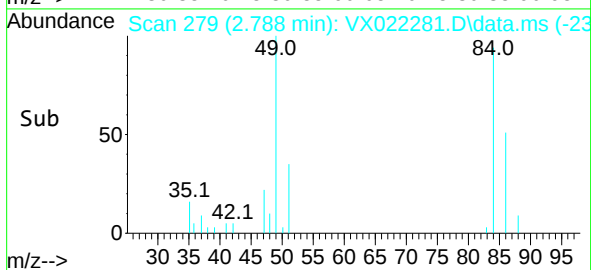

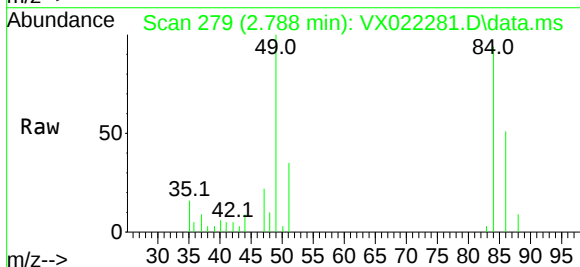




#25
2-Butanone
Concen: 3.97 ug/l
RT: 4.574 min Scan# 572
Delta R.T. 0.006 min
Lab File: VX022281.D
Acq: 29 May 2021 03:27




Instrument :
MSVOA_X
ClientSampleId :
PB136709TB


Tgt Ion: 43 Resp: 2770
Ion Ratio Lower Upper
43 100
72 16.3 23.7 35.5#

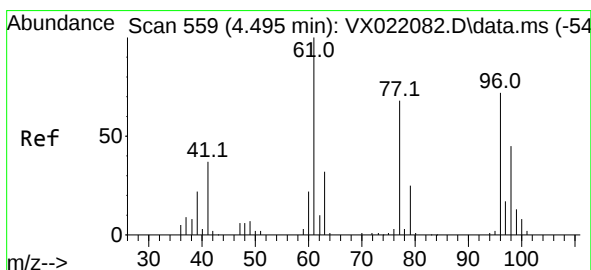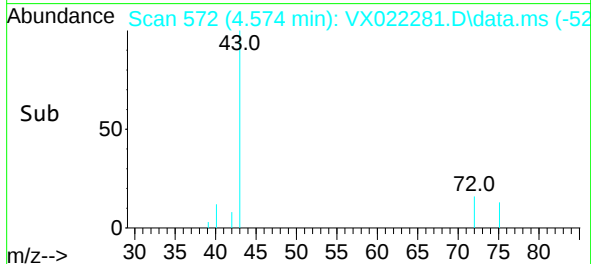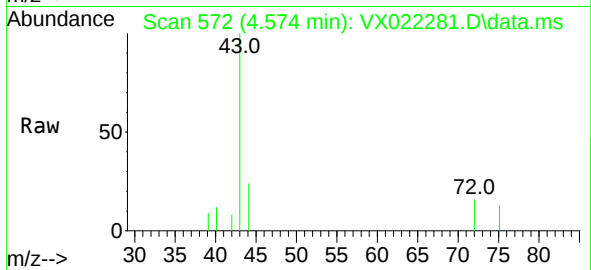

#27
cis-1,2-Dichloroethene
Concen: 3.29 ug/l
RT: 4.495 min Scan# 559
Delta R.T. -0.000 min
Lab File: VX022281.D
Acq: 29 May 2021 03:27

Tgt Ion: 96 Resp: 3206
Ion Ratio Lower Upper
96 100
61 127.5 0.0 285.6
98 67.6 0.0 129.6

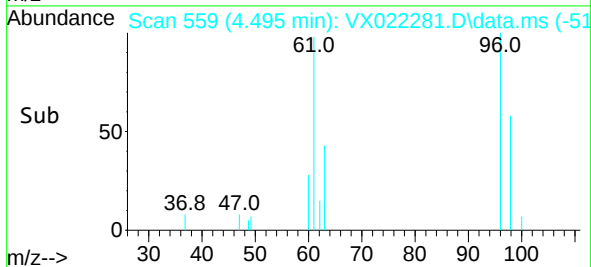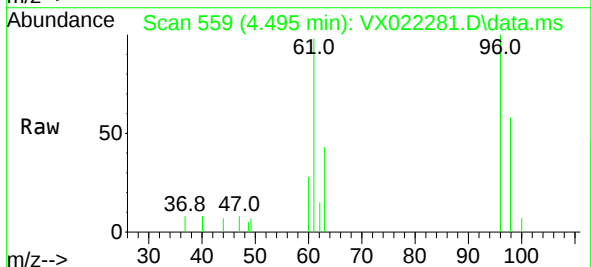

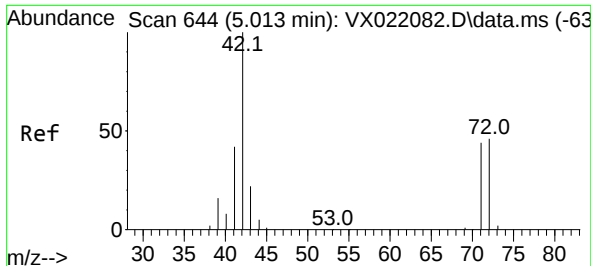

#29

Tetrahydrofuran

Concen: 0.76 ug/l

RT: 5.025 min Scan# 646





Delta R.T. 0.012 min

Lab File: VX022281.D

Acq: 29 May 2021 03:27

Tgt Ion:	42	Resp:	316
Ion	Ratio	Lower	Upper
42	100		
72	54.4	41.7	62.5
71	30.7	38.4	57.6

Instrument :
MSVOA_X
ClientSampleId :
PB136709TB

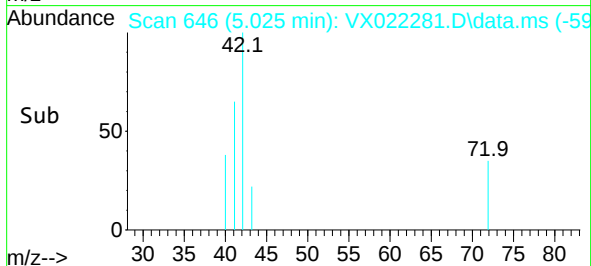

#31

Cyclohexane

Concen: 1.41 ug/l




RT: 5.556 min Scan# 733


Delta R.T. 0.073 min

Lab File: VX022281.D

Acq: 29 May 2021 03:27

Tgt Ion:	56	Resp:	1753
Ion	Ratio	Lower	Upper
56	100		
69	98.5	25.3	37.9
84	94.9	71.4	107.0

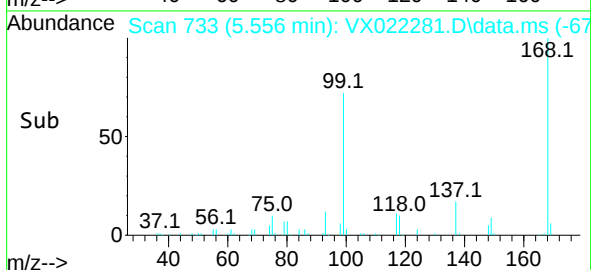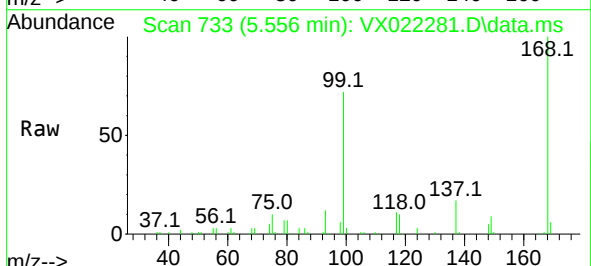

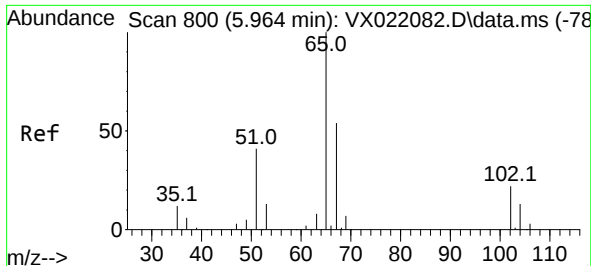

#33

1,2-Dichloroethane-d4

Concen: 55.84 ug/l

RT: 5.964 min Scan# 800

Delta R.T. 0.000 min

Lab File: VX022281.D





Acq: 29 May 2021 03:27

Tgt Ion: 65 Resp: 55343

Ion Ratio Lower Upper

65 100

67 52.8 0.0 105.4

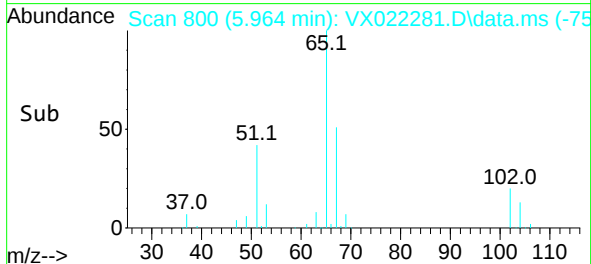

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 6.769 min Scan# 932

Delta R.T. -0.000 min

Lab File: VX022281.D

Acq: 29 May 2021 03:27




Tgt Ion: 114 Resp: 138745


Ion Ratio Lower Upper

114 100

63 20.9 0.0 40.8

88 17.6 0.0 32.8

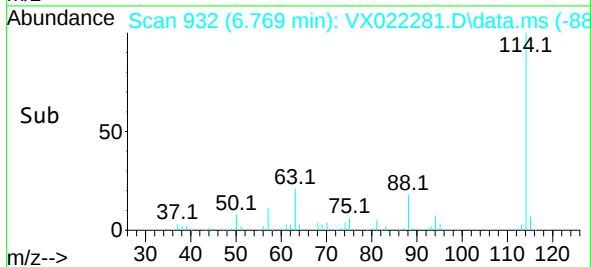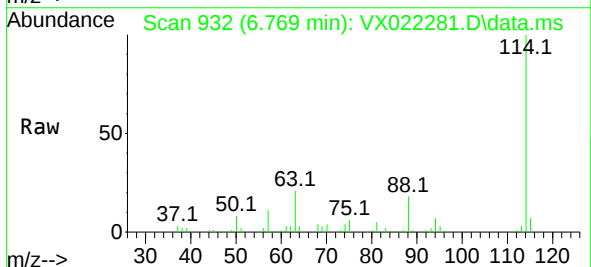

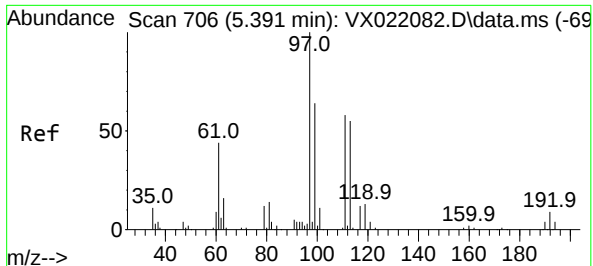

#35

Dibromofluoromethane

Concen: 47.35 ug/l

RT: 5.391 min Scan# 706





Delta R.T. -0.000 min

Lab File: VX022281.D

Acq: 29 May 2021 03:27

Tgt Ion:	113	Resp:	41661
Ion	Ratio	Lower	Upper
113	100		
111	105.2	81.9	122.9
192	16.0	16.7	25.1#

Instrument :
MSVOA_X
ClientSampleId :
PB136709TB

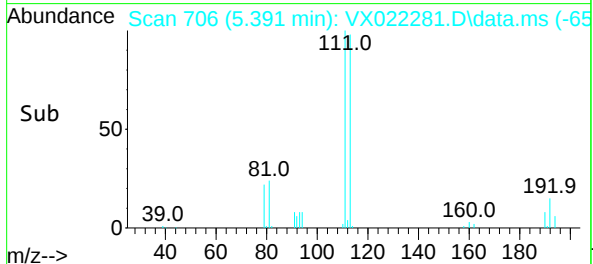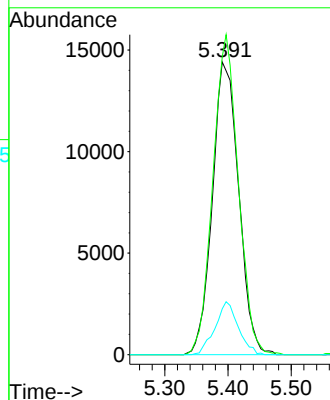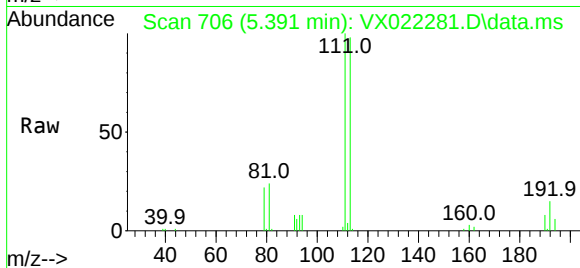

#36

1,1-Dichloropropene

Concen: 4.80 ug/l




RT: 5.562 min Scan# 734


Delta R.T. -0.140 min

Lab File: VX022281.D

Acq: 29 May 2021 03:27


Tgt Ion:	75	Resp:	6161
Ion	Ratio	Lower	Upper
75	100		
110	8.0	18.1	54.4#
77	0.0	25.3	37.9#

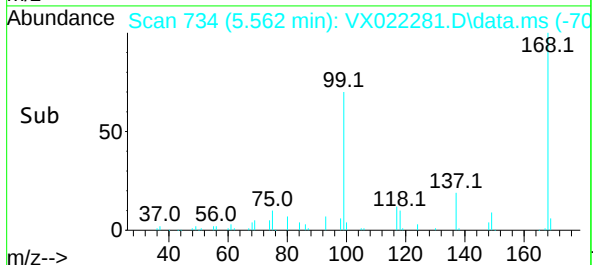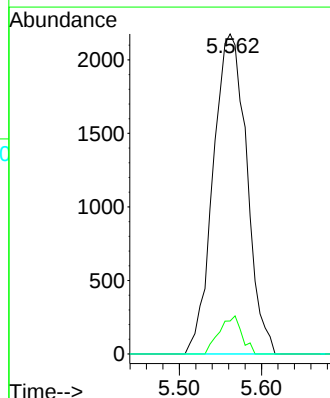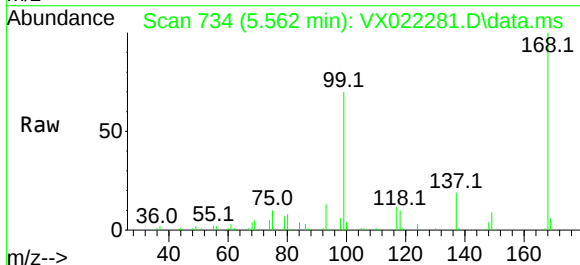



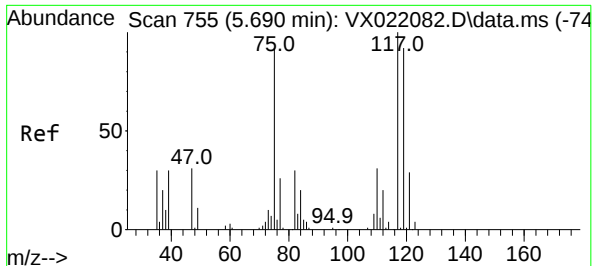


#38
Carbon Tetrachloride
Concen: 5.99 ug/l
RT: 5.568 min Scan# 735
Delta R.T. -0.122 min
Lab File: VX022281.D
Acq: 29 May 2021 03:27


Instrument :
MSVOA_X
ClientSampleId :
PB136709TB





Tgt Ion:117 Resp: 7518
Ion Ratio Lower Upper
117 100
119 4.8 76.2 114.2#
121 0.0 24.8 37.2#




#43
Isopropyl Acetate
Concen: 5.84 ug/l
RT: 6.348 min Scan# 863
Delta R.T. -0.001 min
Lab File: VX022281.D
Acq: 29 May 2021 03:27



Tgt Ion: 43 Resp: 15015
Ion Ratio Lower Upper
43 100
61 19.3 18.2 27.4
87 13.3 12.5 18.7




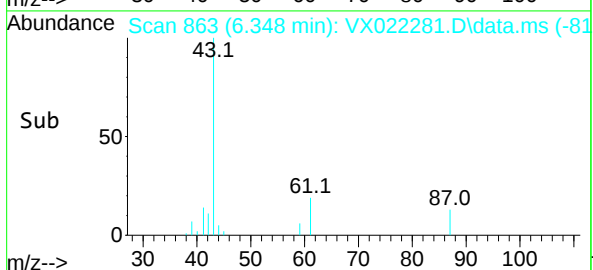




#44
Trichloroethene
Concen: 7.48 ug/l
RT: 7.135 min Scan# 992
Delta R.T. 0.006 min
Lab File: VX022281.D
Acq: 29 May 2021 03:27




Instrument :
MSVOA_X
ClientSampleId :
PB136709TB


Tgt Ion:130 Resp: 7335
Ion Ratio Lower Upper
130 100
95 104.9 0.0 198.0

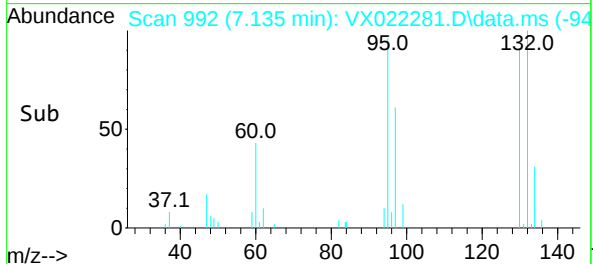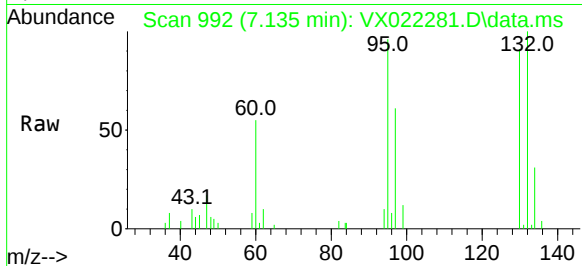

#48
Methyl methacrylate
Concen: 3.70 ug/l
RT: 7.598 min Scan# 1068
Delta R.T. -0.098 min
Lab File: VX022281.D
Acq: 29 May 2021 03:27

Tgt Ion: 41 Resp: 4386
Ion Ratio Lower Upper
41 100
69 0.0 76.0 114.0#
39 0.0 44.6 67.0#

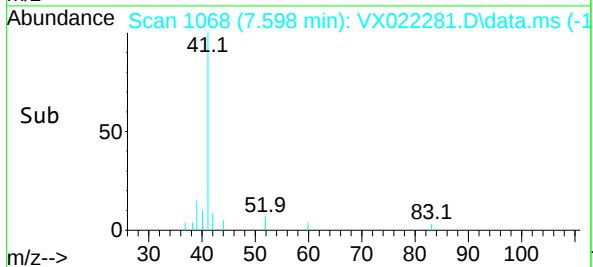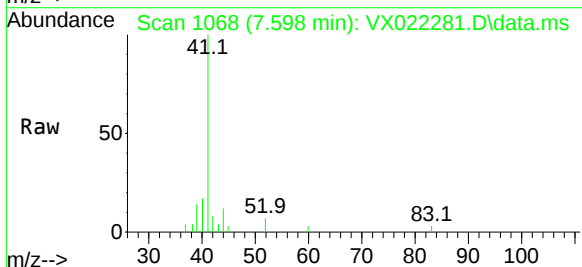



#49

1,4-Dioxane

Concen: 1.39 ug/l

RT: 7.799 min Scan# 1101

Delta R.T. 0.115 min

Lab File: VX022281.D

Acq: 29 May 2021 03:27





Tgt Ion: 88 Resp: 32

Ion Ratio Lower Upper

88 100

43 2718503.1 23.2 34.8#

58 10768.8 55.0 82.4#

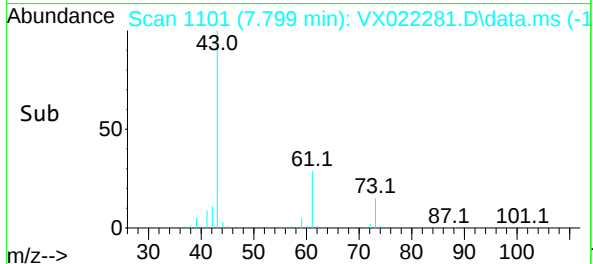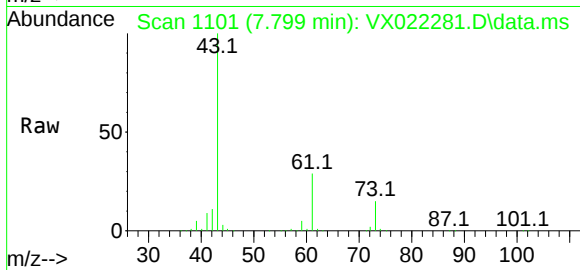

#50

Toluene-d8

Concen: 50.65 ug/l

RT: 8.653 min Scan# 1241

Delta R.T. -0.000 min

Lab File: VX022281.D




Acq: 29 May 2021 03:27

Tgt Ion: 98 Resp: 171670

Ion Ratio Lower Upper

98 100

100 67.3 51.9 77.9

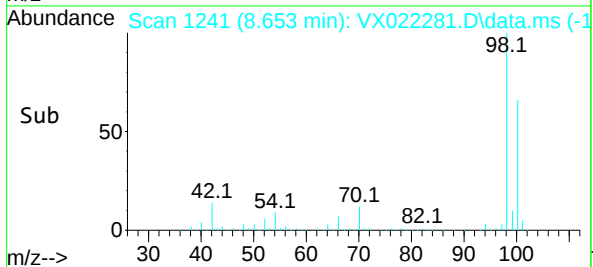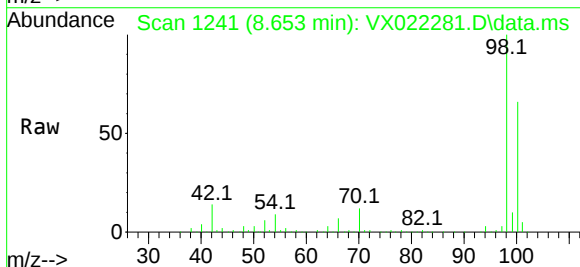


Instrument :

MSVOA_X

ClientSampleId :





PB136709TB



#51
4-Methyl-2-Pentanone
Concen: 34.85 ug/l
RT: 8.555 min Scan# 1225
Delta R.T. -0.025 min
Lab File: VX022281.D
Acq: 29 May 2021 03:27




Instrument :
MSVOA_X
ClientSampleId :
PB136709TB


Tgt Ion: 43 Resp: 53707
Ion Ratio Lower Upper
43 100
58 8.6 35.4 53.0#

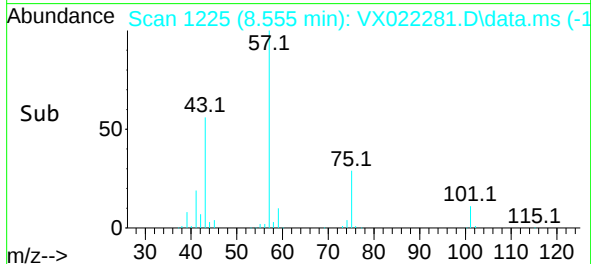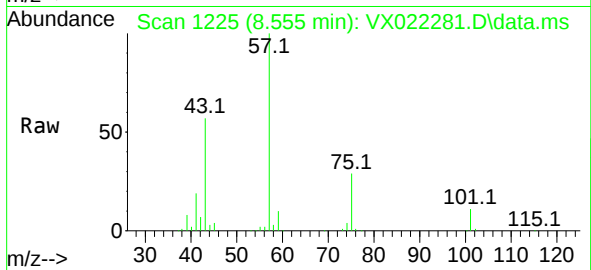

#52
Toluene
Concen: 0.23 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. -0.006 min
Lab File: VX022281.D
Acq: 29 May 2021 03:27

Tgt Ion: 92 Resp: 573
Ion Ratio Lower Upper
92 100
91 192.1 137.1 205.7


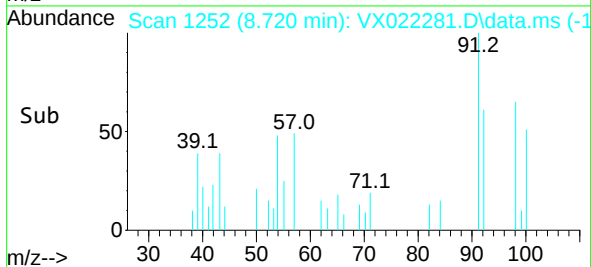

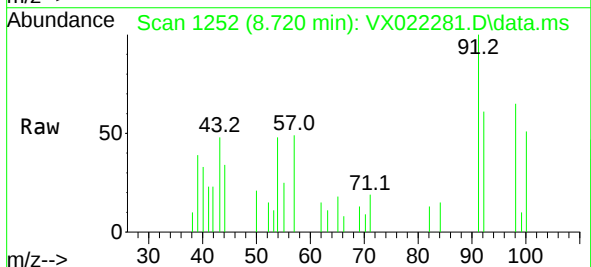




#54
cis-1,3-Dichloropropene
Concen: 14.83 ug/l
RT: 8.555 min Scan# 1225
Delta R.T. 0.182 min
Lab File: VX022281.D
Acq: 29 May 2021 03:27




Instrument :
MSVOA_X
ClientSampleId :
PB136709TB


Tgt Ion: 75 Resp: 25160
Ion Ratio Lower Upper
75 100
77 0.8 25.7 38.5#
39 27.7 35.1 52.7#

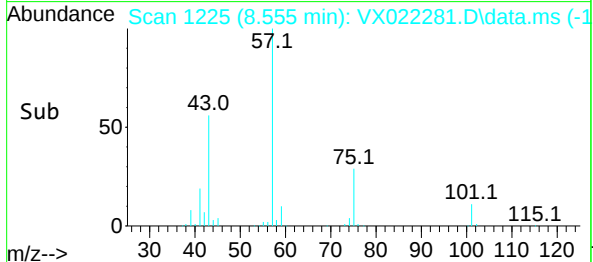

#57
1,3-Dichloropropane
Concen: 8.75 ug/l
RT: 9.488 min Scan# 1378
Delta R.T. 0.177 min
Lab File: VX022281.D
Acq: 29 May 2021 03:27

Tgt Ion: 76 Resp: 15161
Ion Ratio Lower Upper
76 100
78 0.0 26.2 39.2#


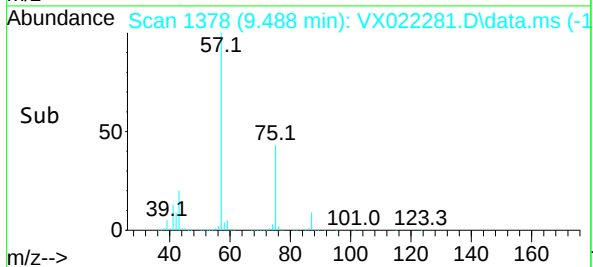

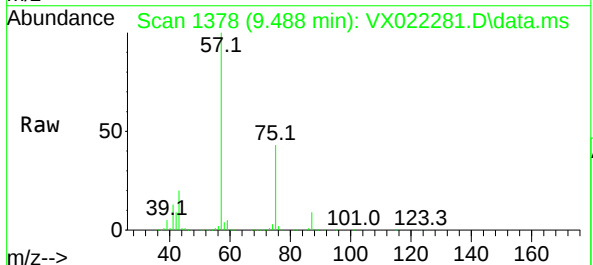




#59
2-Hexanone
Concen: 174.10 ug/l
RT: 9.488 min Scan# 1378
Delta R.T. 0.055 min
Lab File: VX022281.D
Acq: 29 May 2021 03:27




Instrument :
MSVOA_X
ClientSampled :
PB136709TB


Tgt Ion: 43 Resp: 201768
Ion Ratio Lower Upper
43 100
58 19.2 30.9 92.8#

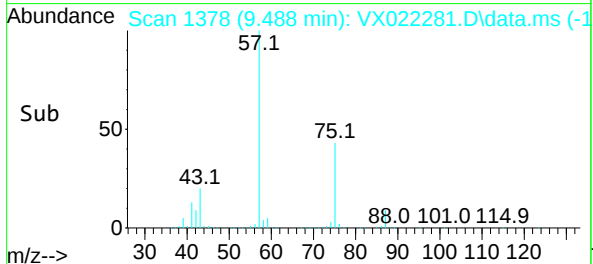

#62
4-Bromofluorobenzene
Concen: 52.06 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX022281.D
Acq: 29 May 2021 03:27

Tgt Ion: 95 Resp: 65216
Ion Ratio Lower Upper
95 100
174 63.6 0.0 154.6
176 60.8 0.0 155.8


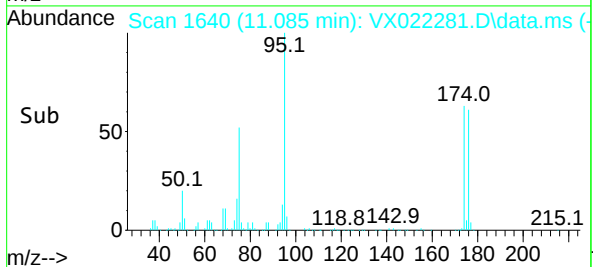

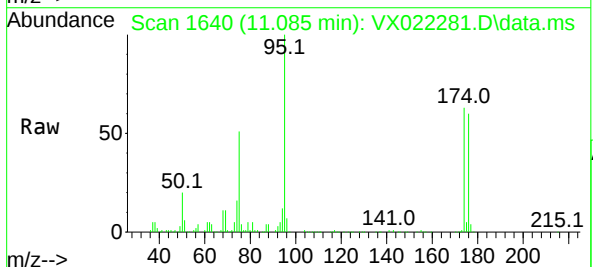




#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.061 min Scan# 1472
Delta R.T. -0.000 min
Lab File: VX022281.D
Acq: 29 May 2021 03:27




Instrument :
MSVOA_X
ClientSampleId :
PB136709TB


Tgt Ion:117 Resp: 127908
Ion Ratio Lower Upper
117 100
82 59.0 47.4 71.2
119 30.9 26.6 39.8

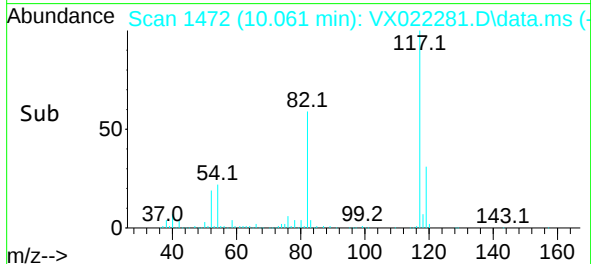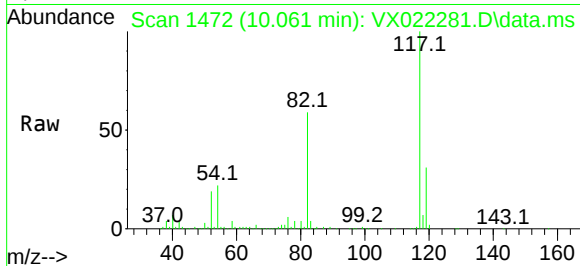

#71
Bromoform
Concen: 1.44 ug/l
RT: 10.927 min Scan# 1614
Delta R.T. 0.122 min
Lab File: VX022281.D
Acq: 29 May 2021 03:27

Tgt Ion:173 Resp: 21
Ion Ratio Lower Upper
173 100
175 0.0 23.9 71.8#
254 0.0 0.1 0.1#


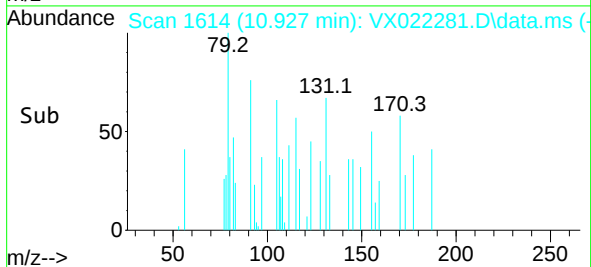

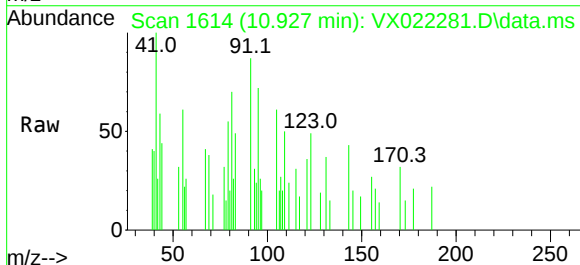




#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX022281.D
Acq: 29 May 2021 03:27




Instrument :
MSVOA_X
ClientSampleId :
PB136709TB


Tgt Ion:152 Resp: 56484
Ion Ratio Lower Upper
152 100
115 68.5 41.1 123.3
150 159.4 0.0 349.0

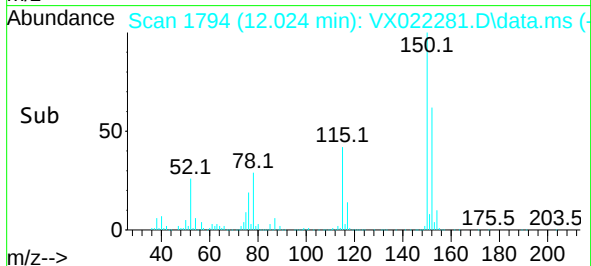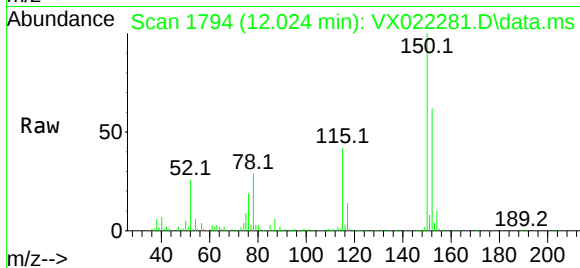

#74
N-ethyl acetate
Concen: 0.36 ug/l
RT: 10.774 min Scan# 1589
Delta R.T. -0.074 min
Lab File: VX022281.D
Acq: 29 May 2021 03:27

Tgt Ion: 43 Resp: 813
Ion Ratio Lower Upper
43 100
70 0.0 39.0 58.6#
55 60.5 21.5 32.3#
61 0.0 22.1 33.1#


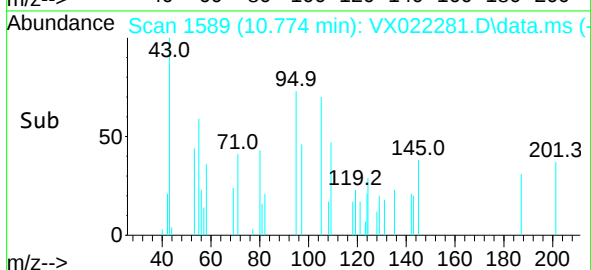
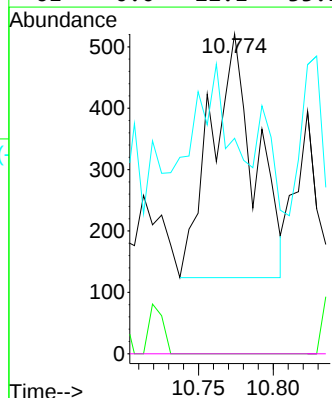
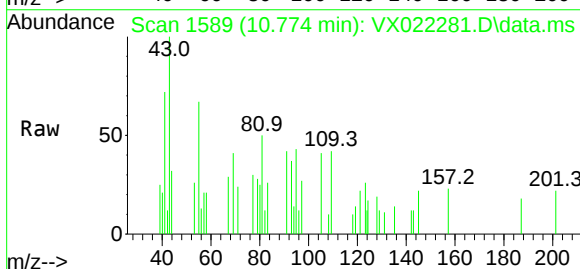


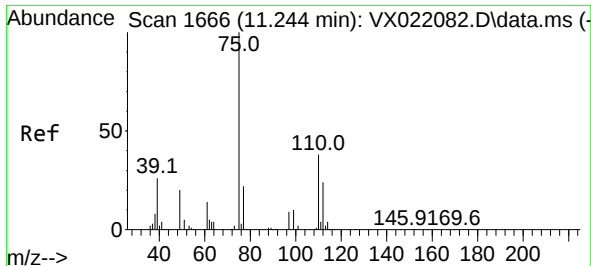

#76
1,2,3-Trichloropropane
Concen: 24.32 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. -0.159 min
Lab File: VX022281.D
Acq: 29 May 2021 03:27




Instrument :
MSVOA_X
ClientSampleId :
PB136709TB


Tgt Ion: 75 Resp: 33887
Ion Ratio Lower Upper
75 100
77 2.1 19.1 57.5#

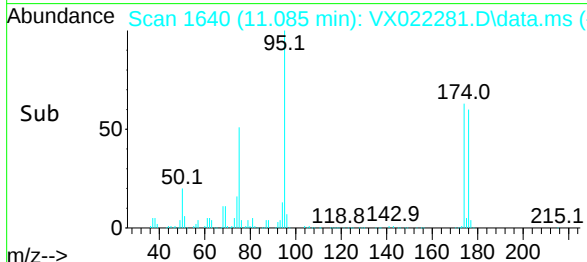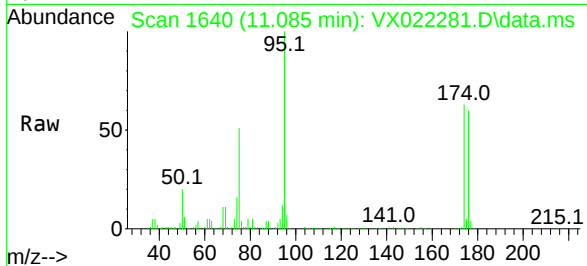

#80
1,3,5-Trimethylbenzene
Concen: 0.90 ug/l
RT: 11.457 min Scan# 1701
Delta R.T. -0.000 min
Lab File: VX022281.D
Acq: 29 May 2021 03:27

Tgt Ion:105 Resp: 3560
Ion Ratio Lower Upper
105 100
120 55.1 23.8 71.5


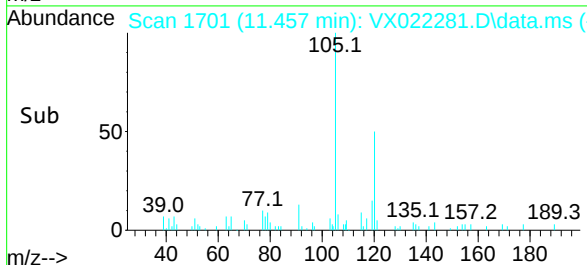

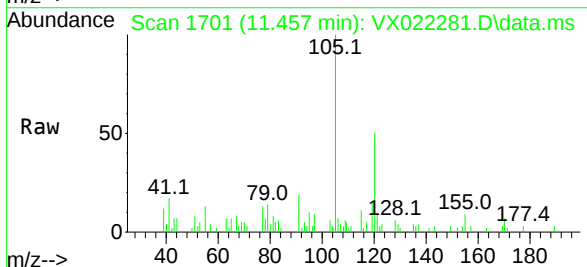




#81
trans-1,4-Dichloro-2-butene
Concen: 57.62 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.060 min
Lab File: VX022281.D
Acq: 29 May 2021 03:27




Instrument :
MSVOA_X
ClientSampleId :
PB136709TB


Tgt Ion: 75 Resp: 33887
Ion Ratio Lower Upper
75 100
53 0.4 74.5 111.7#
89 0.1 37.9 56.9#

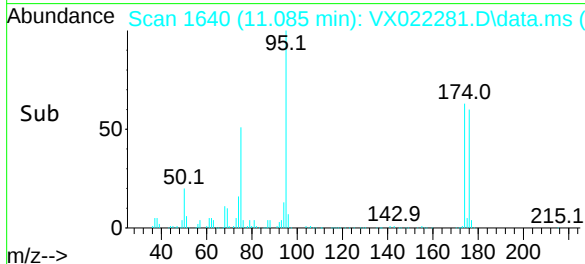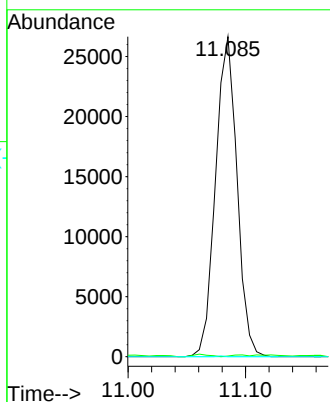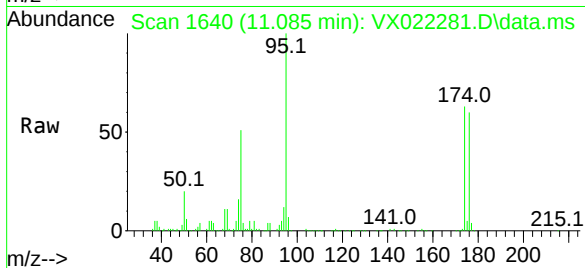

#82
4-Chlorotoluene
Concen: 0.28 ug/l
RT: 11.463 min Scan# 1702
Delta R.T. 0.006 min
Lab File: VX022281.D
Acq: 29 May 2021 03:27


Tgt Ion: 91 Resp: 1111
Ion Ratio Lower Upper
91 100
126 0.0 14.9 44.5#

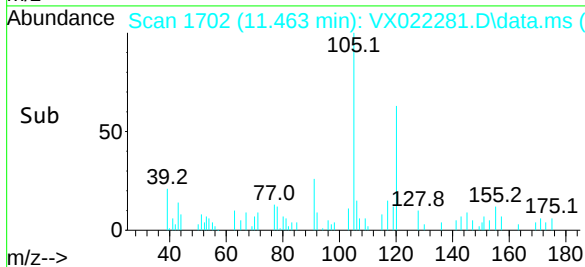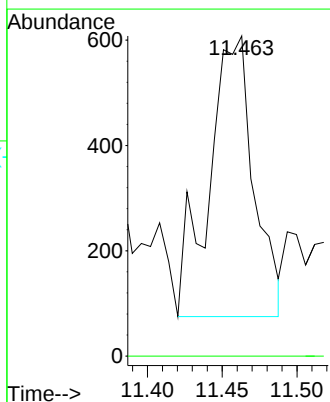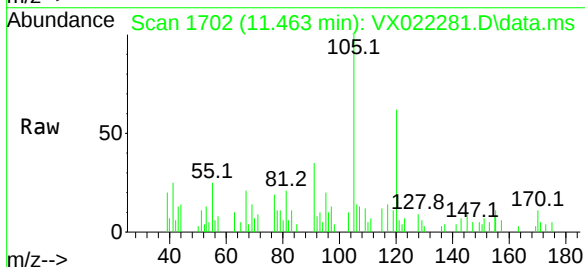

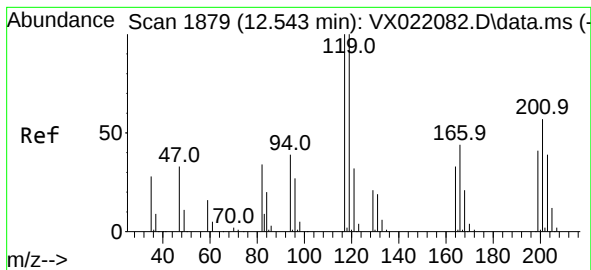

#90
Hexachloroethane
Concen: 0.26 ug/l
RT: 12.377 min Scan# 1852
Delta R.T. -0.166 min
Lab File: VX022281.D
Acq: 29 May 2021 03:27

Instrument :
MSVOA_X
ClientSampleId :
PB136709TB

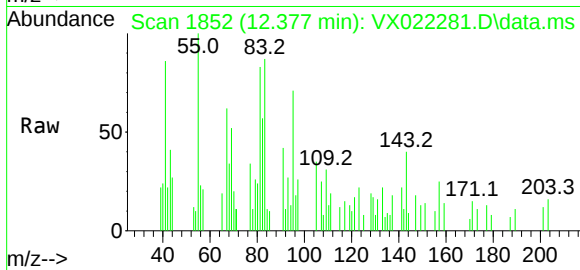

Tgt Ion:117 Resp: 172
Ion Ratio Lower Upper
117 100
201 61.6 40.4 121.2

