


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052921\
Data File : VX022248.D
Acq On : 28 May 2021 09:50
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X051321W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Thu May 13 06:11:35 2021

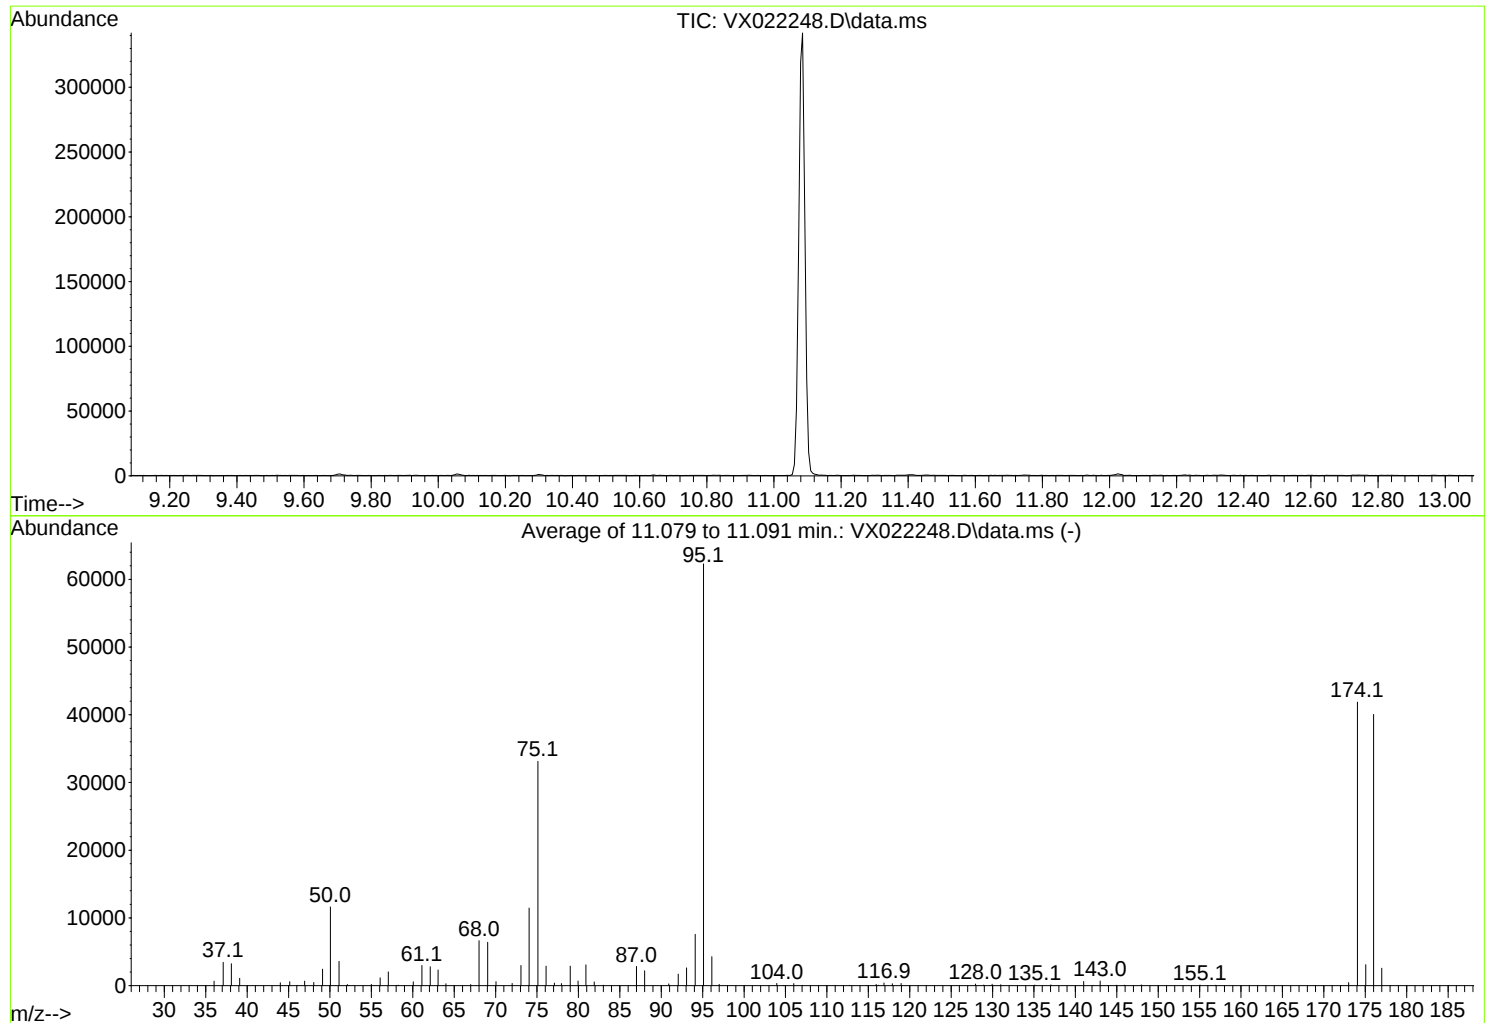

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1633

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.7	11625	PASS
75	95	30	60	53.2	33128	PASS
95	95	100	100	100.0	62285	PASS
96	95	5	9	6.9	4271	PASS
173	174	0.00	2	1.1	454	PASS
174	95	50	100	67.2	41875	PASS
175	174	5	9	7.4	3089	PASS
176	174	95	101	95.6	40048	PASS
177	176	5	9	6.4	2568	PASS