

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052921\
Data File : VX022258.D
Acq On : 28 May 2021 17:10
Operator : JC/MD
Sample : M2483-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DSN-001-SEWER-OUTLET-001

Integration Parameters: RTEINT3.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X051321W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

Signal : TIC: VX022258.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.386	206	213	222	rBV	42254	69344	6.90%	2.854%
2	2.550	231	240	259	rBV	570116	1005161	100.00%	41.375%
3	4.910	612	627	641	rBV2	41216	121221	12.06%	4.990%
4	5.105	648	659	673	rVB2	33492	97025	9.65%	3.994%
5	5.964	786	800	811	rBV	43437	117133	11.65%	4.821%
6	6.769	921	932	943	rBV	98661	230938	22.98%	9.506%
7	7.830	1099	1106	1111	rBV	13161	23592	2.35%	0.971%
8	8.653	1234	1241	1251	rBV	207636	316415	31.48%	13.024%
9	10.055	1465	1471	1478	rBV	191906	262371	26.10%	10.800%
10	11.085	1634	1640	1651	rVB	143444	186202	18.52%	7.665%




Sum of corrected areas: 2429402

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052921\
Data File : VX022258.D
Acq On : 28 May 2021 17:10
Operator : JC/MD
Sample : M2483-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DSN-001-SEWER-OUTLET-001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X051321W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library :
TIC Integration Parameters: RTEINT3.P

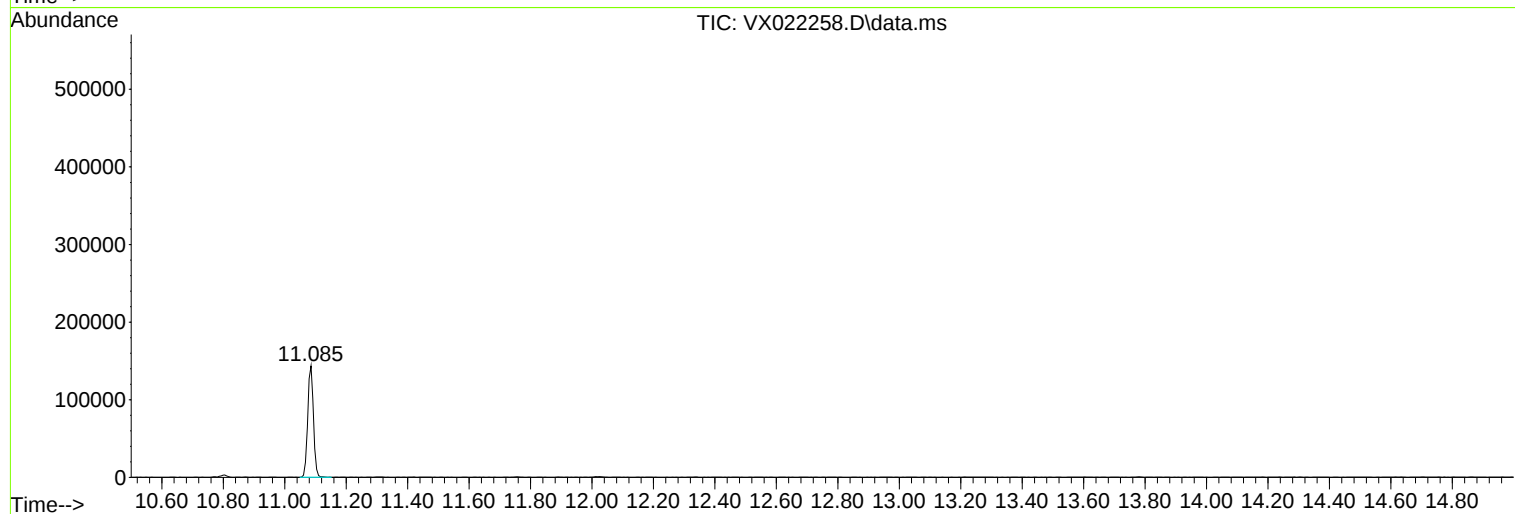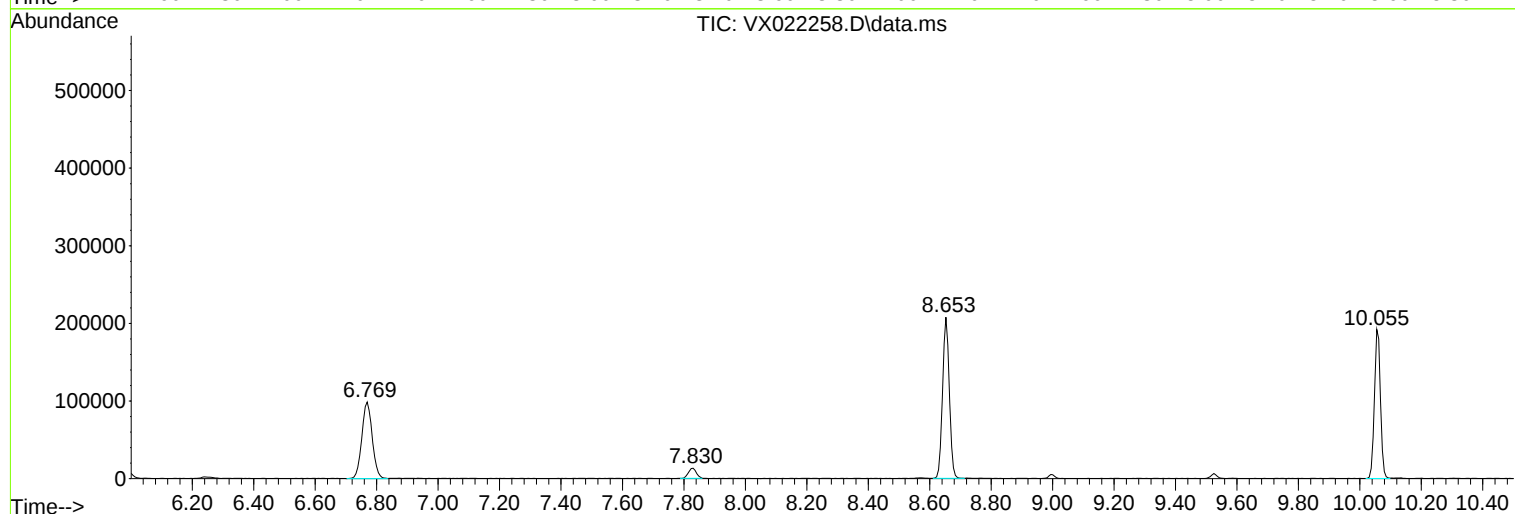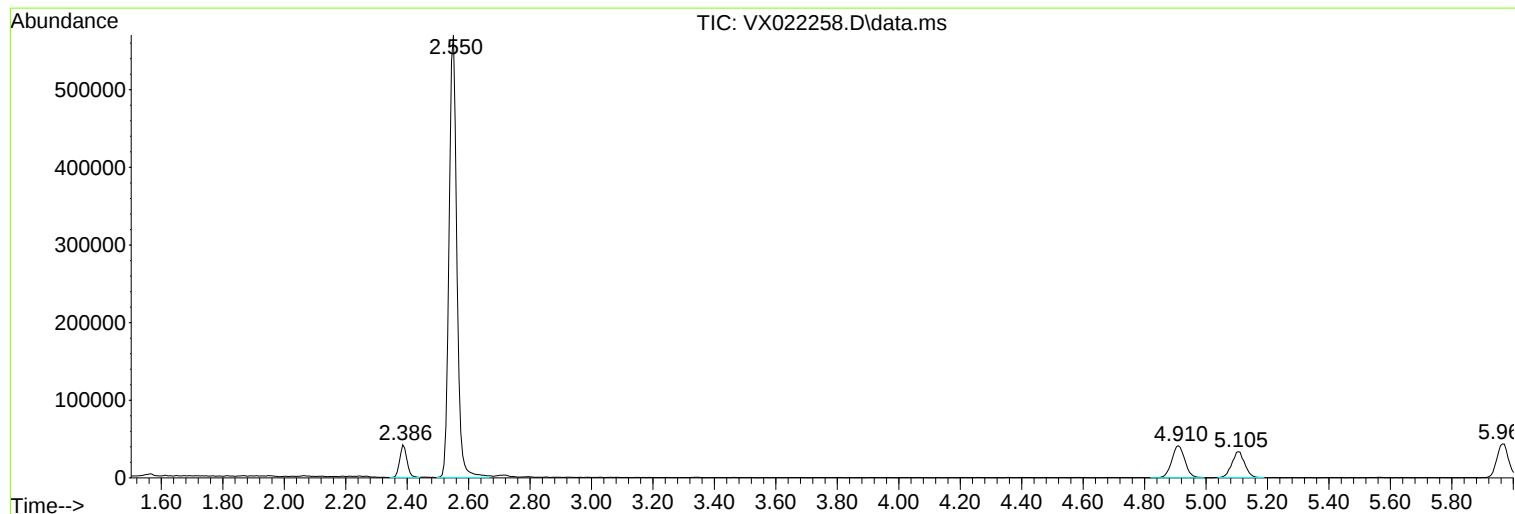

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052921\
Data File : VX022258.D
Acq On : 28 May 2021 17:10
Operator : JC/MD
Sample : M2483-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DSN-001-SEWER-OUTLET-001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X051321W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library :
TIC Integration Parameters: RTEINT3.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052921\
Data File : VX022258.D
Acq On : 28 May 2021 17:10
Operator : JC/MD
Sample : M2483-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DSN-001-SEWER-OUTLET-001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\624X051321W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library :
TIC Integration Parameters: RTEINT3.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------