

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX052921\  
 Data File : VX022268.D  
 Acq On : 28 May 2021 22:21  
 Operator : JC/MD  
 Sample : M2561-01  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 24 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 TB02-20210526

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X051921W.M

Title : SW846 8260

Signal : TIC: VX022268.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 2.386       | 209           | 213         | 218          | rBV      | 3420           | 4919          | 1.04%           | 0.207%        |
| 2         | 2.544       | 230           | 239         | 247          | rBV      | 9392           | 18619         | 3.94%           | 0.783%        |
| 3         | 2.794       | 273           | 280         | 286          | rBV4     | 4005           | 7664          | 1.62%           | 0.322%        |
| 4         | 2.867       | 286           | 292         | 300          | rVB      | 7611           | 14364         | 3.04%           | 0.604%        |
| 5         | 5.391       | 695           | 706         | 718          | rBV      | 49472          | 142784        | 30.20%          | 6.004%        |
| 6         | 5.562       | 721           | 734         | 750          | rVB2     | 79679          | 220729        | 46.69%          | 9.282%        |
| 7         | 5.964       | 789           | 800         | 813          | rBV      | 64343          | 165104        | 34.93%          | 6.943%        |
| 8         | 6.769       | 922           | 932         | 942          | rBV      | 141010         | 337136        | 71.32%          | 14.177%       |
| 9         | 8.653       | 1234          | 1241        | 1249         | rBV      | 311967         | 472724        | 100.00%         | 19.879%       |
| 10        | 8.720       | 1249          | 1252        | 1257         | rVB2     | 4163           | 6270          | 1.33%           | 0.264%        |
| 11        | 10.055      | 1466          | 1471        | 1487         | rVB      | 293712         | 394043        | 83.36%          | 16.571%       |
| 12        | 11.085      | 1634          | 1640        | 1649         | rBV      | 214815         | 271234        | 57.38%          | 11.406%       |
| 13        | 12.024      | 1789          | 1794        | 1802         | rBV      | 266836         | 322377        | 68.20%          | 13.557%       |




Sum of corrected areas: 2377967

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX052921\  
Data File : VX022268.D  
Acq On : 28 May 2021 22:21  
Operator : JC/MD  
Sample : M2561-01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 24 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
TB02-20210526

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X051921W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

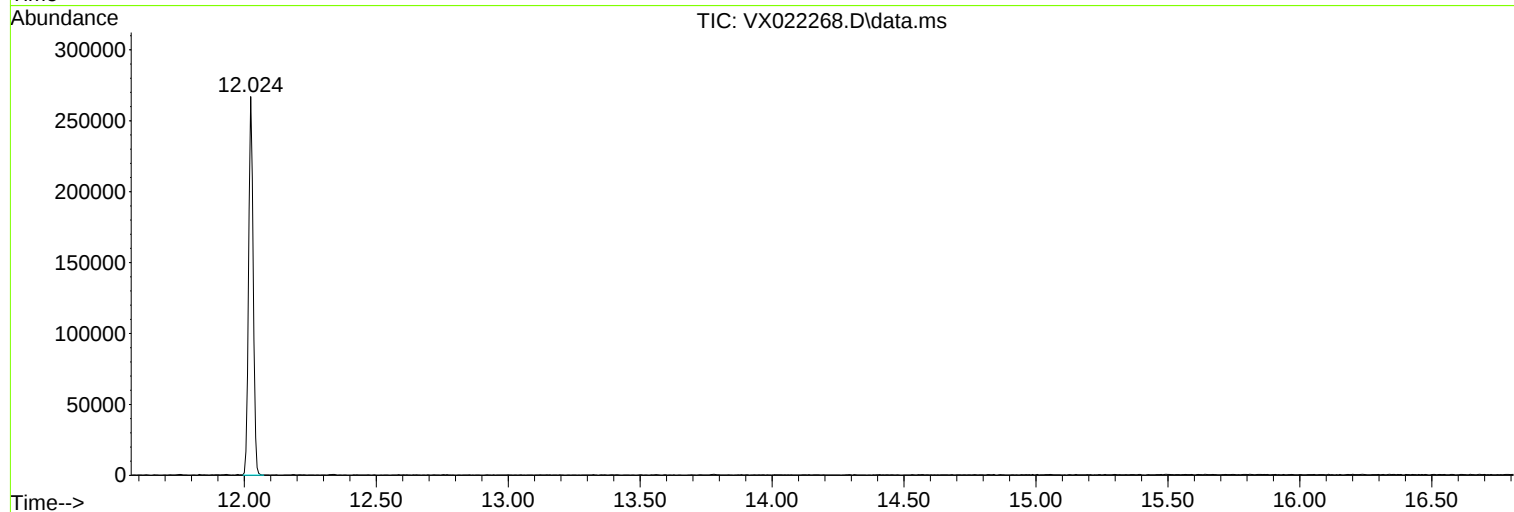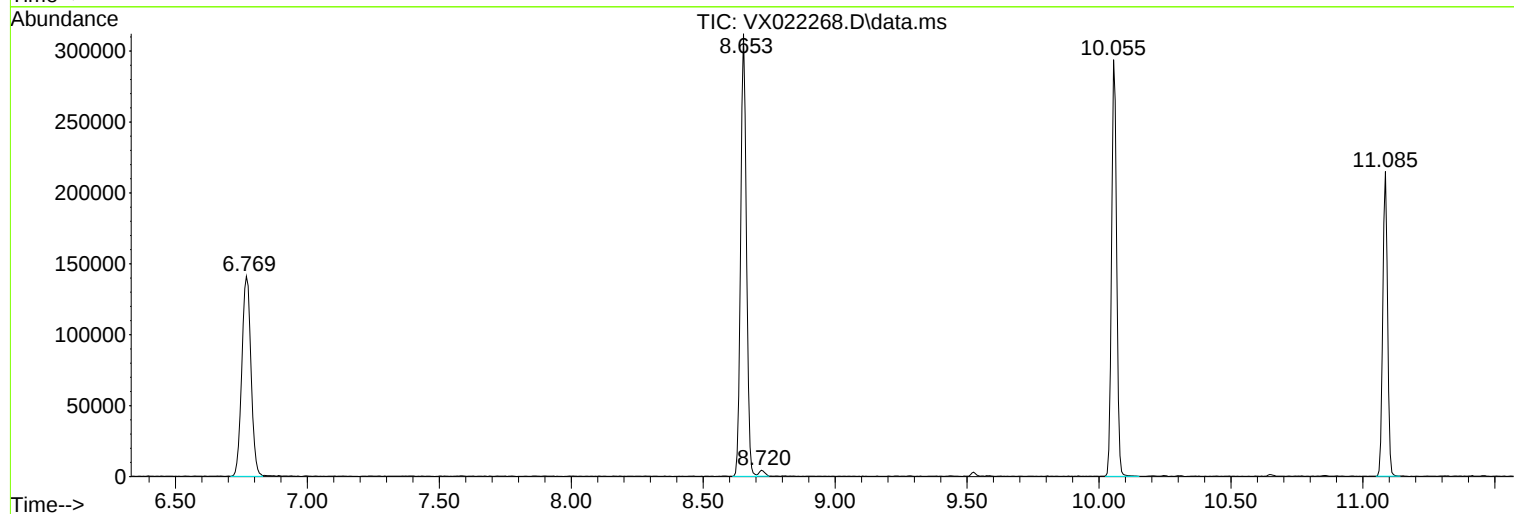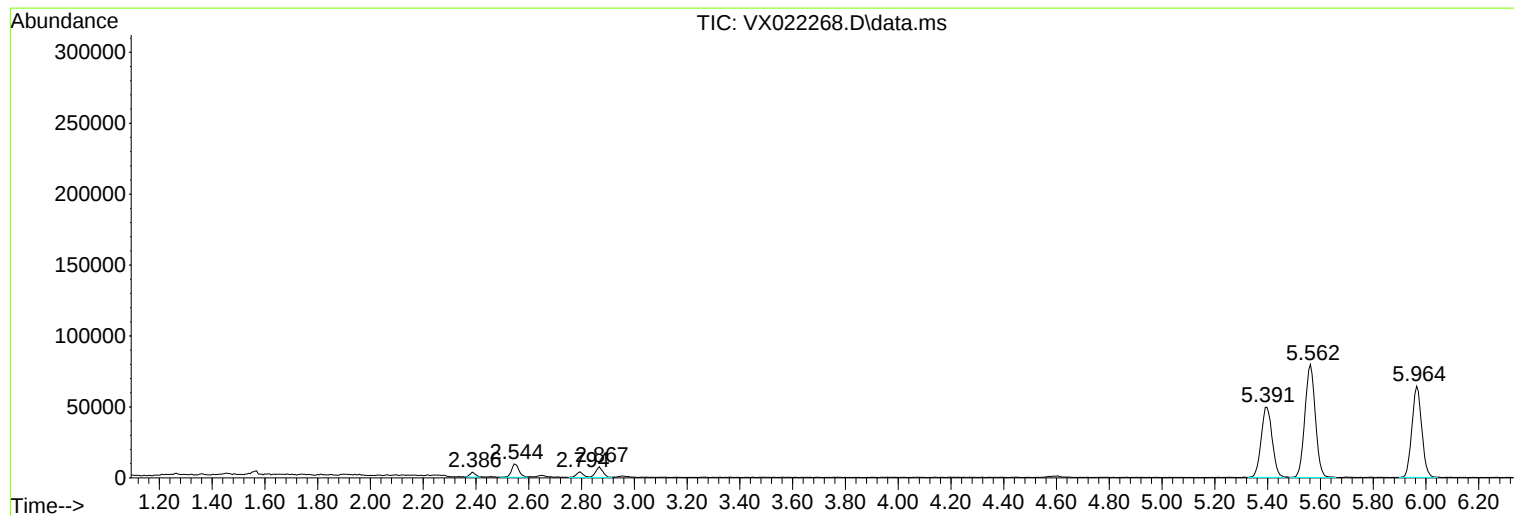

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX052921\  
Data File : VX022268.D  
Acq On : 28 May 2021 22:21  
Operator : JC/MD  
Sample : M2561-01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 24 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
TB02-20210526

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X051921W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX052921\  
Data File : VX022268.D  
Acq On : 28 May 2021 22:21  
Operator : JC/MD  
Sample : M2561-01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 24 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
TB02-20210526

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X051921W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |    |      |      |
|------------------|----|---------|-------|----------|-----------------------|----|------|------|
|                  |    |         |       |          | #                     | RT | Resp | Conc |

-----