

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052921\
 Data File : VX022269.D
 Acq On : 28 May 2021 22:45
 Operator : JC/MD
 Sample : M2545-01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TB-01-20210526

Integration Parameters: RTEINT.P

Integrator: RTE

Smoother: ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M

Title : SW846 8260

Signal : TIC: VX022269.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.270	26	30	35	rBV2	8252	8175	1.76%	0.349%
2	1.453	57	60	65	rBV	3892	4932	1.06%	0.211%
3	1.563	72	78	82	rVB4	2762	4994	1.07%	0.213%
4	2.386	207	213	220	rVB	3988	6726	1.44%	0.287%
5	2.550	230	240	249	rBV2	7834	15800	3.39%	0.675%
6	5.397	696	707	718	rBV	49068	139534	29.97%	5.961%
7	5.562	722	734	746	rBV	77091	214418	46.06%	9.160%
8	5.970	788	801	816	rBV2	61162	161524	34.70%	6.900%
9	6.769	922	932	943	rBV	139915	331302	71.17%	14.153%
10	8.653	1234	1241	1256	rBV	301322	465527	100.00%	19.887%
11	10.055	1465	1471	1484	rVB	287465	388459	83.44%	16.594%
12	11.085	1634	1640	1648	rBV	222393	273154	58.68%	11.669%
13	12.024	1789	1794	1802	rVB	270650	326347	70.10%	13.941%


Sum of corrected areas: 2340892

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052921\
Data File : VX022269.D
Acq On : 28 May 2021 22:45
Operator : JC/MD
Sample : M2545-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-01-20210526

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

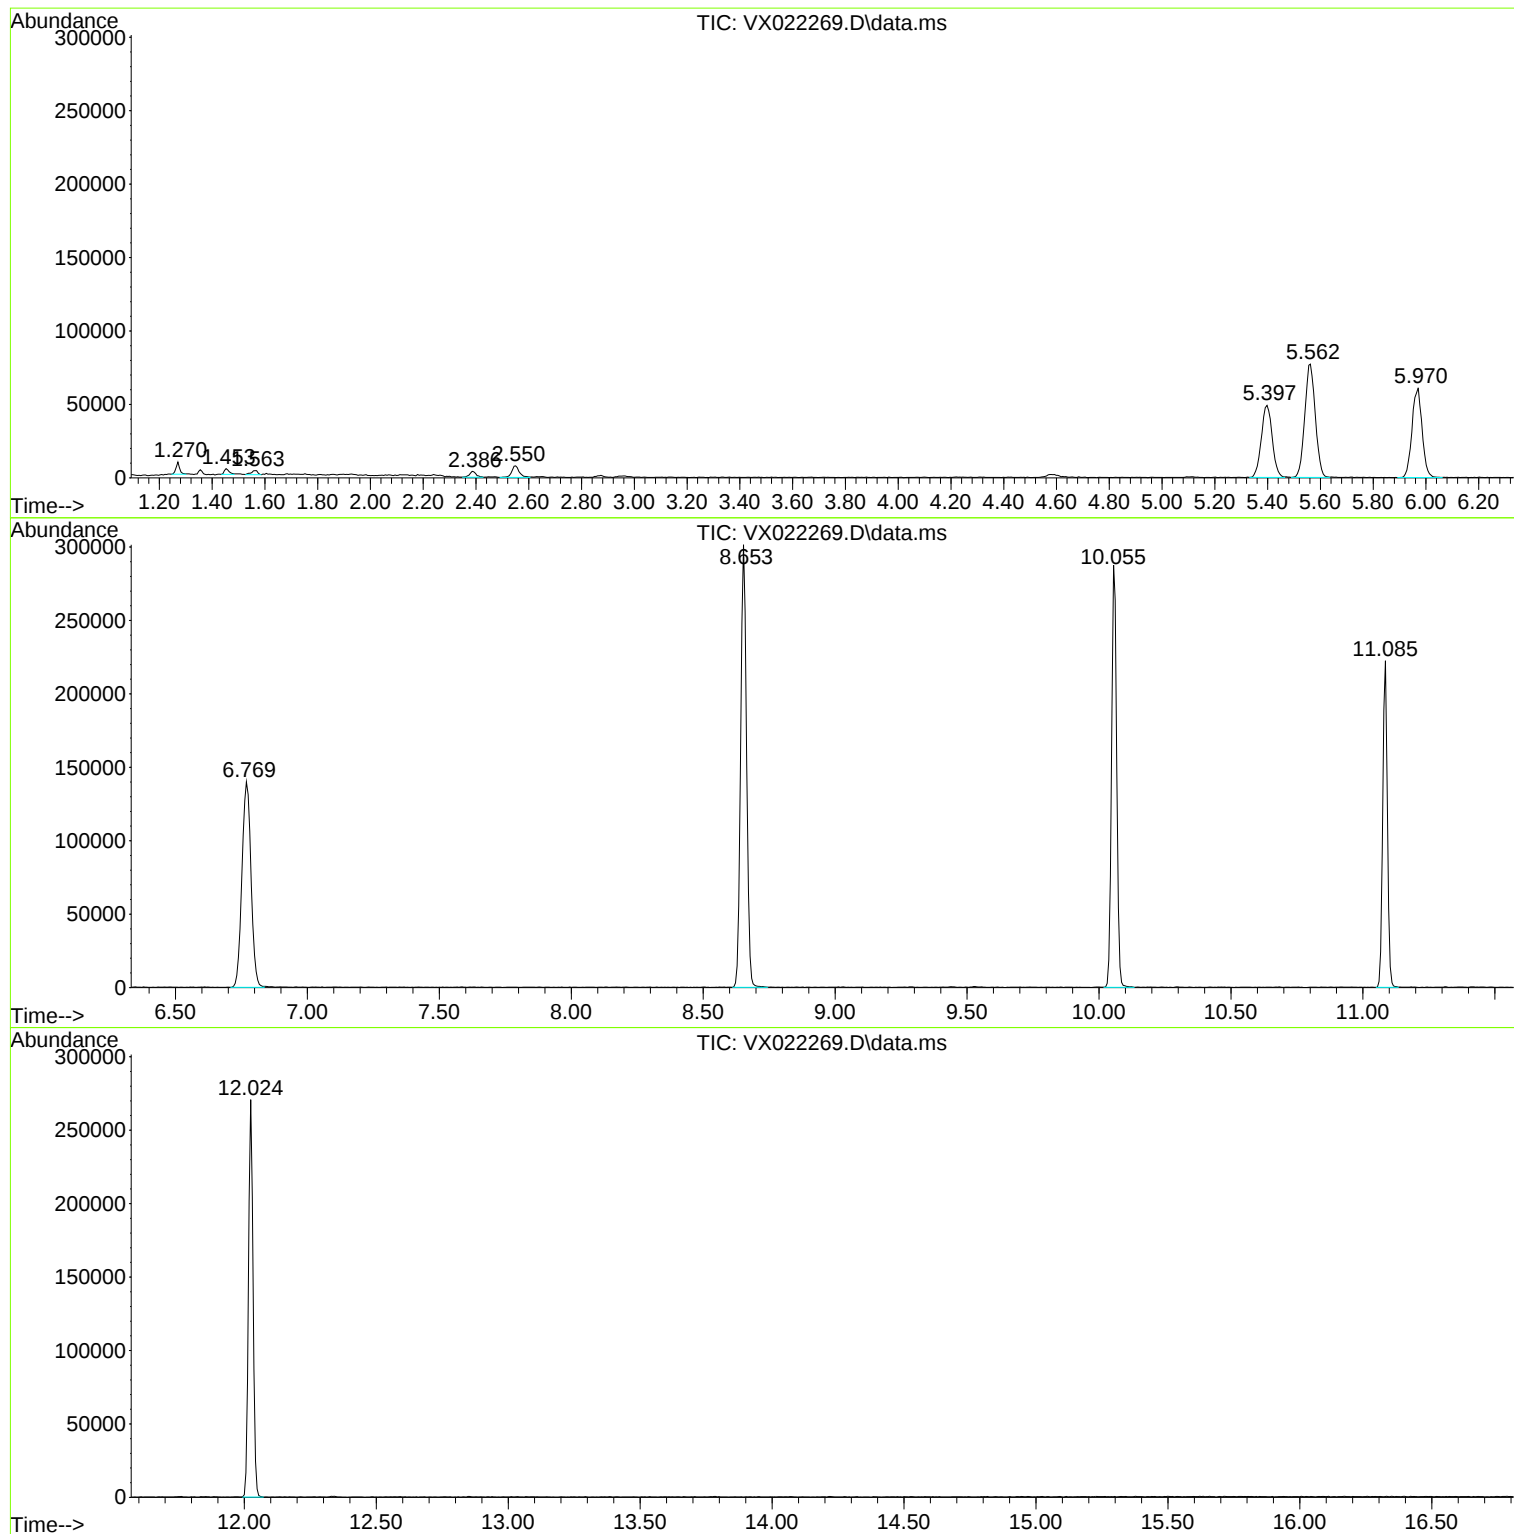

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052921\
Data File : VX022269.D
Acq On : 28 May 2021 22:45
Operator : JC/MD
Sample : M2545-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-01-20210526

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052921\
Data File : VX022269.D
Acq On : 28 May 2021 22:45
Operator : JC/MD
Sample : M2545-01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-01-20210526

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc