

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052925\
 Data File : VX046396.D
 Acq On : 29 May 2025 13:53
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

Quant Time: May 30 01:28:05 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X050525W.M
 Quant Title : SW846 8260
 QLast Update : Tue May 06 07:12:22 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	59077	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	120458	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	114905	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	47413	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	60150	54.613	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 109.220%			
35) Dibromofluoromethane	5.379	113	43007	49.580	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 99.160%			
50) Toluene-d8	8.647	98	152958	50.947	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 101.900%			
62) 4-Bromofluorobenzene	11.079	95	57462	49.896	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery = 99.800%			
Target Compounds						Qvalue
5) Bromomethane	1.599	94	60	0.159	ug/l #	59
6) Chloroethane	1.599	64	46	0.106	ug/l #	44
14) Allyl chloride	2.642	41	47	0.035	ug/l #	21
16) Acetone	2.386	43	192	0.435	ug/l #	48
17) Carbon Disulfide	2.508	76	277	0.167	ug/l #	76
18) Methyl Acetate	2.703	43	198	0.193	ug/l #	55
20) Methylene Chloride	2.782	84	163	0.193	ug/l #	69
31) Cyclohexane	5.550	56	2021	1.540	ug/l #	21
36) 1,1-Dichloropropene	5.550	75	6127	5.257	ug/l #	51
38) Carbon Tetrachloride	5.538	117	7022	5.362	ug/l #	15
43) Isopropyl Acetate	6.220	43	19	0.009	ug/l #	63
51) 4-Methyl-2-Pentanone	8.647	43	850	0.583	ug/l #	1
65) Chlorobenzene	10.080	112	55	0.022	ug/l #	43
67) Ethyl Benzene	10.201	91	601	0.136	ug/l #	88
68) m/p-Xylenes	10.311	106	202	0.125	ug/l	96
73) Isopropylbenzene	10.970	105	215	0.058	ug/l #	49
76) 1,2,3-Trichloropropane	11.079	75	33518	29.369	ug/l #	36
78) n-propylbenzene	11.311	91	644	0.150	ug/l #	73
79) 2-Chlorotoluene	11.360	91	23	0.008	ug/l #	44
80) 1,3,5-Trimethylbenzene	11.616	105	328	0.106	ug/l	77
81) trans-1,4-Dichloro-2-b...	11.079	75	33518	95.618	ug/l #	1
82) 4-Chlorotoluene	11.476	91	30	0.010	ug/l #	48
83) tert-Butylbenzene	11.762	119	50	0.016	ug/l #	26
84) 1,2,4-Trimethylbenzene	11.756	105	896	0.287	ug/l	95
85) sec-Butylbenzene	11.890	105	113	0.030	ug/l #	57
86) p-Isopropyltoluene	12.012	119	55	0.017	ug/l #	1
87) 1,3-Dichlorobenzene	11.976	146	62	0.040	ug/l #	24
88) 1,4-Dichlorobenzene	12.030	146	143	0.090	ug/l #	1
89) n-Butylbenzene	12.341	91	145	0.053	ug/l #	45
90) Hexachloroethane	12.646	117	160	0.288	ug/l #	19
93) 1,2,4-Trichlorobenzene	13.603	180	79	0.088	ug/l #	12
95) Naphthalene	13.780	128	1729	0.523	ug/l #	94
96) 1,2,3-Trichlorobenzene	13.963	180	60	0.065	ug/l #	12


(#) = qualifier out of range (m) = manual integration (+) = signals summed


Instrument :
MSVOA_X
ClientSampleId :
IBLK

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052925\
Data File : VX046396.D
Acq On : 29 May 2025 13:53
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Time: May 30 01:28:05 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X050525W.M
Quant Title : SW846 8260
QLast Update : Tue May 06 07:12:22 2025
Response via : Initial Calibration




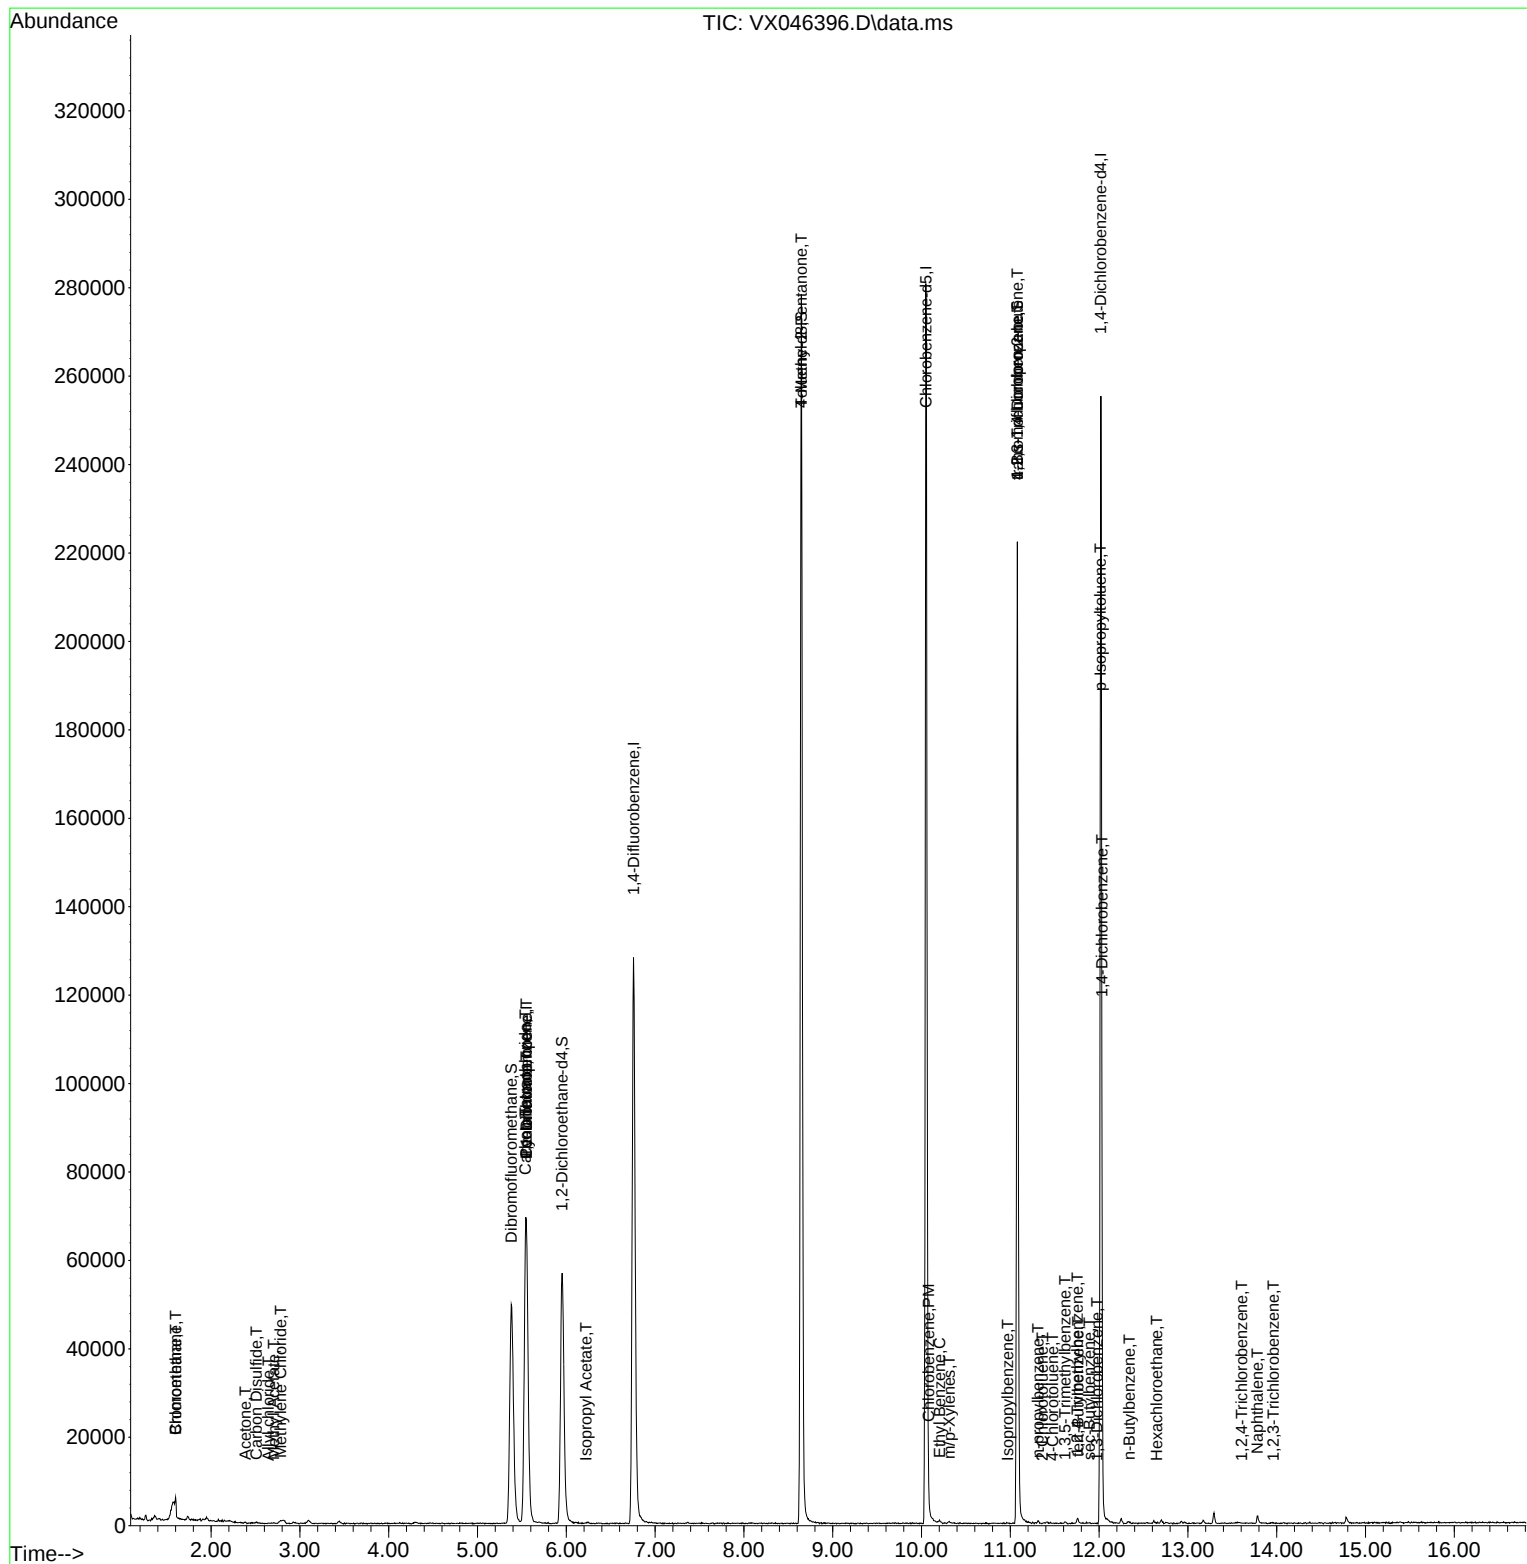




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX046396.D
Acq: 29 May 2025 13:53




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion:168 Resp: 59077
Ion Ratio Lower Upper
168 100
99 71.2 54.9 82.3

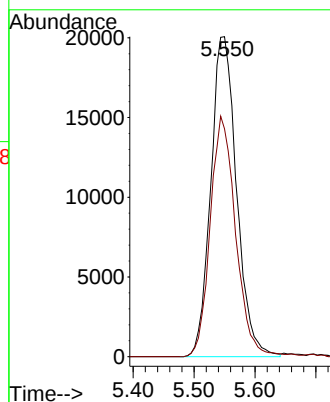

#5
Bromomethane
Concen: 0.159 ug/l
RT: 1.599 min Scan# 84
Delta R.T. 0.006 min
Lab File: VX046396.D
Acq: 29 May 2025 13:53

Tgt Ion: 94 Resp: 60
Ion Ratio Lower Upper
94 100
96 130.0 72.8 109.2#


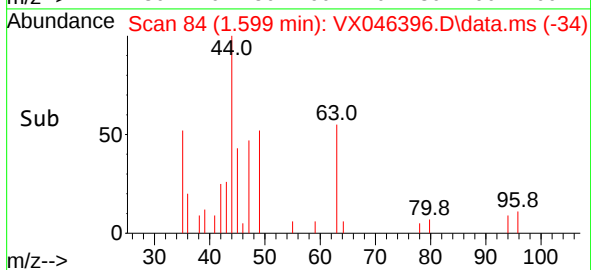
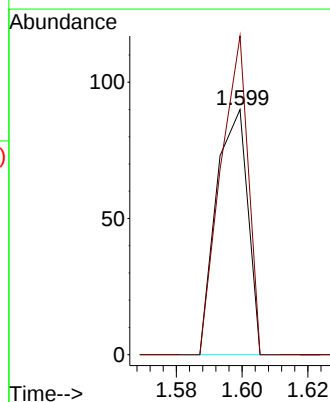
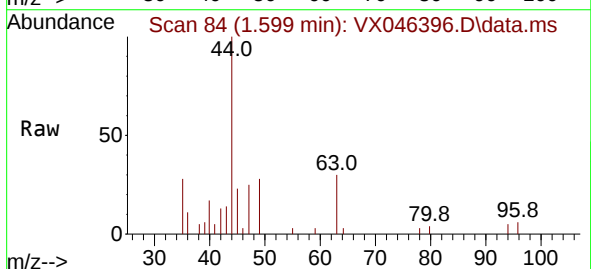


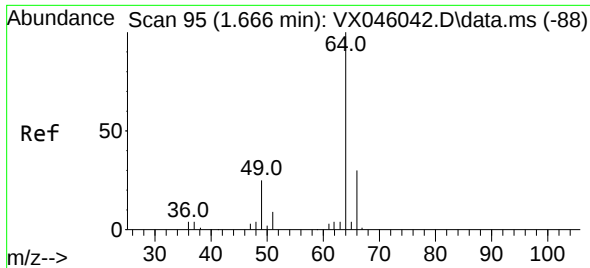

#6
Chloroethane
Concen: 0.106 ug/l
RT: 1.599 min Scan# 84
Delta R.T. -0.067 min
Lab File: VX046396.D
Acq: 29 May 2025 13:53




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion: 64 Resp: 46
Ion Ratio Lower Upper
64 100
66 0.0 24.3 36.5#

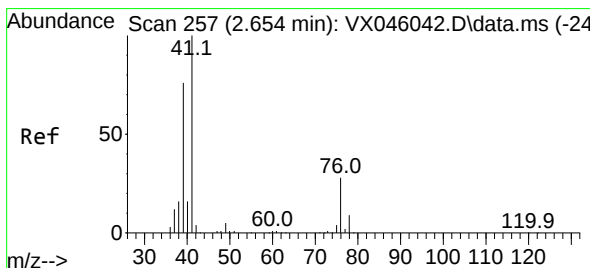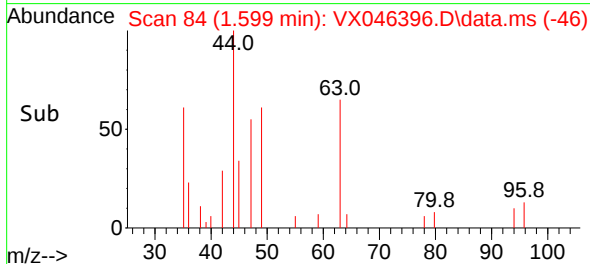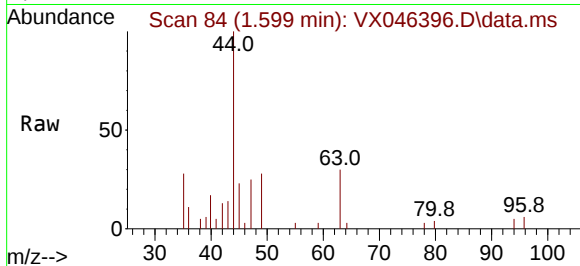

#14
Allyl chloride
Concen: 0.035 ug/l
RT: 2.642 min Scan# 255
Delta R.T. -0.012 min
Lab File: VX046396.D
Acq: 29 May 2025 13:53

Tgt Ion: 41 Resp: 47
Ion Ratio Lower Upper
41 100
39 0.0 60.6 90.8#
76 0.0 24.9 37.3#


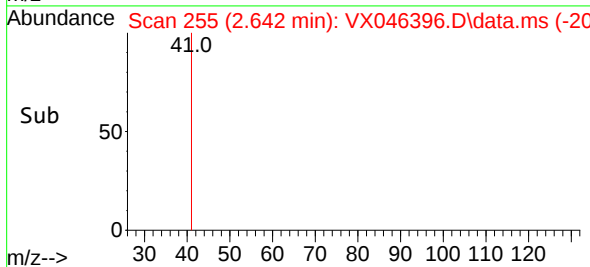

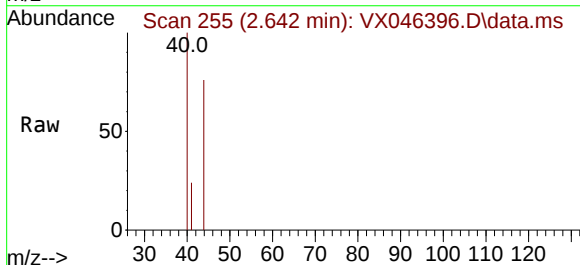




#16
Acetone
Concen: 0.435 ug/l
RT: 2.386 min Scan# 213
Delta R.T. 0.000 min
Lab File: VX046396.D
Acq: 29 May 2025 13:53




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion: 43 Resp: 192
Ion Ratio Lower Upper
43 100
58 0.0 21.2 31.8#

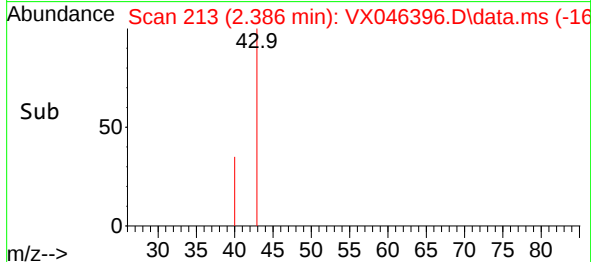

#17
Carbon Disulfide
Concen: 0.167 ug/l
RT: 2.508 min Scan# 233
Delta R.T. 0.006 min
Lab File: VX046396.D
Acq: 29 May 2025 13:53

Tgt Ion: 76 Resp: 277
Ion Ratio Lower Upper
76 100
78 0.0 7.0 10.4#




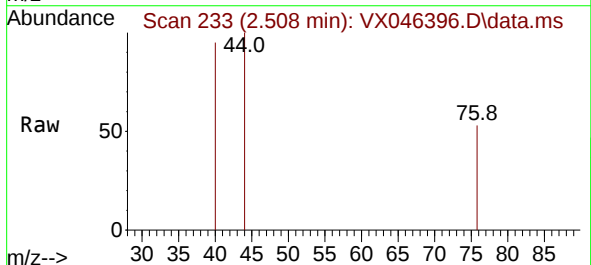




#18
Methyl Acetate
Concen: 0.193 ug/l
RT: 2.703 min Scan# 265
Delta R.T. 0.000 min
Lab File: VX046396.D
Acq: 29 May 2025 13:53




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion: 43 Resp: 198
Ion Ratio Lower Upper
43 100
74 0.0 16.7 25.1#



#20
Methylene Chloride
Concen: 0.193 ug/l
RT: 2.782 min Scan# 278
Delta R.T. 0.000 min
Lab File: VX046396.D
Acq: 29 May 2025 13:53

Tgt Ion: 84 Resp: 163
Ion Ratio Lower Upper
84 100
49 122.5 113.9 170.9
51 0.0 33.5 50.3#
86 35.9 53.8 80.8#



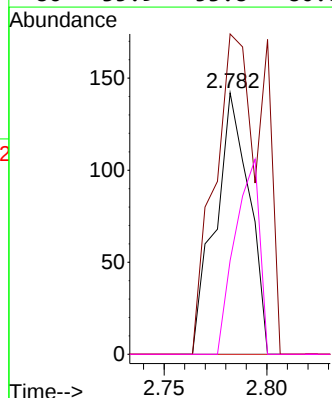



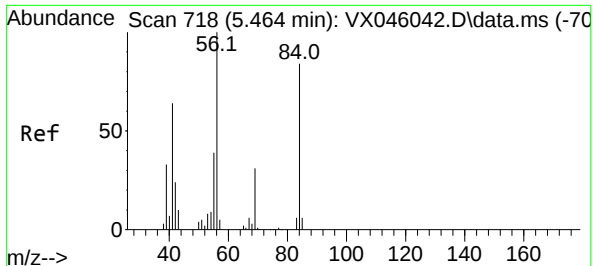

#31
Cyclohexane
Concen: 1.540 ug/l
RT: 5.550 min Scan# 718
Delta R.T. 0.085 min
Lab File: VX046396.D
Acq: 29 May 2025 13:53




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion: 56 Resp: 2021
Ion Ratio Lower Upper
56 100
69 168.2 24.4 36.6#
84 97.4 66.9 100.3

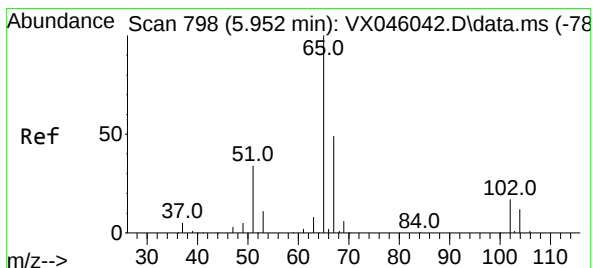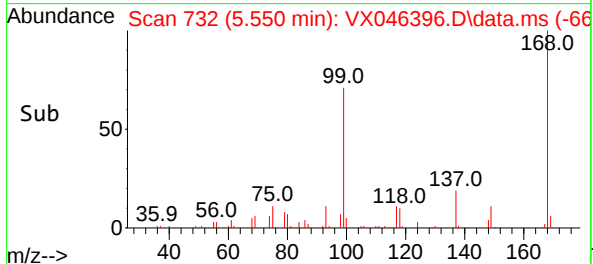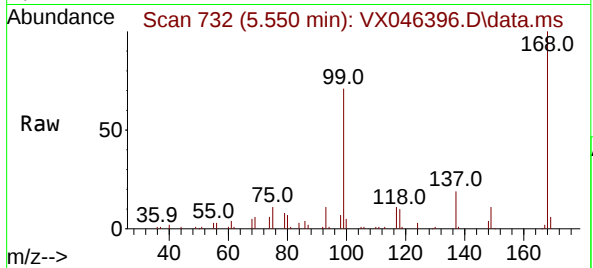

#33
1,2-Dichloroethane-d4
Concen: 54.613 ug/l
RT: 5.952 min Scan# 798
Delta R.T. 0.000 min
Lab File: VX046396.D
Acq: 29 May 2025 13:53

Tgt Ion: 65 Resp: 60150
Ion Ratio Lower Upper
65 100
67 48.2 0.0 99.0


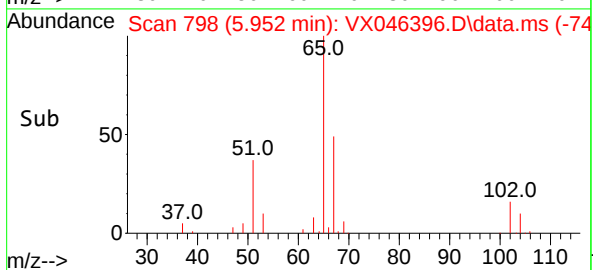

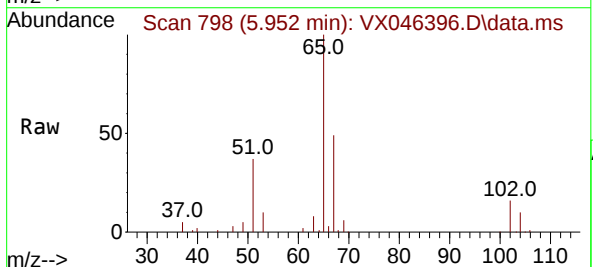




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.757 min Scan# 91
 Delta R.T. 0.000 min
 Lab File: VX046396.D
 Acq: 29 May 2025 13:53




Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK


Tgt Ion:	114	Resp:	120458
Ion	Ratio	Lower	Upper
114	100		
63	24.3	0.0	49.2
88	17.5	0.0	33.6

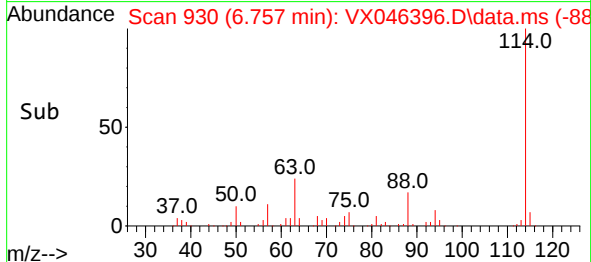

#35
 Dibromofluoromethane
 Concen: 49.580 ug/l
 RT: 5.379 min Scan# 704
 Delta R.T. 0.000 min
 Lab File: VX046396.D
 Acq: 29 May 2025 13:53

Tgt Ion:	113	Resp:	43007
Ion	Ratio	Lower	Upper
113	100		
111	105.1	83.1	124.7
192	17.2	13.3	19.9




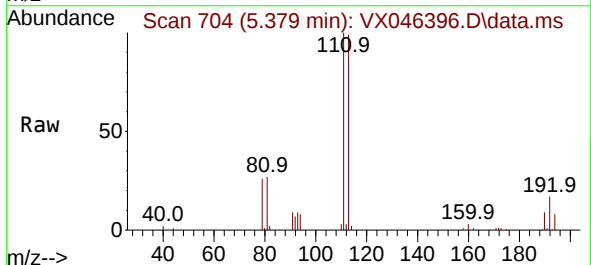




#36
1,1-Dichloropropene
Concen: 5.257 ug/l
RT: 5.550 min Scan# 710
Delta R.T. -0.134 min
Lab File: VX046396.D
Acq: 29 May 2025 13:53




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion: 75 Resp: 6127
Ion Ratio Lower Upper
75 100
110 8.6 16.3 48.9#
77 0.0 24.3 36.5#

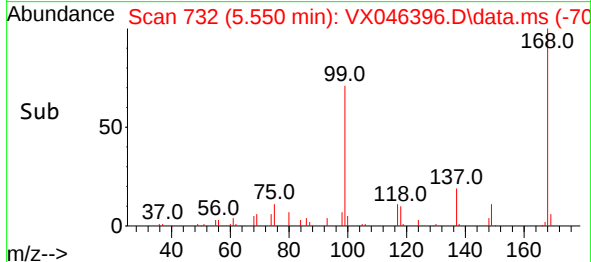

#38
Carbon Tetrachloride
Concen: 5.362 ug/l
RT: 5.538 min Scan# 730
Delta R.T. -0.134 min
Lab File: VX046396.D
Acq: 29 May 2025 13:53

Tgt Ion: 117 Resp: 7022
Ion Ratio Lower Upper
117 100
119 3.4 75.2 112.8#
121 0.0 24.2 36.4#


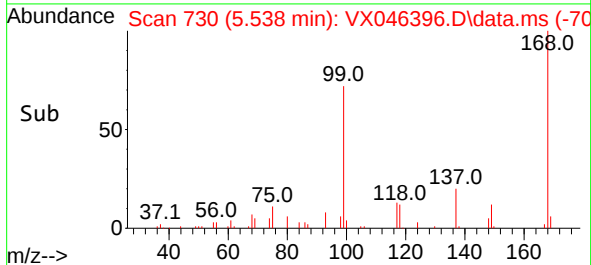






#43
Isopropyl Acetate
Concen: 0.009 ug/l
RT: 6.220 min Scan# 84
Delta R.T. -0.116 min
Lab File: VX046396.D
Acq: 29 May 2025 13:53




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion: 43 Resp: 19
Ion Ratio Lower Upper
43 100
61 0.0 14.3 21.5#
87 0.0 9.5 14.3#

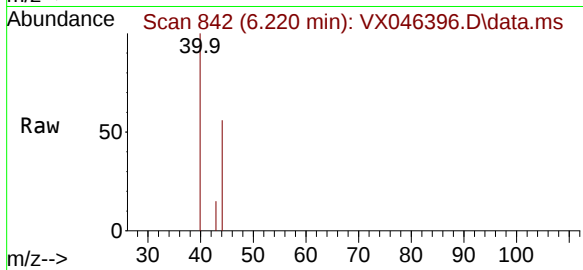

#50
Toluene-d8
Concen: 50.947 ug/l
RT: 8.647 min Scan# 1240
Delta R.T. 0.000 min
Lab File: VX046396.D
Acq: 29 May 2025 13:53

Tgt Ion: 98 Resp: 152958
Ion Ratio Lower Upper
98 100
100 65.3 53.5 80.3




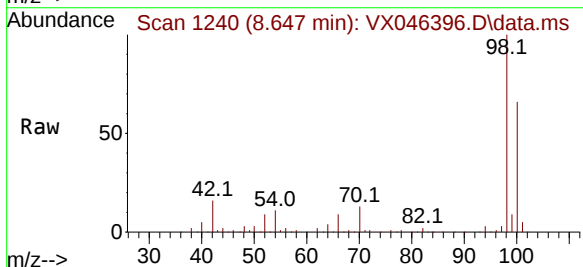


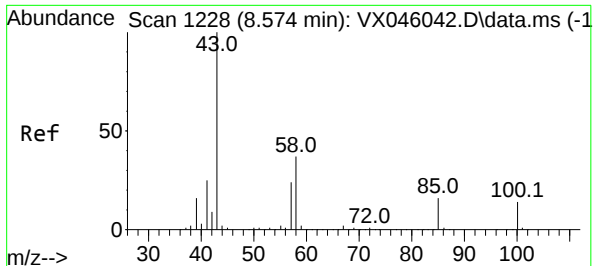

#51
4-Methyl-2-Pentanone
Concen: 0.583 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.073 min
Lab File: VX046396.D
Acq: 29 May 2025 13:53




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion: 43 Resp: 850
Ion Ratio Lower Upper
43 100
58 161.6 28.9 43.3#

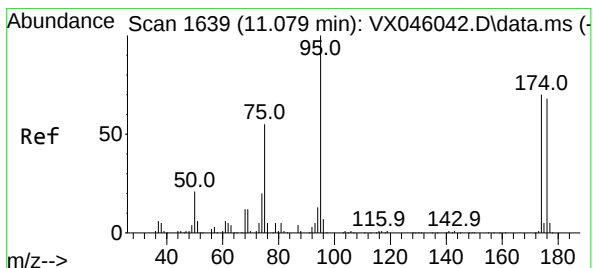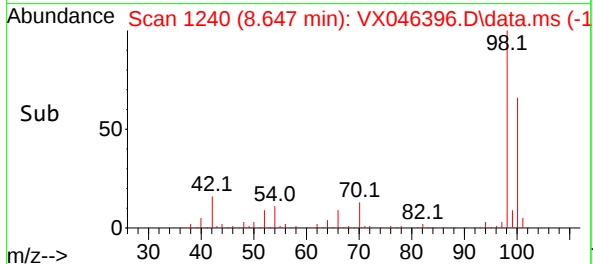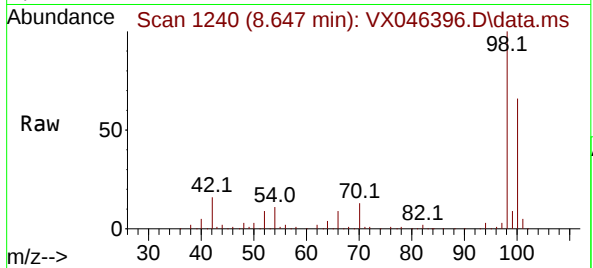

#62
4-Bromofluorobenzene
Concen: 49.896 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX046396.D
Acq: 29 May 2025 13:53

Tgt Ion: 95 Resp: 57462
Ion Ratio Lower Upper
95 100
174 68.1 0.0 135.8
176 64.8 0.0 131.4


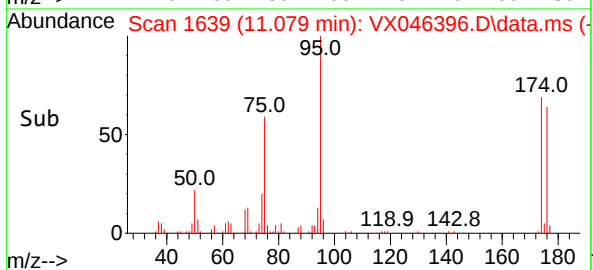

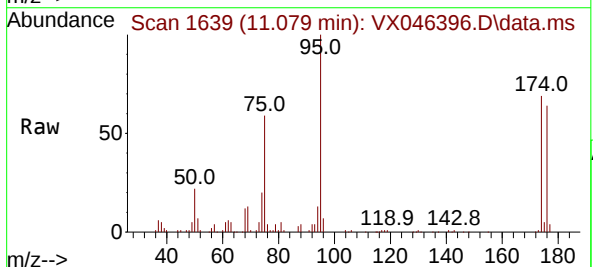




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.049 min Scan# 1470
Delta R.T. 0.000 min
Lab File: VX046396.D
Acq: 29 May 2025 13:53




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion:117 Resp: 114905
Ion Ratio Lower Upper
117 100
82 63.8 50.6 76.0
119 31.7 25.8 38.6

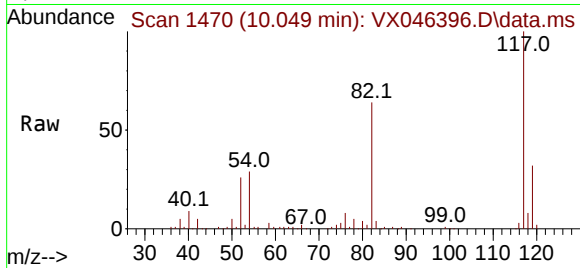

#65
Chlorobenzene
Concen: 0.022 ug/l
RT: 10.080 min Scan# 1475
Delta R.T. 0.000 min
Lab File: VX046396.D
Acq: 29 May 2025 13:53

Tgt Ion:112 Resp: 55
Ion Ratio Lower Upper
112 100
114 0.0 25.4 38.2#

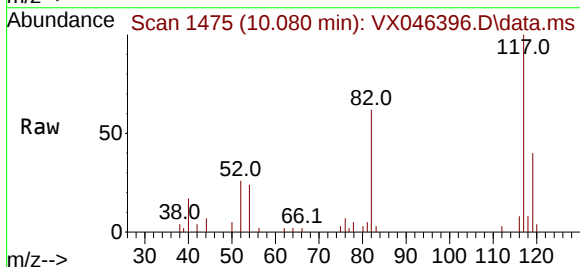



#67

Ethyl Benzene

Concen: 0.136 ug/l

RT: 10.201 min Scan# 1495

Delta R.T. 0.012 min

Lab File: VX046396.D

Acq: 29 May 2025 13:53

Instrument :

MSVOA_X

ClientSampleId :





IBLK

Tgt Ion: 91 Resp: 601

Ion Ratio Lower Upper

91 100

106 23.1 23.4 35.2#

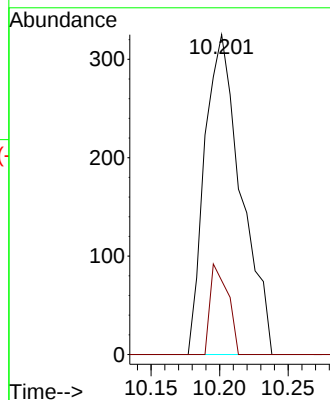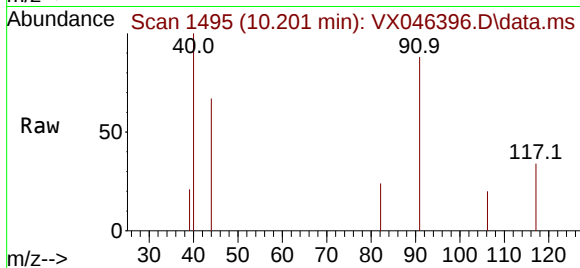

#68

m/p-Xylenes

Concen: 0.125 ug/l

RT: 10.311 min Scan# 1513

Delta R.T. 0.012 min

Lab File: VX046396.D




Acq: 29 May 2025 13:53


Tgt Ion:106 Resp: 202

Ion Ratio Lower Upper

106 100

91 220.8 171.2 256.8


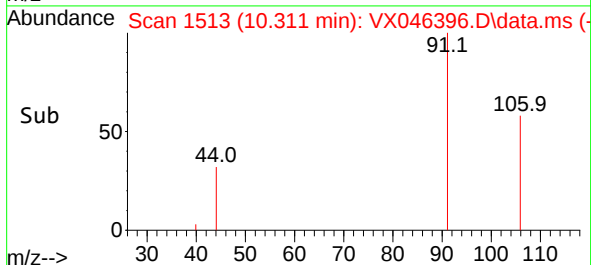
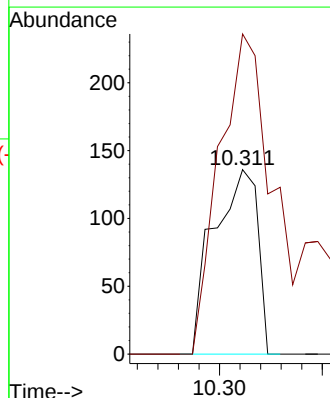
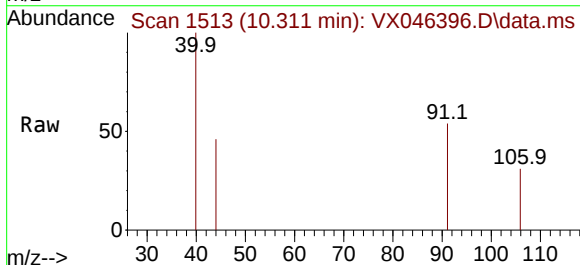




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX046396.D
Acq: 29 May 2025 13:53




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion:152 Resp: 47413
Ion Ratio Lower Upper
152 100
115 65.0 46.9 140.7
150 157.0 0.0 351.0

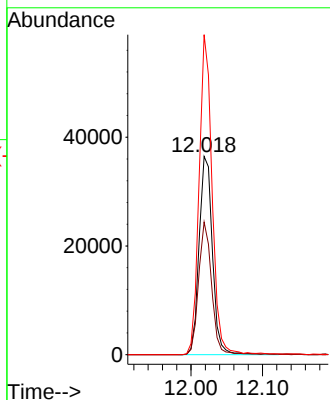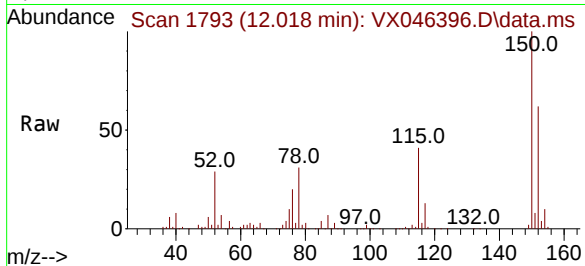

#73
Isopropylbenzene
Concen: 0.058 ug/l
RT: 10.970 min Scan# 1621
Delta R.T. 0.012 min
Lab File: VX046396.D
Acq: 29 May 2025 13:53

Tgt Ion:105 Resp: 215
Ion Ratio Lower Upper
105 100
120 0.0 12.8 38.4#

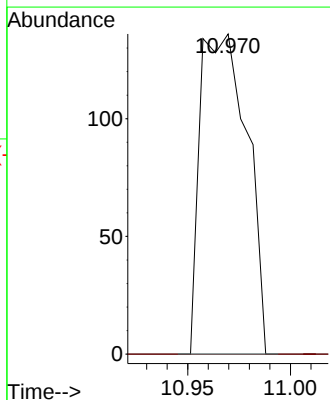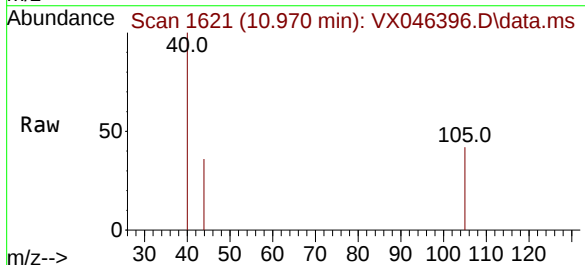



#76

1,2,3-Trichloropropane

Concen: 29.369 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. -0.158 min

Lab File: VX046396.D

Acq: 29 May 2025 13:53

Instrument :

MSVOA_X

ClientSampleId :





IBLK

Tgt Ion: 75 Resp: 33518

Ion Ratio Lower Upper

75 100

77 0.9 20.5 61.5#

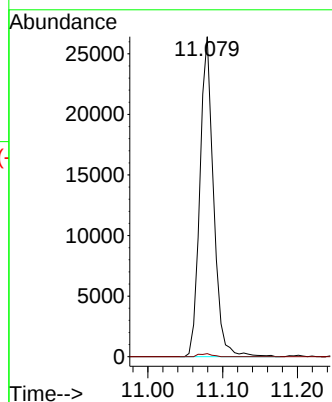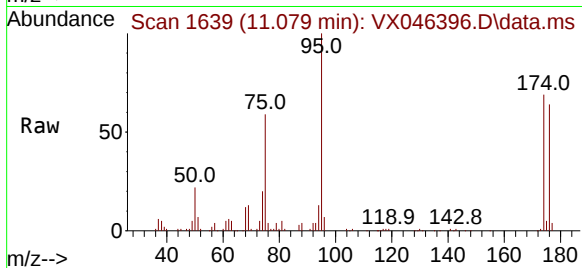

#78

n-propylbenzene

Concen: 0.150 ug/l

RT: 11.311 min Scan# 1677

Delta R.T. 0.012 min

Lab File: VX046396.D




Acq: 29 May 2025 13:53


Tgt Ion: 91 Resp: 644

Ion Ratio Lower Upper

91 100

120 8.7 10.8 32.4#


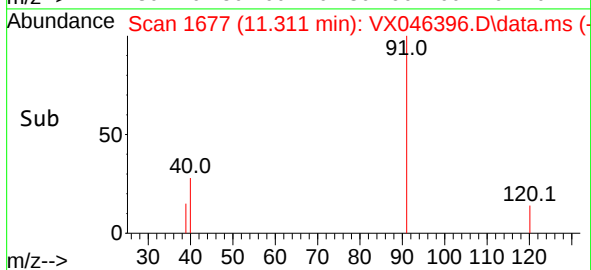
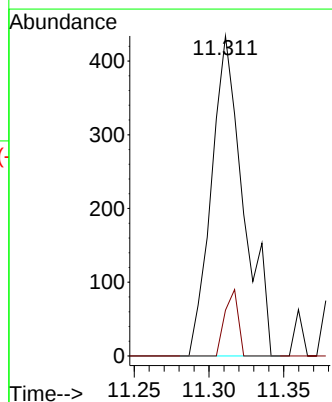
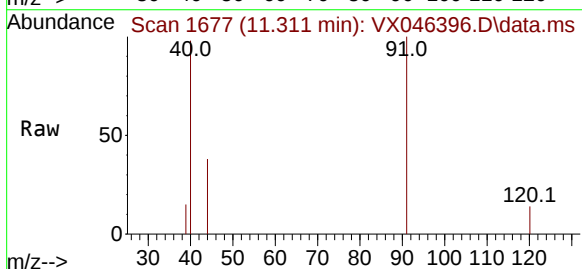




#79
2-Chlorotoluene
Concen: 0.008 ug/l
RT: 11.360 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX046396.D
Acq: 29 May 2025 13:53




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion: 91 Resp: 23
Ion Ratio Lower Upper
91 100
126 0.0 15.6 46.7#

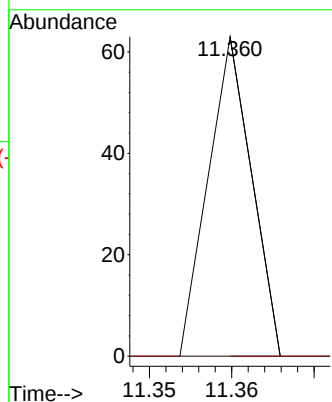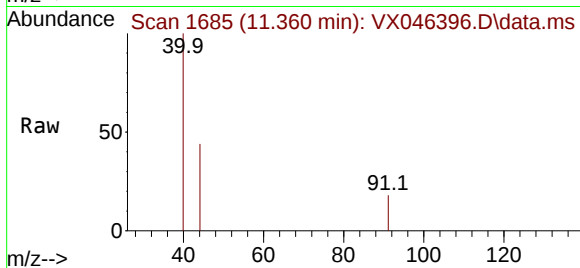

#80
1,3,5-Trimethylbenzene
Concen: 0.106 ug/l
RT: 11.616 min Scan# 1727
Delta R.T. 0.165 min
Lab File: VX046396.D
Acq: 29 May 2025 13:53

Tgt Ion: 105 Resp: 328
Ion Ratio Lower Upper
105 100
120 30.8 23.1 69.2



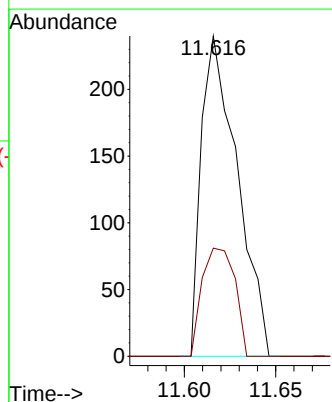
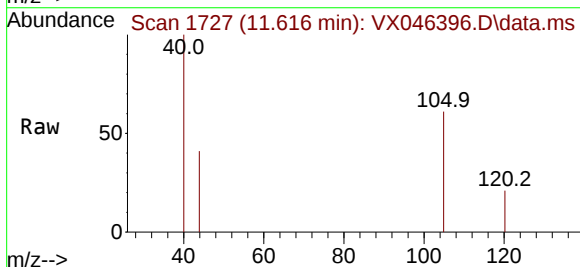




#81
trans-1,4-Dichloro-2-butene
Concen: 95.618 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.061 min
Lab File: VX046396.D
Acq: 29 May 2025 13:53




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion: 75 Resp: 33518
Ion Ratio Lower Upper
75 100
53 0.0 100.5 150.7#
89 0.0 37.0 55.6#

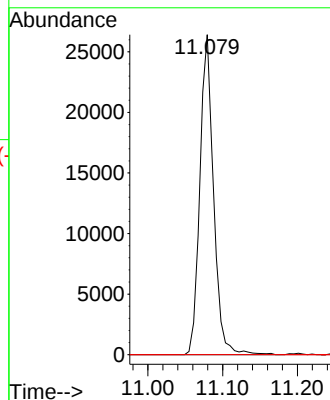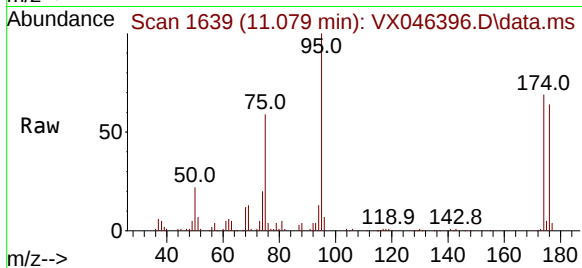

#82
4-Chlorotoluene
Concen: 0.010 ug/l
RT: 11.476 min Scan# 1704
Delta R.T. 0.024 min
Lab File: VX046396.D
Acq: 29 May 2025 13:53

Tgt Ion: 91 Resp: 30
Ion Ratio Lower Upper
91 100
126 0.0 13.3 39.8#

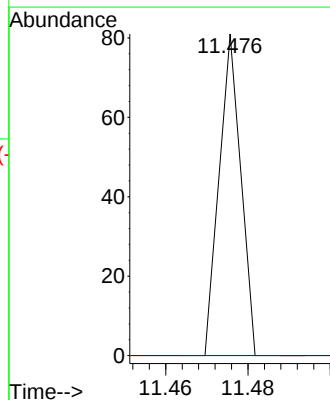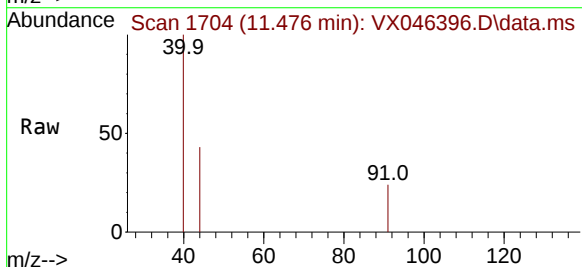



#83

tert-Butylbenzene

Concen: 0.016 ug/l

RT: 11.762 min Scan# 11

Delta R.T. 0.049 min

Lab File: VX046396.D

Acq: 29 May 2025 13:53

Instrument :

MSVOA_X

ClientSampleId :

IBLK





Tgt Ion:119 Resp: 50

Ion Ratio Lower Upper

119 100

91 0.0 32.9 98.7#

134 0.0 11.4 34.1#

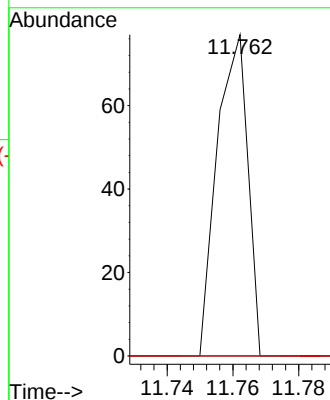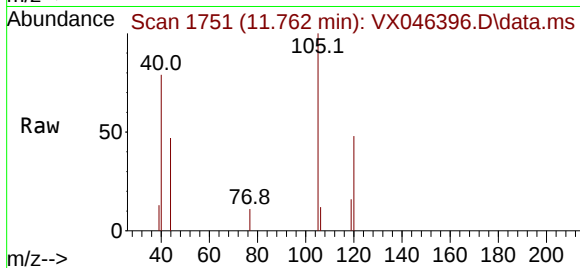

#84

1,2,4-Trimethylbenzene

Concen: 0.287 ug/l

RT: 11.756 min Scan# 1750

Delta R.T. 0.006 min

Lab File: VX046396.D




Acq: 29 May 2025 13:53


Tgt Ion:105 Resp: 896

Ion Ratio Lower Upper

105 100

120 39.3 21.2 63.6


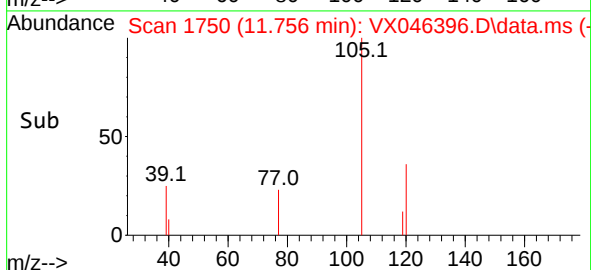
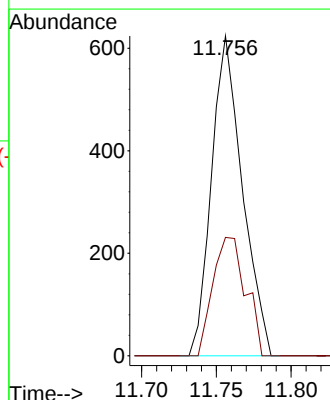
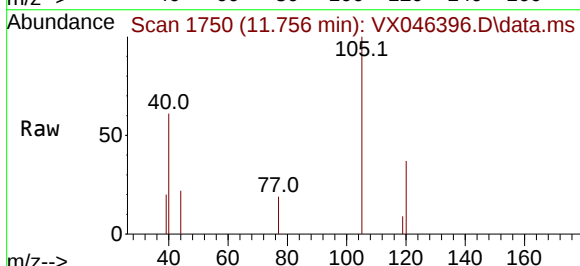




#85
 sec-Butylbenzene
 Concen: 0.030 ug/l
 RT: 11.890 min Scan# 1772
 Delta R.T. 0.000 min
 Lab File: VX046396.D
 Acq: 29 May 2025 13:53




Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK


Tgt Ion:105 Resp: 113
 Ion Ratio Lower Upper
 105 100
 134 0.0 9.7 29.1#



#86
 p-Isopropyltoluene
 Concen: 0.017 ug/l
 RT: 12.012 min Scan# 1792
 Delta R.T. 0.006 min
 Lab File: VX046396.D
 Acq: 29 May 2025 13:53

Tgt Ion:119 Resp: 55
 Ion Ratio Lower Upper
 119 100
 134 85.5 12.5 37.5#
 91 358.2 13.8 41.4#

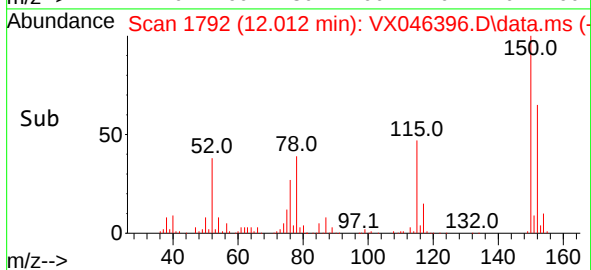



#87

1,3-Dichlorobenzene

Concen: 0.040 ug/l

RT: 11.976 min Scan# 1785

Delta R.T. 0.006 min

Lab File: VX046396.D

Acq: 29 May 2025 13:53

Instrument :

MSVOA_X

ClientSampleId :

IBLK





Tgt Ion:146 Resp: 62

Ion Ratio Lower Upper

146 100

111 0.0 22.1 66.3#

148 0.0 32.1 96.5#

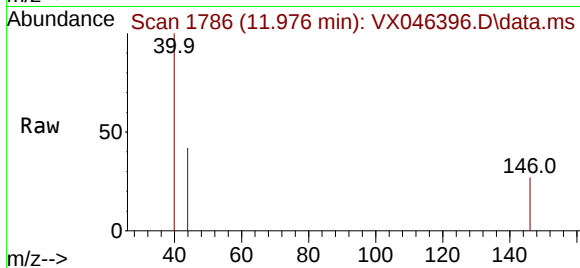

#88

1,4-Dichlorobenzene

Concen: 0.090 ug/l

RT: 12.030 min Scan# 1795

Delta R.T. -0.006 min

Lab File: VX046396.D

Acq: 29 May 2025 13:53




Tgt Ion:146 Resp: 143


Ion Ratio Lower Upper

146 100

111 576.9 21.3 63.9#

148 130.1 31.9 95.5#









#89
n-Butylbenzene
Concen: 0.053 ug/l
RT: 12.341 min Scan# 1846
Delta R.T. 0.012 min
Lab File: VX046396.D
Acq: 29 May 2025 13:53




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion: 91 Resp: 145
Ion Ratio Lower Upper
91 100
92 30.3 26.9 80.7
134 74.5 11.8 35.3#

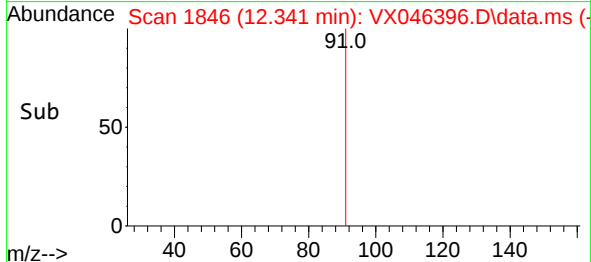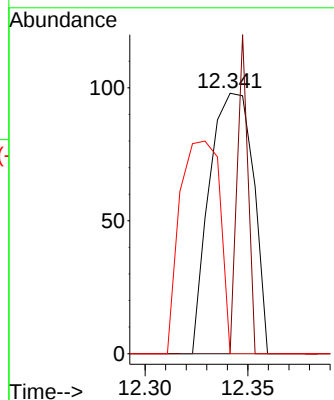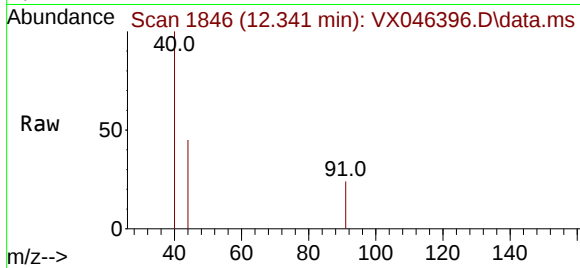

#90
Hexachloroethane
Concen: 0.288 ug/l
RT: 12.646 min Scan# 1896
Delta R.T. 0.110 min
Lab File: VX046396.D
Acq: 29 May 2025 13:53

Tgt Ion: 117 Resp: 160
Ion Ratio Lower Upper
117 100
201 0.0 31.6 94.7#



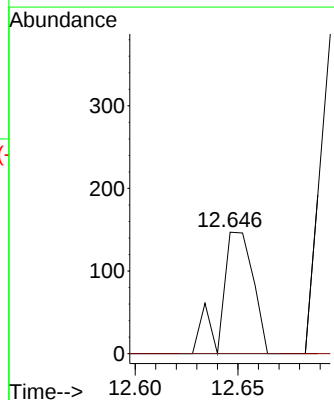
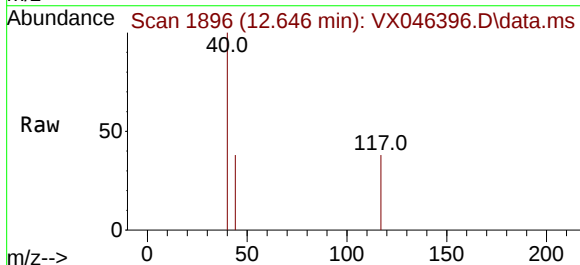




#93
 1,2,4-Trichlorobenzene
 Concen: 0.088 ug/l
 RT: 13.603 min Scan# 2053
 Delta R.T. 0.018 min
 Lab File: VX046396.D
 Acq: 29 May 2025 13:53




Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK


Tgt Ion:180 Resp: 79
 Ion Ratio Lower Upper
 180 100
 182 0.0 47.9 143.8#
 145 0.0 17.1 51.2#

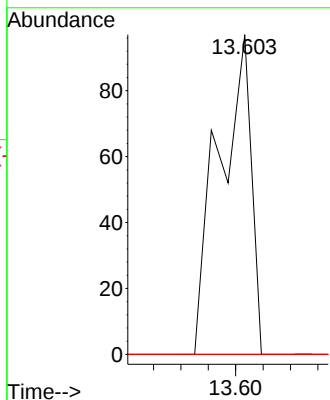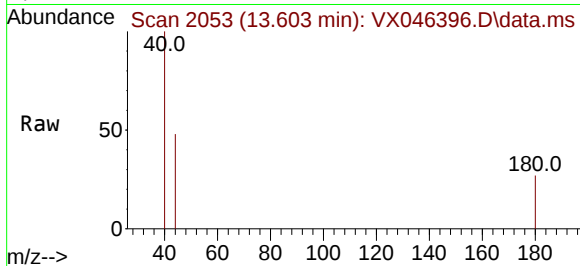

#95
 Naphthalene
 Concen: 0.523 ug/l
 RT: 13.780 min Scan# 2082
 Delta R.T. 0.006 min
 Lab File: VX046396.D
 Acq: 29 May 2025 13:53

Tgt Ion:128 Resp: 1729
 Ion Ratio Lower Upper
 128 100
 127 9.5 10.4 15.6#
 129 9.5 8.6 13.0

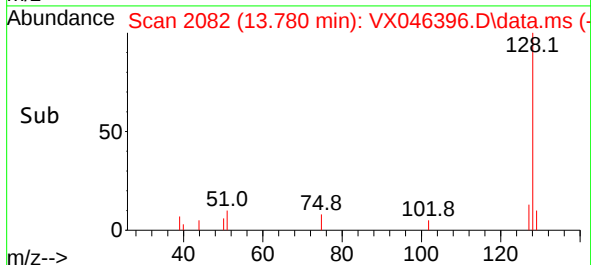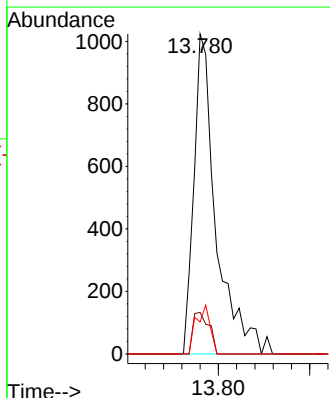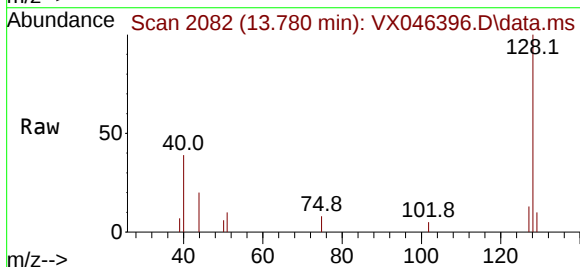



#96
 1,2,3-Trichlorobenzene
 Concen: 0.065 ug/l
 RT: 13.963 min Scan# 21
 Delta R.T. 0.006 min
 Lab File: VX046396.D
 Acq: 29 May 2025 13:53

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

Tgt Ion:180 Resp: 60
 Ion Ratio Lower Upper
 180 100
 182 0.0 47.8 143.3#
 145 0.0 18.1 54.3#

