

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052925\
 Data File : VX046401.D
 Acq On : 29 May 2025 15:57
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

Quant Time: May 30 01:31:58 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X050525W.M
 Quant Title : SW846 8260
 QLast Update : Tue May 06 07:12:22 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.550	168	66575	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	133510	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	128473	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	56641	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.952	65	65463	52.743	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 105.480%	
35) Dibromofluoromethane	5.379	113	46844	48.724	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 97.440%	
50) Toluene-d8	8.647	98	166728	50.105	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 100.200%	
62) 4-Bromofluorobenzene	11.079	95	66237	51.893	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	= 103.780%	
Target Compounds						
						Qvalue
3) Chloromethane	1.301	50	40	0.040	ug/l #	43
5) Bromomethane	1.599	94	29	0.068	ug/l	97
16) Acetone	2.380	43	275	0.553	ug/l #	48
17) Carbon Disulfide	2.502	76	157	0.084	ug/l #	76
18) Methyl Acetate	2.703	43	146	0.126	ug/l #	55
20) Methylene Chloride	2.782	84	284	0.298	ug/l #	59
21) trans-1,2-Dichloroethene	3.087	96	1794	2.260	ug/l	88
23) Vinyl Acetate	3.440	43	24	0.009	ug/l #	74
31) Cyclohexane	5.550	56	2021	1.366	ug/l #	22
36) 1,1-Dichloropropene	5.538	75	6605	5.113	ug/l #	51
38) Carbon Tetrachloride	5.544	117	8073	5.562	ug/l #	18
42) 1,2-Dichloroethane	6.092	62	20	0.012	ug/l #	78
51) 4-Methyl-2-Pentanone	8.641	43	1013	0.627	ug/l #	1
52) Toluene	8.726	92	168	0.072	ug/l	82
67) Ethyl Benzene	10.208	91	91	0.018	ug/l #	45
68) m/p-Xylenes	10.305	106	19	0.010	ug/l #	1
73) Isopropylbenzene	10.970	105	48	0.011	ug/l #	49
74) N-amyl acetate	10.890	43	50	0.023	ug/l #	47
75) 1,1,2,2-Tetrachloroethane	11.073	83	75	0.049	ug/l #	55
76) 1,2,3-Trichloropropane	11.079	75	38353	28.131	ug/l #	36
78) n-propylbenzene	11.311	91	261	0.051	ug/l #	54
79) 2-Chlorotoluene	11.372	91	86	0.026	ug/l #	44
80) 1,3,5-Trimethylbenzene	11.445	105	66	0.018	ug/l #	30
81) trans-1,4-Dichloro-2-b...	11.079	75	38353	91.585	ug/l #	1
82) 4-Chlorotoluene	11.372	91	86	0.023	ug/l #	48
84) 1,2,4-Trimethylbenzene	11.762	105	327	0.088	ug/l	71
85) sec-Butylbenzene	11.896	105	45	0.010	ug/l #	57
89) n-Butylbenzene	12.335	91	148	0.045	ug/l #	33
90) Hexachloroethane	12.695	117	59	0.089	ug/l #	19
95) Naphthalene	13.786	128	514	0.130	ug/l #	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX052925\
Data File : VX046401.D
Acq On : 29 May 2025 15:57
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Time: May 30 01:31:58 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X050525W.M
Quant Title : SW846 8260
QLast Update : Tue May 06 07:12:22 2025
Response via : Initial Calibration




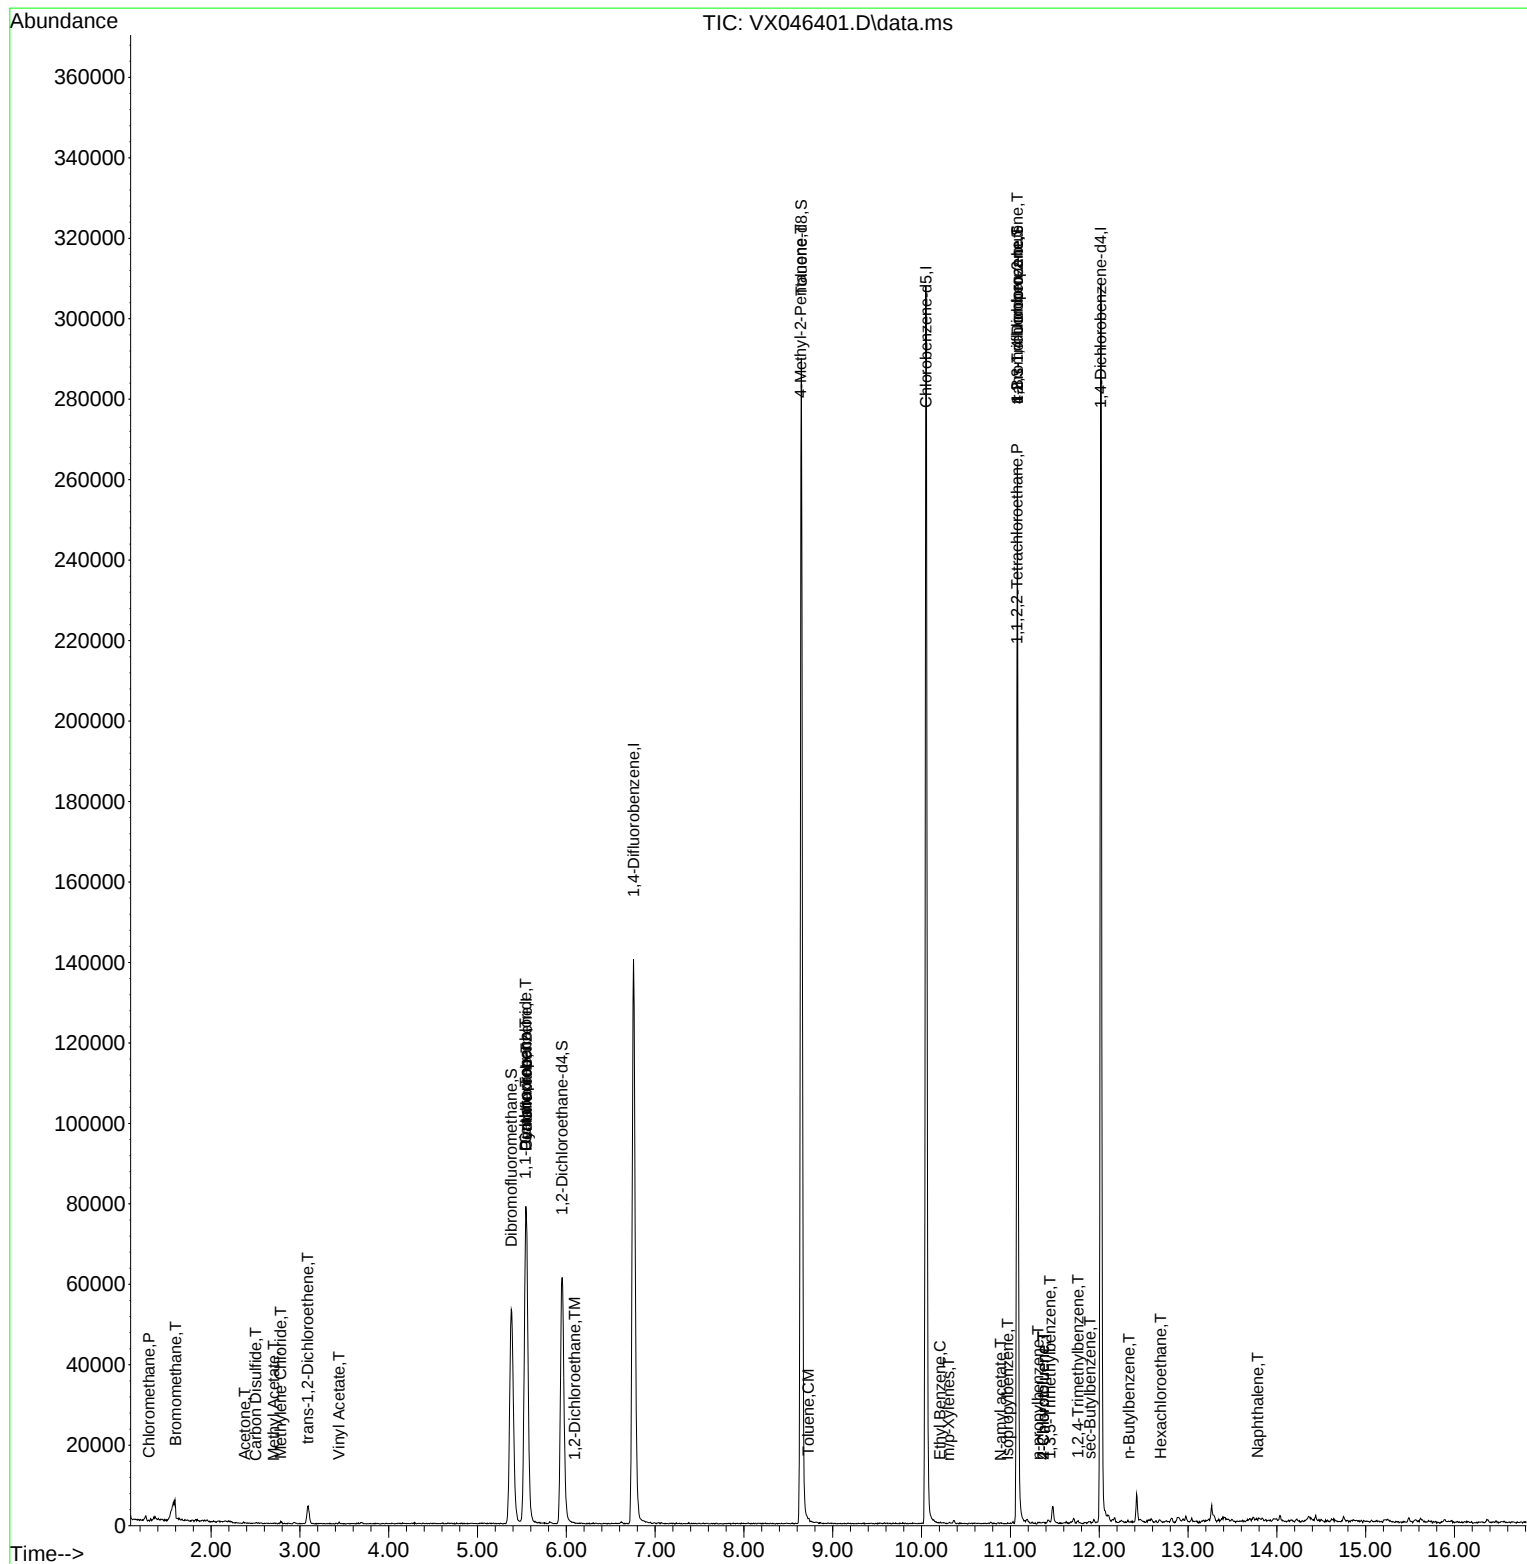




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX046401.D
Acq: 29 May 2025 15:57




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion:168 Resp: 66575
Ion Ratio Lower Upper
168 100
99 68.6 54.9 82.3



#3
Chloromethane
Concen: 0.040 ug/l
RT: 1.301 min Scan# 35
Delta R.T. -0.006 min
Lab File: VX046401.D
Acq: 29 May 2025 15:57

Tgt Ion: 50 Resp: 40
Ion Ratio Lower Upper
50 100
52 0.0 25.4 38.2#


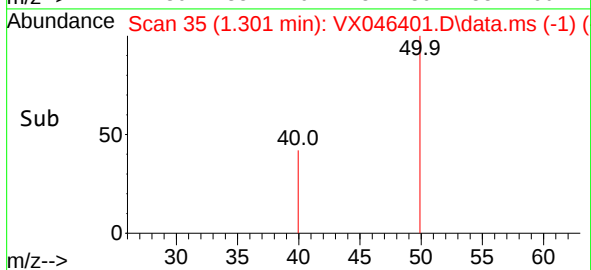




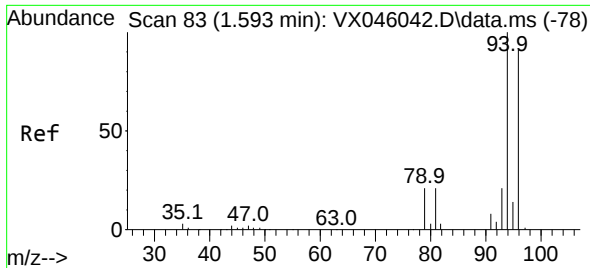

#5
Bromomethane
Concen: 0.068 ug/l
RT: 1.599 min Scan# 84
Delta R.T. 0.006 min
Lab File: VX046401.D
Acq: 29 May 2025 15:57




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion: 94 Resp: 29
Ion Ratio Lower Upper
94 100
96 93.7 72.8 109.2

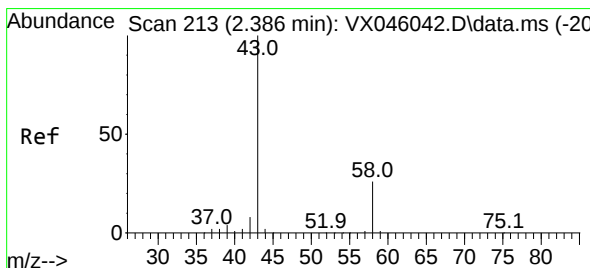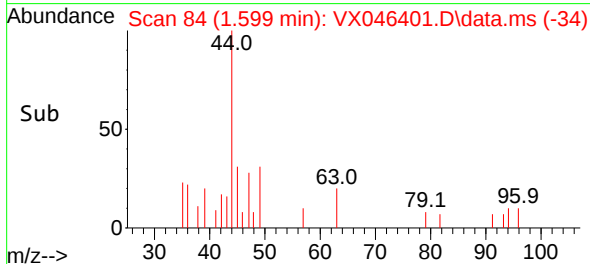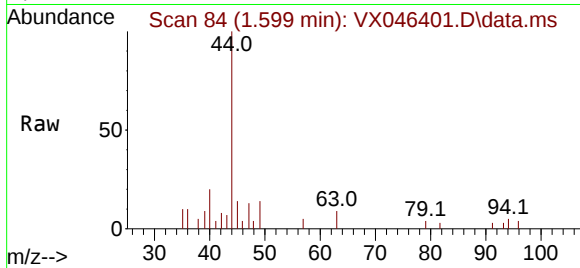

#16
Acetone
Concen: 0.553 ug/l
RT: 2.380 min Scan# 212
Delta R.T. -0.006 min
Lab File: VX046401.D
Acq: 29 May 2025 15:57

Tgt Ion: 43 Resp: 275
Ion Ratio Lower Upper
43 100
58 0.0 21.2 31.8#

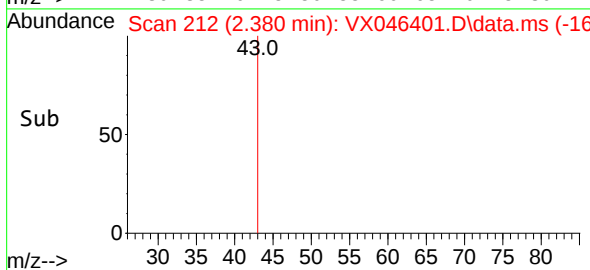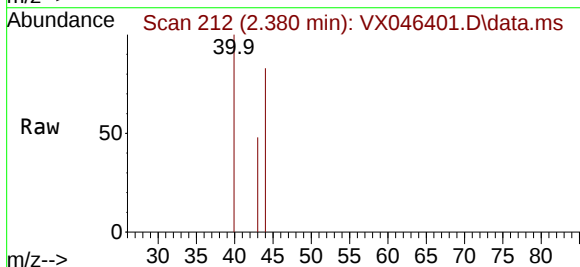



#17

Carbon Disulfide

Concen: 0.084 ug/l

RT: 2.502 min Scan# 21

Delta R.T. -0.000 min

Lab File: VX046401.D

Acq: 29 May 2025 15:57

Instrument :

MSVOA_X

ClientSampleId :





IBLK

Tgt Ion: 76 Resp: 157

Ion Ratio Lower Upper

76 100

78 0.0 7.0 10.4#

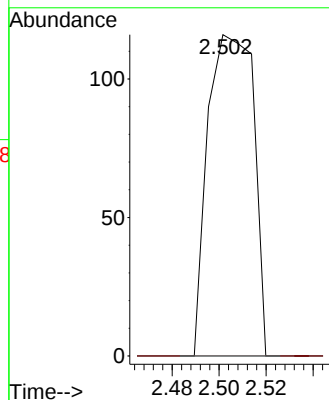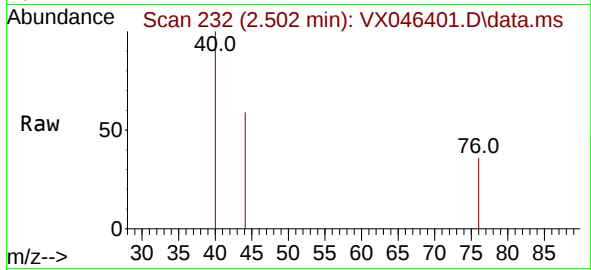

#18

Methyl Acetate

Concen: 0.126 ug/l

RT: 2.703 min Scan# 265

Delta R.T. -0.000 min

Lab File: VX046401.D




Acq: 29 May 2025 15:57


Tgt Ion: 43 Resp: 146

Ion Ratio Lower Upper

43 100

74 0.0 16.7 25.1#



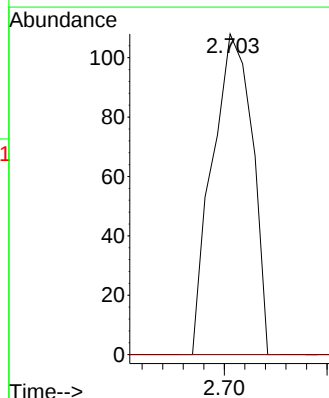





#20
Methylene Chloride
Concen: 0.298 ug/l
RT: 2.782 min Scan# 21
Delta R.T. 0.000 min
Lab File: VX046401.D
Acq: 29 May 2025 15:57




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion: 84 Resp: 284
Ion Ratio Lower Upper
84 100
49 125.2 113.9 170.9
51 0.0 33.5 50.3#
86 0.0 53.8 80.8#



#21
trans-1,2-Dichloroethene
Concen: 2.260 ug/l
RT: 3.087 min Scan# 328
Delta R.T. 0.000 min
Lab File: VX046401.D
Acq: 29 May 2025 15:57

Tgt Ion: 96 Resp: 1794
Ion Ratio Lower Upper
96 100
61 130.6 119.5 179.3
98 67.6 50.0 75.0




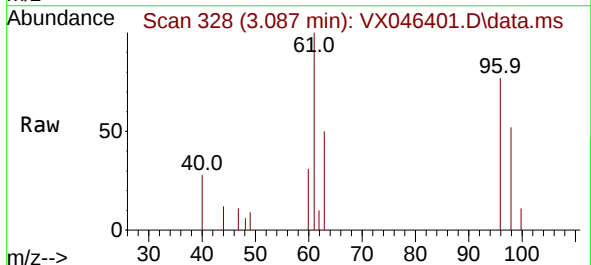




#23
 Vinyl Acetate
 Concen: 0.009 ug/l
 RT: 3.440 min Scan# 31
 Delta R.T. -0.280 min
 Lab File: VX046401.D
 Acq: 29 May 2025 15:57




Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK


Tgt Ion: 43 Resp: 24
 Ion Ratio Lower Upper
 43 100
 86 0.0 7.5 11.3#



#31
 Cyclohexane
 Concen: 1.366 ug/l
 RT: 5.550 min Scan# 732
 Delta R.T. 0.085 min
 Lab File: VX046401.D
 Acq: 29 May 2025 15:57

Tgt Ion: 56 Resp: 2021
 Ion Ratio Lower Upper
 56 100
 69 176.9 24.4 36.6#
 84 91.3 66.9 100.3

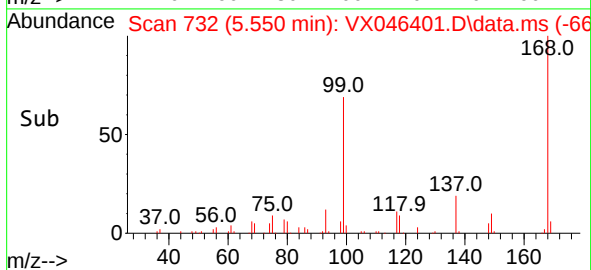



#33

1,2-Dichloroethane-d4

Concen: 52.743 ug/l

RT: 5.952 min Scan# 798

Delta R.T. -0.000 min

Lab File: VX046401.D

Acq: 29 May 2025 15:57

Instrument :

MSVOA_X

ClientSampleId :





IBLK

Tgt Ion: 65 Resp: 65463

Ion Ratio Lower Upper

65 100

67 49.4 0.0 99.0



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.757 min Scan# 930

Delta R.T. -0.000 min

Lab File: VX046401.D

Acq: 29 May 2025 15:57




Tgt Ion: 114 Resp: 133510


Ion Ratio Lower Upper

114 100

63 24.5 0.0 49.2

88 16.9 0.0 33.6



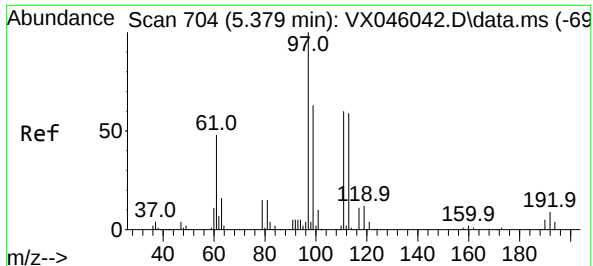

#35

Dibromofluoromethane

Concen: 48.724 ug/l

RT: 5.379 min Scan# 704

Delta R.T. -0.000 min

Lab File: VX046401.D


Acq: 29 May 2025 15:57

Instrument :




MSVOA_X

ClientSampleId :

IBLK

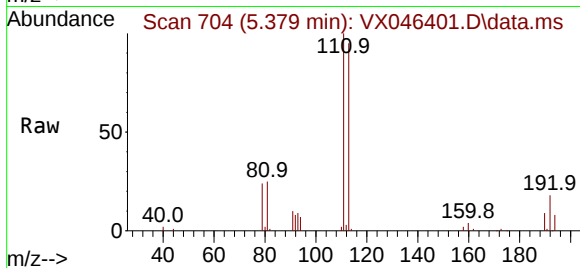

Tgt Ion:	113	Resp:	46844
Ion	Ratio	Lower	Upper
113	100		
111	104.4	83.1	124.7
192	17.1	13.3	19.9

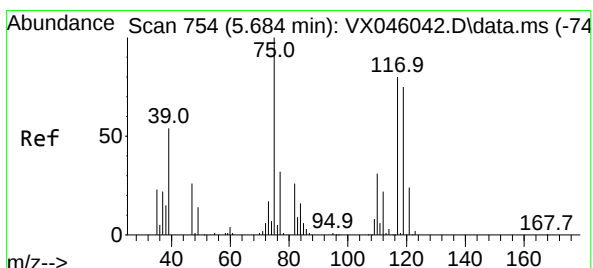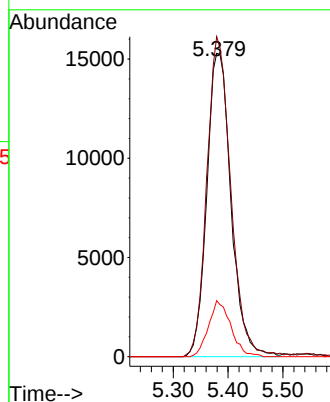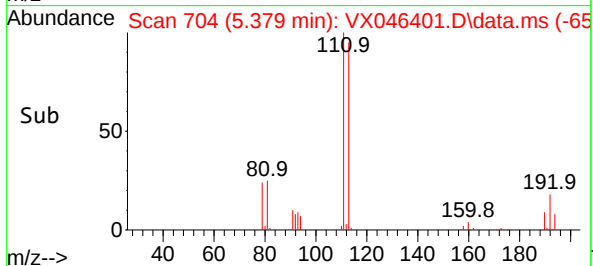

#36

1,1-Dichloropropene

Concen: 5.113 ug/l




RT: 5.538 min Scan# 730


Delta R.T. -0.146 min

Lab File: VX046401.D

Acq: 29 May 2025 15:57

Tgt Ion:	75	Resp:	6605
Ion	Ratio	Lower	Upper
75	100		
110	8.9	16.3	48.9#
77	0.0	24.3	36.5#


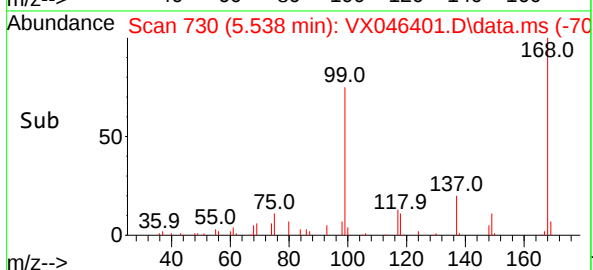

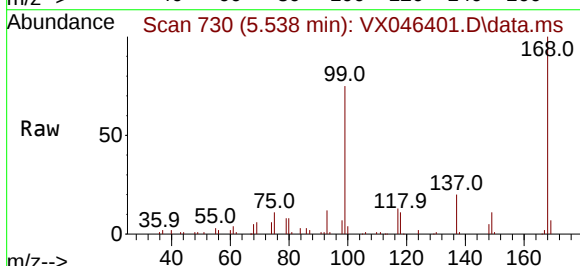




#38
Carbon Tetrachloride
Concen: 5.562 ug/l
RT: 5.544 min Scan# 71
Delta R.T. -0.128 min
Lab File: VX046401.D
Acq: 29 May 2025 15:57




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion:117 Resp: 8073
Ion Ratio Lower Upper
117 100
119 6.0 75.2 112.8#
121 0.0 24.2 36.4#



#42
1,2-Dichloroethane
Concen: 0.012 ug/l
RT: 6.092 min Scan# 821
Delta R.T. 0.012 min
Lab File: VX046401.D
Acq: 29 May 2025 15:57

Tgt Ion: 62 Resp: 20
Ion Ratio Lower Upper
62 100
98 0.0 0.0 15.2


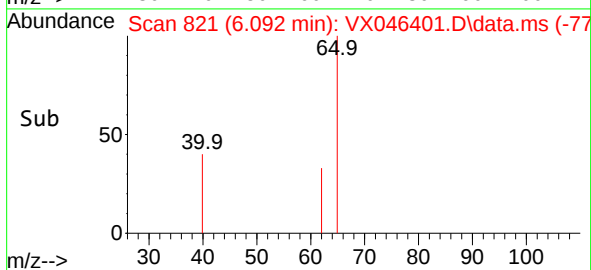






#50
Toluene-d8
Concen: 50.105 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX046401.D
Acq: 29 May 2025 15:57




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion: 98 Resp: 166728
Ion Ratio Lower Upper
98 100
100 65.6 53.5 80.3



#51
4-Methyl-2-Pentanone
Concen: 0.627 ug/l
RT: 8.641 min Scan# 1239
Delta R.T. 0.067 min
Lab File: VX046401.D
Acq: 29 May 2025 15:57

Tgt Ion: 43 Resp: 1013
Ion Ratio Lower Upper
43 100
58 157.5 28.9 43.3#


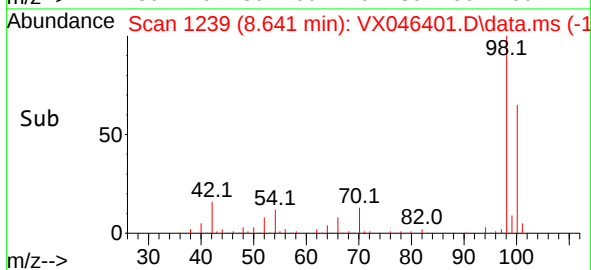






#52
Toluene
Concen: 0.072 ug/l
RT: 8.726 min Scan# 1253
Delta R.T. 0.012 min
Lab File: VX046401.D
Acq: 29 May 2025 15:57




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion: 92 Resp: 168
Ion Ratio Lower Upper
92 100
91 195.8 136.6 205.0

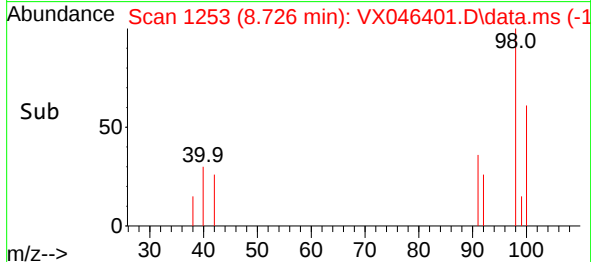

#62
4-Bromofluorobenzene
Concen: 51.893 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX046401.D
Acq: 29 May 2025 15:57

Tgt Ion: 95 Resp: 66237
Ion Ratio Lower Upper
95 100
174 69.4 0.0 135.8
176 65.3 0.0 131.4




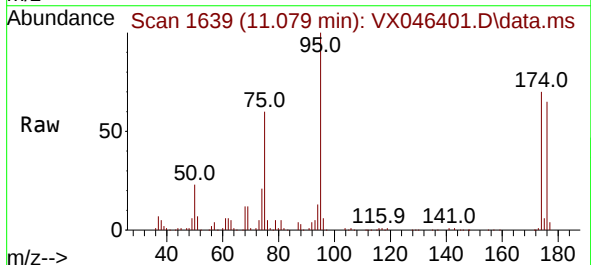




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.049 min Scan# 1470
Delta R.T. 0.000 min
Lab File: VX046401.D
Acq: 29 May 2025 15:57




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion:117 Resp: 128473
Ion Ratio Lower Upper
117 100
82 63.0 50.6 76.0
119 31.7 25.8 38.6

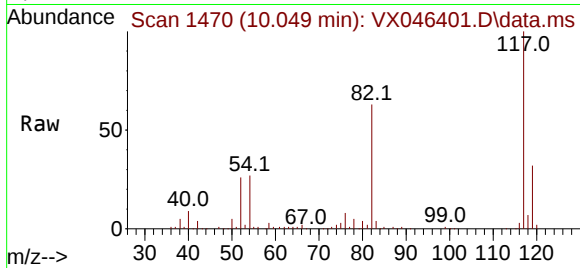

#67
Ethyl Benzene
Concen: 0.018 ug/l
RT: 10.208 min Scan# 1496
Delta R.T. 0.018 min
Lab File: VX046401.D
Acq: 29 May 2025 15:57

Tgt Ion: 91 Resp: 91
Ion Ratio Lower Upper
91 100
106 0.0 23.4 35.2#




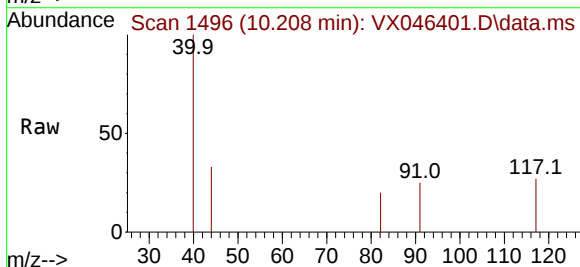




#68
m/p-Xylenes
Concen: 0.010 ug/l
RT: 10.305 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX046401.D
Acq: 29 May 2025 15:57




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion:106 Resp: 19
Ion Ratio Lower Upper
106 100
91 826.3 171.2 256.8#

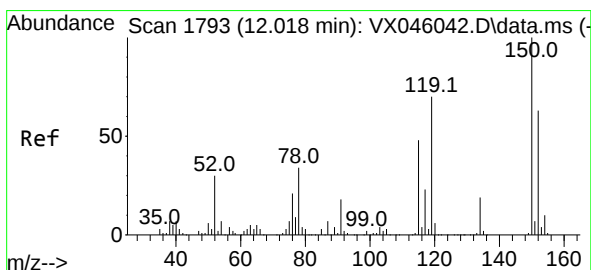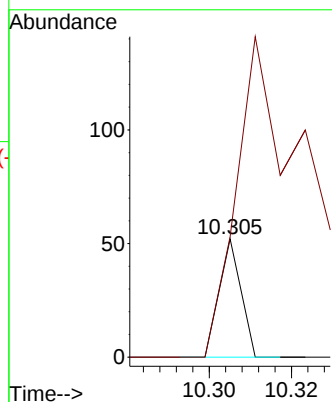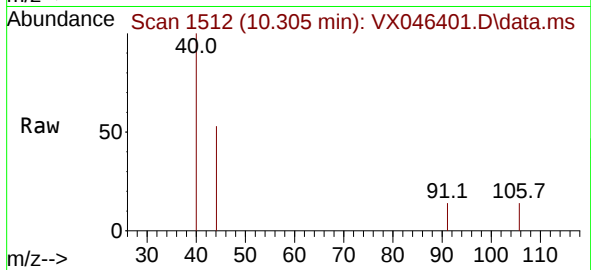

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. -0.000 min
Lab File: VX046401.D
Acq: 29 May 2025 15:57

Tgt Ion:152 Resp: 56641
Ion Ratio Lower Upper
152 100
115 66.3 46.9 140.7
150 156.7 0.0 351.0


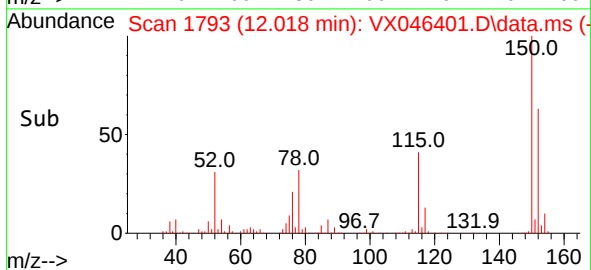
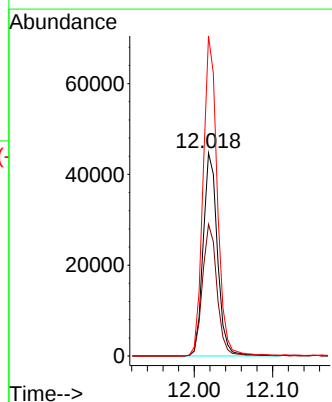





#73
Isopropylbenzene
Concen: 0.011 ug/l
RT: 10.970 min Scan# 1621
Delta R.T. 0.012 min
Lab File: VX046401.D
Acq: 29 May 2025 15:57




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion:105 Resp: 48
Ion Ratio Lower Upper
105 100
120 0.0 12.8 38.4#

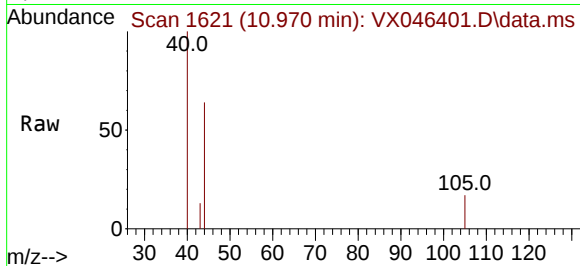

#74
N-ethyl acetate
Concen: 0.023 ug/l
RT: 10.890 min Scan# 1608
Delta R.T. 0.049 min
Lab File: VX046401.D
Acq: 29 May 2025 15:57

Tgt Ion: 43 Resp: 50
Ion Ratio Lower Upper
43 100
70 0.0 30.9 46.3#
55 44.0 18.7 28.1#
61 0.0 17.1 25.7#



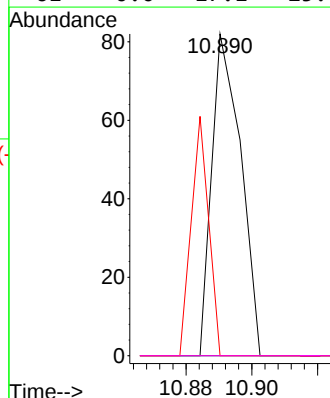
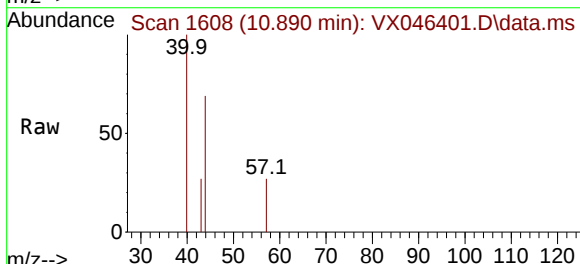




#75
 1,1,2-Tetrachloroethane
 Concen: 0.049 ug/l
 RT: 11.073 min Scan# 1638
 Delta R.T. -0.134 min
 Lab File: VX046401.D
 Acq: 29 May 2025 15:57




Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK


Tgt Ion: 83 Resp: 75
 Ion Ratio Lower Upper
 83 100
 131 0.0 5.0 14.9#
 85 26.7 31.9 95.7#

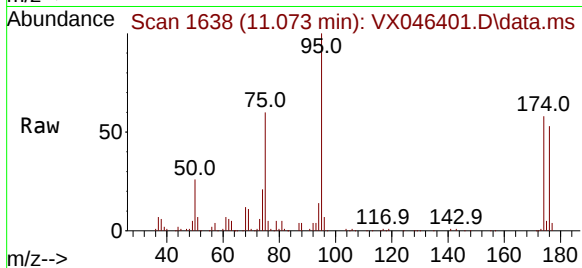

#76
 1,2,3-Trichloropropane
 Concen: 28.131 ug/l
 RT: 11.079 min Scan# 1639
 Delta R.T. -0.159 min
 Lab File: VX046401.D
 Acq: 29 May 2025 15:57

Tgt Ion: 75 Resp: 38353
 Ion Ratio Lower Upper
 75 100
 77 1.2 20.5 61.5#


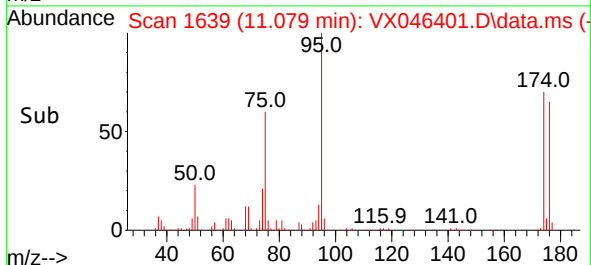

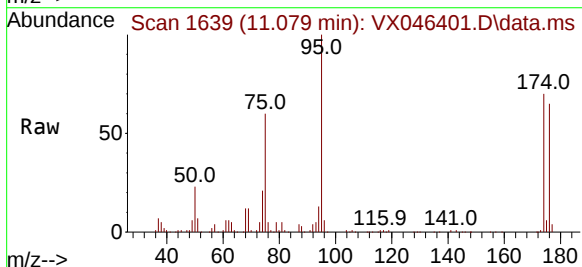




#78
n-propylbenzene
Concen: 0.051 ug/l
RT: 11.311 min Scan# 1677
Delta R.T. 0.012 min
Lab File: VX046401.D
Acq: 29 May 2025 15:57




Instrument :
MSVOA_X
ClientSampleId :
IBLK


Tgt Ion: 91 Resp: 261
Ion Ratio Lower Upper
91 100
120 0.0 10.8 32.4#

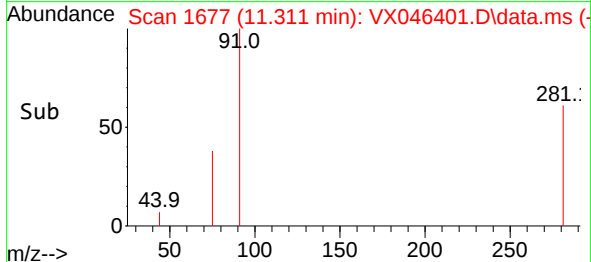

#79
2-Chlorotoluene
Concen: 0.026 ug/l
RT: 11.372 min Scan# 1687
Delta R.T. 0.012 min
Lab File: VX046401.D
Acq: 29 May 2025 15:57

Tgt Ion: 91 Resp: 86
Ion Ratio Lower Upper
91 100
126 0.0 15.6 46.7#

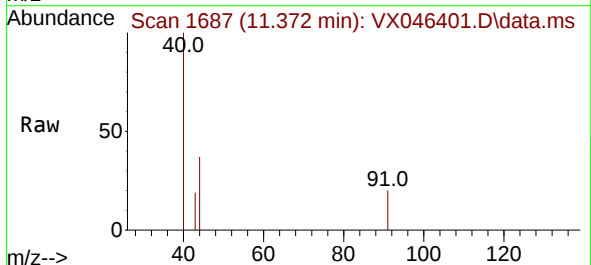



#80

1,3,5-Trimethylbenzene

Concen: 0.018 ug/l

RT: 11.445 min Scan# 1

Delta R.T. -0.006 min

Lab File: VX046401.D

Acq: 29 May 2025 15:57

Instrument :

MSVOA_X

ClientSampleId :





IBLK

Tgt Ion:105 Resp: 66

Ion Ratio Lower Upper

105 100

120 0.0 23.1 69.2#

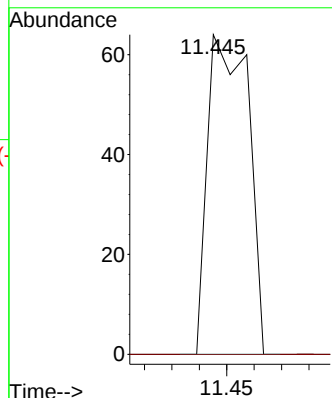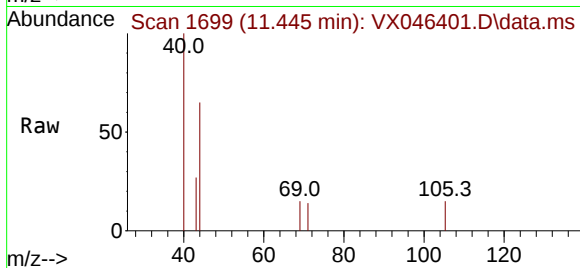

#81

trans-1,4-Dichloro-2-butene

Concen: 91.585 ug/l

RT: 11.079 min Scan# 1639

Delta R.T. 0.061 min

Lab File: VX046401.D

Acq: 29 May 2025 15:57




Tgt Ion: 75 Resp: 38353


Ion Ratio Lower Upper

75 100

53 0.0 100.5 150.7#

89 0.1 37.0 55.6#

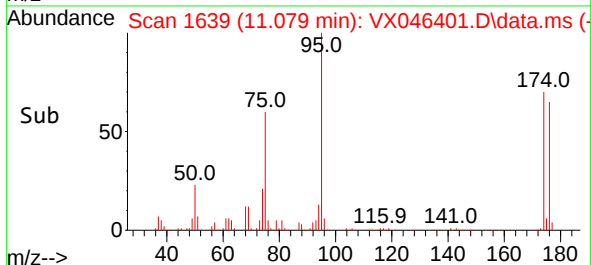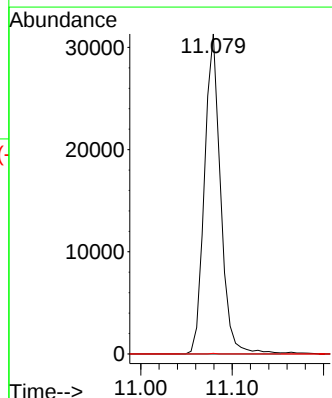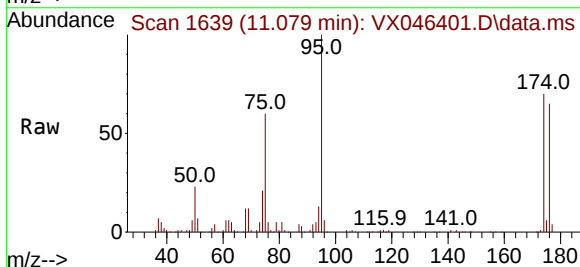



#82

4-Chlorotoluene

Concen: 0.023 ug/l

RT: 11.372 min Scan# 1

Delta R.T. -0.079 min

Lab File: VX046401.D

Acq: 29 May 2025 15:57

Instrument :

MSVOA_X

ClientSampleId :





IBLK

Tgt Ion: 91 Resp: 86

Ion Ratio Lower Upper

91 100

126 0.0 13.3 39.8#

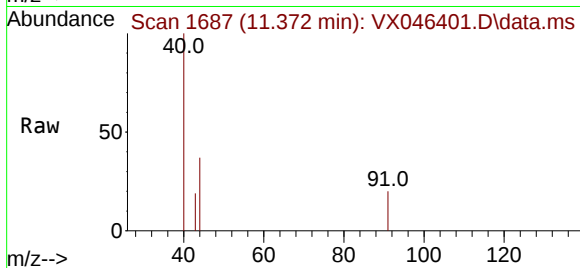

#84

1,2,4-Trimethylbenzene

Concen: 0.088 ug/l

RT: 11.762 min Scan# 1751

Delta R.T. 0.012 min

Lab File: VX046401.D




Acq: 29 May 2025 15:57


Tgt Ion: 105 Resp: 327

Ion Ratio Lower Upper

105 100

120 24.2 21.2 63.6




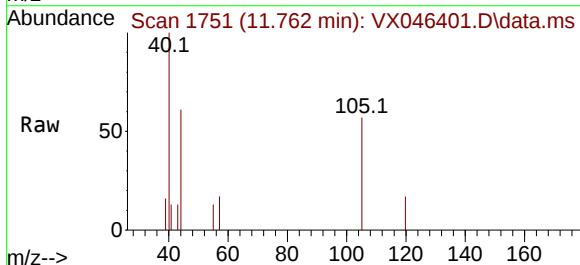




#85
 sec-Butylbenzene
 Concen: 0.010 ug/l
 RT: 11.896 min Scan# 11
 Delta R.T. 0.006 min
 Lab File: VX046401.D
 Acq: 29 May 2025 15:57




Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK


Tgt Ion:105 Resp: 45
 Ion Ratio Lower Upper
 105 100
 134 0.0 9.7 29.1#

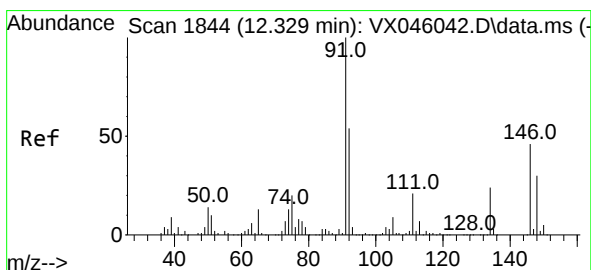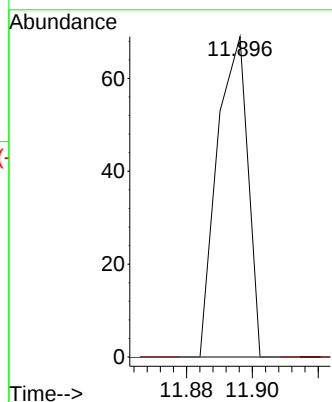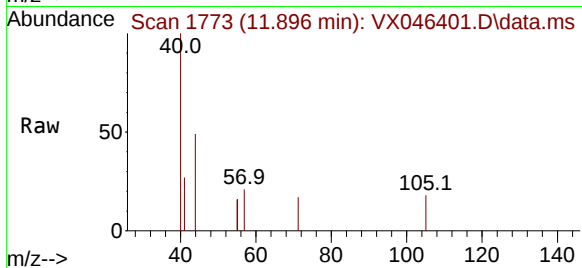

#89
 n-Butylbenzene
 Concen: 0.045 ug/l
 RT: 12.335 min Scan# 1845
 Delta R.T. 0.006 min
 Lab File: VX046401.D
 Acq: 29 May 2025 15:57

Tgt Ion: 91 Resp: 148
 Ion Ratio Lower Upper
 91 100
 92 0.0 26.9 80.7#
 134 0.0 11.8 35.3#

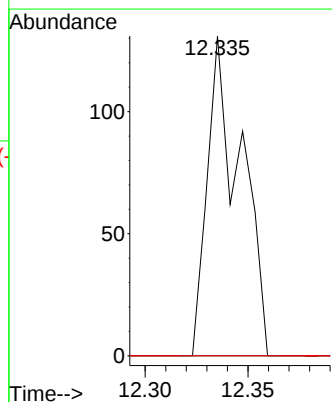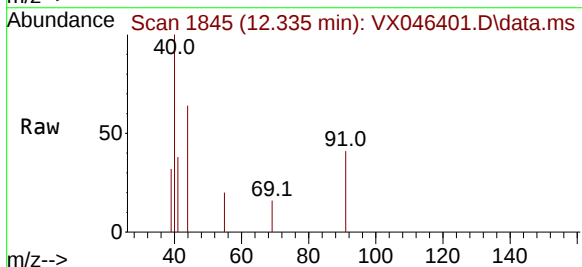



#90

Hexachloroethane

Concen: 0.089 ug/l

RT: 12.695 min Scan# 1904

Delta R.T. 0.159 min

Lab File: VX046401.D

Acq: 29 May 2025 15:57

Instrument :

MSVOA_X

ClientSampleId :





IBLK

Tgt Ion:117 Resp: 59

Ion Ratio Lower Upper

117 100

201 0.0 31.6 94.7#

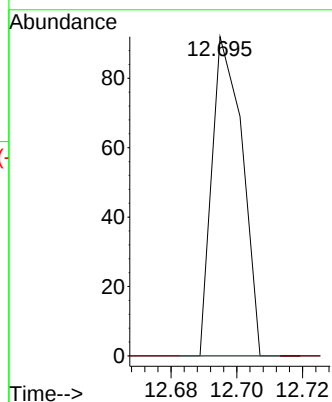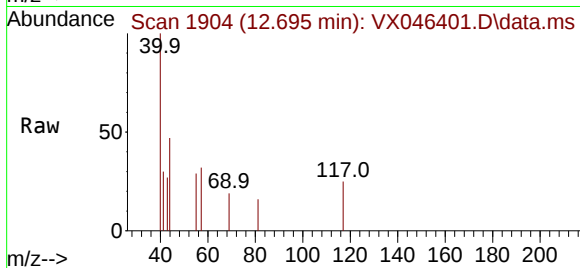

#95

Naphthalene

Concen: 0.130 ug/l

RT: 13.786 min Scan# 2083

Delta R.T. 0.012 min

Lab File: VX046401.D

Acq: 29 May 2025 15:57

Tgt Ion:128 Resp: 514

Ion Ratio Lower Upper

128 100

127 0.0 10.4 15.6#

129 0.0 8.6 13.0#

