
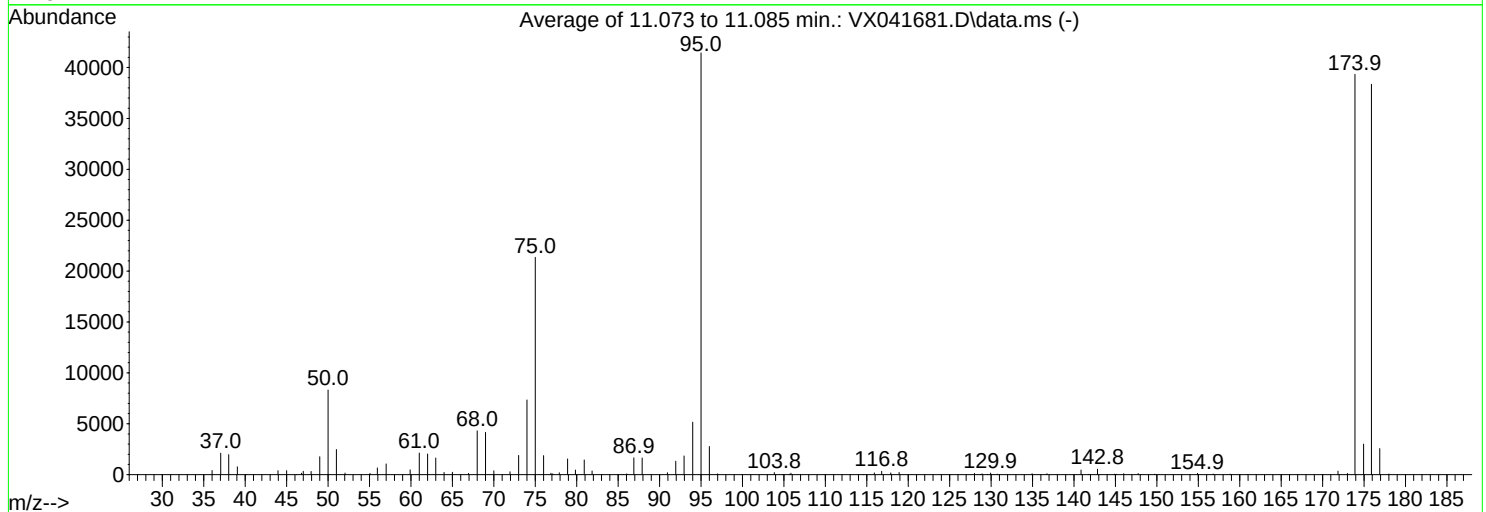


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX053024\  
Data File : VX041681.D  
Acq On : 30 May 2024 08:53  
Operator : JC/MD  
Sample : BFB  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\624X051524W.M  
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS  
Last Update : Thu May 16 05:13:13 2024

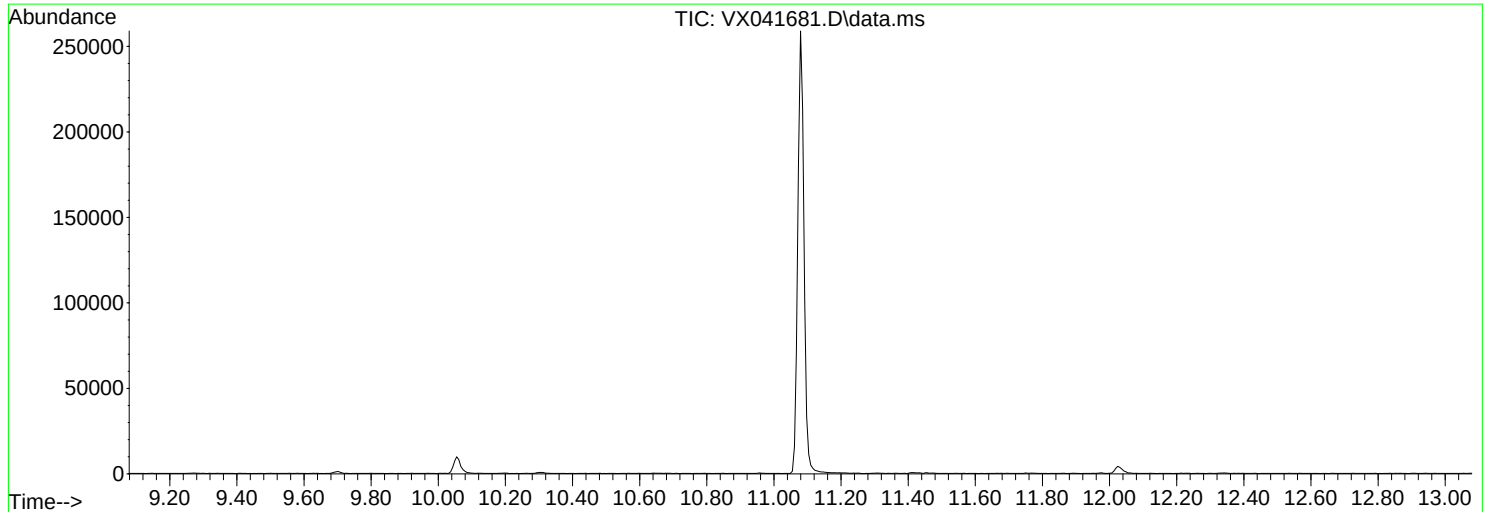

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw   | Result    |
|--------|---------|--------|--------|-------|-------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn   | Pass/Fail |
| 50     | 95      | 15     | 40     | 20.1  | 8317  | PASS      |
| 75     | 95      | 30     | 60     | 51.5  | 21341 | PASS      |
| 95     | 95      | 100    | 100    | 100.0 | 41440 | PASS      |
| 96     | 95      | 5      | 9      | 6.7   | 2772  | PASS      |
| 173    | 174     | 0.00   | 2      | 0.3   | 131   | PASS      |
| 174    | 95      | 50     | 100    | 94.9  | 39325 | PASS      |
| 175    | 174     | 5      | 9      | 7.6   | 3006  | PASS      |
| 176    | 174     | 95     | 101    | 97.5  | 38357 | PASS      |
| 177    | 176     | 5      | 9      | 6.7   | 2570  | PASS      |