

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX053025\
 Data File : VX046411.D
 Acq On : 30 May 2025 11:06
 Operator : JC/MD
 Sample : VX0530WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0530WBL01

Quant Time: May 30 23:23:32 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X050525W.M
 Quant Title : SW846 8260
 QLast Update : Tue May 06 07:12:22 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	64533	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.757	114	129905	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.049	117	123011	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	51208	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.946	65	64990	54.019	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 108.040%	
35) Dibromofluoromethane	5.379	113	46982	50.224	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 100.440%	
50) Toluene-d8	8.647	98	162314	50.132	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 100.260%	
62) 4-Bromofluorobenzene	11.079	95	63110	50.815	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	= 101.640%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX053025\
Data File : VX046411.D
Acq On : 30 May 2025 11:06
Operator : JC/MD
Sample : VX0530WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0530WBL01

Quant Time: May 30 23:23:32 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X050525W.M
Quant Title : SW846 8260
QLast Update : Tue May 06 07:12:22 2025
Response via : Initial Calibration




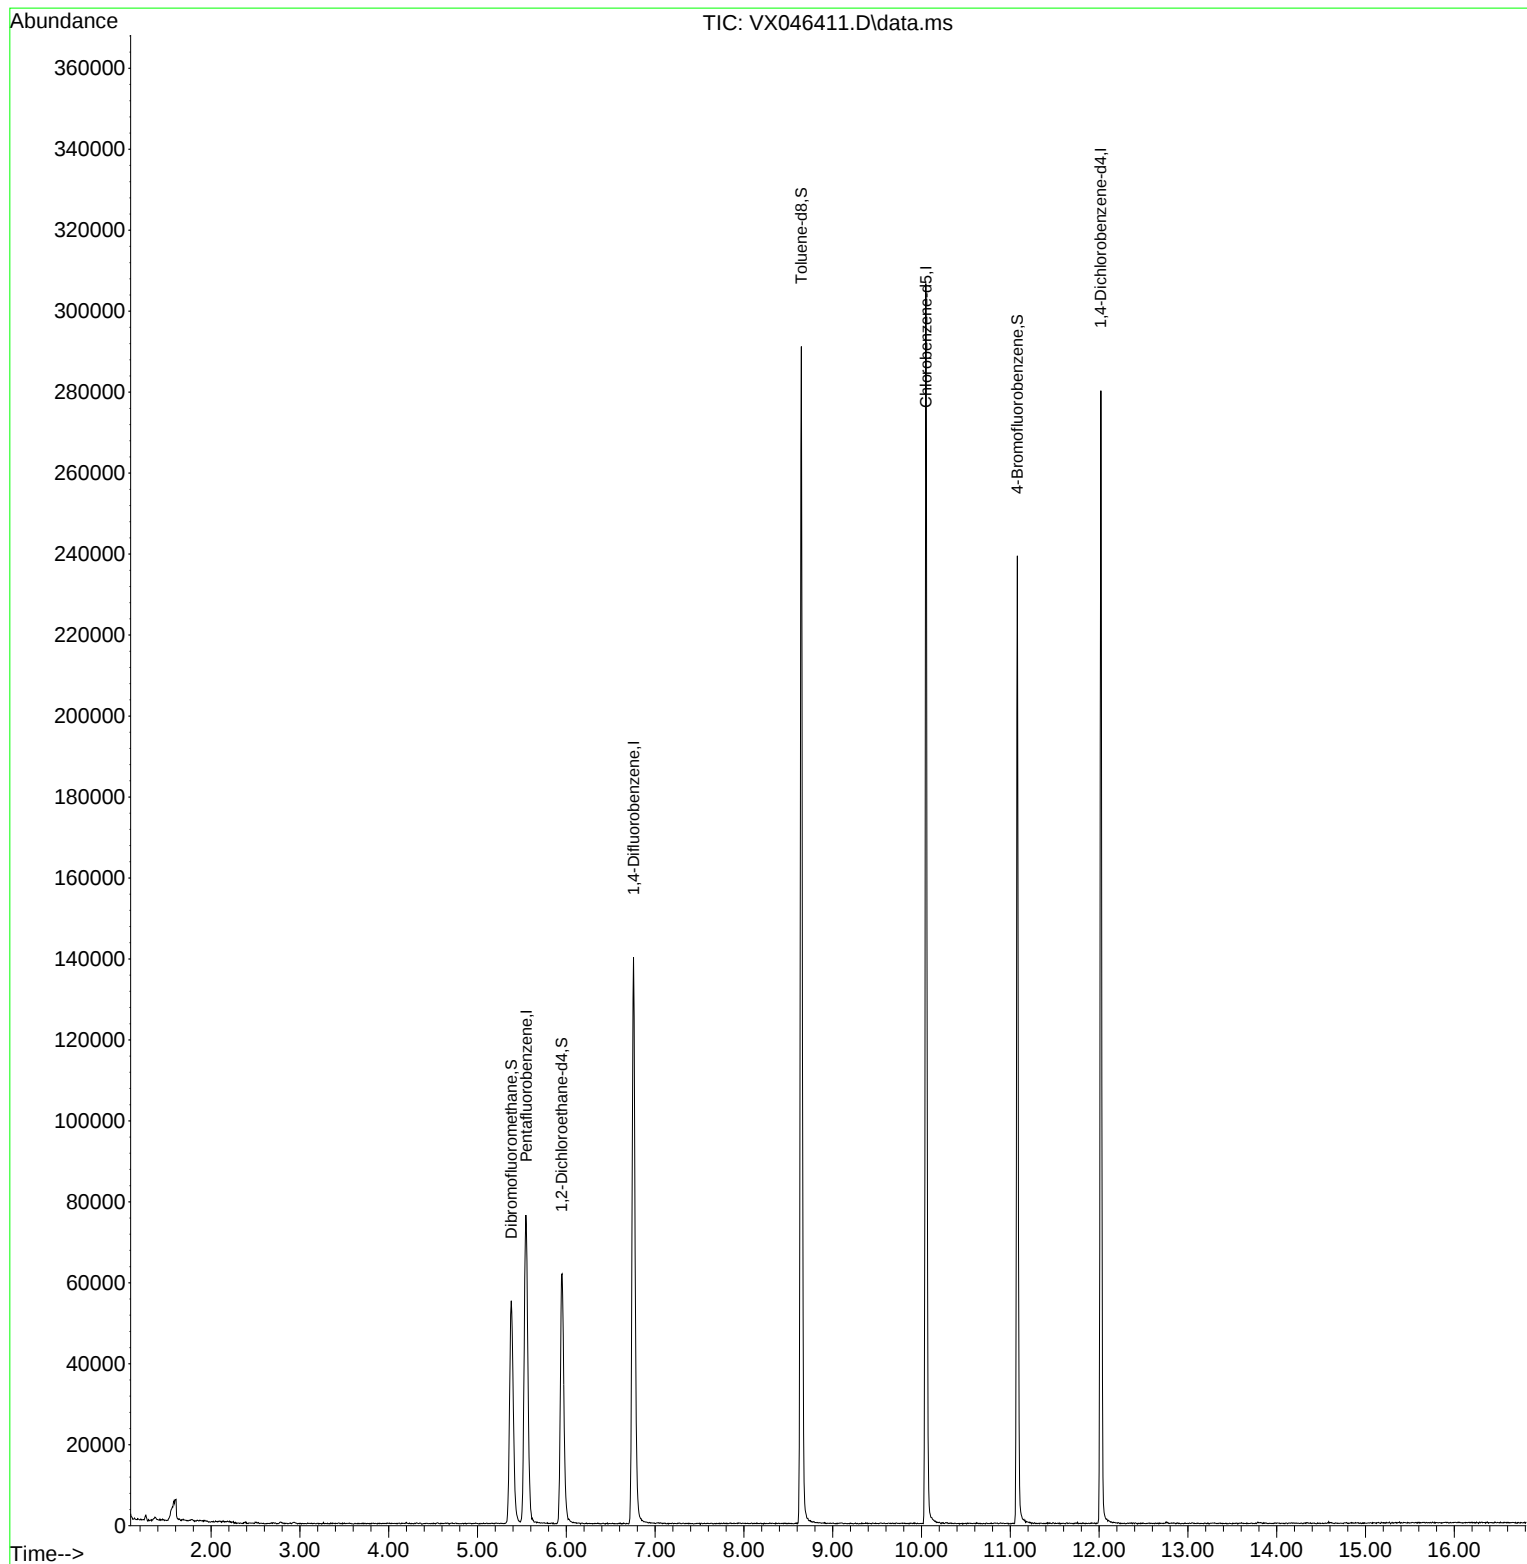


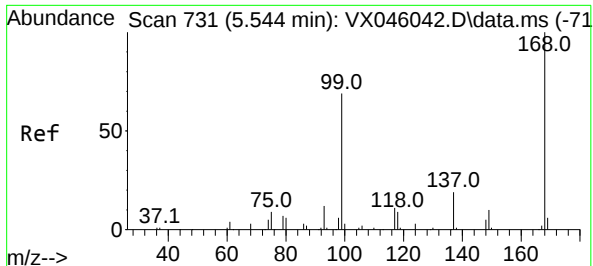

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 71
Delta R.T. 0.006 min
Lab File: VX046411.D
Acq: 30 May 2025 11:06




Instrument :
MSVOA_X
ClientSampleId :
VX0530WBL01


Tgt Ion:168 Resp: 64533
Ion Ratio Lower Upper
168 100
99 67.1 54.9 82.3

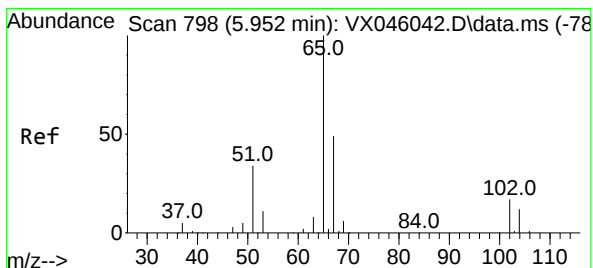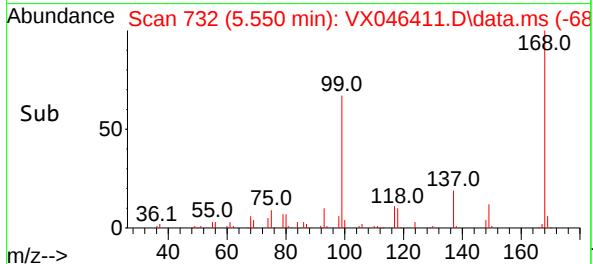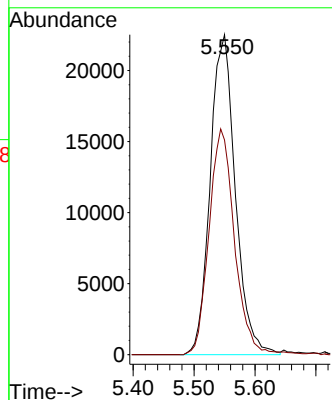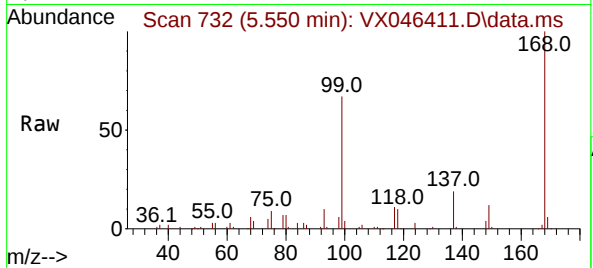

#33
1,2-Dichloroethane-d4
Concen: 54.019 ug/l
RT: 5.946 min Scan# 797
Delta R.T. -0.006 min
Lab File: VX046411.D
Acq: 30 May 2025 11:06

Tgt Ion: 65 Resp: 64990
Ion Ratio Lower Upper
65 100
67 48.5 0.0 99.0


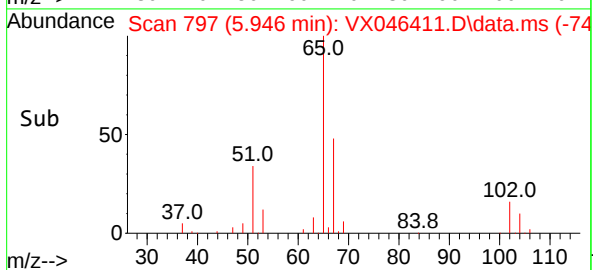
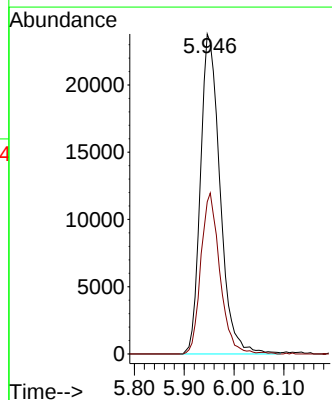
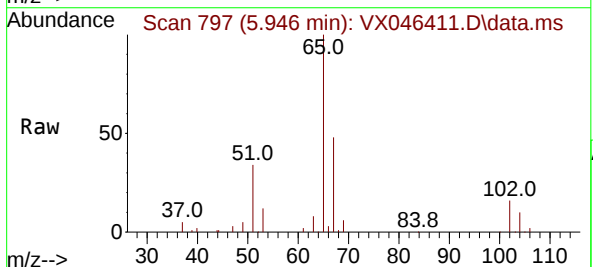


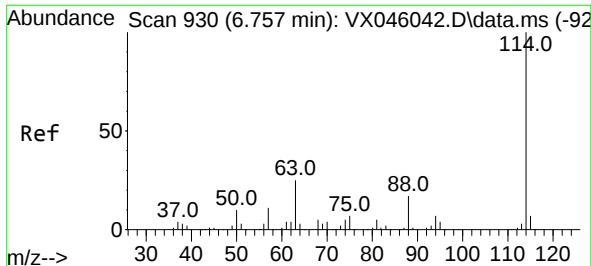

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.757 min Scan# 911
Delta R.T. 0.000 min
Lab File: VX046411.D
Acq: 30 May 2025 11:06




Instrument :
MSVOA_X
ClientSampleId :
VX0530WBL01


Tgt Ion:114 Resp: 129905
Ion Ratio Lower Upper
114 100
63 23.8 0.0 49.2
88 17.1 0.0 33.6

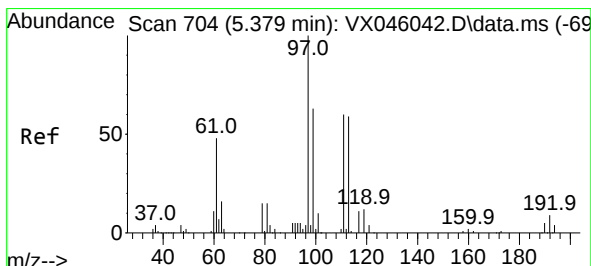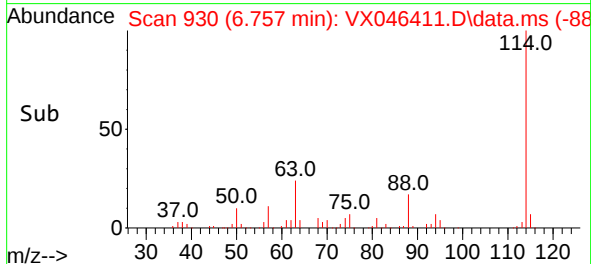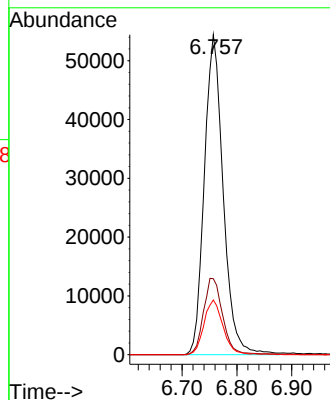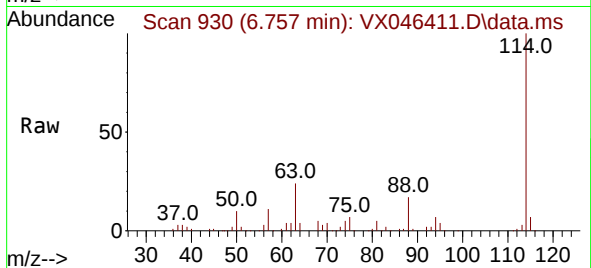

#35
Dibromofluoromethane
Concen: 50.224 ug/l
RT: 5.379 min Scan# 704
Delta R.T. 0.000 min
Lab File: VX046411.D
Acq: 30 May 2025 11:06

Tgt Ion:113 Resp: 46982
Ion Ratio Lower Upper
113 100
111 103.8 83.1 124.7
192 17.1 13.3 19.9


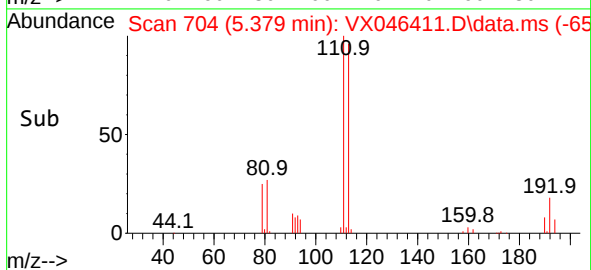
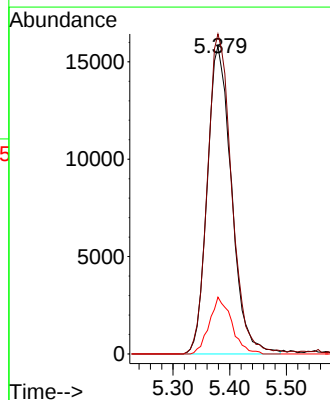
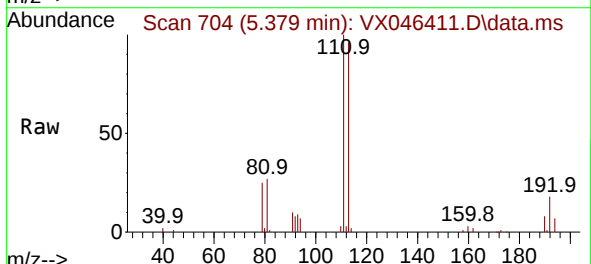


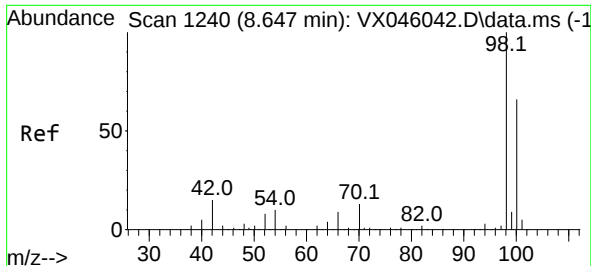

#50
Toluene-d8
Concen: 50.132 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX046411.D
Acq: 30 May 2025 11:06




Instrument :
MSVOA_X
ClientSampleId :
VX0530WBL01


Tgt Ion: 98 Resp: 162314
Ion Ratio Lower Upper
98 100
100 65.7 53.5 80.3

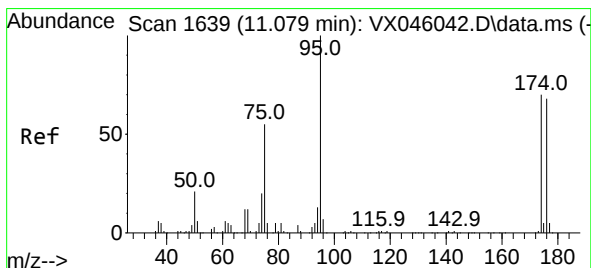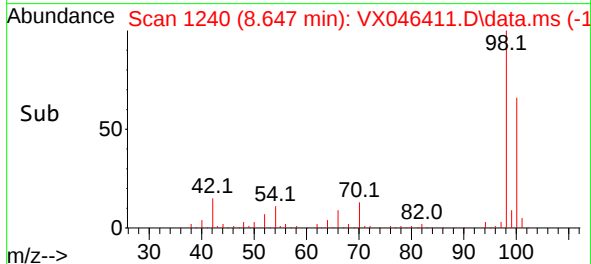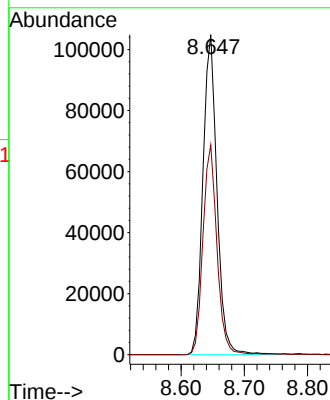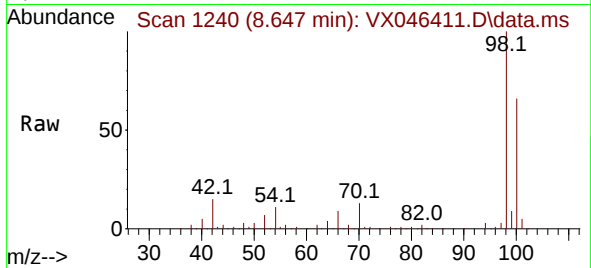

#62
4-Bromofluorobenzene
Concen: 50.815 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX046411.D
Acq: 30 May 2025 11:06

Tgt Ion: 95 Resp: 63110
Ion Ratio Lower Upper
95 100
174 66.6 0.0 135.8
176 62.3 0.0 131.4

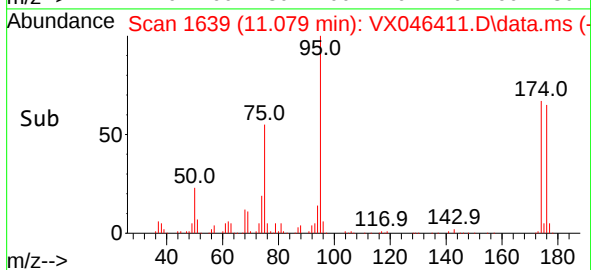
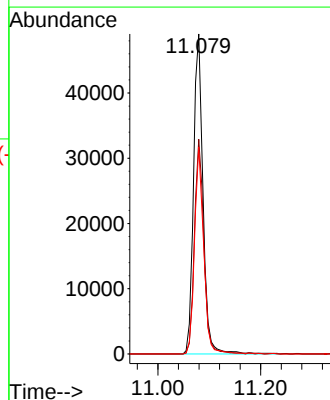
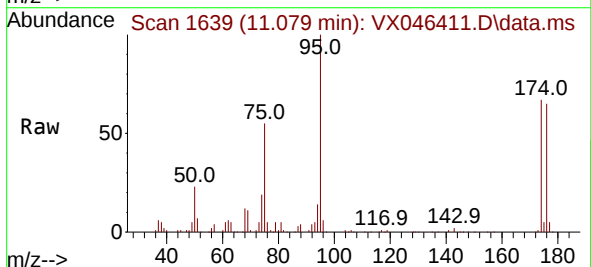


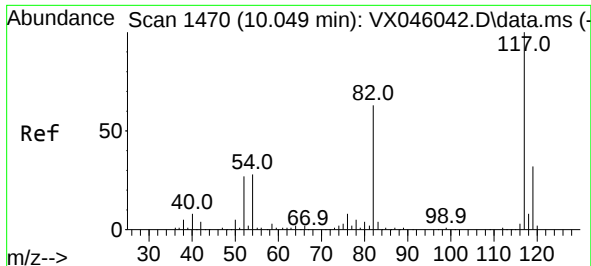

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.049 min Scan# 1470
Delta R.T. 0.000 min
Lab File: VX046411.D
Acq: 30 May 2025 11:06

Instrument :
MSVOA_X
ClientSampleId :
VX0530WBL01

Tgt Ion:117 Resp: 123011
Ion Ratio Lower Upper
117 100
82 62.6 50.6 76.0
119 31.1 25.8 38.6

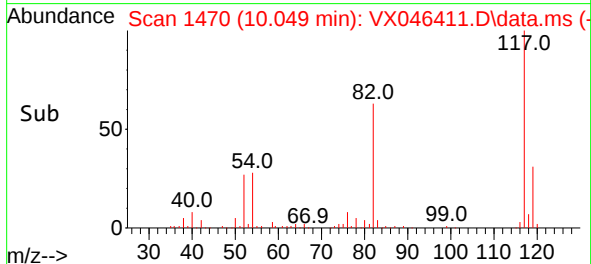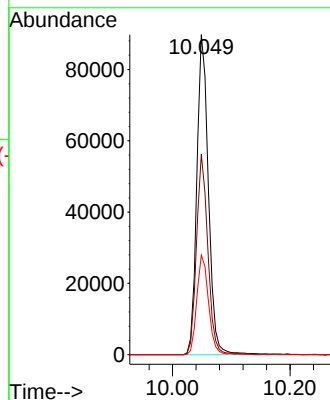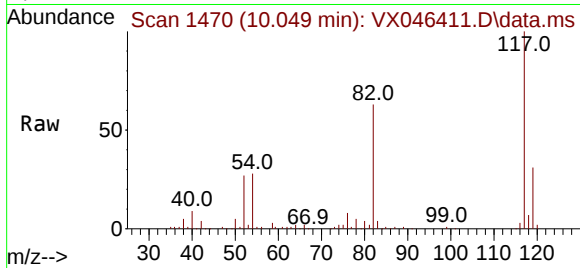

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. 0.000 min
Lab File: VX046411.D
Acq: 30 May 2025 11:06

Tgt Ion:152 Resp: 51208
Ion Ratio Lower Upper
152 100
115 66.9 46.9 140.7
150 157.0 0.0 351.0

