


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX053119\
 Data File : VX009998.D
 Acq On : 31 May 2019 20:17
 Operator : JC/SP
 Sample : BFB
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X052819W.M
 Title : SW846 8260
 Last Update : Wed May 29 04:00:56 2019

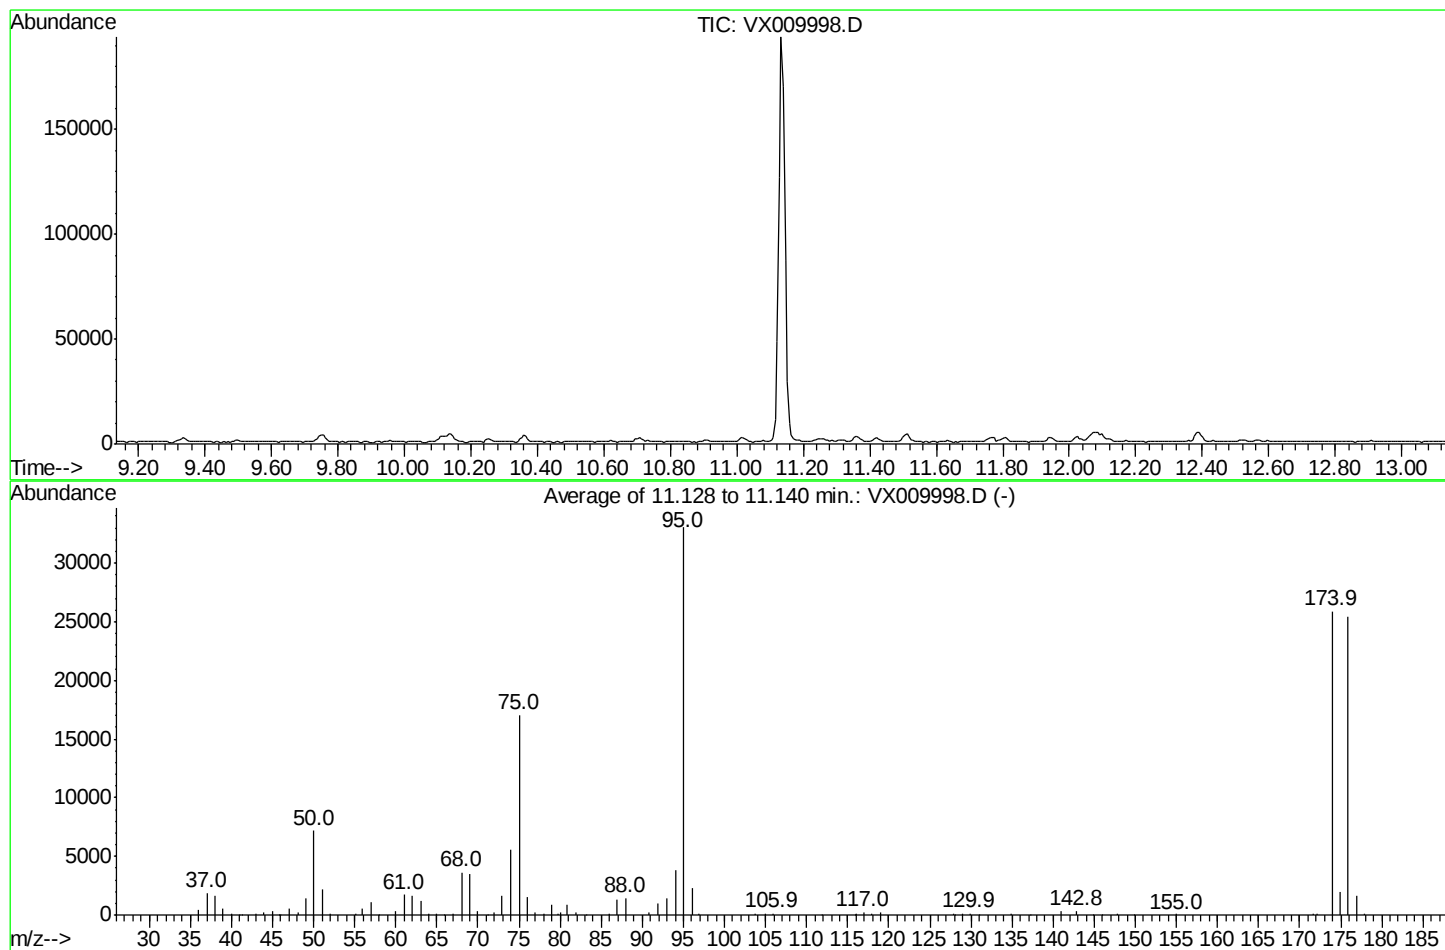

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.7	7173	PASS
75	95	30	60	51.6	17056	PASS
95	95	100	100	100.0	33048	PASS
96	95	5	9	6.8	2248	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	78.4	25901	PASS
175	174	5	9	7.7	2003	PASS
176	174	95	101	98.2	25432	PASS
177	176	5	9	6.3	1594	PASS