

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX060120\
 Data File : VX016519.D
 Acq On : 01 Jun 2020 11:34
 Operator : JC/SP
 Sample : L2799-02
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 Z2-TB7-200527

Quant Time: Jun 02 02:01:07 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X052720W.M
 Quant Title : SW846 8260
 QLast Update : Wed May 27 16:31:05 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.63	168	346679	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.83	114	556499	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	562794	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	282618	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	6.03	65	197967	45.98	ug/l	0.00
Spiked Amount 50.000			Recovery	=	91.96%	
35) Dibromofluoromethane	5.46	113	158482	46.25	ug/l	0.00
Spiked Amount 50.000			Recovery	=	92.50%	
50) Toluene-d8	8.70	98	698078	52.34	ug/l	0.00
Spiked Amount 50.000			Recovery	=	104.68%	
62) 4-Bromofluorobenzene	11.12	95	284461	55.20	ug/l	0.00
Spiked Amount 50.000			Recovery	=	110.40%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX060120\
Data File : VX016519.D
Acq On : 01 Jun 2020 11:34
Operator : JC/SP
Sample : L2799-02
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
Z2-TB7-200527

Quant Time: Jun 02 02:01:07 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X052720W.M
Quant Title : SW846 8260
QLast Update : Wed May 27 16:31:05 2020
Response via : Initial Calibration

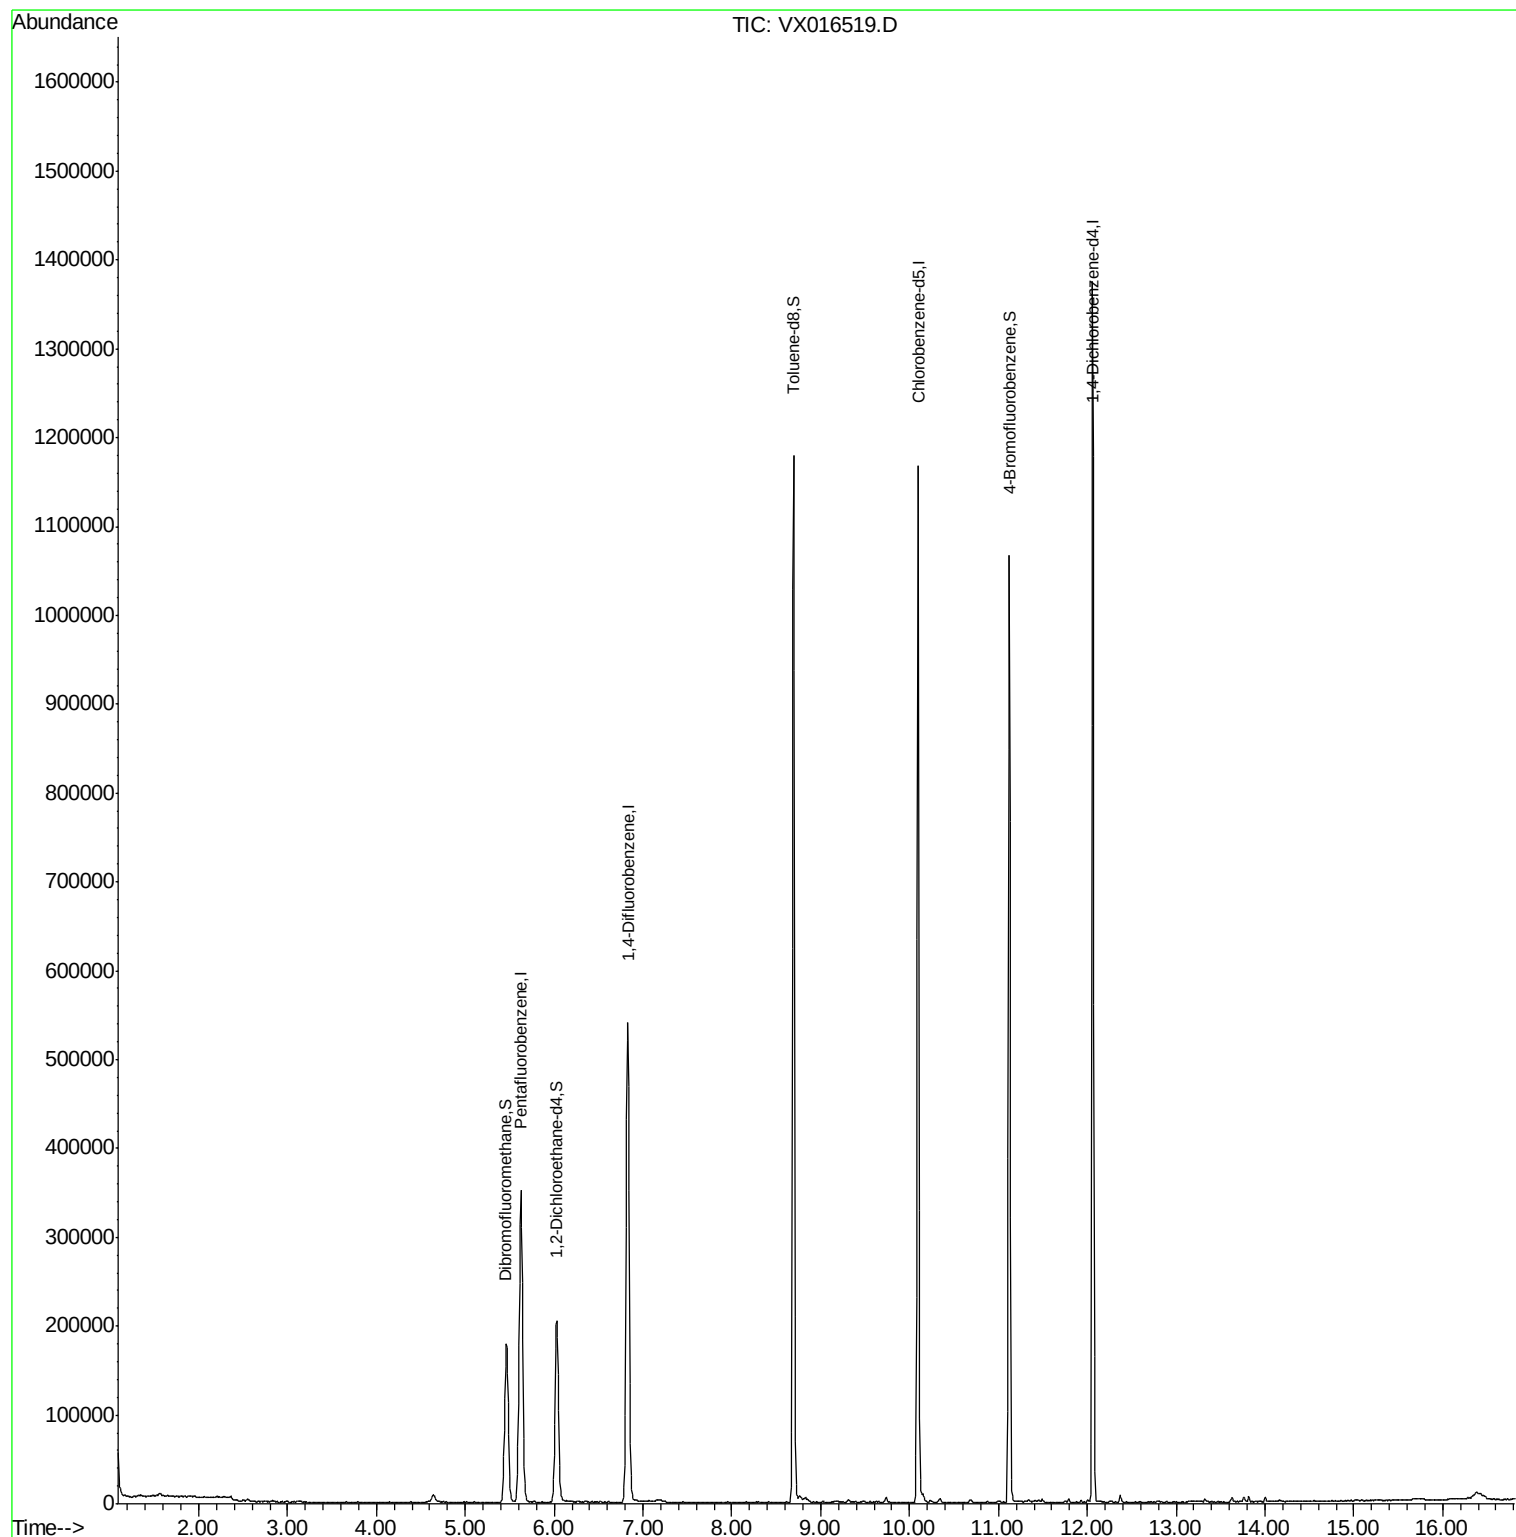

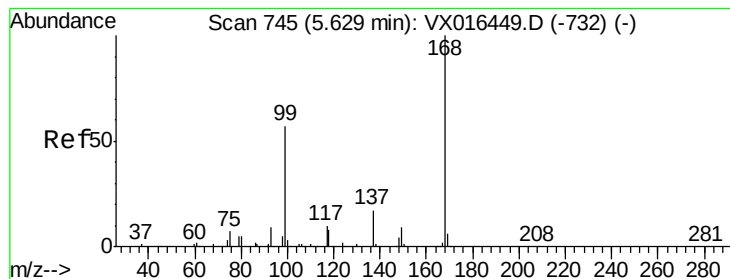

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.63 min Scan# 745

Delta R.T. -0.00 min

Lab File: VX016519.D

Acq: 01 Jun 2020 11:34

Instrument :

MSVOA_X

ClientSampleId :


Z2-TB7-200527

Tot Ion:168 Resp: 346679

Ion Ratio Lower Upper

168 100

99 53.9 45.2 67.8

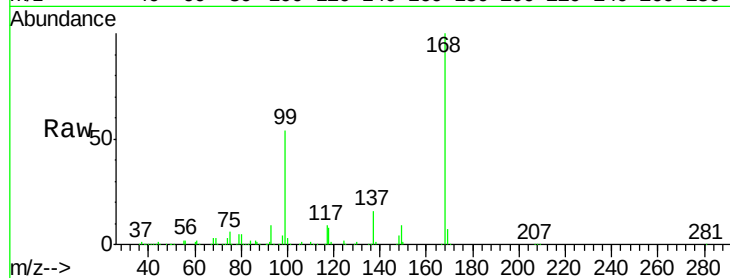

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.63



150000

100000

50000

0

Time-->

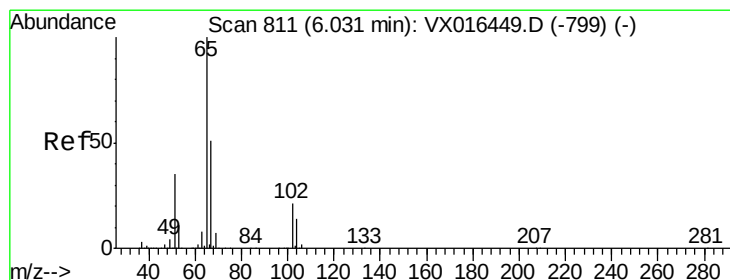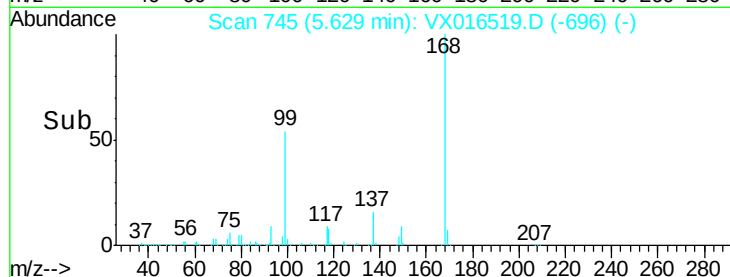

#33

1,2-Dichloroethane-d4

Concen: 45.982 ug/l

RT: 6.03 min Scan# 811

Delta R.T. -0.00 min

Lab File: VX016519.D


Acq: 01 Jun 2020 11:34

Tgt Ion: 65 Resp: 197967

Ion Ratio Lower Upper

65 100

67 52.4 0.0 104.8

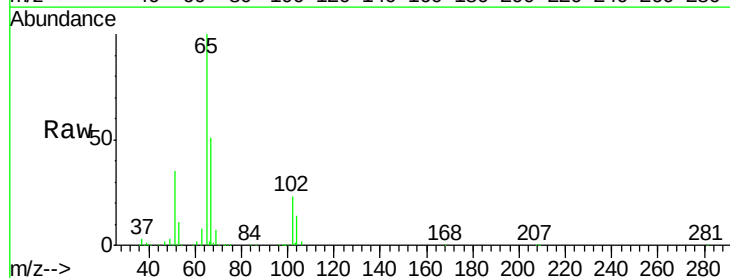

Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.03

80000


60000


40000

20000

0

Time-->

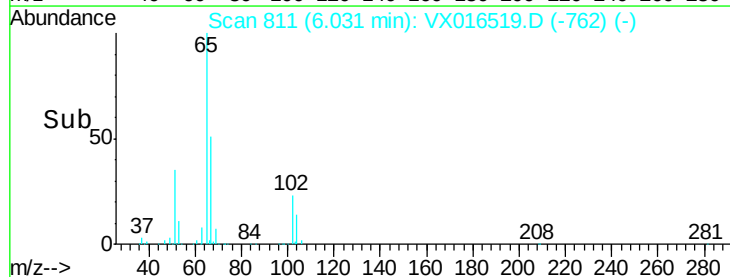

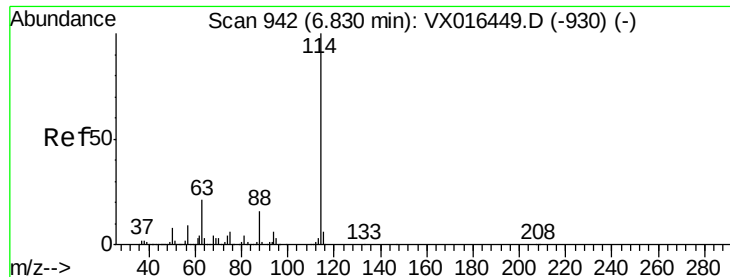

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.83 min Scan# 942

Delta R.T. -0.00 min

Lab File: VX016519.D

Acq: 01 Jun 2020 11:34

Instrument :

MSVOA_X

ClientSampleId :

Z2-TB7-200527


Tot Ion:114 Resp: 556499

Ion Ratio Lower Upper

114 100

63 20.4 0.0 42.6




88 16.0 0.0 32.8

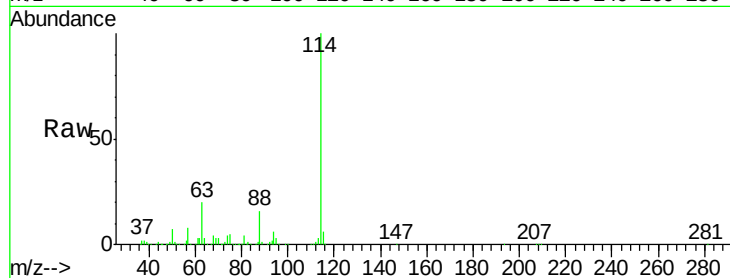

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

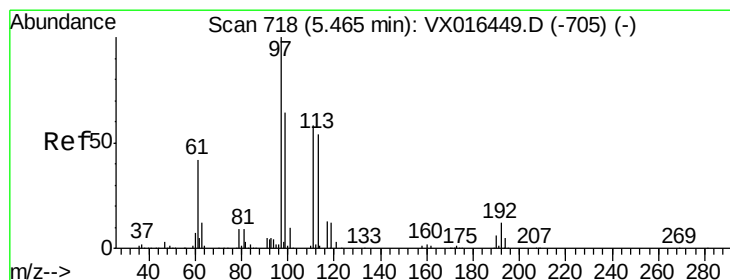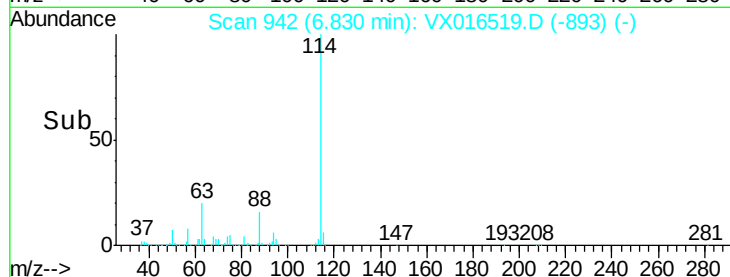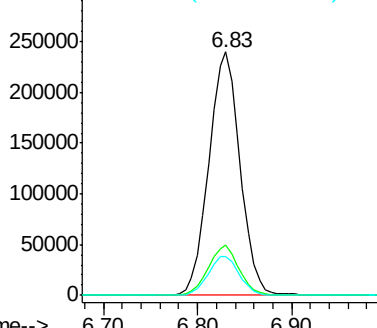

#35

Dibromofluoromethane

Concen: 46.250 ug/l

RT: 5.46 min Scan# 718

Delta R.T. -0.00 min

Lab File: VX016519.D

Acq: 01 Jun 2020 11:34


Tgt Ion:113 Resp: 158482

Ion Ratio Lower Upper

113 100

111 103.5 83.0 124.6



192 22.5 17.7 26.5

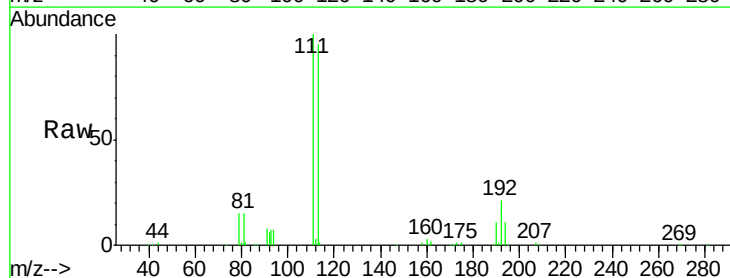


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V



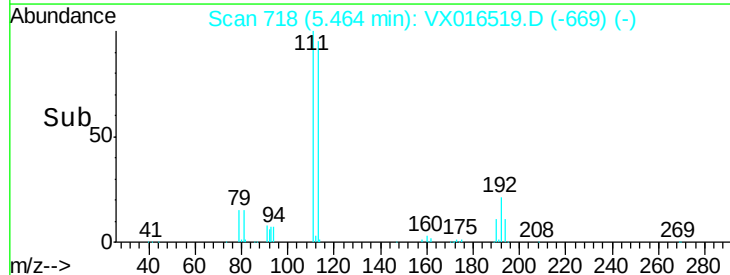
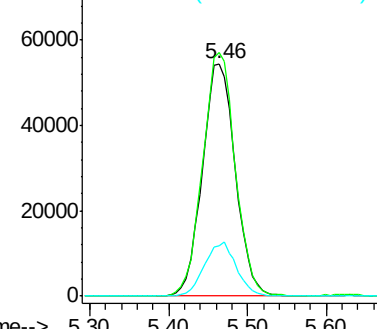


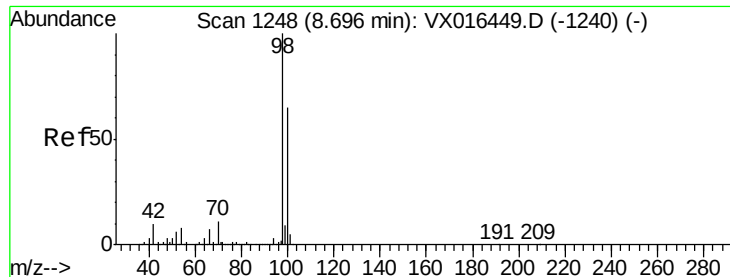

#50
Toluene-d8
Concen: 52.341 ug/l
RT: 8.70 min Scan# 1248
Delta R.T. -0.00 min
Lab File: VX016519.D
Acq: 01 Jun 2020 11:34




Instrument :
MSVOA_X
ClientSampleId :
Z2-TB7-200527


Tot Ion: 98 Resp: 698078
Ion Ratio Lower Upper
98 100
100 66.6 53.8 80.6

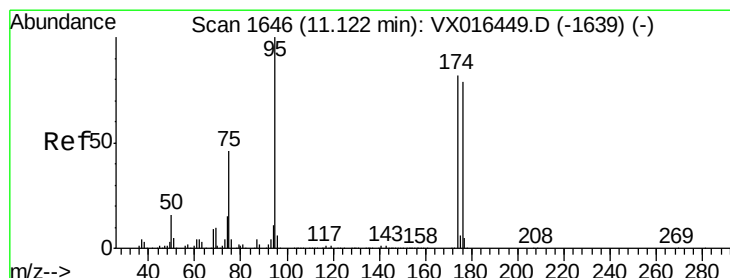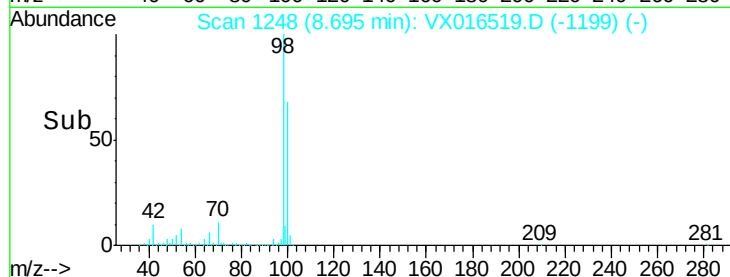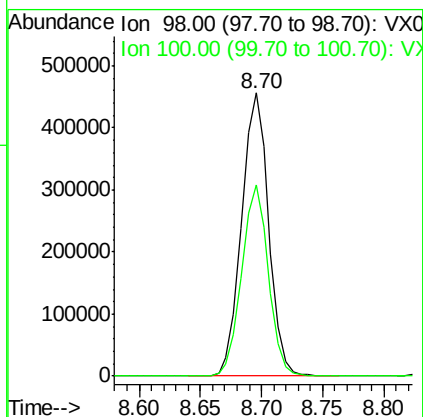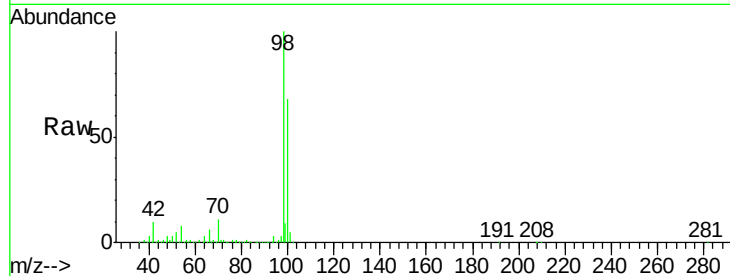

#62
4-Bromofluorobenzene
Concen: 55.198 ug/l
RT: 11.12 min Scan# 1646
Delta R.T. -0.00 min
Lab File: VX016519.D
Acq: 01 Jun 2020 11:34

Tgt Ion: 95 Resp: 284461
Ion Ratio Lower Upper
95 100
174 81.2 0.0 163.0
176 79.0 0.0 156.8


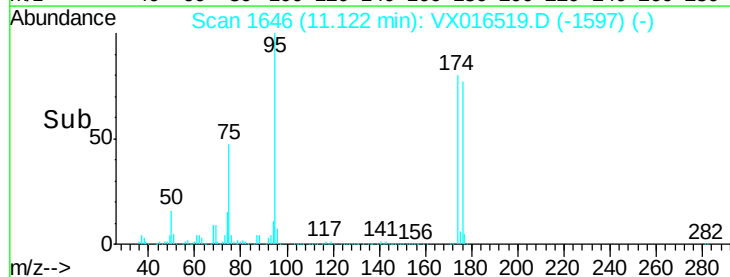
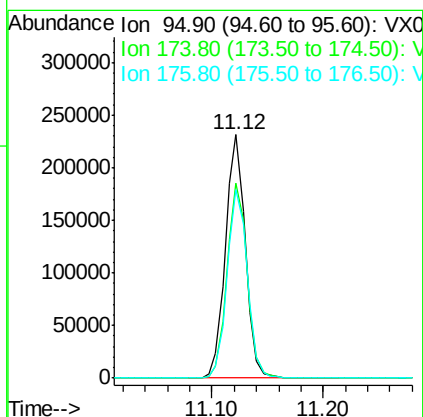
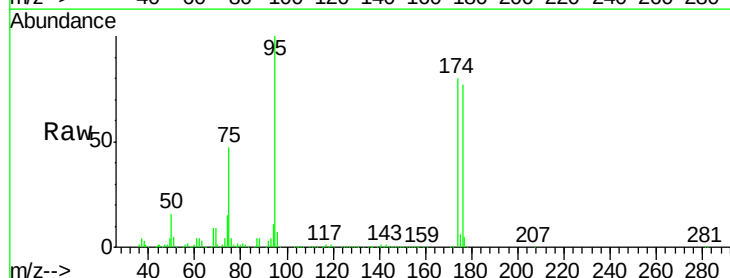


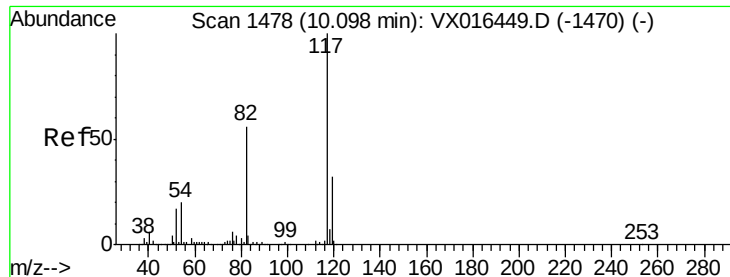

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.10 min Scan# 1478
Delta R.T. -0.00 min
Lab File: VX016519.D
Acq: 01 Jun 2020 11:34

Instrument :
MSVOA_X
ClientSampled :
Z2-TB7-200527

Tot Ion:117 Resp: 562794
Ion Ratio Lower Upper
117 100
82 54.8 45.0 67.6
119 31.8 25.8 38.8

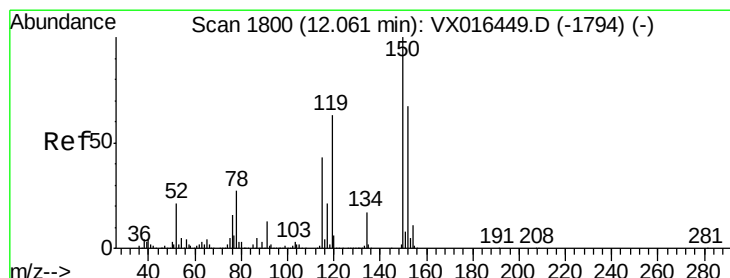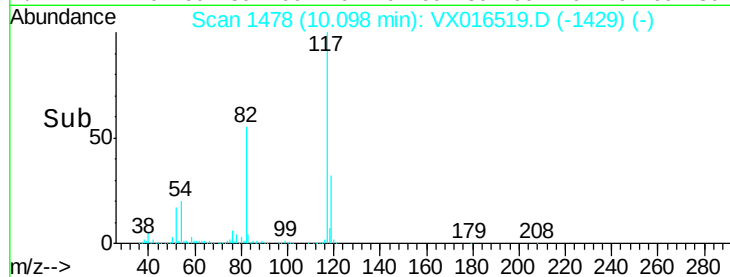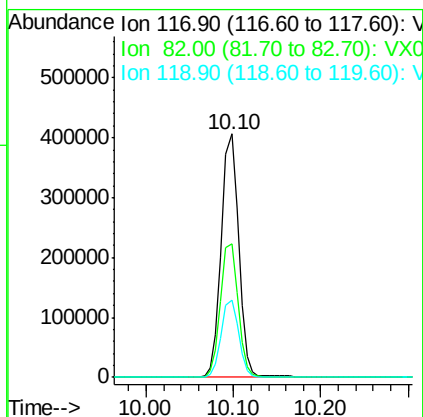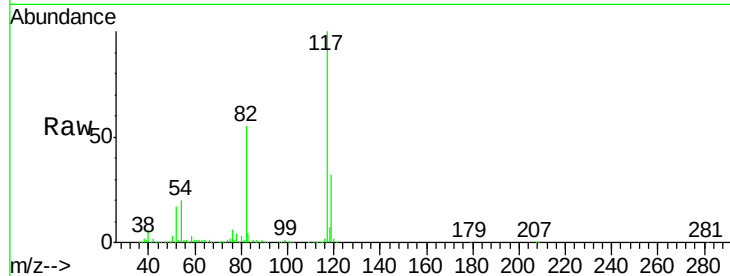

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.06 min Scan# 1800
Delta R.T. -0.00 min
Lab File: VX016519.D
Acq: 01 Jun 2020 11:34

Tgt Ion:152 Resp: 282618
Ion Ratio Lower Upper
152 100
115 59.1 39.9 119.6
150 155.7 0.0 341.0

