

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060121\
 Data File : VX022288.D
 Acq On : 01 Jun 2021 13:27
 Operator : JC/MD
 Sample : VX0601WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0601WBL01

Quant Time: Jun 01 16:07:12 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
 Quant Title : SW846 8260
 QLast Update : Wed May 19 14:23:10 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.568	168	70068	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	147183	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	128665	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	49035	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	58901	54.50	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	109.00%
35) Dibromofluoromethane	5.397	113	45786	49.05	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	98.10%
50) Toluene-d8	8.653	98	180535	50.21	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	100.42%
62) 4-Bromofluorobenzene	11.085	95	62342	46.91	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	93.82%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060121\
Data File : VX022288.D
Acq On : 01 Jun 2021 13:27
Operator : JC/MD
Sample : VX0601WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0601WBL01

Quant Time: Jun 01 16:07:12 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
Quant Title : SW846 8260
QLast Update : Wed May 19 14:23:10 2021
Response via : Initial Calibration




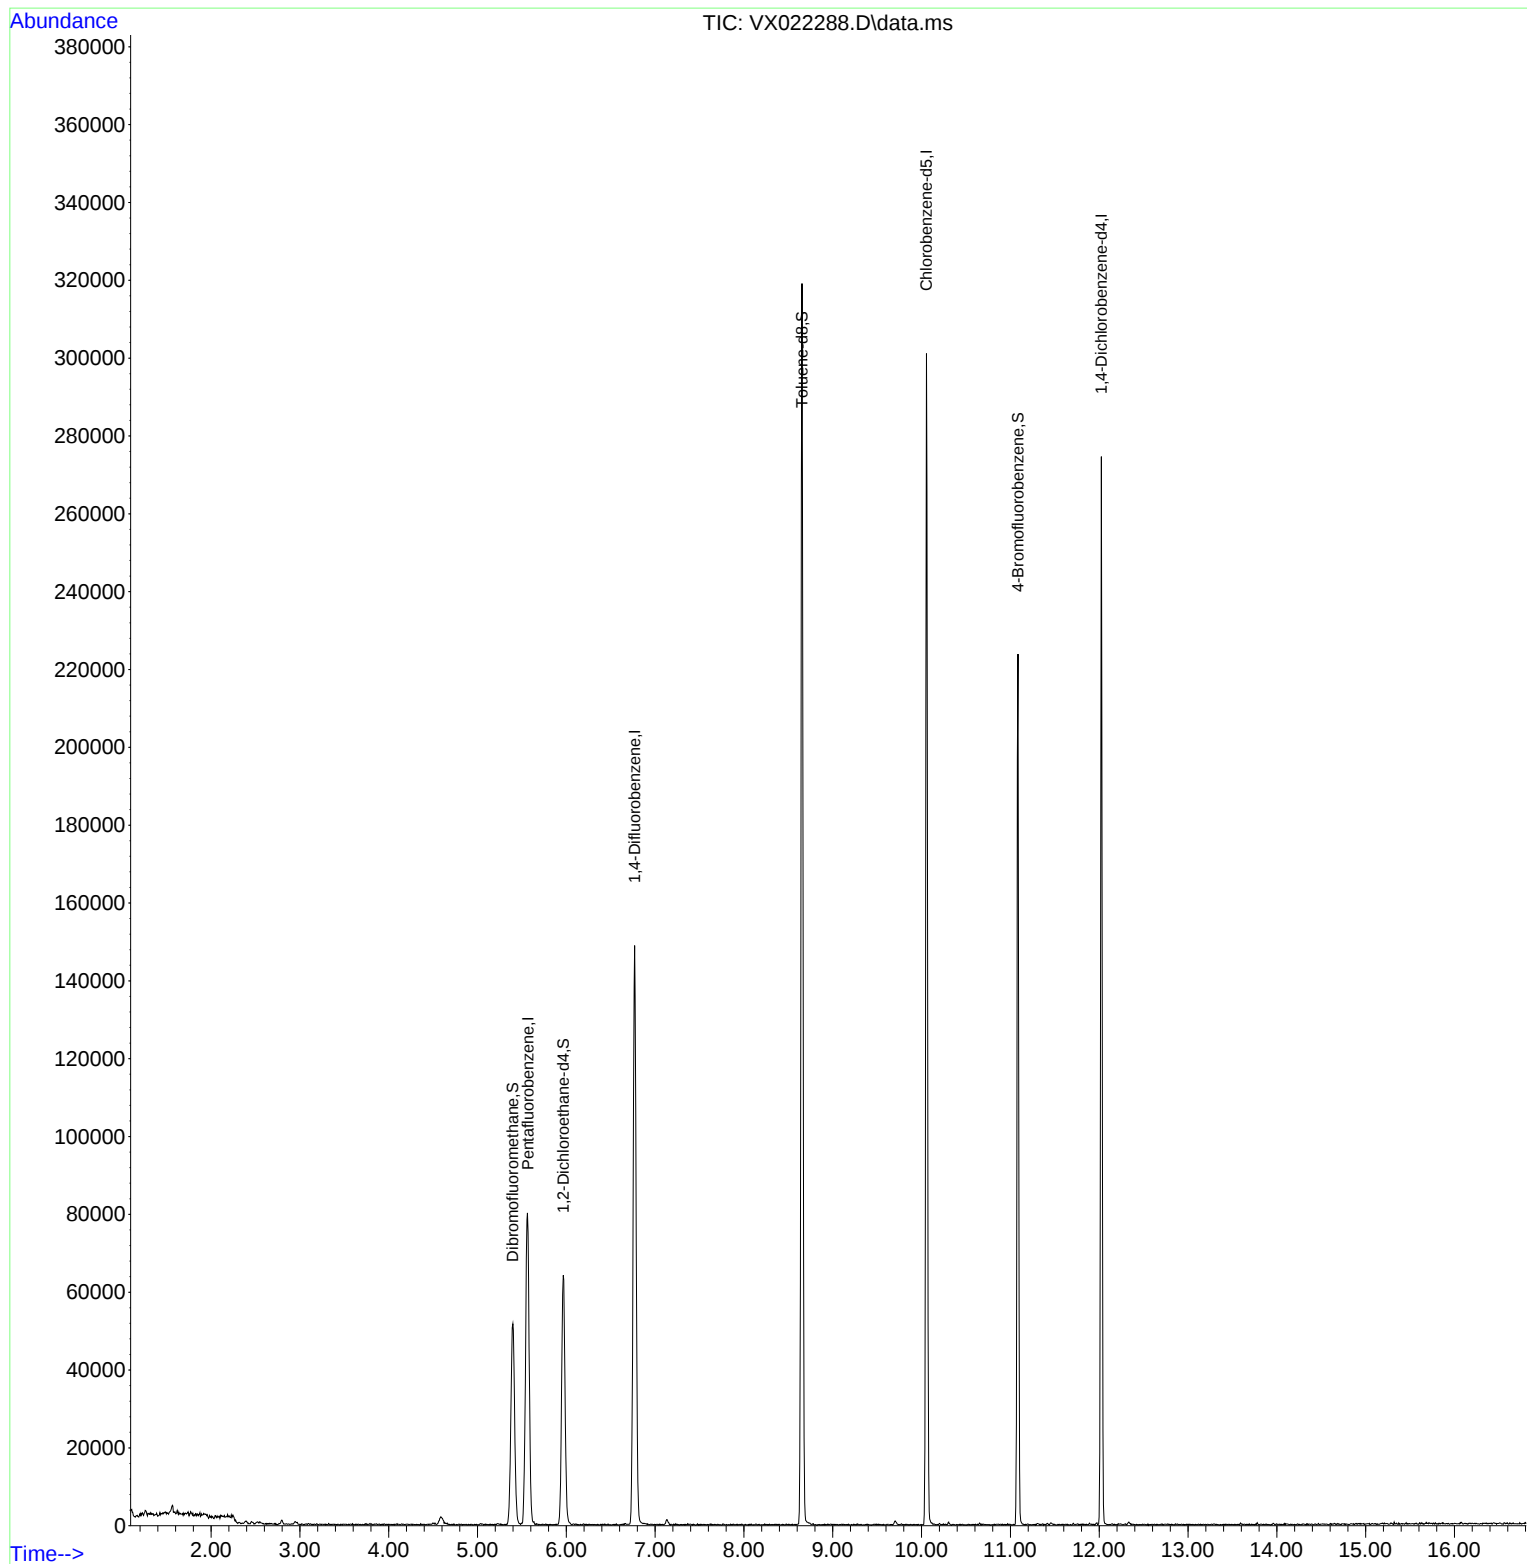


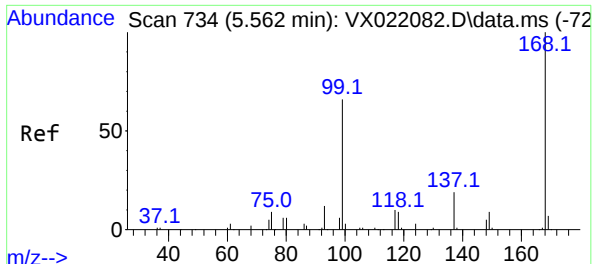

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.568 min Scan# 735
Delta R.T. 0.006 min
Lab File: VX022288.D
Acq: 01 Jun 2021 13:27




Instrument :
MSVOA_X
ClientSampleId :
VX0601WBL01


Tgt Ion:168 Resp: 70068
Ion Ratio Lower Upper
168 100
99 60.1 45.8 68.6

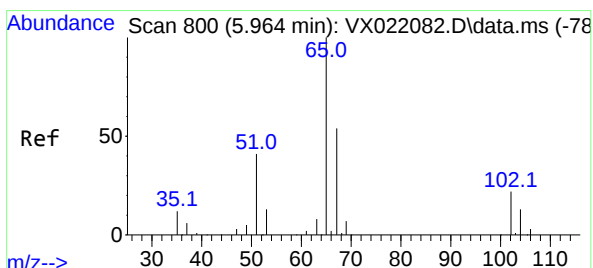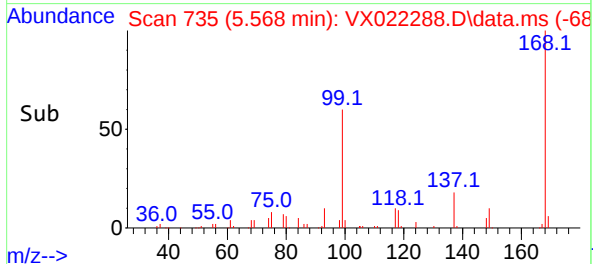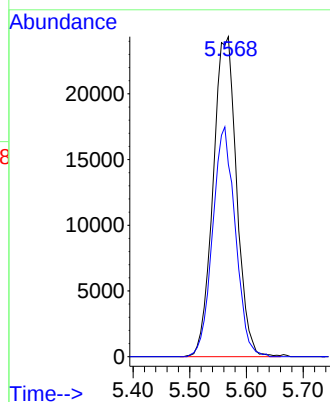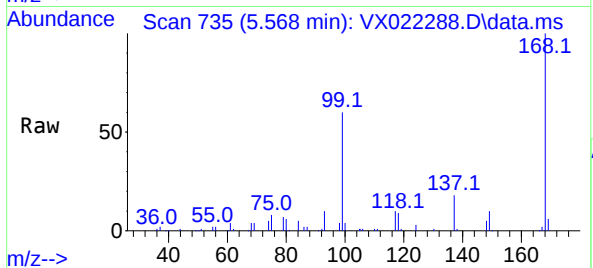

#33
1,2-Dichloroethane-d4
Concen: 54.50 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.000 min
Lab File: VX022288.D
Acq: 01 Jun 2021 13:27





Tgt Ion: 65 Resp: 58901
Ion Ratio Lower Upper
65 100
67 53.7 0.0 105.4

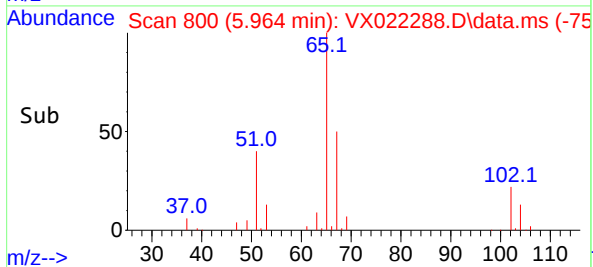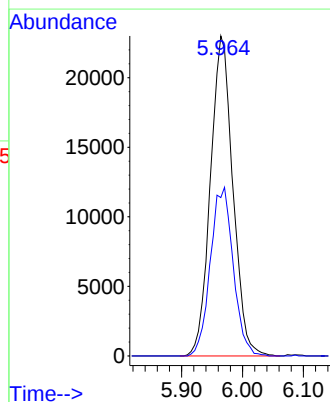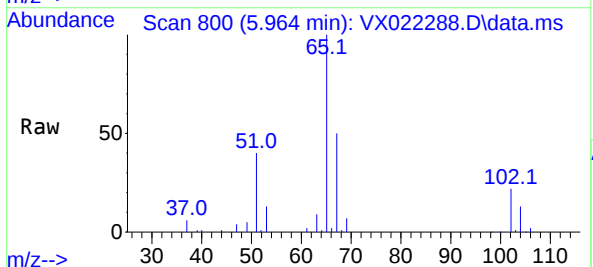

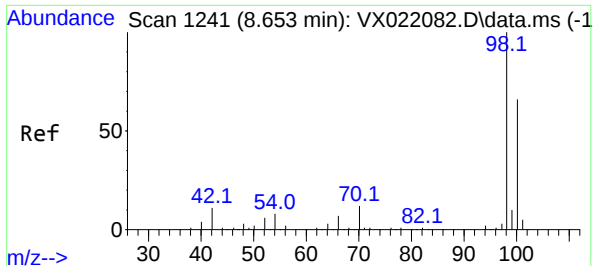




#50
Toluene-d8
Concen: 50.21 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX022288.D
Acq: 01 Jun 2021 13:27

Tgt Ion: 98 Resp: 180535
Ion Ratio Lower Upper
98 100
100 65.8 51.9 77.9

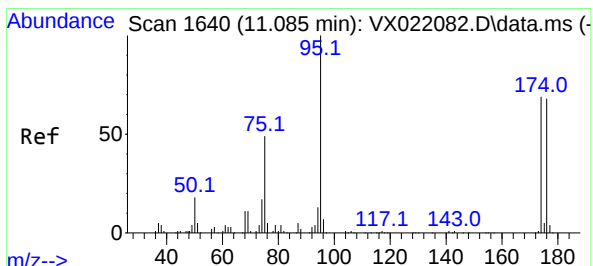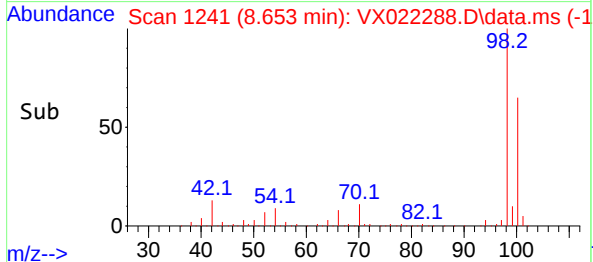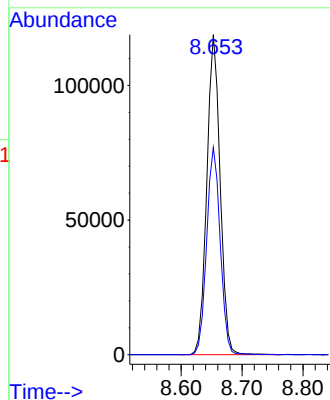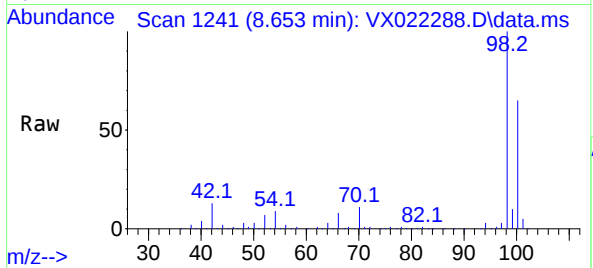


#62
4-Bromofluorobenzene
Concen: 46.91 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX022288.D
Acq: 01 Jun 2021 13:27

Tgt Ion: 95 Resp: 62342
Ion Ratio Lower Upper
95 100
174 61.8 0.0 154.6
176 59.9 0.0 155.8

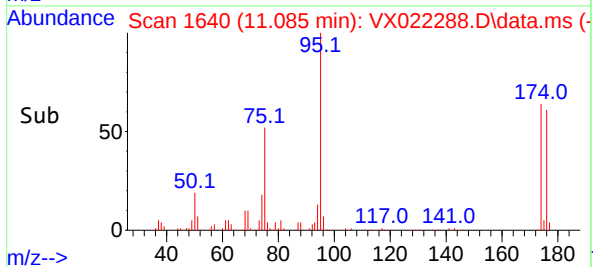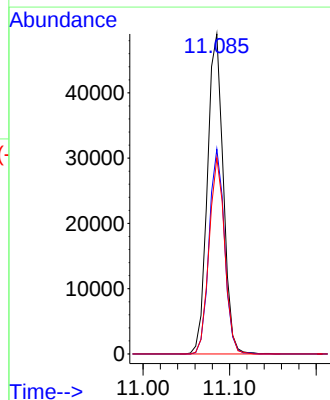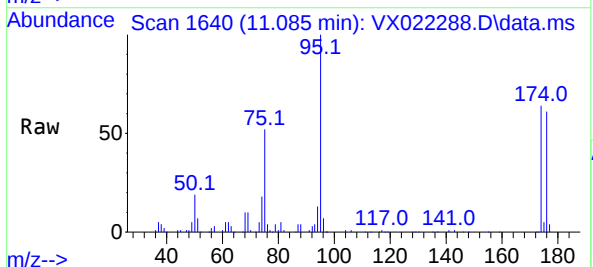





Instrument :
MSVOA_X
ClientSampleId :
VX0601WBL01

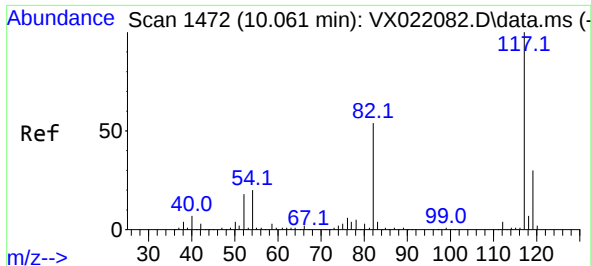

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.006 min
Lab File: VX022288.D
Acq: 01 Jun 2021 13:27

Instrument :
MSVOA_X
ClientSampleId :
VX0601WBL01

Tgt Ion:117 Resp: 128665
Ion Ratio Lower Upper
117 100
82 59.9 47.4 71.2
119 30.8 26.6 39.8

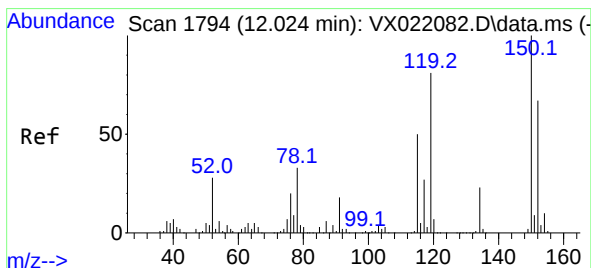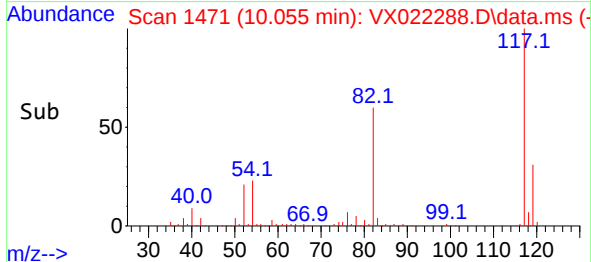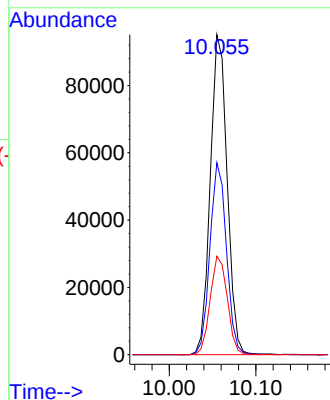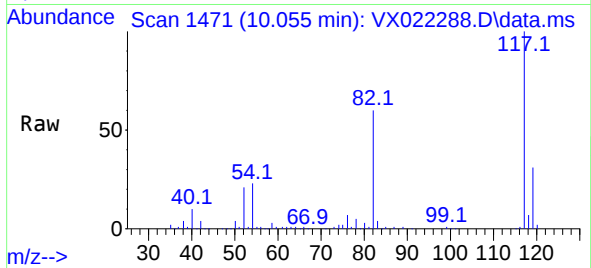

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX022288.D
Acq: 01 Jun 2021 13:27

Tgt Ion:152 Resp: 49035
Ion Ratio Lower Upper
152 100
115 65.9 41.1 123.3
150 159.2 0.0 349.0

