

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060121\
 Data File : VX022291.D
 Acq On : 01 Jun 2021 15:26
 Operator : JC/MD
 Sample : M2518-05 200X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 118-119

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M

Title : SW846 8260

Signal : TIC: VX022291.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.386	206	213	222	rBV	237529	370275	43.34%	7.394%
2	2.794	272	280	293	rBV	247094	446517	52.26%	8.916%
3	3.867	449	456	467	rBV2	8759	22680	2.65%	0.453%
4	4.586	563	574	589	rBV3	4356	14552	1.70%	0.291%
5	5.397	695	707	720	rBV	52434	147497	17.26%	2.945%
6	5.562	723	734	746	rVV	77686	226111	26.47%	4.515%
7	5.842	772	780	790	rBV2	5401	13461	1.58%	0.269%
8	5.964	790	800	812	rBV	63445	169429	19.83%	3.383%
9	6.769	923	932	945	rBV	146592	343910	40.25%	6.867%
10	8.653	1234	1241	1248	rBV	311858	481706	56.38%	9.619%
11	8.720	1248	1252	1259	rVB	5774	9384	1.10%	0.187%
12	9.275	1337	1343	1353	rBV	219333	332207	38.88%	6.633%
13	10.055	1465	1471	1481	rBV	295002	395152	46.25%	7.890%
14	10.195	1488	1494	1506	rBV	152266	192995	22.59%	3.854%
15	10.305	1506	1512	1524	rVB	638884	854350	100.00%	17.059%
16	10.646	1562	1568	1573	rBV	294632	370275	43.34%	7.394%
17	11.085	1634	1640	1650	rBV	215835	275277	32.22%	5.497%
18	11.756	1746	1750	1754	rVB	7623	8934	1.05%	0.178%
19	12.024	1789	1794	1801	rBV	267127	324702	38.01%	6.484%
20	13.292	1991	2002	2006	rBV5	5212	8690	1.02%	0.174%




Sum of corrected areas: 5008104

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060121\
Data File : VX022291.D
Acq On : 01 Jun 2021 15:26
Operator : JC/MD
Sample : M2518-05 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
118-119

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

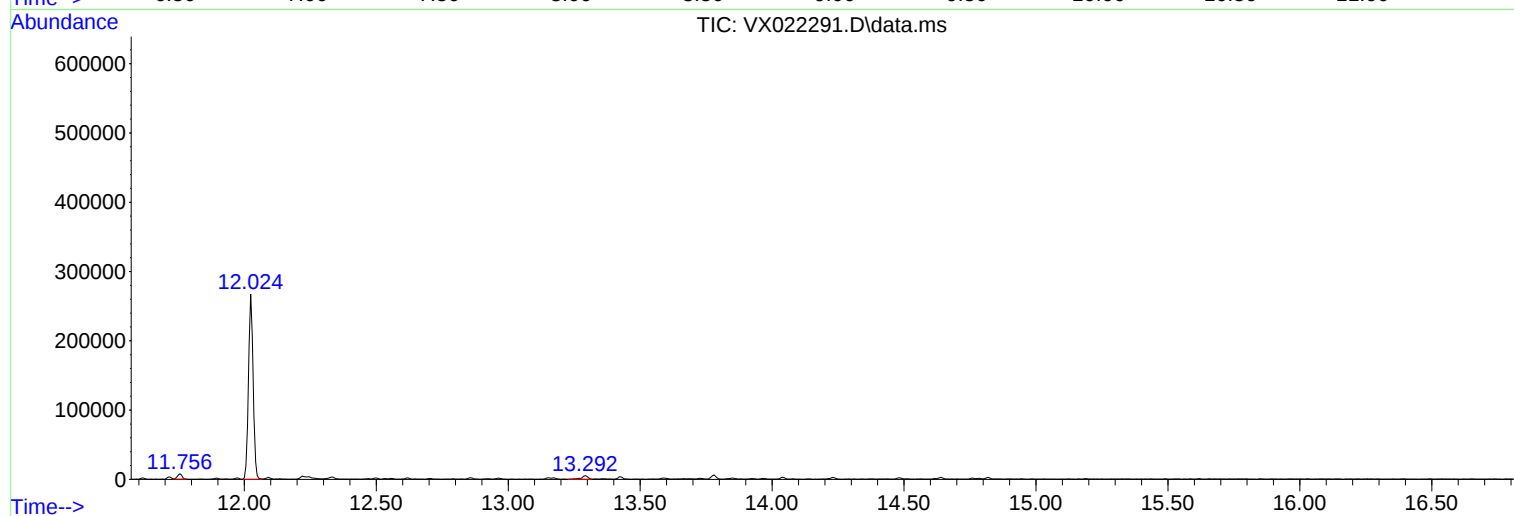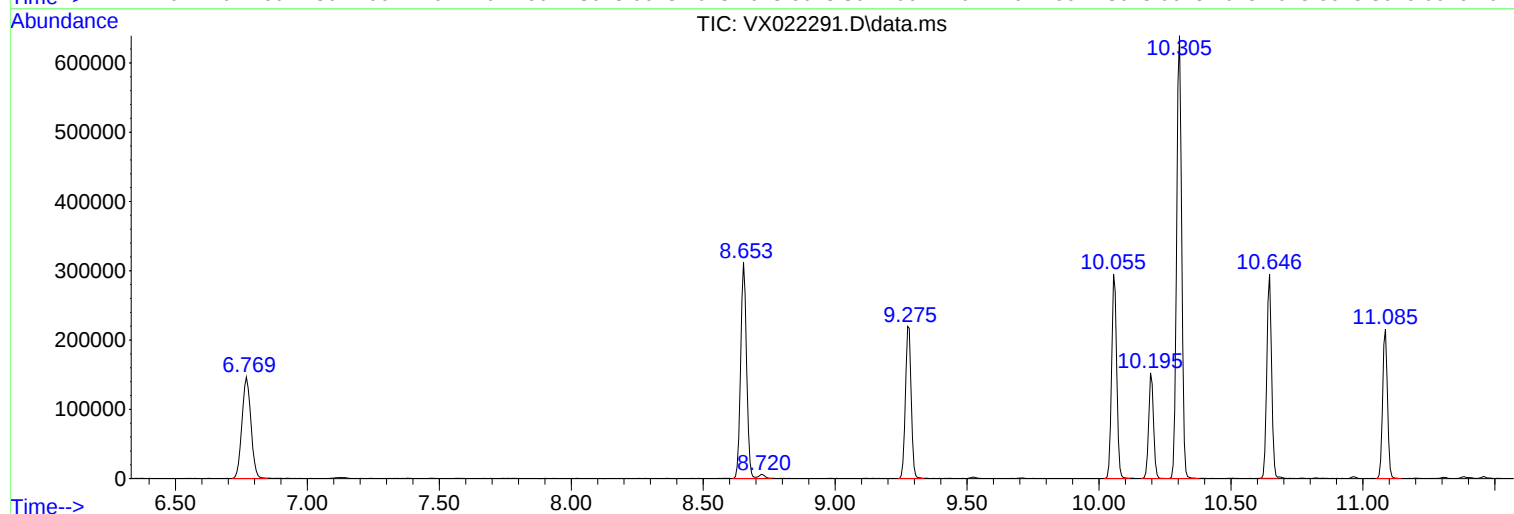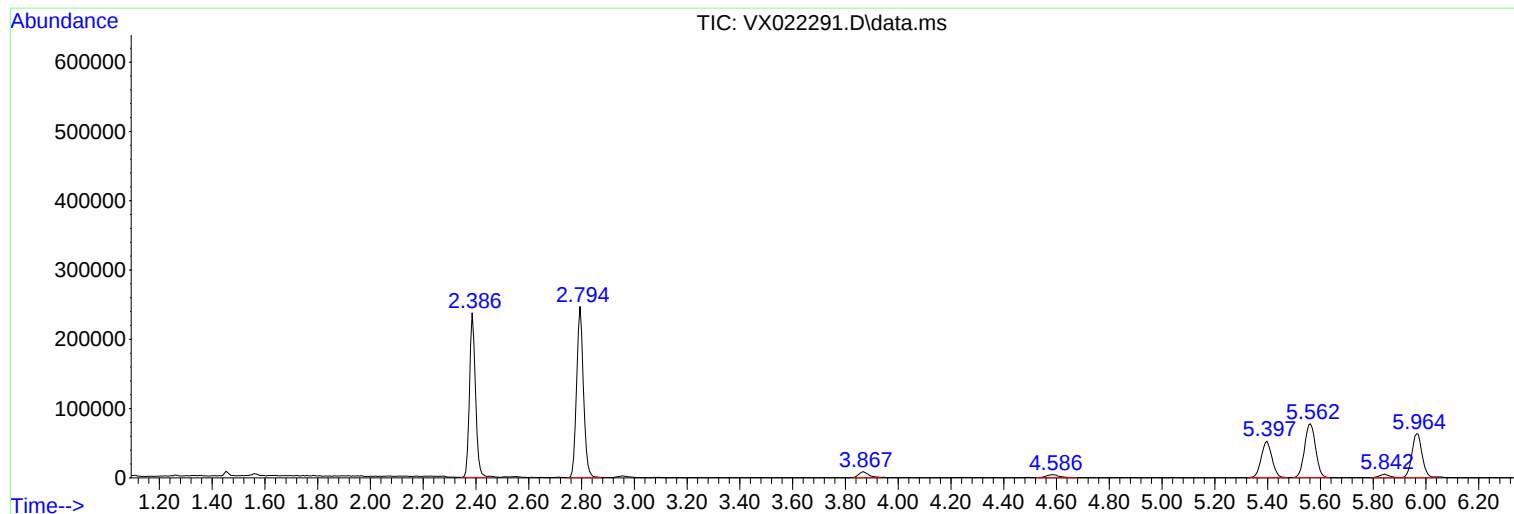

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060121\
Data File : VX022291.D
Acq On : 01 Jun 2021 15:26
Operator : JC/MD
Sample : M2518-05 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampled :
118-119










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 1-Propanol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.867	5.02 ug/l	22680	Pentafluorobenzene	5.562

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	1-Propanol			60	C3H8O	000071-23-8	59
2	2-Fluoropropene			60	C3H5F	001184-60-7	52
3	Allyl fluoride			60	C3H5F	000818-92-8	32
4	(3,3-Dimethyloxiranyl)methanol			102	C5H10O2	1000306-71-7	9
5	Acetaldoxime			59	C2H5NO	000107-29-9	7

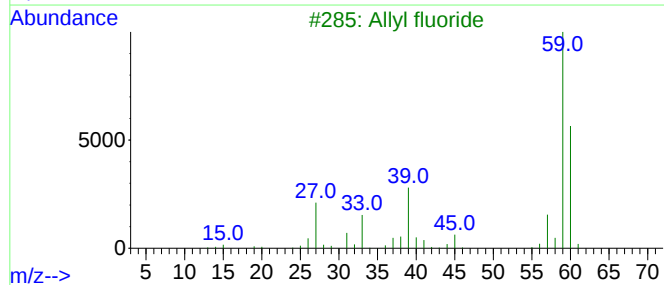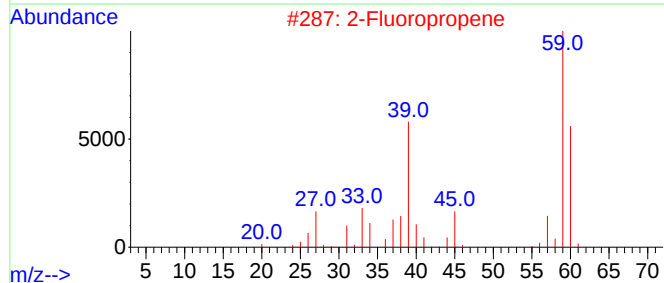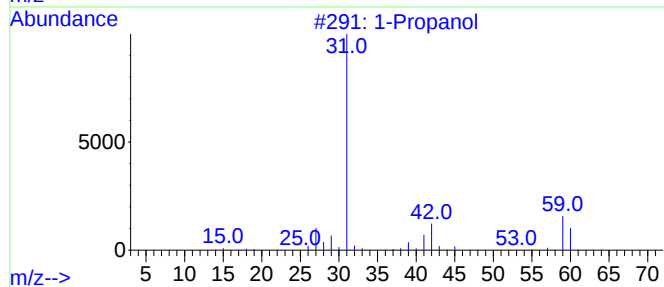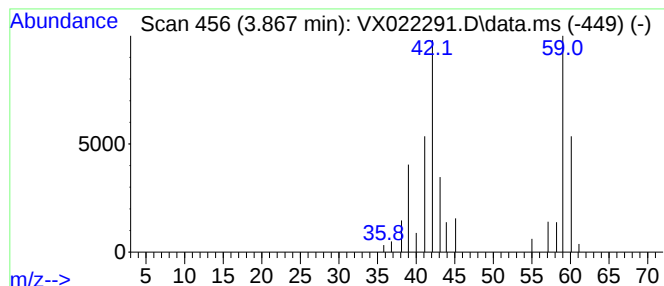

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060121\
Data File : VX022291.D
Acq On : 01 Jun 2021 15:26
Operator : JC/MD
Sample : M2518-05 200X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
118-119

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1-Propanol	3.867	5.0	ug/l	22680	1	5.562	226111	50.0