

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060121\
 Data File : VX022319.D
 Acq On : 02 Jun 2021 03:11
 Operator : JC/MD
 Sample : M2572-03 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 56BR-20210528

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M

Title : SW846 8260

Signal : TIC: VX022319.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	51	rVB	9006	8951	1.04%	0.245%
2	4.495	548	559	572	rBV	119490	331817	38.63%	9.079%
3	5.397	695	707	722	rVB	52069	150429	17.51%	4.116%
4	5.562	722	734	747	rBV2	81237	230406	26.82%	6.304%
5	5.964	789	800	814	rBV2	66570	173025	20.14%	4.734%
6	6.769	923	932	945	rBV2	151065	354924	41.32%	9.711%
7	7.129	979	991	1003	rBV	400684	858942	100.00%	23.502%
8	8.653	1234	1241	1252	rBV	321895	499628	58.17%	13.671%
9	10.055	1465	1471	1482	rBV	304590	414238	48.23%	11.334%
10	11.085	1634	1640	1649	rVB	227245	288653	33.61%	7.898%
11	12.024	1789	1794	1803	rVB	279808	343675	40.01%	9.404%




Sum of corrected areas: 3654688

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060121\
Data File : VX022319.D
Acq On : 02 Jun 2021 03:11
Operator : JC/MD
Sample : M2572-03 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
56BR-20210528

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

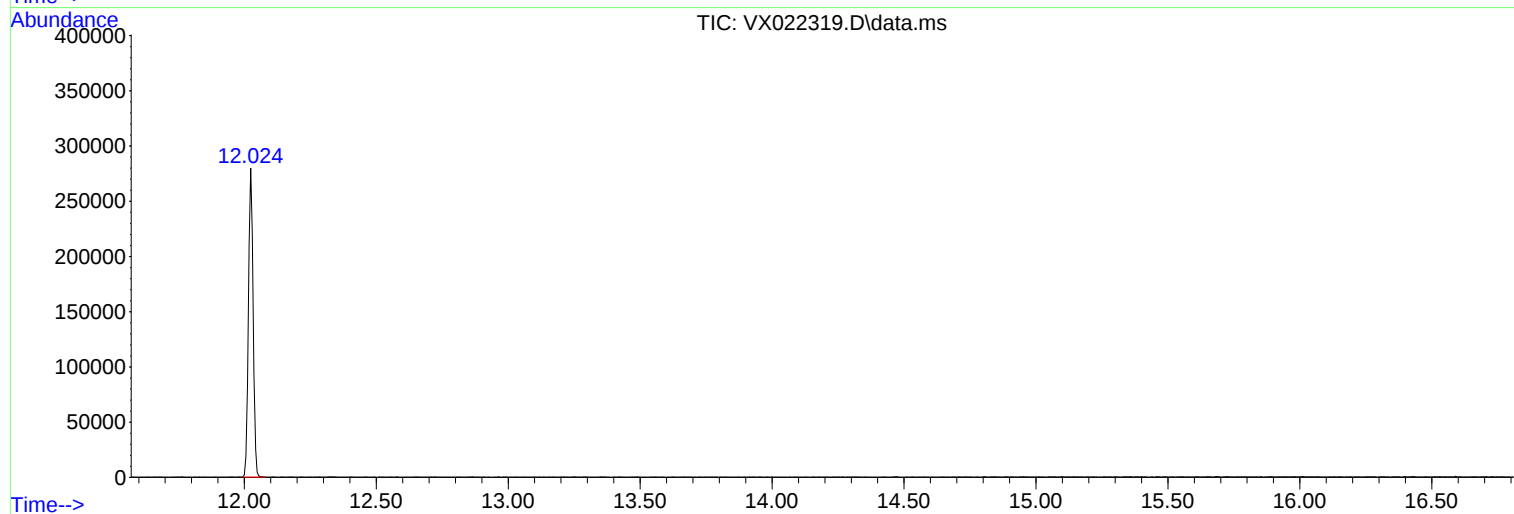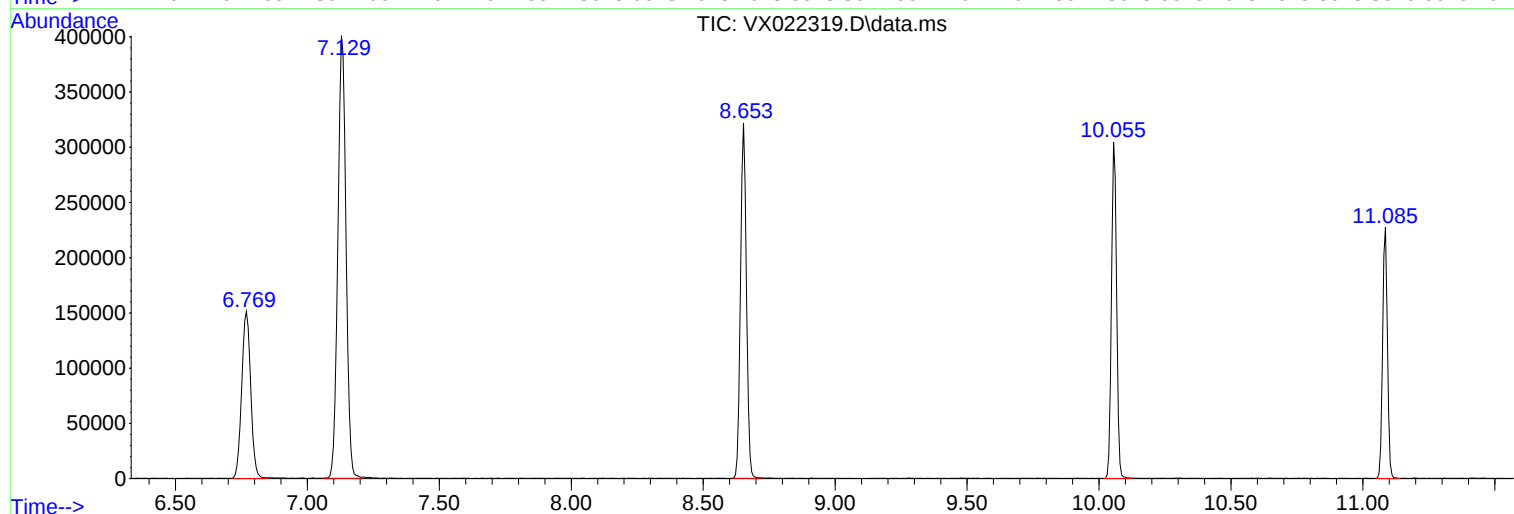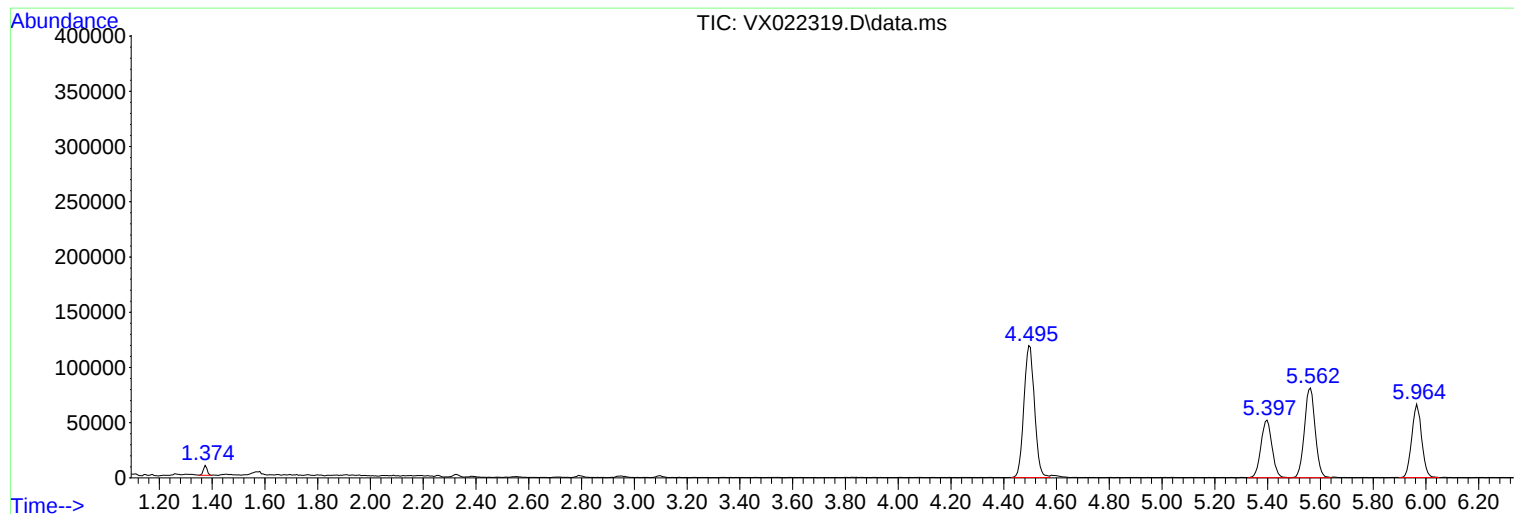

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060121\
Data File : VX022319.D
Acq On : 02 Jun 2021 03:11
Operator : JC/MD
Sample : M2572-03 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
56BR-20210528

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060121\
Data File : VX022319.D
Acq On : 02 Jun 2021 03:11
Operator : JC/MD
Sample : M2572-03 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
56BR-20210528

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
