

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060121\
 Data File : VX022320.D
 Acq On : 02 Jun 2021 03:34
 Operator : JC/MD
 Sample : M2572-04 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 15BR-20210528

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M

Title : SW846 8260

Signal : TIC: VX022320.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	44	47	51	rBV	14159	14046	1.41%	0.367%
2	4.495	548	559	572	rBV	247354	662258	66.40%	17.284%
3	5.397	695	707	722	rBV	46528	134930	13.53%	3.521%
4	5.562	722	734	747	rVB2	73020	205716	20.63%	5.369%
5	5.964	790	800	817	rVB	58217	153106	15.35%	3.996%
6	6.769	922	932	943	rBV	131099	317653	31.85%	8.290%
7	7.129	982	991	1005	rBV	461384	997325	100.00%	26.029%
8	8.653	1233	1241	1251	rBV	288340	449223	45.04%	11.724%
9	10.055	1465	1471	1480	rBV	270593	360967	36.19%	9.421%
10	11.085	1634	1640	1649	rBV	195348	250486	25.12%	6.537%
11	12.024	1789	1794	1803	rVB	235102	285947	28.67%	7.463%




Sum of corrected areas: 3831657

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060121\
Data File : VX022320.D
Acq On : 02 Jun 2021 03:34
Operator : JC/MD
Sample : M2572-04 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
15BR-20210528

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

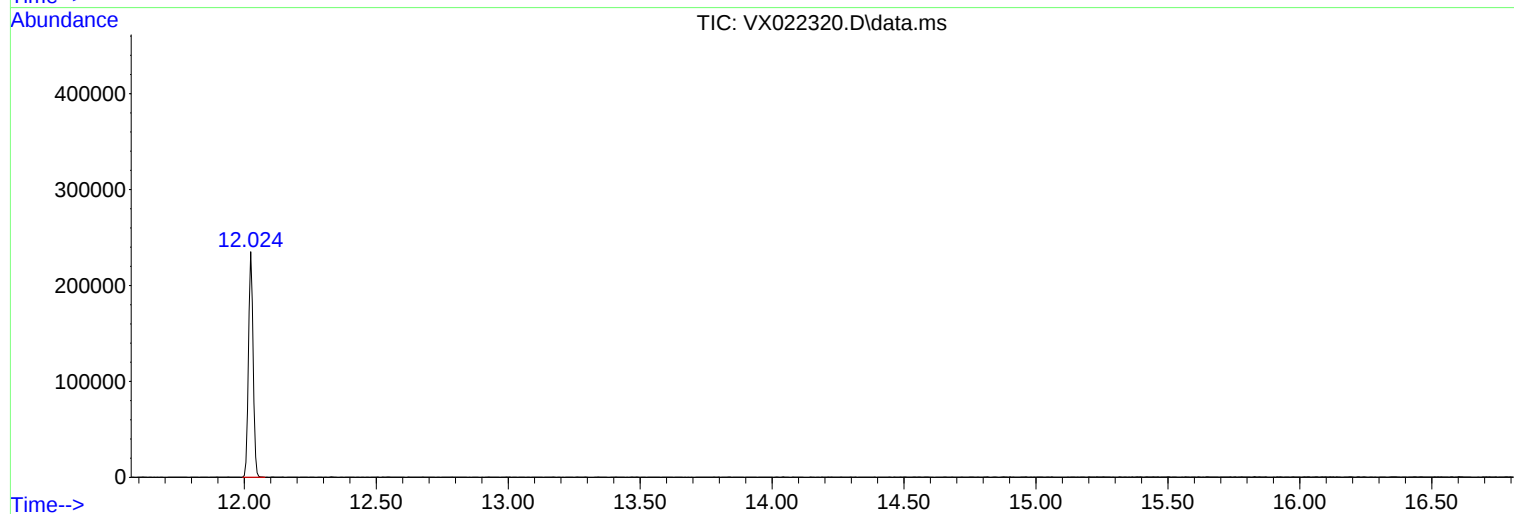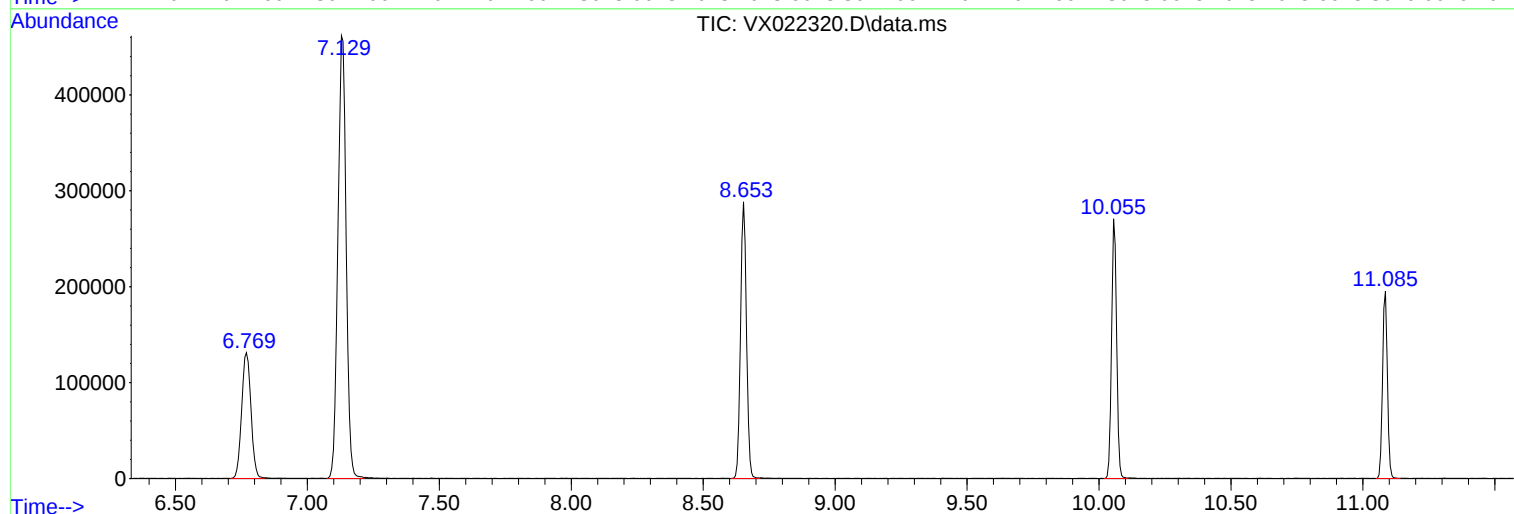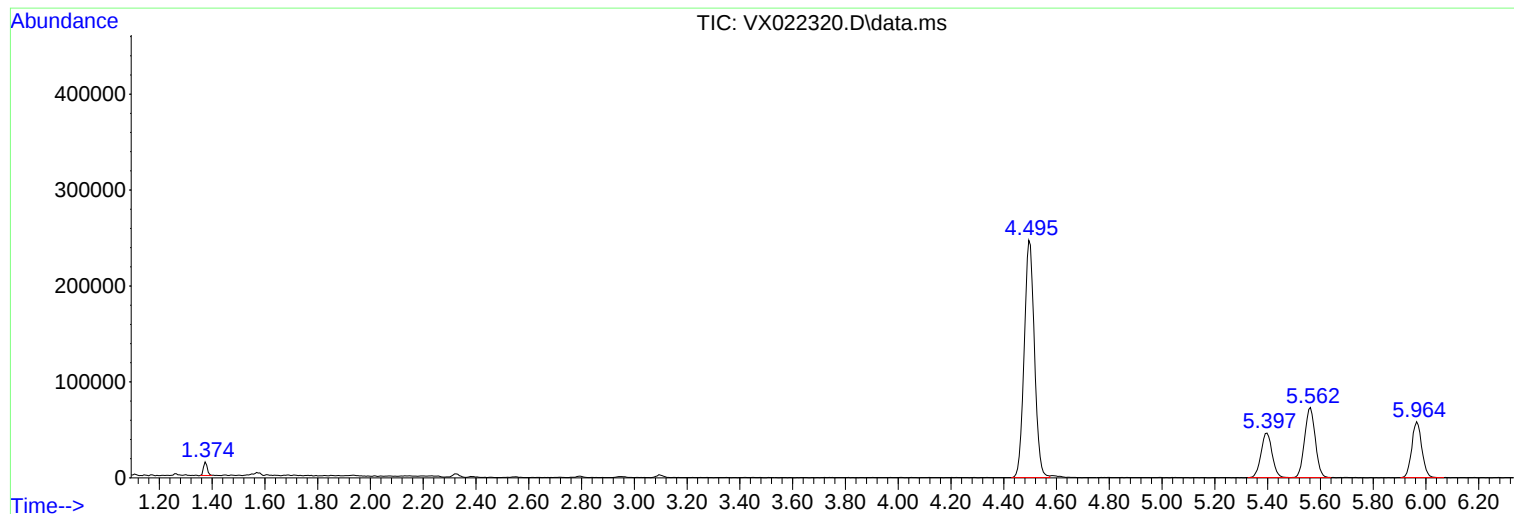

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060121\
Data File : VX022320.D
Acq On : 02 Jun 2021 03:34
Operator : JC/MD
Sample : M2572-04 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
15BR-20210528

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060121\
Data File : VX022320.D
Acq On : 02 Jun 2021 03:34
Operator : JC/MD
Sample : M2572-04 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
15BR-20210528

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
