

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060121\
 Data File : VX022323.D
 Acq On : 02 Jun 2021 04:45
 Operator : JC/MD
 Sample : M2572-11 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DUP02-20210528

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M

Title : SW846 8260

Signal : TIC: VX022323.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	44	47	51	rVB	8433	8221	1.17%	0.255%
2	4.495	548	559	571	rBV	105857	285540	40.76%	8.869%
3	5.391	695	706	719	rBV	46943	135028	19.27%	4.194%
4	5.562	722	734	747	rVB2	72906	207209	29.58%	6.436%
5	5.964	789	800	813	rBV	60281	157835	22.53%	4.902%
6	6.769	922	932	943	rBV	137440	322706	46.06%	10.023%
7	7.129	981	991	1010	rBV	323152	700567	100.00%	21.759%
8	8.653	1234	1241	1252	rBV	291974	456809	65.21%	14.188%
9	10.055	1466	1471	1479	rBV	281315	378039	53.96%	11.741%
10	11.085	1634	1640	1650	rBV	208929	262746	37.50%	8.161%
11	12.024	1789	1794	1802	rBV	251728	305004	43.54%	9.473%




Sum of corrected areas: 3219704

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060121\
Data File : VX022323.D
Acq On : 02 Jun 2021 04:45
Operator : JC/MD
Sample : M2572-11 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP02-20210528

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

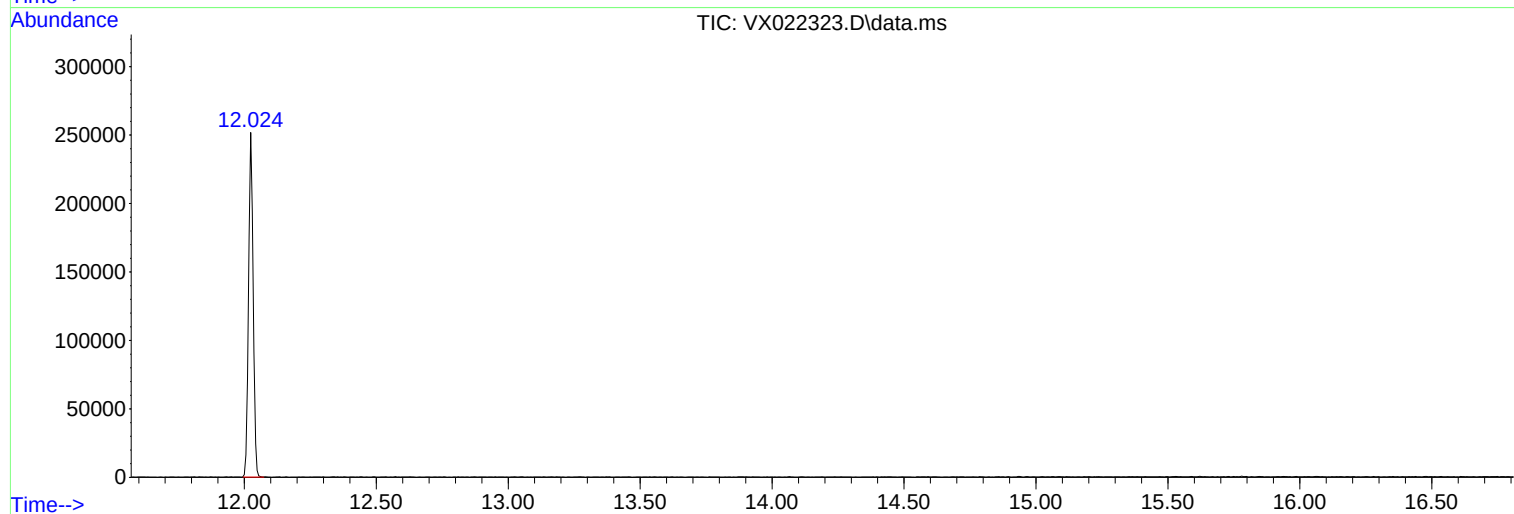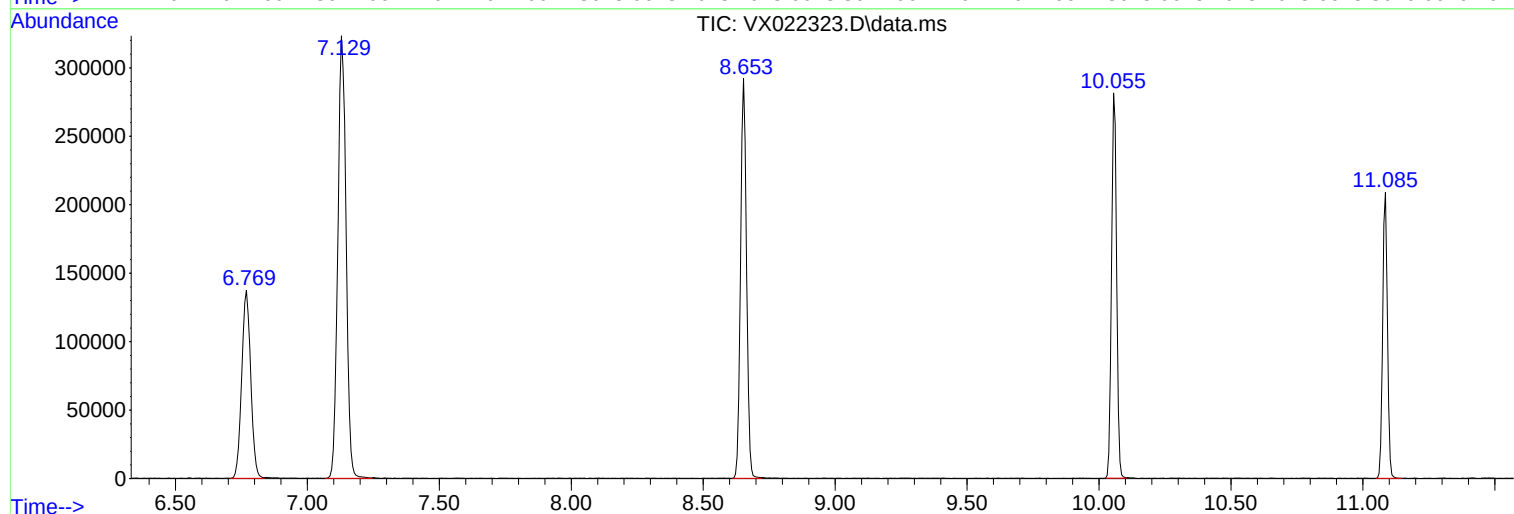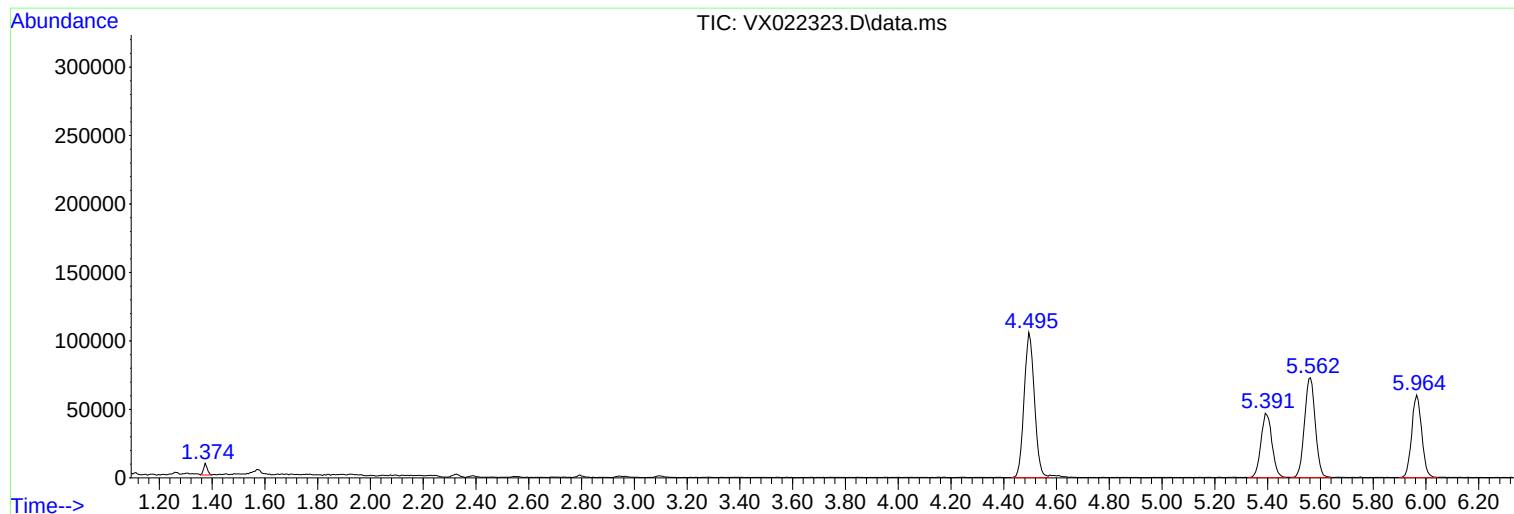

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060121\
Data File : VX022323.D
Acq On : 02 Jun 2021 04:45
Operator : JC/MD
Sample : M2572-11 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP02-20210528

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060121\
Data File : VX022323.D
Acq On : 02 Jun 2021 04:45
Operator : JC/MD
Sample : M2572-11 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP02-20210528

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------