
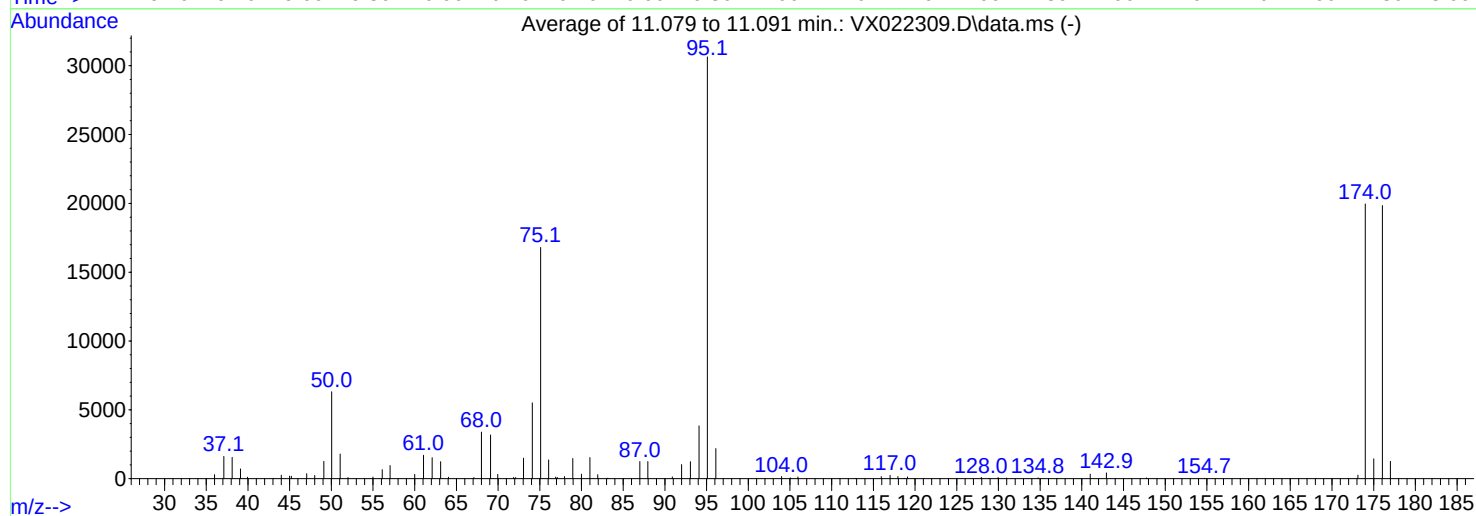


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060121\
 Data File : VX022309.D
 Acq On : 01 Jun 2021 22:52
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
 Title : SW846 8260
 Last Update : Wed May 19 14:23:10 2021

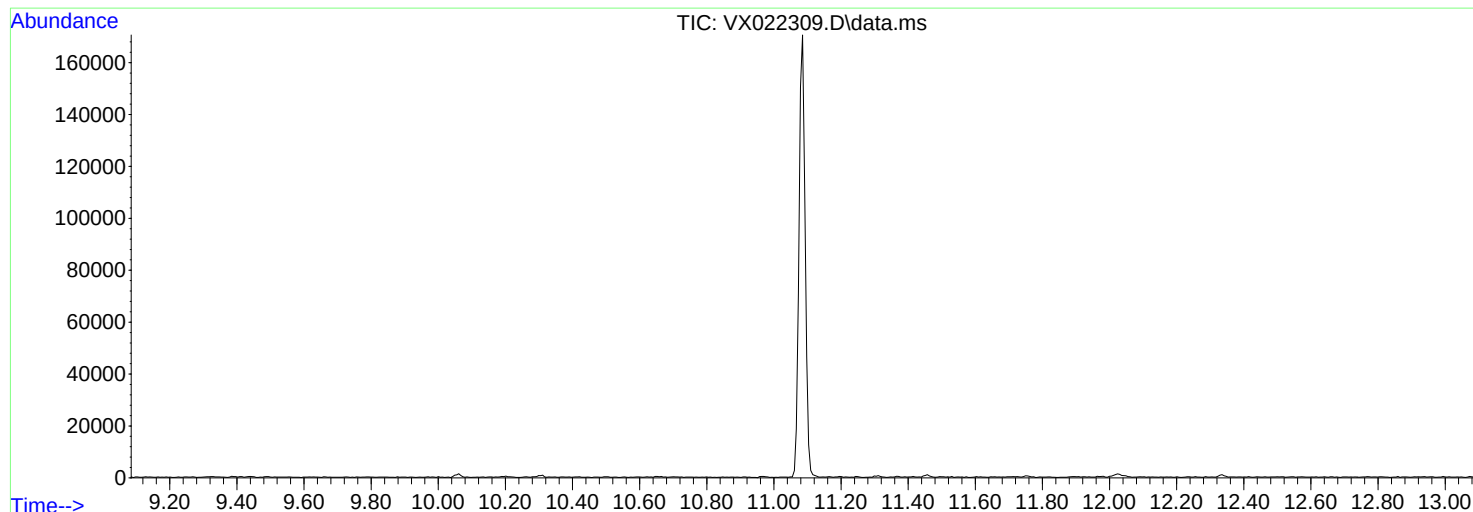

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.6	6308	PASS
75	95	30	60	54.8	16803	PASS
95	95	100	100	100.0	30645	PASS
96	95	5	9	7.1	2187	PASS
173	174	0.00	2	1.3	260	PASS
174	95	50	100	65.1	19965	PASS
175	174	5	9	7.2	1445	PASS
176	174	95	101	99.4	19848	PASS
177	176	5	9	6.3	1255	PASS