

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060122\
Data File : VX029114.D
Acq On : 01 Jun 2022 13:37
Operator : JC/MD
Sample : N3022-16
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RB06-20220525

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M

Title : SW846 8260

Signal : TIC: VX029114.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.258	21	28	38	rBV	10593	22929	1.36%	0.246%
2	2.380	205	212	221	rBV	19987	32331	1.92%	0.348%
3	2.538	230	238	249	rBV	20386	41035	2.44%	0.441%
4	5.391	690	706	721	rBV	211736	616129	36.56%	6.623%
5	5.556	721	733	746	rVV	327063	917073	54.42%	9.858%
6	5.958	787	799	816	rBV	198018	525723	31.20%	5.651%
7	6.763	921	931	948	rBV	514765	1229533	72.96%	13.217%
8	8.653	1234	1241	1249	rBV	1089254	1685151	100.00%	18.114%
9	10.055	1465	1471	1485	rBV	1158448	1532205	90.92%	16.470%
10	11.085	1634	1640	1656	rBV	919831	1196815	71.02%	12.865%
11	12.024	1789	1794	1801	rBV	1253761	1504049	89.25%	16.167%




Sum of corrected areas: 9302973

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060122\
Data File : VX029114.D
Acq On : 01 Jun 2022 13:37
Operator : JC/MD
Sample : N3022-16
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RB06-20220525

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

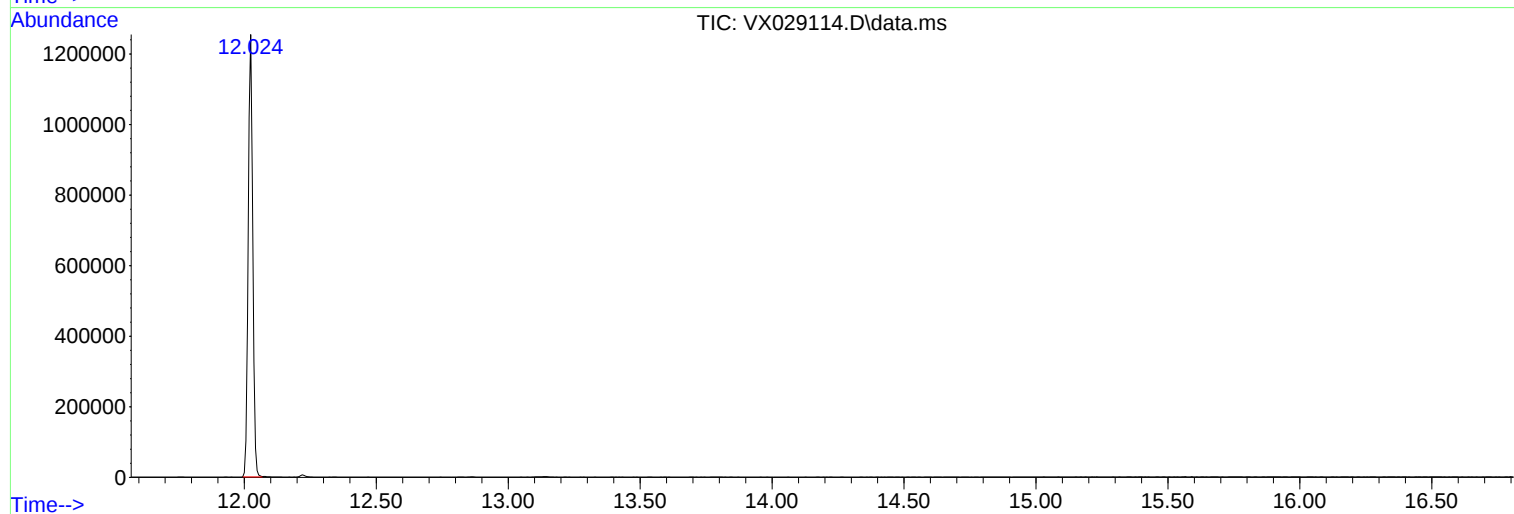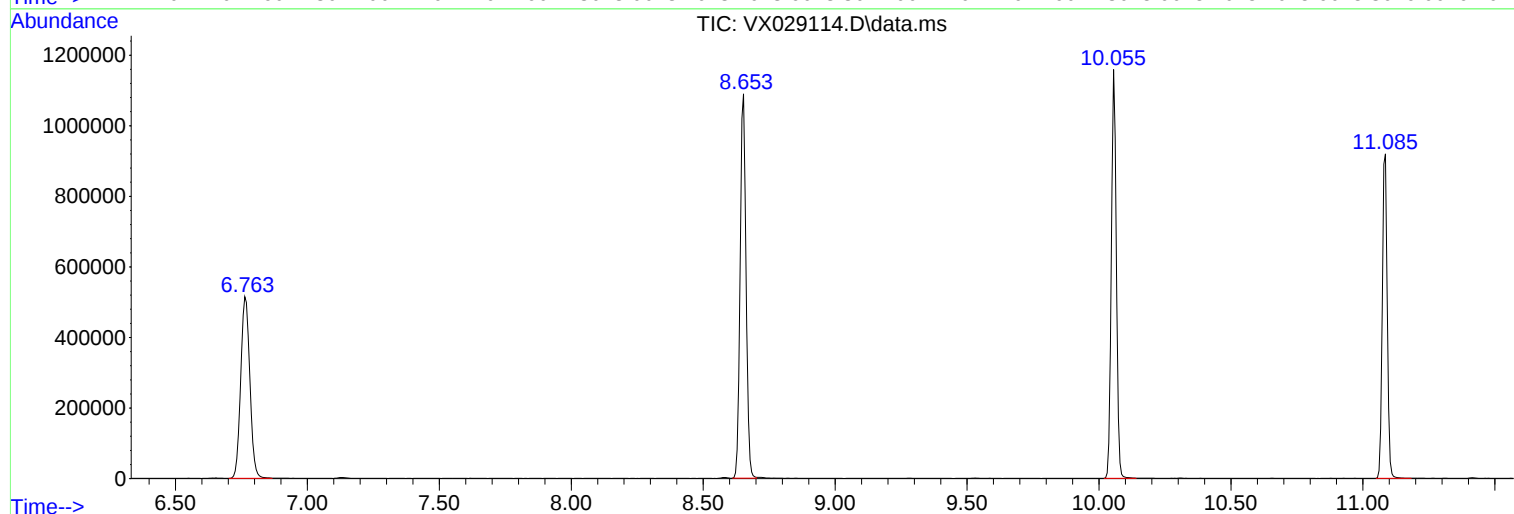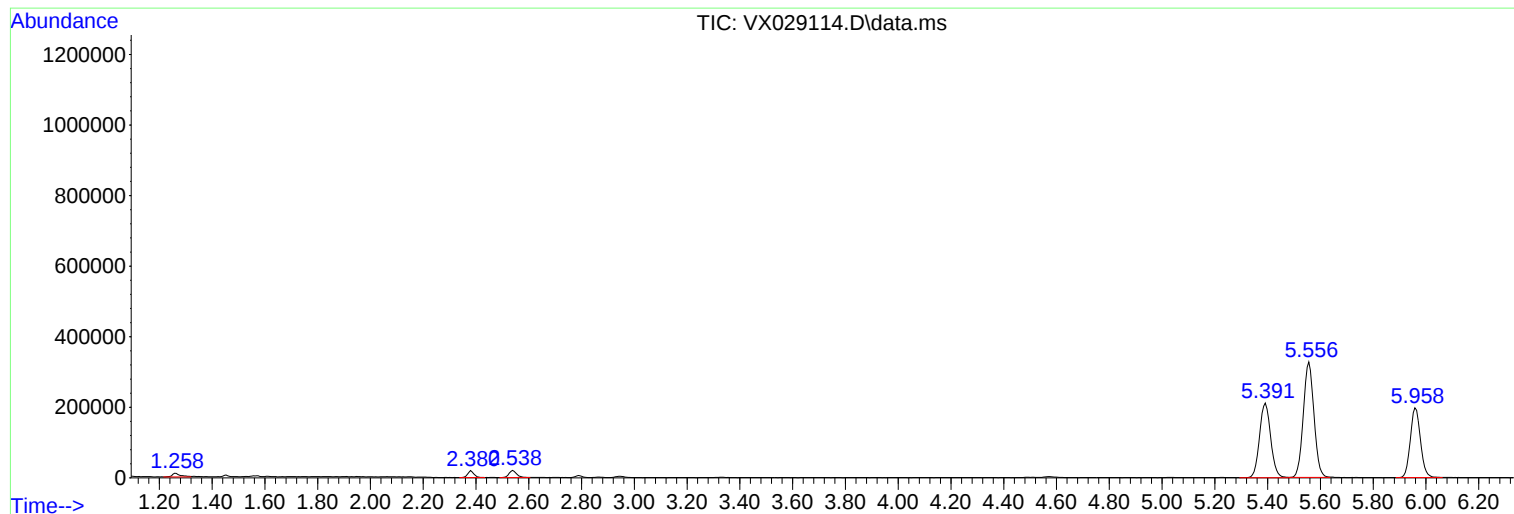

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060122\
Data File : VX029114.D
Acq On : 01 Jun 2022 13:37
Operator : JC/MD
Sample : N3022-16
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RB06-20220525

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060122\
Data File : VX029114.D
Acq On : 01 Jun 2022 13:37
Operator : JC/MD
Sample : N3022-16
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RB06-20220525

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------