

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060122\
 Data File : VX029119.D
 Acq On : 01 Jun 2022 15:34
 Operator : JC/MD
 Sample : N3022-04 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 45BR-20220525

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M

Title : SW846 8260

Signal : TIC: VX029119.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.947	297	305	313	rBV	21503	49399	1.75%	0.400%
2	4.489	548	558	569	rBV	213355	588002	20.80%	4.760%
3	5.391	694	706	721	rBV	198954	585757	20.72%	4.742%
4	5.556	721	733	750	rVB	310601	891300	31.53%	7.215%
5	5.958	789	799	816	rBV	186992	503748	17.82%	4.078%
6	6.763	921	931	948	rBV	497078	1176269	41.61%	9.522%
7	7.129	981	991	1005	rBV	1331909	2826792	100.00%	22.884%
8	8.653	1234	1241	1260	rBV	1032155	1615410	57.15%	13.077%
9	10.055	1465	1471	1485	rBV	1112521	1475228	52.19%	11.942%
10	11.085	1634	1640	1653	rBV	902760	1157755	40.96%	9.372%
11	12.024	1788	1794	1806	rBV	1215187	1483274	52.47%	12.007%




Sum of corrected areas: 12352934

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060122\
Data File : VX029119.D
Acq On : 01 Jun 2022 15:34
Operator : JC/MD
Sample : N3022-04 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
45BR-20220525

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

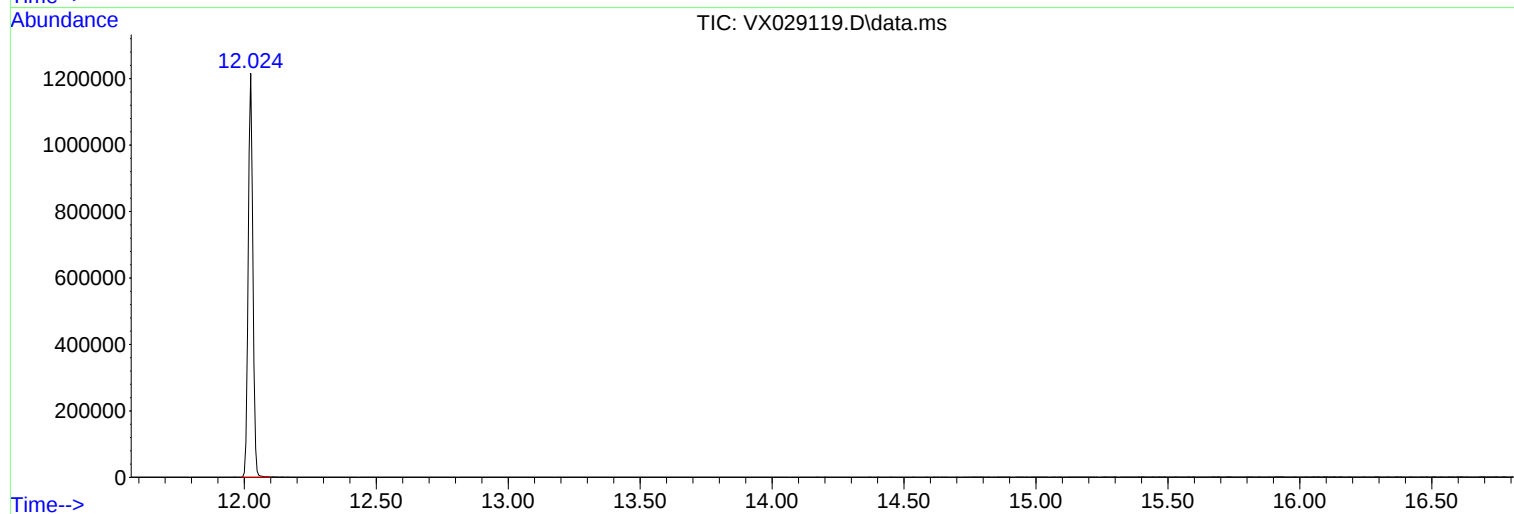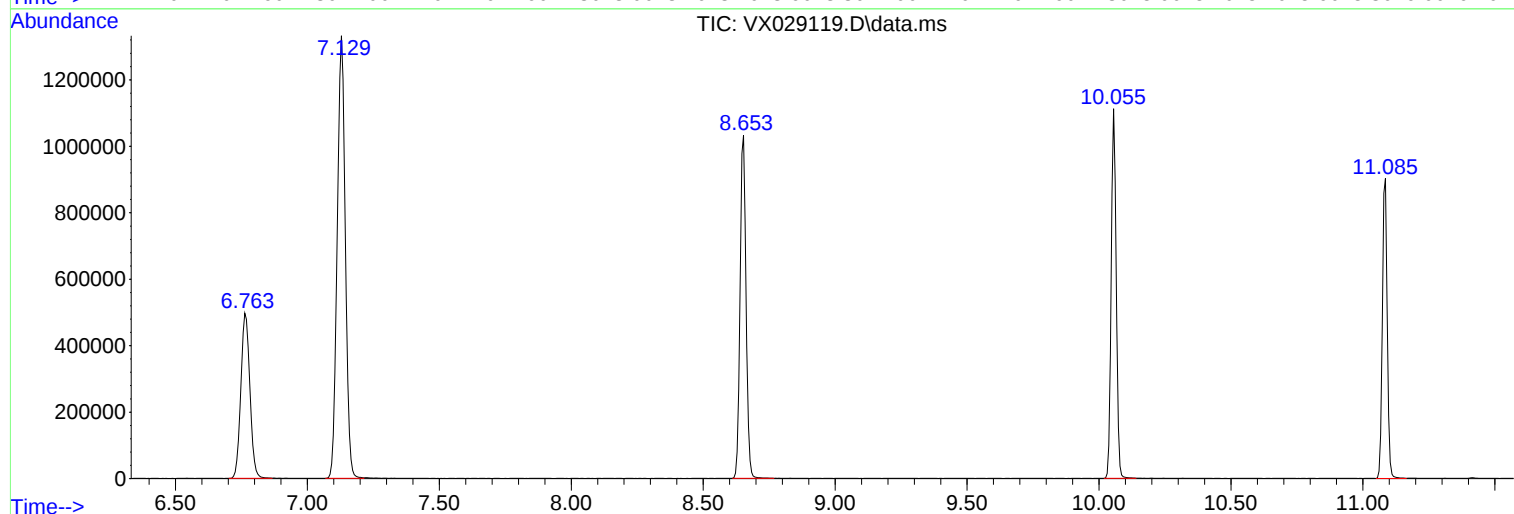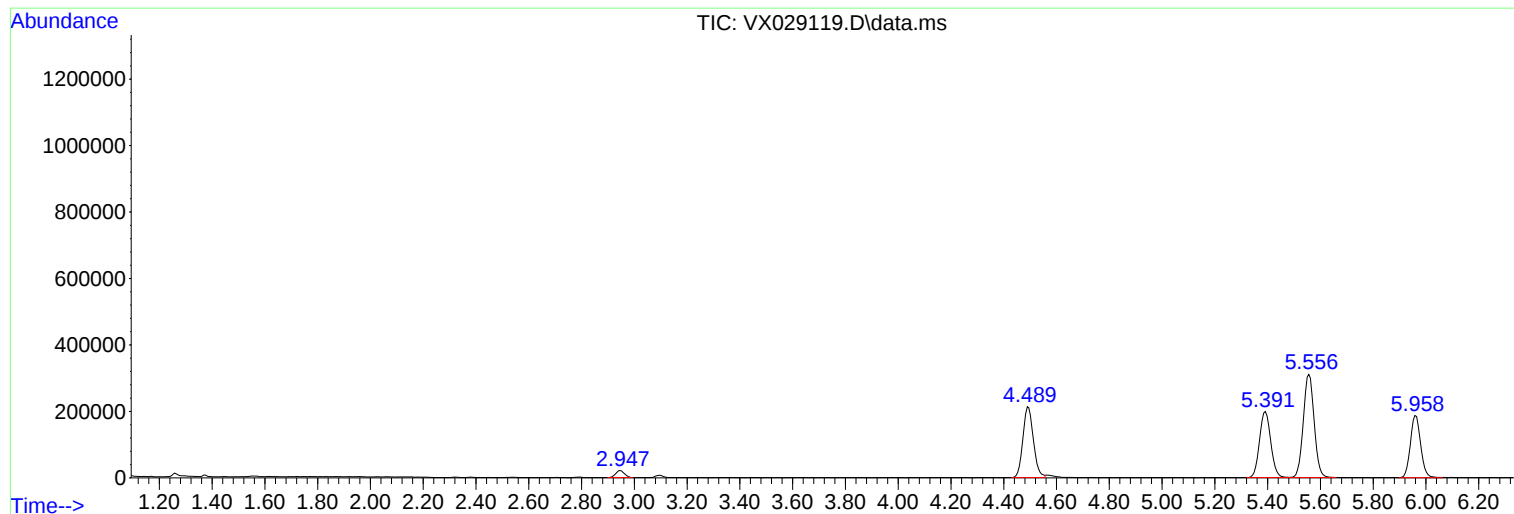

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060122\
Data File : VX029119.D
Acq On : 01 Jun 2022 15:34
Operator : JC/MD
Sample : N3022-04 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
45BR-20220525

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060122\
Data File : VX029119.D
Acq On : 01 Jun 2022 15:34
Operator : JC/MD
Sample : N3022-04 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
45BR-20220525

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------