

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060122\
 Data File : VX029120.D
 Acq On : 01 Jun 2022 15:57
 Operator : JC/MD
 Sample : N3022-15 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 DUP03-20220525

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
 Title : SW846 8260

Signal : TIC: VX029120.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	52	rVB	28279	29004	1.32%	0.228%
2	2.947	297	305	314	rBV	21745	50639	2.30%	0.397%
3	4.489	547	558	583	rBV	495176	1362324	61.84%	10.688%
4	5.391	693	706	722	rBV	205940	603778	27.41%	4.737%
5	5.556	722	733	752	rVB	316080	911755	41.39%	7.153%
6	5.958	789	799	816	rBV	196859	515030	23.38%	4.041%
7	6.763	921	931	947	rBV	509251	1206737	54.78%	9.467%
8	7.129	981	991	1010	rBV	1025841	2202859	100.00%	17.282%
9	8.653	1234	1241	1250	rBV	1079356	1654070	75.09%	12.976%
10	10.055	1465	1471	1489	rBV	1156722	1515624	68.80%	11.890%
11	11.085	1634	1640	1651	rBV	918459	1180143	53.57%	9.258%
12	12.024	1788	1794	1803	rBV	1236740	1514703	68.76%	11.883%




Sum of corrected areas: 12746666

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060122\
Data File : VX029120.D
Acq On : 01 Jun 2022 15:57
Operator : JC/MD
Sample : N3022-15 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP03-20220525

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

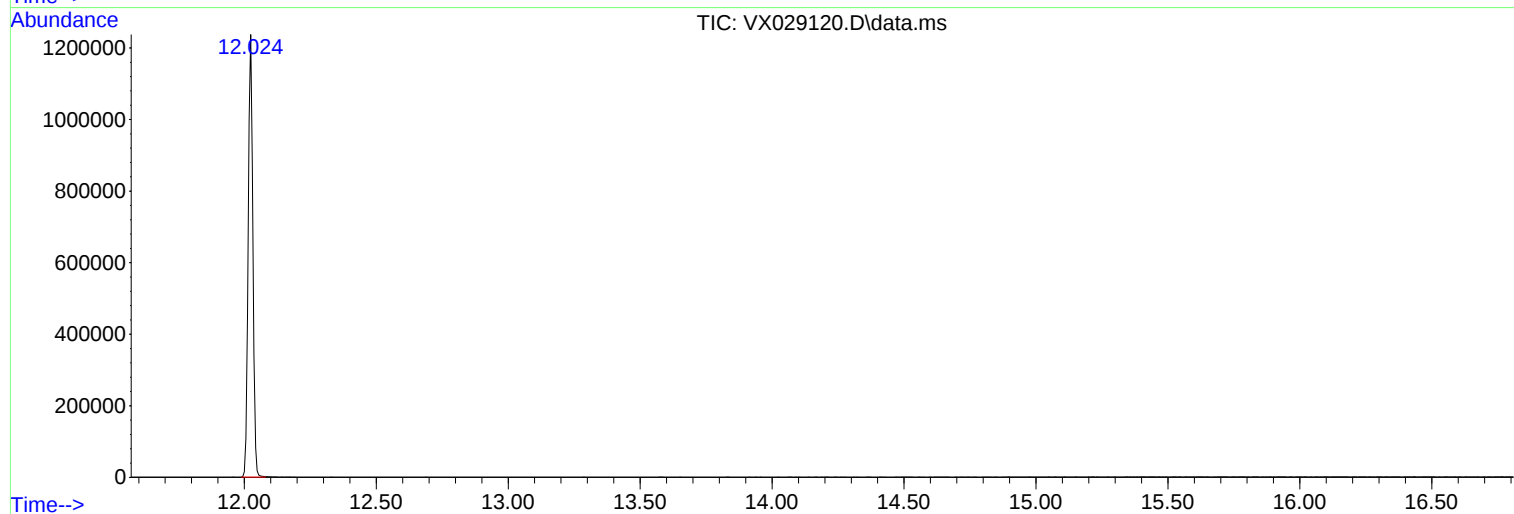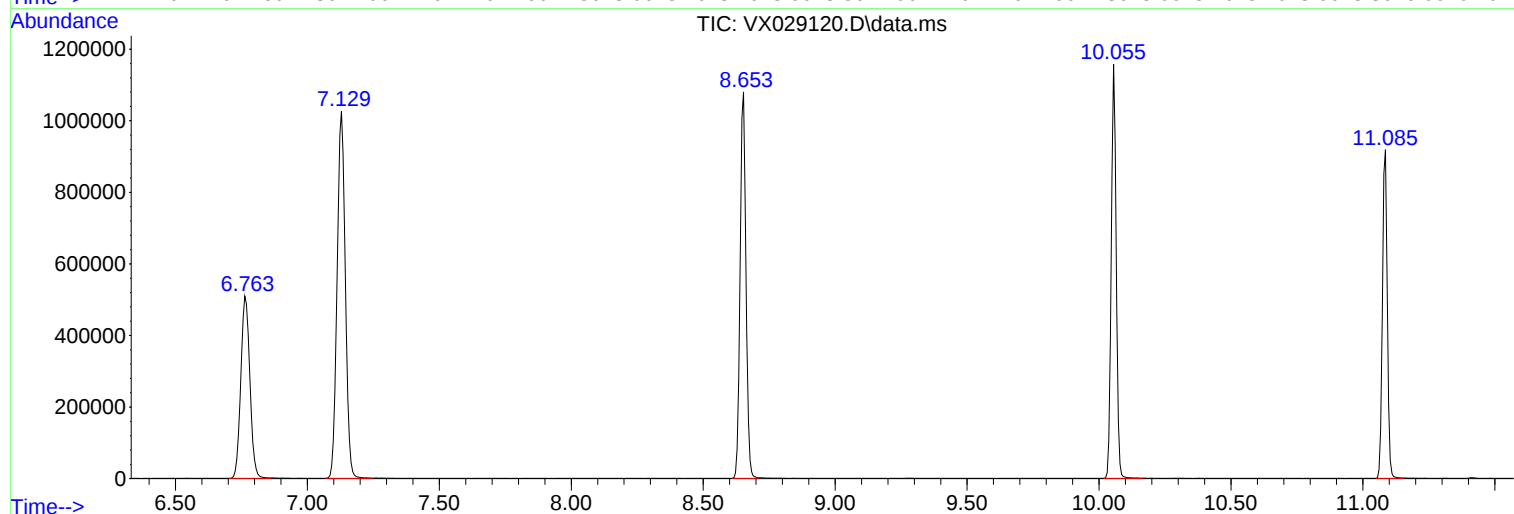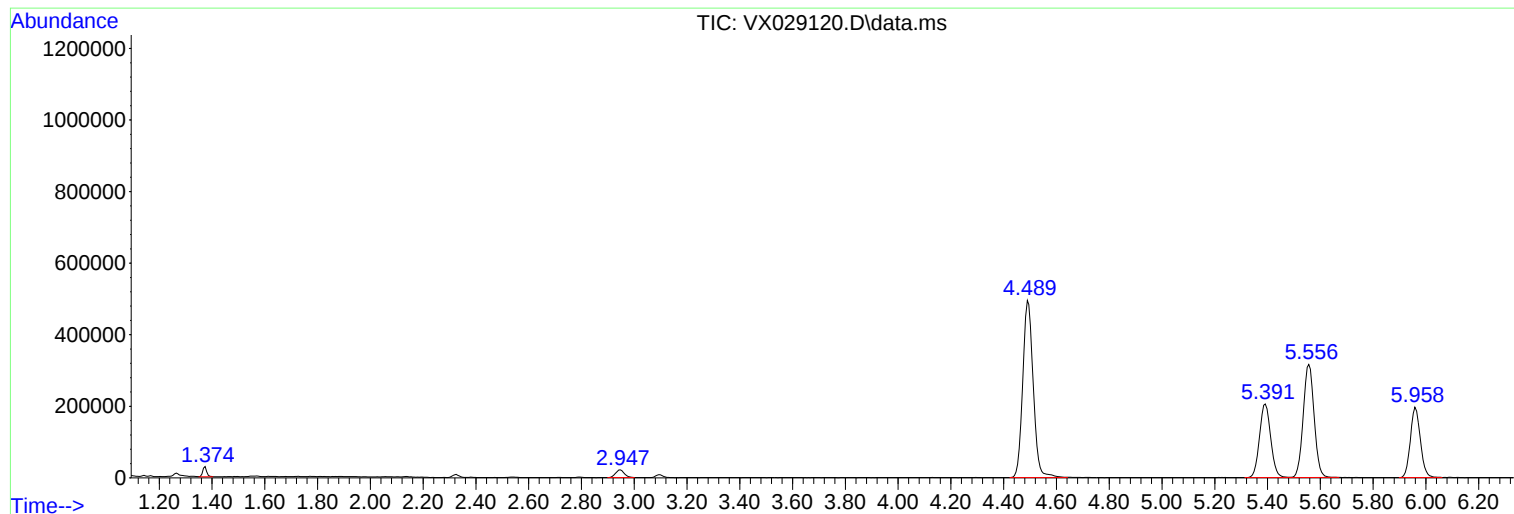

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060122\
Data File : VX029120.D
Acq On : 01 Jun 2022 15:57
Operator : JC/MD
Sample : N3022-15 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP03-20220525

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060122\
Data File : VX029120.D
Acq On : 01 Jun 2022 15:57
Operator : JC/MD
Sample : N3022-15 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
DUP03-20220525

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------