

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060122\
 Data File : VX029122.D
 Acq On : 01 Jun 2022 16:44
 Operator : JC/MD
 Sample : N3022-14 25X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 29BR-20220525

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M

Title : SW846 8260

Signal : TIC: VX029122.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.947	297	305	314	rBV2	28238	67120	2.36%	0.547%
2	4.495	548	559	568	rBV	68646	196515	6.91%	1.600%
3	5.391	693	706	721	rBV	211575	612844	21.55%	4.991%
4	5.556	721	733	752	rVB	327186	925820	32.56%	7.540%
5	5.958	790	799	818	rBV	194682	519794	18.28%	4.233%
6	6.763	921	931	951	rBV	520023	1226936	43.14%	9.993%
7	7.129	981	991	1011	rBV	1325212	2843757	100.00%	23.161%
8	8.653	1234	1241	1253	rBV	1087670	1687229	59.33%	13.741%
9	10.055	1465	1471	1483	rBV	1138817	1524009	53.59%	12.412%
10	11.085	1634	1640	1651	rBV	931907	1184281	41.64%	9.645%
11	12.024	1789	1794	1808	rVB	1234483	1490145	52.40%	12.136%




Sum of corrected areas: 12278450

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060122\
Data File : VX029122.D
Acq On : 01 Jun 2022 16:44
Operator : JC/MD
Sample : N3022-14 25X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
29BR-20220525

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

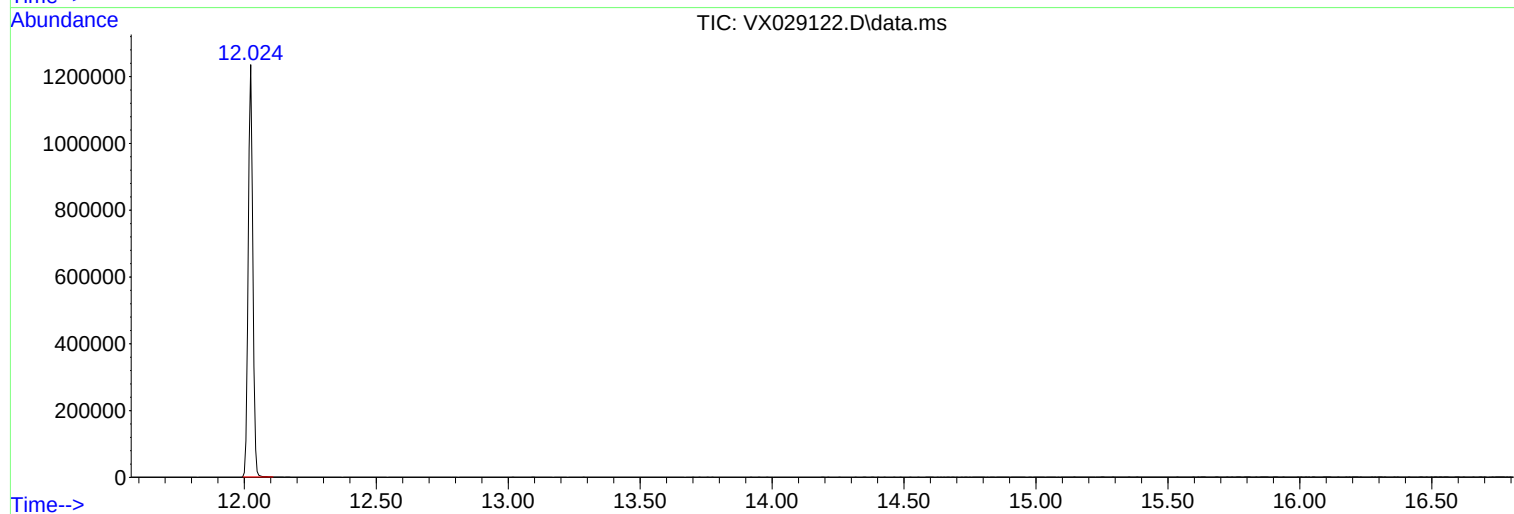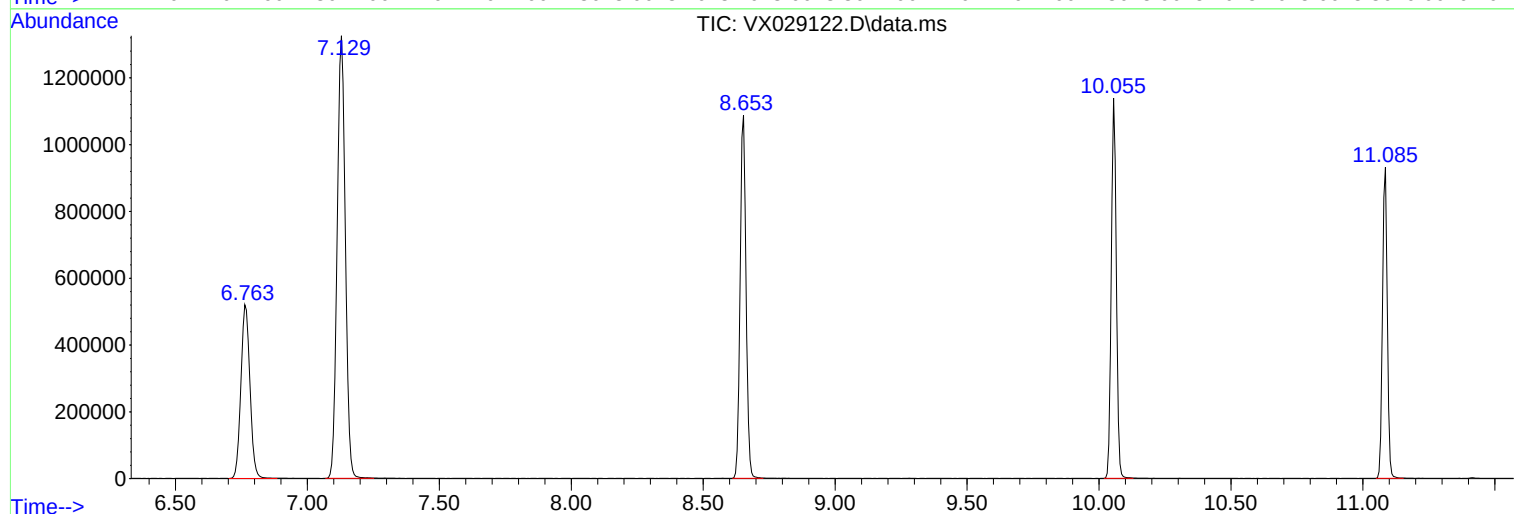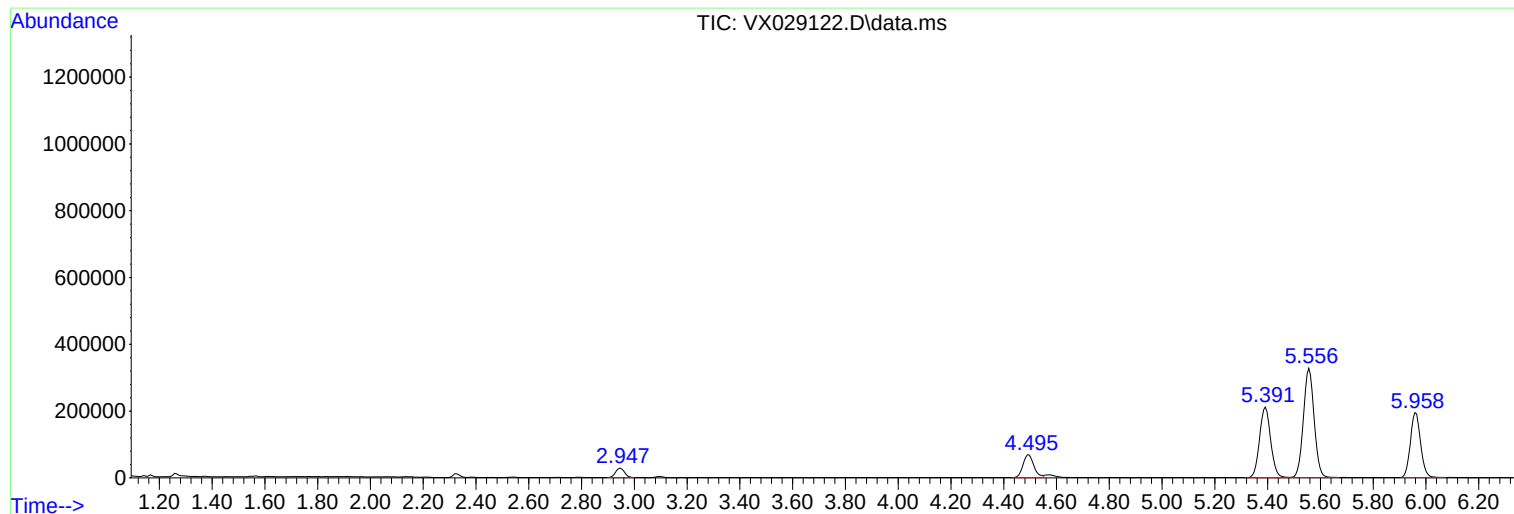

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060122\
Data File : VX029122.D
Acq On : 01 Jun 2022 16:44
Operator : JC/MD
Sample : N3022-14 25X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
29BR-20220525

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060122\
Data File : VX029122.D
Acq On : 01 Jun 2022 16:44
Operator : JC/MD
Sample : N3022-14 25X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
29BR-20220525

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc