

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060122\
 Data File : VX029123.D
 Acq On : 01 Jun 2022 17:07
 Operator : JC/MD
 Sample : N3022-03 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 25BR-20220525

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M

Title : SW846 8260

Signal : TIC: VX029123.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.947	297	305	318	rVB	11636	26666	1.23%	0.220%
2	4.489	547	558	581	rBV	332577	919659	42.26%	7.589%
3	5.391	693	706	721	rBV2	206735	599455	27.55%	4.947%
4	5.556	721	733	751	rVB	318512	904289	41.55%	7.462%
5	5.958	789	799	815	rBV	190576	508087	23.35%	4.193%
6	6.763	920	931	951	rBV	507023	1199869	55.14%	9.902%
7	7.129	981	991	1006	rBV	1011947	2176221	100.00%	17.959%
8	8.653	1234	1241	1256	rBV	1060399	1649306	75.79%	13.611%
9	10.055	1465	1471	1485	rBV	1154024	1499407	68.90%	12.374%
10	11.085	1634	1640	1652	rBV	914378	1167256	53.64%	9.633%
11	12.024	1789	1794	1805	rBV	1222249	1467587	67.44%	12.111%




Sum of corrected areas: 12117802

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060122\
Data File : VX029123.D
Acq On : 01 Jun 2022 17:07
Operator : JC/MD
Sample : N3022-03 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
25BR-20220525

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

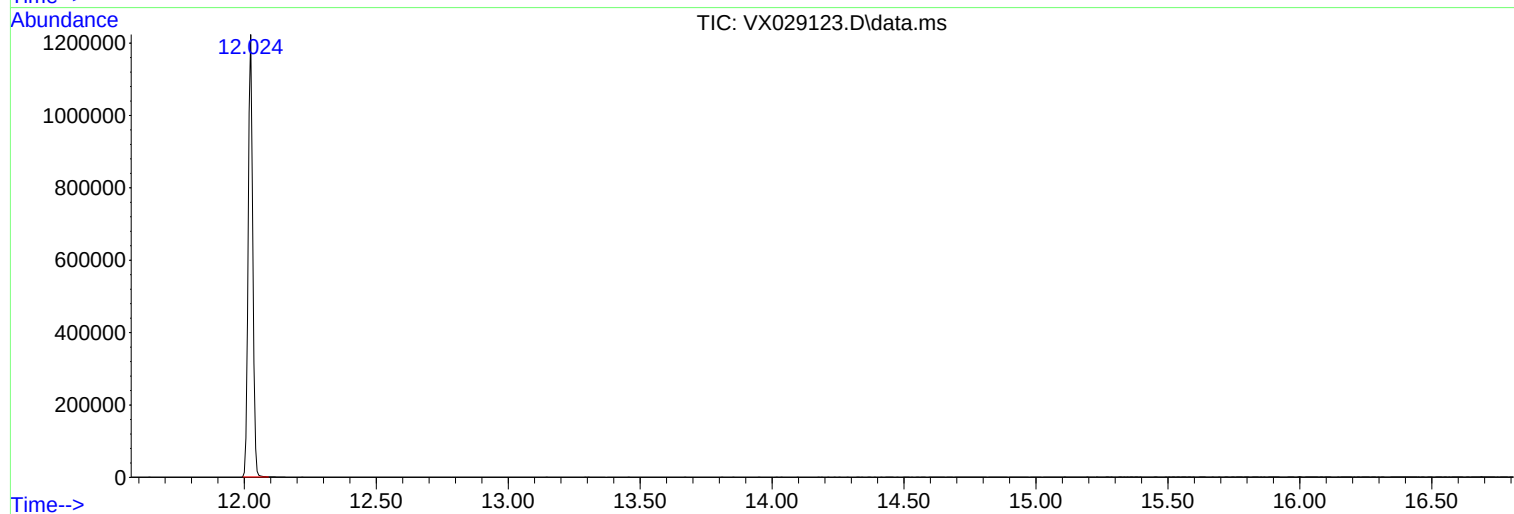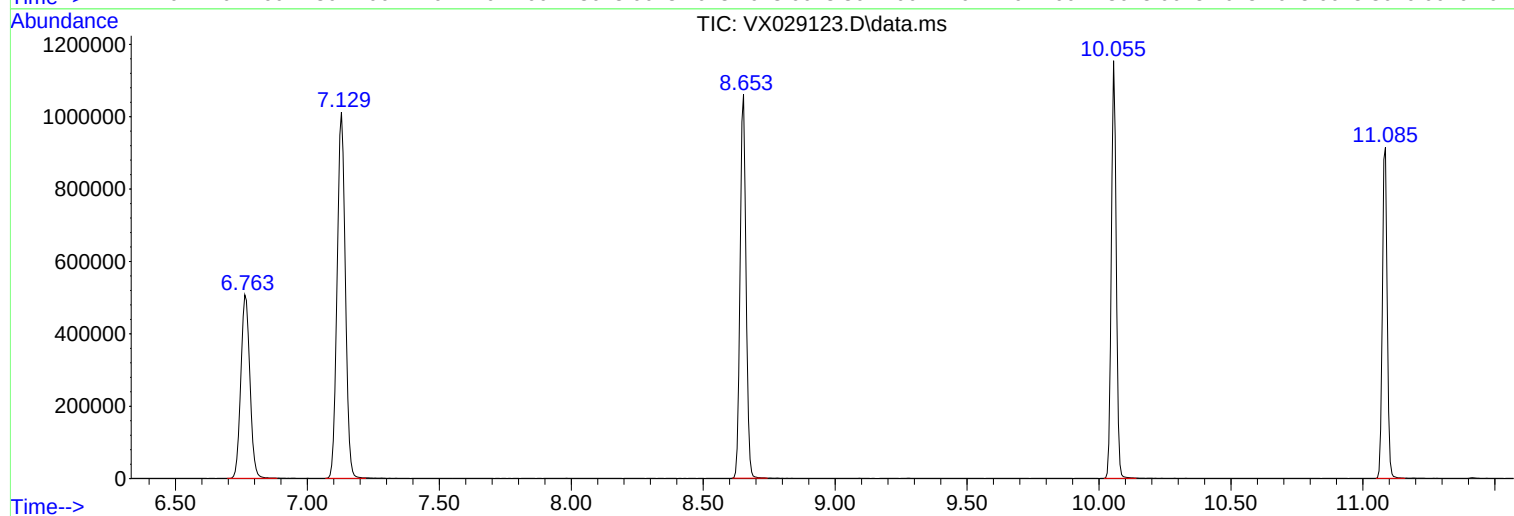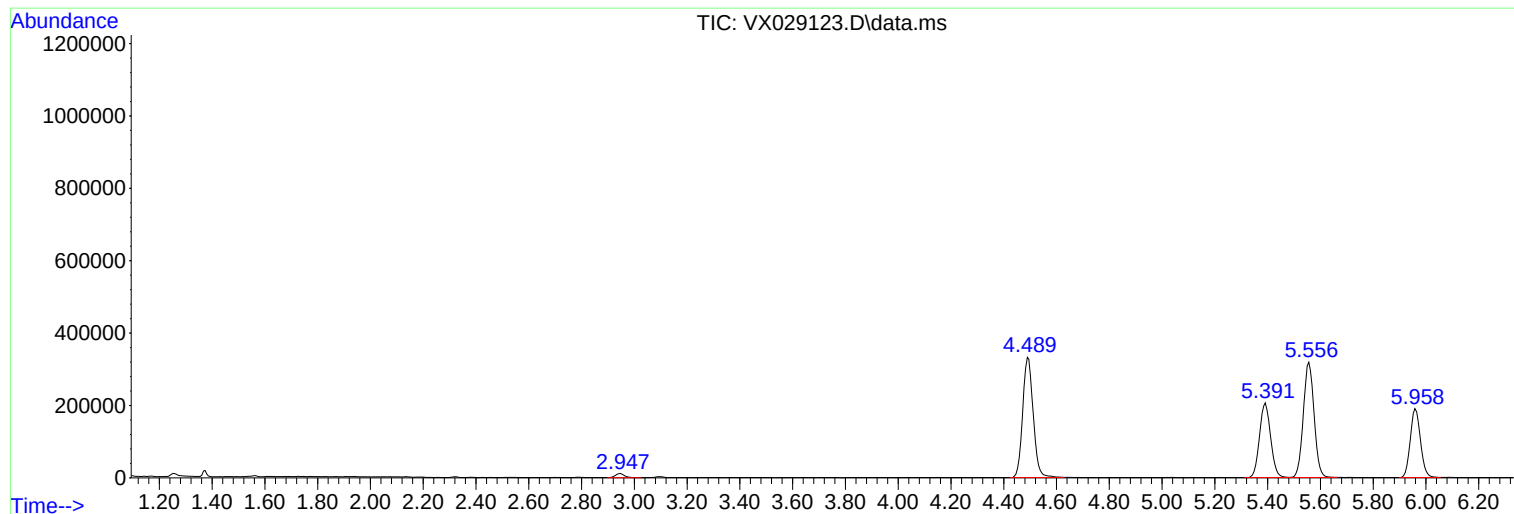

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060122\
Data File : VX029123.D
Acq On : 01 Jun 2022 17:07
Operator : JC/MD
Sample : N3022-03 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
25BR-20220525

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060122\
Data File : VX029123.D
Acq On : 01 Jun 2022 17:07
Operator : JC/MD
Sample : N3022-03 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
25BR-20220525

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------