

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060122\
 Data File : VX029124.D
 Acq On : 01 Jun 2022 17:31
 Operator : JC/MD
 Sample : N3022-05 100X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 56BR-20220525

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
 Title : SW846 8260

Signal : TIC: VX029124.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.947	295	305	315	rBV	25338	59560	3.48%	0.523%
2	4.495	547	559	569	rBV2	86142	244424	14.29%	2.145%
3	5.391	694	706	720	rBV	212957	620619	36.28%	5.446%
4	5.556	720	733	747	rVB	333260	936230	54.74%	8.215%
5	5.958	785	799	815	rBV	199549	526371	30.77%	4.619%
6	6.763	921	931	947	rBV	531417	1247598	72.94%	10.948%
7	7.129	978	991	1008	rBV	788152	1690924	98.86%	14.838%
8	8.653	1234	1241	1252	rBV	1112146	1710429	100.00%	15.009%
9	10.055	1465	1471	1486	rBV	1213506	1565402	91.52%	13.736%
10	11.085	1634	1640	1652	rBV	939286	1227252	71.75%	10.769%
11	12.024	1789	1794	1809	rVB	1264734	1567165	91.62%	13.752%




Sum of corrected areas: 11395974

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060122\
Data File : VX029124.D
Acq On : 01 Jun 2022 17:31
Operator : JC/MD
Sample : N3022-05 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
56BR-20220525

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

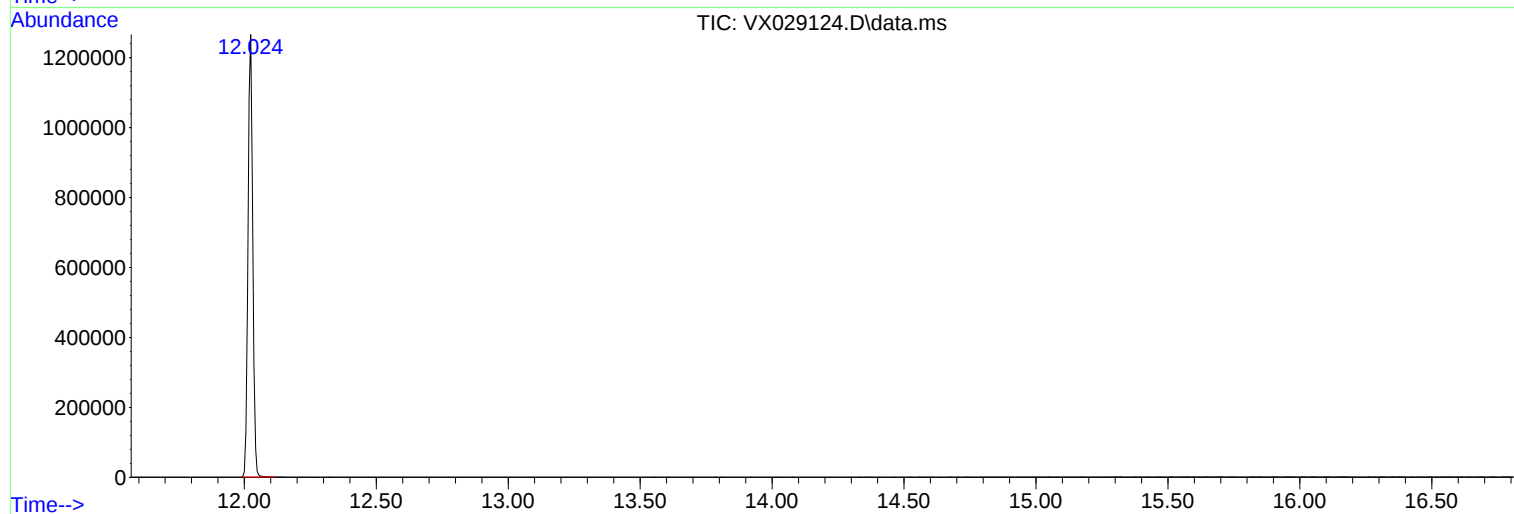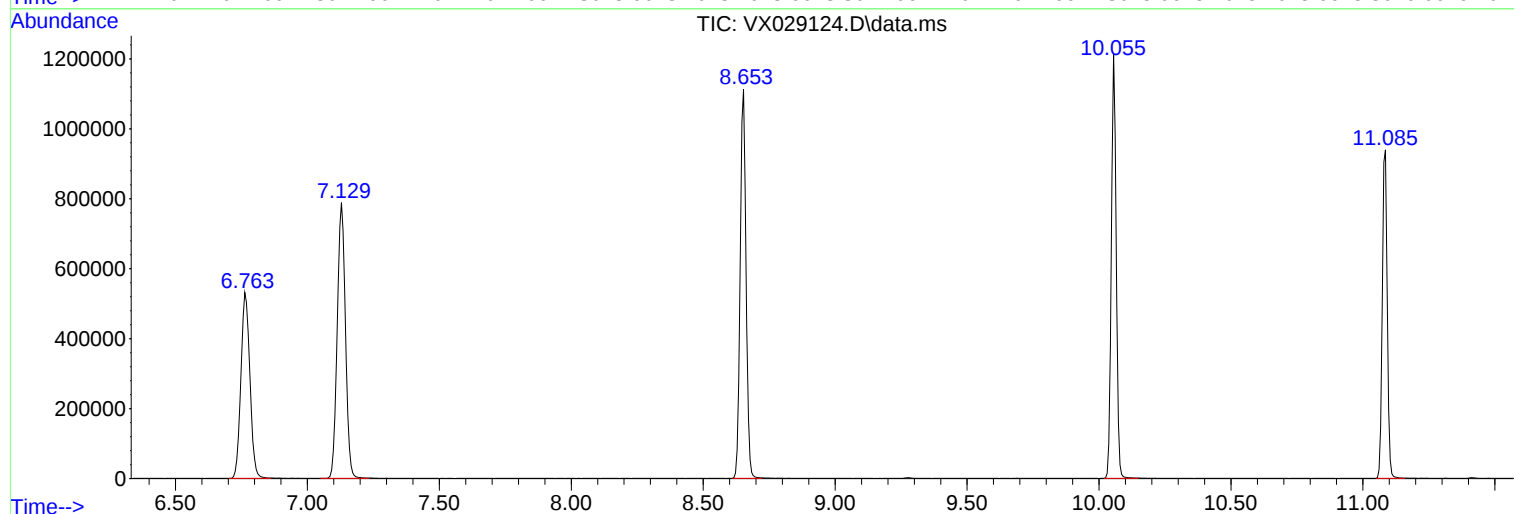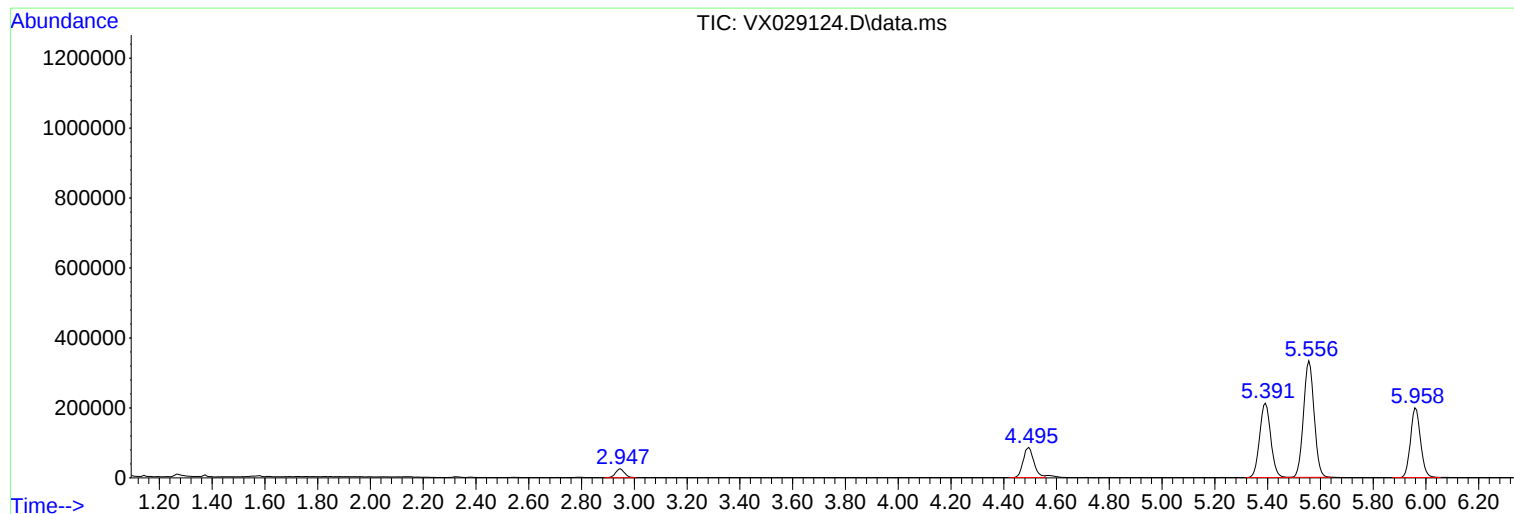

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060122\
Data File : VX029124.D
Acq On : 01 Jun 2022 17:31
Operator : JC/MD
Sample : N3022-05 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
56BR-20220525

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060122\
Data File : VX029124.D
Acq On : 01 Jun 2022 17:31
Operator : JC/MD
Sample : N3022-05 100X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
56BR-20220525

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------