


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060122\
Data File : VX029105.D
Acq On : 01 Jun 2022 09:42
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
Title : SW846 8260
Last Update : Wed Jun 01 04:45:42 2022

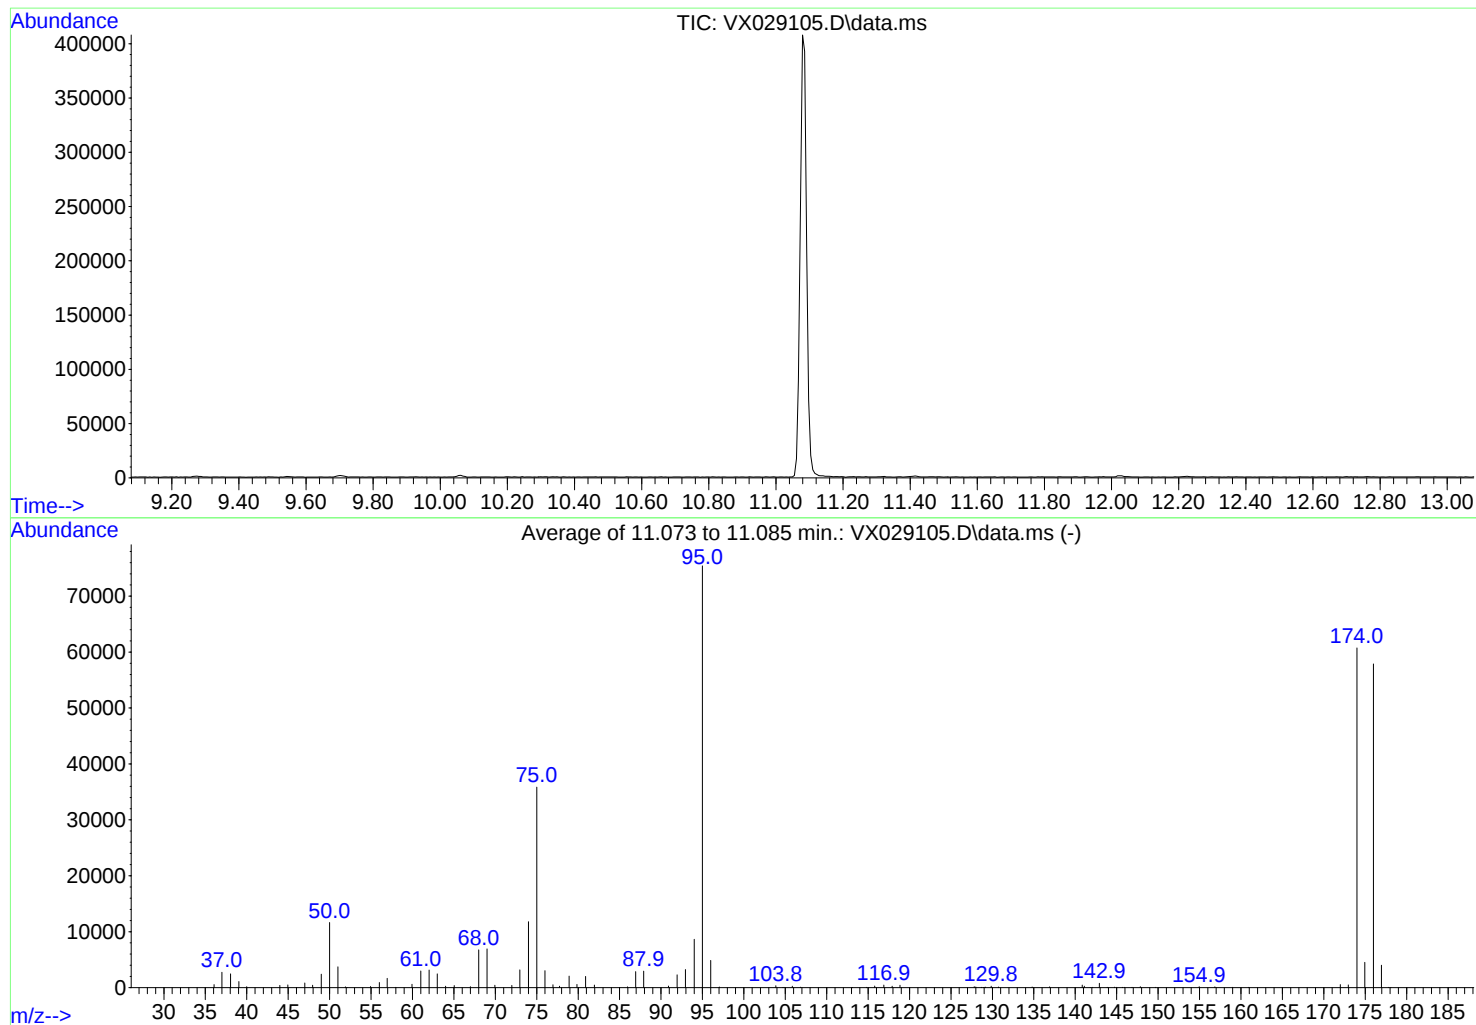

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.4	11650	PASS
75	95	30	60	47.5	35859	PASS
95	95	100	100	100.0	75424	PASS
96	95	5	9	6.5	4867	PASS
173	174	0.00	2	0.8	485	PASS
174	95	50	100	80.5	60736	PASS
175	174	5	9	7.4	4521	PASS
176	174	95	101	95.3	57891	PASS
177	176	5	9	6.9	4021	PASS