

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX060123\  
Data File : VX035957.D  
Acq On : 01 Jun 2023 14:14  
Operator : JC/MD  
Sample : 03002-10  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-48

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X053123W.M

Title : SW846 8260

Signal : TIC: VX035957.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.618       | 76            | 87          | 90           | rBV      | 16040          | 53121         | 4.57%           | 0.833%        |
| 2         | 5.385       | 691           | 705         | 720          | rBV      | 129288         | 377605        | 32.47%          | 5.923%        |
| 3         | 5.550       | 720           | 732         | 749          | rVB      | 255610         | 726946        | 62.51%          | 11.403%       |
| 4         | 5.952       | 788           | 798         | 816          | rBV      | 157650         | 429454        | 36.93%          | 6.736%        |
| 5         | 6.763       | 920           | 931         | 943          | rBV      | 370840         | 891144        | 76.63%          | 13.978%       |
| 6         | 8.647       | 1233          | 1240        | 1250         | rBV      | 749306         | 1162991       | 100.00%         | 18.242%       |
| 7         | 10.055      | 1465          | 1471        | 1485         | rBV      | 718279         | 1011465       | 86.97%          | 15.866%       |
| 8         | 11.079      | 1634          | 1639        | 1651         | rBV      | 599166         | 756659        | 65.06%          | 11.869%       |
| 9         | 12.018      | 1788          | 1793        | 1806         | rBV      | 745295         | 965845        | 83.05%          | 15.150%       |




Sum of corrected areas: 6375230

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX060123\  
Data File : VX035957.D  
Acq On : 01 Jun 2023 14:14  
Operator : JC/MD  
Sample : 03002-10  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-48

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X053123W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

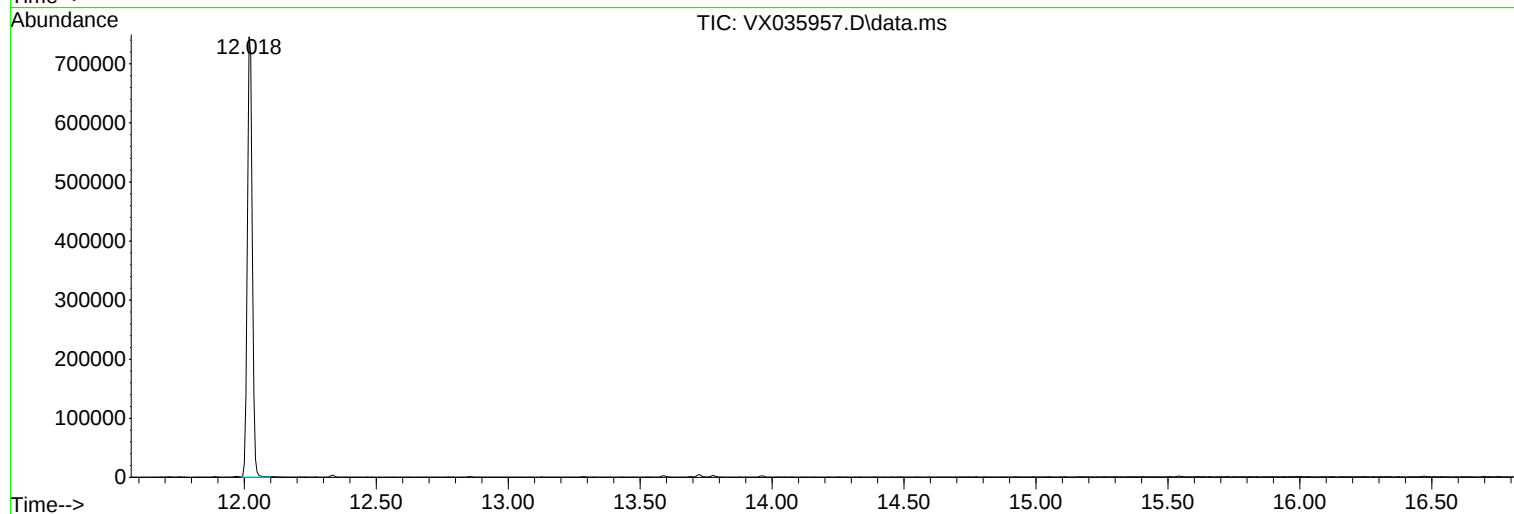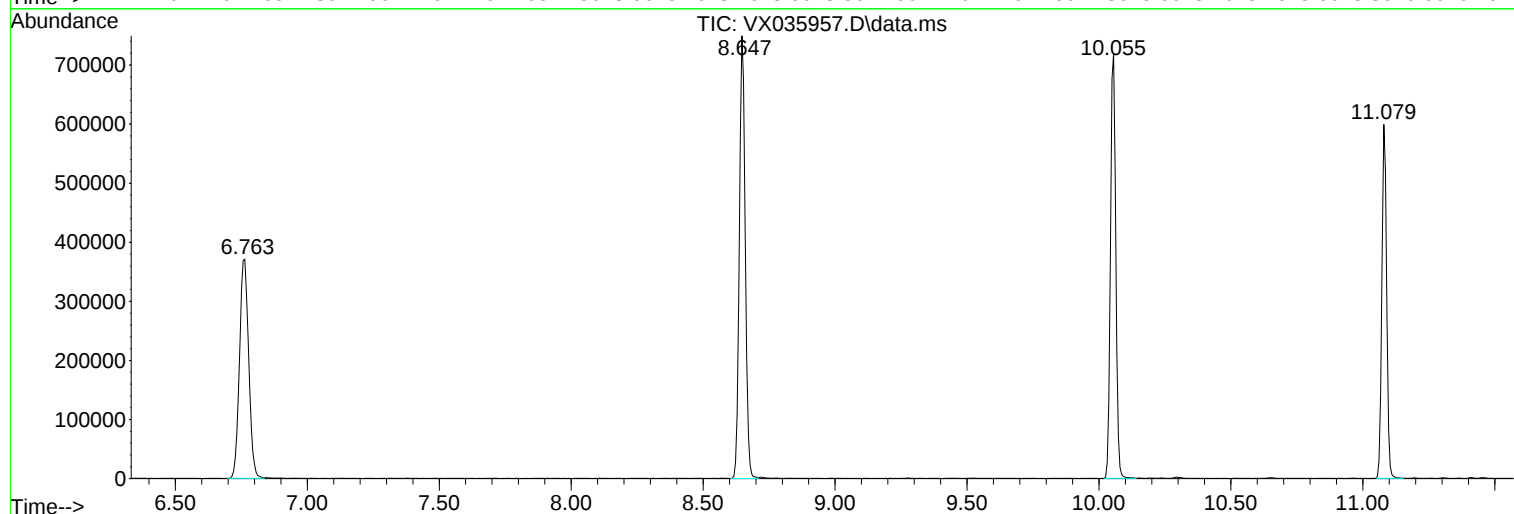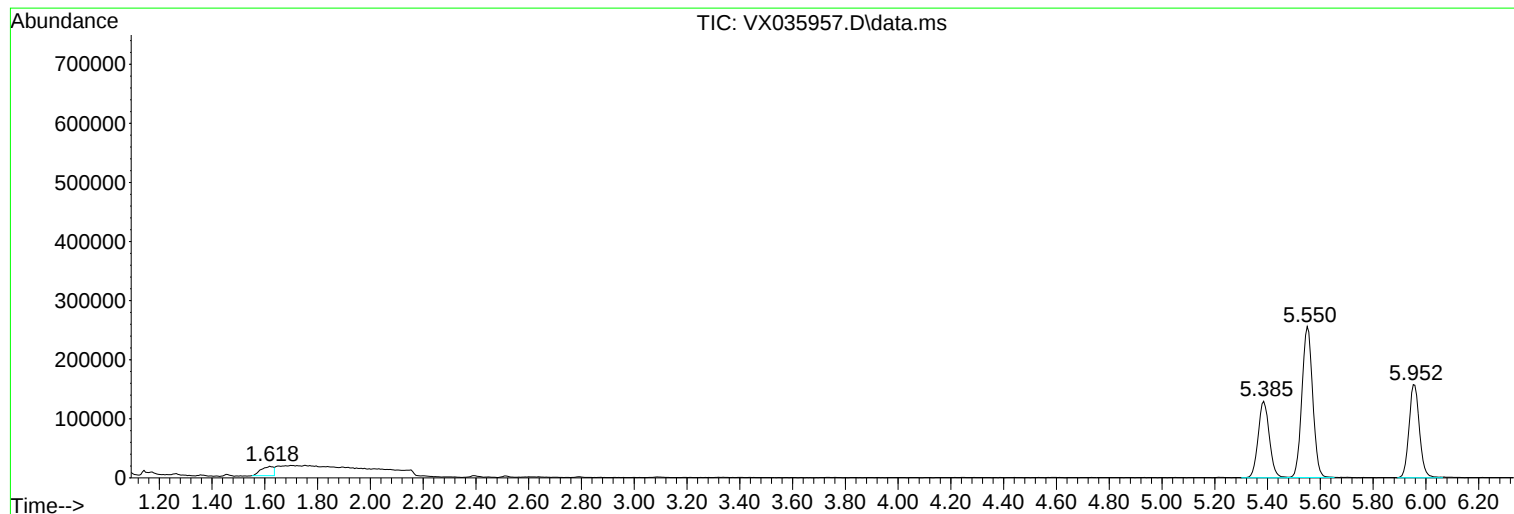

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX060123\  
Data File : VX035957.D  
Acq On : 01 Jun 2023 14:14  
Operator : JC/MD  
Sample : 03002-10  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-48

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X053123W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX060123\  
Data File : VX035957.D  
Acq On : 01 Jun 2023 14:14  
Operator : JC/MD  
Sample : 03002-10  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
MW-48

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X053123W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|