

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX060123\  
Data File : VX035965.D  
Acq On : 01 Jun 2023 17:22  
Operator : JC/MD  
Sample : 03005-01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 21 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
TP-11

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X053123W.M

Title : SW846 8260

Signal : TIC: VX035965.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 3.111       | 322           | 332         | 341          | rBV2     | 6459           | 16400         | 1.56%           | 0.288%        |
| 2         | 5.385       | 692           | 705         | 720          | rBV2     | 112686         | 336194        | 32.08%          | 5.907%        |
| 3         | 5.550       | 721           | 732         | 750          | rVB      | 232645         | 652439        | 62.25%          | 11.463%       |
| 4         | 5.958       | 785           | 799         | 817          | rBV      | 142645         | 376694        | 35.94%          | 6.618%        |
| 5         | 6.763       | 920           | 931         | 943          | rBV      | 334499         | 795183        | 75.87%          | 13.971%       |
| 6         | 8.647       | 1234          | 1240        | 1250         | rBV      | 655394         | 1048135       | 100.00%         | 18.416%       |
| 7         | 10.055      | 1465          | 1471        | 1482         | rBV      | 684351         | 913299        | 87.14%          | 16.047%       |
| 8         | 11.079      | 1634          | 1639        | 1653         | rVB      | 537254         | 683237        | 65.19%          | 12.004%       |
| 9         | 12.024      | 1788          | 1794        | 1808         | rBV      | 684137         | 869978        | 83.00%          | 15.285%       |




Sum of corrected areas: 5691559

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX060123\  
Data File : VX035965.D  
Acq On : 01 Jun 2023 17:22  
Operator : JC/MD  
Sample : 03005-01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 21 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
TP-11

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X053123W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

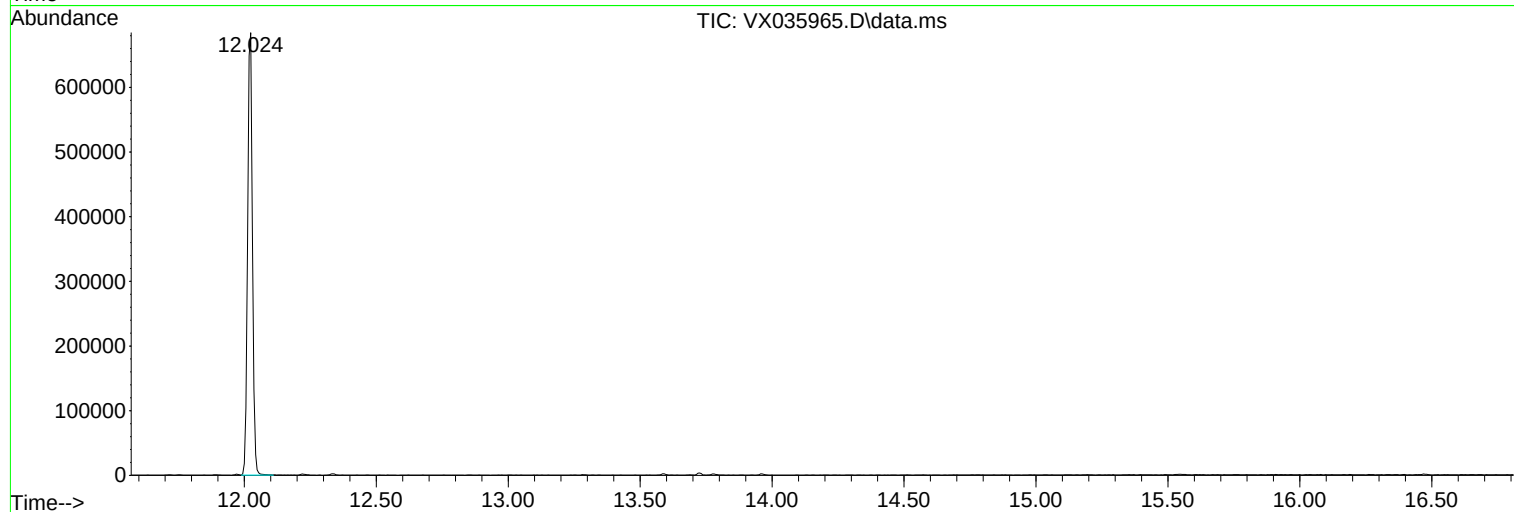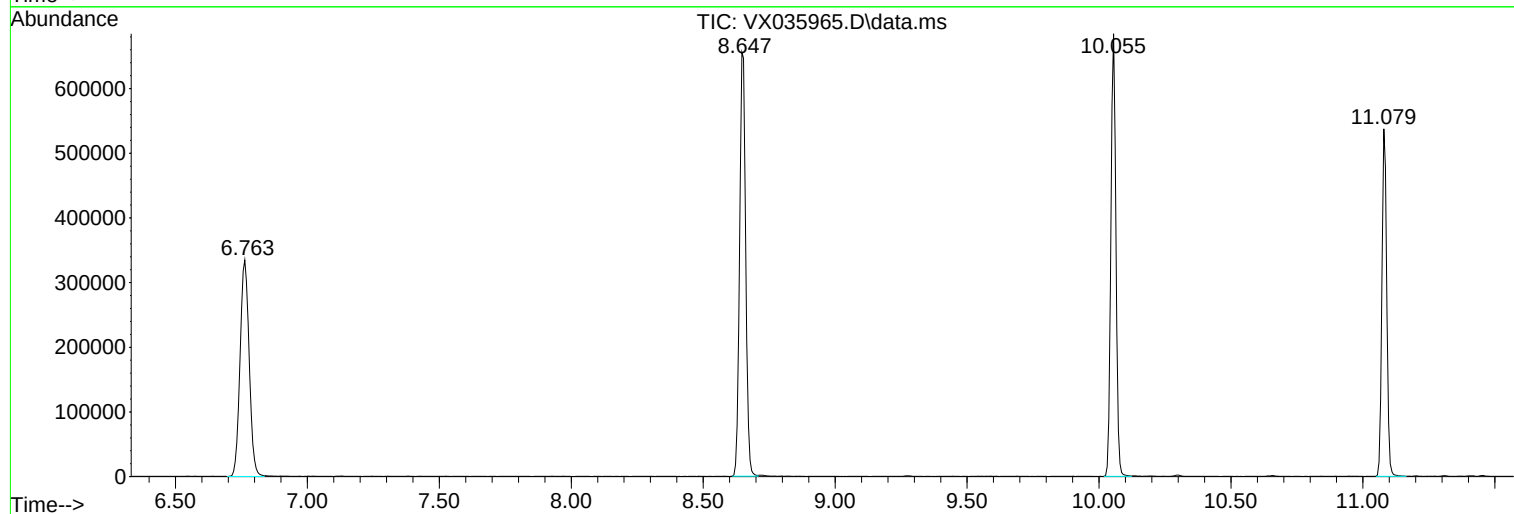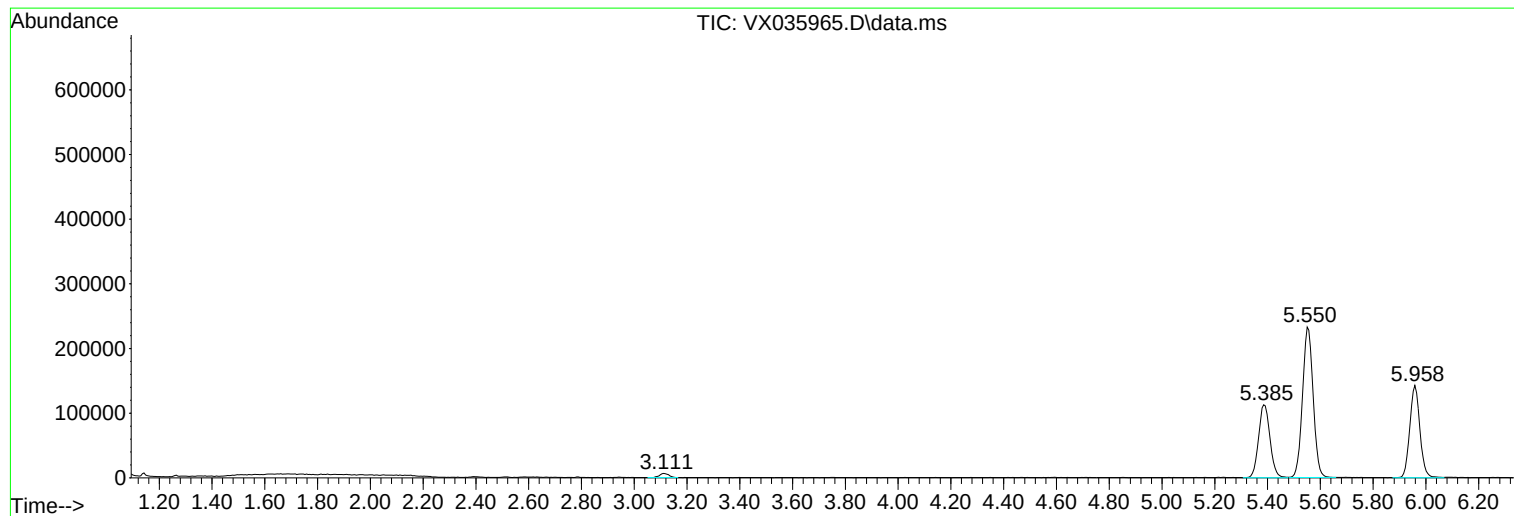

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX060123\  
Data File : VX035965.D  
Acq On : 01 Jun 2023 17:22  
Operator : JC/MD  
Sample : 03005-01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 21 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
TP-11

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X053123W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX060123\  
Data File : VX035965.D  
Acq On : 01 Jun 2023 17:22  
Operator : JC/MD  
Sample : 03005-01  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 21 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
TP-11

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X053123W.M  
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|