

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060222\
 Data File : VX029171.D
 Acq On : 03 Jun 2022 06:18
 Operator : JC/MD
 Sample : N3164-11 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 34BR-20220531

Quant Time: Jun 03 09:42:54 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 01 04:45:42 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	310199	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	572306	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	554324	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	252214	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	200961	57.451	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	114.900%
35) Dibromofluoromethane	5.391	113	190248	50.047	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	100.100%
50) Toluene-d8	8.653	98	673012	48.407	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	96.820%
62) 4-Bromofluorobenzene	11.079	95	265664	49.432	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	98.860%
Target Compounds						
						Qvalue
20) Methylene Chloride	2.794	84	918	0.286	ug/l	# 83
37) Ethyl Acetate	4.727	43	9485	2.001	ug/l	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060222\
Data File : VX029171.D
Acq On : 03 Jun 2022 06:18
Operator : JC/MD
Sample : N3164-11 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
34BR-20220531

Quant Time: Jun 03 09:42:54 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 01 04:45:42 2022
Response via : Initial Calibration




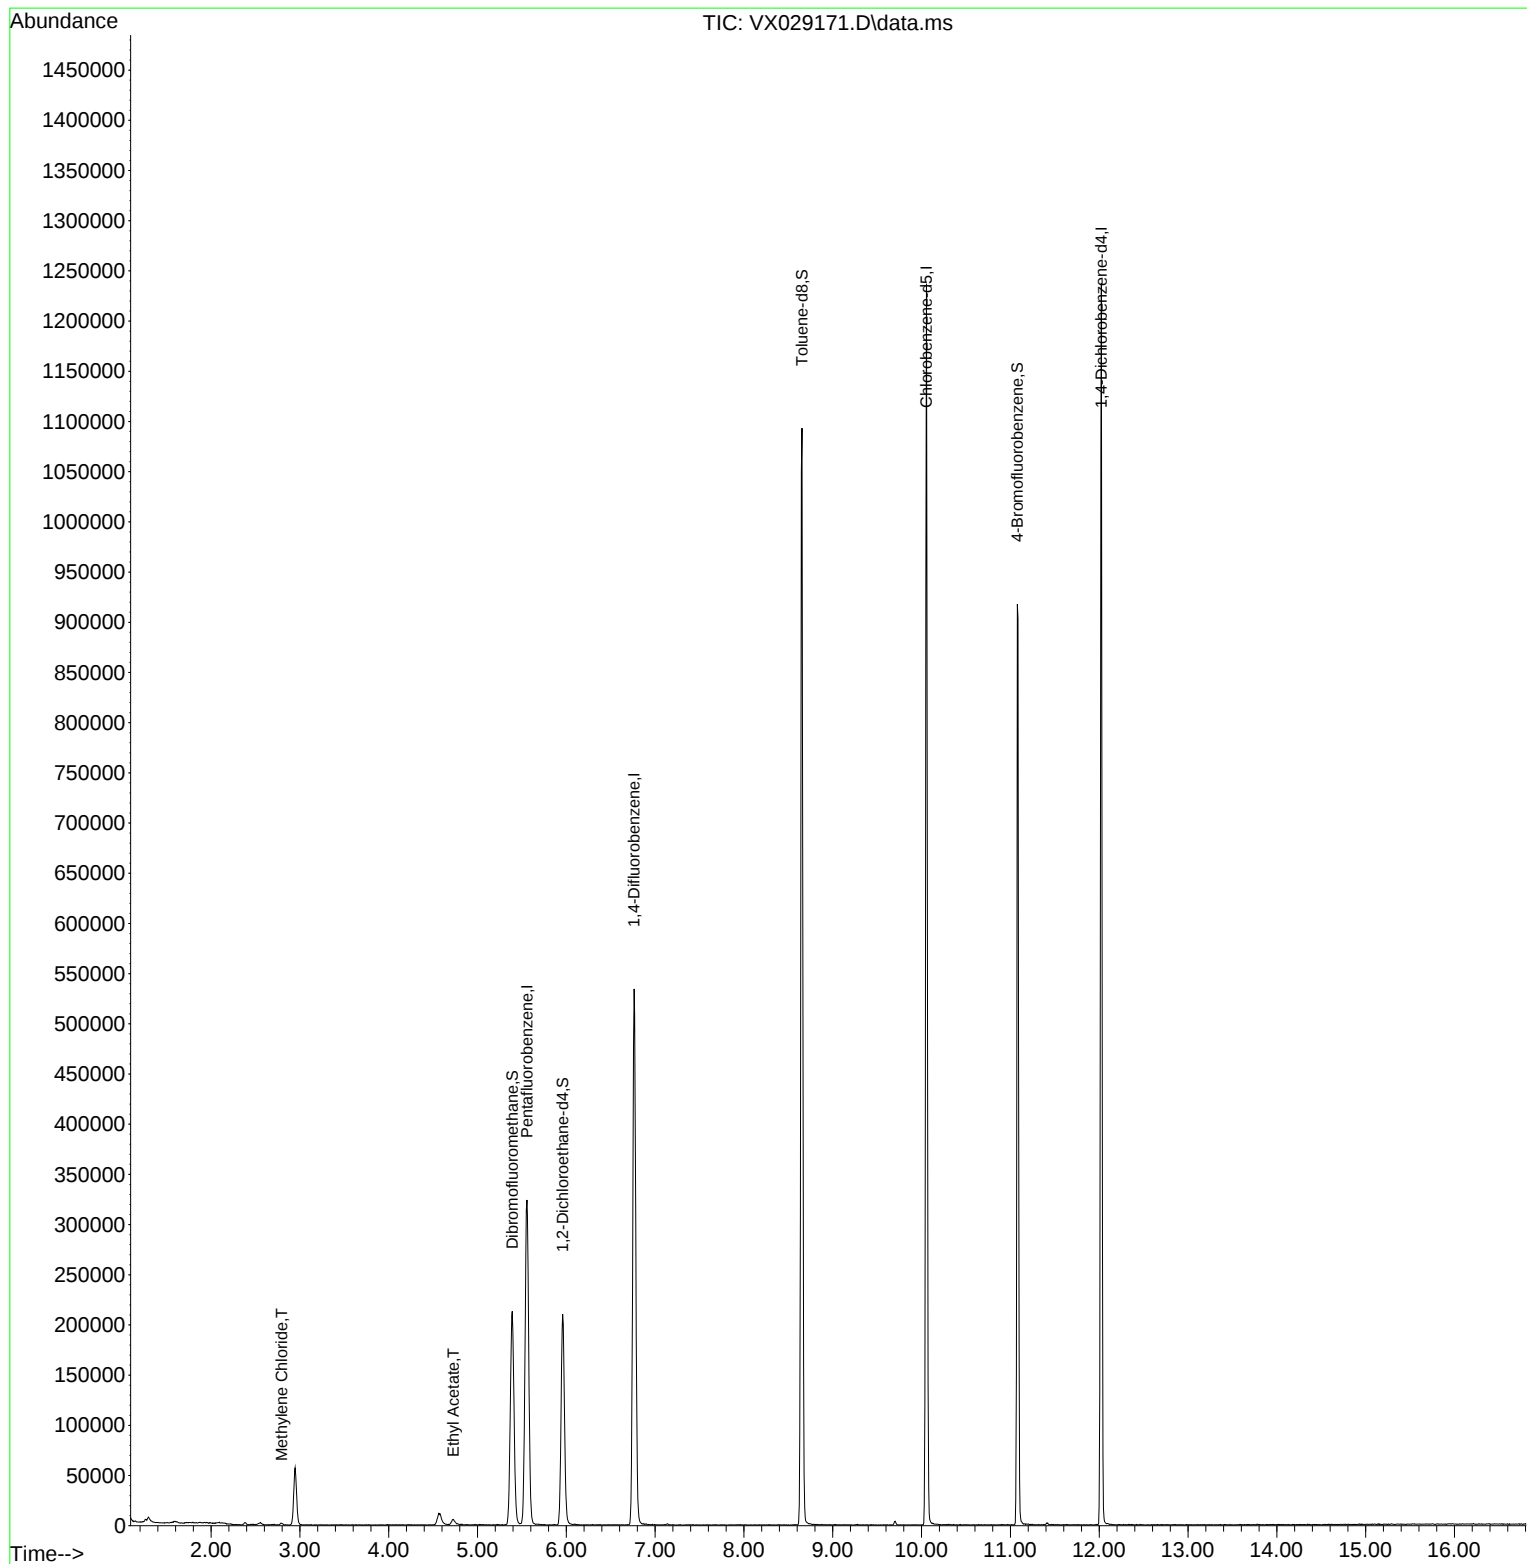


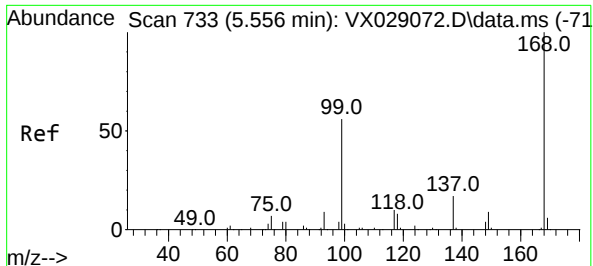

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX029171.D
Acq: 03 Jun 2022 06:18




Instrument :
MSVOA_X
ClientSampleId :
34BR-20220531


Tgt Ion:168 Resp: 310199
Ion Ratio Lower Upper
168 100
99 59.6 41.7 62.5

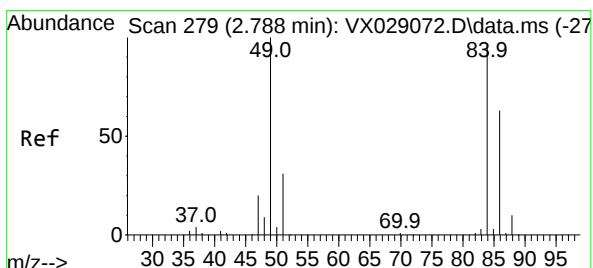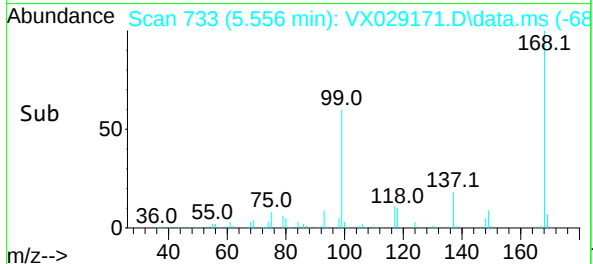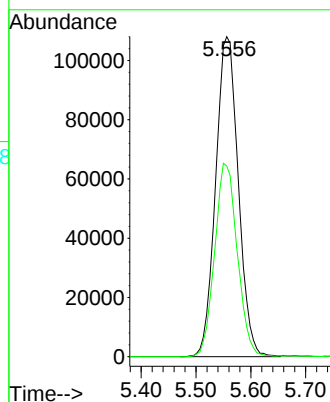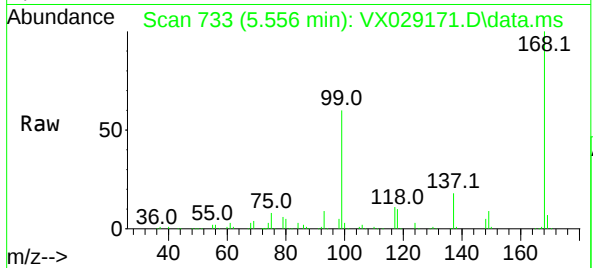

#20
Methylene Chloride
Concen: 0.286 ug/l
RT: 2.794 min Scan# 280
Delta R.T. 0.006 min
Lab File: VX029171.D
Acq: 03 Jun 2022 06:18

Tgt Ion: 84 Resp: 918
Ion Ratio Lower Upper
84 100
49 89.8 85.5 128.3
51 53.3 26.6 39.8#
86 71.6 51.5 77.3

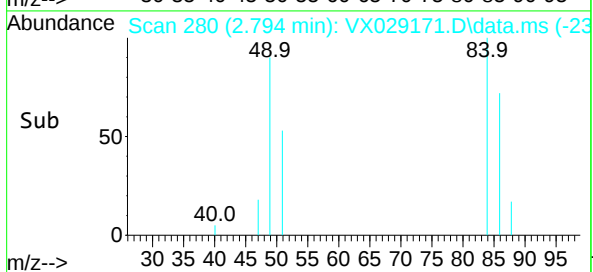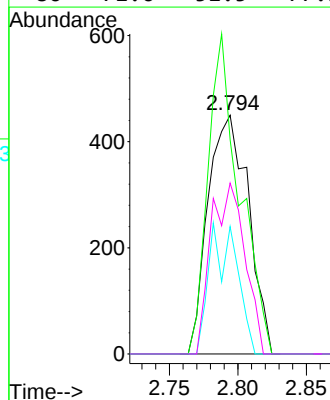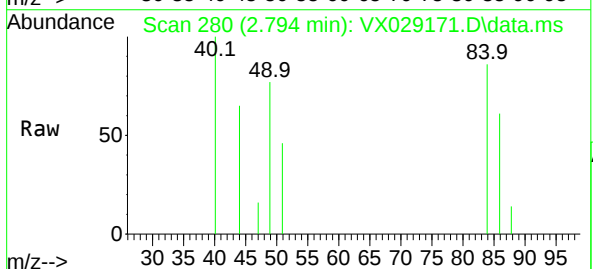

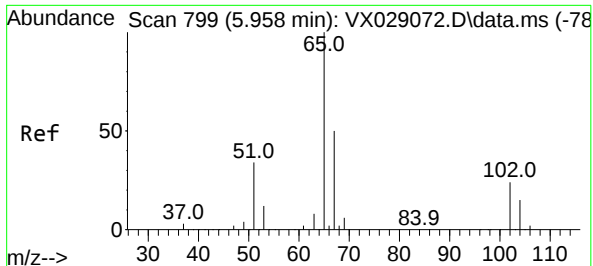

#33

1,2-Dichloroethane-d4

Concen: 57.451 ug/l

RT: 5.958 min Scan# 799

Delta R.T. 0.000 min

Lab File: VX029171.D

Acq: 03 Jun 2022 06:18

Instrument :

MSVOA_X

ClientSampleId :





34BR-20220531

Tgt Ion: 65 Resp: 200961

Ion Ratio Lower Upper

65 100

67 53.3 0.0 107.4

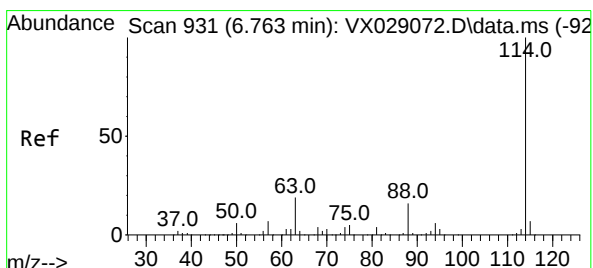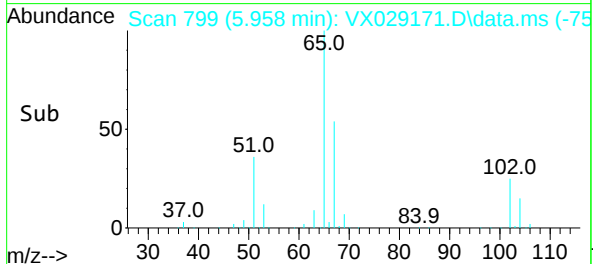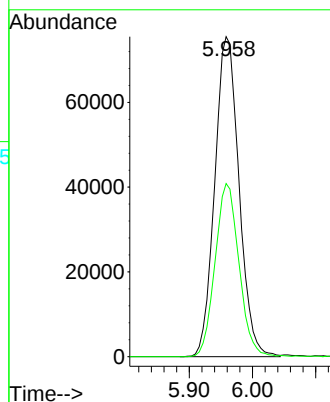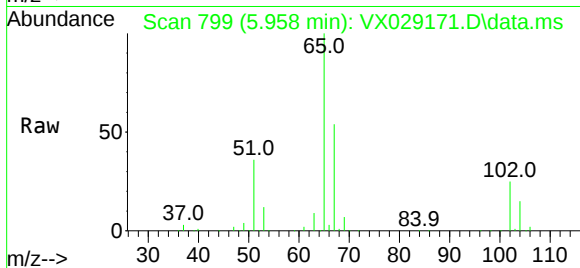

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. 0.000 min

Lab File: VX029171.D

Acq: 03 Jun 2022 06:18




Tgt Ion: 114 Resp: 572306


Ion Ratio Lower Upper

114 100

63 18.2 0.0 36.8

88 17.1 0.0 32.4


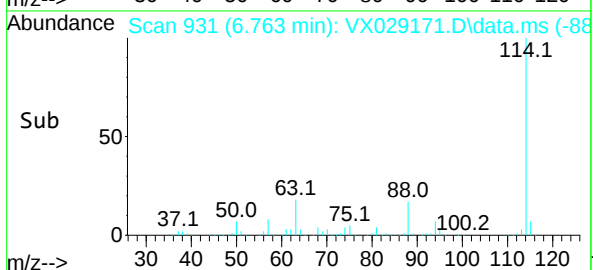
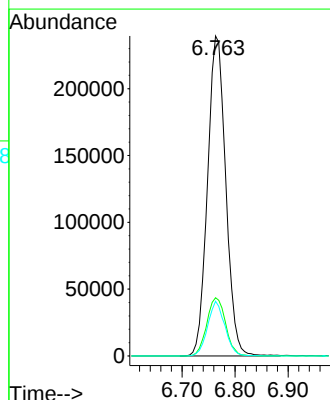
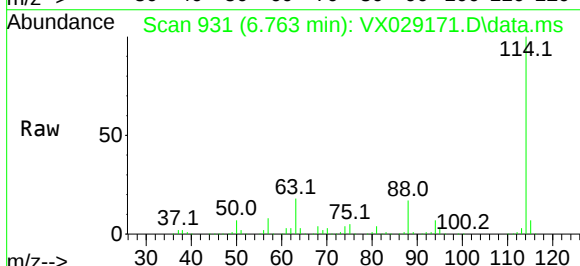


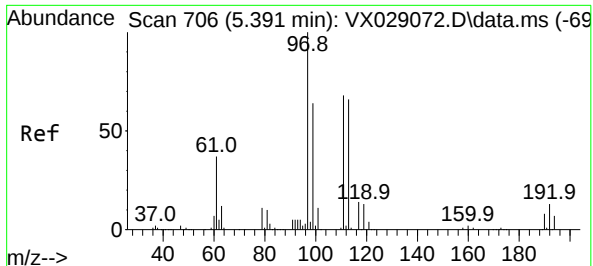

#35
Dibromofluoromethane
Concen: 50.047 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX029171.D
Acq: 03 Jun 2022 06:18




Instrument :
MSVOA_X
ClientSampleId :
34BR-20220531


Tgt Ion:113 Resp: 190248
Ion Ratio Lower Upper
113 100
111 102.2 82.8 124.2
192 18.5 16.9 25.3

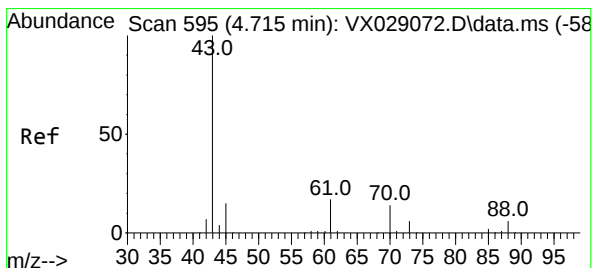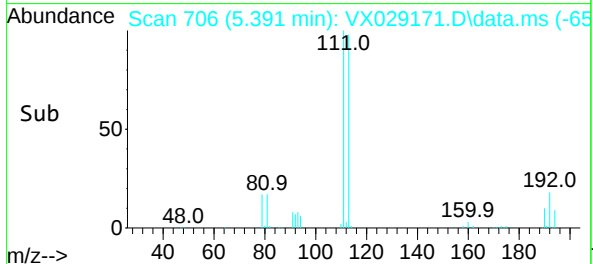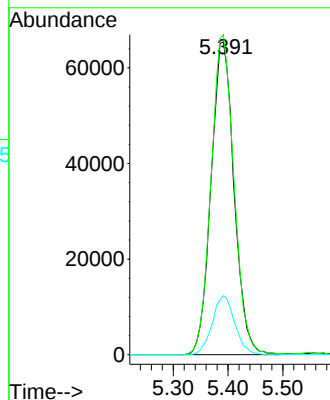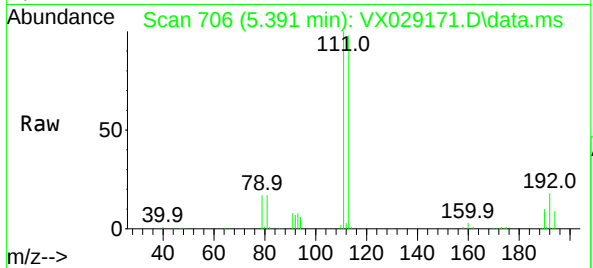

#37
Ethyl Acetate
Concen: 2.001 ug/l
RT: 4.727 min Scan# 597
Delta R.T. 0.012 min
Lab File: VX029171.D
Acq: 03 Jun 2022 06:18

Tgt Ion: 43 Resp: 9485
Ion Ratio Lower Upper
43 100
61 18.0 12.6 19.0
70 11.4 10.2 15.2


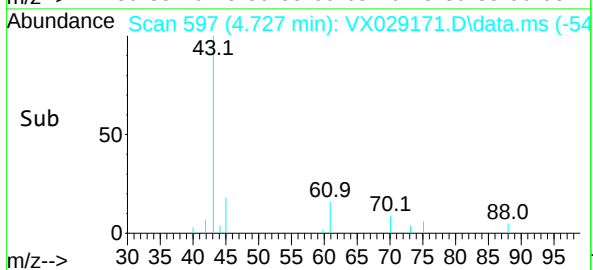
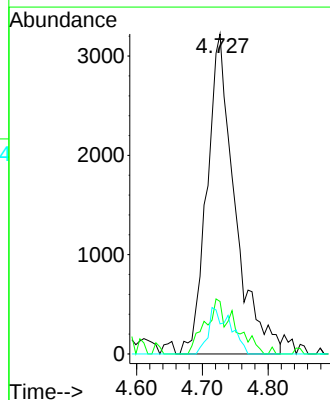
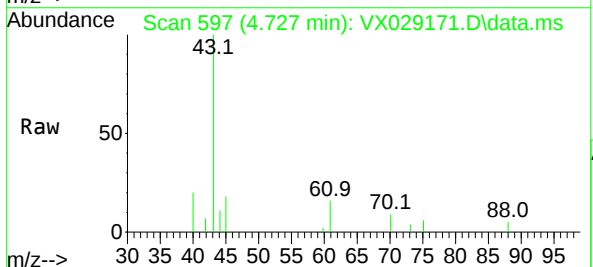


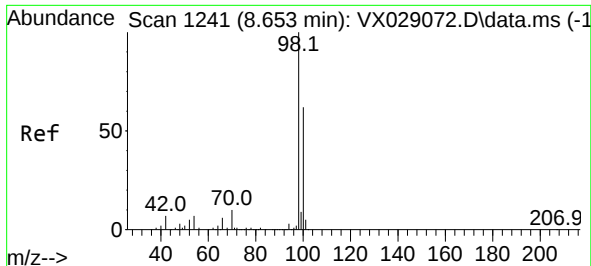

#50
Toluene-d8
Concen: 48.407 ug/l
RT: 8.653 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX029171.D
Acq: 03 Jun 2022 06:18




Instrument :
MSVOA_X
ClientSampleId :
34BR-20220531


Tgt Ion: 98 Resp: 673012
Ion Ratio Lower Upper
98 100
100 66.5 52.6 78.8

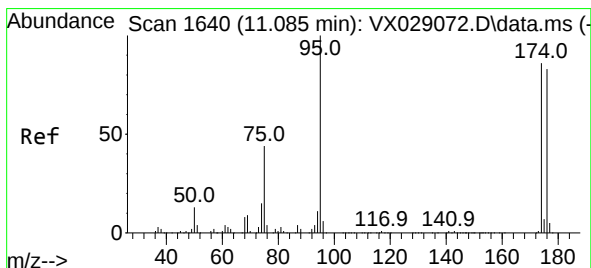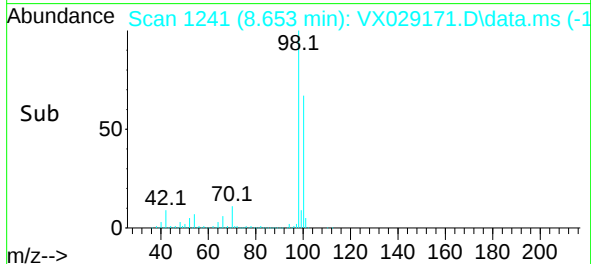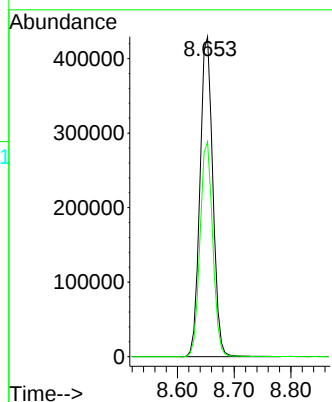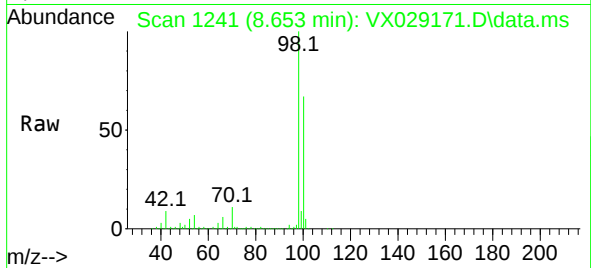

#62
4-Bromofluorobenzene
Concen: 49.432 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.006 min
Lab File: VX029171.D
Acq: 03 Jun 2022 06:18

Tgt Ion: 95 Resp: 265664
Ion Ratio Lower Upper
95 100
174 73.6 0.0 163.0
176 70.9 0.0 155.0


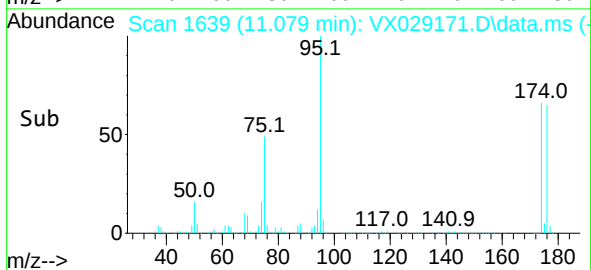
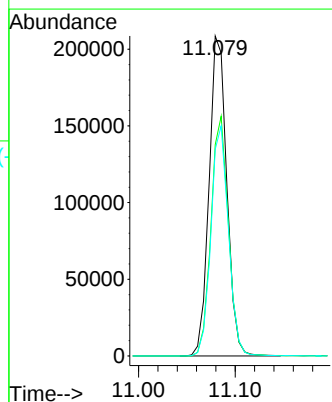
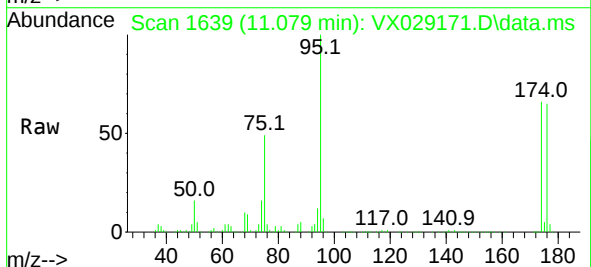


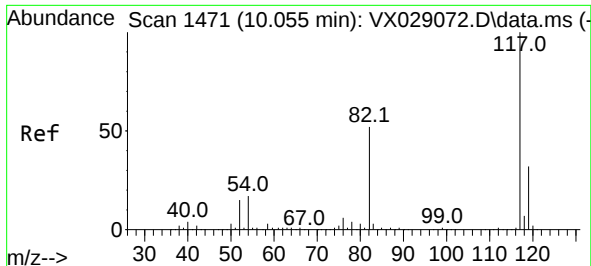

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX029171.D
Acq: 03 Jun 2022 06:18

Instrument :
MSVOA_X
ClientSampleId :
34BR-20220531

Tgt Ion:117 Resp: 554324
Ion Ratio Lower Upper
117 100
82 54.9 41.8 62.8
119 33.0 24.8 37.2

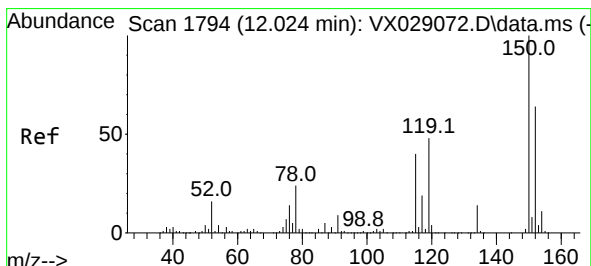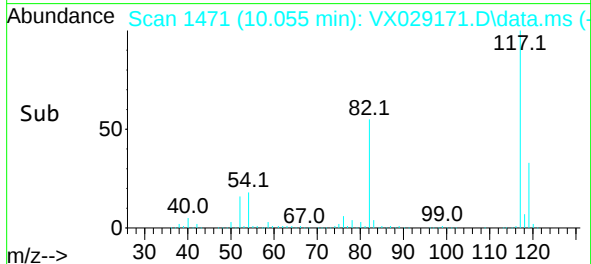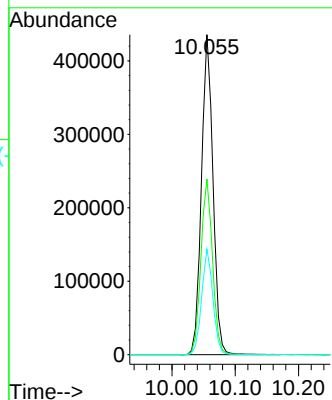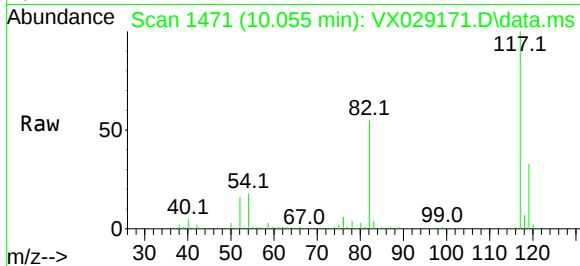

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX029171.D
Acq: 03 Jun 2022 06:18

Tgt Ion:152 Resp: 252214
Ion Ratio Lower Upper
152 100
115 63.9 37.5 112.7
150 157.7 0.0 338.2

