

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060222\
 Data File : VX029146.D
 Acq On : 02 Jun 2022 19:26
 Operator : JC/MD
 Sample : N3022-04 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 45BR-20220525

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
 Title : SW846 8260

Signal : TIC: VX029146.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.947	294	305	316	rBV	21718	50524	1.87%	0.411%
2	4.489	548	558	569	rBV	210157	580345	21.52%	4.723%
3	5.391	694	706	721	rBV	201031	583402	21.64%	4.748%
4	5.556	721	733	749	rVB	310357	878640	32.59%	7.151%
5	5.958	789	799	814	rBV	197482	531130	19.70%	4.322%
6	6.763	921	931	944	rBV	517787	1211885	44.94%	9.863%
7	7.129	979	991	1014	rBV	1260775	2696417	100.00%	21.944%
8	8.653	1233	1241	1255	rBV	1043540	1658203	61.50%	13.495%
9	10.055	1465	1471	1485	rBV	1120694	1512114	56.08%	12.306%
10	11.079	1634	1639	1652	rBV	871517	1145631	42.49%	9.323%
11	12.024	1788	1794	1802	rBV	1203362	1439306	53.38%	11.713%




Sum of corrected areas: 12287597

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060222\
Data File : VX029146.D
Acq On : 02 Jun 2022 19:26
Operator : JC/MD
Sample : N3022-04 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
45BR-20220525

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

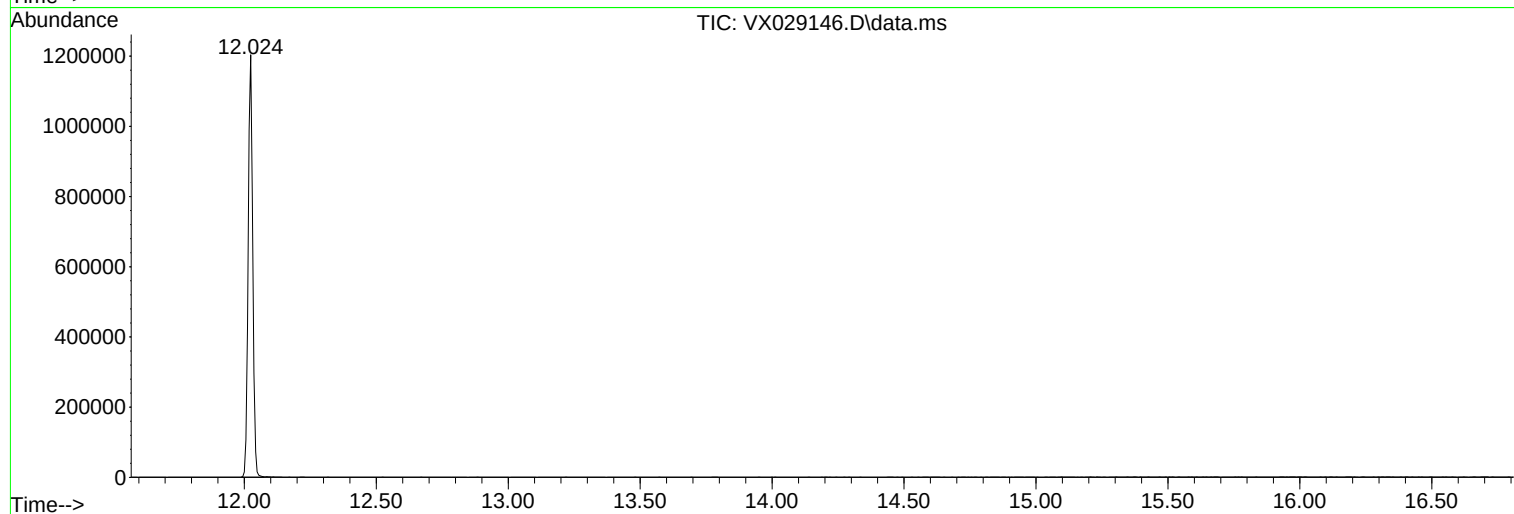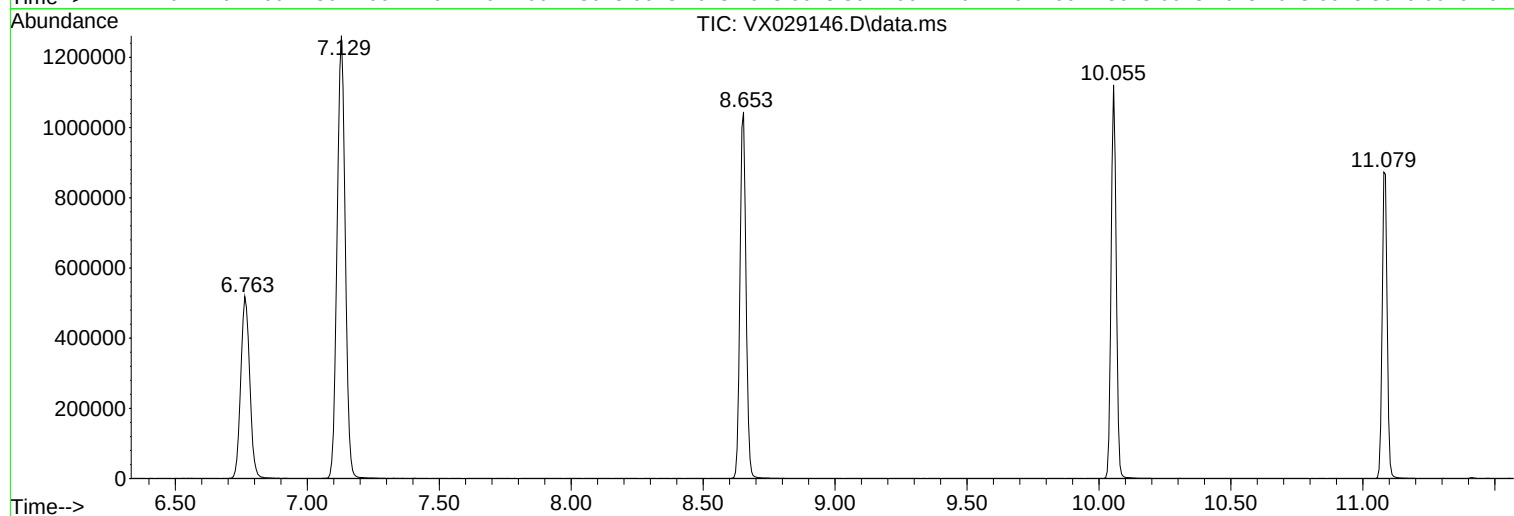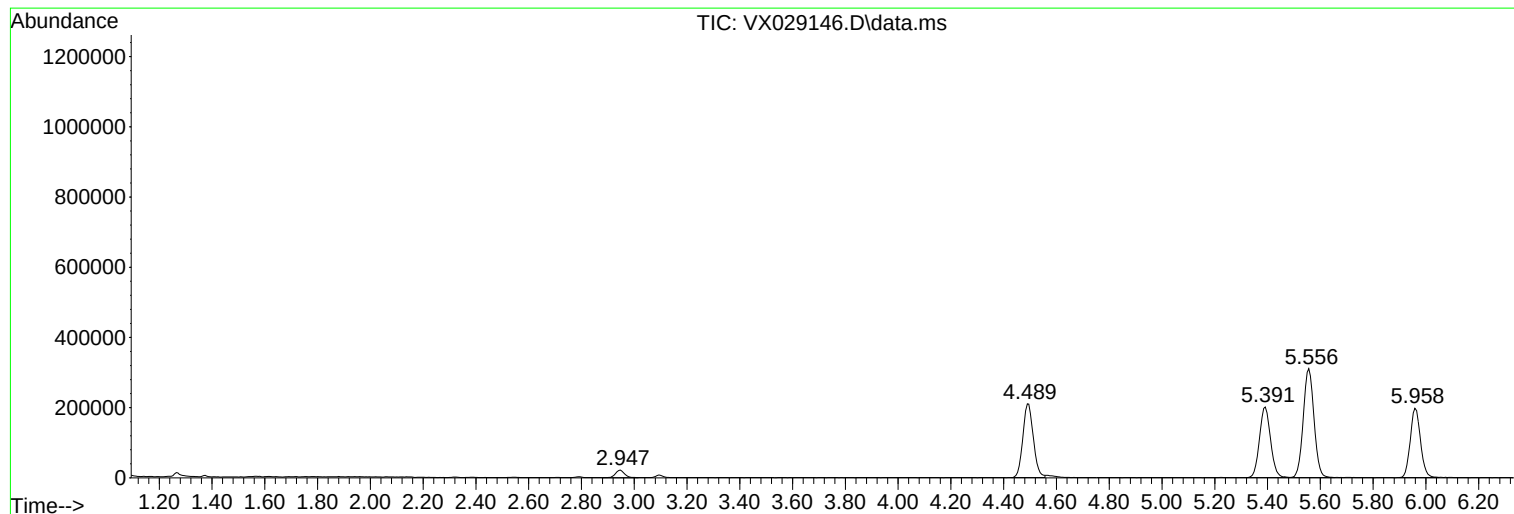

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060222\
Data File : VX029146.D
Acq On : 02 Jun 2022 19:26
Operator : JC/MD
Sample : N3022-04 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
45BR-20220525

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060222\
Data File : VX029146.D
Acq On : 02 Jun 2022 19:26
Operator : JC/MD
Sample : N3022-04 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
45BR-20220525

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------