

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060222\
 Data File : VX029175.D
 Acq On : 03 Jun 2022 07:51
 Operator : JC/MD
 Sample : N3164-15 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 38BR-20220531

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M

Title : SW846 8260

Signal : TIC: VX029175.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	54	rVB	30782	31012	1.75%	0.316%
2	2.947	296	305	319	rBV	57656	132445	7.48%	1.351%
3	4.562	562	570	585	rVB	10745	36410	2.06%	0.371%
4	5.391	693	706	721	rBV2	215158	626096	35.36%	6.386%
5	5.556	721	733	750	rVB	333080	937565	52.95%	9.563%
6	5.958	789	799	817	rBV	215805	570715	32.23%	5.821%
7	6.763	919	931	948	rBV	558049	1305842	73.75%	13.320%
8	8.653	1234	1241	1258	rBV	1114372	1770679	100.00%	18.061%
9	10.055	1465	1471	1485	rBV	1237033	1619670	91.47%	16.521%
10	11.079	1634	1639	1656	rBV	947695	1227516	69.32%	12.521%
11	12.024	1788	1794	1802	rBV	1259874	1545760	87.30%	15.767%




Sum of corrected areas: 9803710

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060222\
Data File : VX029175.D
Acq On : 03 Jun 2022 07:51
Operator : JC/MD
Sample : N3164-15 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
38BR-20220531

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

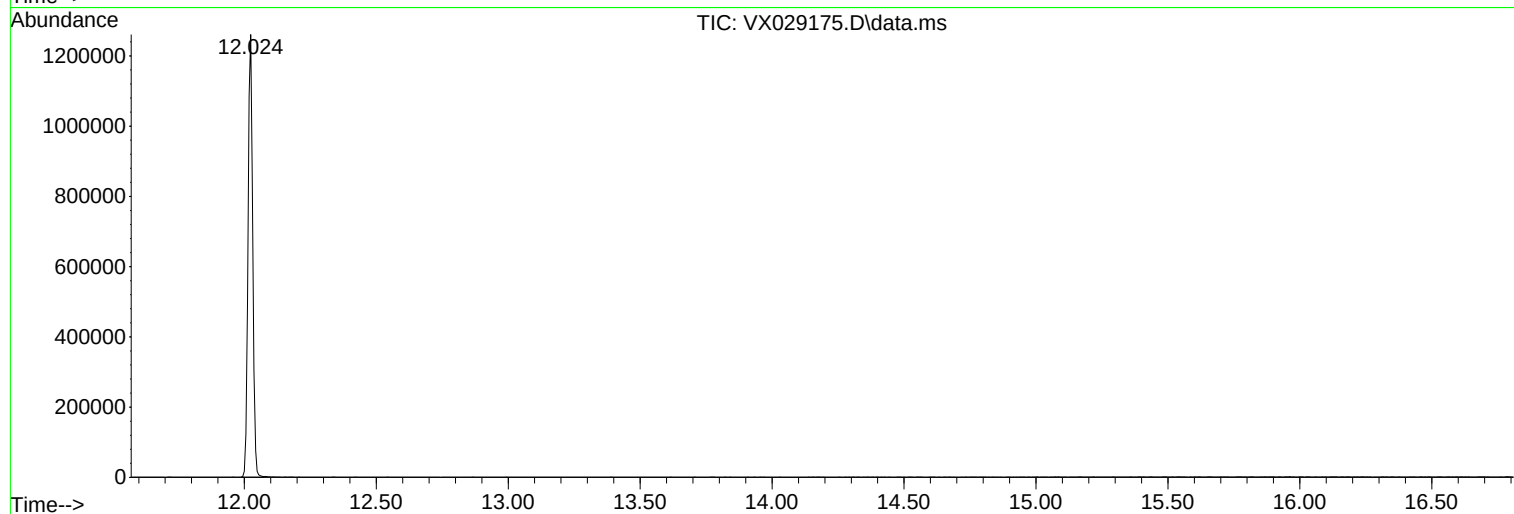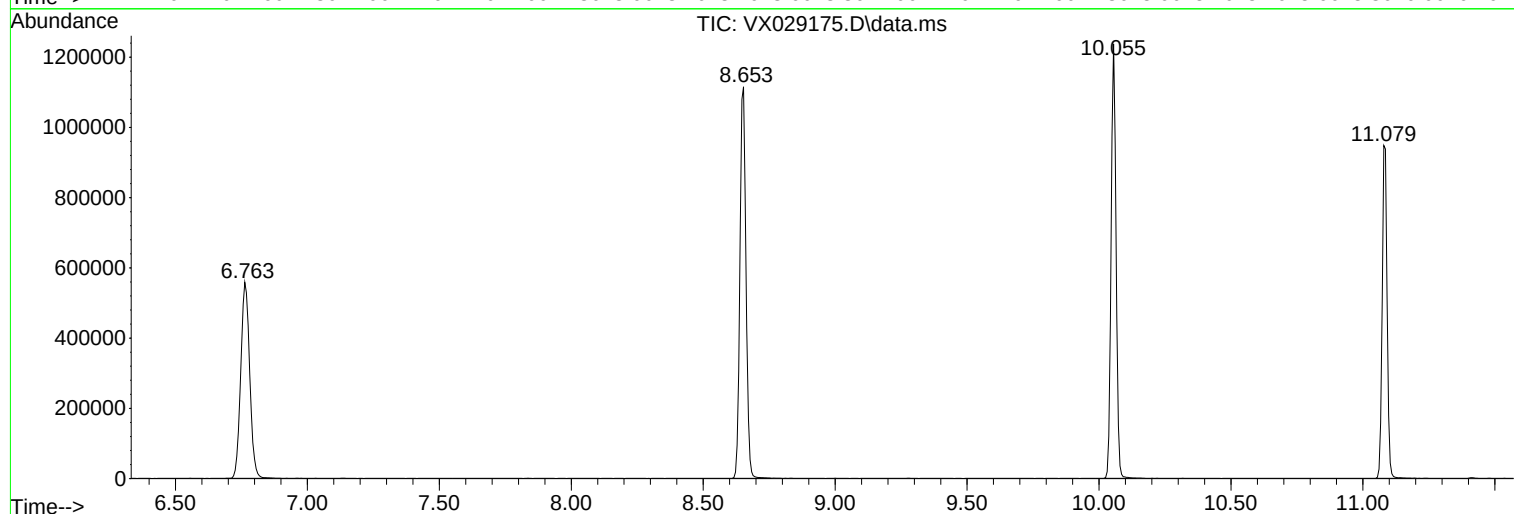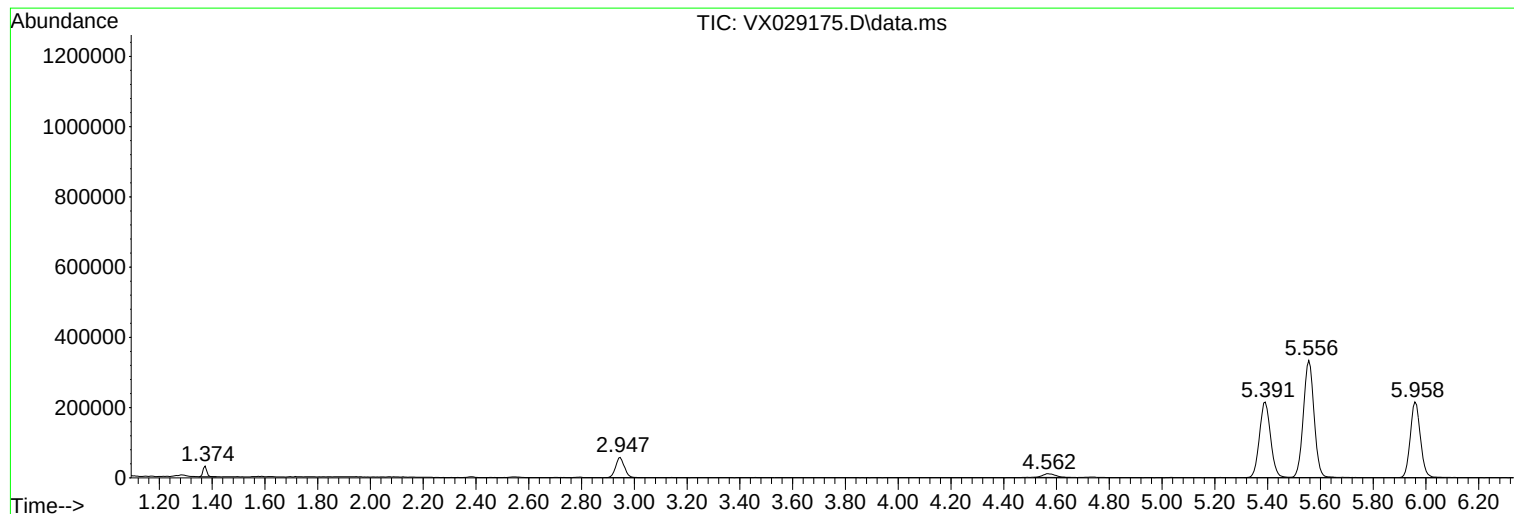

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060222\
Data File : VX029175.D
Acq On : 03 Jun 2022 07:51
Operator : JC/MD
Sample : N3164-15 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
38BR-20220531

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060222\
Data File : VX029175.D
Acq On : 03 Jun 2022 07:51
Operator : JC/MD
Sample : N3164-15 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
38BR-20220531

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------