

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060222\
 Data File : VX029176.D
 Acq On : 03 Jun 2022 08:15
 Operator : JC/MD
 Sample : N3164-16 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 39BR-20220531

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M

Title : SW846 8260

Signal : TIC: VX029176.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.270	25	30	45	rVB3	8901	24609	1.38%	0.249%
2	2.946	296	305	316	rBV	66757	150828	8.44%	1.523%
3	4.568	558	571	585	rBV	15040	51017	2.86%	0.515%
4	5.391	693	706	721	rBV	216146	626719	35.09%	6.330%
5	5.556	721	733	749	rVB	330905	934225	52.31%	9.436%
6	5.958	787	799	814	rBV	209839	568036	31.80%	5.738%
7	6.763	919	931	947	rBV	545005	1308129	73.24%	13.213%
8	8.653	1233	1241	1258	rBV	1144426	1786071	100.00%	18.041%
9	10.055	1465	1471	1482	rBV	1230747	1633048	91.43%	16.495%
10	11.085	1634	1640	1654	rBV	932813	1240621	69.46%	12.531%
11	12.024	1788	1794	1803	rBV	1315565	1576866	88.29%	15.928%




Sum of corrected areas: 9900169

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060222\
Data File : VX029176.D
Acq On : 03 Jun 2022 08:15
Operator : JC/MD
Sample : N3164-16 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
39BR-20220531

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

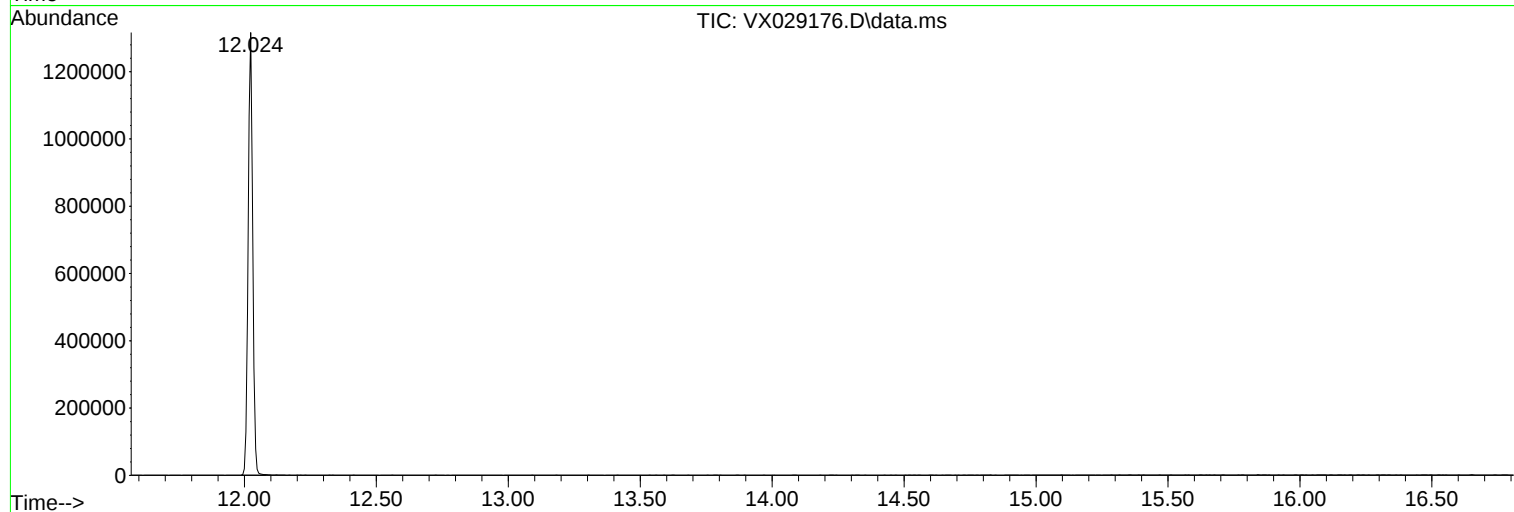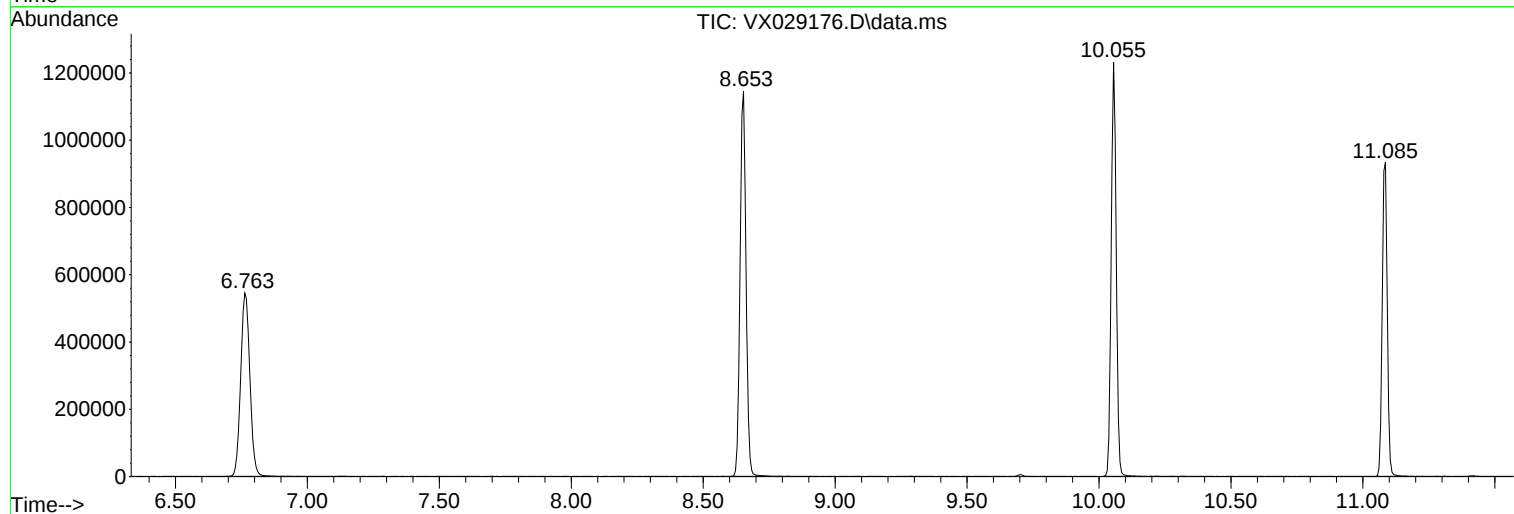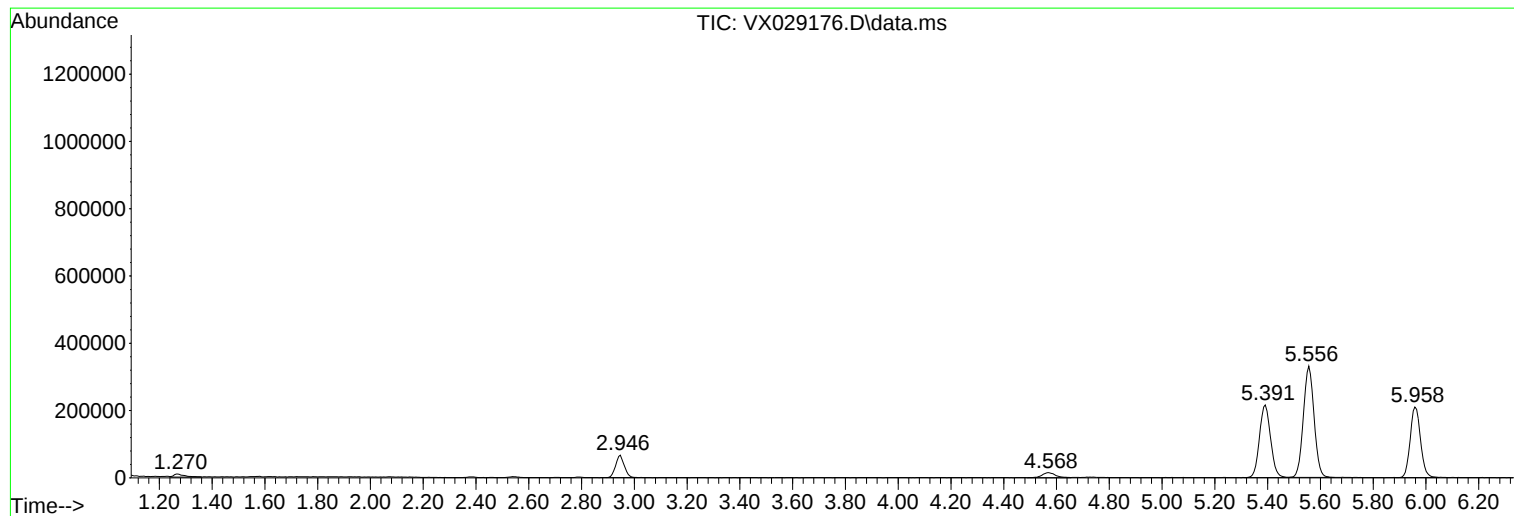

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060222\
Data File : VX029176.D
Acq On : 03 Jun 2022 08:15
Operator : JC/MD
Sample : N3164-16 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
39BR-20220531

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060222\
Data File : VX029176.D
Acq On : 03 Jun 2022 08:15
Operator : JC/MD
Sample : N3164-16 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
39BR-20220531

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------