

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060222\
 Data File : VX029177.D
 Acq On : 03 Jun 2022 08:38
 Operator : JC/MD
 Sample : N3164-17 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 40BR-20220531

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M

Title : SW846 8260

Signal : TIC: VX029177.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.946	295	305	316	rBV	65885	156121	9.03%	1.612%
2	4.495	550	559	565	rBV3	20557	57496	3.33%	0.594%
3	4.568	565	571	585	rVV	12699	44900	2.60%	0.463%
4	5.391	694	706	721	rBV2	209652	614034	35.53%	6.339%
5	5.556	721	733	748	rVB	321016	908900	52.60%	9.382%
6	5.958	789	799	815	rBV	210775	557605	32.27%	5.756%
7	6.763	921	931	947	rBV	527569	1272220	73.62%	13.133%
8	8.653	1234	1241	1255	rBV	1081208	1727983	100.00%	17.838%
9	10.055	1465	1471	1487	rBV	1210047	1596552	92.39%	16.481%
10	11.085	1634	1640	1650	rBV	931541	1206747	69.84%	12.457%
11	12.024	1788	1794	1808	rBV	1252940	1544734	89.40%	15.946%




Sum of corrected areas: 9687292

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060222\
Data File : VX029177.D
Acq On : 03 Jun 2022 08:38
Operator : JC/MD
Sample : N3164-17 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
40BR-20220531

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

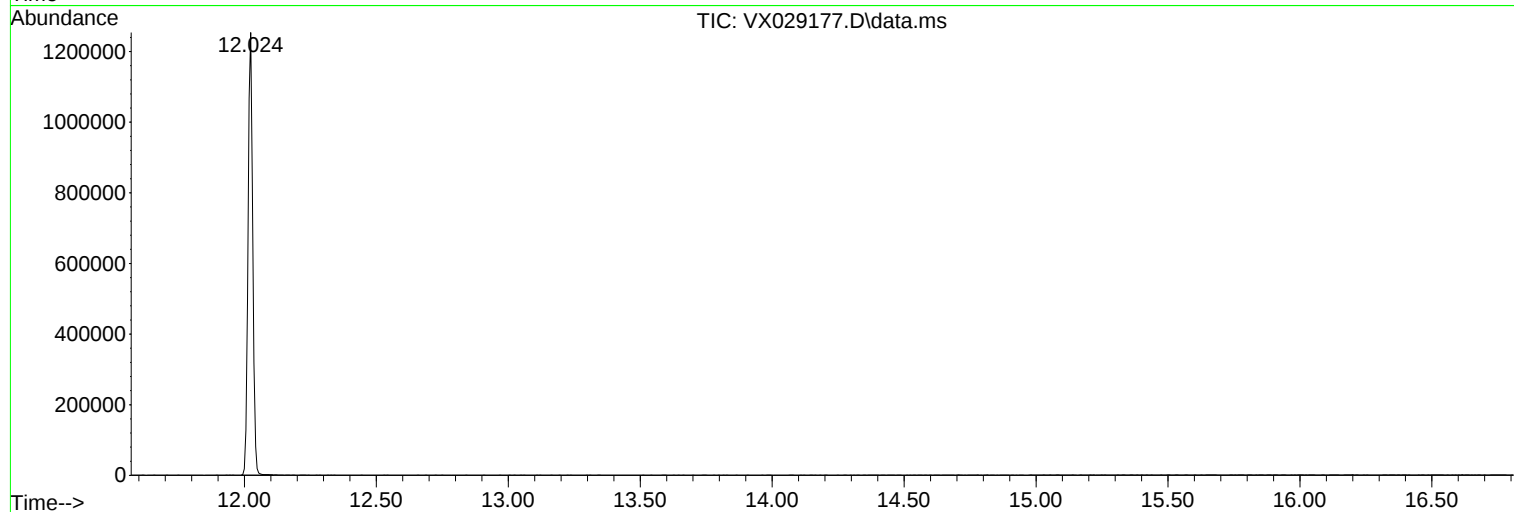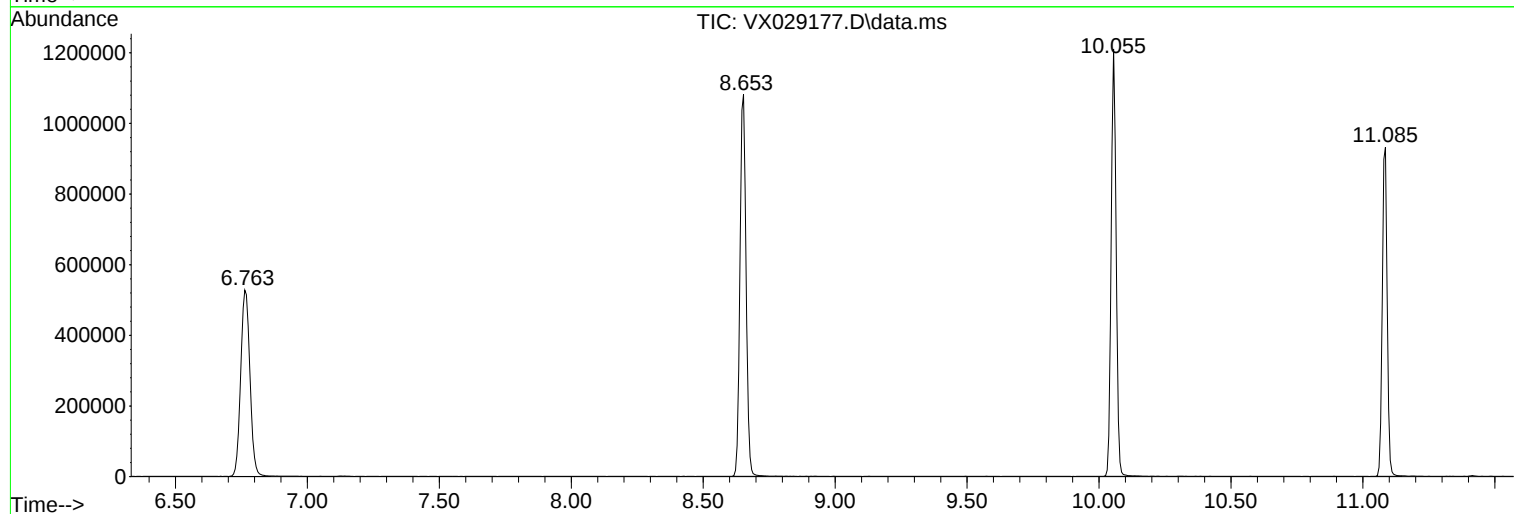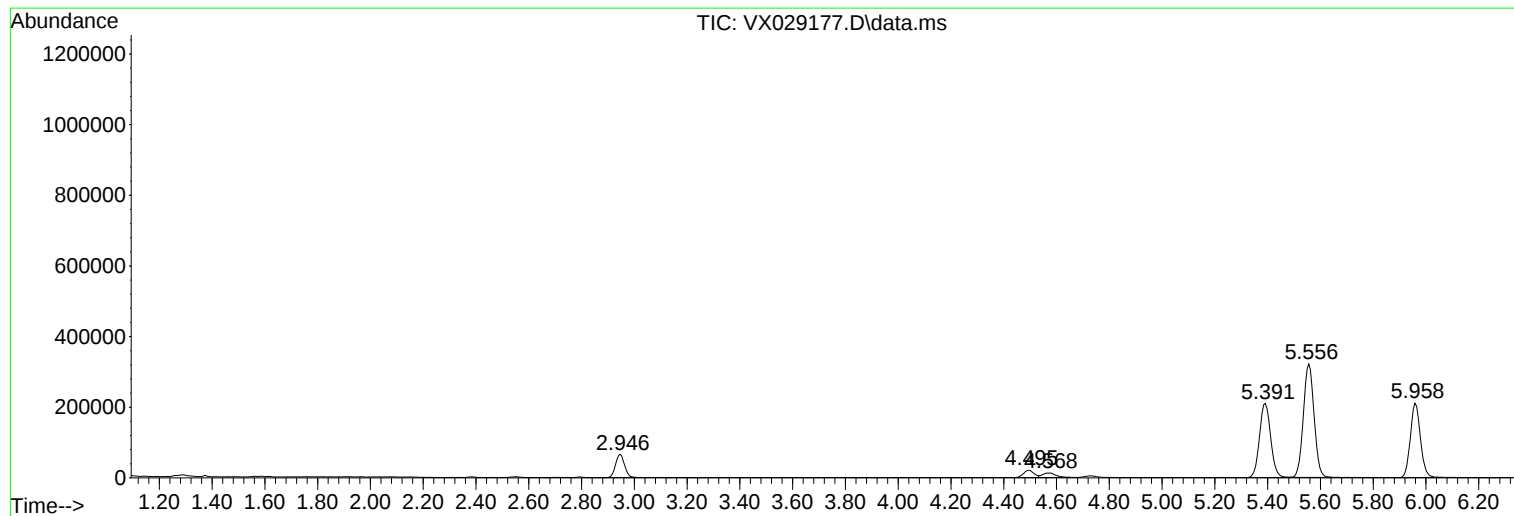

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060222\
Data File : VX029177.D
Acq On : 03 Jun 2022 08:38
Operator : JC/MD
Sample : N3164-17 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
40BR-20220531

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060222\
Data File : VX029177.D
Acq On : 03 Jun 2022 08:38
Operator : JC/MD
Sample : N3164-17 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
40BR-20220531

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------