
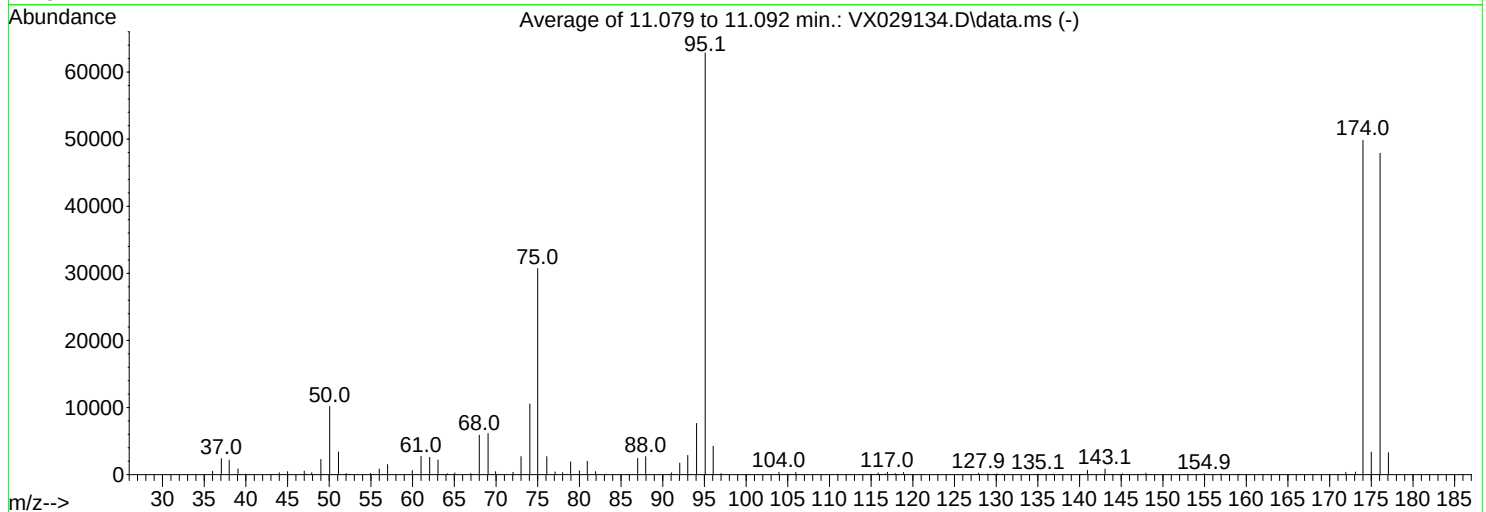


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060222\
Data File : VX029134.D
Acq On : 02 Jun 2022 14:31
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
Title : SW846 8260
Last Update : Wed Jun 01 04:45:42 2022

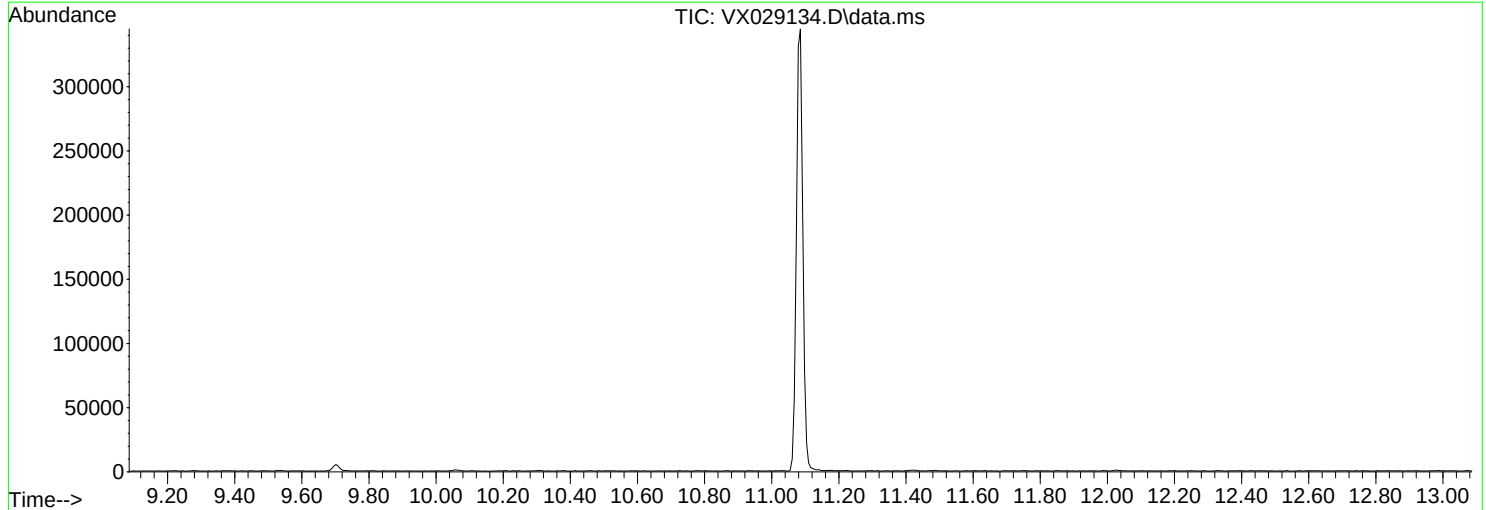

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	10164	PASS
75	95	30	60	48.9	30723	PASS
95	95	100	100	100.0	62864	PASS
96	95	5	9	6.8	4249	PASS
173	174	0.00	2	0.8	375	PASS
174	95	50	100	79.2	49819	PASS
175	174	5	9	6.7	3354	PASS
176	174	95	101	96.2	47909	PASS
177	176	5	9	6.8	3276	PASS