
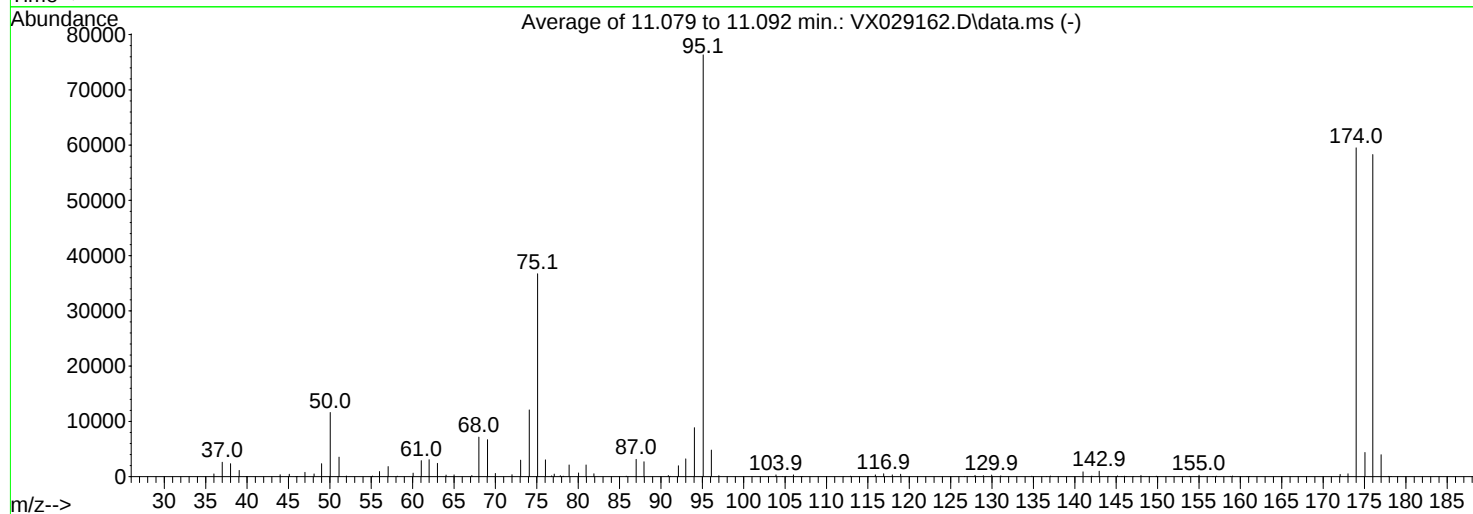


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060222\
Data File : VX029162.D
Acq On : 03 Jun 2022 02:25
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
Title : SW846 8260
Last Update : Wed Jun 01 04:45:42 2022

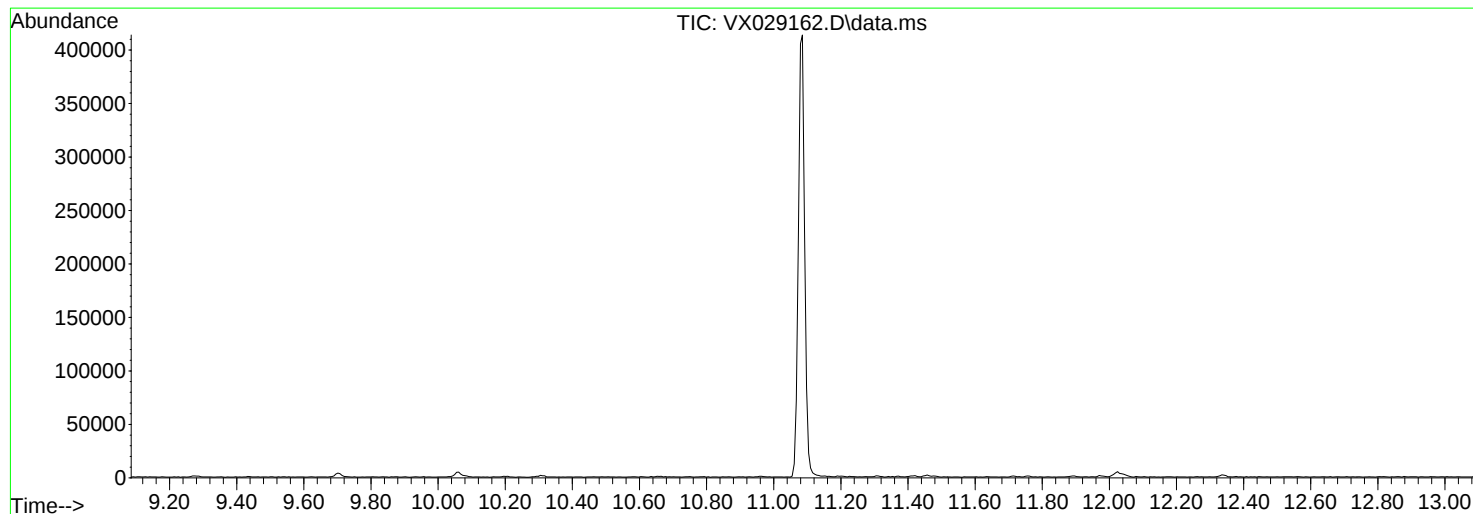

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.2	11624	PASS
75	95	30	60	48.1	36725	PASS
95	95	100	100	100.0	76339	PASS
96	95	5	9	6.3	4808	PASS
173	174	0.00	2	0.9	531	PASS
174	95	50	100	78.0	59515	PASS
175	174	5	9	7.3	4371	PASS
176	174	95	101	98.0	58299	PASS
177	176	5	9	6.8	3956	PASS