

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060223\
 Data File : VX035980.D
 Acq On : 02 Jun 2023 13:44
 Operator : JC/MD
 Sample : 03022-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BP-VPB-RW11-GW-578-580

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053123W.M

Title : SW846 8260

Signal : TIC: VX035980.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	5	9	18	rVB2	14939	17560	1.49%	0.272%
2	2.398	207	215	223	rBV	7305	15362	1.30%	0.238%
3	4.587	562	574	587	rBV3	5790	21483	1.82%	0.332%
4	5.385	693	705	720	rBV2	126333	373920	31.76%	5.786%
5	5.550	720	732	746	rVV	266653	745268	63.29%	11.532%
6	5.958	786	799	813	rBV	156277	421229	35.77%	6.518%
7	6.763	919	931	945	rBV	377868	906257	76.97%	14.023%
8	8.647	1233	1240	1250	rBV	741012	1177486	100.00%	18.220%
9	10.055	1465	1471	1485	rBV	761011	1031626	87.61%	15.963%
10	11.079	1634	1639	1653	rVB	611973	771791	65.55%	11.943%
11	12.024	1788	1794	1803	rBV	744444	980444	83.27%	15.171%




Sum of corrected areas: 6462426

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060223\
Data File : VX035980.D
Acq On : 02 Jun 2023 13:44
Operator : JC/MD
Sample : 03022-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-RW11-GW-578-580

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

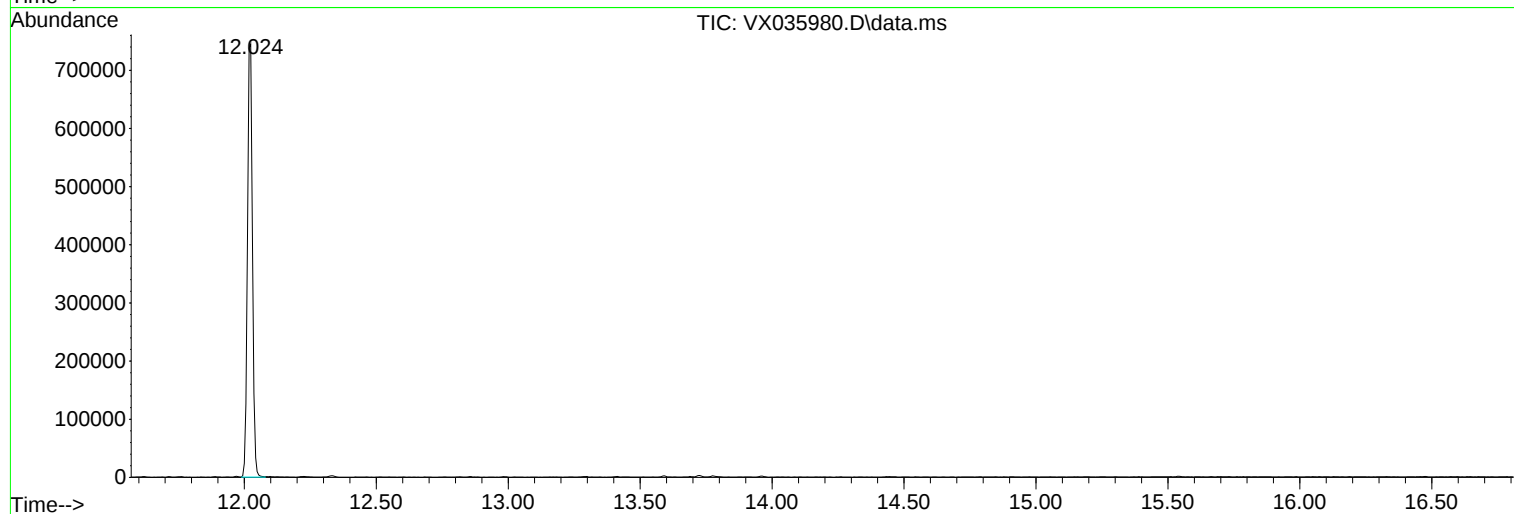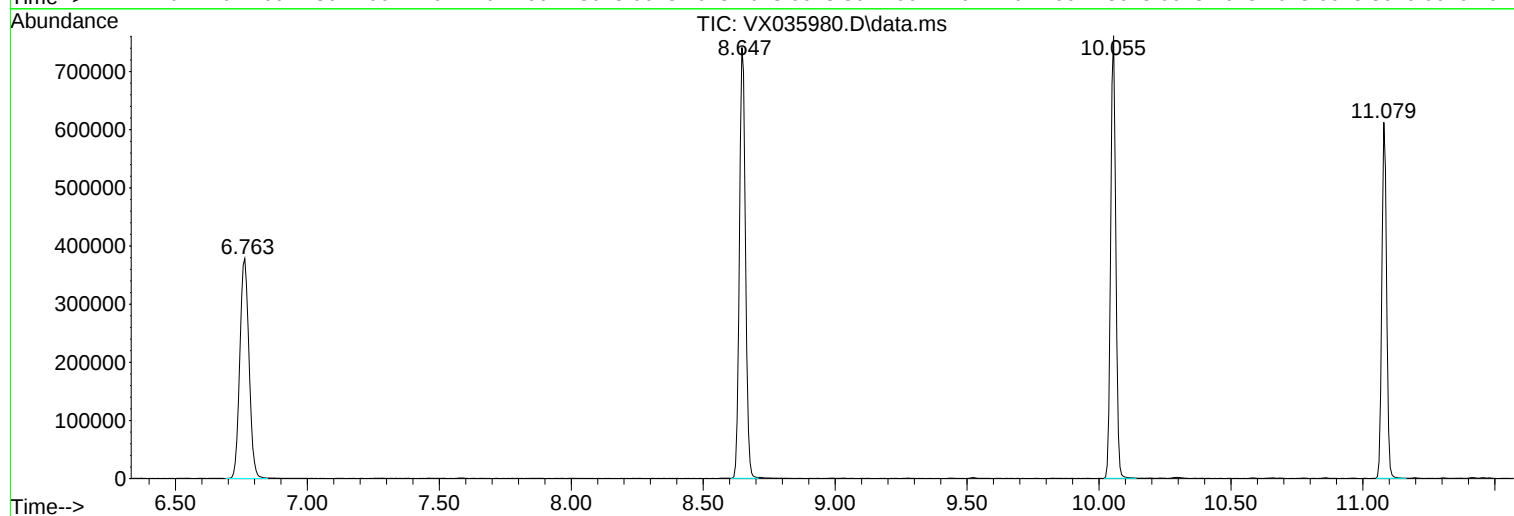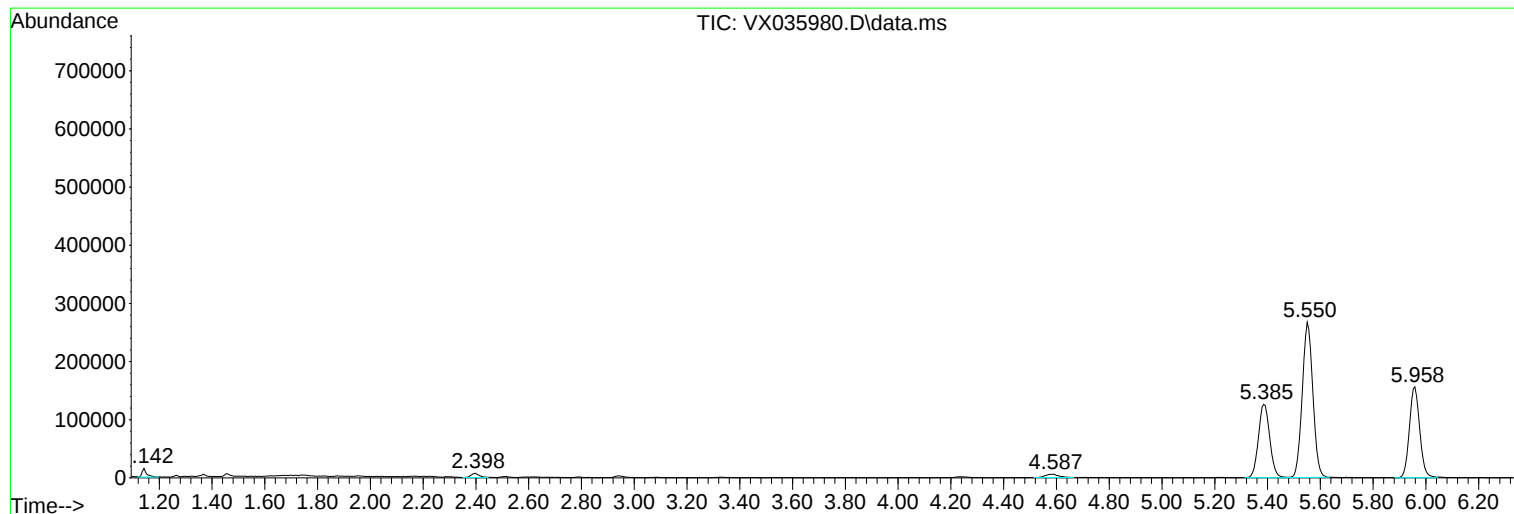

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060223\
Data File : VX035980.D
Acq On : 02 Jun 2023 13:44
Operator : JC/MD
Sample : 03022-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-RW11-GW-578-580

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060223\
Data File : VX035980.D
Acq On : 02 Jun 2023 13:44
Operator : JC/MD
Sample : 03022-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BP-VPB-RW11-GW-578-580

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053123W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc