



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX060223\  
Data File : VX035969.D  
Acq On : 02 Jun 2023 08:36  
Operator : JC/MD  
Sample : BFB  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X053123W.M  
Title : SW846 8260  
Last Update : Wed May 31 12:50:30 2023

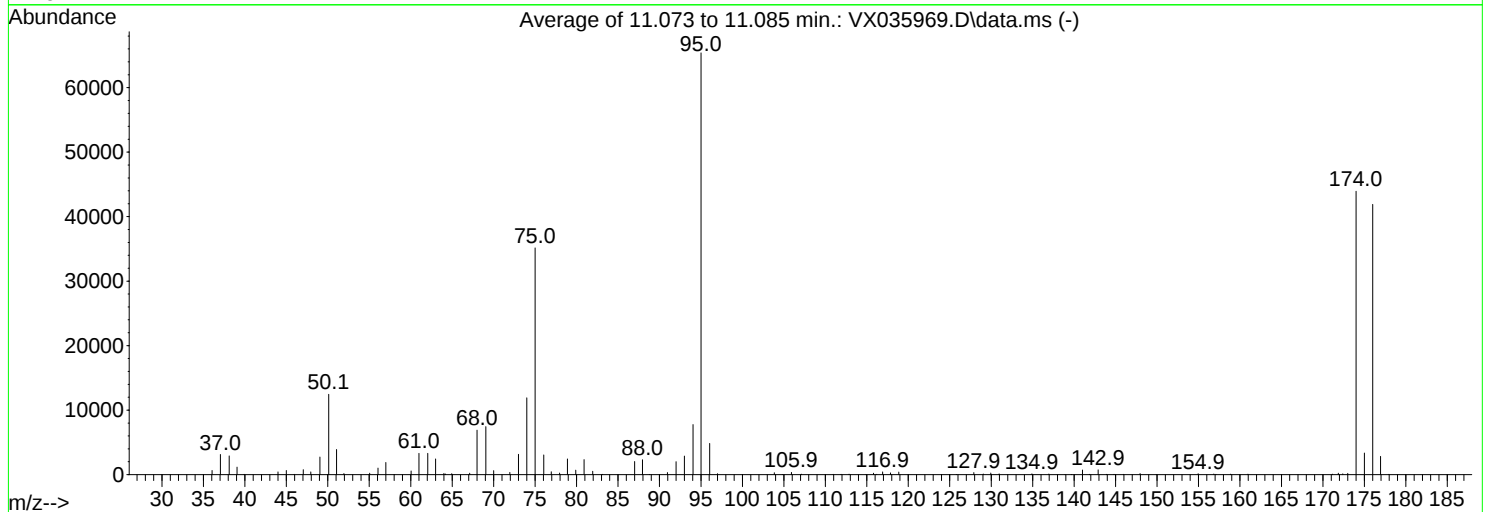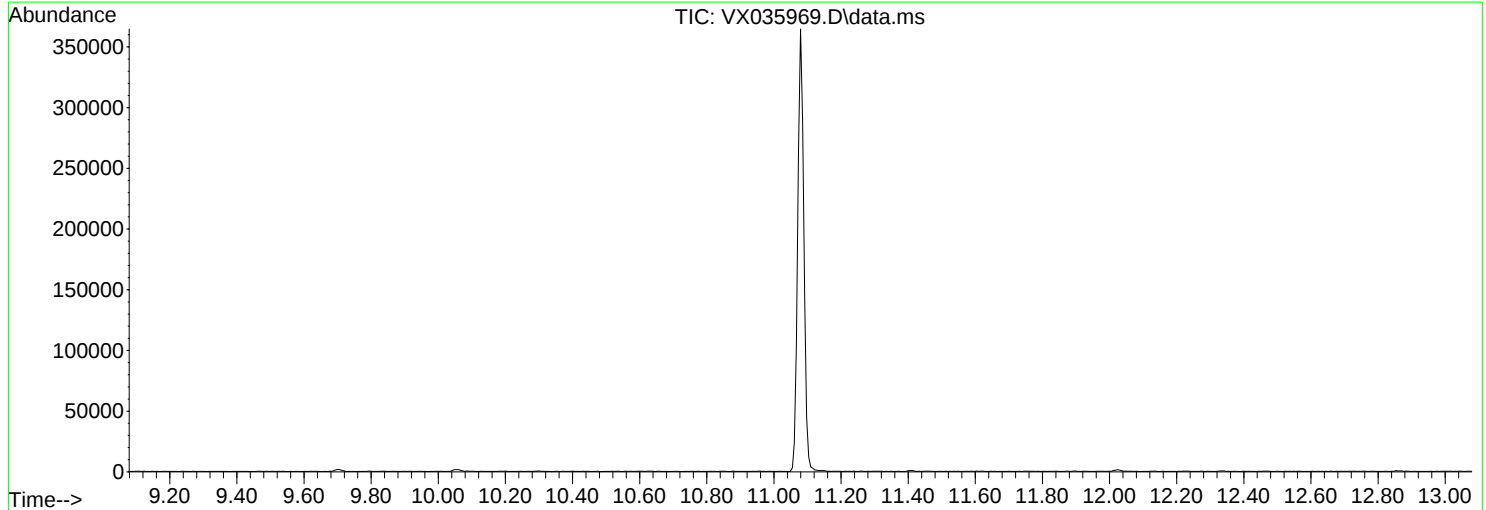

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 19.1         | 12467      | PASS                |
| 75             | 95              | 30              | 60              | 53.8         | 35157      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 65392      | PASS                |
| 96             | 95              | 5               | 9               | 7.4          | 4838       | PASS                |
| 173            | 174             | 0.00            | 2               | 0.4          | 196        | PASS                |
| 174            | 95              | 50              | 100             | 67.2         | 43920      | PASS                |
| 175            | 174             | 5               | 9               | 7.6          | 3343       | PASS                |
| 176            | 174             | 95              | 101             | 95.4         | 41888      | PASS                |
| 177            | 176             | 5               | 9               | 6.8          | 2837       | PASS                |