

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060225\
 Data File : VX046453.D
 Acq On : 02 Jun 2025 18:42
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 IBLK

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X050525W.M
 Title : SW846 8260

Signal : TIC: VX046453.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.593	76	83	88	rVB5	5420	12860	2.71%	0.467%
2	3.440	379	386	393	rVB4	2184	4948	1.04%	0.180%
3	5.379	694	704	718	rBV	52926	157693	33.25%	5.729%
4	5.544	720	731	747	rVV	75561	220961	46.59%	8.028%
5	5.952	787	798	816	rBV	61552	170442	35.94%	6.193%
6	6.757	921	930	953	rBV	140155	340886	71.88%	12.385%
7	8.647	1233	1240	1253	rBV	305220	474273	100.00%	17.232%
8	10.049	1465	1470	1483	rBV	310733	437294	92.20%	15.888%
9	11.079	1633	1639	1652	rBV	258961	350228	73.85%	12.725%
10	12.018	1788	1793	1802	rBV	311496	391619	82.57%	14.229%
11	13.457	2020	2029	2031	rBV8	13124	38323	8.08%	1.392%
12	14.164	2143	2145	2148	rBV4	5308	7035	1.48%	0.256%
13	14.621	2216	2220	2230	rVB5	14811	38363	8.09%	1.394%
14	15.207	2313	2316	2321	rVB2	10075	13898	2.93%	0.505%
15	15.487	2357	2362	2368	rVB4	12981	21819	4.60%	0.793%
16	15.743	2400	2404	2409	rBV7	3787	7437	1.57%	0.270%
17	16.084	2457	2460	2466	rVB8	4901	7958	1.68%	0.289%
18	16.371	2500	2507	2514	rVB4	13835	32310	6.81%	1.174%
19	16.597	2540	2544	2548	rVB6	6971	12411	2.62%	0.451%
20	16.651	2549	2553	2558	rBV4	6697	11582	2.44%	0.421%




Sum of corrected areas: 2752340

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060225\
Data File : VX046453.D
Acq On : 02 Jun 2025 18:42
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X050525W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

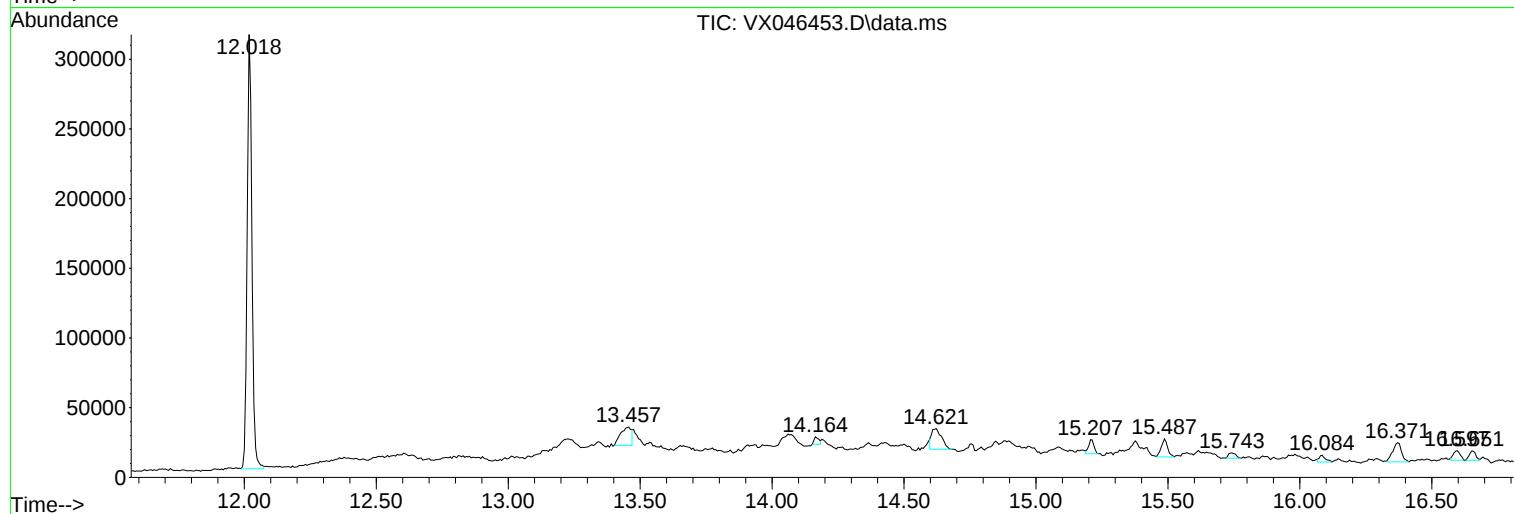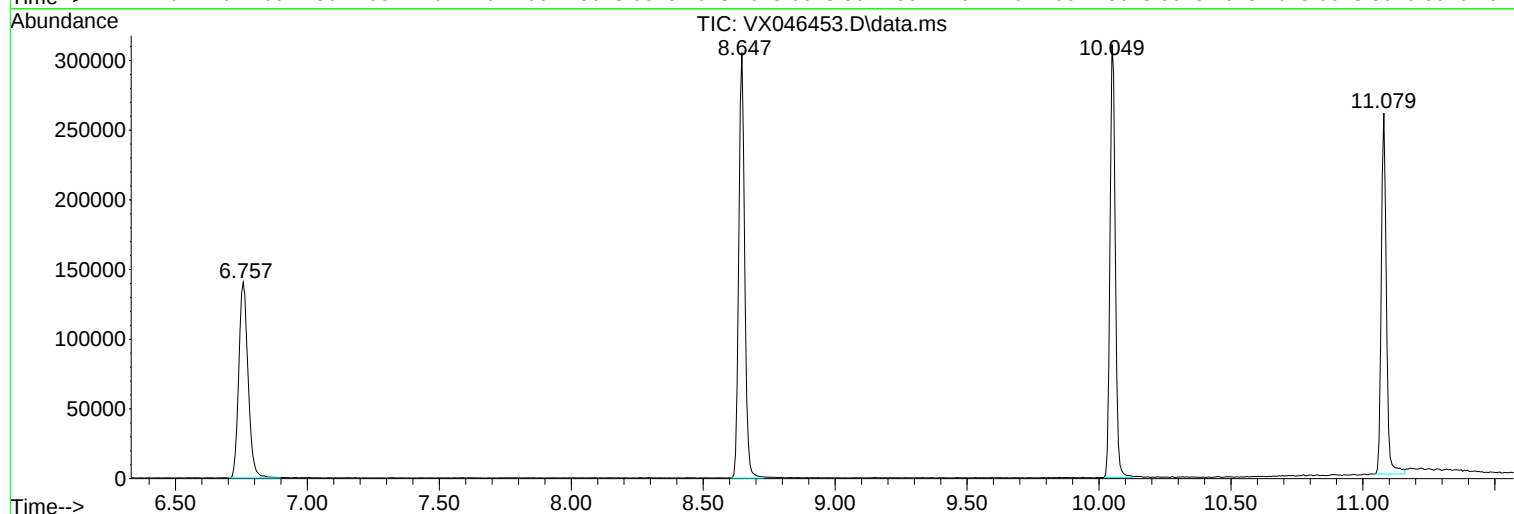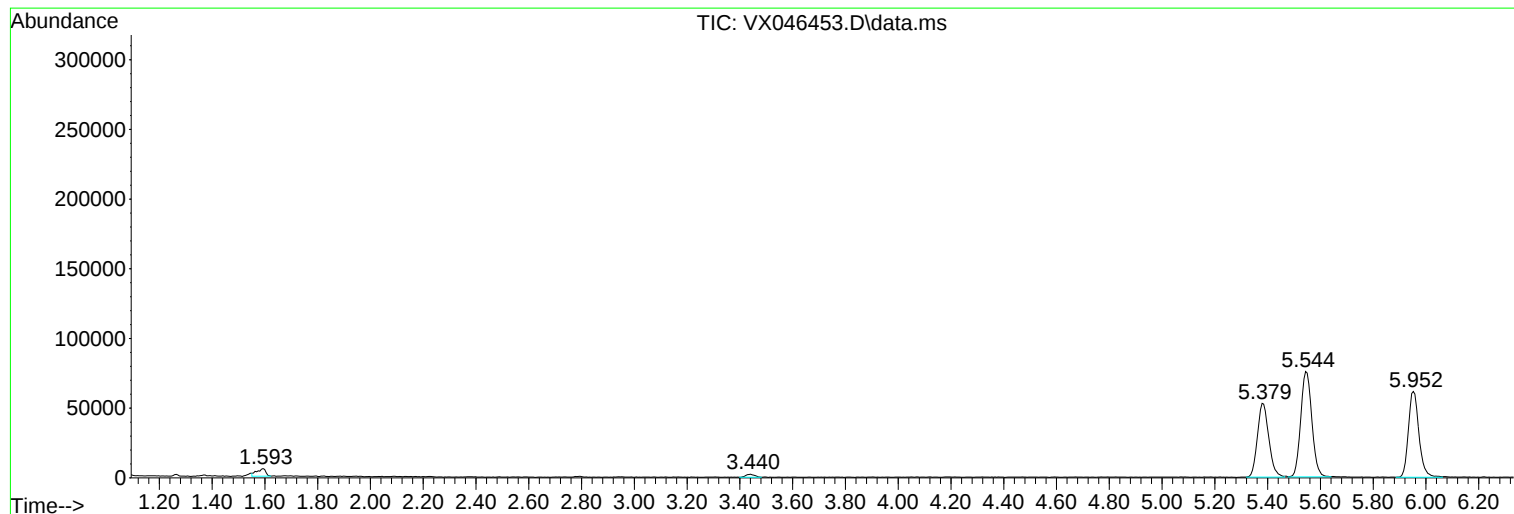

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060225\
Data File : VX046453.D
Acq On : 02 Jun 2025 18:42
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X050525W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060225\
Data File : VX046453.D
Acq On : 02 Jun 2025 18:42
Operator : JC/MD
Sample : IBLK
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
IBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X050525W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------