

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX060320\
 Data File : VX016561.D
 Acq On : 03 Jun 2020 12:33
 Operator : JC/SP
 Sample : L2866-01
 Misc : 5.0mL/MSVOA X/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 TB-01-200602

Quant Time: Jun 04 08:52:28 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X052720W.M
 Quant Title : SW846 8260
 QLast Update : Wed May 27 16:31:05 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.63	168	284782	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	6.83	114	455901	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.10	117	447565	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.06	152	215245	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.03	65	162363	45.91	ug/l	0.00
Spiked Amount	50.000		Recovery	=	91.82%	
35) Dibromofluoromethane	5.46	113	130535	46.50	ug/l	0.00
Spiked Amount	50.000		Recovery	=	93.00%	
50) Toluene-d8	8.70	98	565968	51.80	ug/l	0.00
Spiked Amount	50.000		Recovery	=	103.60%	
62) 4-Bromofluorobenzene	11.12	95	223222	52.87	ug/l	0.00
Spiked Amount	50.000		Recovery	=	105.74%	


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX060320\
Data File : VX016561.D
Acq On : 03 Jun 2020 12:33
Operator : JC/SP
Sample : L2866-01
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
TB-01-200602

Quant Time: Jun 04 08:52:28 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X052720W.M
Quant Title : SW846 8260
QLast Update : Wed May 27 16:31:05 2020
Response via : Initial Calibration

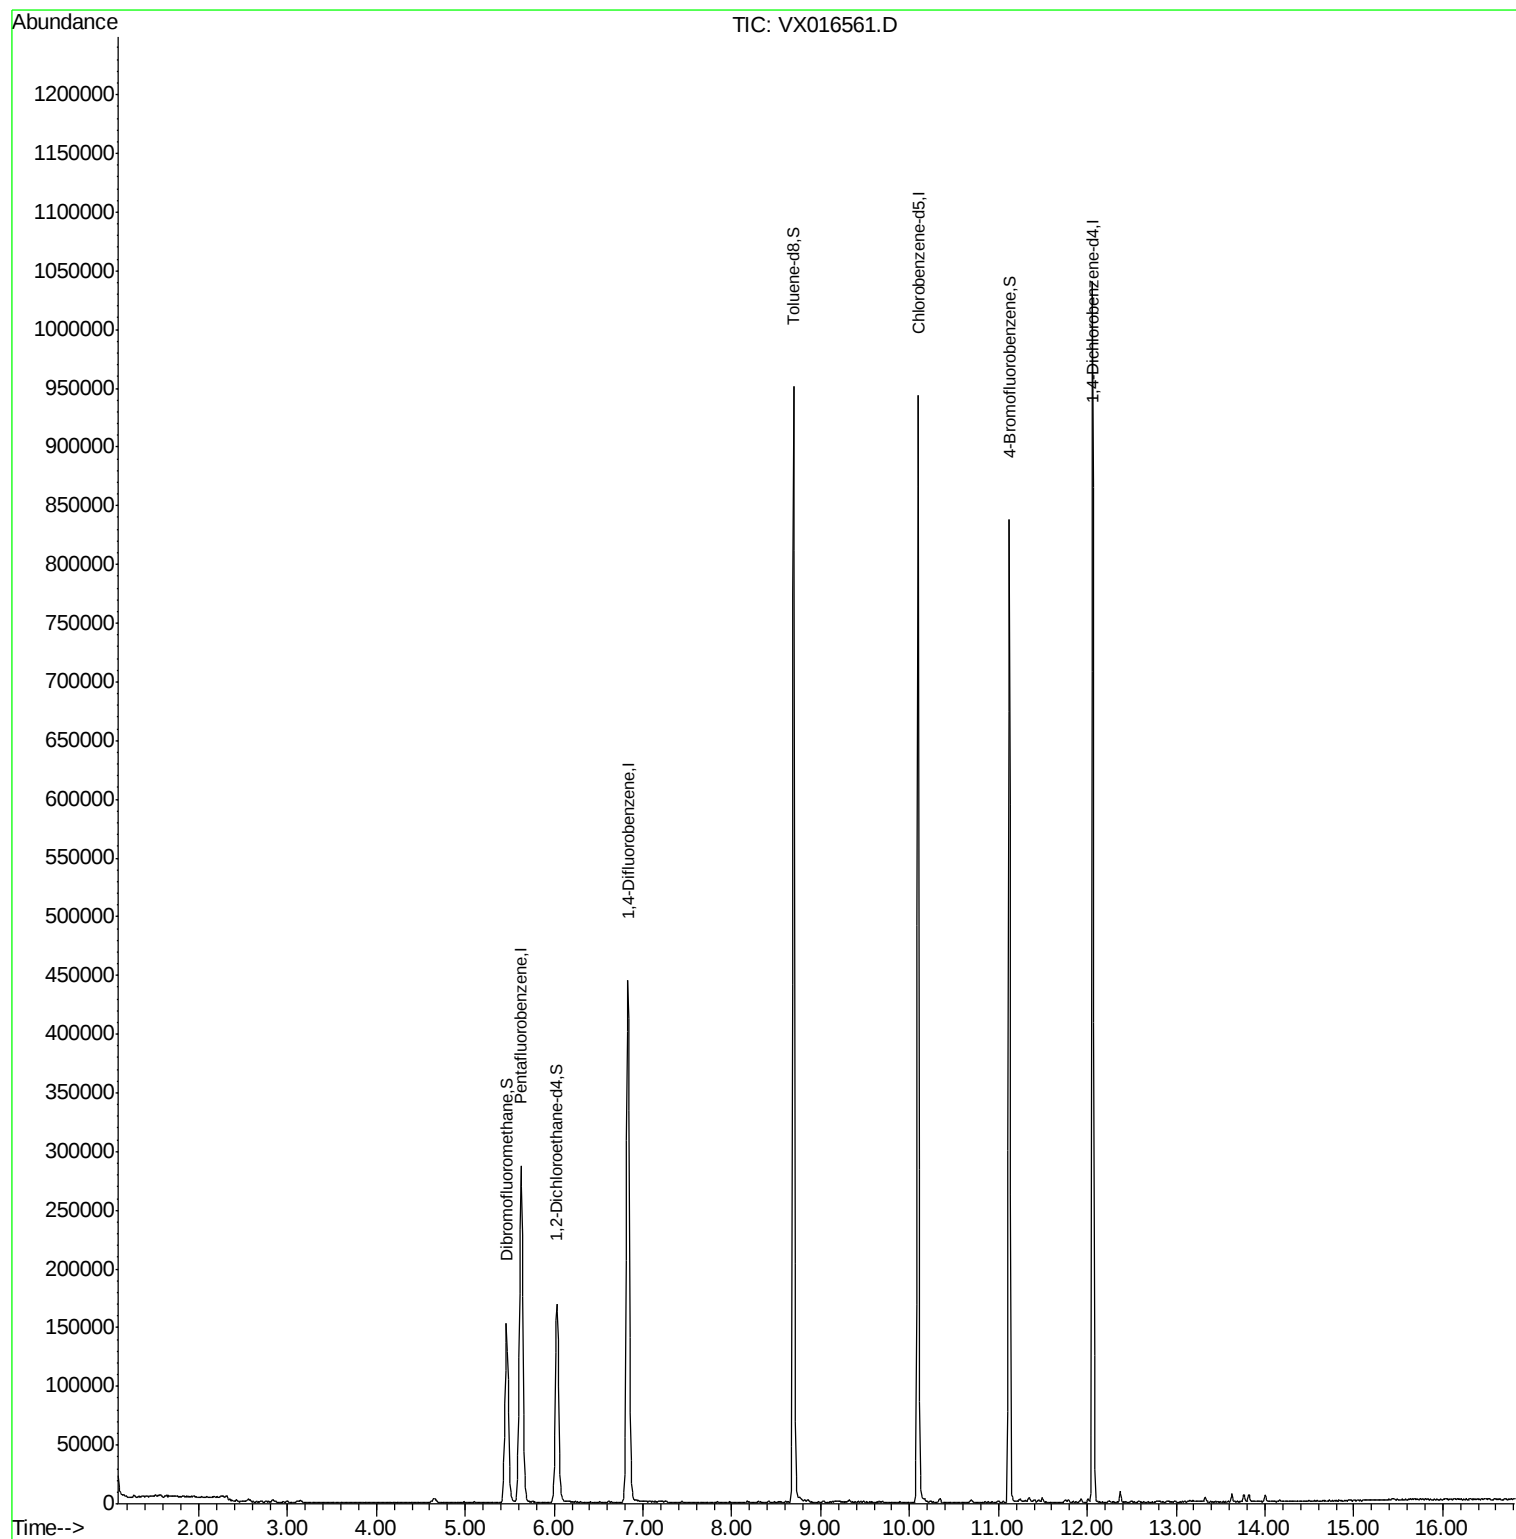



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.63 min Scan# 745

Delta R.T. -0.00 min

Lab File: VX016561.D

Acq: 03 Jun 2020 12:33

Instrument :

MSVOA_X

ClientSampleId :


TB-01-200602

Tot Ion:168 Resp: 284782

Ion Ratio Lower Upper

168 100

99 55.8 45.2 67.8



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VX0

5.63

100000

80000



60000

40000

20000

0

Time-->

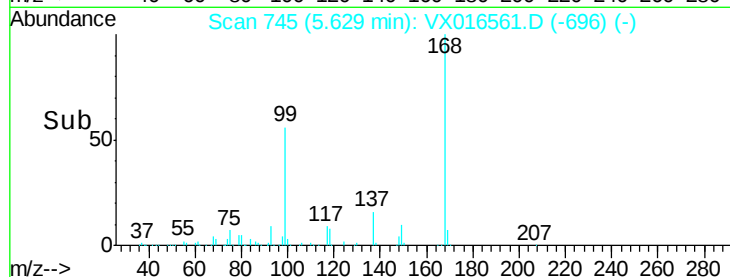

#33

1,2-Dichloroethane-d4

Concen: 45.909 ug/l

RT: 6.03 min Scan# 811

Delta R.T. -0.00 min

Lab File: VX016561.D


Acq: 03 Jun 2020 12:33

Tgt Ion: 65 Resp: 162363

Ion Ratio Lower Upper

65 100

67 52.6 0.0 104.8



Abundance Ion 64.90 (64.60 to 65.60): VX0

Ion 66.90 (66.60 to 67.60): VX0

6.03


60000


40000

20000

0

Time-->

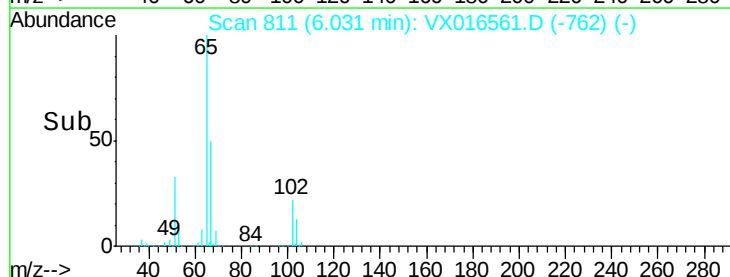

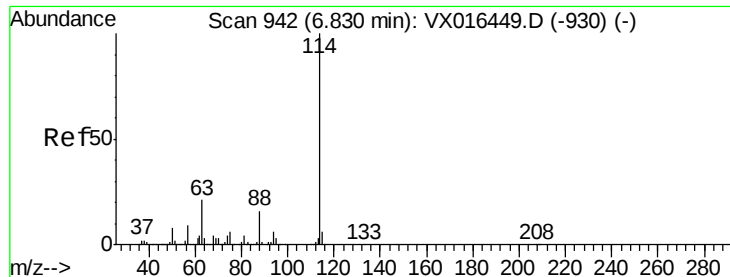

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.83 min Scan# 942

Delta R.T. -0.00 min

Lab File: VX016561.D

Acq: 03 Jun 2020 12:33

Instrument :

MSVOA_X

ClientSampleId :

TB-01-200602


Tot Ion:114 Resp: 455901

Ion Ratio Lower Upper

114 100

63 20.3 0.0 42.6

88 16.1 0.0 32.8



Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VX0

Ion 87.90 (87.60 to 88.60): VX0

250000

200000

150000



100000

50000

0

6.70 6.80 6.90

Time-->

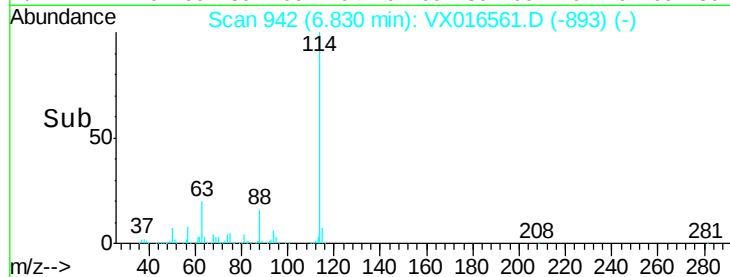

#35

Dibromofluoromethane

Concen: 46.500 ug/l

RT: 5.46 min Scan# 718

Delta R.T. -0.00 min

Lab File: VX016561.D

Acq: 03 Jun 2020 12:33


Tgt Ion:113 Resp: 130535

Ion Ratio Lower Upper

113 100

111 103.7 83.0 124.6

192 22.6 17.7 26.5



Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

60000

50000

40000

30000


20000


10000

0

5.30 5.40 5.50 5.60

Time-->

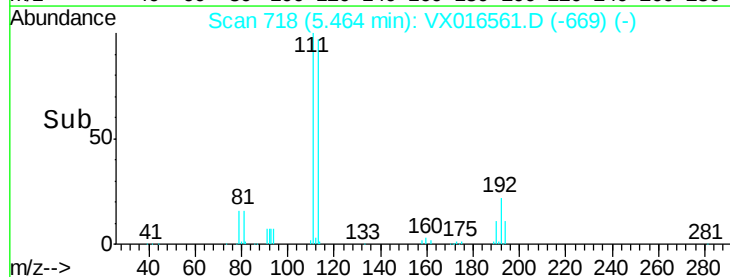

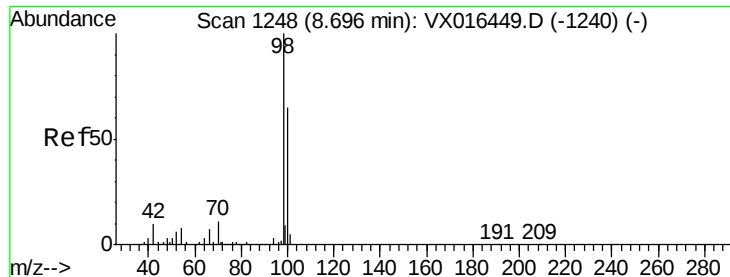

#50

Toluene-d8

Concen: 51.799 ug/l

RT: 8.70 min Scan# 1248

Delta R.T. -0.00 min

Lab File: VX016561.D

Acq: 03 Jun 2020 12:33

Instrument :

MSVOA_X

ClientSampleId :


TB-01-200602

Tot Ion: 98 Resp: 565968

Ion Ratio Lower Upper

98 100

100 66.5 53.8 80.6



Abundance Ion 98.00 (97.70 to 98.70): VX0

Ion 100.00 (99.70 to 100.70): VX

8.70

400000



300000

200000

100000

0

Time-->

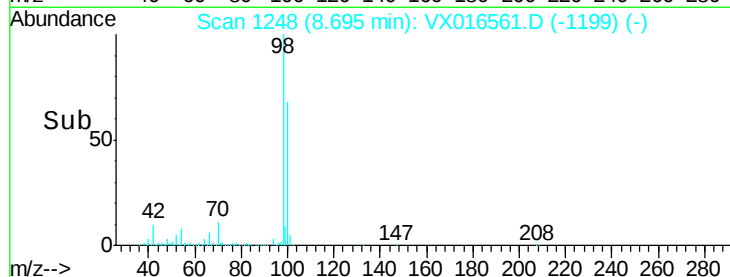

#62

4-Bromofluorobenzene

Concen: 52.873 ug/l

RT: 11.12 min Scan# 1646

Delta R.T. -0.00 min

Lab File: VX016561.D

Acq: 03 Jun 2020 12:33


Tgt Ion: 95 Resp: 223222

Ion Ratio Lower Upper

95 100

174 80.9 0.0 163.0

176 80.5 0.0 156.8



Abundance Ion 94.90 (94.60 to 95.60): VX0

Ion 173.80 (173.50 to 174.50): V

Ion 175.80 (175.50 to 176.50): V

250000

200000


150000


100000

50000

0

Time-->




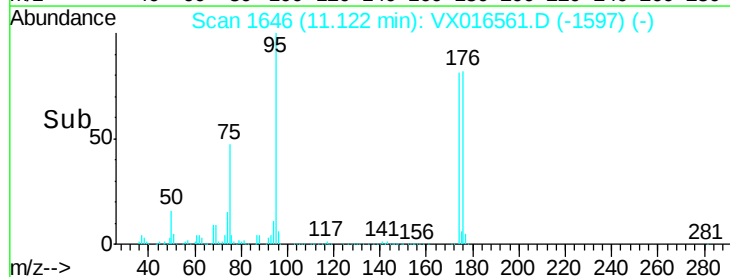


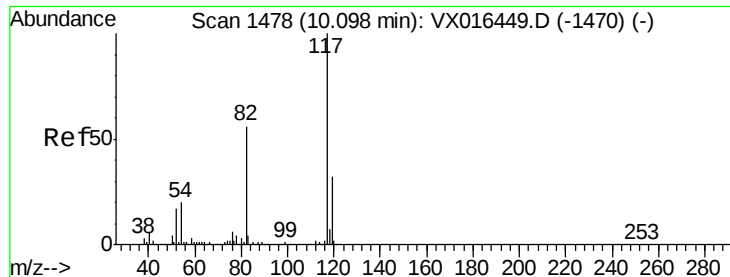

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.10 min Scan# 1478
Delta R.T. -0.00 min
Lab File: VX016561.D
Acq: 03 Jun 2020 12:33

Instrument :
MSVOA_X
ClientSampleId :
TB-01-200602

Tot Ion:117 Resp: 447565
Ion Ratio Lower Upper
117 100
82 55.0 45.0 67.6
119 32.3 25.8 38.8

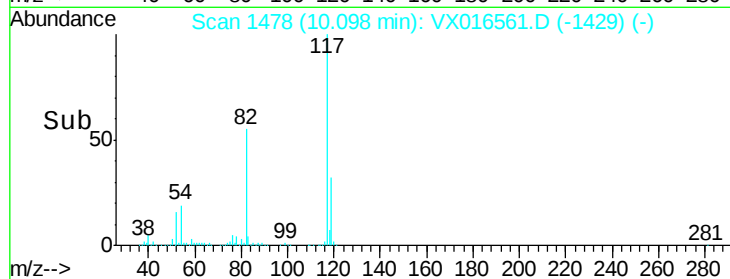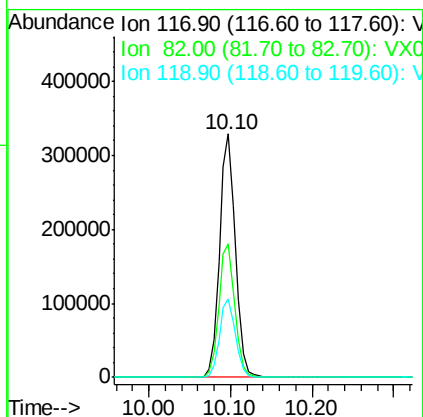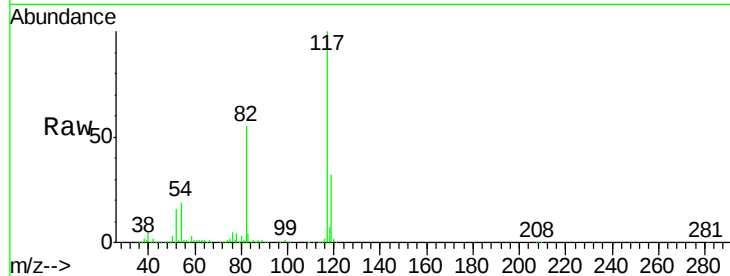

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.06 min Scan# 1800
Delta R.T. -0.00 min
Lab File: VX016561.D
Acq: 03 Jun 2020 12:33

Tgt Ion:152 Resp: 215245
Ion Ratio Lower Upper
152 100
115 59.5 39.9 119.6
150 159.1 0.0 341.0

