

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060321\
 Data File : VX022377.D
 Acq On : 03 Jun 2021 19:32
 Operator : JC/MD
 Sample : M2512-08 40X
 Misc : 1.10g/10mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMP-1-3

Quant Time: Jun 04 03:54:20 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
 Quant Title : SW846 8260
 QLast Update : Wed May 19 14:23:10 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	61637	50.00	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.769	114	134620	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	119115	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	46361	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.970	65	53940	56.73	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	= 113.46%	
35) Dibromofluoromethane	5.397	113	39522	46.30	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 92.60%	
50) Toluene-d8	8.653	98	164876	50.14	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	= 100.28%	
62) 4-Bromofluorobenzene	11.085	95	57282	47.13	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 94.26%	

Target Compounds						Qvalue
5) Bromomethane	1.611	94	105	0.21	ug/l	# 58
11) Tert butyl alcohol	2.953	59	1704	7.84	ug/l	# 73
14) Allyl chloride	2.782	41	556	0.43	ug/l	# 66
16) Acetone	2.392	43	718	1.73	ug/l	# 72
17) Carbon Disulfide	2.514	76	1607	0.87	ug/l	97
18) Methyl Acetate	2.825	43	7143	6.49	ug/l	# 47
20) Methylene Chloride	2.794	84	308	0.34	ug/l	# 67
31) Cyclohexane	5.483	56	5873	4.92	ug/l	94
36) 1,1-Dichloropropene	5.556	75	6222	5.00	ug/l	# 48
38) Carbon Tetrachloride	5.562	117	7155	5.88	ug/l	# 16
39) Methylcyclohexane	7.385	83	11751	8.32	ug/l	93
40) Benzene	6.050	78	8598	2.24	ug/l	98
48) Methyl methacrylate	7.647	41	517	0.45	ug/l	# 73
51) 4-Methyl-2-Pentanone	8.598	43	617	0.41	ug/l	# 32
52) Toluene	8.720	92	11583	4.78	ug/l	98
55) 1,1,2-Trichloroethane	9.104	97	1179	1.20	ug/l	# 15
59) 2-Hexanone	9.390	43	1895	1.69	ug/l	# 19
67) Ethyl Benzene	10.195	91	5785	1.27	ug/l	93
68) m/p-Xylenes	10.305	106	14667	8.51	ug/l	99
69) o-Xylene	10.646	106	4977	2.97	ug/l	99
73) Isopropylbenzene	10.963	105	1260	0.32	ug/l	88
74) N-amyl acetate	10.854	43	1286	0.69	ug/l	# 1
75) 1,1,2,2-Tetrachloroethane	11.219	83	283	0.22	ug/l	# 26
76) 1,2,3-Trichloropropane	11.085	75	30160	26.37	ug/l	# 39
78) n-propylbenzene	11.305	91	2913	0.63	ug/l	99
79) 2-Chlorotoluene	11.384	91	1798	0.64	ug/l	# 41
80) 1,3,5-Trimethylbenzene	11.457	105	9136	2.81	ug/l	95
81) trans-1,4-Dichloro-2-b...	11.085	75	30160	62.48	ug/l	# 13
82) 4-Chlorotoluene	11.451	91	1197	0.37	ug/l	# 45
83) tert-Butylbenzene	11.975	119	1976	0.63	ug/l	80
84) 1,2,4-Trimethylbenzene	11.756	105	18702	5.71	ug/l	97
85) sec-Butylbenzene	11.890	105	1246	0.31	ug/l	95
89) n-Butylbenzene	12.329	91	3110	1.00	ug/l	# 40
90) Hexachloroethane	12.530	117	329	0.59	ug/l	# 9
95) Naphthalene	13.780	128	9996	2.76	ug/l	# 85
96) 1,2,3-Trichlorobenzene	13.975	180	625	0.67	ug/l	# 38

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060321\
Data File : VX022377.D
Acq On : 03 Jun 2021 19:32
Operator : JC/MD
Sample : M2512-08 40X
Misc : 1.10g/10mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMP-1-3

Quant Time: Jun 04 03:54:20 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
Quant Title : SW846 8260
QLast Update : Wed May 19 14:23:10 2021
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060321\
Data File : VX022377.D
Acq On : 03 Jun 2021 19:32
Operator : JC/MD
Sample : M2512-08 40X
Misc : 1.10g/10mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMP-1-3


Quant Time: Jun 04 03:54:20 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
Quant Title : SW846 8260
QLast Update : Wed May 19 14:23:10 2021
Response via : Initial Calibration

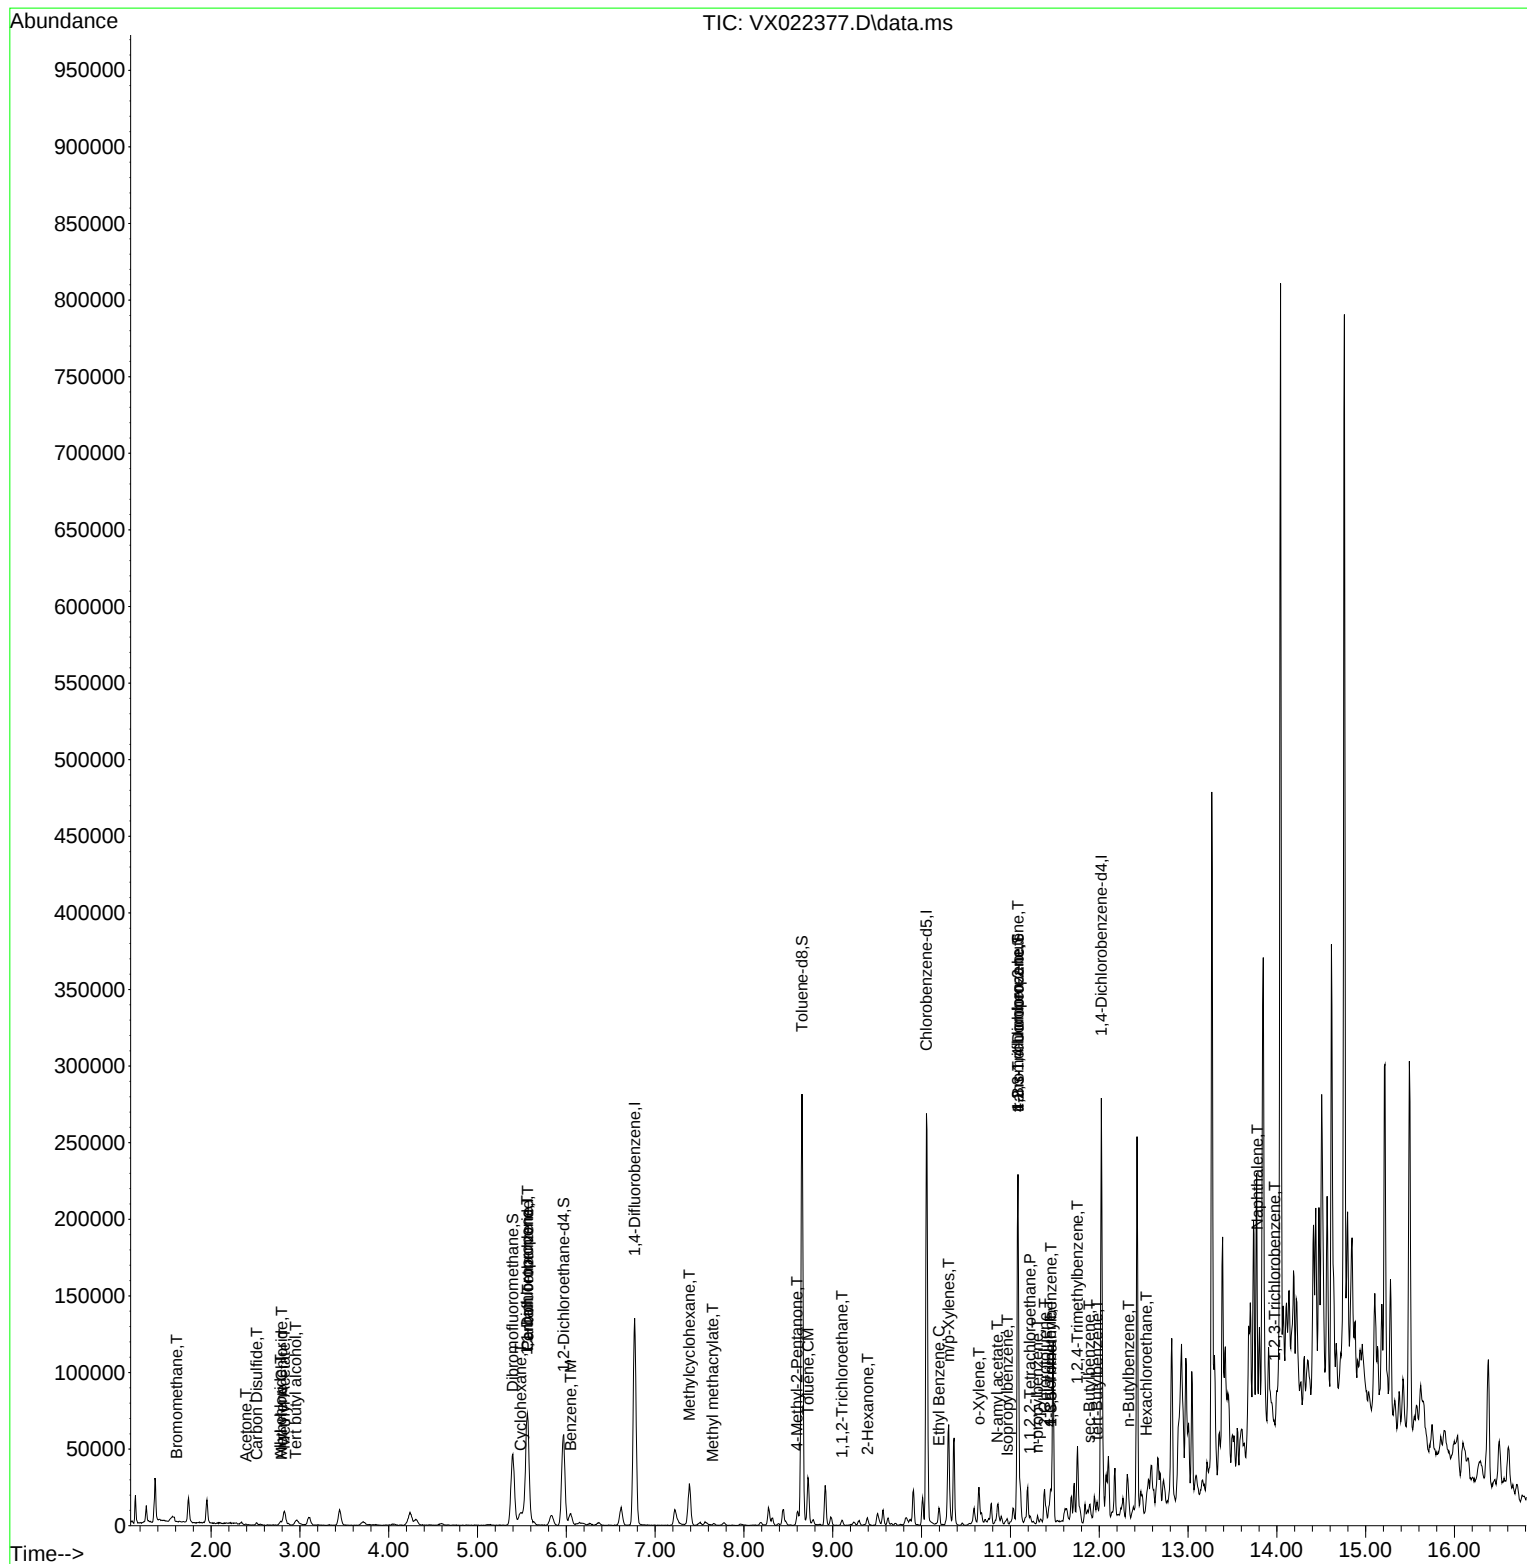



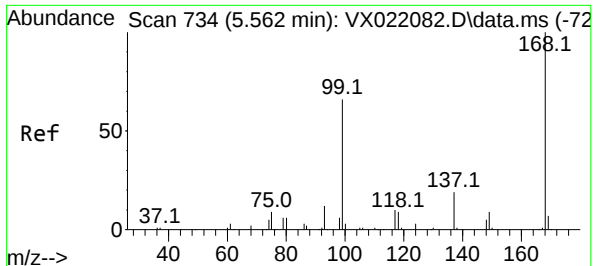


#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.000 min
Lab File: VX022377.D
Acq: 03 Jun 2021 19:32

Instrument :
MSVOA_X
ClientSampleId :
COMP-1-3







Tgt Ion:168 Resp: 61637
Ion Ratio Lower Upper
168 100
99 71.4 45.8 68.6#



#5
Bromomethane
Concen: 0.21 ug/l
RT: 1.611 min Scan# 86
Delta R.T. -0.001 min
Lab File: VX022377.D
Acq: 03 Jun 2021 19:32

Tgt Ion: 94 Resp: 105
Ion Ratio Lower Upper
94 100
96 54.2 76.4 114.6#

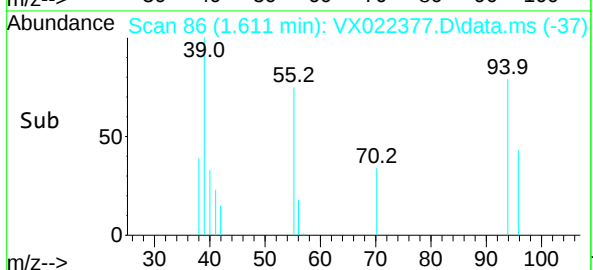







#11

Tert butyl alcohol
Concen: 7.84 ug/l
RT: 2.953 min Scan# 306
Delta R.T. -0.036 min
Lab File: VX022377.D
Acq: 03 Jun 2021 19:32

Instrument :
MSVOA_X
ClientSampled :
COMP-1-3




Tgt Ion: 59 Resp: 1704
Ion Ratio Lower Upper
59 100
57 0.0 7.8 11.8#




#14

Allyl chloride
Concen: 0.43 ug/l
RT: 2.782 min Scan# 278
Delta R.T. 0.116 min
Lab File: VX022377.D
Acq: 03 Jun 2021 19:32

Tgt Ion: 41 Resp: 556
Ion Ratio Lower Upper
41 100
39 51.4 51.6 77.4#
76 0.0 30.5 45.7#


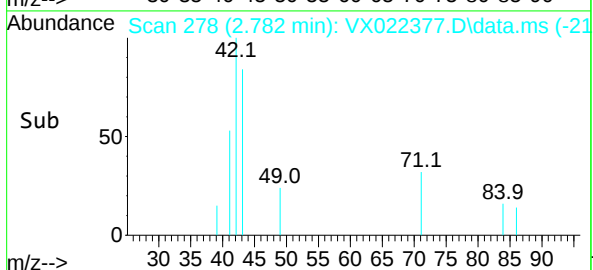




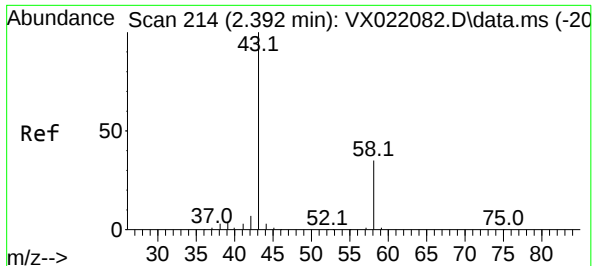

#16
Acetone
Concen: 1.73 ug/l
RT: 2.392 min Scan# 214
Delta R.T. -0.000 min
Lab File: VX022377.D
Acq: 03 Jun 2021 19:32




Instrument :
MSVOA_X
ClientSampled :
COMP-1-3


Tgt Ion: 43 Resp: 718
Ion Ratio Lower Upper
43 100
58 18.4 27.8 41.8#

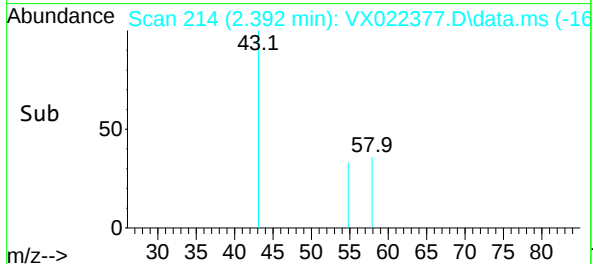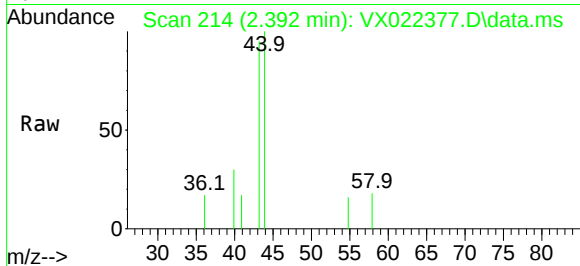

#17
Carbon Disulfide
Concen: 0.87 ug/l
RT: 2.514 min Scan# 234
Delta R.T. -0.000 min
Lab File: VX022377.D
Acq: 03 Jun 2021 19:32


Tgt Ion: 76 Resp: 1607
Ion Ratio Lower Upper
76 100
78 7.9 7.2 10.8

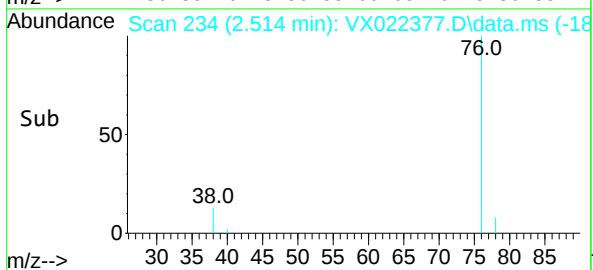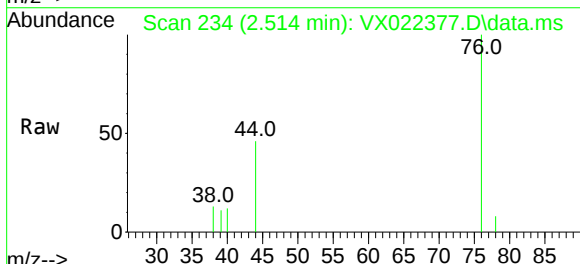






#18
Methyl Acetate
Concen: 6.49 ug/l
RT: 2.825 min Scan# 285
Delta R.T. 0.116 min
Lab File: VX022377.D
Acq: 03 Jun 2021 19:32

Instrument :
MSVOA_X
ClientSampleId :
COMP-1-3







Tgt Ion: 43 Resp: 7143
Ion Ratio Lower Upper
43 100
74 0.0 21.9 32.9#

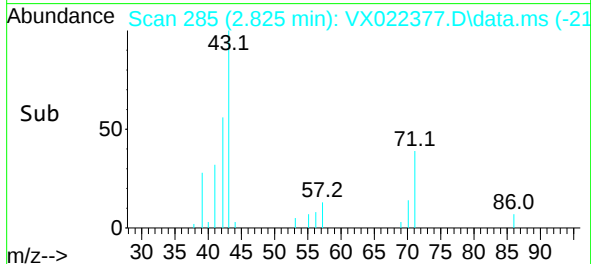

#20
Methylene Chloride
Concen: 0.34 ug/l
RT: 2.794 min Scan# 280
Delta R.T. 0.000 min
Lab File: VX022377.D
Acq: 03 Jun 2021 19:32

Tgt Ion: 84 Resp: 308
Ion Ratio Lower Upper
84 100
49 86.1 88.6 132.8#
51 0.0 27.0 40.6#
86 34.4 50.3 75.5#


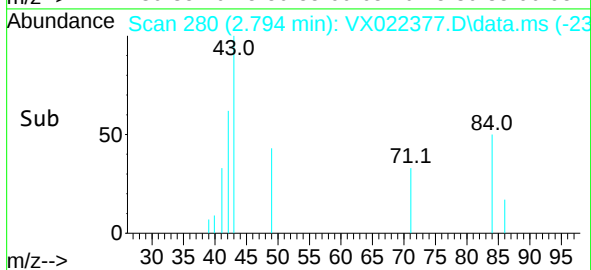
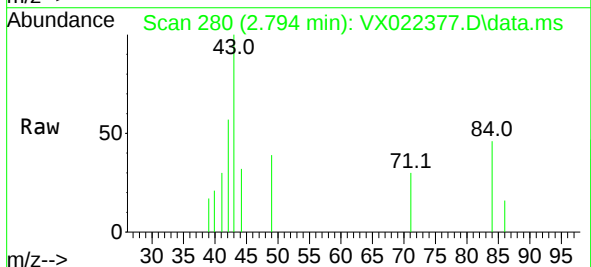





#31
Cyclohexane
Concen: 4.92 ug/l
RT: 5.483 min Scan# 721
Delta R.T. -0.000 min
Lab File: VX022377.D
Acq: 03 Jun 2021 19:32




Instrument :
MSVOA_X
ClientSampleId :
COMP-1-3


Tgt Ion: 56 Resp: 5873
Ion Ratio Lower Upper
56 100
69 31.8 25.3 37.9
84 81.8 71.4 107.0

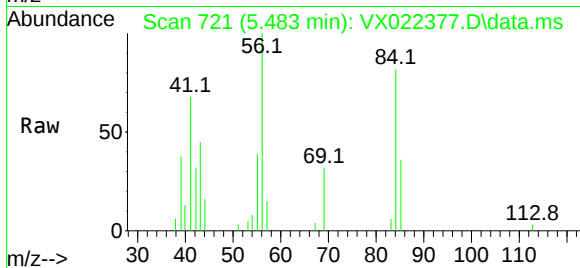

#33
1,2-Dichloroethane-d4
Concen: 56.73 ug/l
RT: 5.970 min Scan# 801
Delta R.T. 0.006 min
Lab File: VX022377.D
Acq: 03 Jun 2021 19:32

Tgt Ion: 65 Resp: 53940
Ion Ratio Lower Upper
65 100
67 53.9 0.0 105.4


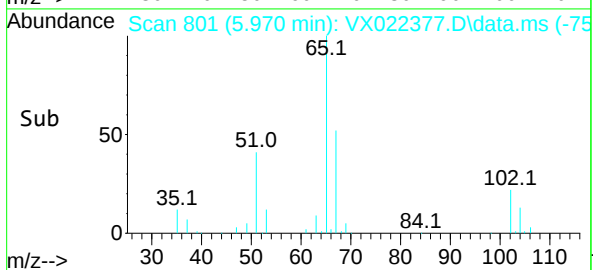

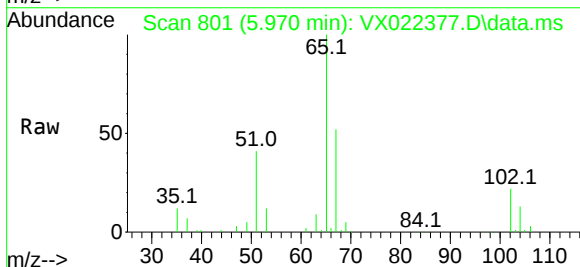


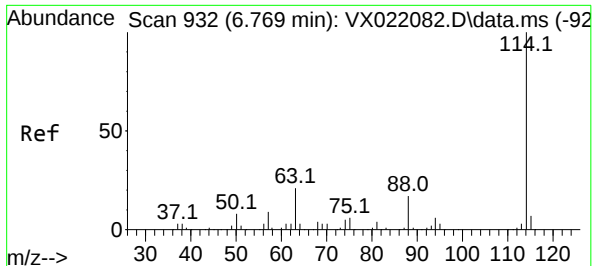

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 6.769 min Scan# 932
Delta R.T. -0.000 min
Lab File: VX022377.D
Acq: 03 Jun 2021 19:32




Instrument :
MSVOA_X
ClientSampleId :
COMP-1-3


Tgt Ion:114 Resp: 134620
Ion Ratio Lower Upper
114 100
63 22.7 0.0 40.8
88 18.7 0.0 32.8

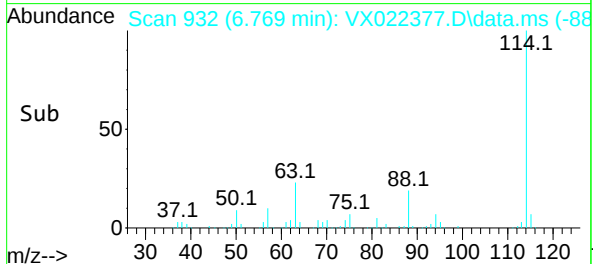

#35
Dibromofluoromethane
Concen: 46.30 ug/l
RT: 5.397 min Scan# 707
Delta R.T. 0.006 min
Lab File: VX022377.D
Acq: 03 Jun 2021 19:32


Tgt Ion:113 Resp: 39522
Ion Ratio Lower Upper
113 100
111 104.0 81.9 122.9
192 15.4 16.7 25.1#

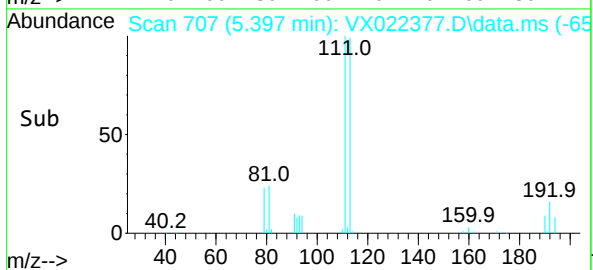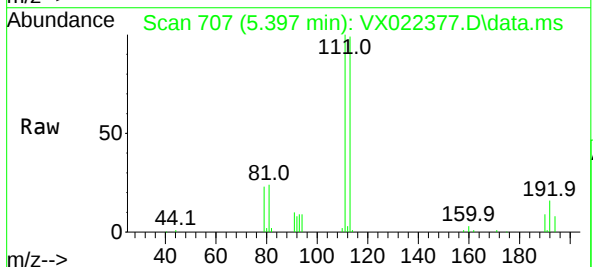



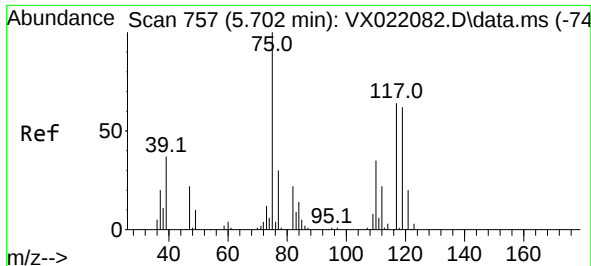


#36
1,1-Dichloropropene
Concen: 5.00 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.146 min
Lab File: VX022377.D
Acq: 03 Jun 2021 19:32

Instrument :
MSVOA_X
ClientSampleId :
COMP-1-3



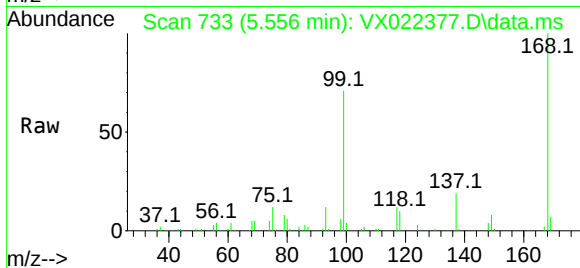



Tgt Ion: 75 Resp: 6222
Ion Ratio Lower Upper
75 100
110 8.2 18.1 54.4#
77 0.0 25.3 37.9#

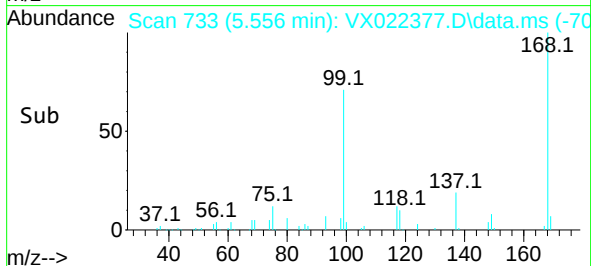

#38
Carbon Tetrachloride
Concen: 5.88 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.128 min
Lab File: VX022377.D
Acq: 03 Jun 2021 19:32

Tgt Ion: 117 Resp: 7155
Ion Ratio Lower Upper
117 100
119 5.2 76.2 114.2#
121 0.0 24.8 37.2#

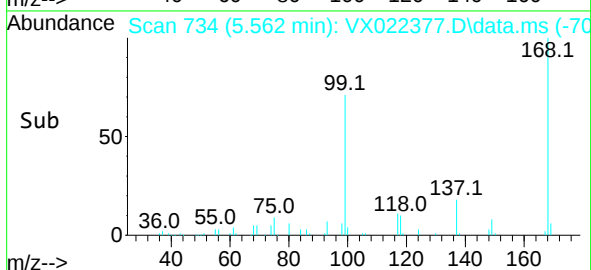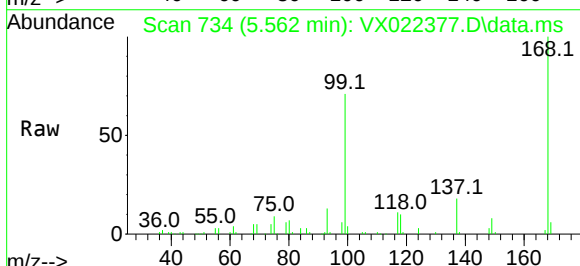



#39

Methylcyclohexane

Concen: 8.32 ug/l

RT: 7.385 min Scan# 1033





Delta R.T. -0.000 min

Lab File: VX022377.D

Acq: 03 Jun 2021 19:32

Tgt Ion: 83 Resp: 11751

Ion	Ratio	Lower	Upper
83	100		
55	81.7	58.9	88.3
98	46.0	38.1	57.1

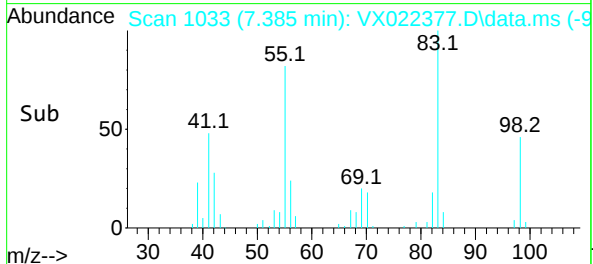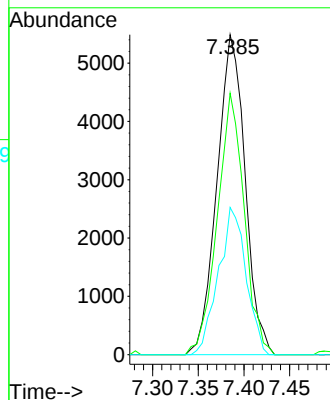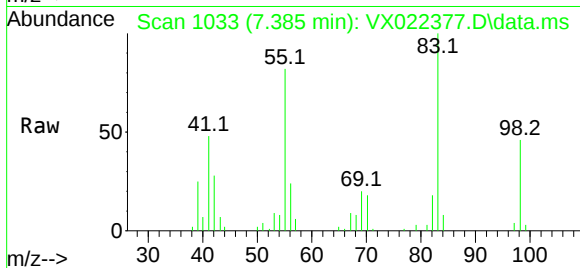

#40

Benzene

Concen: 2.24 ug/l

RT: 6.050 min Scan# 814




Delta R.T. 0.006 min


Lab File: VX022377.D

Acq: 03 Jun 2021 19:32

Tgt Ion: 78 Resp: 8598

Ion	Ratio	Lower	Upper
78	100		
77	22.8	18.9	28.3


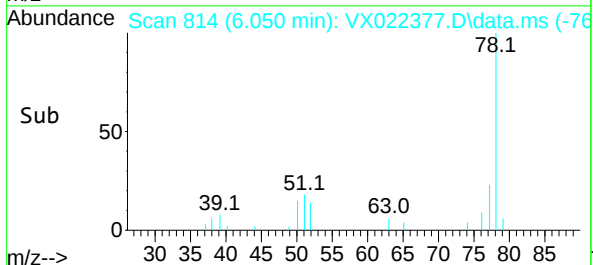
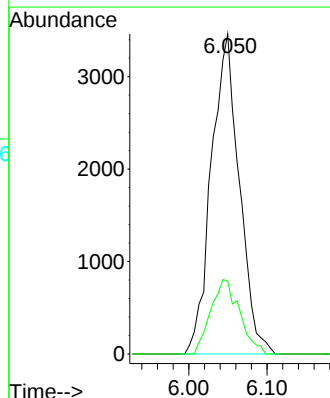
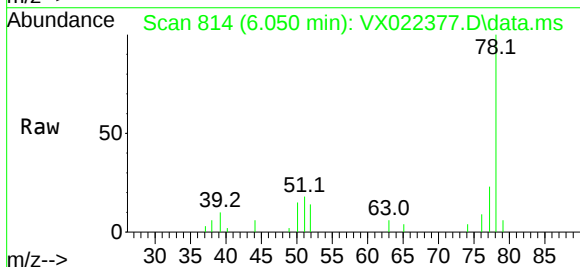




#48
Methyl methacrylate
Concen: 0.45 ug/l
RT: 7.647 min Scan# 1076
Delta R.T. -0.049 min
Lab File: VX022377.D
Acq: 03 Jun 2021 19:32




Instrument :
MSVOA_X
ClientSampled :
COMP-1-3


Tgt Ion: 41 Resp: 517
Ion Ratio Lower Upper
41 100
69 63.1 76.0 114.0#
39 68.7 44.6 67.0#

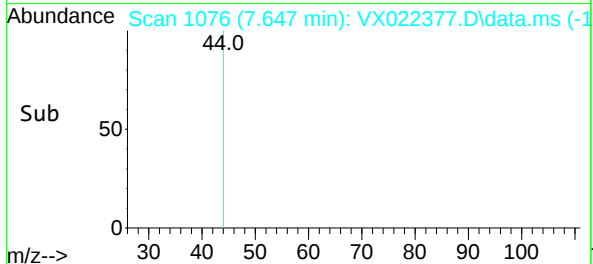

#50
Toluene-d8
Concen: 50.14 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX022377.D
Acq: 03 Jun 2021 19:32

Tgt Ion: 98 Resp: 164876
Ion Ratio Lower Upper
98 100
100 65.5 51.9 77.9


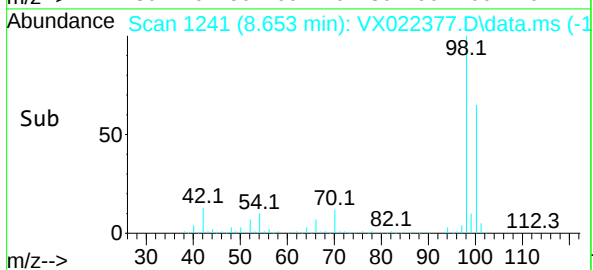

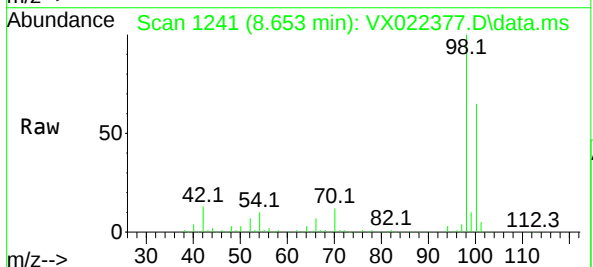




#51
4-Methyl-2-Pentanone
Concen: 0.41 ug/l
RT: 8.598 min Scan# 1232
Delta R.T. 0.018 min
Lab File: VX022377.D
Acq: 03 Jun 2021 19:32




Instrument :
MSVOA_X
ClientSampled :
COMP-1-3


Tgt Ion: 43 Resp: 617
Ion Ratio Lower Upper
43 100
58 0.0 35.4 53.0#



#52
Toluene
Concen: 4.78 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. -0.006 min
Lab File: VX022377.D
Acq: 03 Jun 2021 19:32


Tgt Ion: 92 Resp: 11583
Ion Ratio Lower Upper
92 100
91 168.0 137.1 205.7

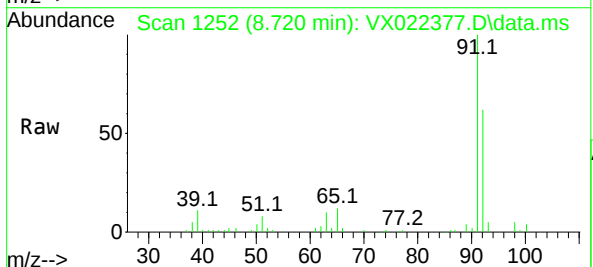






#55
1,1,2-Trichloroethane
Concen: 1.20 ug/l
RT: 9.104 min Scan# 1315
Delta R.T. -0.055 min
Lab File: VX022377.D
Acq: 03 Jun 2021 19:32

Instrument :
MSVOA_X
ClientSampled :
COMP-1-3







Tgt Ion	Ratio	Lower	Upper
97	100		
83	0.0	69.3	103.9#
85	0.0	44.3	66.5#
99	0.0	50.3	75.5#

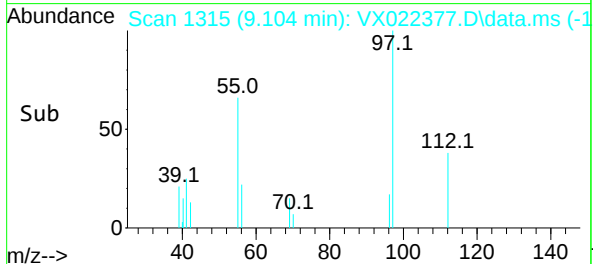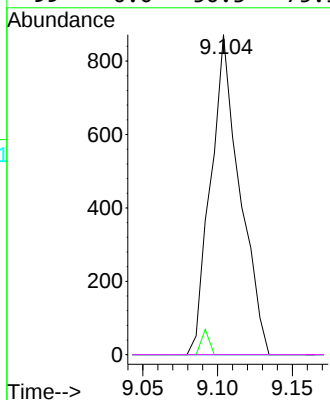

#59
2-Hexanone
Concen: 1.69 ug/l
RT: 9.390 min Scan# 1362
Delta R.T. -0.043 min
Lab File: VX022377.D
Acq: 03 Jun 2021 19:32

Tgt Ion	Ratio	Lower	Upper
43	100		
58	0.0	30.9	92.8#


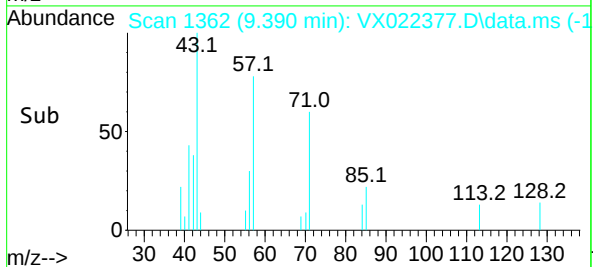
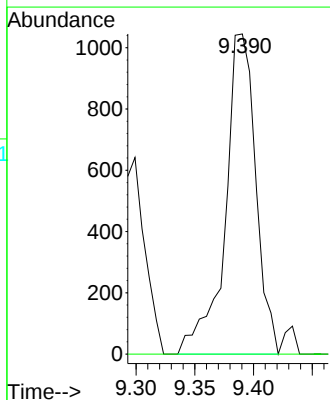
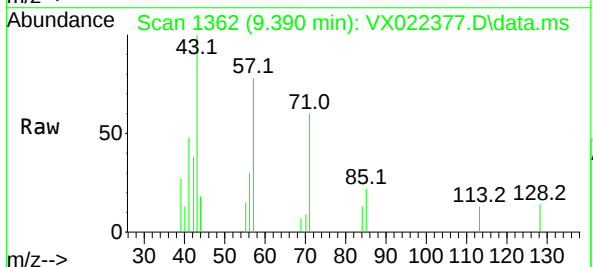




#62
4-Bromofluorobenzene
Concen: 47.13 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX022377.D
Acq: 03 Jun 2021 19:32




Instrument :
MSVOA_X
ClientSampleId :
COMP-1-3


Tgt Ion: 95 Resp: 57282
Ion Ratio Lower Upper
95 100
174 63.1 0.0 154.6
176 60.8 0.0 155.8

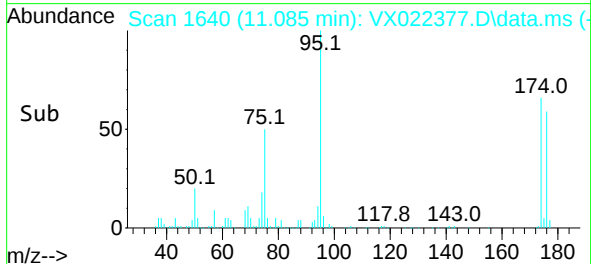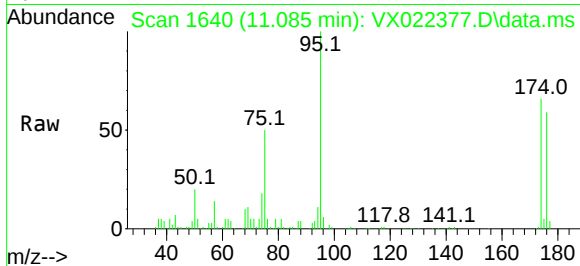

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.006 min
Lab File: VX022377.D
Acq: 03 Jun 2021 19:32

Tgt Ion: 117 Resp: 119115
Ion Ratio Lower Upper
117 100
82 60.4 47.4 71.2
119 30.4 26.6 39.8


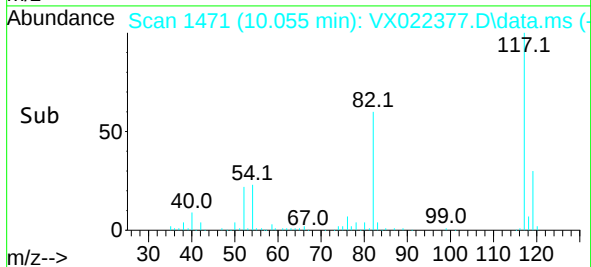

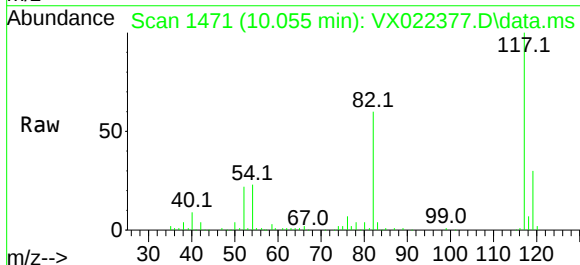




#67
Ethyl Benzene
Concen: 1.27 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX022377.D
Acq: 03 Jun 2021 19:32




Instrument :
MSVOA_X
ClientSampleId :
COMP-1-3


Tgt Ion: 91 Resp: 5785
Ion Ratio Lower Upper
91 100
106 26.7 24.6 37.0

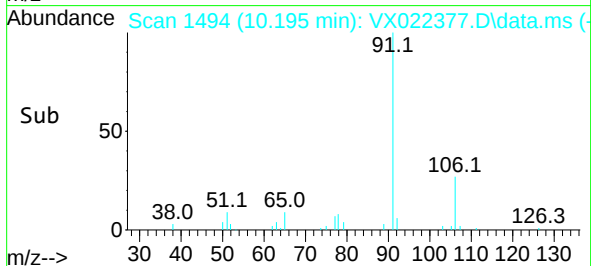

#68
m/p-Xylenes
Concen: 8.51 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. -0.000 min
Lab File: VX022377.D
Acq: 03 Jun 2021 19:32

Tgt Ion: 106 Resp: 14667
Ion Ratio Lower Upper
106 100
91 204.5 162.8 244.2


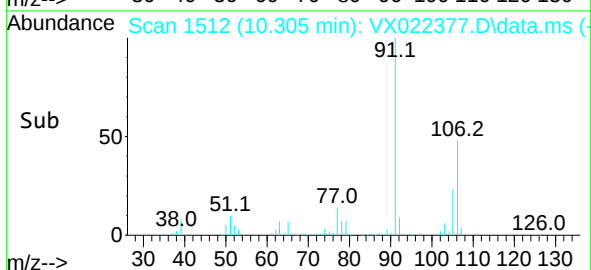

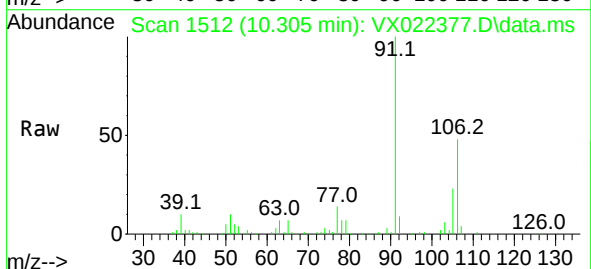




#69
o-Xylene
Concen: 2.97 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. -0.001 min
Lab File: VX022377.D
Acq: 03 Jun 2021 19:32




Instrument :
MSVOA_X
ClientSampled :
COMP-1-3


Tgt Ion:106 Resp: 4977
Ion Ratio Lower Upper
106 100
91 218.0 108.1 324.2

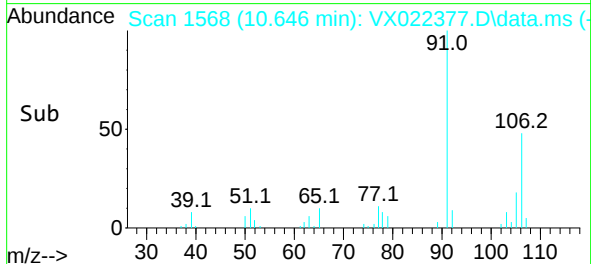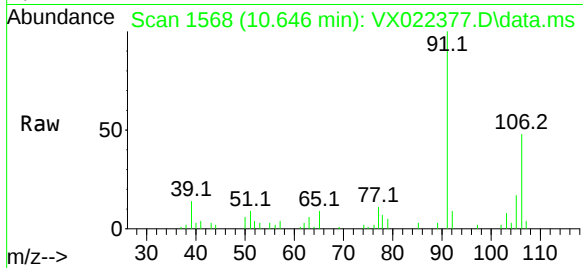

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX022377.D
Acq: 03 Jun 2021 19:32

Tgt Ion:152 Resp: 46361
Ion Ratio Lower Upper
152 100
115 68.5 41.1 123.3
150 164.0 0.0 349.0


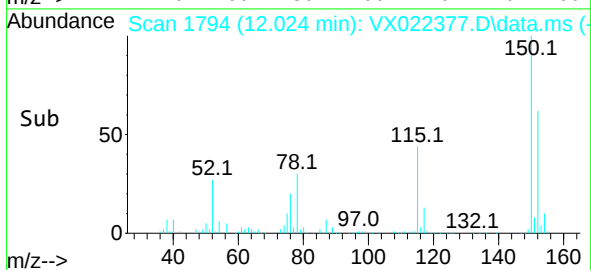

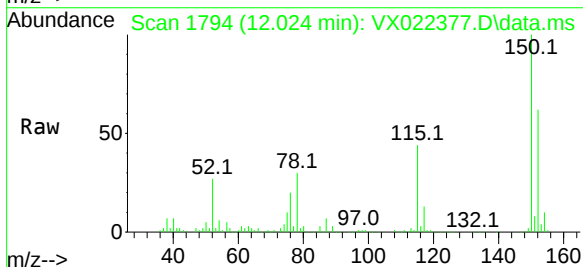




#73
Isopropylbenzene
Concen: 0.32 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. -0.001 min
Lab File: VX022377.D
Acq: 03 Jun 2021 19:32




Instrument :
MSVOA_X
ClientSampled :
COMP-1-3


Tgt Ion:105 Resp: 1260
Ion Ratio Lower Upper
105 100
120 32.6 13.2 39.6

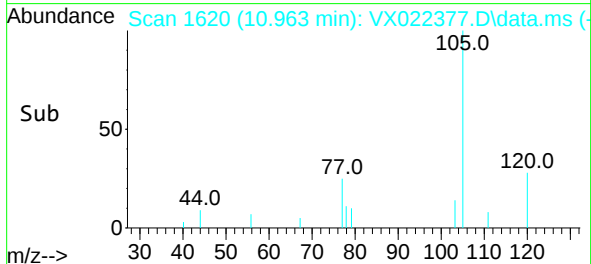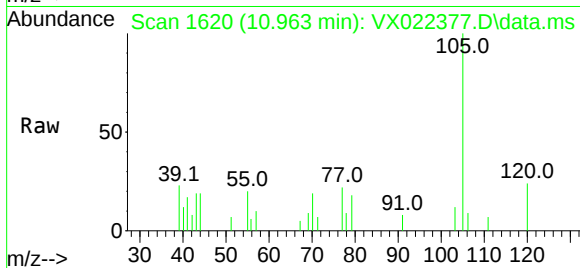

#74
N-ethyl acetate
Concen: 0.69 ug/l
RT: 10.854 min Scan# 1602
Delta R.T. 0.006 min
Lab File: VX022377.D
Acq: 03 Jun 2021 19:32

Tgt Ion: 43 Resp: 1286
Ion Ratio Lower Upper
43 100
70 17.4 39.0 58.6#
55 191.6 21.5 32.3#
61 0.0 22.1 33.1#


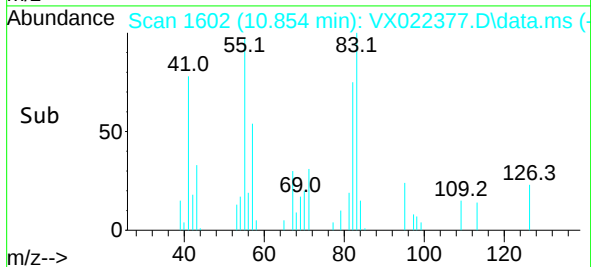

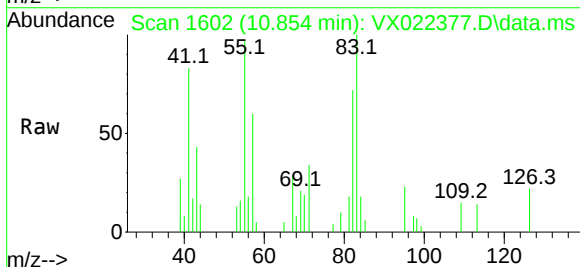




#75
1,1,2,2-Tetrachloroethane
Concen: 0.22 ug/l
RT: 11.219 min Scan# 1662
Delta R.T. 0.005 min
Lab File: VX022377.D
Acq: 03 Jun 2021 19:32




Instrument :
MSVOA_X
ClientSampleId :
COMP-1-3


Tgt Ion: 83 Resp: 283
Ion Ratio Lower Upper
83 100
131 0.0 5.1 15.2#
85 0.0 31.8 95.4#

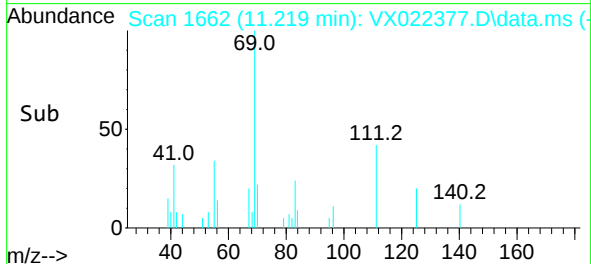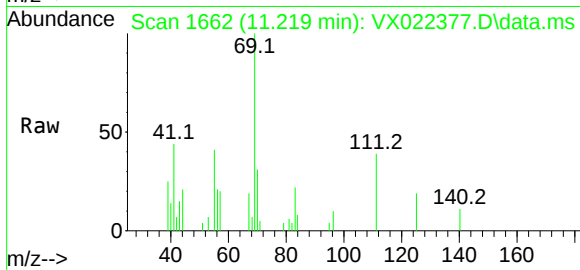

#76
1,2,3-Trichloropropane
Concen: 26.37 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. -0.159 min
Lab File: VX022377.D
Acq: 03 Jun 2021 19:32

Tgt Ion: 75 Resp: 30160
Ion Ratio Lower Upper
75 100
77 1.4 19.1 57.5#




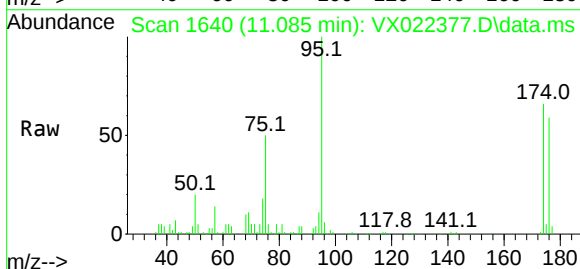


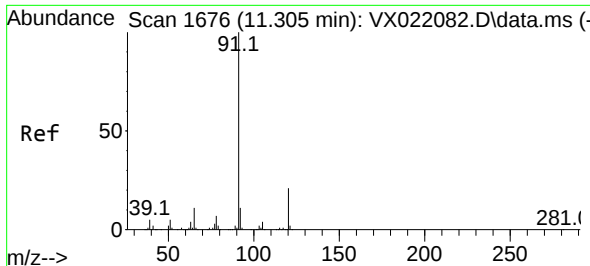

#78
n-propylbenzene
Concen: 0.63 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX022377.D
Acq: 03 Jun 2021 19:32




Instrument :
MSVOA_X
ClientSampleId :
COMP-1-3


Tgt Ion: 91 Resp: 2913
Ion Ratio Lower Upper
91 100
120 22.6 11.5 34.5

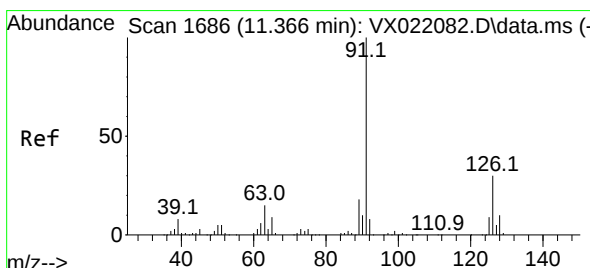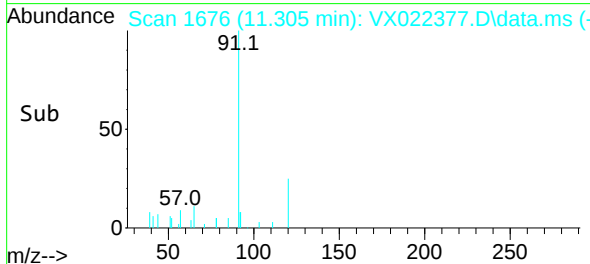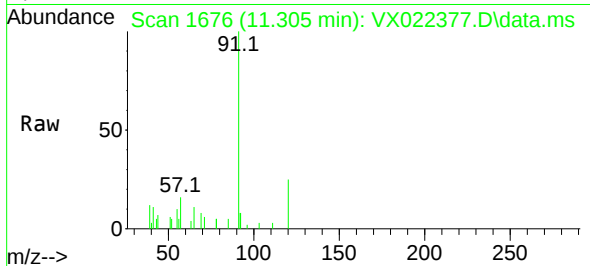

#79
2-Chlorotoluene
Concen: 0.64 ug/l
RT: 11.384 min Scan# 1689
Delta R.T. 0.018 min
Lab File: VX022377.D
Acq: 03 Jun 2021 19:32

Tgt Ion: 91 Resp: 1798
Ion Ratio Lower Upper
91 100
126 0.0 16.6 49.8#


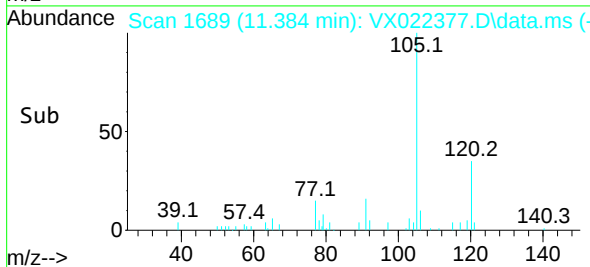

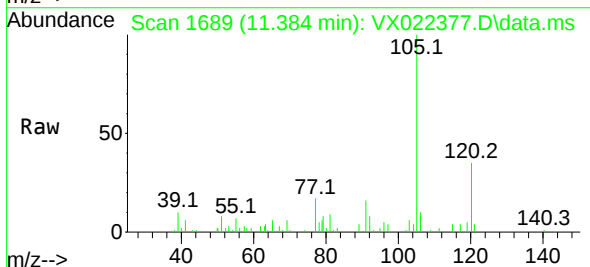




#80
1,3,5-Trimethylbenzene
Concen: 2.81 ug/l
RT: 11.457 min Scan# 1701
Delta R.T. 0.000 min
Lab File: VX022377.D
Acq: 03 Jun 2021 19:32




Instrument :
MSVOA_X
ClientSampled :
COMP-1-3


Tgt Ion:105 Resp: 9136
Ion Ratio Lower Upper
105 100
120 44.4 23.8 71.5

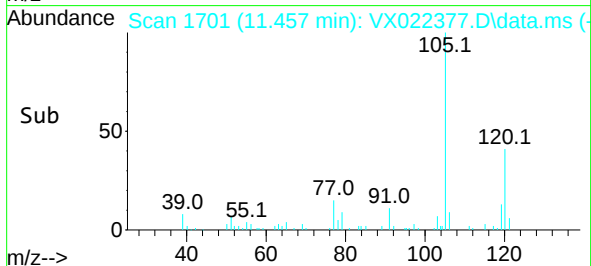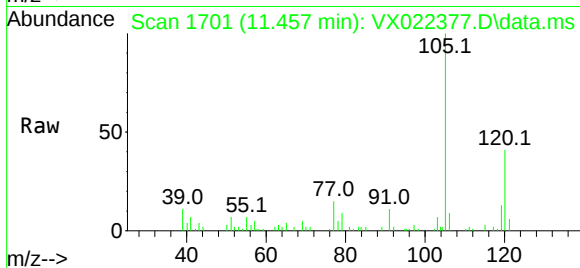

#81
trans-1,4-Dichloro-2-butene
Concen: 62.48 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.060 min
Lab File: VX022377.D
Acq: 03 Jun 2021 19:32

Tgt Ion: 75 Resp: 30160
Ion Ratio Lower Upper
75 100
53 1.1 74.5 111.7#
89 0.1 37.9 56.9#


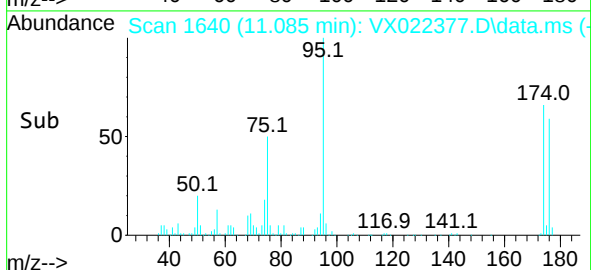

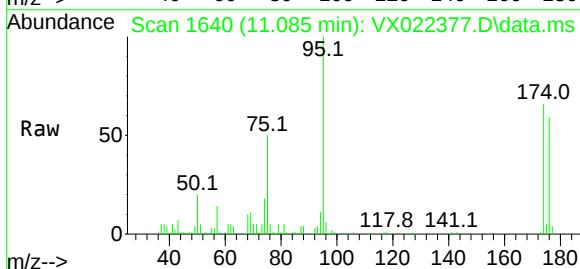




#82
4-Chlorotoluene
Concen: 0.37 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. -0.006 min
Lab File: VX022377.D
Acq: 03 Jun 2021 19:32




Instrument :
MSVOA_X
ClientSampleId :
COMP-1-3


Tgt Ion: 91 Resp: 1197
Ion Ratio Lower Upper
91 100
126 0.0 14.9 44.5#

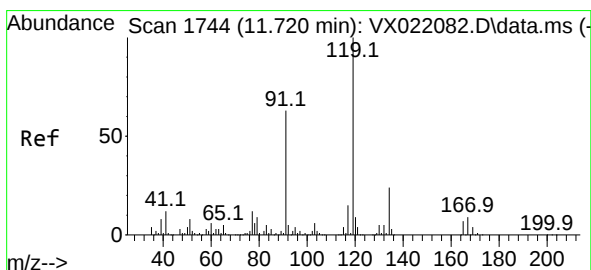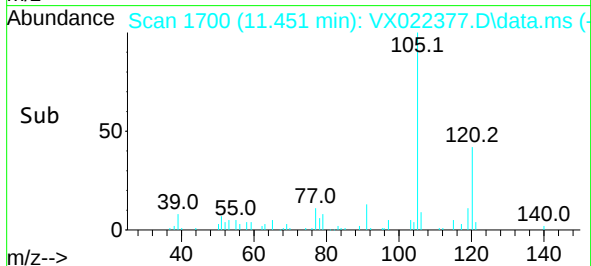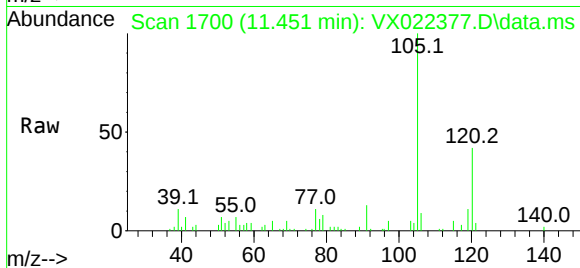

#83
tert-Butylbenzene
Concen: 0.63 ug/l
RT: 11.975 min Scan# 1786
Delta R.T. 0.255 min
Lab File: VX022377.D
Acq: 03 Jun 2021 19:32

Tgt Ion: 119 Resp: 1976
Ion Ratio Lower Upper
119 100
91 37.0 27.9 83.7
134 25.3 11.3 33.9


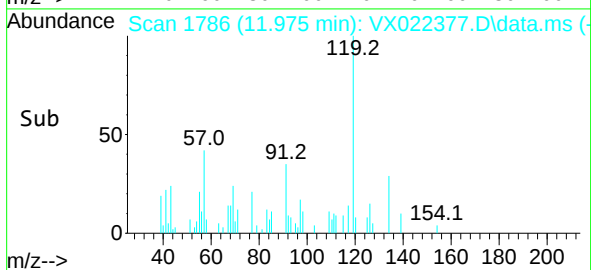

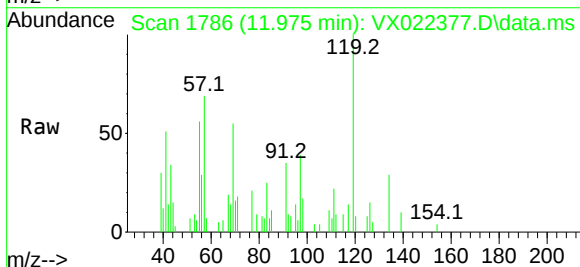




#84
1,2,4-Trimethylbenzene
Concen: 5.71 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.000 min
Lab File: VX022377.D
Acq: 03 Jun 2021 19:32




Instrument :
MSVOA_X
ClientSampleId :
COMP-1-3


Tgt Ion:105 Resp: 18702
Ion Ratio Lower Upper
105 100
120 42.6 22.4 67.3

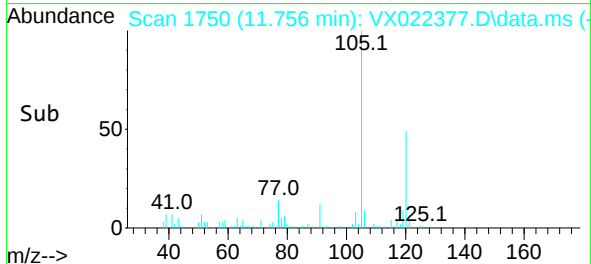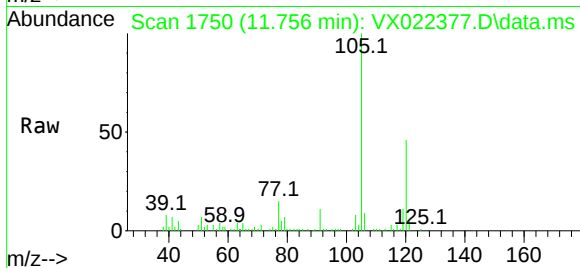

#85
sec-Butylbenzene
Concen: 0.31 ug/l
RT: 11.890 min Scan# 1772
Delta R.T. -0.006 min
Lab File: VX022377.D
Acq: 03 Jun 2021 19:32

Tgt Ion:105 Resp: 1246
Ion Ratio Lower Upper
105 100
134 17.8 10.0 29.8


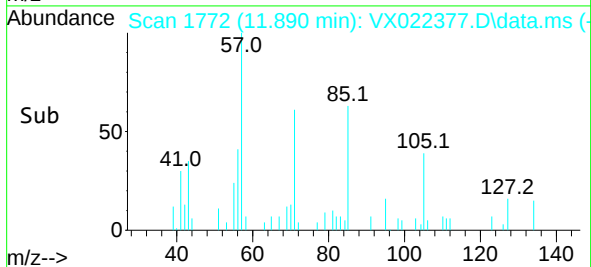

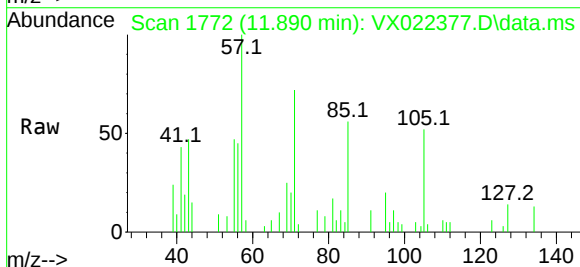


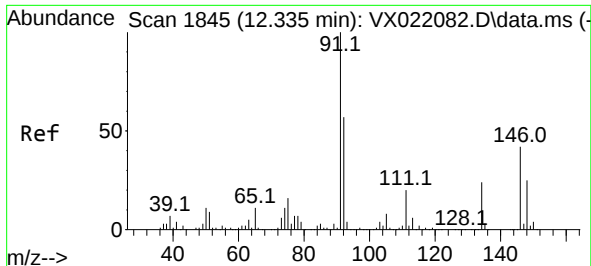

#89
n-Butylbenzene
Concen: 1.00 ug/l
RT: 12.329 min Scan# 1844
Delta R.T. -0.006 min
Lab File: VX022377.D
Acq: 03 Jun 2021 19:32




Instrument :
MSVOA_X
ClientSampleId :
COMP-1-3


Tgt Ion: 91 Resp: 3110
Ion Ratio Lower Upper
91 100
92 25.5 27.4 82.0#
134 78.1 13.2 39.5#

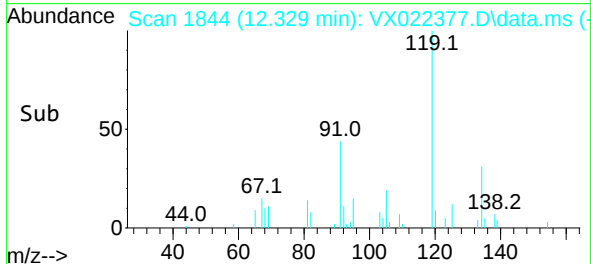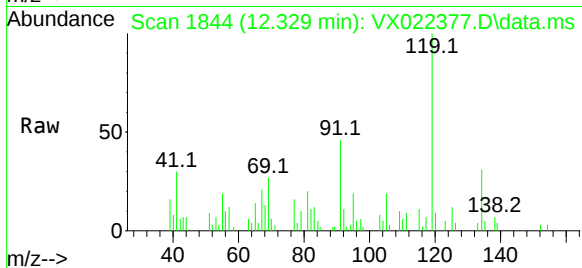

#90
Hexachloroethane
Concen: 0.59 ug/l
RT: 12.530 min Scan# 1877
Delta R.T. -0.013 min
Lab File: VX022377.D
Acq: 03 Jun 2021 19:32

Tgt Ion: 117 Resp: 329
Ion Ratio Lower Upper
117 100
201 0.0 40.4 121.2#


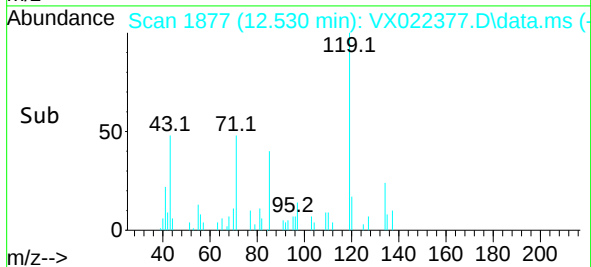

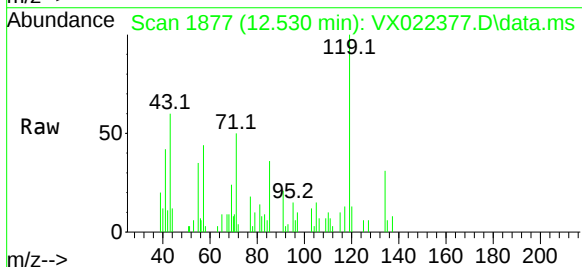




#95
Naphthalene
Concen: 2.76 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. -0.000 min
Lab File: VX022377.D
Acq: 03 Jun 2021 19:32

Instrument :
MSVOA_X
ClientSampled :
COMP-1-3

Tgt Ion:128 Resp: 9996
Ion Ratio Lower Upper
128 100
127 20.9 10.3 15.5#
129 14.2 8.8 13.2#

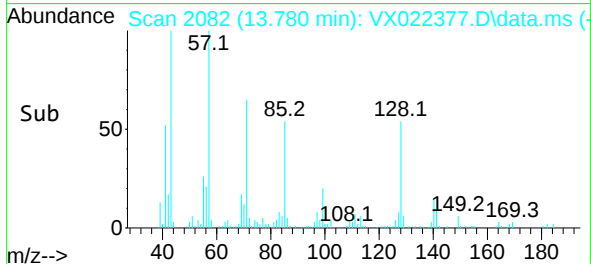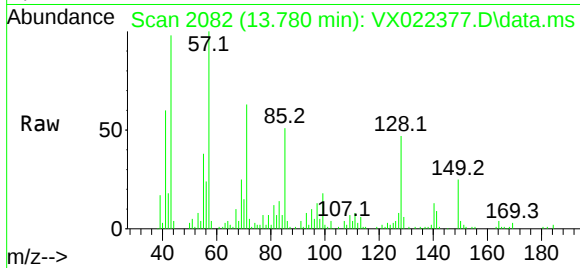

#96
1,2,3-Trichlorobenzene
Concen: 0.67 ug/l
RT: 13.975 min Scan# 2114
Delta R.T. 0.012 min
Lab File: VX022377.D
Acq: 03 Jun 2021 19:32

Tgt Ion:180 Resp: 625
Ion Ratio Lower Upper
180 100
182 75.8 47.6 142.9
145 137.0 16.1 48.3#

