

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060321\
 Data File : VX022378.D
 Acq On : 03 Jun 2021 19:55
 Operator : JC/MD
 Sample : M2512-09 40X
 Misc : 1.20g/10mL/100uL/5.0mL/MSVOA_X/MEOH
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 COMP-4-6

Quant Time: Jun 04 04:56:29 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
 Quant Title : SW846 8260
 QLast Update : Wed May 19 14:23:10 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.568	168	63836	50.00	ug/l	# 0.00
34) 1,4-Difluorobenzene	6.769	114	135223	50.00	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	122491	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	52272	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	54336	55.18	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery = 110.36%			
35) Dibromofluoromethane	5.391	113	40080	46.74	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 93.48%			
50) Toluene-d8	8.653	98	169007	51.16	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery = 102.32%			
62) 4-Bromofluorobenzene	11.085	95	61320	50.22	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 100.44%			
Target Compounds						Qvalue
11) Tert butyl alcohol	2.947	59	1625	7.22	ug/l	# 73
13) Acrolein	2.252	56	39	0.26	ug/l	# 1
14) Allyl chloride	2.788	41	391	0.29	ug/l	# 33
16) Acetone	2.392	43	619	1.44	ug/l	# 84
17) Carbon Disulfide	2.508	76	1207	0.63	ug/l	99
18) Methyl Acetate	2.825	43	4256	3.73	ug/l	# 47
20) Methylene Chloride	2.794	84	418	0.44	ug/l	# 72
23) Vinyl Acetate	3.453	43	1376	0.55	ug/l	# 59
31) Cyclohexane	5.483	56	3562	2.88	ug/l	# 79
36) 1,1-Dichloropropene	5.562	75	6071	4.86	ug/l	# 48
38) Carbon Tetrachloride	5.562	117	7512	6.14	ug/l	# 15
39) Methylcyclohexane	7.391	83	7220	5.09	ug/l	89
40) Benzene	6.050	78	5135	1.33	ug/l	95
51) 4-Methyl-2-Pentanone	8.592	43	417	0.28	ug/l	# 32
52) Toluene	8.720	92	7660	3.14	ug/l	93
55) 1,1,2-Trichloroethane	9.104	97	696	0.70	ug/l	# 15
67) Ethyl Benzene	10.195	91	4490	0.96	ug/l	99
68) m/p-Xylenes	10.305	106	10329	5.83	ug/l	99
69) o-Xylene	10.646	106	3398	1.97	ug/l	82
73) Isopropylbenzene	10.963	105	1356	0.31	ug/l	91
76) 1,2,3-Trichloropropane	11.085	75	31472	24.41	ug/l	# 39
78) n-propylbenzene	11.305	91	2409	0.46	ug/l	98
79) 2-Chlorotoluene	11.378	91	1623	0.52	ug/l	# 41
80) 1,3,5-Trimethylbenzene	11.457	105	6487	1.77	ug/l	96
81) trans-1,4-Dichloro-2-b...	11.085	75	31472	57.82	ug/l	# 12
82) 4-Chlorotoluene	11.451	91	899	0.25	ug/l	# 45
83) tert-Butylbenzene	11.975	119	1538	0.44	ug/l	80
84) 1,2,4-Trimethylbenzene	11.756	105	12997	3.52	ug/l	95
85) sec-Butylbenzene	11.890	105	956	0.21	ug/l	98
86) p-Isopropyltoluene	12.012	119	1068	0.28	ug/l	# 72
89) n-Butylbenzene	12.329	91	2546	0.73	ug/l	# 47
90) Hexachloroethane	12.536	117	334	0.54	ug/l	# 9
93) 1,2,4-Trichlorobenzene	13.847	180	245	0.23	ug/l	65
95) Naphthalene	13.780	128	6895	1.69	ug/l	# 78
96) 1,2,3-Trichlorobenzene	13.847	180	518	0.49	ug/l	69

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060321\
Data File : VX022378.D
Acq On : 03 Jun 2021 19:55
Operator : JC/MD
Sample : M2512-09 40X
Misc : 1.20g/10mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMP-4-6

Quant Time: Jun 04 04:56:29 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
Quant Title : SW846 8260
QLast Update : Wed May 19 14:23:10 2021
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
----------	------	------	----------	------	-------	----------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060321\
Data File : VX022378.D
Acq On : 03 Jun 2021 19:55
Operator : JC/MD
Sample : M2512-09 40X
Misc : 1.20g/10mL/100uL/5.0mL/MSVOA_X/MEOH
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
COMP-4-6

Quant Time: Jun 04 04:56:29 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
Quant Title : SW846 8260
QLast Update : Wed May 19 14:23:10 2021
Response via : Initial Calibration




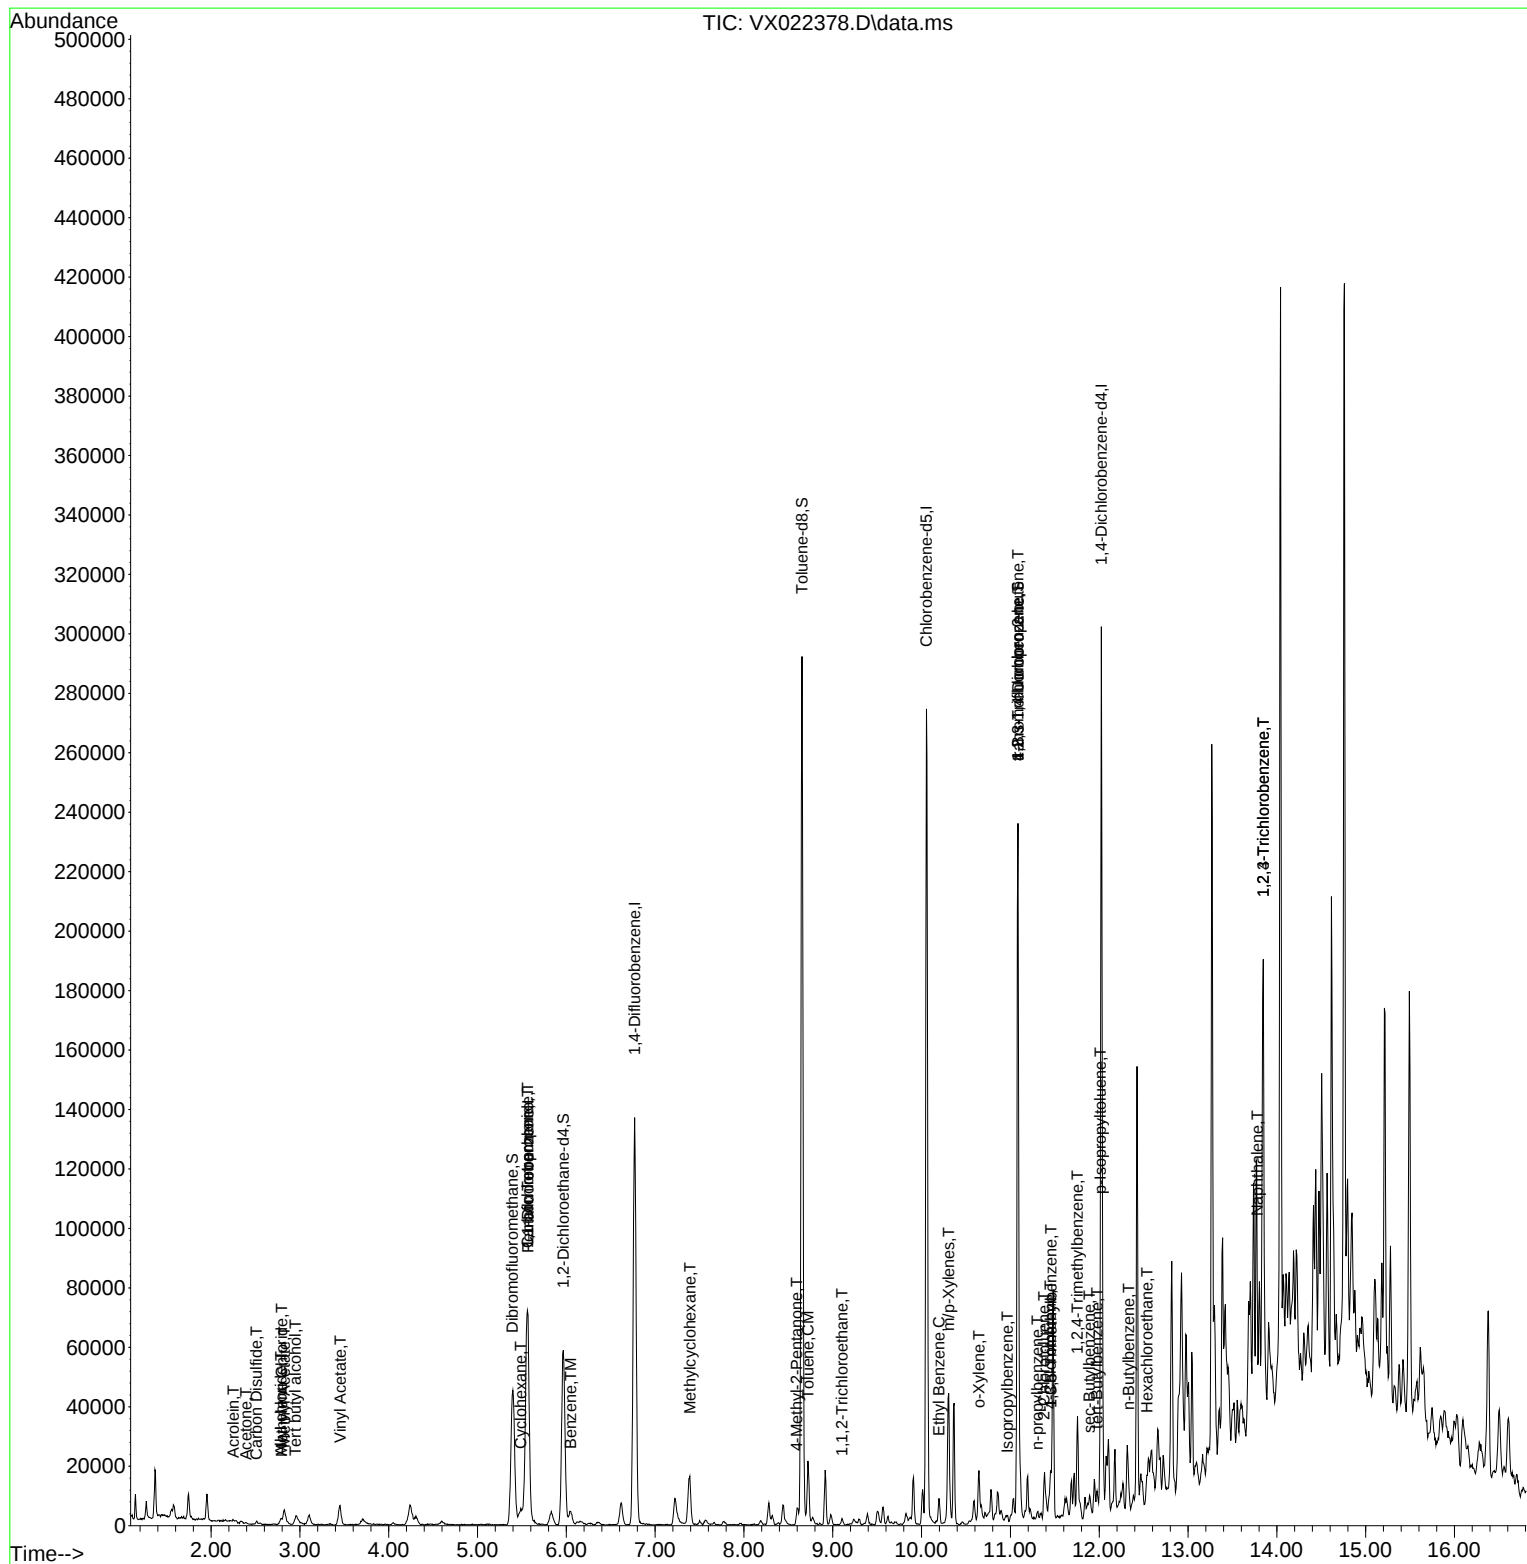


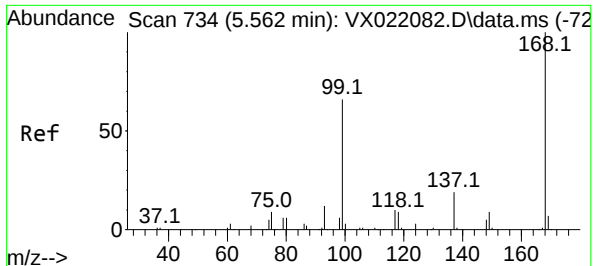

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 5.568 min Scan# 735
Delta R.T. 0.006 min
Lab File: VX022378.D
Acq: 03 Jun 2021 19:55




Instrument :
MSVOA_X
ClientSampleId :
COMP-4-6


Tgt Ion:168 Resp: 63836
Ion Ratio Lower Upper
168 100
99 68.7 45.8 68.6#

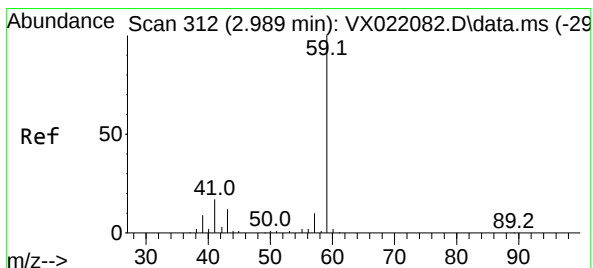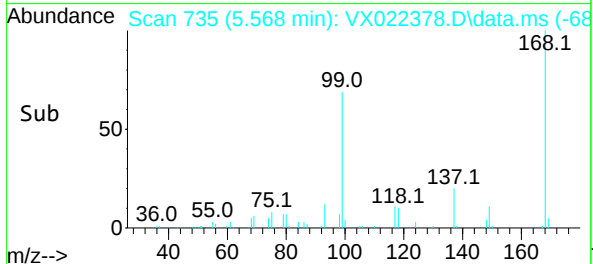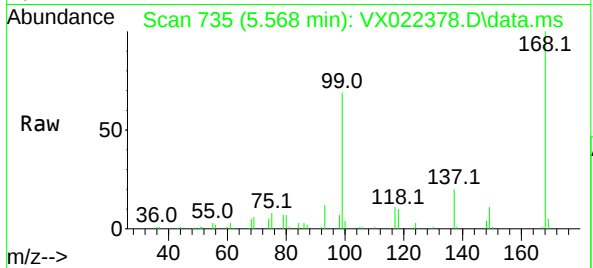

#11
Tert butyl alcohol
Concen: 7.22 ug/l
RT: 2.947 min Scan# 305
Delta R.T. -0.042 min
Lab File: VX022378.D
Acq: 03 Jun 2021 19:55

Tgt Ion: 59 Resp: 1625
Ion Ratio Lower Upper
59 100
57 0.0 7.8 11.8#


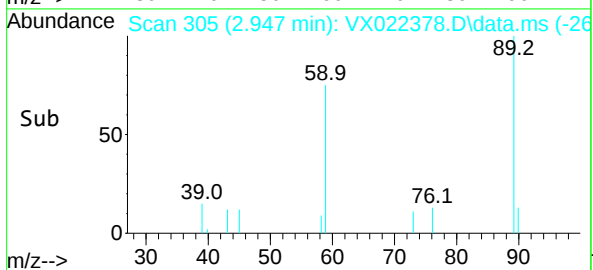

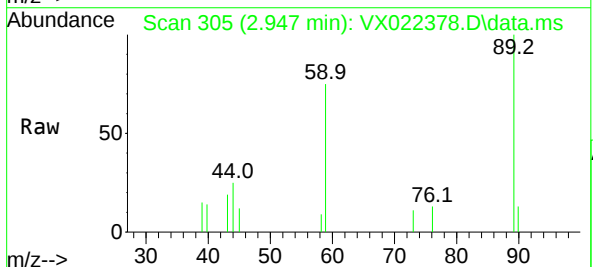


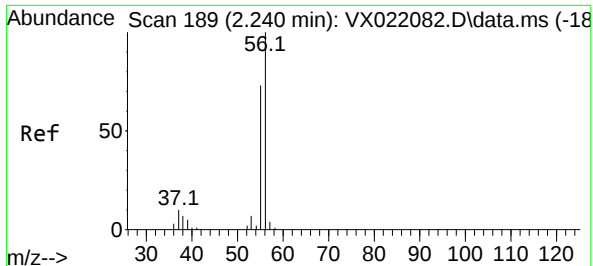

#13
Acrolein
Concen: 0.26 ug/l
RT: 2.252 min Scan# 191
Delta R.T. 0.012 min
Lab File: VX022378.D
Acq: 03 Jun 2021 19:55




Instrument :
MSVOA_X
ClientSampleId :
COMP-4-6


Tgt Ion: 56 Resp: 39
Ion Ratio Lower Upper
56 100
55 243.6 56.4 84.6#

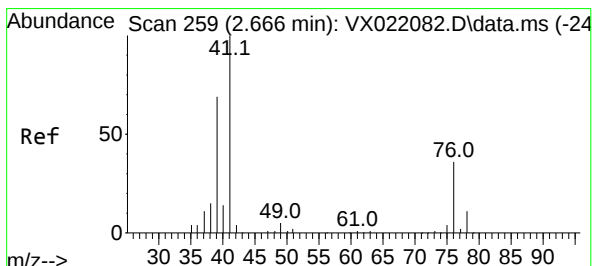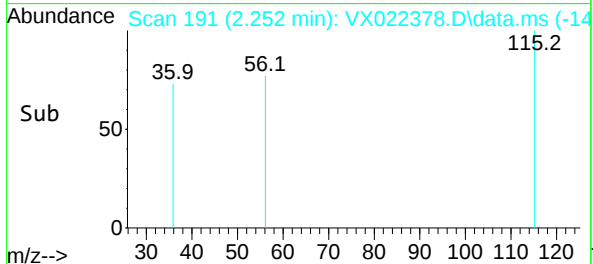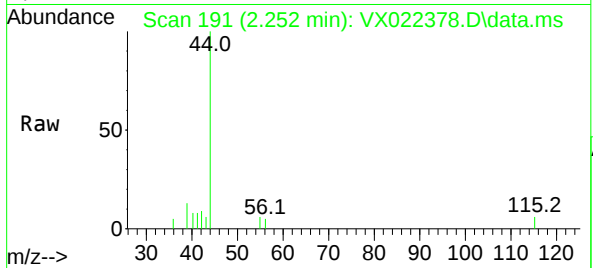

#14
Allyl chloride
Concen: 0.29 ug/l
RT: 2.788 min Scan# 279
Delta R.T. 0.122 min
Lab File: VX022378.D
Acq: 03 Jun 2021 19:55

Tgt Ion: 41 Resp: 391
Ion Ratio Lower Upper
41 100
39 119.2 51.6 77.4#
76 0.0 30.5 45.7#


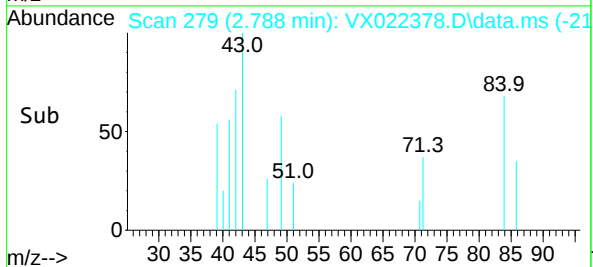

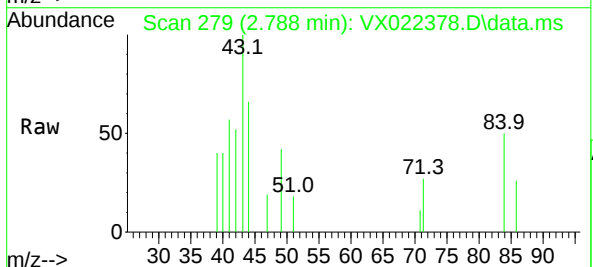




#16
Acetone
Concen: 1.44 ug/l
RT: 2.392 min Scan# 214
Delta R.T. -0.000 min
Lab File: VX022378.D
Acq: 03 Jun 2021 19:55




Instrument :
MSVOA_X
ClientSampleId :
COMP-4-6


Tgt Ion: 43 Resp: 619
Ion Ratio Lower Upper
43 100
58 25.4 27.8 41.8#

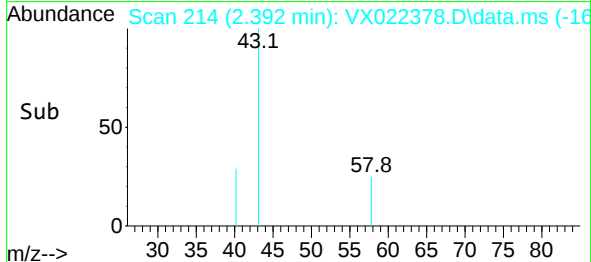

#17
Carbon Disulfide
Concen: 0.63 ug/l
RT: 2.508 min Scan# 233
Delta R.T. -0.006 min
Lab File: VX022378.D
Acq: 03 Jun 2021 19:55

Tgt Ion: 76 Resp: 1207
Ion Ratio Lower Upper
76 100
78 9.4 7.2 10.8



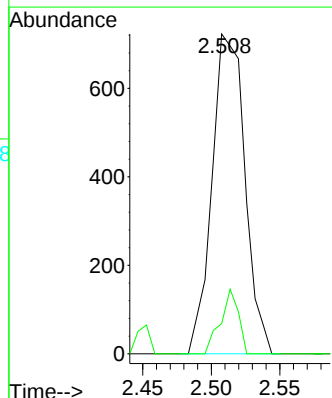





#18
Methyl Acetate
Concen: 3.73 ug/l
RT: 2.825 min Scan# 285
Delta R.T. 0.116 min
Lab File: VX022378.D
Acq: 03 Jun 2021 19:55




Instrument :
MSVOA_X
ClientSampleId :
COMP-4-6


Tgt Ion: 43 Resp: 4256
Ion Ratio Lower Upper
43 100
74 0.0 21.9 32.9#



#20
Methylene Chloride
Concen: 0.44 ug/l
RT: 2.794 min Scan# 280
Delta R.T. 0.000 min
Lab File: VX022378.D
Acq: 03 Jun 2021 19:55

Tgt Ion: 84 Resp: 418
Ion Ratio Lower Upper
84 100
49 68.8 88.6 132.8#
51 18.5 27.0 40.6#
86 56.5 50.3 75.5


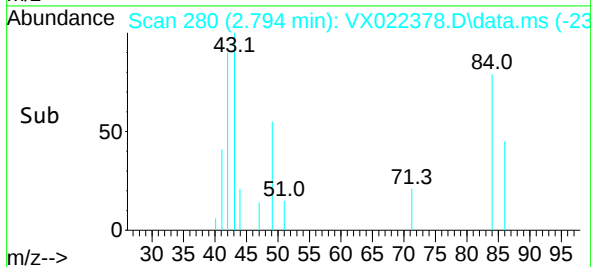

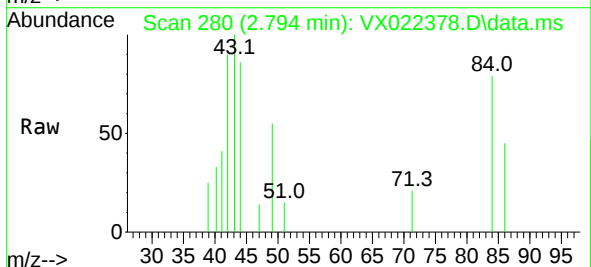




#23
 Vinyl Acetate
 Concen: 0.55 ug/l
 RT: 3.453 min Scan# 388
 Delta R.T. -0.274 min
 Lab File: VX022378.D
 Acq: 03 Jun 2021 19:55




Instrument :
 MSVOA_X
 ClientSampleId :
 COMP-4-6


Tgt Ion: 43 Resp: 1376
 Ion Ratio Lower Upper
 43 100
 86 28.4 9.9 14.9#

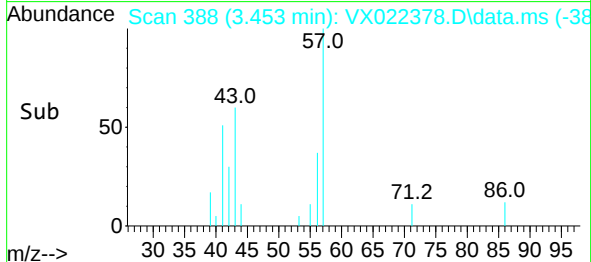

#31
 Cyclohexane
 Concen: 2.88 ug/l
 RT: 5.483 min Scan# 721
 Delta R.T. -0.000 min
 Lab File: VX022378.D
 Acq: 03 Jun 2021 19:55

Tgt Ion: 56 Resp: 3562
 Ion Ratio Lower Upper
 56 100
 69 18.2 25.3 37.9#
 84 70.5 71.4 107.0#

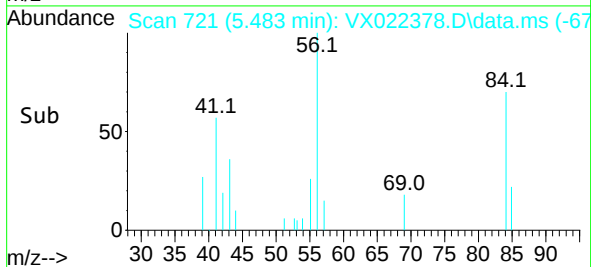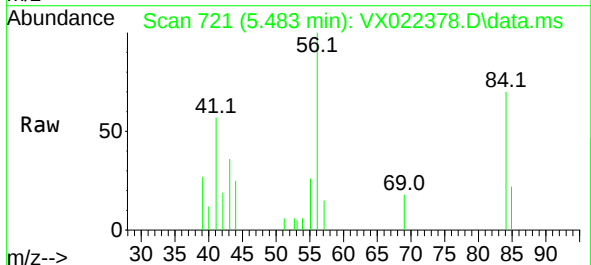



#33

1,2-Dichloroethane-d4

Concen: 55.18 ug/l

RT: 5.964 min Scan# 800

Delta R.T. 0.000 min

Lab File: VX022378.D





Acq: 03 Jun 2021 19:55

Tgt Ion: 65 Resp: 54336

Ion Ratio Lower Upper

65 100

67 51.9 0.0 105.4

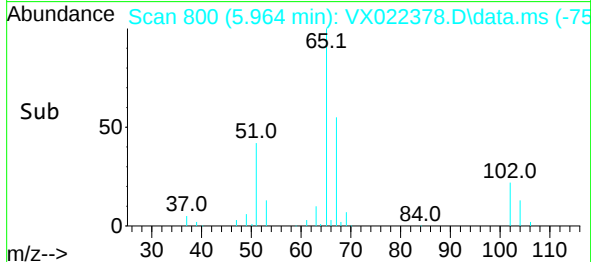

#34

1,4-Difluorobenzene

Concen: 50.00 ug/l

RT: 6.769 min Scan# 932

Delta R.T. 0.000 min

Lab File: VX022378.D

Acq: 03 Jun 2021 19:55




Tgt Ion: 114 Resp: 135223


Ion Ratio Lower Upper

114 100

63 21.1 0.0 40.8

88 18.2 0.0 32.8

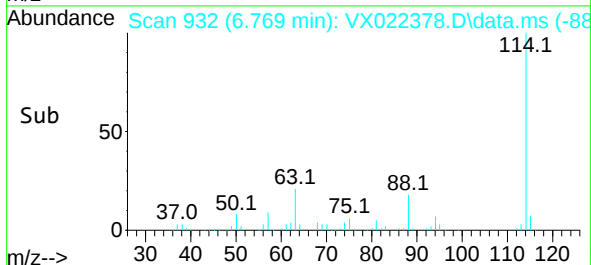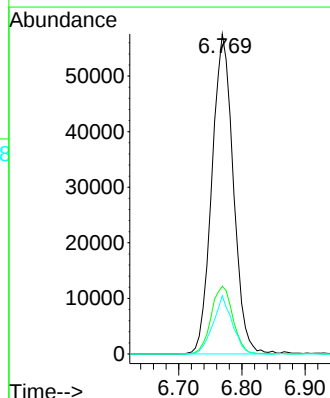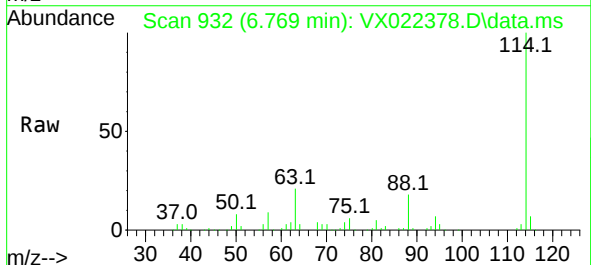

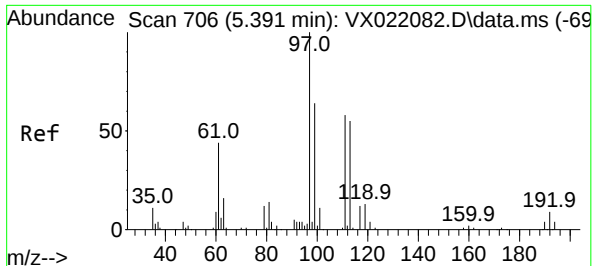

#35

Dibromofluoromethane

Concen: 46.74 ug/l

RT: 5.391 min Scan# 706

Delta R.T. 0.000 min

Lab File: VX022378.D

Acq: 03 Jun 2021 19:55

Tgt Ion:113 Resp: 40080

Ion Ratio Lower Upper

113 100

111 104.4 81.9 122.9





192 17.2 16.7 25.1

Instrument :

MSVOA_X

ClientSampleId :

COMP-4-6

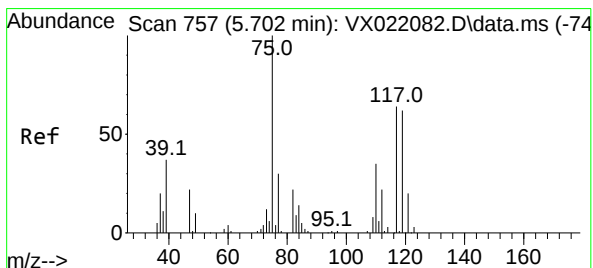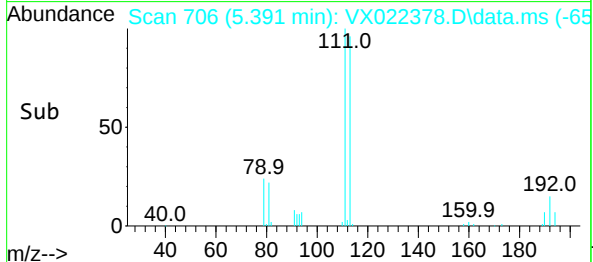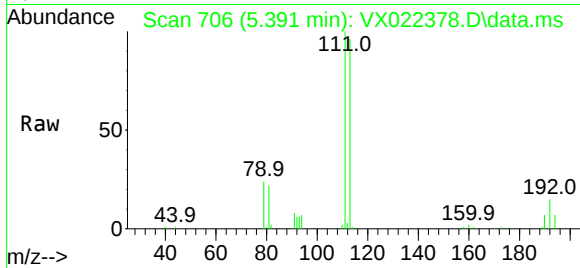

#36

1,1-Dichloropropene

Concen: 4.86 ug/l

RT: 5.562 min Scan# 734

Delta R.T. -0.140 min

Lab File: VX022378.D

Acq: 03 Jun 2021 19:55




Tgt Ion: 75 Resp: 6071


Ion Ratio Lower Upper

75 100

110 7.8 18.1 54.4#


77 0.0 25.3 37.9#

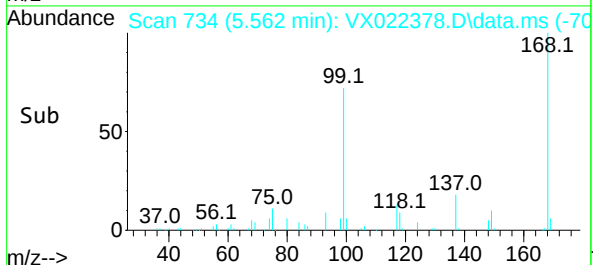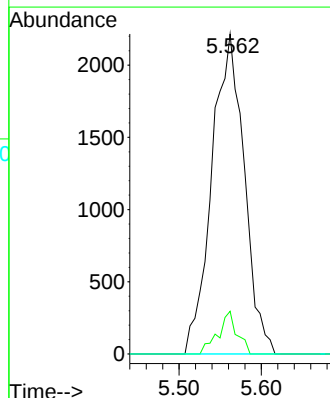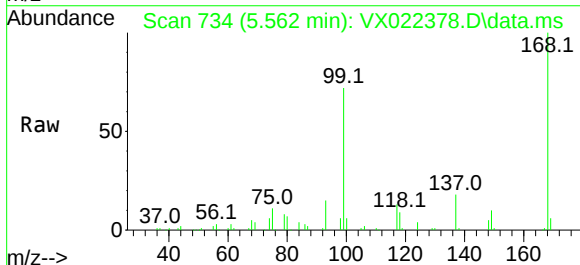






#38
Carbon Tetrachloride
Concen: 6.14 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.128 min
Lab File: VX022378.D
Acq: 03 Jun 2021 19:55

Instrument :
MSVOA_X
ClientSampleId :
COMP-4-6



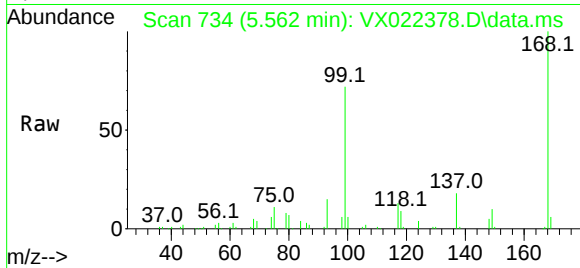



Tgt Ion:117 Resp: 7512
Ion Ratio Lower Upper
117 100
119 4.0 76.2 114.2#
121 0.0 24.8 37.2#



#39
Methylcyclohexane
Concen: 5.09 ug/l
RT: 7.391 min Scan# 1034
Delta R.T. 0.006 min
Lab File: VX022378.D
Acq: 03 Jun 2021 19:55

Tgt Ion: 83 Resp: 7220
Ion Ratio Lower Upper
83 100
55 82.2 58.9 88.3
98 55.4 38.1 57.1


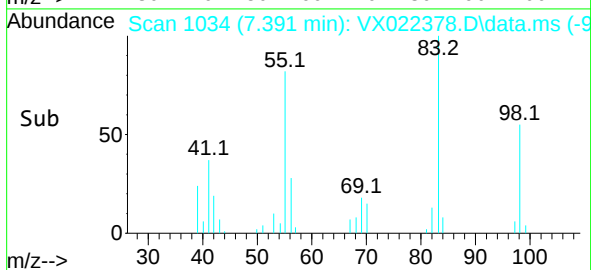

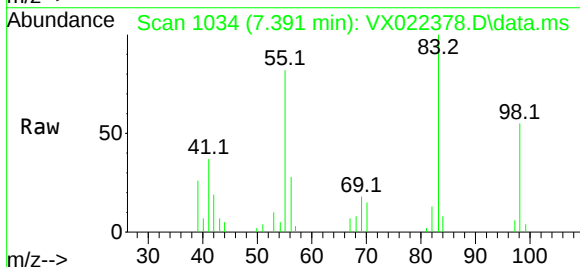


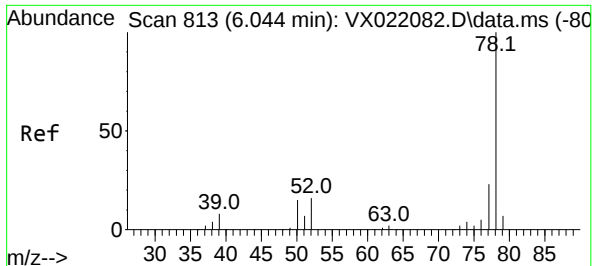

#40
Benzene
Concen: 1.33 ug/l
RT: 6.050 min Scan# 814
Delta R.T. 0.006 min
Lab File: VX022378.D
Acq: 03 Jun 2021 19:55




Instrument :
MSVOA_X
ClientSampled :
COMP-4-6


Tgt Ion: 78 Resp: 5135
Ion Ratio Lower Upper
78 100
77 26.0 18.9 28.3

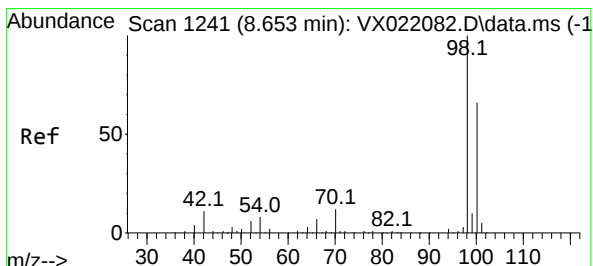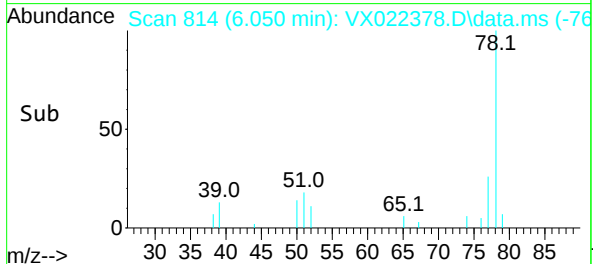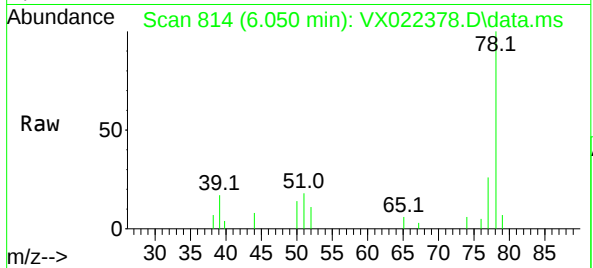

#50
Toluene-d8
Concen: 51.16 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX022378.D
Acq: 03 Jun 2021 19:55

Tgt Ion: 98 Resp: 169007
Ion Ratio Lower Upper
98 100
100 65.0 51.9 77.9


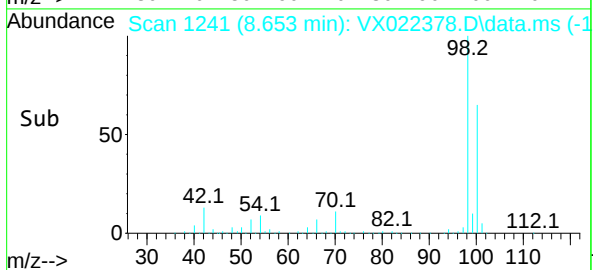

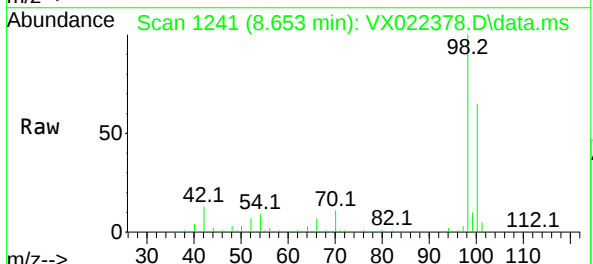


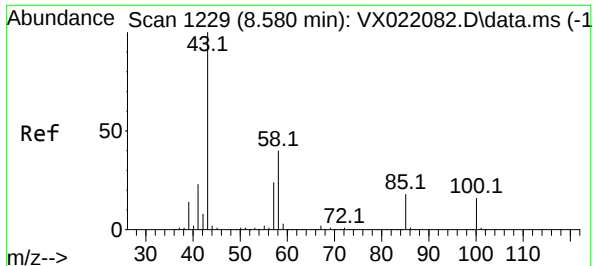

#51
4-Methyl-2-Pentanone
Concen: 0.28 ug/l
RT: 8.592 min Scan# 1231
Delta R.T. 0.012 min
Lab File: VX022378.D
Acq: 03 Jun 2021 19:55




Instrument :
MSVOA_X
ClientSampleId :
COMP-4-6


Tgt Ion: 43 Resp: 417
Ion Ratio Lower Upper
43 100
58 0.0 35.4 53.0#

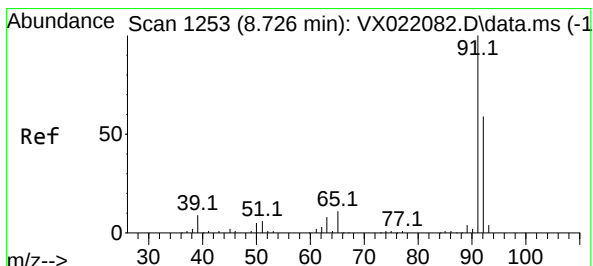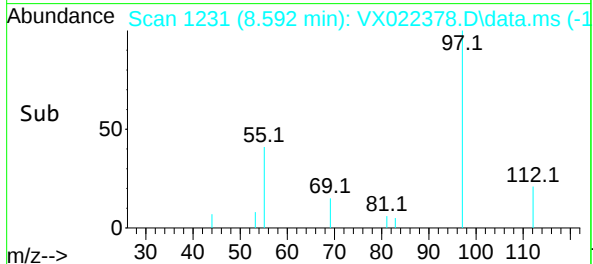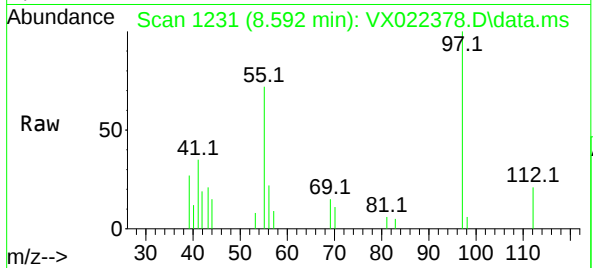

#52
Toluene
Concen: 3.14 ug/l
RT: 8.720 min Scan# 1252
Delta R.T. -0.006 min
Lab File: VX022378.D
Acq: 03 Jun 2021 19:55

Tgt Ion: 92 Resp: 7660
Ion Ratio Lower Upper
92 100
91 161.2 137.1 205.7


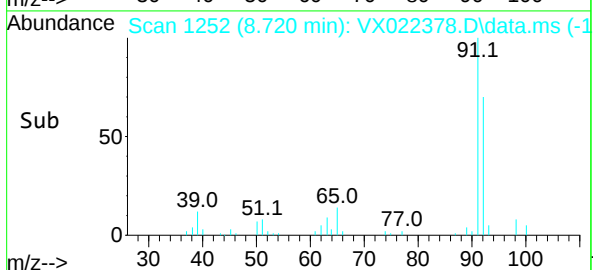

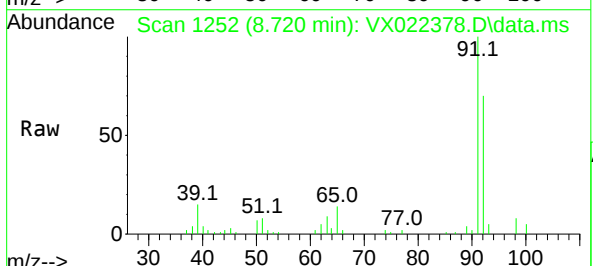




#55
1,1,2-Trichloroethane
Concen: 0.70 ug/l
RT: 9.104 min Scan# 1315
Delta R.T. -0.055 min
Lab File: VX022378.D
Acq: 03 Jun 2021 19:55




Instrument :
MSVOA_X
ClientSampleId :
COMP-4-6


Tgt Ion: 97	Resp: 696
Ion Ratio	Lower Upper
97 100	
83 0.0	69.3 103.9#
85 0.0	44.3 66.5#
99 0.0	50.3 75.5#



#62
4-Bromofluorobenzene
Concen: 50.22 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX022378.D
Acq: 03 Jun 2021 19:55

Tgt Ion: 95	Resp: 61320
Ion Ratio	Lower Upper
95 100	
174 63.5	0.0 154.6
176 60.3	0.0 155.8


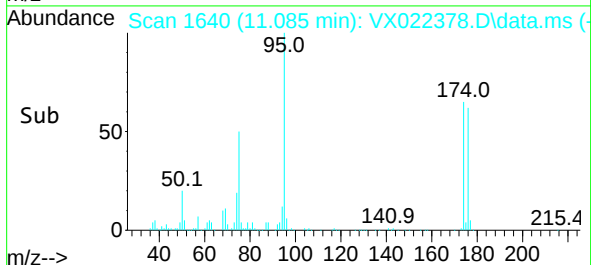

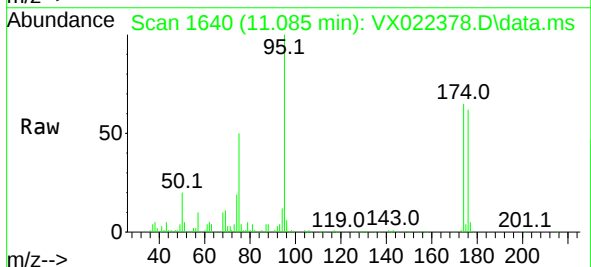




#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.006 min
Lab File: VX022378.D
Acq: 03 Jun 2021 19:55




Instrument :
MSVOA_X
ClientSampleId :
COMP-4-6


Tgt Ion:117 Resp: 122491
Ion Ratio Lower Upper
117 100
82 59.2 47.4 71.2
119 29.6 26.6 39.8

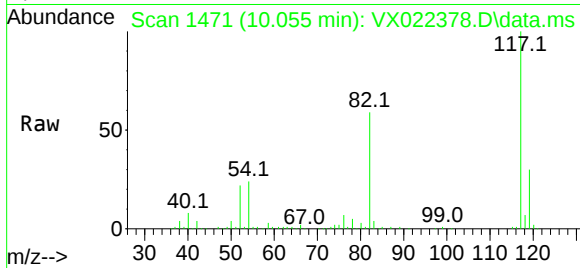

#67
Ethyl Benzene
Concen: 0.96 ug/l
RT: 10.195 min Scan# 1494
Delta R.T. 0.000 min
Lab File: VX022378.D
Acq: 03 Jun 2021 19:55

Tgt Ion: 91 Resp: 4490
Ion Ratio Lower Upper
91 100
106 31.3 24.6 37.0


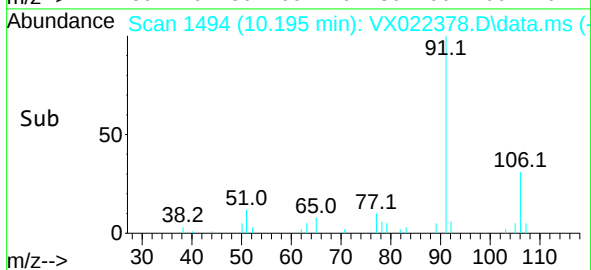

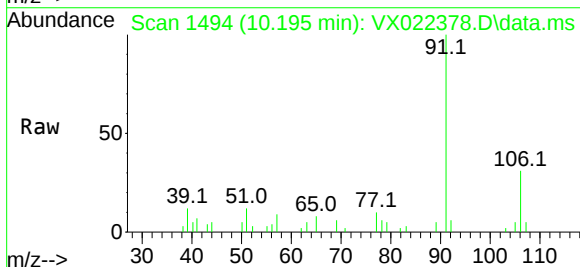




#68
m/p-Xylenes
Concen: 5.83 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. -0.000 min
Lab File: VX022378.D
Acq: 03 Jun 2021 19:55




Instrument :
MSVOA_X
ClientSampleId :
COMP-4-6


Tgt Ion:106 Resp: 10329
Ion Ratio Lower Upper
106 100
91 204.6 162.8 244.2

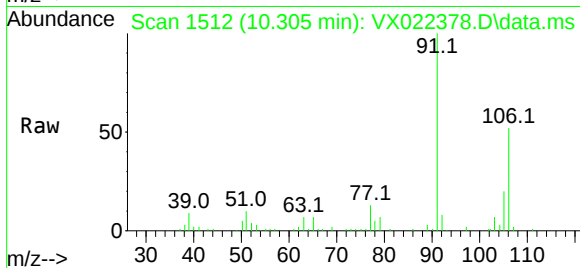

#69
o-Xylene
Concen: 1.97 ug/l
RT: 10.646 min Scan# 1568
Delta R.T. -0.001 min
Lab File: VX022378.D
Acq: 03 Jun 2021 19:55

Tgt Ion:106 Resp: 3398
Ion Ratio Lower Upper
106 100
91 244.9 108.1 324.2


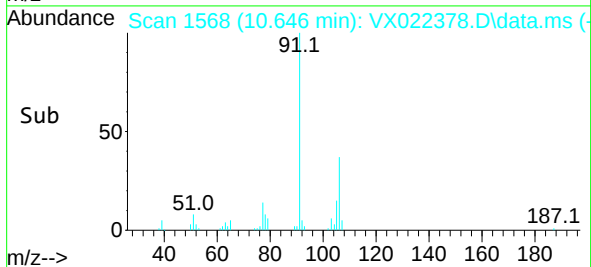

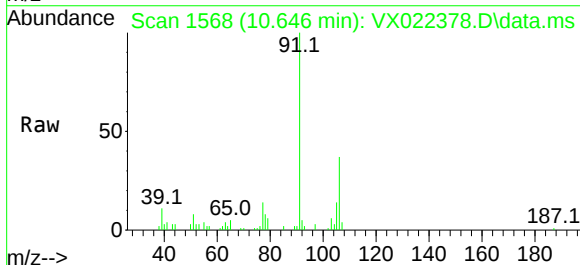




#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX022378.D
Acq: 03 Jun 2021 19:55




Instrument :
MSVOA_X
ClientSampled :
COMP-4-6


Tgt Ion:152 Resp: 52272
Ion Ratio Lower Upper
152 100
115 64.5 41.1 123.3
150 154.1 0.0 349.0

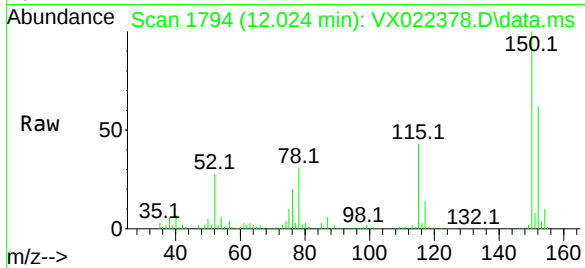

#73
Isopropylbenzene
Concen: 0.31 ug/l
RT: 10.963 min Scan# 1620
Delta R.T. -0.001 min
Lab File: VX022378.D
Acq: 03 Jun 2021 19:55

Tgt Ion:105 Resp: 1356
Ion Ratio Lower Upper
105 100
120 21.5 13.2 39.6


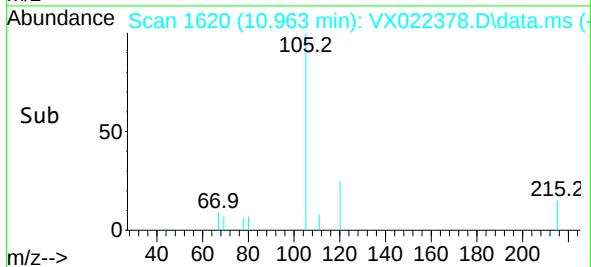

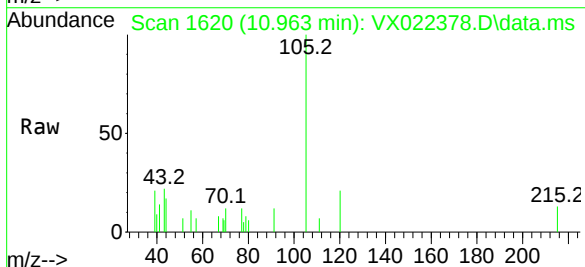




#76
1,2,3-Trichloropropane
Concen: 24.41 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. -0.159 min
Lab File: VX022378.D
Acq: 03 Jun 2021 19:55




Instrument :
MSVOA_X
ClientSampleId :
COMP-4-6


Tgt Ion: 75 Resp: 31472
Ion Ratio Lower Upper
75 100
77 1.7 19.1 57.5#

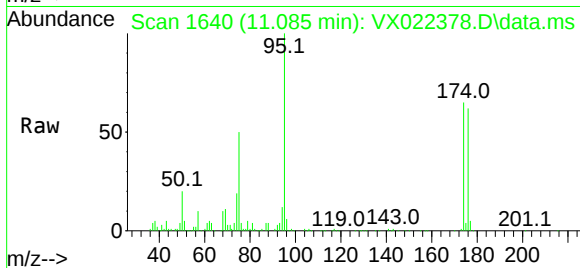

#78
n-propylbenzene
Concen: 0.46 ug/l
RT: 11.305 min Scan# 1676
Delta R.T. -0.000 min
Lab File: VX022378.D
Acq: 03 Jun 2021 19:55

Tgt Ion: 91 Resp: 2409
Ion Ratio Lower Upper
91 100
120 24.1 11.5 34.5


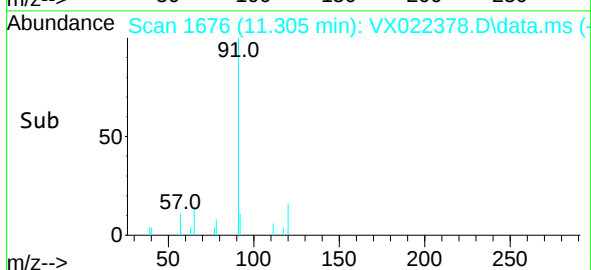

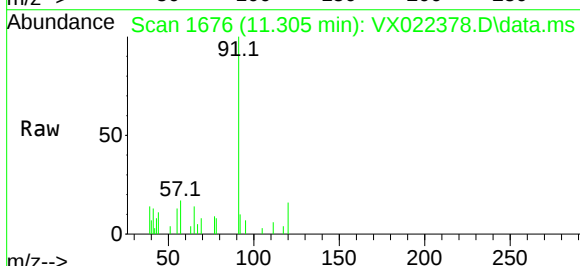




#79
2-Chlorotoluene
Concen: 0.52 ug/l
RT: 11.378 min Scan# 1688
Delta R.T. 0.012 min
Lab File: VX022378.D
Acq: 03 Jun 2021 19:55




Instrument :
MSVOA_X
ClientSampled :
COMP-4-6


Tgt Ion: 91 Resp: 1623
Ion Ratio Lower Upper
91 100
126 0.0 16.6 49.8#

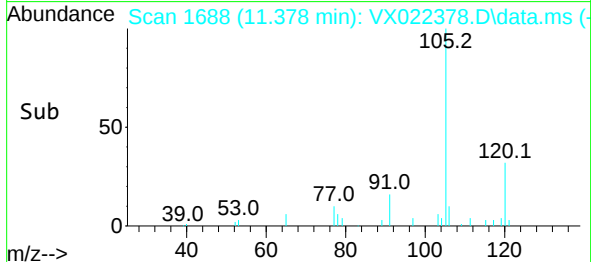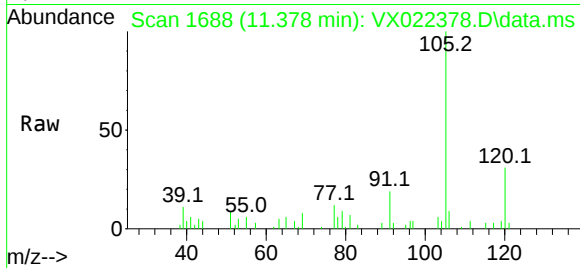

#80
1,3,5-Trimethylbenzene
Concen: 1.77 ug/l
RT: 11.457 min Scan# 1701
Delta R.T. 0.000 min
Lab File: VX022378.D
Acq: 03 Jun 2021 19:55

Tgt Ion: 105 Resp: 6487
Ion Ratio Lower Upper
105 100
120 45.2 23.8 71.5


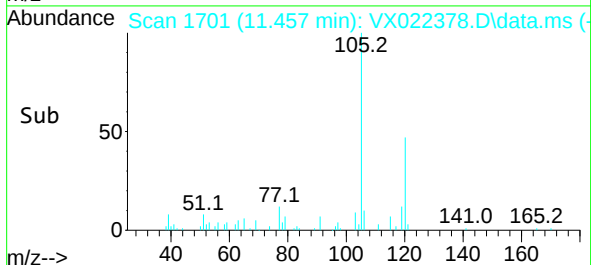

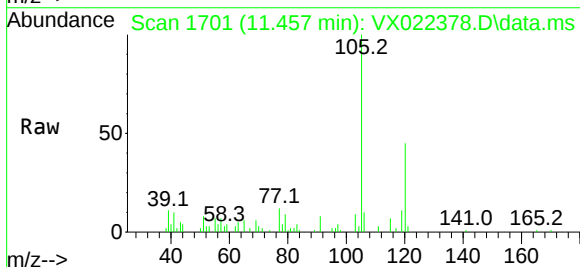




#81
trans-1,4-Dichloro-2-butene
Concen: 57.82 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.060 min
Lab File: VX022378.D
Acq: 03 Jun 2021 19:55




Instrument :
MSVOA_X
ClientSampleId :
COMP-4-6


Tgt Ion: 75 Resp: 31472
Ion Ratio Lower Upper
75 100
53 0.7 74.5 111.7#
89 0.1 37.9 56.9#

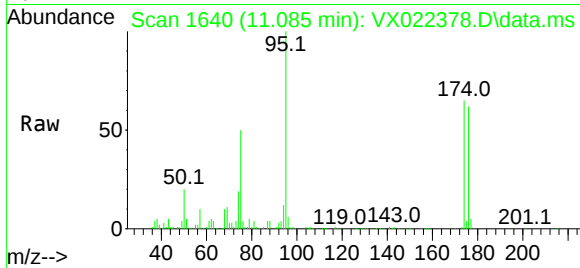

#82
4-Chlorotoluene
Concen: 0.25 ug/l
RT: 11.451 min Scan# 1700
Delta R.T. -0.006 min
Lab File: VX022378.D
Acq: 03 Jun 2021 19:55

Tgt Ion: 91 Resp: 899
Ion Ratio Lower Upper
91 100
126 0.0 14.9 44.5#


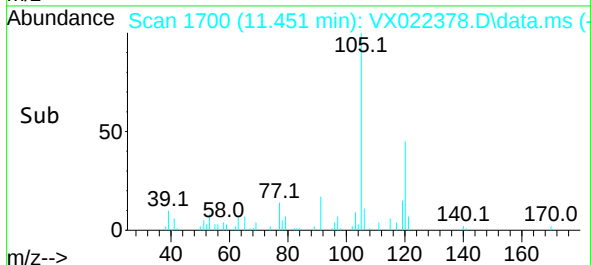

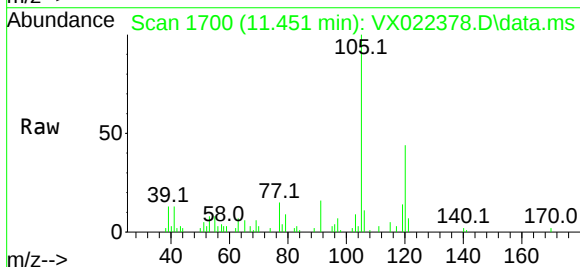




#83
tert-Butylbenzene
Concen: 0.44 ug/l
RT: 11.975 min Scan# 1786
Delta R.T. 0.255 min
Lab File: VX022378.D
Acq: 03 Jun 2021 19:55




Instrument :
MSVOA_X
ClientSampleId :
COMP-4-6


Tgt Ion:119 Resp: 1538
Ion Ratio Lower Upper
119 100
91 35.5 27.9 83.7
134 22.0 11.3 33.9

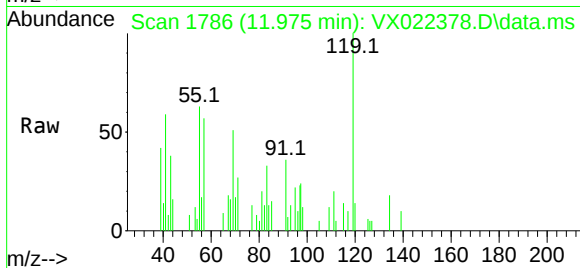

#84
1,2,4-Trimethylbenzene
Concen: 3.52 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.000 min
Lab File: VX022378.D
Acq: 03 Jun 2021 19:55

Tgt Ion:105 Resp: 12997
Ion Ratio Lower Upper
105 100
120 41.5 22.4 67.3


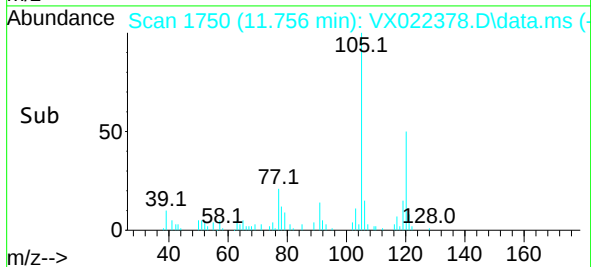

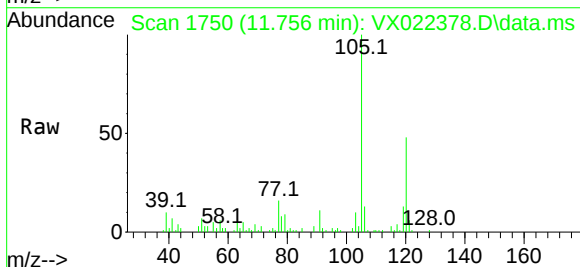




#85
sec-Butylbenzene
Concen: 0.21 ug/l
RT: 11.890 min Scan# 1772
Delta R.T. -0.006 min
Lab File: VX022378.D
Acq: 03 Jun 2021 19:55




Instrument :
MSVOA_X
ClientSampled :
COMP-4-6


Tgt Ion:105 Resp: 956
Ion Ratio Lower Upper
105 100
134 19.1 10.0 29.8



#86
p-Isopropyltoluene
Concen: 0.28 ug/l
RT: 12.012 min Scan# 1792
Delta R.T. -0.000 min
Lab File: VX022378.D
Acq: 03 Jun 2021 19:55

Tgt Ion:119 Resp: 1068
Ion Ratio Lower Upper
119 100
134 27.7 12.9 38.7
91 49.7 11.7 35.0#


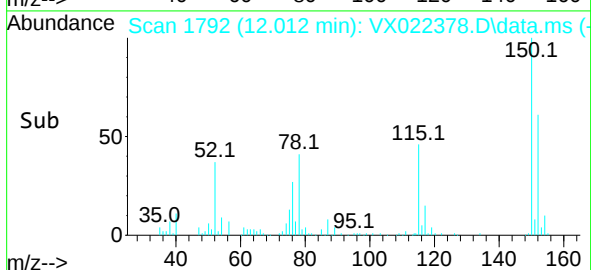

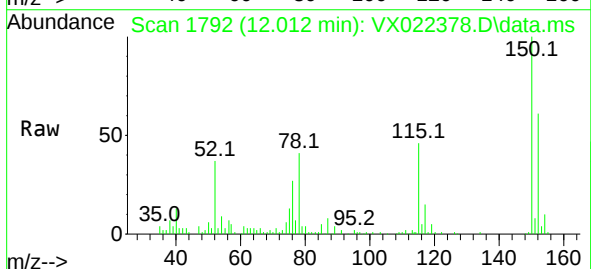




#89
n-Butylbenzene
Concen: 0.73 ug/l
RT: 12.329 min Scan# 1844
Delta R.T. -0.006 min
Lab File: VX022378.D
Acq: 03 Jun 2021 19:55




Instrument :
MSVOA_X
ClientSampleId :
COMP-4-6


Tgt Ion: 91 Resp: 2546
Ion Ratio Lower Upper
91 100
92 28.9 27.4 82.0
134 71.0 13.2 39.5#

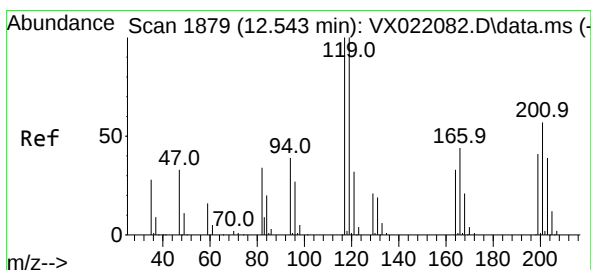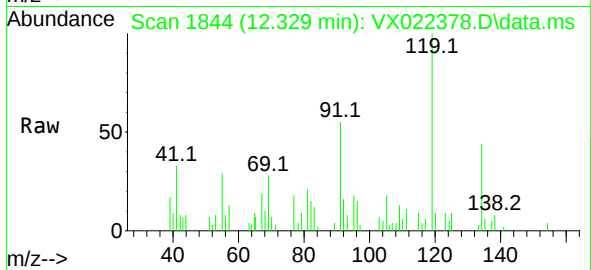

#90
Hexachloroethane
Concen: 0.54 ug/l
RT: 12.536 min Scan# 1878
Delta R.T. -0.007 min
Lab File: VX022378.D
Acq: 03 Jun 2021 19:55

Tgt Ion: 117 Resp: 334
Ion Ratio Lower Upper
117 100
201 0.0 40.4 121.2#


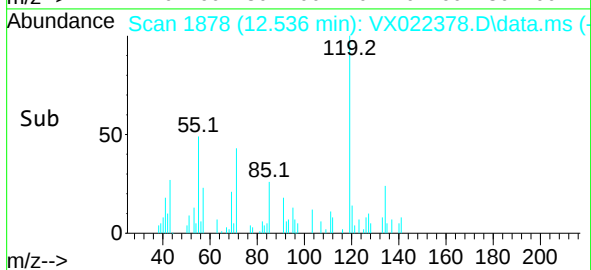

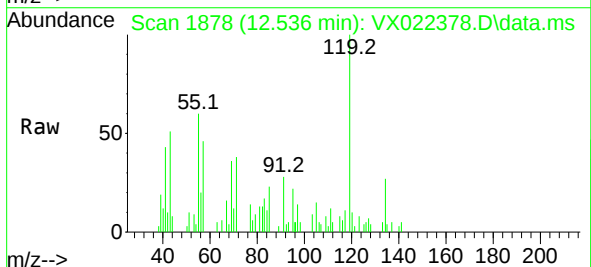




#93
1,2,4-Trichlorobenzene
Concen: 0.23 ug/l
RT: 13.847 min Scan# 2093
Delta R.T. 0.256 min
Lab File: VX022378.D
Acq: 03 Jun 2021 19:55




Instrument :
MSVOA_X
ClientSampled :
COMP-4-6


Tgt Ion:180 Resp: 245
Ion Ratio Lower Upper
180 100
182 133.9 47.7 143.1
145 41.2 15.0 45.0

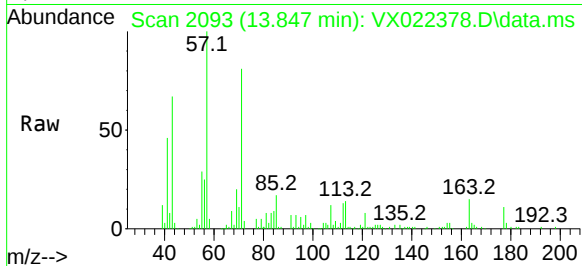

#95
Naphthalene
Concen: 1.69 ug/l
RT: 13.780 min Scan# 2082
Delta R.T. -0.000 min
Lab File: VX022378.D
Acq: 03 Jun 2021 19:55


Tgt Ion:128 Resp: 6895
Ion Ratio Lower Upper
128 100
127 22.4 10.3 15.5#
129 18.4 8.8 13.2#

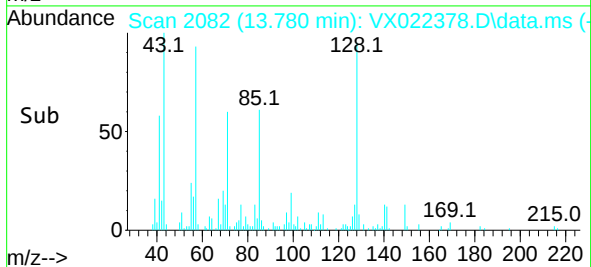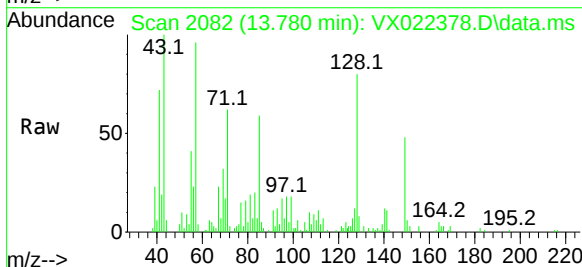

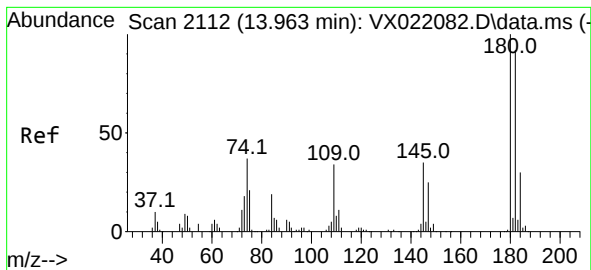

#96
 1,2,3-Trichlorobenzene
 Concen: 0.49 ug/l
 RT: 13.847 min Scan# 2093
 Delta R.T. -0.116 min
 Lab File: VX022378.D
 Acq: 03 Jun 2021 19:55

Instrument :
 MSVOA_X
 ClientSampleId :
 COMP-4-6

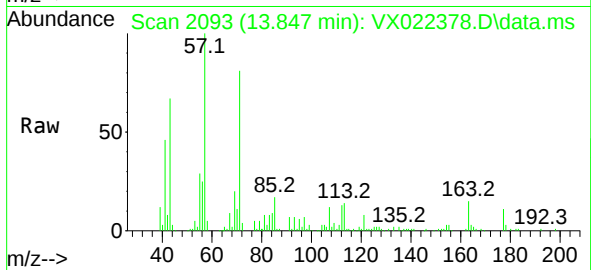

Tgt Ion:180 Resp: 518
 Ion Ratio Lower Upper
 180 100
 182 63.3 47.6 142.9
 145 45.9 16.1 48.3

