

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX060321\  
 Data File : VX022374.D  
 Acq On : 03 Jun 2021 18:21  
 Operator : JC/MD  
 Sample : M2583-20 50X  
 Misc : 5.0mL/MSVOA\_X/WATER  
 ALS Vial : 24 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 35-38

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X051921W.M

Title : SW846 8260

Signal : TIC: VX022374.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.568       | 73            | 79          | 83           | rBV5     | 3622           | 6442          | 1.56%           | 0.303%        |
| 2         | 2.385       | 206           | 213         | 218          | rBV      | 3317           | 6363          | 1.54%           | 0.299%        |
| 3         | 2.952       | 297           | 306         | 315          | rBV2     | 1907           | 4948          | 1.20%           | 0.232%        |
| 4         | 4.586       | 565           | 574         | 581          | rBV2     | 2107           | 5272          | 1.27%           | 0.248%        |
| 5         | 5.397       | 696           | 707         | 720          | rVB      | 42872          | 124691        | 30.15%          | 5.857%        |
| 6         | 5.562       | 723           | 734         | 745          | rBV      | 70248          | 193493        | 46.78%          | 9.088%        |
| 7         | 5.964       | 791           | 800         | 814          | rBV      | 55594          | 147877        | 35.75%          | 6.946%        |
| 8         | 6.769       | 920           | 932         | 947          | rBV      | 125008         | 300461        | 72.64%          | 14.112%       |
| 9         | 8.653       | 1234          | 1241        | 1248         | rBV      | 262461         | 413631        | 100.00%         | 19.428%       |
| 10        | 8.720       | 1248          | 1252        | 1258         | rVB      | 10279          | 17260         | 4.17%           | 0.811%        |
| 11        | 10.061      | 1466          | 1472        | 1489         | rVB      | 249308         | 351297        | 84.93%          | 16.500%       |
| 12        | 11.085      | 1634          | 1640        | 1651         | rBV      | 196087         | 244782        | 59.18%          | 11.497%       |
| 13        | 12.024      | 1789          | 1794        | 1801         | rVB      | 250301         | 296248        | 71.62%          | 13.915%       |
| 14        | 12.859      | 1928          | 1931        | 1938         | rBV3     | 3394           | 5311          | 1.28%           | 0.249%        |
| 15        | 13.109      | 1968          | 1972        | 1976         | rBV5     | 3096           | 4874          | 1.18%           | 0.229%        |
| 16        | 13.731      | 2071          | 2074        | 2083         | rVB6     | 3639           | 6093          | 1.47%           | 0.286%        |




Sum of corrected areas: 2129043

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX060321\  
Data File : VX022374.D  
Acq On : 03 Jun 2021 18:21  
Operator : JC/MD  
Sample : M2583-20 50X  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 24 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
35-38

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X051921W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

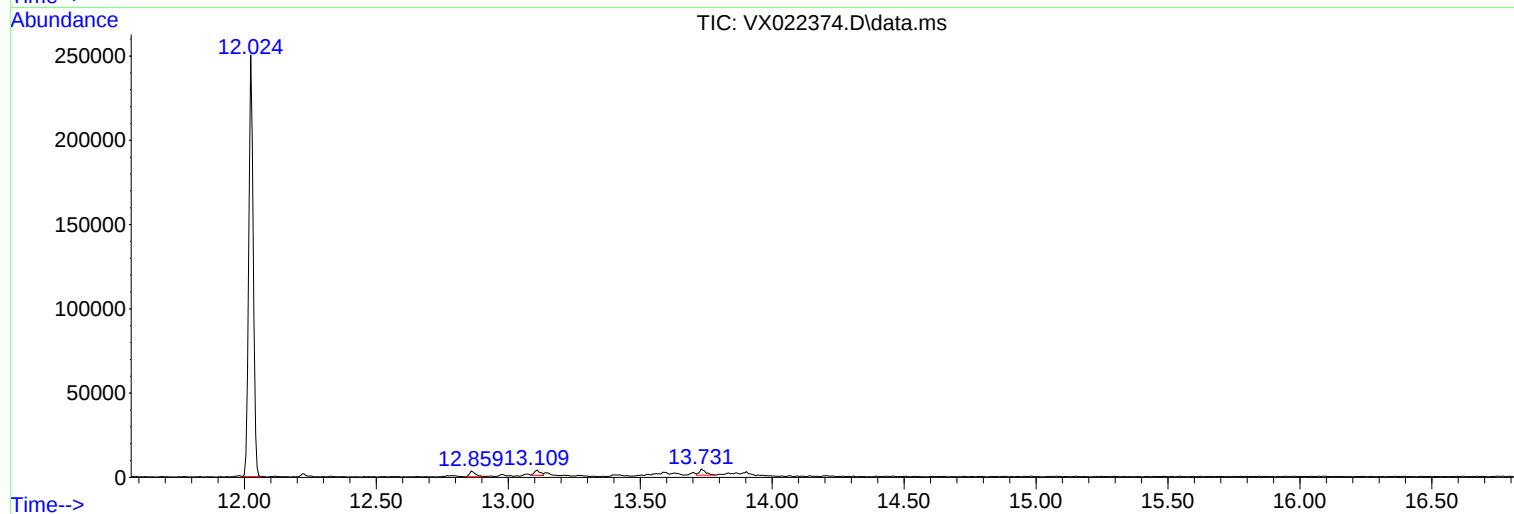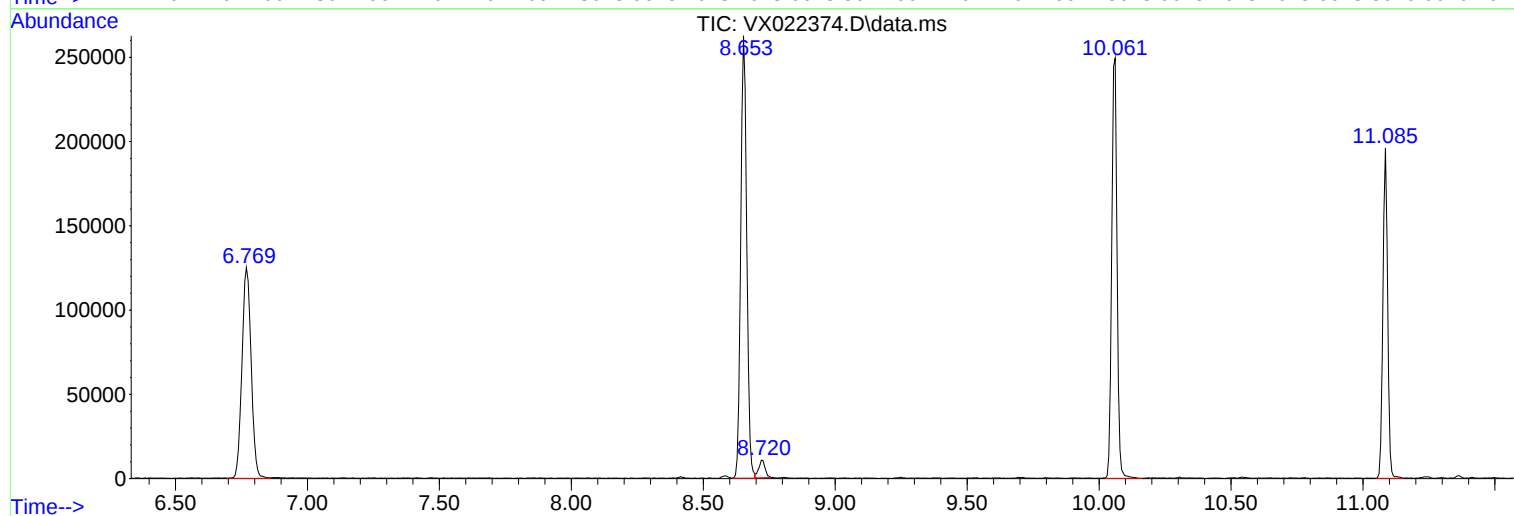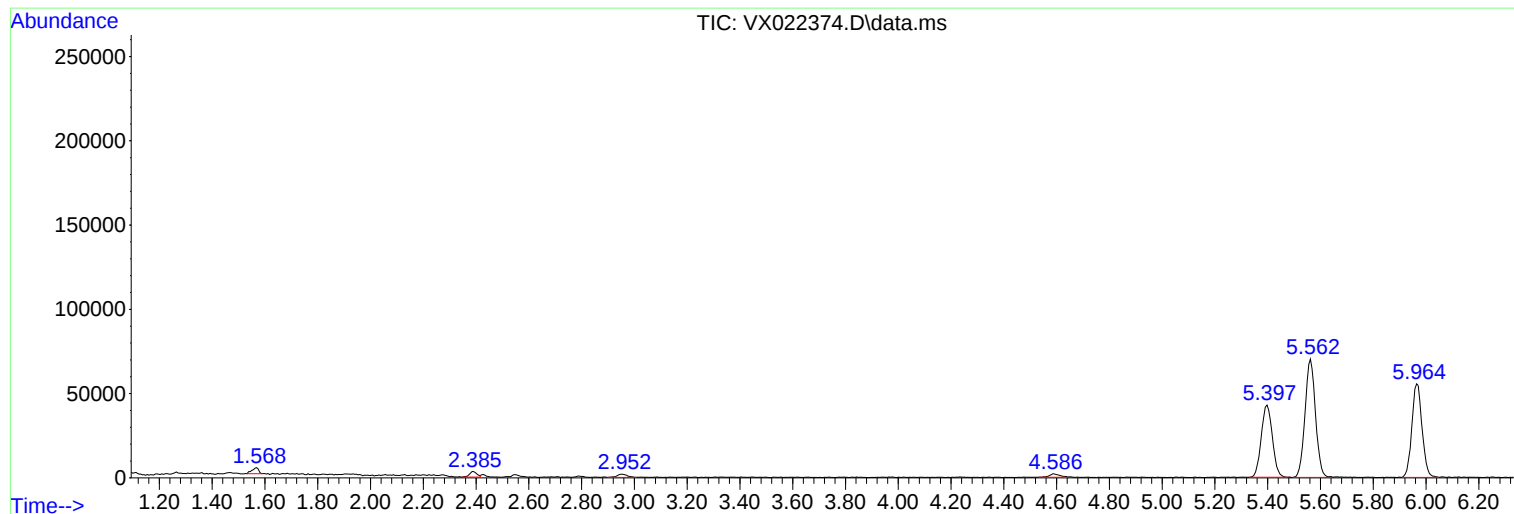

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX060321\  
Data File : VX022374.D  
Acq On : 03 Jun 2021 18:21  
Operator : JC/MD  
Sample : M2583-20 50X  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 24 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
35-38

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X051921W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_X\Data\VX060321\  
Data File : VX022374.D  
Acq On : 03 Jun 2021 18:21  
Operator : JC/MD  
Sample : M2583-20 50X  
Misc : 5.0mL/MSVOA\_X/WATER  
ALS Vial : 24 Sample Multiplier: 1

Instrument :  
MSVOA\_X  
ClientSampleId :  
35-38

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_X\Method\82X051921W.M  
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | --Internal Standard-- |    |      |      |
|------------------|----|---------|-------|----------|-----------------------|----|------|------|
|                  |    |         |       |          | #                     | RT | Resp | Conc |

-----