

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060322\
 Data File : VX029193.D
 Acq On : 03 Jun 2022 16:26
 Operator : JC/MD
 Sample : N3164-10
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 32S-20220531

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M

Title : SW846 8260

Signal : TIC: VX029193.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.270	24	30	39	rBV4	10996	25357	1.43%	0.255%
2	4.715	585	595	610	rBV	80420	229857	12.95%	2.316%
3	5.391	694	706	721	rBV	214760	629385	35.46%	6.341%
4	5.556	721	733	746	rBV	325918	927756	52.27%	9.347%
5	5.958	789	799	812	rBV	213735	568722	32.04%	5.730%
6	6.763	921	931	944	rBV	539789	1287251	72.53%	12.968%
7	8.653	1234	1241	1257	rBV	1125338	1774892	100.00%	17.881%
8	10.055	1465	1471	1485	rBV	1240103	1632652	91.99%	16.448%
9	11.085	1634	1640	1650	rBV	953028	1243623	70.07%	12.529%
10	12.024	1788	1794	1803	rBV	1289259	1581036	89.08%	15.928%
11	12.219	1821	1826	1831	rBV	18413	25493	1.44%	0.257%




Sum of corrected areas: 9926024

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060322\
Data File : VX029193.D
Acq On : 03 Jun 2022 16:26
Operator : JC/MD
Sample : N3164-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
32S-20220531

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

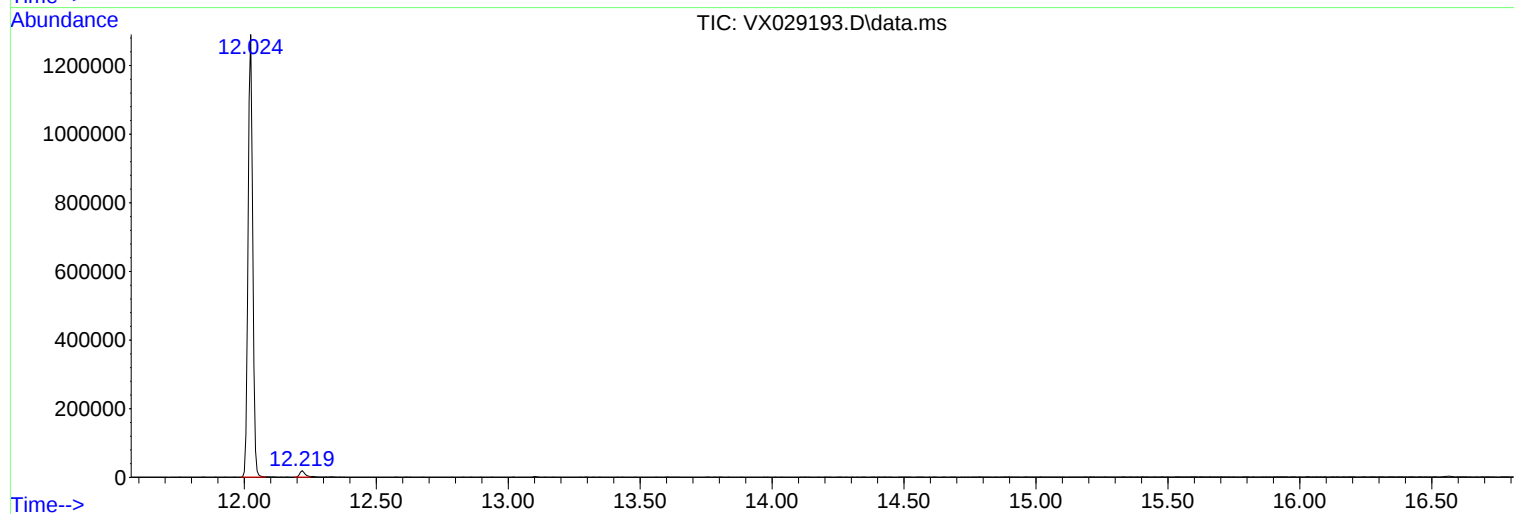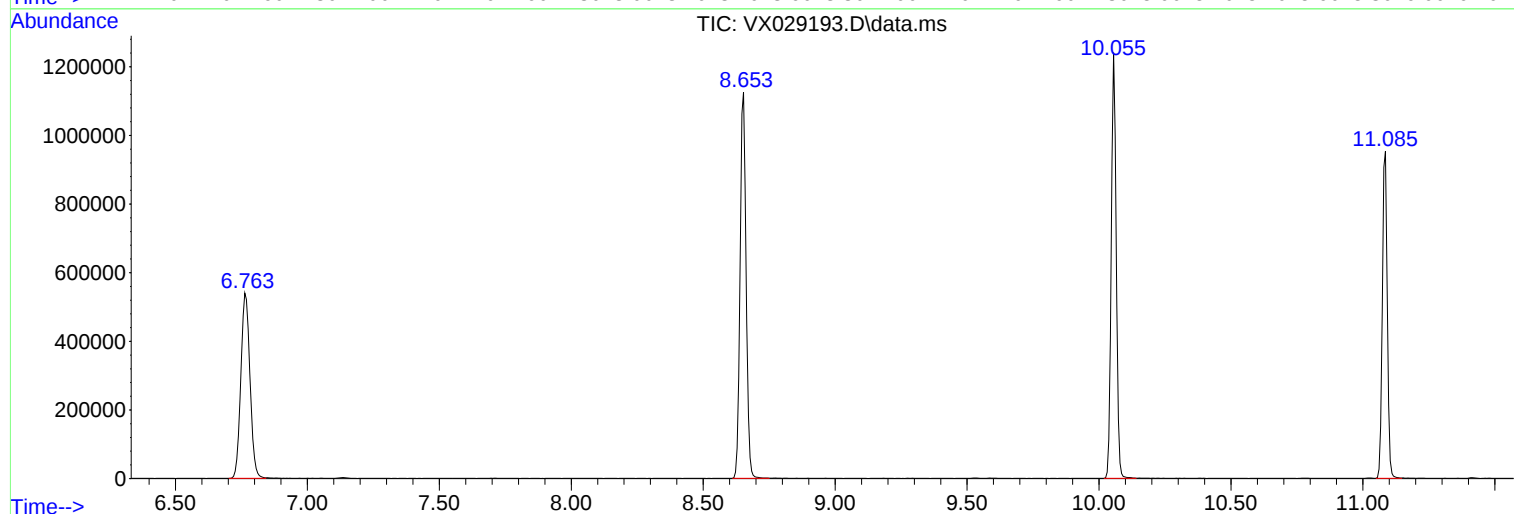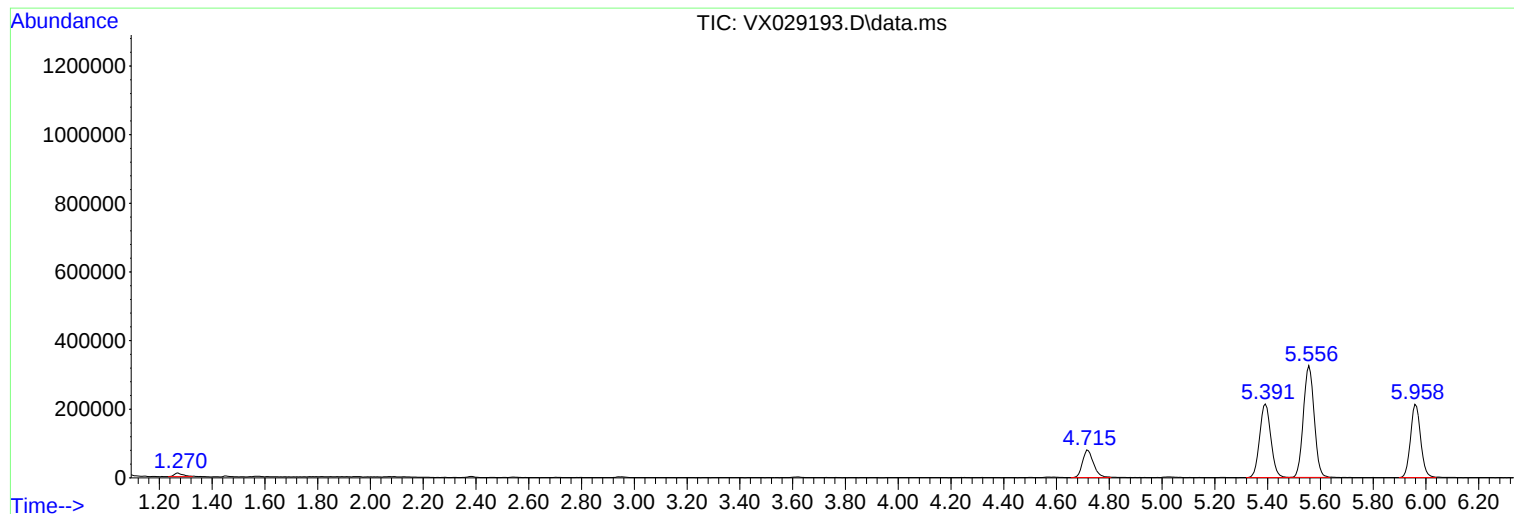

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060322\
Data File : VX029193.D
Acq On : 03 Jun 2022 16:26
Operator : JC/MD
Sample : N3164-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
32S-20220531

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060322\
Data File : VX029193.D
Acq On : 03 Jun 2022 16:26
Operator : JC/MD
Sample : N3164-10
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
32S-20220531

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------