

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060322\
 Data File : VX029203.D
 Acq On : 03 Jun 2022 20:18
 Operator : JC/MD
 Sample : N3022-09
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 91BR-20220525

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M

Title : SW846 8260

Signal : TIC: VX029203.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	56	rVB	1075399	1074577	13.36%	5.695%
2	4.489	545	558	581	rBV	2944172	8043632	100.00%	42.626%
3	5.391	694	706	722	rBV	208455	615441	7.65%	3.261%
4	5.556	722	733	750	rVB	317564	906767	11.27%	4.805%
5	5.958	787	799	816	rBV	213083	559120	6.95%	2.963%
6	6.763	921	931	946	rBV	537248	1269170	15.78%	6.726%
7	7.129	982	991	1004	rBV	147739	318816	3.96%	1.690%
8	8.653	1234	1241	1255	rBV	1105724	1734760	21.57%	9.193%
9	10.055	1465	1471	1483	rBV	1187390	1589329	19.76%	8.422%
10	11.085	1634	1640	1651	rBV	917830	1215176	15.11%	6.440%
11	12.024	1788	1794	1805	rBV	1264152	1543527	19.19%	8.180%




Sum of corrected areas: 18870315

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060322\
Data File : VX029203.D
Acq On : 03 Jun 2022 20:18
Operator : JC/MD
Sample : N3022-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
91BR-20220525

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

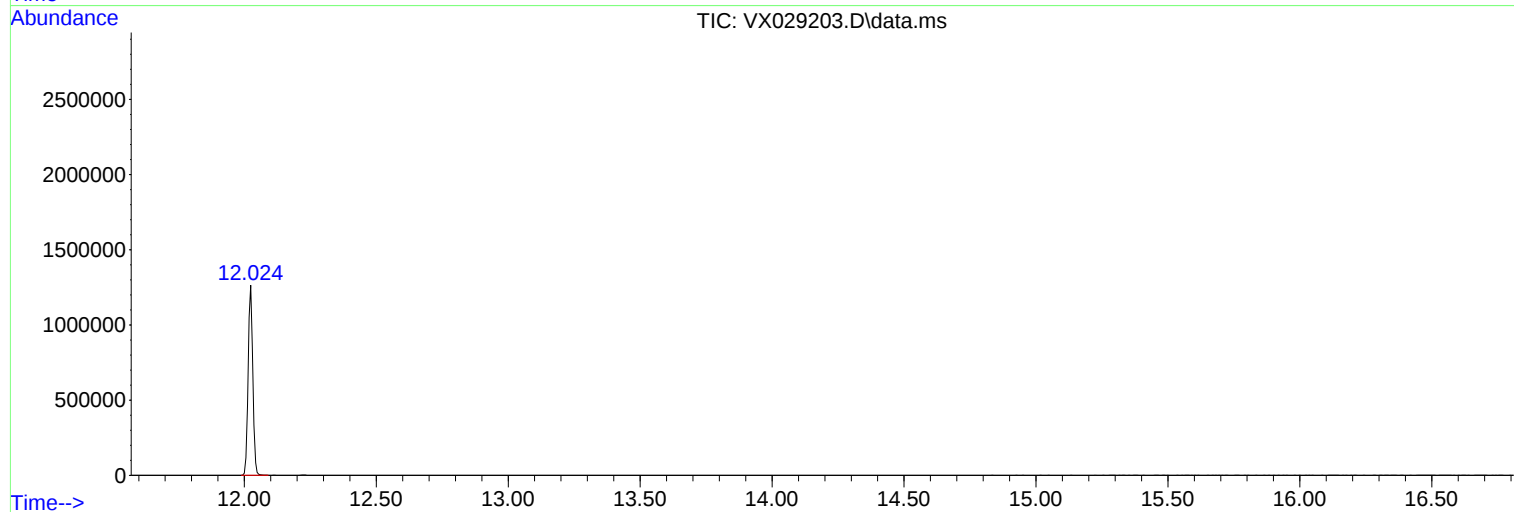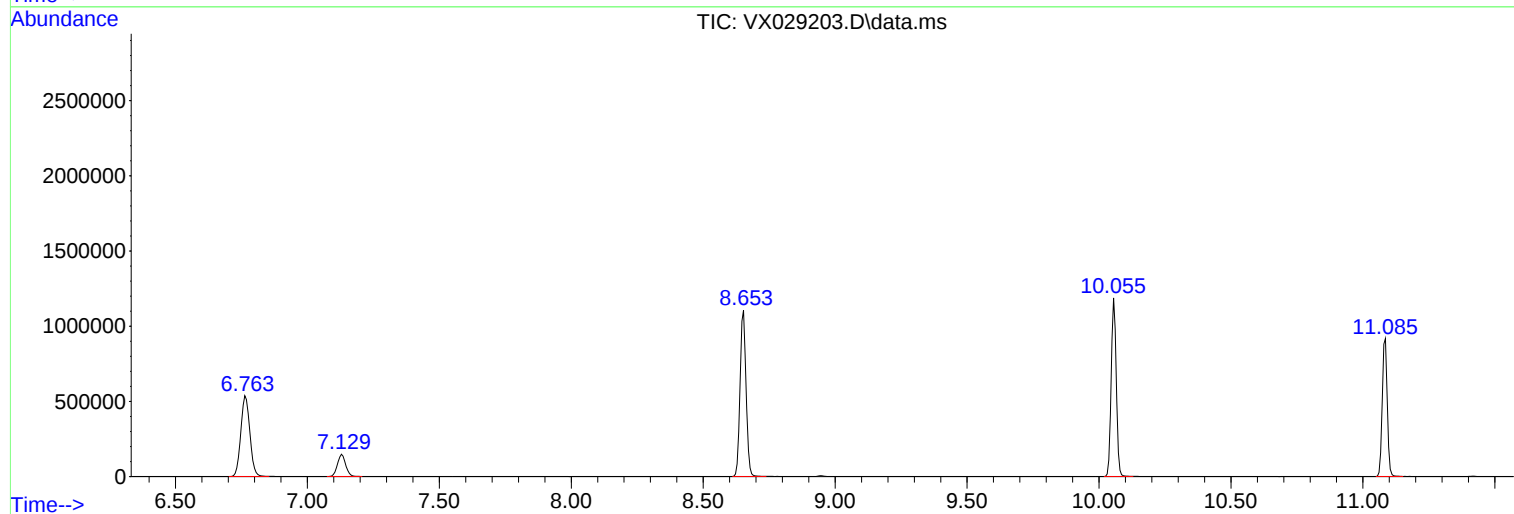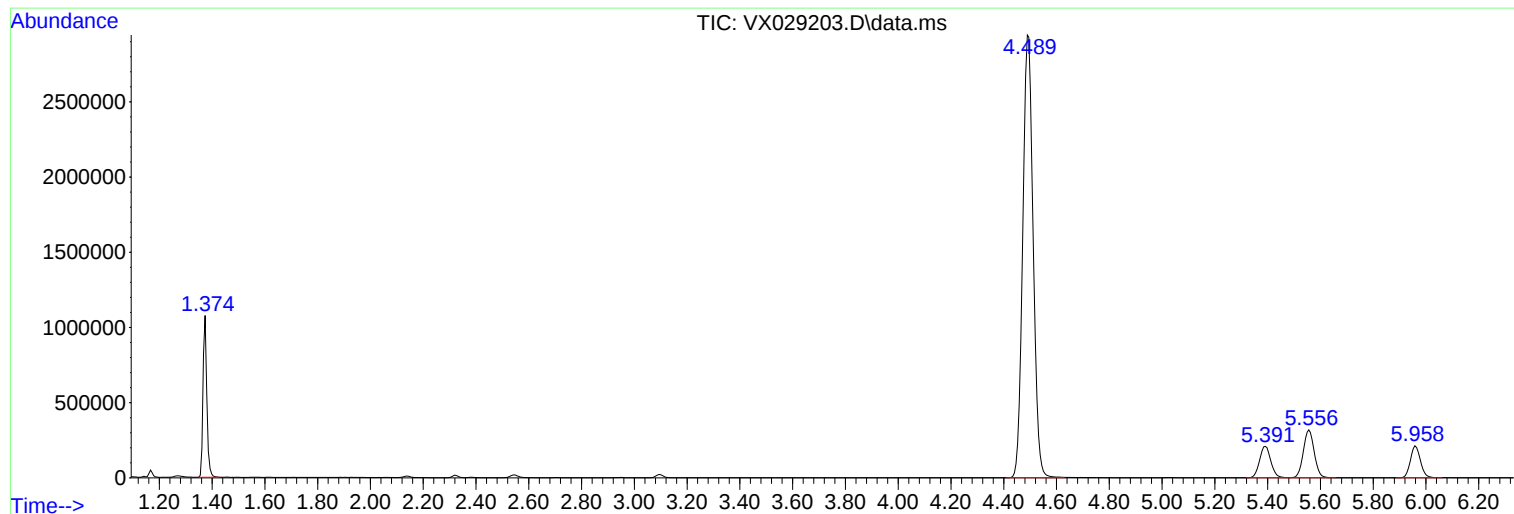

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060322\
Data File : VX029203.D
Acq On : 03 Jun 2022 20:18
Operator : JC/MD
Sample : N3022-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
91BR-20220525

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060322\
Data File : VX029203.D
Acq On : 03 Jun 2022 20:18
Operator : JC/MD
Sample : N3022-09
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
91BR-20220525

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc