
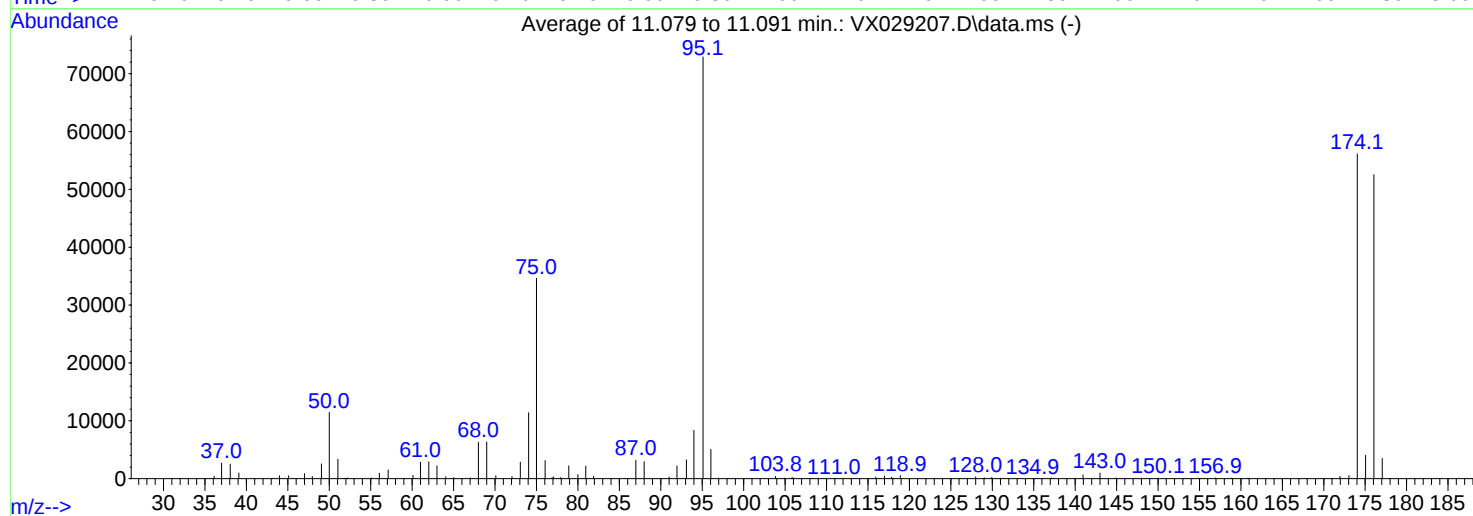


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060322\
 Data File : VX029207.D
 Acq On : 03 Jun 2022 21:51
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053122W.M
 Title : SW846 8260
 Last Update : Wed Jun 01 04:45:42 2022

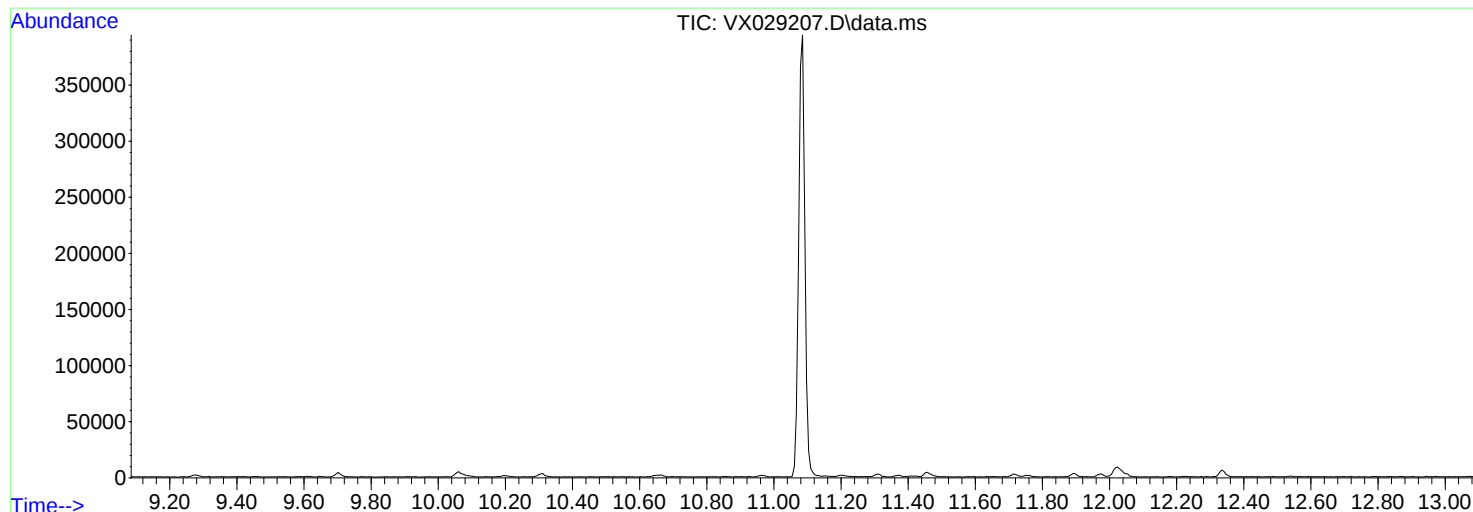

AutoFind: Scans 1639, 1640, 1641; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.7	11451	PASS
75	95	30	60	47.5	34616	PASS
95	95	100	100	100.0	72912	PASS
96	95	5	9	6.9	5060	PASS
173	174	0.00	2	1.0	541	PASS
174	95	50	100	77.0	56141	PASS
175	174	5	9	7.2	4030	PASS
176	174	95	101	93.6	52563	FAIL*
177	176	5	9	6.6	3495	PASS