


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX060519\
Data File : VX010092.D
Acq On : 05 Jun 2019 21:08
Operator : JC/SP
Sample : BFB
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X052819W.M
Title : SW846 8260
Last Update : Wed May 29 04:00:56 2019

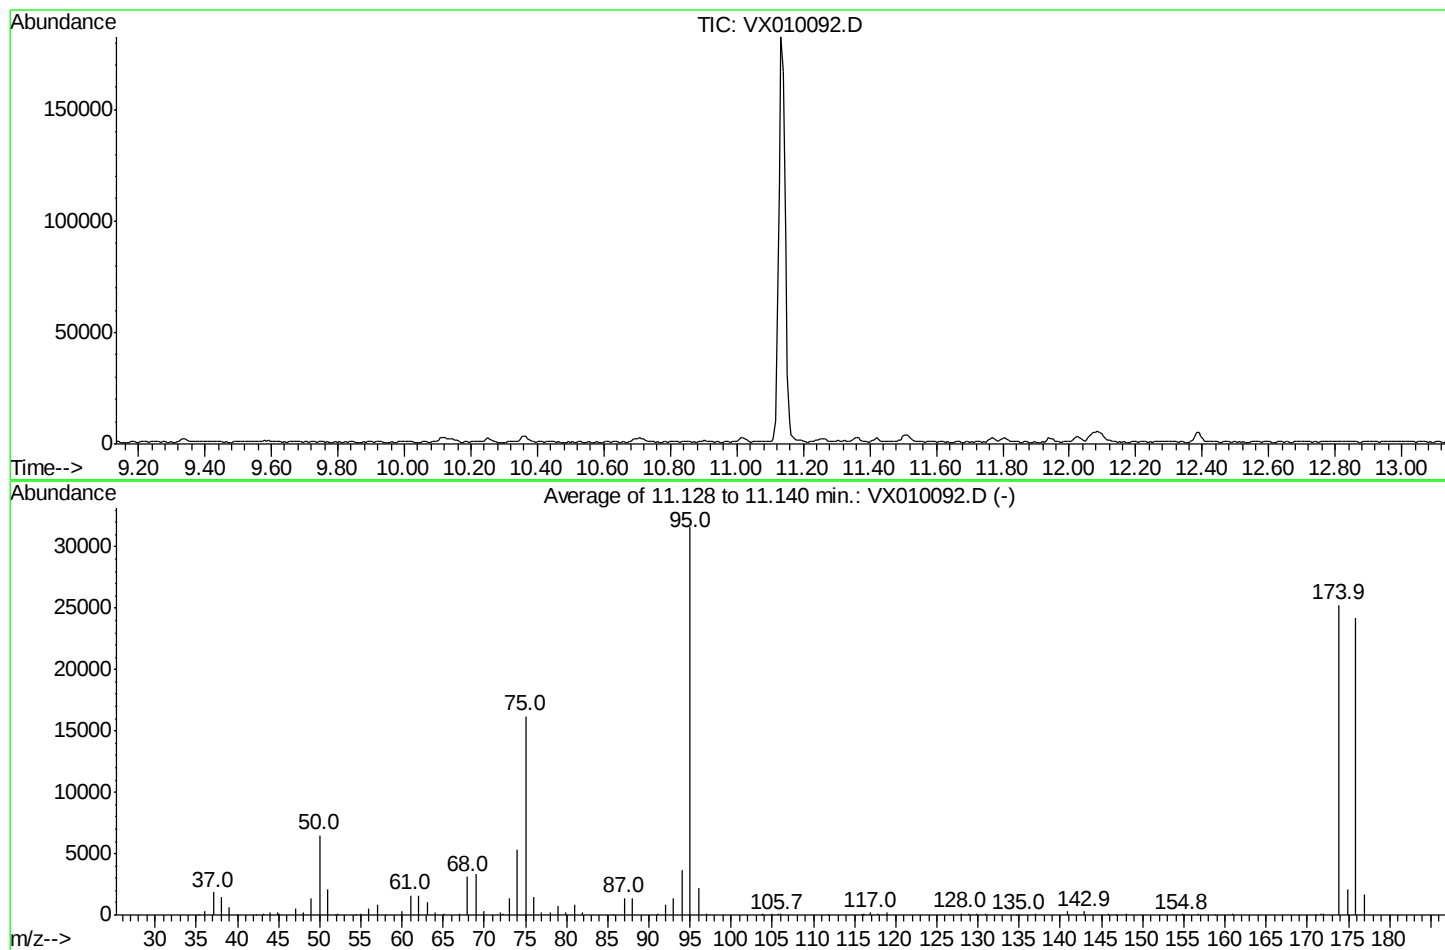

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	6472	PASS
75	95	30	60	51.2	16175	PASS
95	95	100	100	100.0	31592	PASS
96	95	5	9	6.9	2167	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	80.0	25287	PASS
175	174	5	9	8.2	2072	PASS
176	174	95	101	95.6	24169	PASS
177	176	5	9	7.1	1704	PASS