
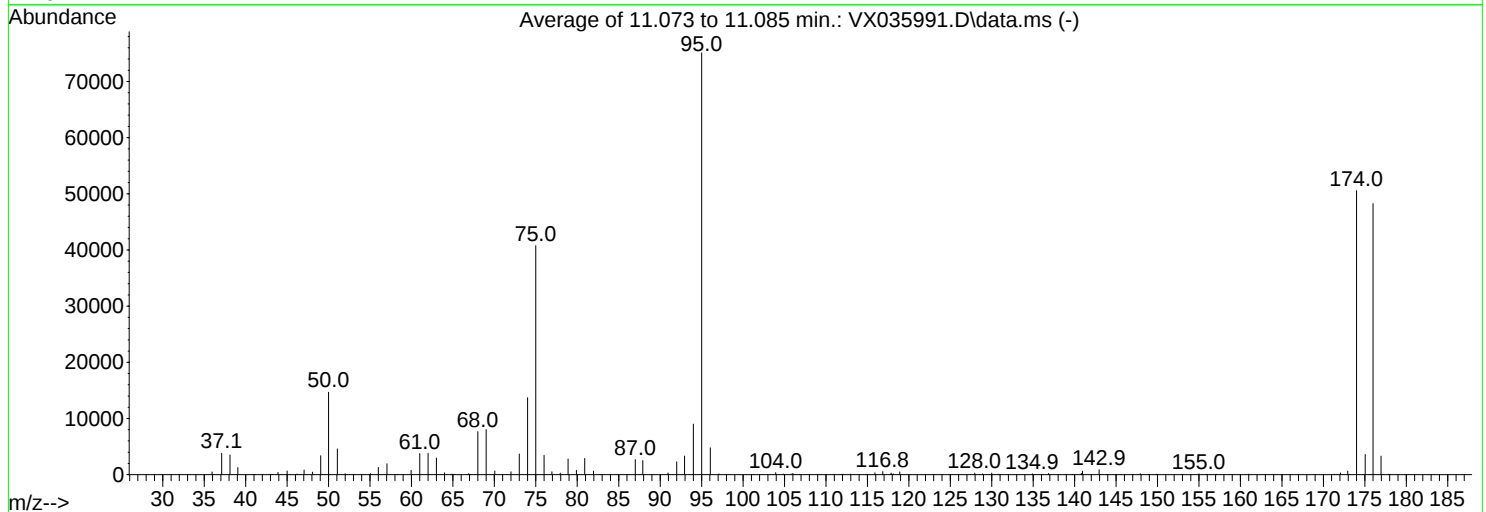


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060523\
Data File : VX035991.D
Acq On : 05 Jun 2023 09:00
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X053123W.M
Title : SW846 8260
Last Update : Wed May 31 12:50:30 2023

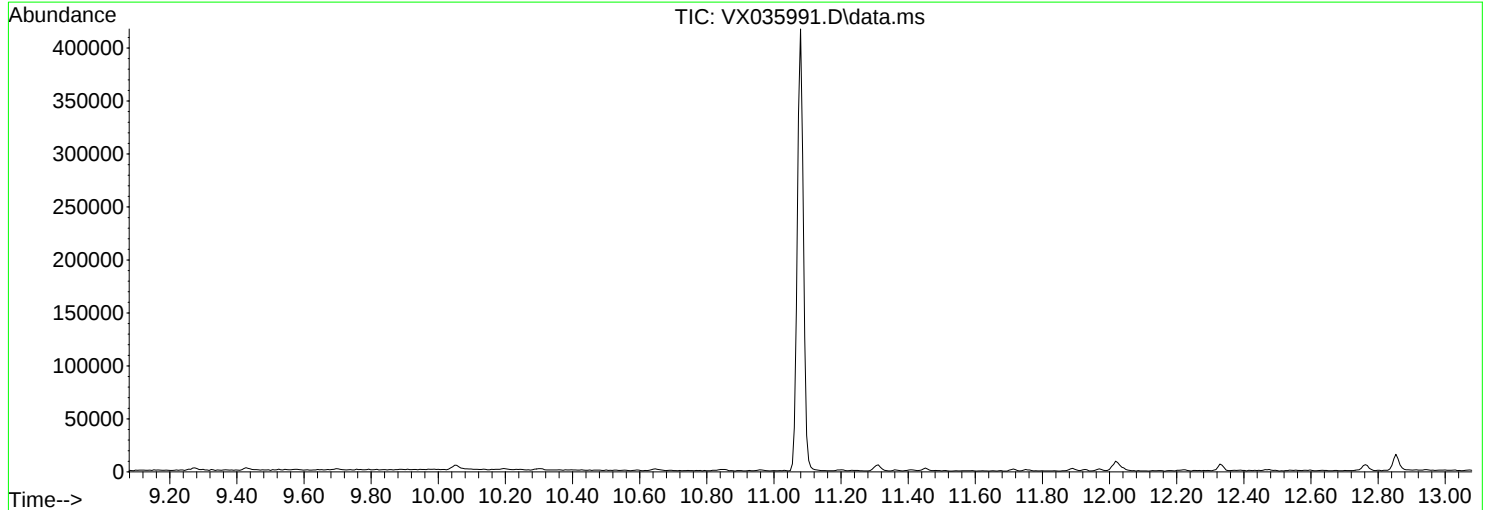

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.5	14669	PASS
75	95	30	60	54.3	40771	PASS
95	95	100	100	100.0	75099	PASS
96	95	5	9	6.4	4799	PASS
173	174	0.00	2	1.2	620	PASS
174	95	50	100	67.3	50576	PASS
175	174	5	9	7.1	3598	PASS
176	174	95	101	95.4	48264	PASS
177	176	5	9	6.8	3301	PASS