

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060621\
 Data File : VX022506.D
 Acq On : 07 Jun 2021 03:09
 Operator : JC/MD
 Sample : PB136857TB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PB136857TB

Quant Time: Jun 07 06:17:48 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
 Quant Title : SW846 8260
 QLast Update : Wed May 19 14:23:10 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	61480	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	123584	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	113304	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	43641	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	49960	52.680	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	105.360%
35) Dibromofluoromethane	5.397	113	36696	46.823	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	93.640%
50) Toluene-d8	8.653	98	155055	51.361	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	102.720%
62) 4-Bromofluorobenzene	11.085	95	55711	49.927	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	99.860%
Target Compounds						
						Qvalue
5) Bromomethane	1.605	94	234	0.470	ug/l	83
10) Methyl Iodide	2.459	142	489	0.625	ug/l #	84
11) Tert butyl alcohol	2.946	59	1962	9.045	ug/l #	73
13) Acrolein	2.239	56	46	0.320	ug/l #	67
16) Acetone	2.392	43	8082	19.571	ug/l	88
17) Carbon Disulfide	2.507	76	591	0.320	ug/l #	75
18) Methyl Acetate	2.715	43	817	0.744	ug/l #	62
20) Methylene Chloride	2.794	84	4132	4.507	ug/l #	88
25) 2-Butanone	4.586	43	1766	2.643	ug/l	90
29) Tetrahydrofuran	5.037	42	721	1.813	ug/l #	52
36) 1,1-Dichloropropene	5.562	75	5877	5.143	ug/l #	47
38) Carbon Tetrachloride	5.562	117	7127	6.375	ug/l #	18
41) Methacrylonitrile	5.031	41	228	0.304	ug/l #	40
43) Isopropyl Acetate	6.354	43	11061	4.827	ug/l	97
48) Methyl methacrylate	7.598	41	3066	2.903	ug/l #	10
49) 1,4-Dioxane	7.799	88	24	1.167	ug/l #	1
51) 4-Methyl-2-Pentanone	8.555	43	40484	29.495	ug/l #	45
54) cis-1,3-Dichloropropene	8.555	75	18511	12.250	ug/l #	64
56) Ethyl methacrylate	9.348	69	327	0.224	ug/l #	1
57) 1,3-Dichloropropane	9.488	76	10485	6.794	ug/l #	42
59) 2-Hexanone	9.384	43	4992	4.836	ug/l #	19
68) m/p-Xylenes	10.305	106	403	0.246	ug/l	83
76) 1,2,3-Trichloropropane	11.085	75	29249	27.167	ug/l #	39
78) n-propylbenzene	11.311	91	870	0.201	ug/l	86
80) 1,3,5-Trimethylbenzene	11.457	105	2326	0.760	ug/l	95
81) trans-1,4-Dichloro-2-b...	11.085	75	29249	64.369	ug/l #	12
82) 4-Chlorotoluene	11.463	91	984	0.325	ug/l	74
84) 1,2,4-Trimethylbenzene	11.756	105	681	0.221	ug/l	95
86) p-Isopropyltoluene	12.012	119	776	0.246	ug/l #	77
87) 1,3-Dichlorobenzene	11.975	146	409	0.271	ug/l	91
88) 1,4-Dichlorobenzene	11.975	146	409	0.262	ug/l	91
89) n-Butylbenzene	12.335	91	925	0.317	ug/l	95
91) 1,2-Dichlorobenzene	12.335	146	299	0.206	ug/l	77
93) 1,2,4-Trichlorobenzene	13.591	180	415	0.474	ug/l	88
94) Hexachlorobutadiene	13.725	225	148	0.433	ug/l #	50
95) Naphthalene	13.774	128	837	0.245	ug/l #	84

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060621\
Data File : VX022506.D
Acq On : 07 Jun 2021 03:09
Operator : JC/MD
Sample : PB136857TB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 34 Sample Multiplier: 1


Instrument :
MSVOA_X
ClientSampleId :
PB136857TB


Quant Time: Jun 07 06:17:48 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
Quant Title : SW846 8260
QLast Update : Wed May 19 14:23:10 2021
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
96) 1,2,3-Trichlorobenzene	13.963	180	301	0.341	ug/l	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Jun 07 06:17:48 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
Quant Title : SW846 8260
QLast Update : Wed May 19 14:23:10 2021
Response via : Initial Calibration









#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.000 min
Lab File: VX022506.D
Acq: 07 Jun 2021 03:09




Instrument :
MSVOA_X
ClientSampled :
PB136857TB


Tgt Ion:168 Resp: 61480
Ion Ratio Lower Upper
168 100
99 68.2 45.8 68.6

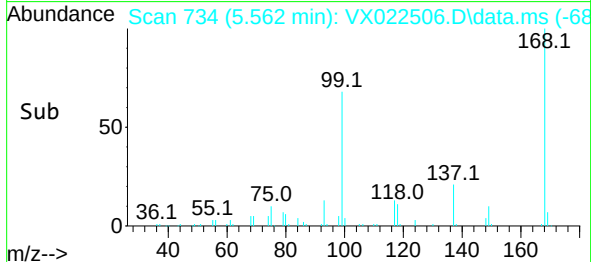

#5
Bromomethane
Concen: 0.470 ug/l
RT: 1.605 min Scan# 85
Delta R.T. -0.007 min
Lab File: VX022506.D
Acq: 07 Jun 2021 03:09


Tgt Ion: 94 Resp: 234
Ion Ratio Lower Upper
94 100
96 79.2 76.4 114.6

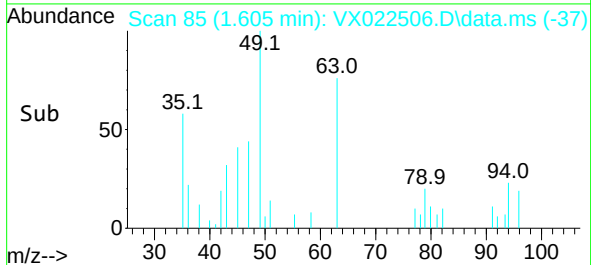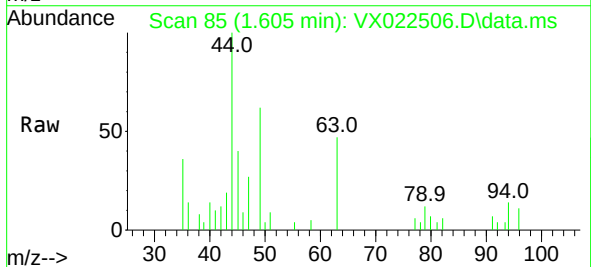






#10
Methyl Iodide
Concen: 0.625 ug/l
RT: 2.459 min Scan# 225
Delta R.T. 0.006 min
Lab File: VX022506.D
Acq: 07 Jun 2021 03:09

Instrument :
MSVOA_X
ClientSampled :
PB136857TB







Tgt Ion:142 Resp: 489
Ion Ratio Lower Upper
142 100
127 35.8 33.3 49.9
141 0.0 11.4 17.0#

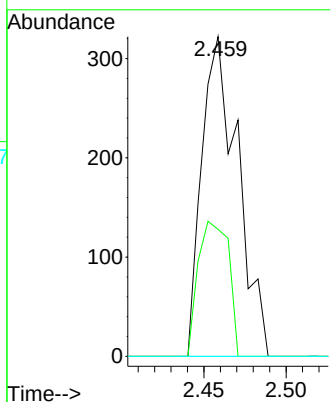

#11
Tert butyl alcohol
Concen: 9.045 ug/l
RT: 2.946 min Scan# 305
Delta R.T. -0.043 min
Lab File: VX022506.D
Acq: 07 Jun 2021 03:09

Tgt Ion: 59 Resp: 1962
Ion Ratio Lower Upper
59 100
57 0.0 7.8 11.8#


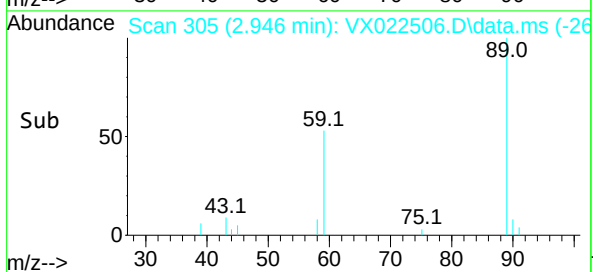
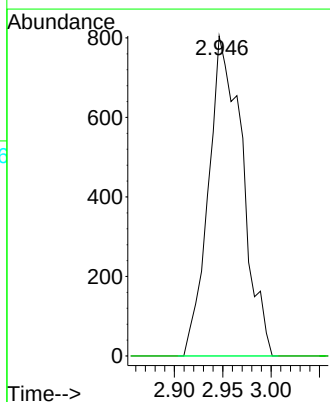





#13
Acrolein
Concen: 0.320 ug/l
RT: 2.239 min Scan# 189
Delta R.T. -0.001 min
Lab File: VX022506.D
Acq: 07 Jun 2021 03:09




Instrument :
MSVOA_X
ClientSampleId :
PB136857TB


Tgt Ion: 56 Resp: 46
Ion Ratio Lower Upper
56 100
55 43.5 56.4 84.6#

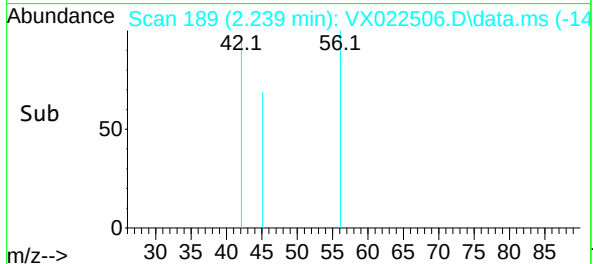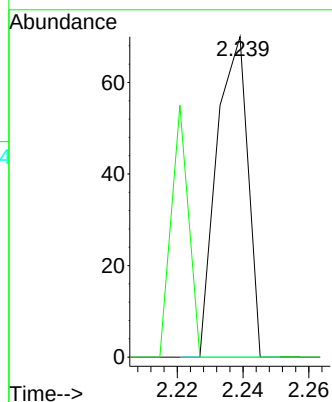

#16
Acetone
Concen: 19.571 ug/l
RT: 2.392 min Scan# 214
Delta R.T. -0.000 min
Lab File: VX022506.D
Acq: 07 Jun 2021 03:09


Tgt Ion: 43 Resp: 8082
Ion Ratio Lower Upper
43 100
58 27.9 27.8 41.8

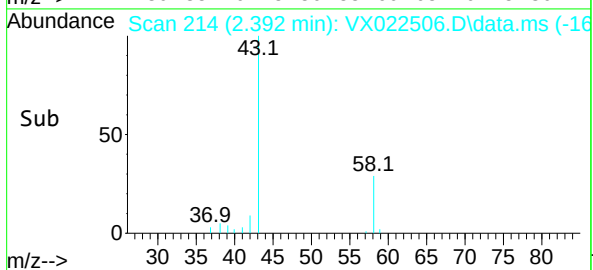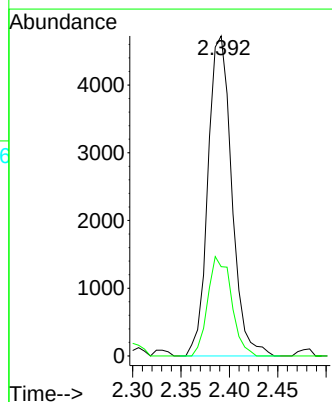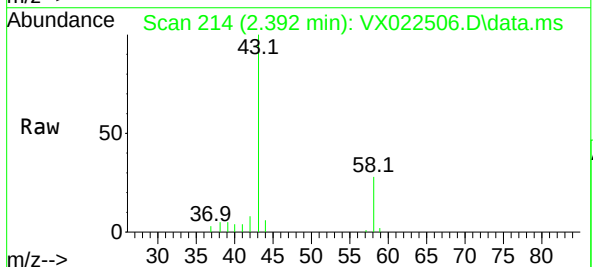






#17
Carbon Disulfide
Concen: 0.320 ug/l
RT: 2.507 min Scan# 233
Delta R.T. -0.007 min
Lab File: VX022506.D
Acq: 07 Jun 2021 03:09

Instrument :
MSVOA_X
ClientSampleId :
PB136857TB







Tgt Ion: 76 Resp: 591
Ion Ratio Lower Upper
76 100
78 0.0 7.2 10.8#

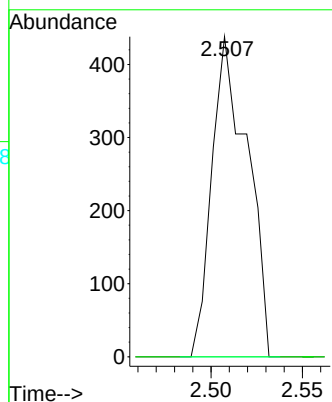

#18
Methyl Acetate
Concen: 0.744 ug/l
RT: 2.715 min Scan# 267
Delta R.T. 0.006 min
Lab File: VX022506.D
Acq: 07 Jun 2021 03:09

Tgt Ion: 43 Resp: 817
Ion Ratio Lower Upper
43 100
74 7.5 21.9 32.9#

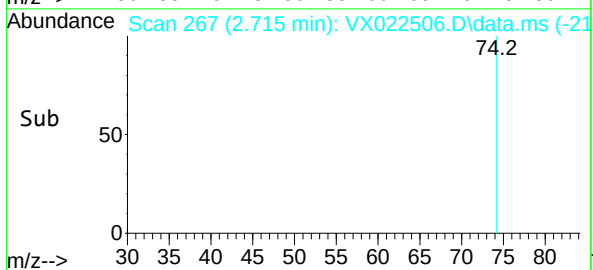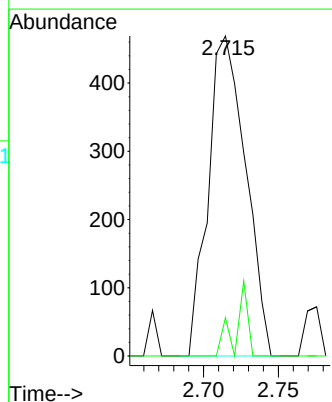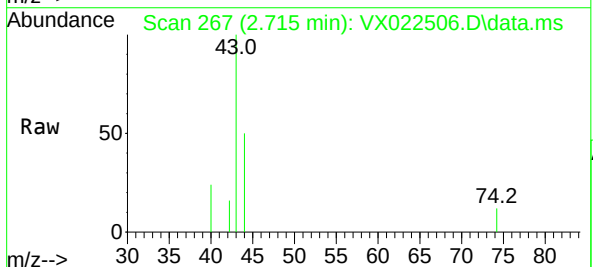



#20

Methylene Chloride

Concen: 4.507 ug/l

RT: 2.794 min Scan# 280

Delta R.T. -0.000 min

Lab File: VX022506.D

Acq: 07 Jun 2021 03:09

Instrument :

MSVOA_X

ClientSampleId :

PB136857TB

Tgt Ion: 84 Resp: 4132





Ion Ratio Lower Upper

84 100

49 124.4 88.6 132.8

51 49.5 27.0 40.6#

86 65.1 50.3 75.5

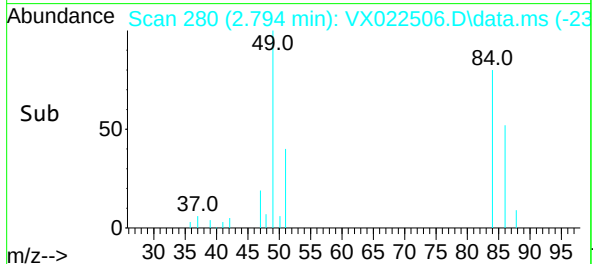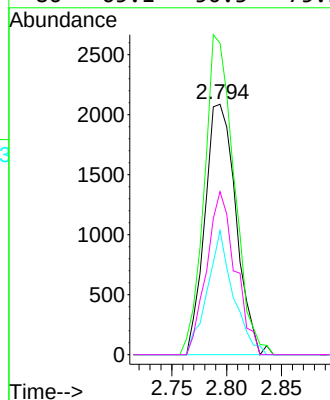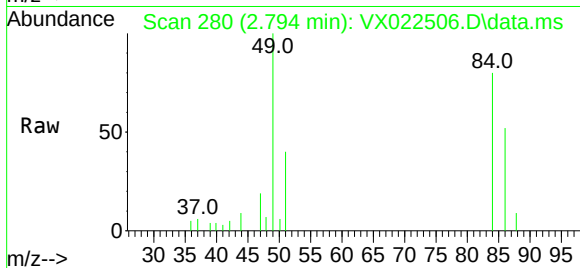

#25

2-Butanone

Concen: 2.643 ug/l

RT: 4.586 min Scan# 574

Delta R.T. 0.018 min

Lab File: VX022506.D




Acq: 07 Jun 2021 03:09


Tgt Ion: 43 Resp: 1766

Ion Ratio Lower Upper

43 100

72 35.1 23.7 35.5

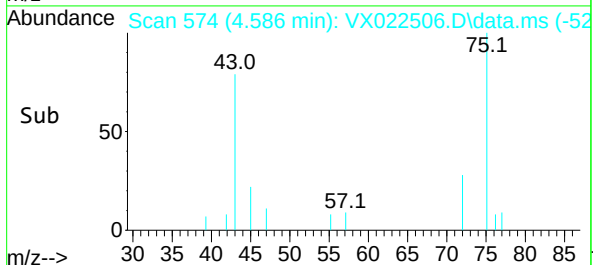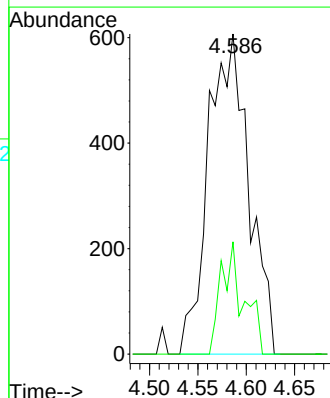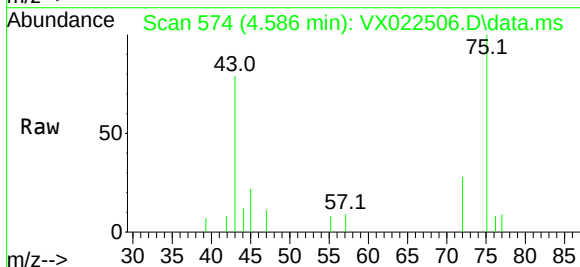



#29

Tetrahydrofuran

Concen: 1.813 ug/l

RT: 5.037 min Scan# 648

Delta R.T. 0.024 min

Lab File: VX022506.D

Acq: 07 Jun 2021 03:09

Tgt Ion: 42 Resp: 721

Ion Ratio Lower Upper

42 100

72 5.8 41.7 62.5#





71 28.3 38.4 57.6#

Instrument :

MSVOA_X

ClientSampleId :

PB136857TB

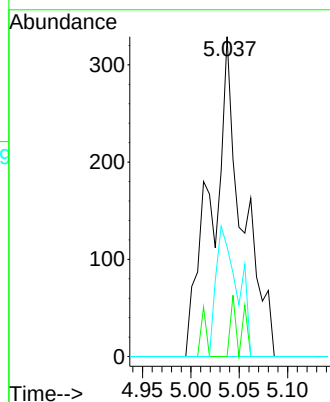

#33

1,2-Dichloroethane-d4

Concen: 52.680 ug/l

RT: 5.964 min Scan# 800

Delta R.T. 0.000 min

Lab File: VX022506.D




Acq: 07 Jun 2021 03:09


Tgt Ion: 65 Resp: 49960

Ion Ratio Lower Upper

65 100

67 52.8 0.0 105.4


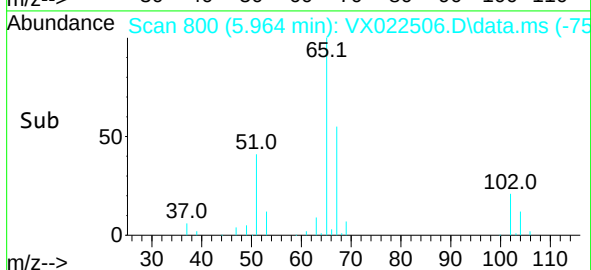
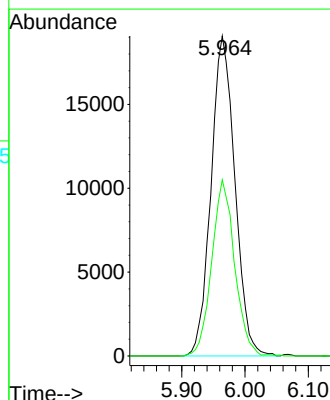





#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 932
Delta R.T. -0.000 min
Lab File: VX022506.D
Acq: 07 Jun 2021 03:09




Instrument :
MSVOA_X
ClientSampleId :
PB136857TB


Tgt Ion:114 Resp: 123584
Ion Ratio Lower Upper
114 100
63 21.1 0.0 40.8
88 15.2 0.0 32.8

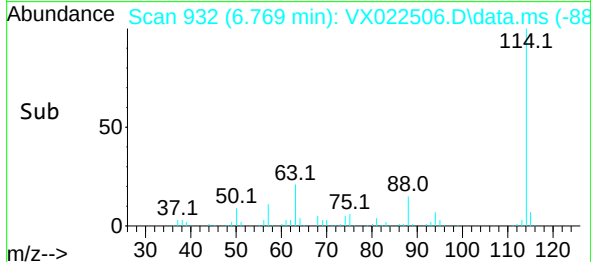

#35
Dibromofluoromethane
Concen: 46.823 ug/l
RT: 5.397 min Scan# 707
Delta R.T. 0.006 min
Lab File: VX022506.D
Acq: 07 Jun 2021 03:09

Tgt Ion:113 Resp: 36696
Ion Ratio Lower Upper
113 100
111 100.7 81.9 122.9
192 14.5 16.7 25.1#


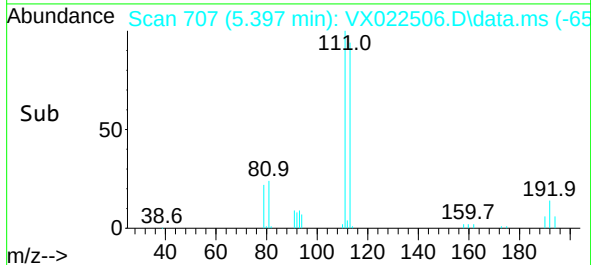

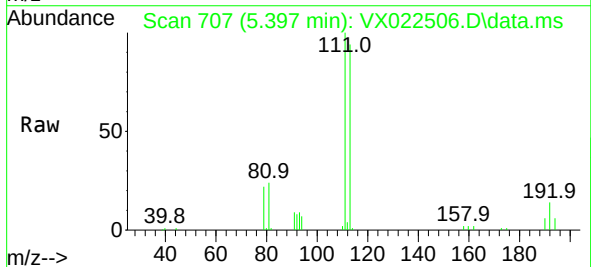




#36
1,1-Dichloropropene
Concen: 5.143 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.140 min
Lab File: VX022506.D
Acq: 07 Jun 2021 03:09




Instrument :
MSVOA_X
ClientSampled :
PB136857TB


Tgt Ion: 75 Resp: 5877
Ion Ratio Lower Upper
75 100
110 7.1 18.1 54.4#
77 0.0 25.3 37.9#

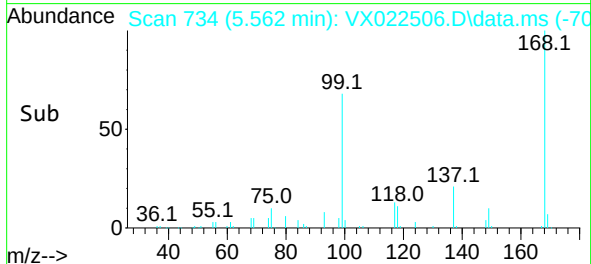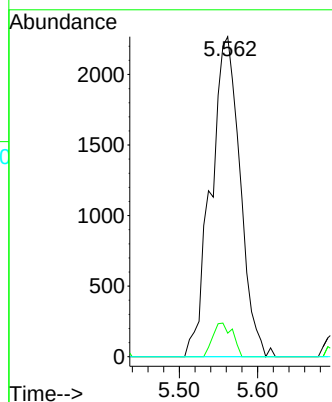

#38
Carbon Tetrachloride
Concen: 6.375 ug/l
RT: 5.562 min Scan# 734
Delta R.T. -0.128 min
Lab File: VX022506.D
Acq: 07 Jun 2021 03:09


Tgt Ion: 117 Resp: 7127
Ion Ratio Lower Upper
117 100
119 7.8 76.2 114.2#
121 0.0 24.8 37.2#

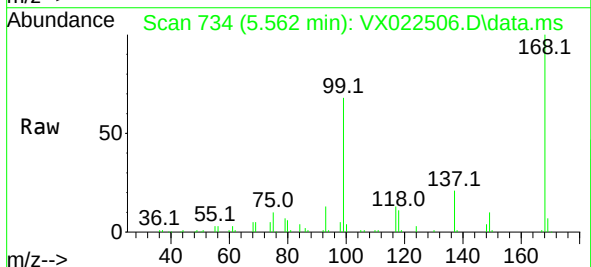






#41
Methacrylonitrile
Concen: 0.304 ug/l
RT: 5.031 min Scan# 647
Delta R.T. 0.103 min
Lab File: VX022506.D
Acq: 07 Jun 2021 03:09

Instrument :
MSVOA_X
ClientSampled :
PB136857TB



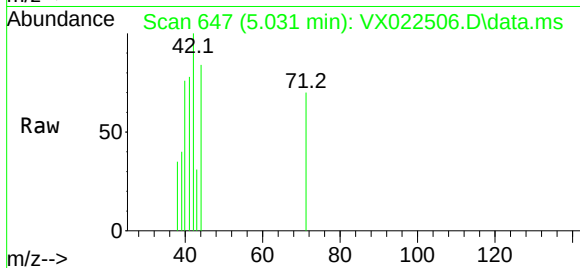



Tgt Ion:	41	Resp:	228
Ion	Ratio	Lower	Upper
41	100		
39	43.0	42.5	63.7
67	0.0	65.0	97.6#
52	0.0	25.3	37.9#

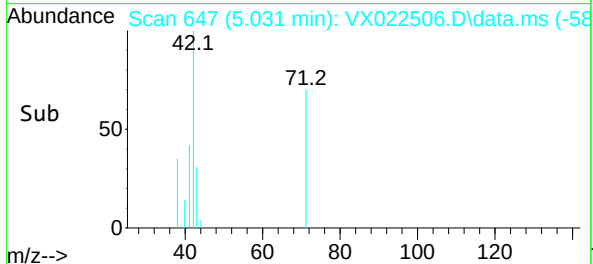

#43
Isopropyl Acetate
Concen: 4.827 ug/l
RT: 6.354 min Scan# 864
Delta R.T. 0.005 min
Lab File: VX022506.D
Acq: 07 Jun 2021 03:09

Tgt Ion:	43	Resp:	11061
Ion	Ratio	Lower	Upper
43	100		
61	20.9	18.2	27.4
87	14.4	12.5	18.7


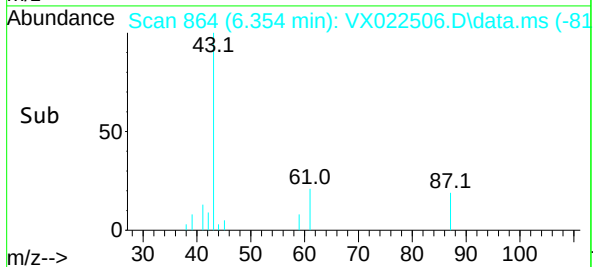

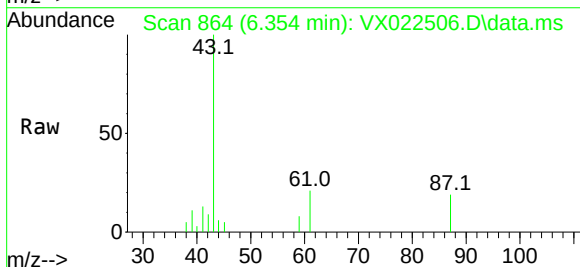




#48
Methyl methacrylate
Concen: 2.903 ug/l
RT: 7.598 min Scan# 1068
Delta R.T. -0.098 min
Lab File: VX022506.D
Acq: 07 Jun 2021 03:09




Instrument :
MSVOA_X
ClientSampleId :
PB136857TB


Tgt Ion: 41 Resp: 3066
Ion Ratio Lower Upper
41 100
69 0.0 76.0 114.0#
39 0.0 44.6 67.0#

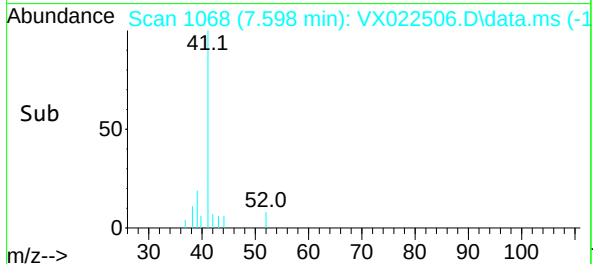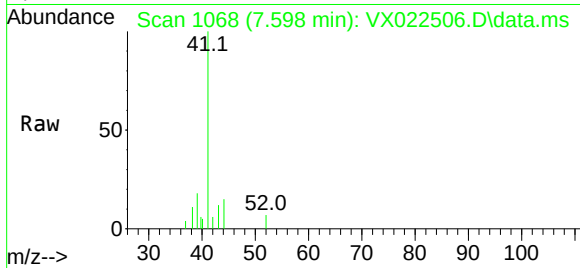

#49
1,4-Dioxane
Concen: 1.167 ug/l
RT: 7.799 min Scan# 1101
Delta R.T. 0.115 min
Lab File: VX022506.D
Acq: 07 Jun 2021 03:09

Tgt Ion: 88 Resp: 24
Ion Ratio Lower Upper
88 100
43 2523816.7 23.2 34.8#
58 10179.2 55.0 82.4#


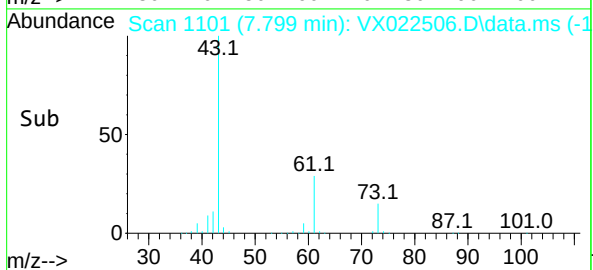

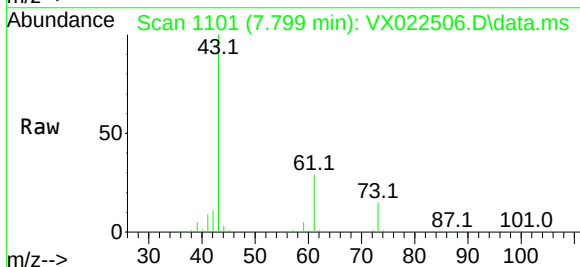




#50
Toluene-d8
Concen: 51.361 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX022506.D
Acq: 07 Jun 2021 03:09




Instrument :
MSVOA_X
ClientSampled :
PB136857TB


Tgt Ion: 98 Resp: 155055
Ion Ratio Lower Upper
98 100
100 66.2 51.9 77.9

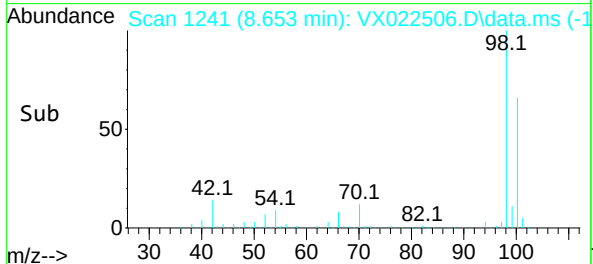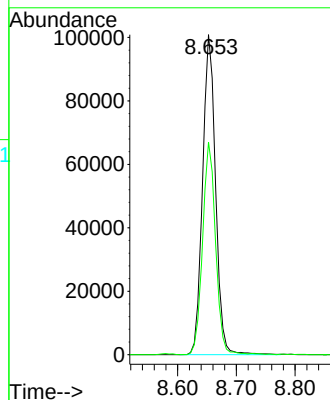

#51
4-Methyl-2-Pentanone
Concen: 29.495 ug/l
RT: 8.555 min Scan# 1225
Delta R.T. -0.025 min
Lab File: VX022506.D
Acq: 07 Jun 2021 03:09

Tgt Ion: 43 Resp: 40484
Ion Ratio Lower Upper
43 100
58 8.7 35.4 53.0#



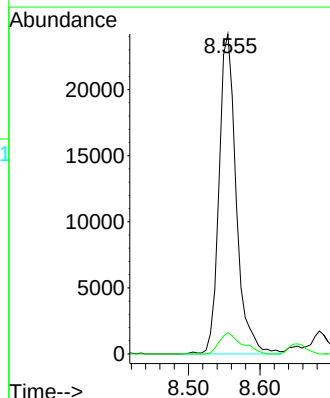
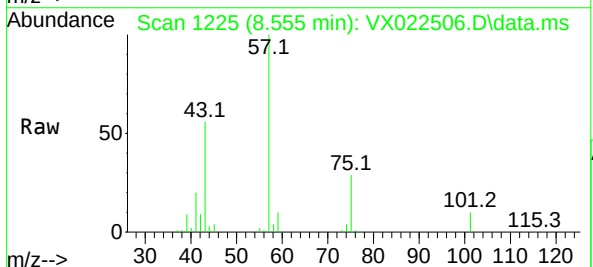




#54
cis-1,3-Dichloropropene
Concen: 12.250 ug/l
RT: 8.555 min Scan# 1225
Delta R.T. 0.182 min
Lab File: VX022506.D
Acq: 07 Jun 2021 03:09




Instrument :
MSVOA_X
ClientSampled :
PB136857TB


Tgt Ion: 75 Resp: 18511
Ion Ratio Lower Upper
75 100
77 0.4 25.7 38.5#
39 30.3 35.1 52.7#

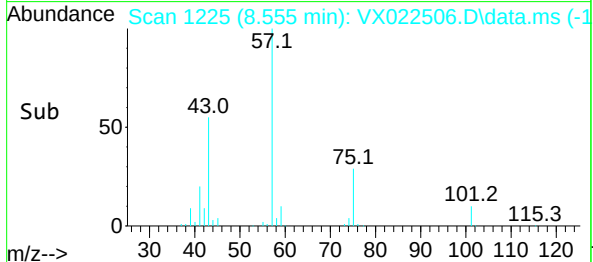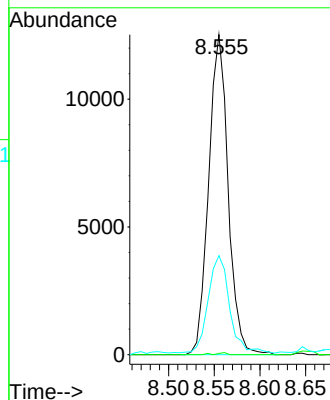

#56
Ethyl methacrylate
Concen: 0.224 ug/l
RT: 9.348 min Scan# 1355
Delta R.T. 0.226 min
Lab File: VX022506.D
Acq: 07 Jun 2021 03:09

Tgt Ion: 69 Resp: 327
Ion Ratio Lower Upper
69 100
41 2945.6 46.8 70.2#
39 1259.0 24.7 37.1#

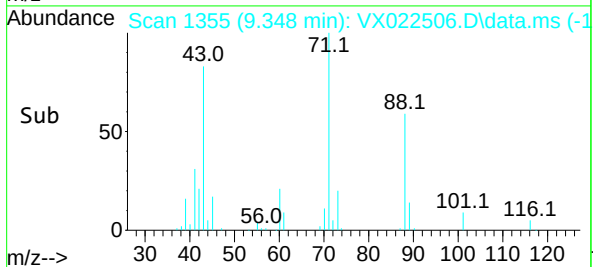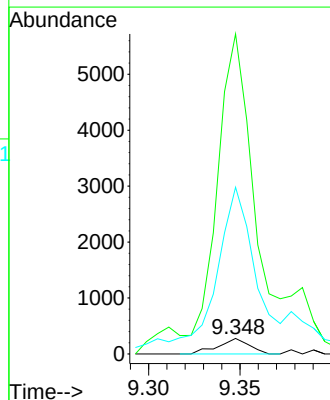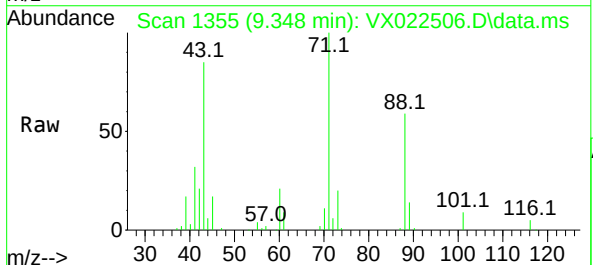







#57

1,3-Dichloropropane
Concen: 6.794 ug/l
RT: 9.488 min Scan# 1378
Delta R.T. 0.177 min
Lab File: VX022506.D
Acq: 07 Jun 2021 03:09

Instrument :
MSVOA_X
ClientSampleId :
PB136857TB




Tgt Ion: 76 Resp: 10485
Ion Ratio Lower Upper
76 100
78 0.0 26.2 39.2#

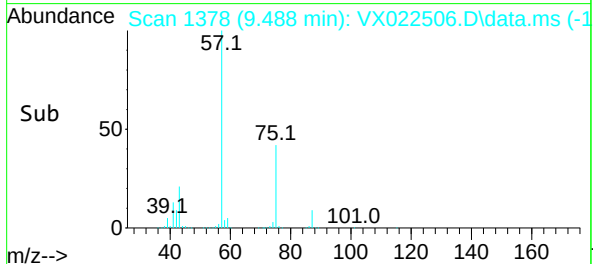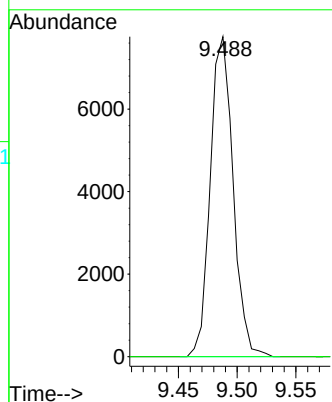


#59

2-Hexanone
Concen: 4.836 ug/l
RT: 9.384 min Scan# 1361
Delta R.T. -0.049 min
Lab File: VX022506.D
Acq: 07 Jun 2021 03:09

Tgt Ion: 43 Resp: 4992
Ion Ratio Lower Upper
43 100
58 0.0 30.9 92.8#


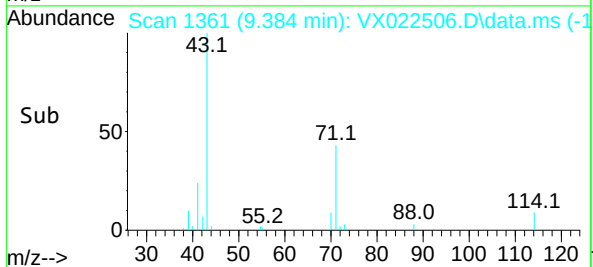
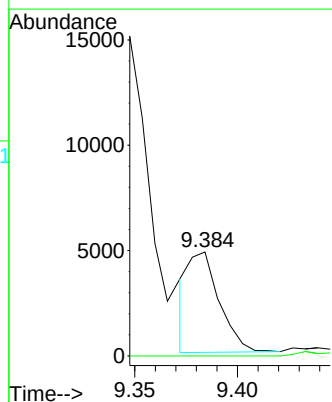
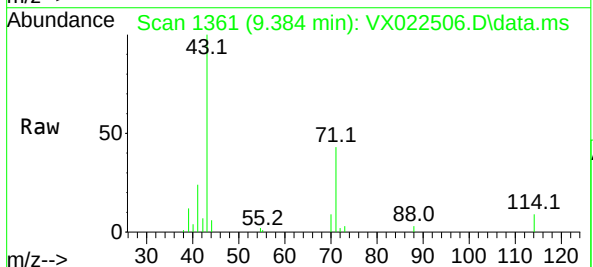




#62
4-Bromofluorobenzene
Concen: 49.927 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX022506.D
Acq: 07 Jun 2021 03:09




Instrument :
MSVOA_X
ClientSampleId :
PB136857TB


Tgt Ion: 95 Resp: 55711
Ion Ratio Lower Upper
95 100
174 62.2 0.0 154.6
176 59.2 0.0 155.8

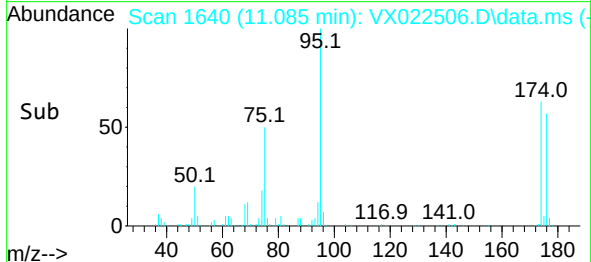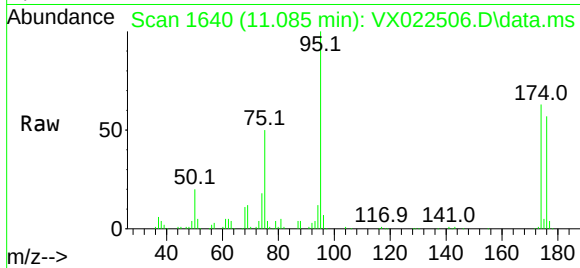

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.006 min
Lab File: VX022506.D
Acq: 07 Jun 2021 03:09

Tgt Ion: 117 Resp: 113304
Ion Ratio Lower Upper
117 100
82 60.6 47.4 71.2
119 30.6 26.6 39.8


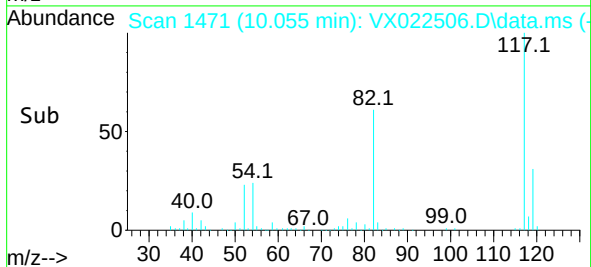

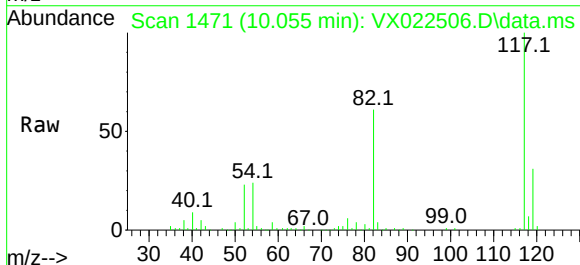




#68
m/p-Xylenes
Concen: 0.246 ug/l
RT: 10.305 min Scan# 1512
Delta R.T. -0.000 min
Lab File: VX022506.D
Acq: 07 Jun 2021 03:09




Instrument :
MSVOA_X
ClientSampled :
PB136857TB


Tgt Ion:106 Resp: 403
Ion Ratio Lower Upper
106 100
91 230.3 162.8 244.2

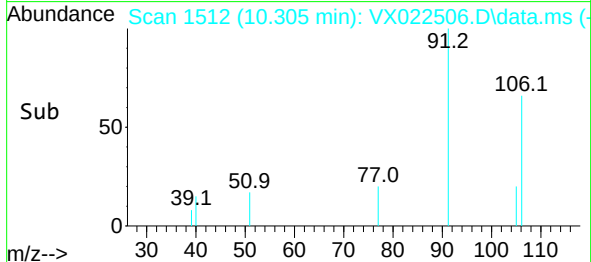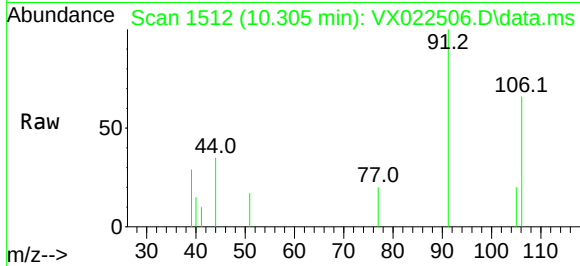

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX022506.D
Acq: 07 Jun 2021 03:09

Tgt Ion:152 Resp: 43641
Ion Ratio Lower Upper
152 100
115 68.8 41.1 123.3
150 163.7 0.0 349.0


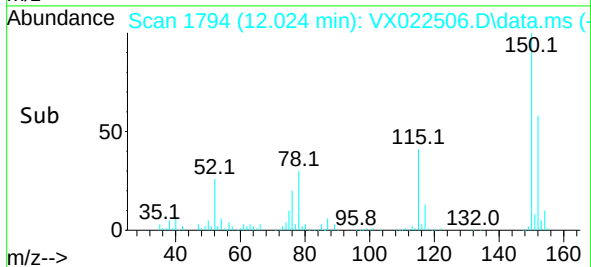

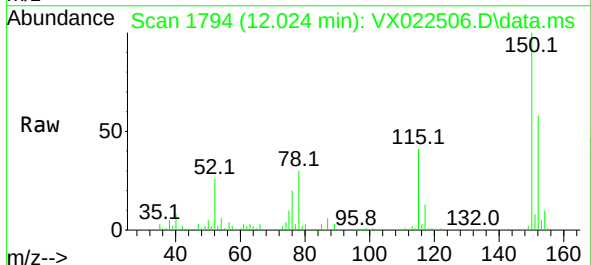




#76
1,2,3-Trichloropropane
Concen: 27.167 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. -0.159 min
Lab File: VX022506.D
Acq: 07 Jun 2021 03:09




Instrument :
MSVOA_X
ClientSampled :
PB136857TB


Tgt Ion: 75 Resp: 29249
Ion Ratio Lower Upper
75 100
77 1.3 19.1 57.5#

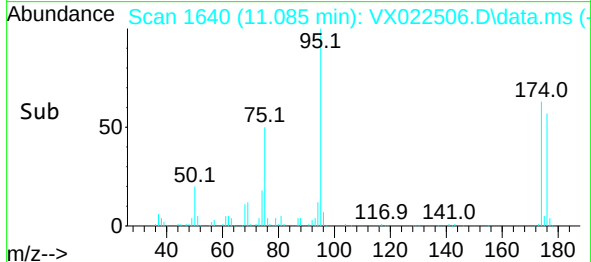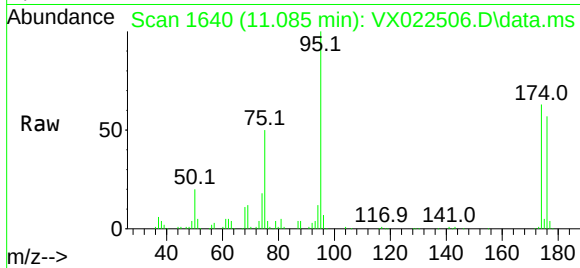

#78
n-propylbenzene
Concen: 0.201 ug/l
RT: 11.311 min Scan# 1677
Delta R.T. 0.006 min
Lab File: VX022506.D
Acq: 07 Jun 2021 03:09

Tgt Ion: 91 Resp: 870
Ion Ratio Lower Upper
91 100
120 29.7 11.5 34.5


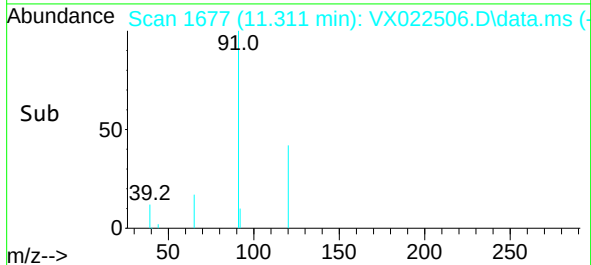

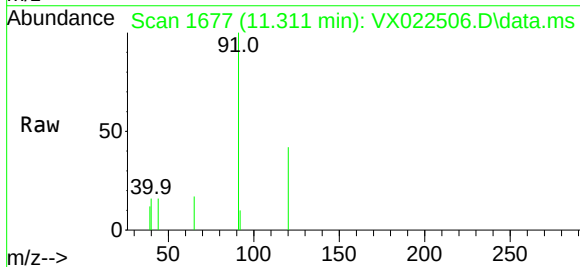




#80
1,3,5-Trimethylbenzene
Concen: 0.760 ug/l
RT: 11.457 min Scan# 1701
Delta R.T. -0.000 min
Lab File: VX022506.D
Acq: 07 Jun 2021 03:09




Instrument :
MSVOA_X
ClientSampled :
PB136857TB


Tgt Ion:105 Resp: 2326
Ion Ratio Lower Upper
105 100
120 51.0 23.8 71.5

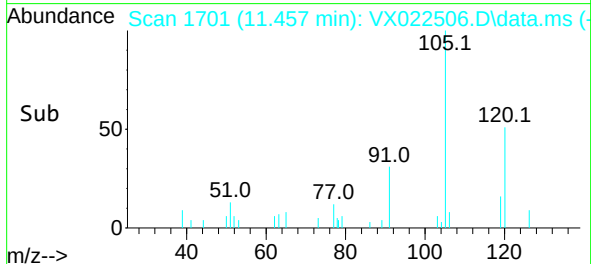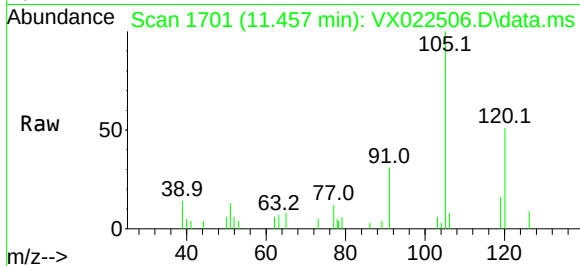

#81
trans-1,4-Dichloro-2-butene
Concen: 64.369 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.060 min
Lab File: VX022506.D
Acq: 07 Jun 2021 03:09

Tgt Ion: 75 Resp: 29249
Ion Ratio Lower Upper
75 100
53 0.0 74.5 111.7#
89 0.0 37.9 56.9#


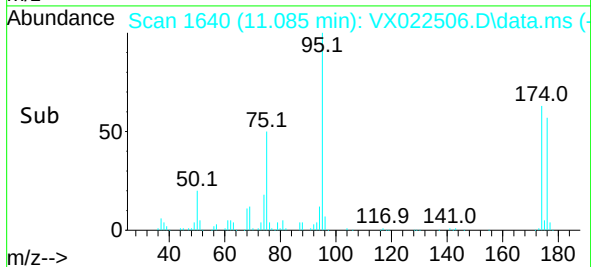

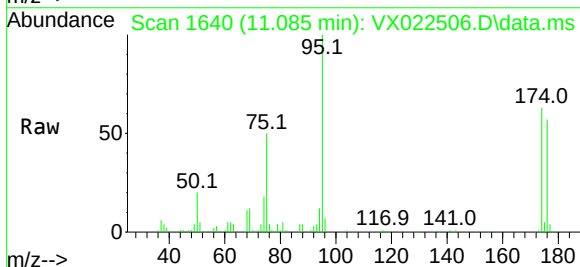




#82
4-Chlorotoluene
Concen: 0.325 ug/l
RT: 11.463 min Scan# 1702
Delta R.T. 0.006 min
Lab File: VX022506.D
Acq: 07 Jun 2021 03:09




Instrument :
MSVOA_X
ClientSampled :
PB136857TB


Tgt Ion: 91 Resp: 984
Ion Ratio Lower Upper
91 100
126 15.5 14.9 44.5

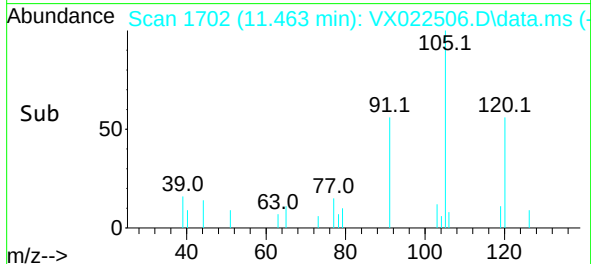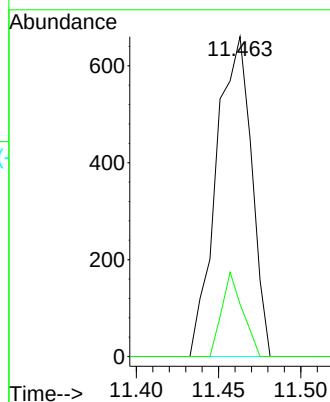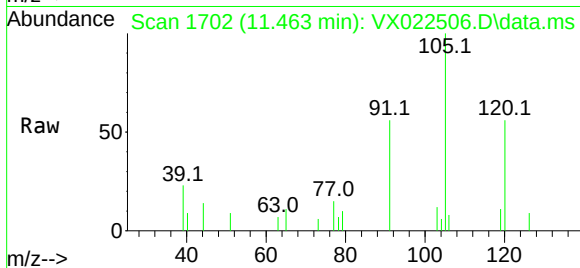

#84
1,2,4-Trimethylbenzene
Concen: 0.221 ug/l
RT: 11.756 min Scan# 1750
Delta R.T. -0.000 min
Lab File: VX022506.D
Acq: 07 Jun 2021 03:09

Tgt Ion: 105 Resp: 681
Ion Ratio Lower Upper
105 100
120 47.9 22.4 67.3


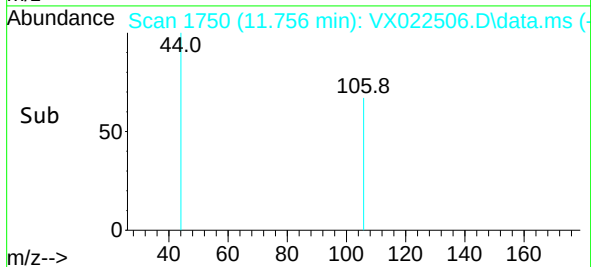
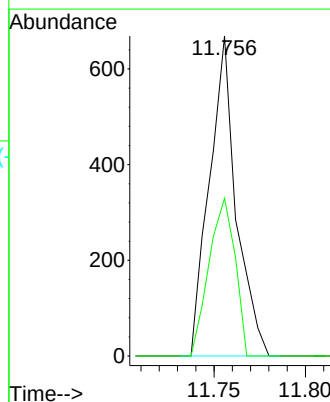
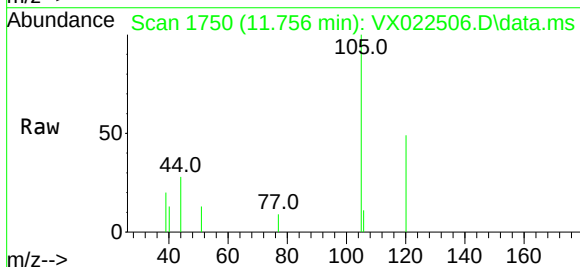




#86
p-Isopropyltoluene
Concen: 0.246 ug/l
RT: 12.012 min Scan# 1792
Delta R.T. -0.000 min
Lab File: VX022506.D
Acq: 07 Jun 2021 03:09




Instrument :
MSVOA_X
ClientSampleId :
PB136857TB


Tgt Ion:119 Resp: 776
Ion Ratio Lower Upper
119 100
134 28.4 12.9 38.7
91 44.6 11.7 35.0#

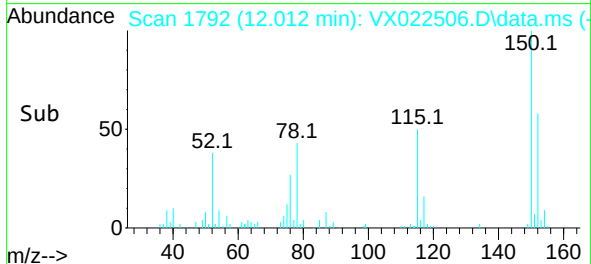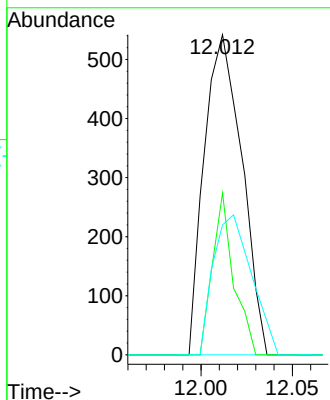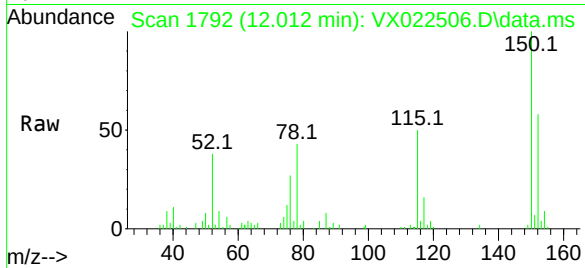

#87
1,3-Dichlorobenzene
Concen: 0.271 ug/l
RT: 11.975 min Scan# 1786
Delta R.T. -0.001 min
Lab File: VX022506.D
Acq: 07 Jun 2021 03:09

Tgt Ion:146 Resp: 409
Ion Ratio Lower Upper
146 100
111 48.7 20.2 60.5
148 59.4 31.9 95.7

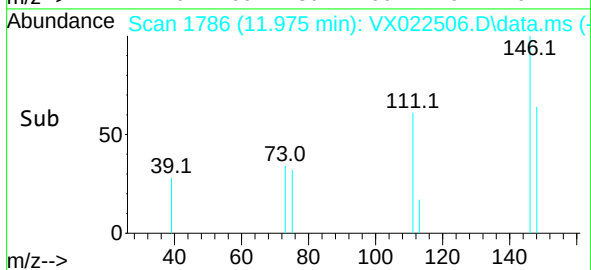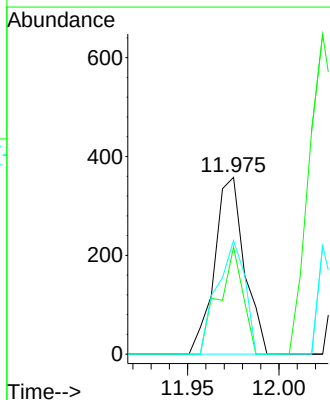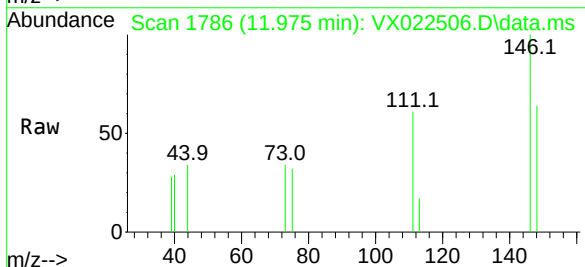







#88
1,4-Dichlorobenzene
Concen: 0.262 ug/l
RT: 11.975 min Scan# 1786
Delta R.T. -0.068 min
Lab File: VX022506.D
Acq: 07 Jun 2021 03:09

Instrument :
MSVOA_X
ClientSampleId :
PB136857TB

Tgt Ion:146 Resp: 409




Ion	Ratio	Lower	Upper
146	100		
111	48.7	19.6	58.8
148	59.4	31.6	95.0

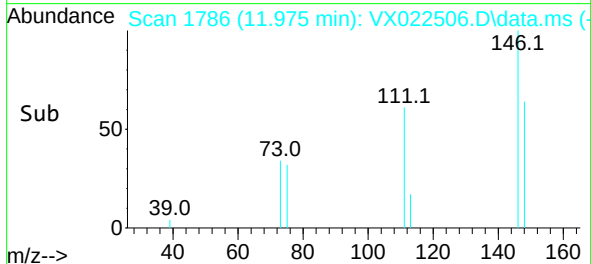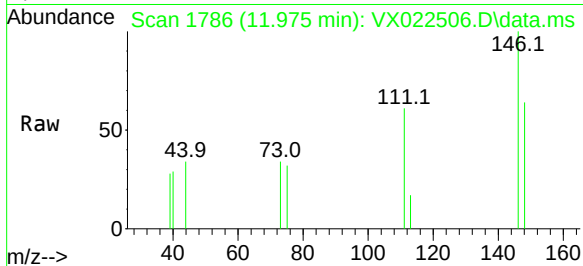


#89
n-Butylbenzene
Concen: 0.317 ug/l
RT: 12.335 min Scan# 1845
Delta R.T. -0.000 min
Lab File: VX022506.D
Acq: 07 Jun 2021 03:09

Tgt Ion: 91 Resp: 925

Ion	Ratio	Lower	Upper
91	100		
92	51.4	27.4	82.0
134	23.5	13.2	39.5


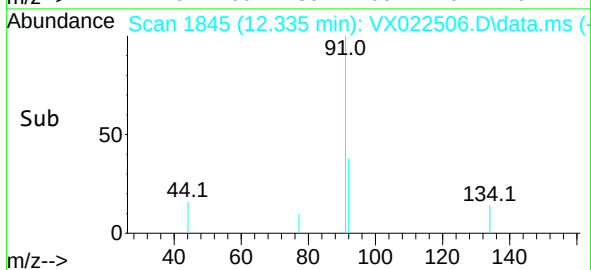

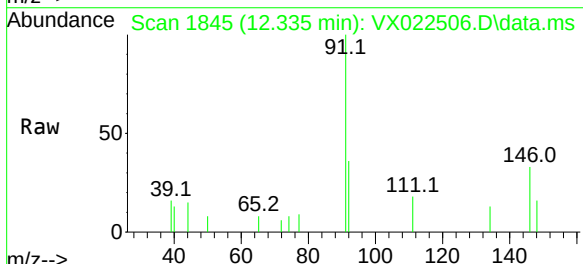




#91
1,2-Dichlorobenzene
Concen: 0.206 ug/l
RT: 12.335 min Scan# 1845
Delta R.T. -0.006 min
Lab File: VX022506.D
Acq: 07 Jun 2021 03:09




Instrument :
MSVOA_X
ClientSampleId :
PB136857TB


Tgt Ion:146	Resp:	299
Ion	Ratio	Lower Upper
146	100	
111	49.2	20.8 62.2
148	40.8	31.9 95.5

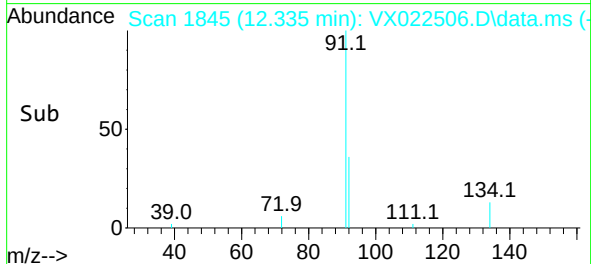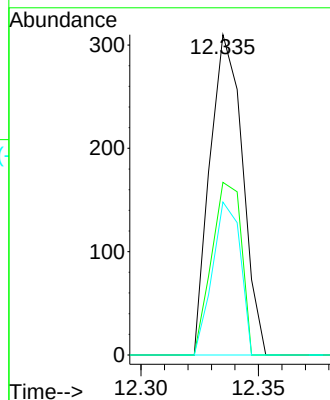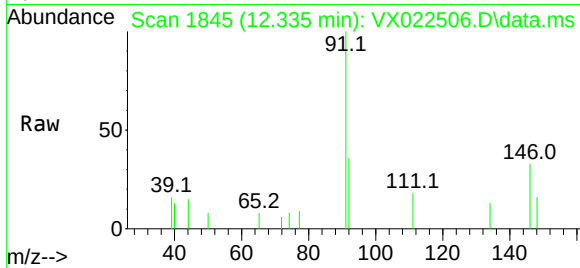

#93
1,2,4-Trichlorobenzene
Concen: 0.474 ug/l
RT: 13.591 min Scan# 2051
Delta R.T. -0.000 min
Lab File: VX022506.D
Acq: 07 Jun 2021 03:09

Tgt Ion:180	Resp:	415
Ion	Ratio	Lower Upper
180	100	
182	82.7	47.7 143.1
145	35.4	15.0 45.0


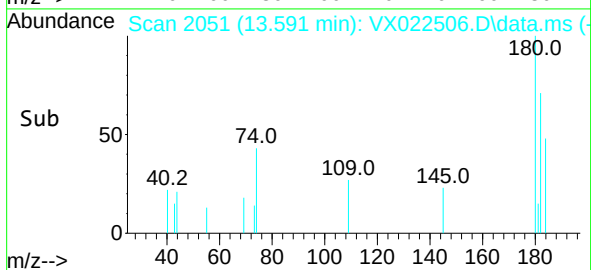
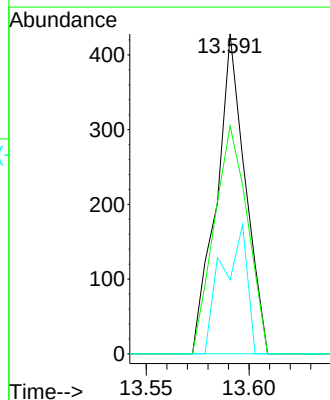
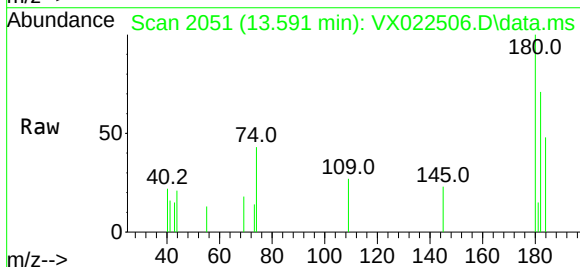




#94
Hexachlorobutadiene
Concen: 0.433 ug/l
RT: 13.725 min Scan# 2073
Delta R.T. -0.006 min
Lab File: VX022506.D
Acq: 07 Jun 2021 03:09




Instrument :
MSVOA_X
ClientSampled :
PB136857TB


Tgt Ion:225 Resp: 148
Ion Ratio Lower Upper
225 100
223 48.0 31.1 93.2
227 0.0 31.6 95.0#

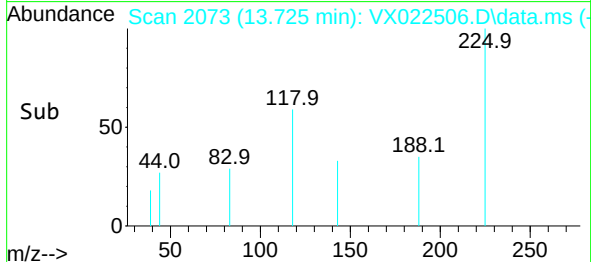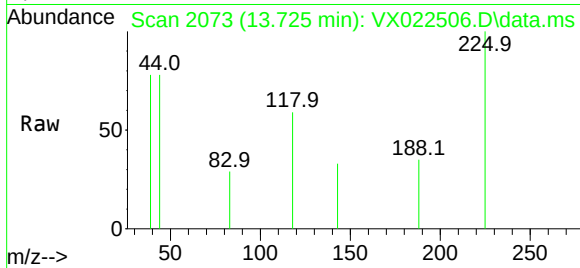

#95
Naphthalene
Concen: 0.245 ug/l
RT: 13.774 min Scan# 2081
Delta R.T. -0.006 min
Lab File: VX022506.D
Acq: 07 Jun 2021 03:09

Tgt Ion:128 Resp: 837
Ion Ratio Lower Upper
128 100
127 15.1 10.3 15.5
129 0.0 8.8 13.2#

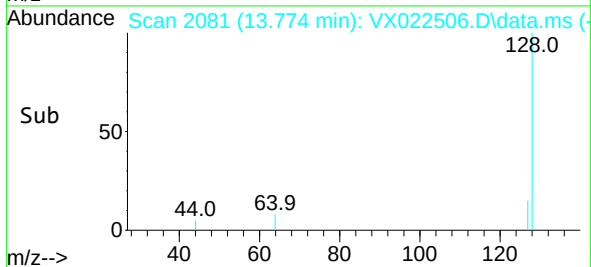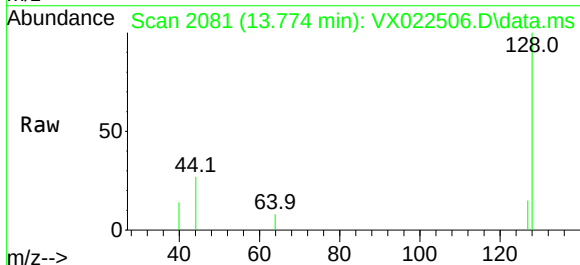



#96
 1,2,3-Trichlorobenzene
 Concen: 0.341 ug/l
 RT: 13.963 min Scan# 2112
 Delta R.T. -0.000 min
 Lab File: VX022506.D
 Acq: 07 Jun 2021 03:09

Instrument :
 MSVOA_X
 ClientSampleId :
 PB136857TB

Tgt Ion:180 Resp: 301
 Ion Ratio Lower Upper
 180 100
 182 84.1 47.6 142.9
 145 36.2 16.1 48.3

