

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060621\
 Data File : VX022485.D
 Acq On : 06 Jun 2021 18:09
 Operator : JC/MD
 Sample : PB136837ZHE#13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PB136837ZHE#13

Quant Time: Jun 07 04:26:24 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
 Quant Title : SW846 8260
 QLast Update : Wed May 19 14:23:10 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.562	168	65416	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	132661	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.061	117	117904	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	46157	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	53529	53.047	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	106.100%
35) Dibromofluoromethane	5.391	113	38905	46.245	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	92.500%
50) Toluene-d8	8.653	98	160436	49.507	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	99.020%
62) 4-Bromofluorobenzene	11.085	95	56574	47.231	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	94.460%
Target Compounds						
						Qvalue
16) Acetone	2.386	43	3956	9.003	ug/l	# 87
20) Methylene Chloride	2.794	84	3218	3.299	ug/l	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX060621\
Data File : VX022485.D
Acq On : 06 Jun 2021 18:09
Operator : JC/MD
Sample : PB136837ZHE#13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PB136837ZHE#13

Quant Time: Jun 07 04:26:24 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X051921W.M
Quant Title : SW846 8260
QLast Update : Wed May 19 14:23:10 2021
Response via : Initial Calibration




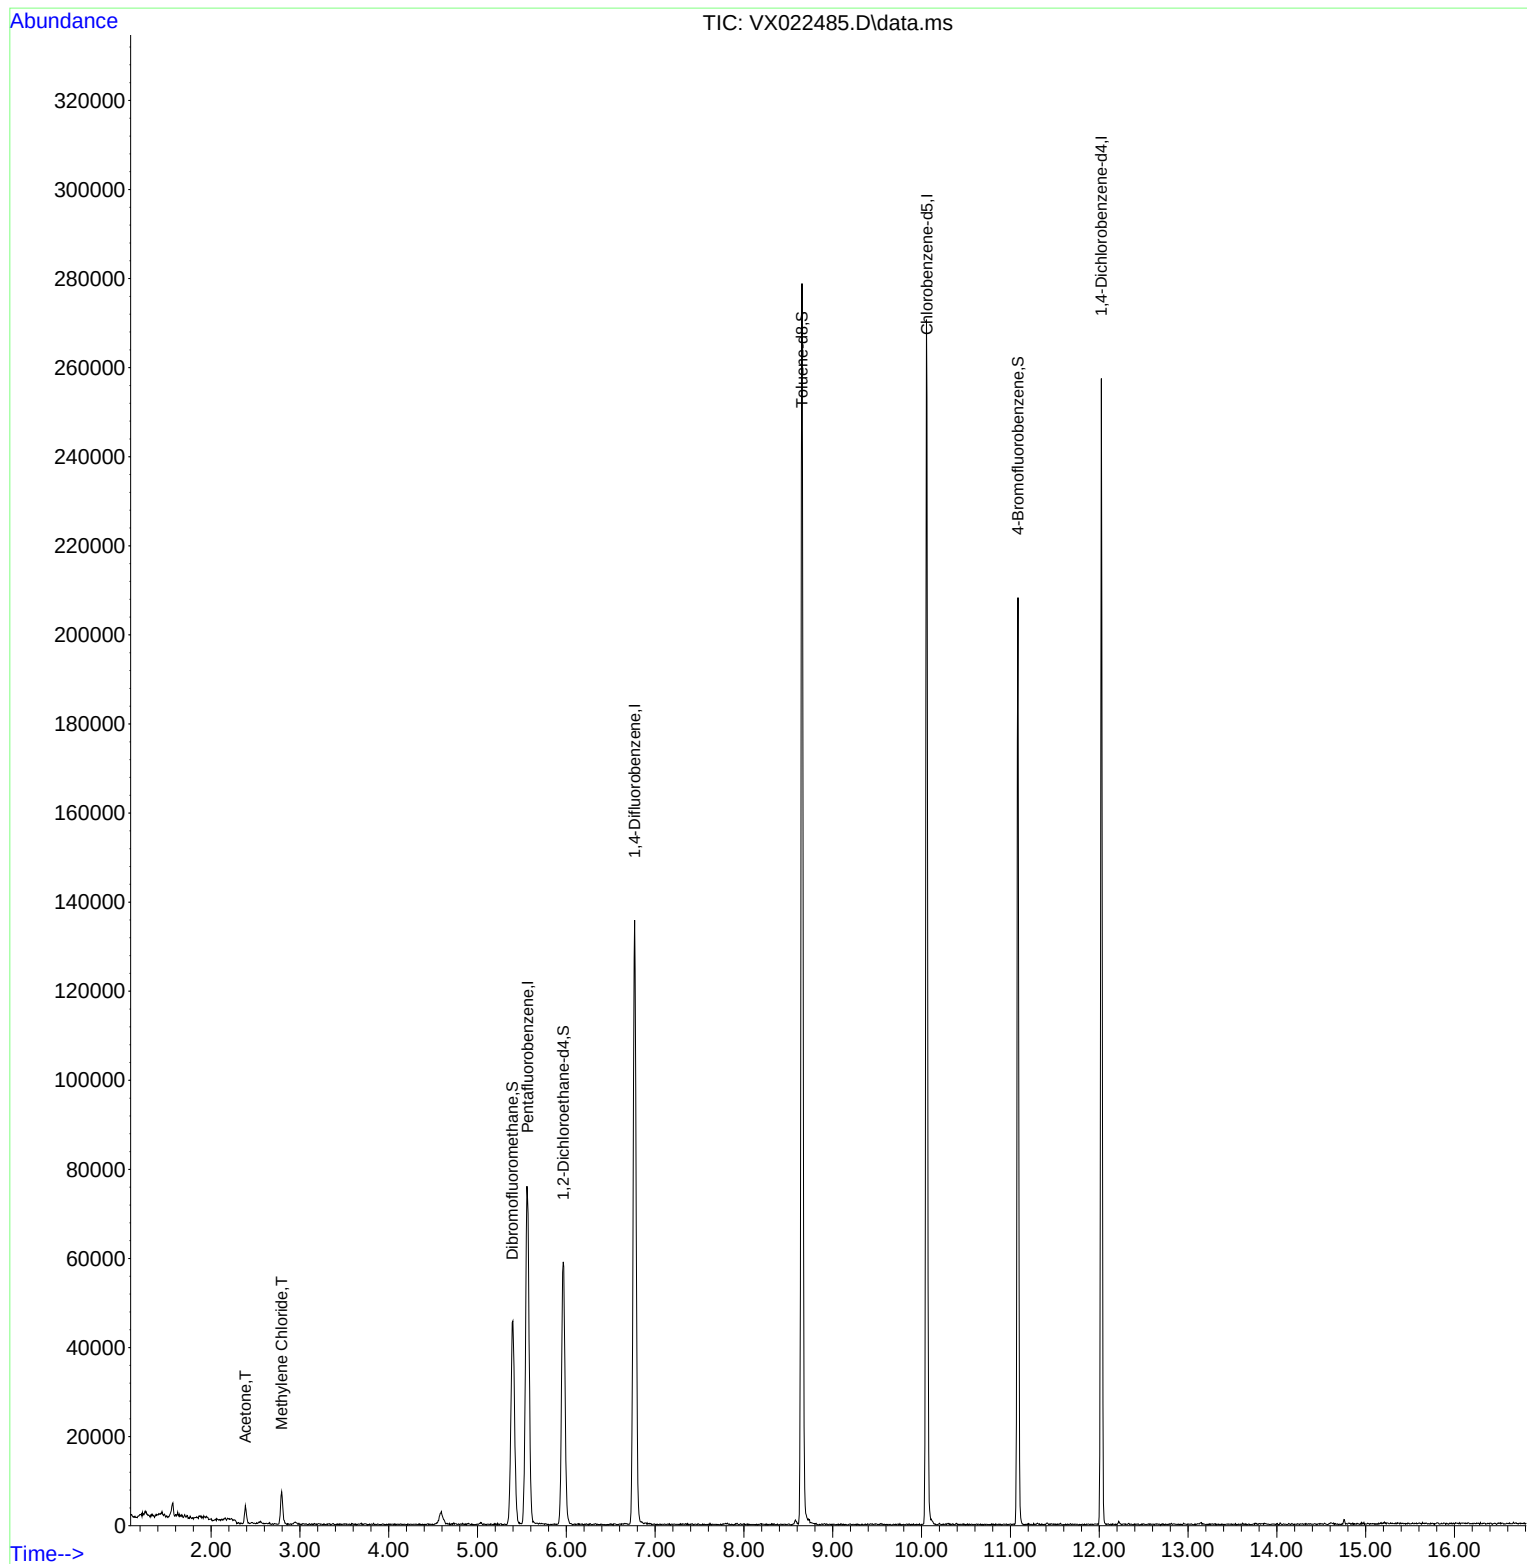


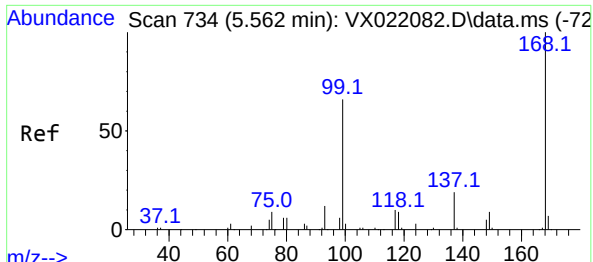

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 734
Delta R.T. 0.000 min
Lab File: VX022485.D
Acq: 06 Jun 2021 18:09




Instrument :
MSVOA_X
ClientSampleId :
PB136837ZHE#13


Tgt Ion:168 Resp: 65416
Ion Ratio Lower Upper
168 100
99 65.4 45.8 68.6

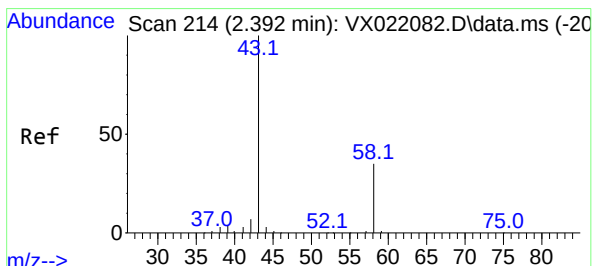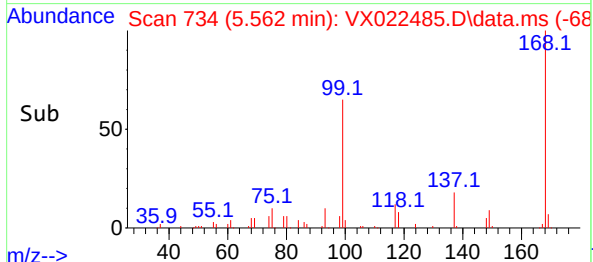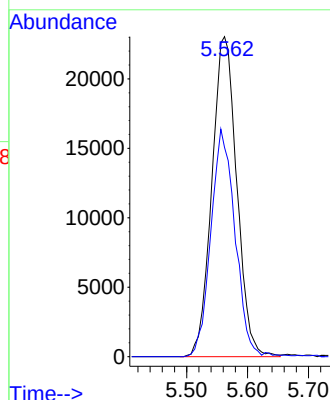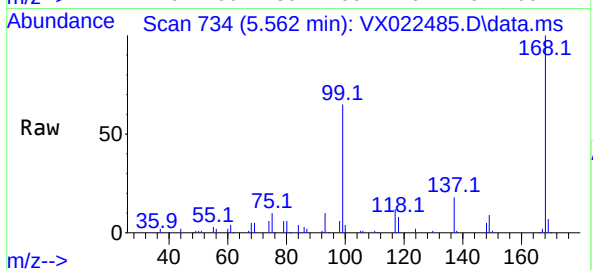

#16
Acetone
Concen: 9.003 ug/l
RT: 2.386 min Scan# 213
Delta R.T. -0.006 min
Lab File: VX022485.D
Acq: 06 Jun 2021 18:09

Tgt Ion: 43 Resp: 3956
Ion Ratio Lower Upper
43 100
58 42.2 27.8 41.8#

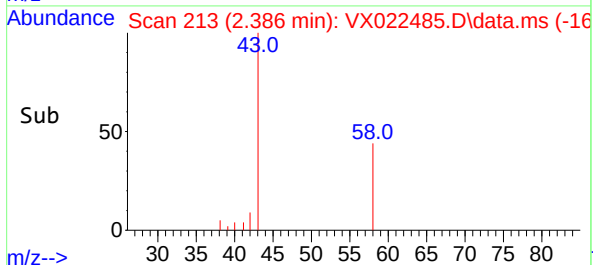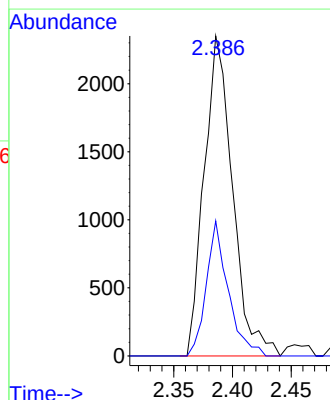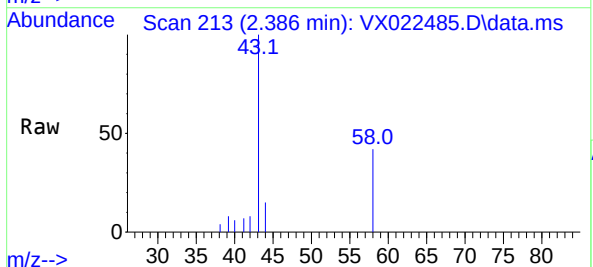




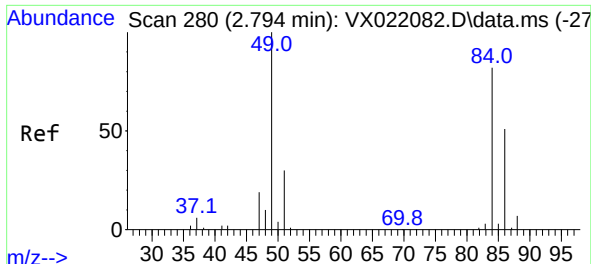


#20
Methylene Chloride
Concen: 3.299 ug/l
RT: 2.794 min Scan# 280
Delta R.T. 0.000 min
Lab File: VX022485.D
Acq: 06 Jun 2021 18:09

Instrument :
MSVOA_X
ClientSampleId :
PB136837ZHE#13

Tgt Ion: 84 Resp: 3218




Ion	Ratio	Lower	Upper
84	100		
49	102.5	88.6	132.8
51	31.4	27.0	40.6
86	59.1	50.3	75.5

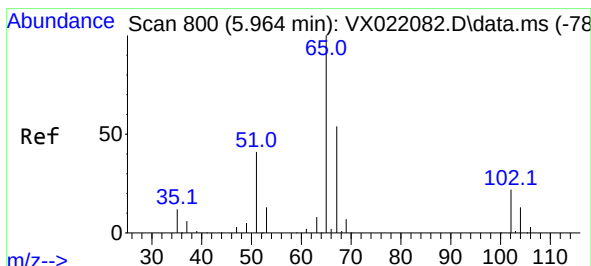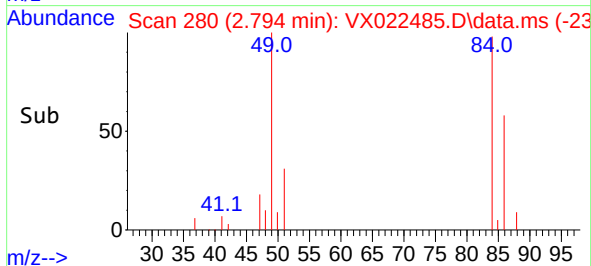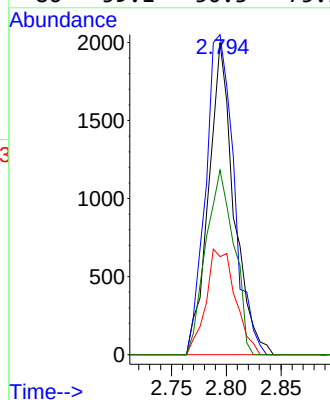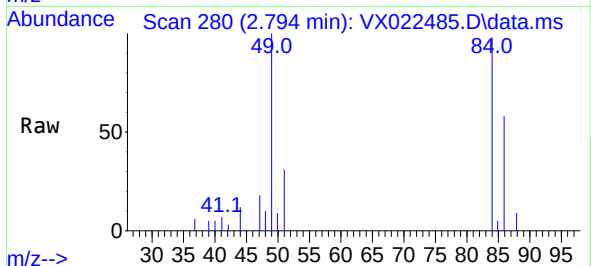


#33
1,2-Dichloroethane-d4
Concen: 53.047 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.000 min
Lab File: VX022485.D
Acq: 06 Jun 2021 18:09

Tgt Ion: 65 Resp: 53529

Ion	Ratio	Lower	Upper
65	100		
67	53.5	0.0	105.4


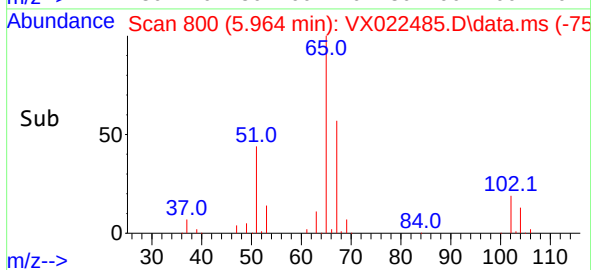
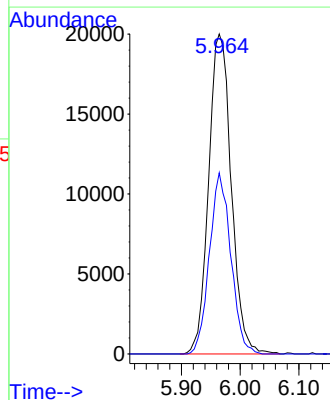
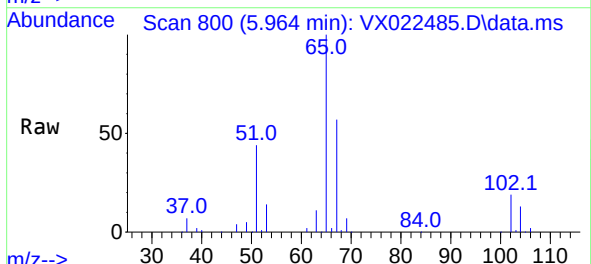


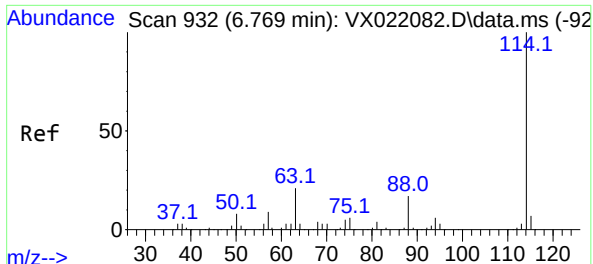

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 932
Delta R.T. 0.000 min
Lab File: VX022485.D
Acq: 06 Jun 2021 18:09




Instrument :
MSVOA_X
ClientSampleId :
PB136837ZHE#13


Tgt Ion:114 Resp: 132661
Ion Ratio Lower Upper
114 100
63 20.3 0.0 40.8
88 16.6 0.0 32.8

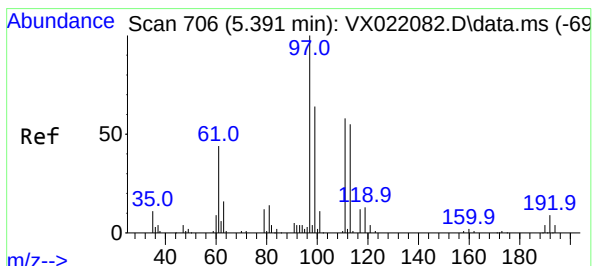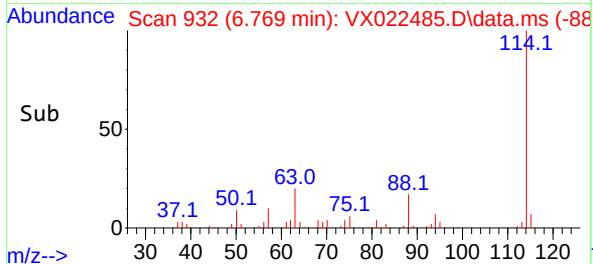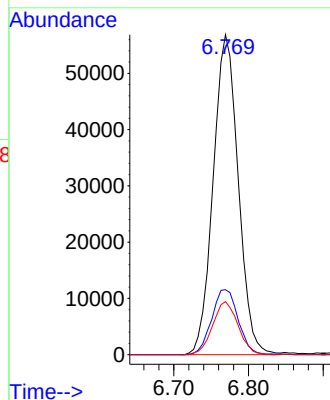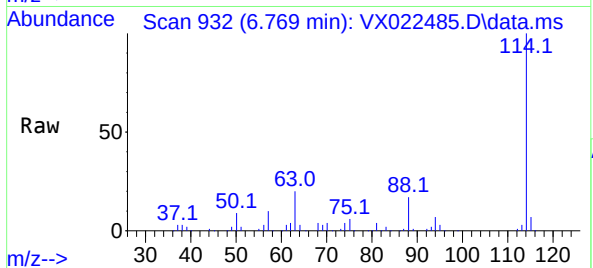

#35
Dibromofluoromethane
Concen: 46.245 ug/l
RT: 5.391 min Scan# 706
Delta R.T. 0.000 min
Lab File: VX022485.D
Acq: 06 Jun 2021 18:09

Tgt Ion:113 Resp: 38905
Ion Ratio Lower Upper
113 100
111 103.8 81.9 122.9
192 15.2 16.7 25.1#


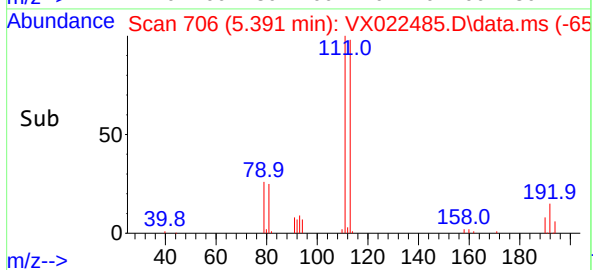
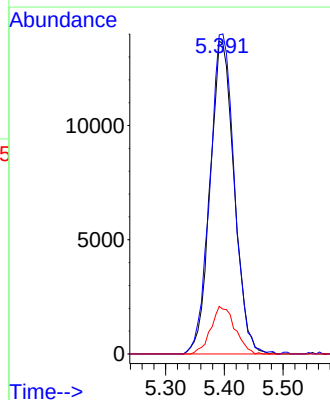
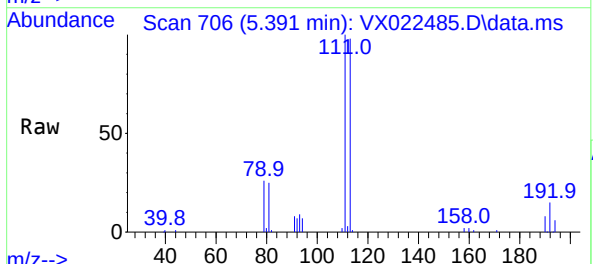


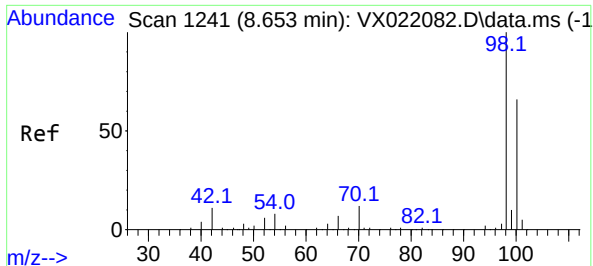

#50
Toluene-d8
Concen: 49.507 ug/l
RT: 8.653 min Scan# 1241
Delta R.T. -0.000 min
Lab File: VX022485.D
Acq: 06 Jun 2021 18:09




Instrument :
MSVOA_X
ClientSampleId :
PB136837ZHE#13


Tgt Ion: 98 Resp: 160436
Ion Ratio Lower Upper
98 100
100 67.2 51.9 77.9

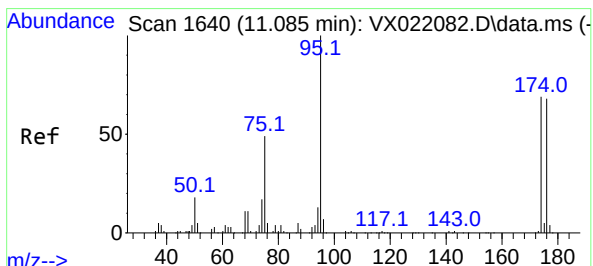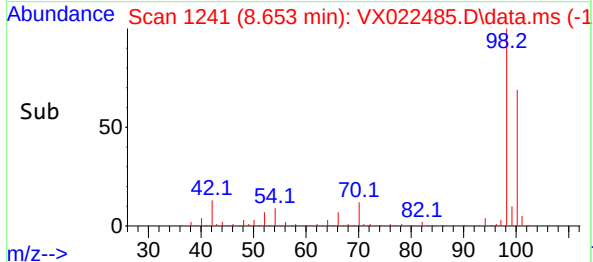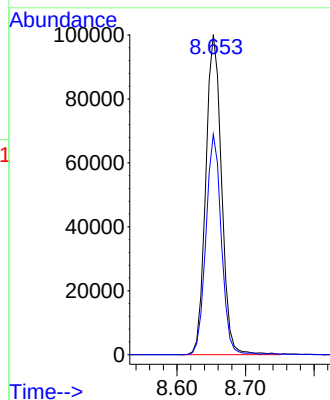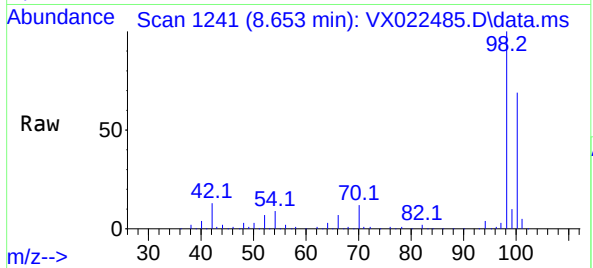

#62
4-Bromofluorobenzene
Concen: 47.231 ug/l
RT: 11.085 min Scan# 1640
Delta R.T. 0.000 min
Lab File: VX022485.D
Acq: 06 Jun 2021 18:09

Tgt Ion: 95 Resp: 56574
Ion Ratio Lower Upper
95 100
174 62.3 0.0 154.6
176 59.5 0.0 155.8


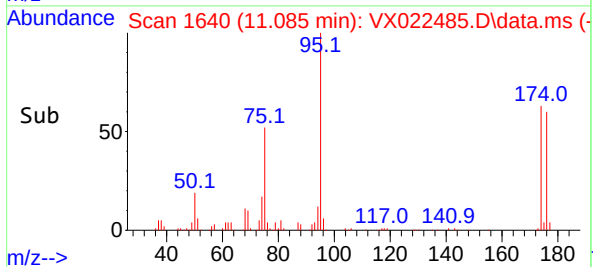
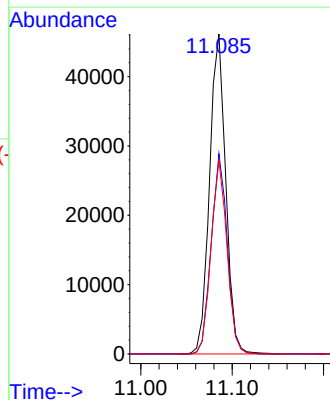
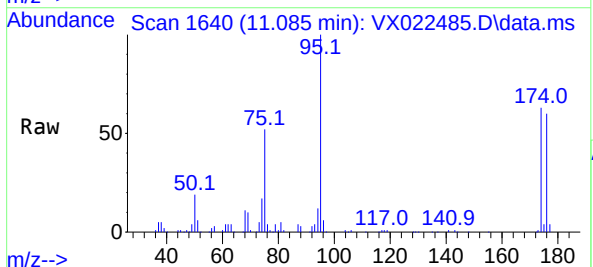


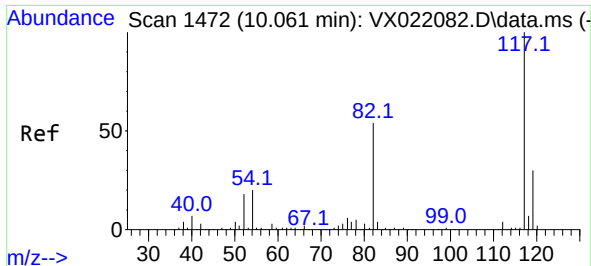

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.061 min Scan# 1472
Delta R.T. 0.000 min
Lab File: VX022485.D
Acq: 06 Jun 2021 18:09

Instrument :
MSVOA_X
ClientSampleId :
PB136837ZHE#13

Tgt Ion:117 Resp: 117904
Ion Ratio Lower Upper
117 100
82 53.7 47.4 71.2
119 29.6 26.6 39.8

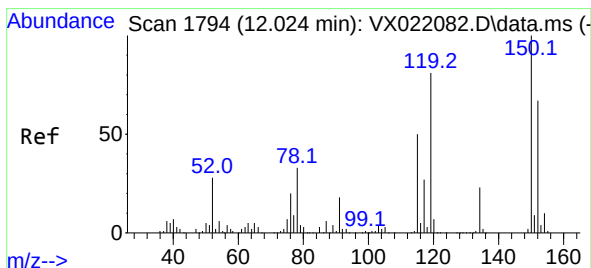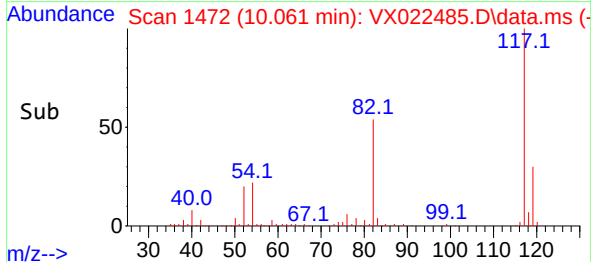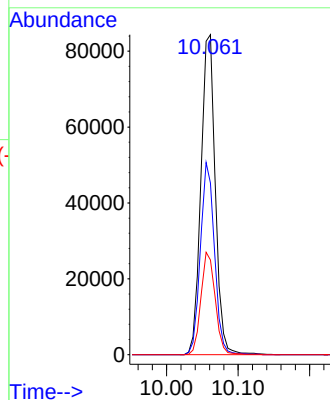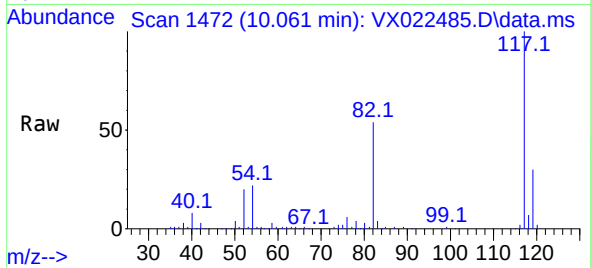

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX022485.D
Acq: 06 Jun 2021 18:09

Tgt Ion:152 Resp: 46157
Ion Ratio Lower Upper
152 100
115 66.8 41.1 123.3
150 155.7 0.0 349.0

